

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
 Data File : PR057668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 15:57
 Operator : AJ\MA
 Sample : N4955-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:44:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 24 18:17:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.691	2.924	48738395	39417628	23.203	19.590
2)	SA Decachlor...	9.634	8.182	49929131	54615552	22.582	23.132
Target Compounds							
8)	L2 AR-1221-1	3.914	3.150	925960	482223	32.486	21.095 #
9)	L2 AR-1221-2	4.004	3.229	1166376	795199	56.151	44.419
10)	L2 AR-1221-3	4.081	3.312	1961006	1242934	32.519	23.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
Data File : PR057668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 15:57
Operator : AJ\MA
Sample : N4955-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:44:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 24 18:17:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

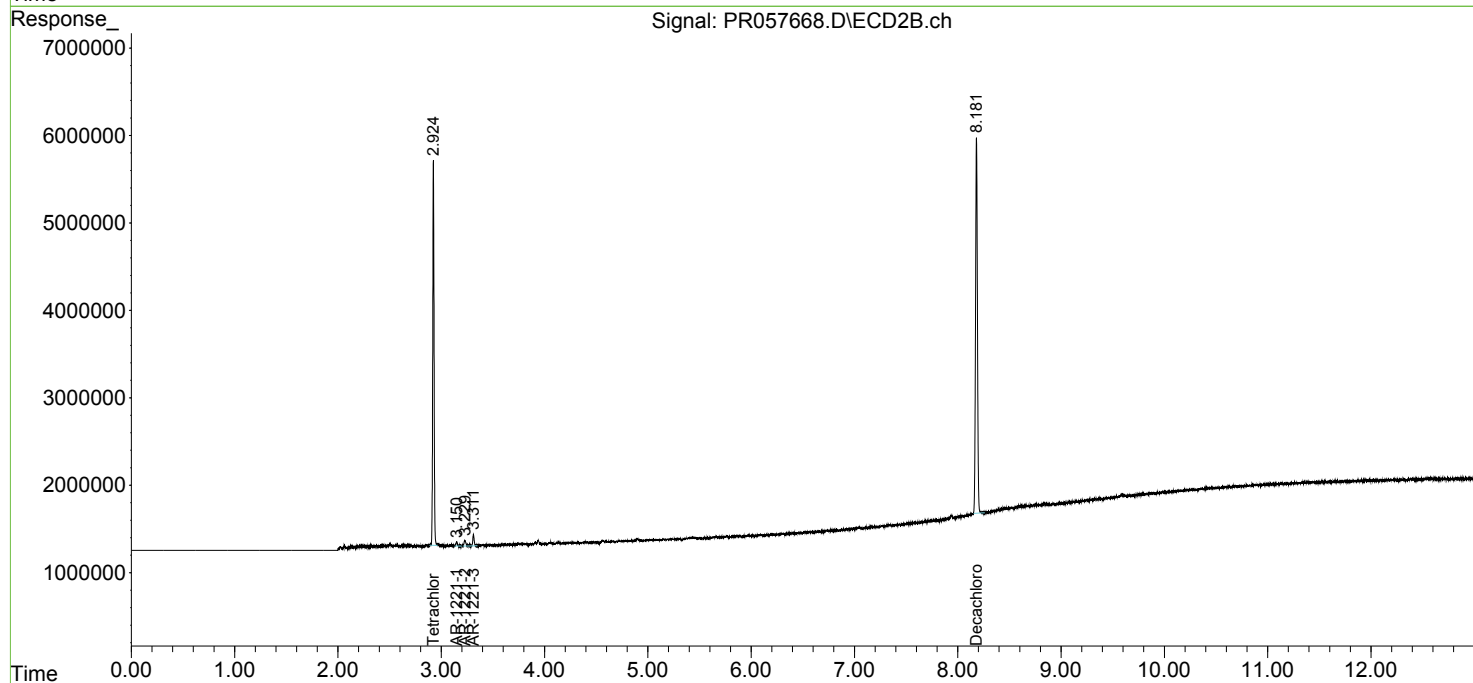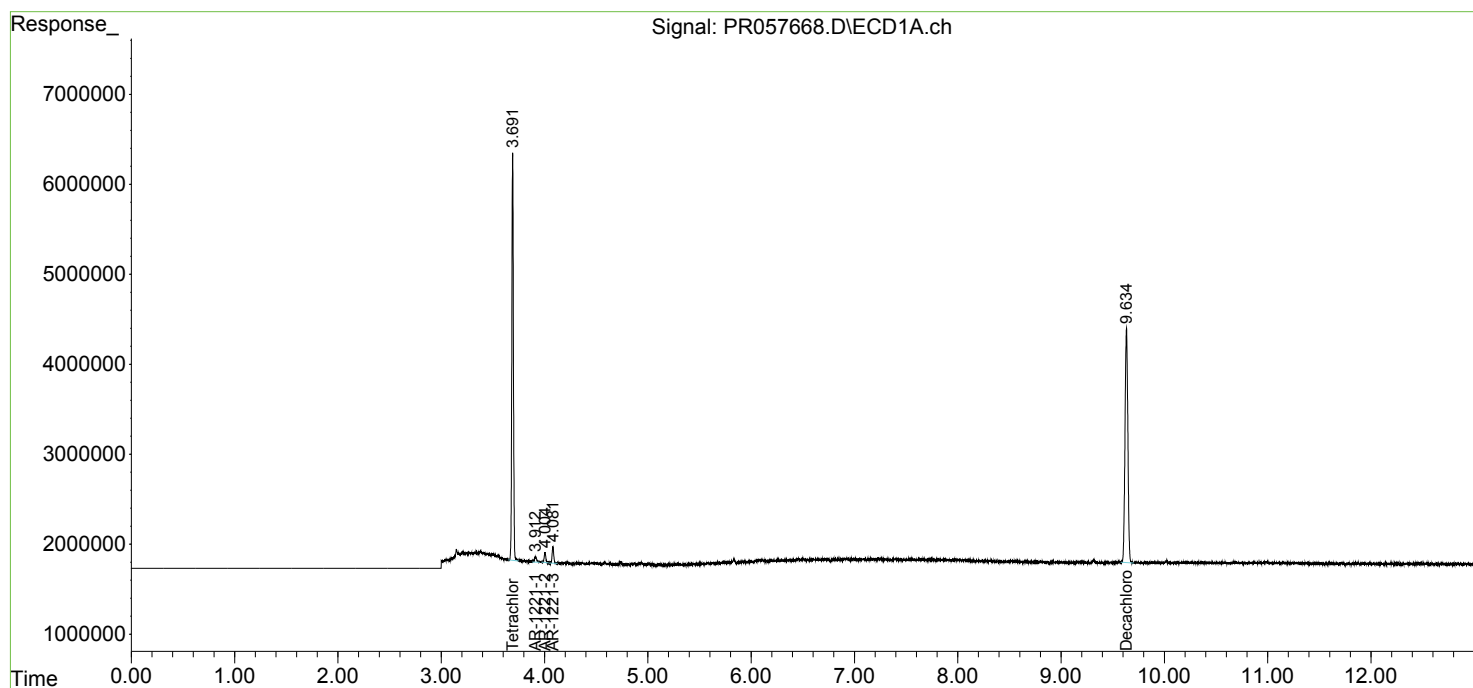


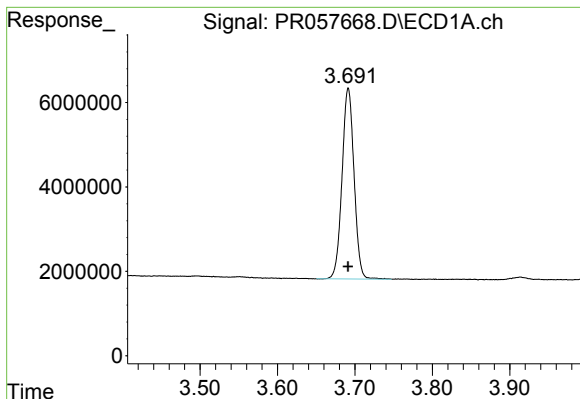

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 48738395
Conc: 23.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

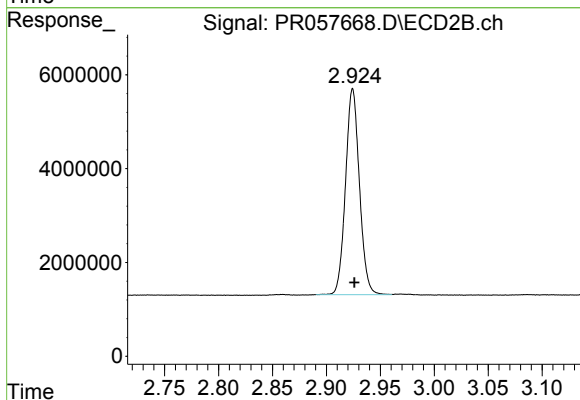


#1 Tetrachloro-m-xylene

R.T.: 2.924 min
Delta R.T.: -0.002 min
Response: 39417628
Conc: 19.59 ng/ml

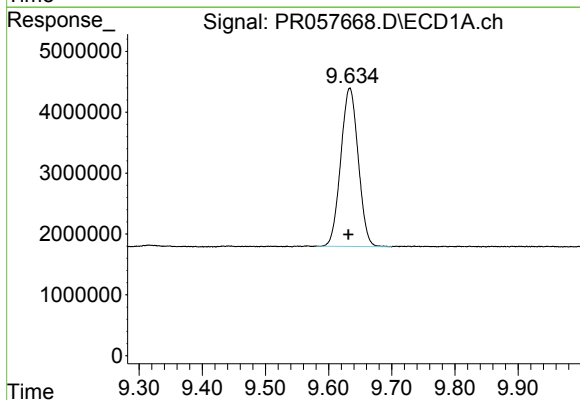


#2 Decachlorobiphenyl

R.T.: 9.634 min
Delta R.T.: 0.002 min
Response: 49929131
Conc: 22.58 ng/ml

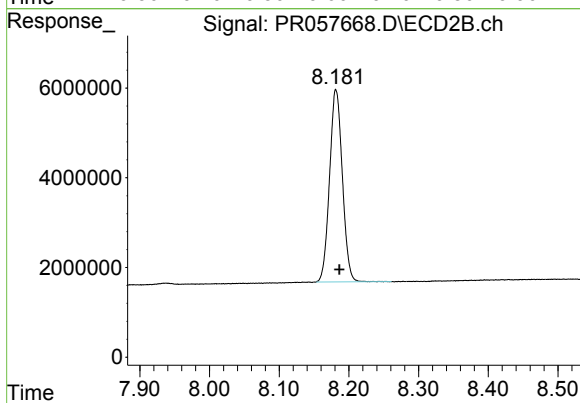

#2 Decachlorobiphenyl


R.T.: 8.182 min
Delta R.T.: -0.005 min
Response: 54615552
Conc: 23.13 ng/ml

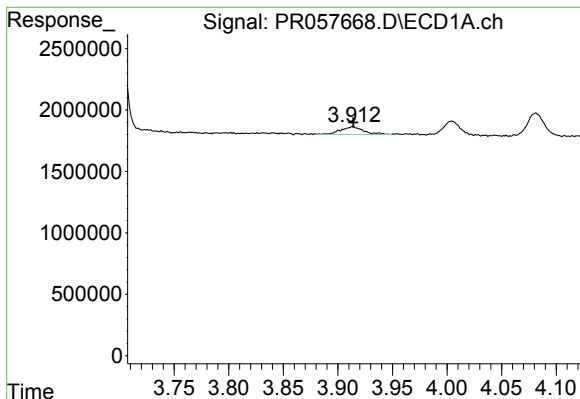

#8 AR-1221-1


R.T.: 3.914 min
Delta R.T.: 0.000 min
Response: 925960
Conc: 32.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

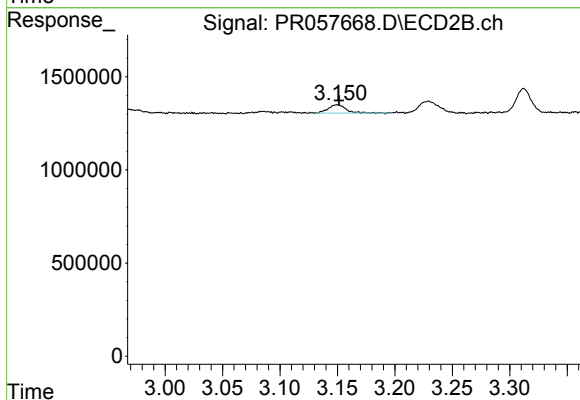


#8 AR-1221-1

R.T.: 3.150 min
Delta R.T.: -0.002 min
Response: 482223
Conc: 21.10 ng/ml

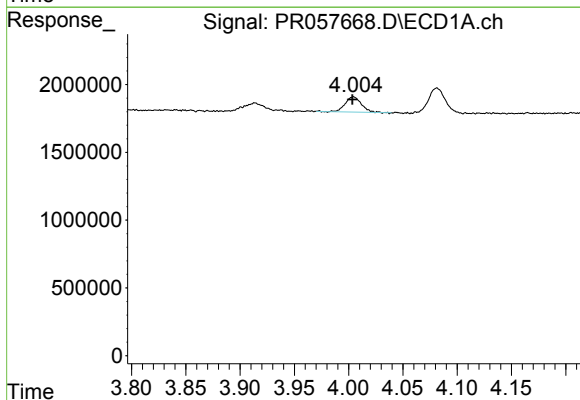


#9 AR-1221-2

R.T.: 4.004 min
Delta R.T.: 0.001 min
Response: 1166376
Conc: 56.15 ng/ml

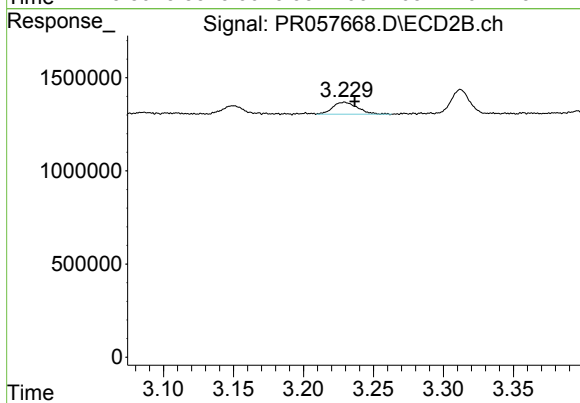

#9 AR-1221-2


R.T.: 3.229 min
Delta R.T.: -0.007 min
Response: 795199
Conc: 44.42 ng/ml

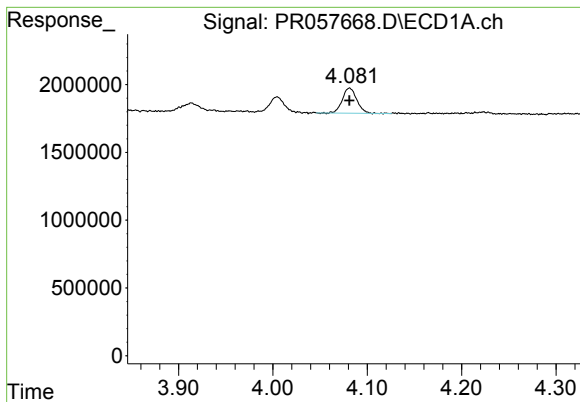

#10 AR-1221-3

R.T.: 4.081 min
Delta R.T.: 0.000 min
Response: 1961006
Conc: 32.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

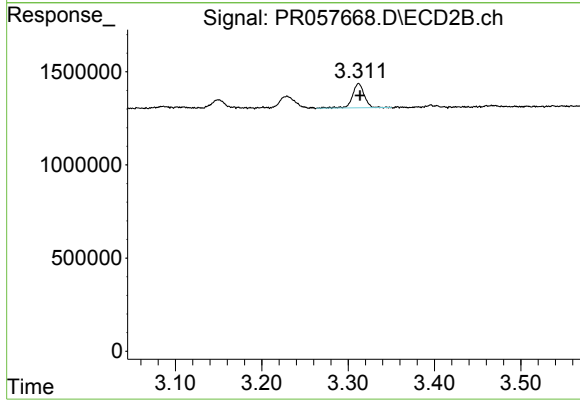

#10 AR-1221-3

R.T.: 3.312 min
Delta R.T.: -0.001 min
Response: 1242934
Conc: 23.06 ng/ml