

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
 Data File : PR057674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 17:31
 Operator : AJ\MA
 Sample : N4955-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:49:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 24 18:17:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	2.924	48832736	39326694	23.248	19.545
2) SA Decachlor...	9.631	8.180	53107300	58281308	24.020	24.685
Target Compounds						
41) L9 AR-1268-1	8.206	7.035	8526280	6761108	23.824	21.610
42) L9 AR-1268-2	8.298	7.103	7579936	6753219	23.731	21.126
43) L9 AR-1268-3	8.518	7.326	6570303	6340122	25.002	23.283
44) L9 AR-1268-4	8.926	7.639	2787028	2479134	24.597	22.666
45) L9 AR-1268-5	9.315	7.935	18407304	19937311	23.155	20.061



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
Data File : PR057674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 17:31
Operator : AJ\MA
Sample : N4955-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:49:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 24 18:17:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

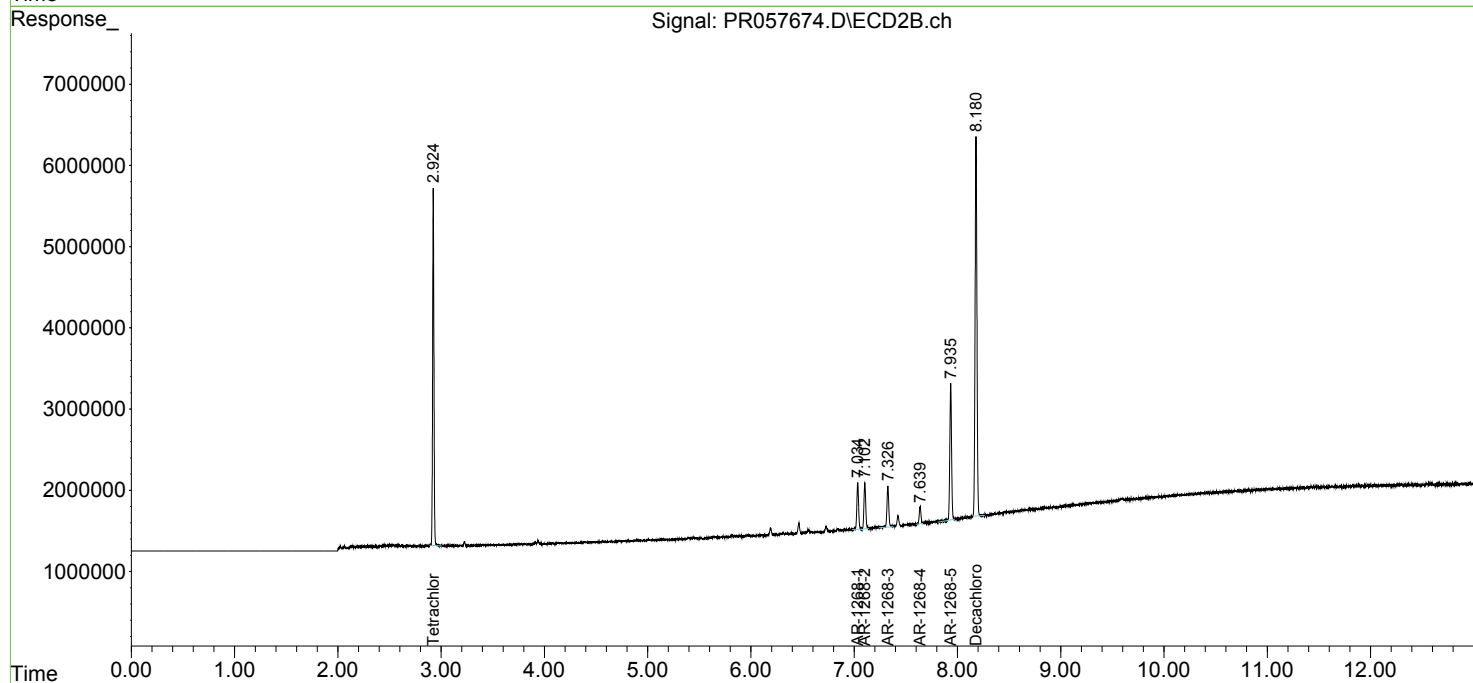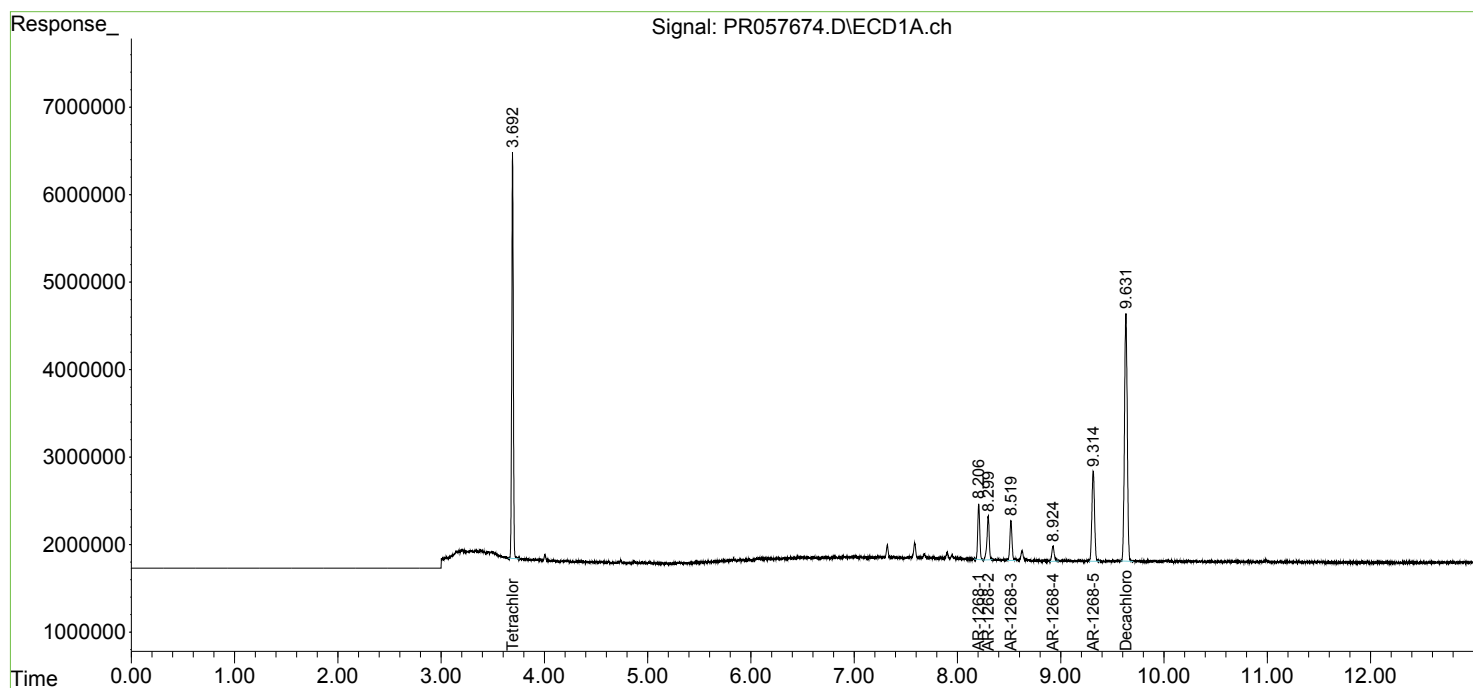


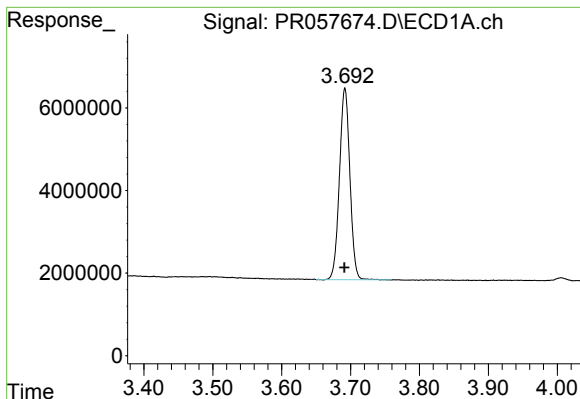

#1 Tetrachloro-m-xylene


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 48832736
Conc: 23.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

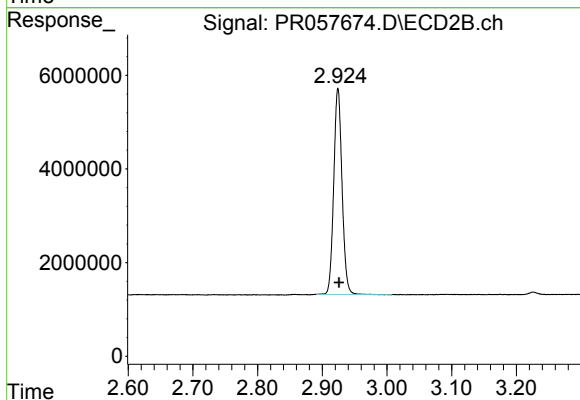


#1 Tetrachloro-m-xylene

R.T.: 2.924 min
Delta R.T.: -0.002 min
Response: 39326694
Conc: 19.54 ng/ml

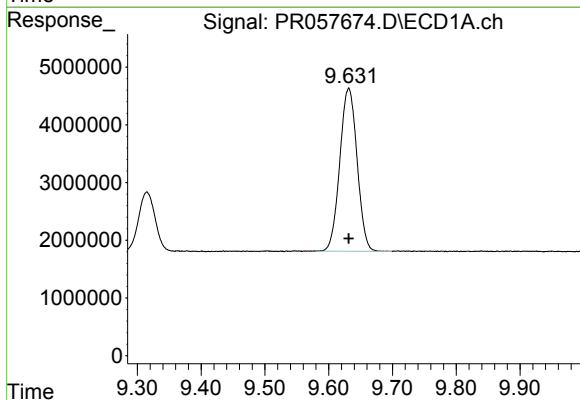


#2 Decachlorobiphenyl

R.T.: 9.631 min
Delta R.T.: 0.000 min
Response: 53107300
Conc: 24.02 ng/ml

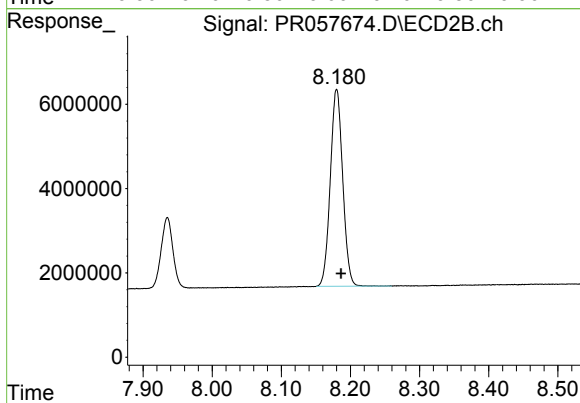

#2 Decachlorobiphenyl


R.T.: 8.180 min
Delta R.T.: -0.006 min
Response: 58281308
Conc: 24.68 ng/ml

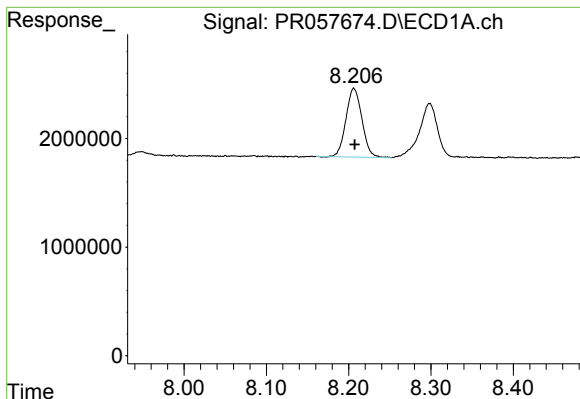

#41 AR-1268-1


R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 8526280
Conc: 23.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

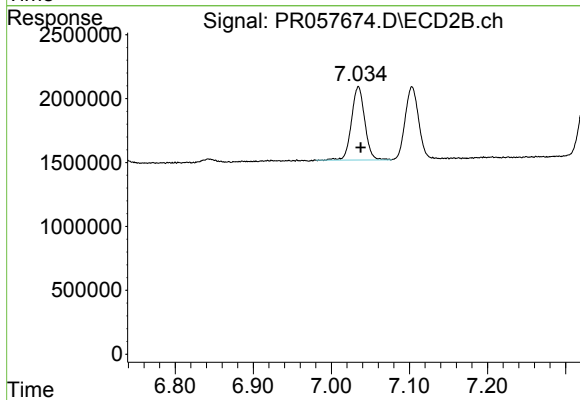


#41 AR-1268-1

R.T.: 7.035 min
Delta R.T.: -0.003 min
Response: 6761108
Conc: 21.61 ng/ml

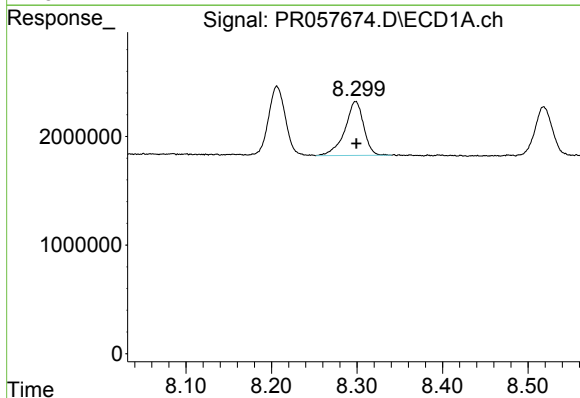


#42 AR-1268-2

R.T.: 8.298 min
Delta R.T.: 0.000 min
Response: 7579936
Conc: 23.73 ng/ml

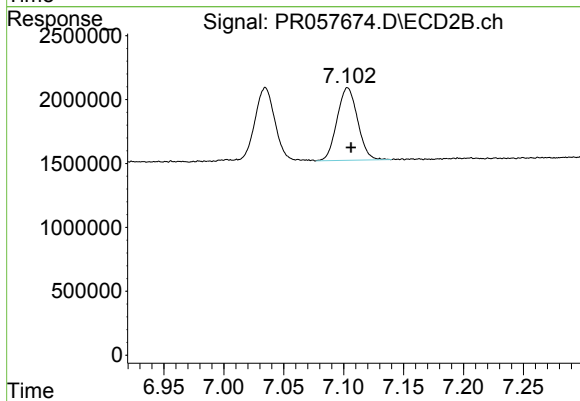

#42 AR-1268-2


R.T.: 7.103 min
Delta R.T.: -0.003 min
Response: 6753219
Conc: 21.13 ng/ml

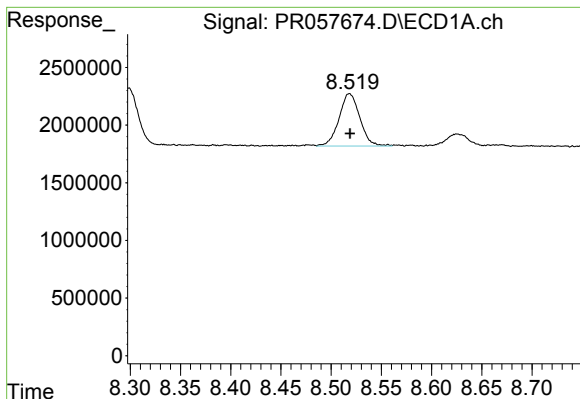

#43 AR-1268-3


R.T.: 8.518 min
Delta R.T.: 0.000 min
Response: 6570303
Conc: 25.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

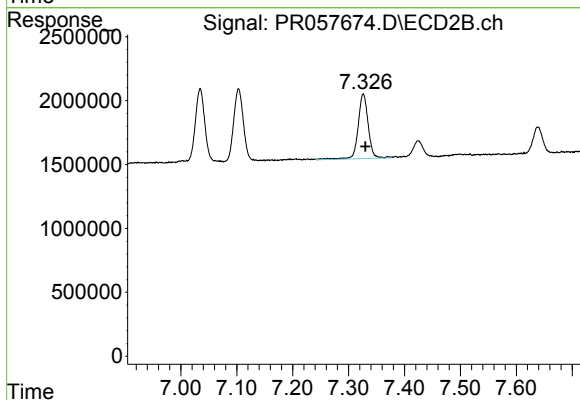


#43 AR-1268-3

R.T.: 7.326 min
Delta R.T.: -0.004 min
Response: 6340122
Conc: 23.28 ng/ml

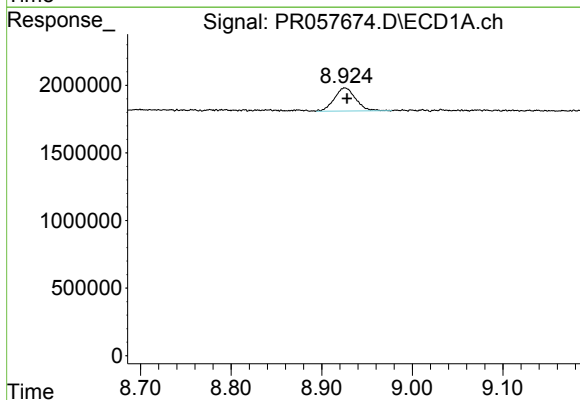


#44 AR-1268-4

R.T.: 8.926 min
Delta R.T.: -0.002 min
Response: 2787028
Conc: 24.60 ng/ml

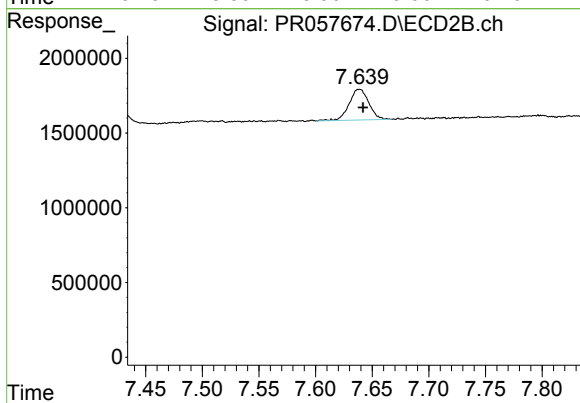

#44 AR-1268-4


R.T.: 7.639 min
Delta R.T.: -0.003 min
Response: 2479134
Conc: 22.67 ng/ml

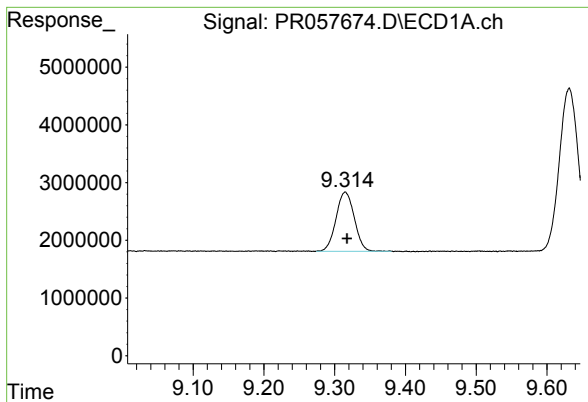

#45 AR-1268-5

R.T.: 9.315 min
Delta R.T.: -0.002 min
Response: 18407304
Conc: 23.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2022

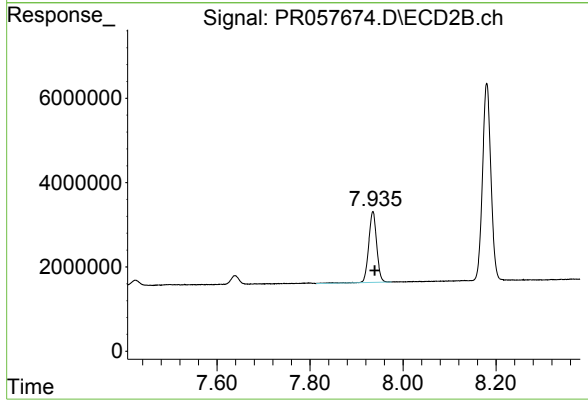

#45 AR-1268-5

R.T.: 7.935 min
Delta R.T.: -0.004 min
Response: 19937311
Conc: 20.06 ng/ml