

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
 Data File : PR057695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 00:20
 Operator : AJ\MA
 Sample : N5226-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20221093-198-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 06:05:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 24 18:17:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	2.924	48573470	39013584	23.125	19.389
2) SA Decachlor...	9.629	8.177	42104588	46219626	19.043	19.576

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
Data File : PR057695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 00:20
Operator : AJ\MA
Sample : N5226-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
20221093-198-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:05:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 24 18:17:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

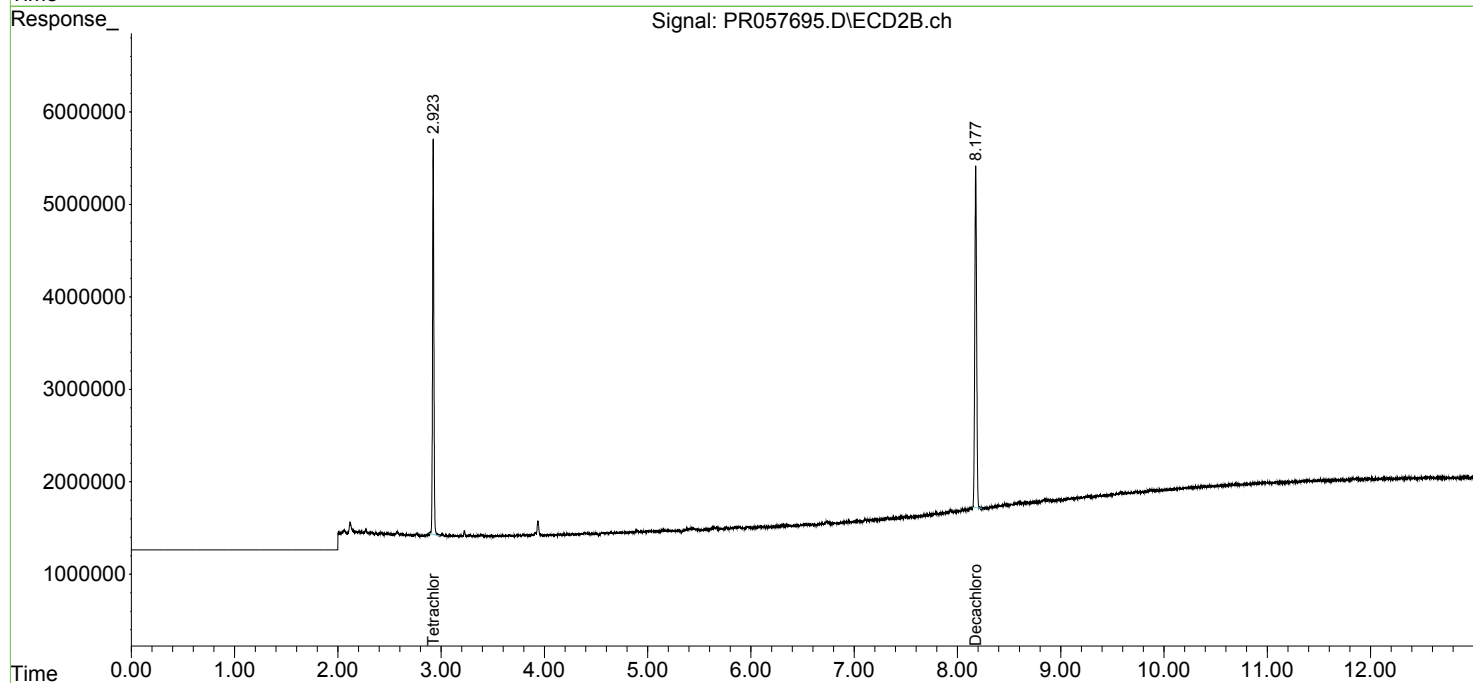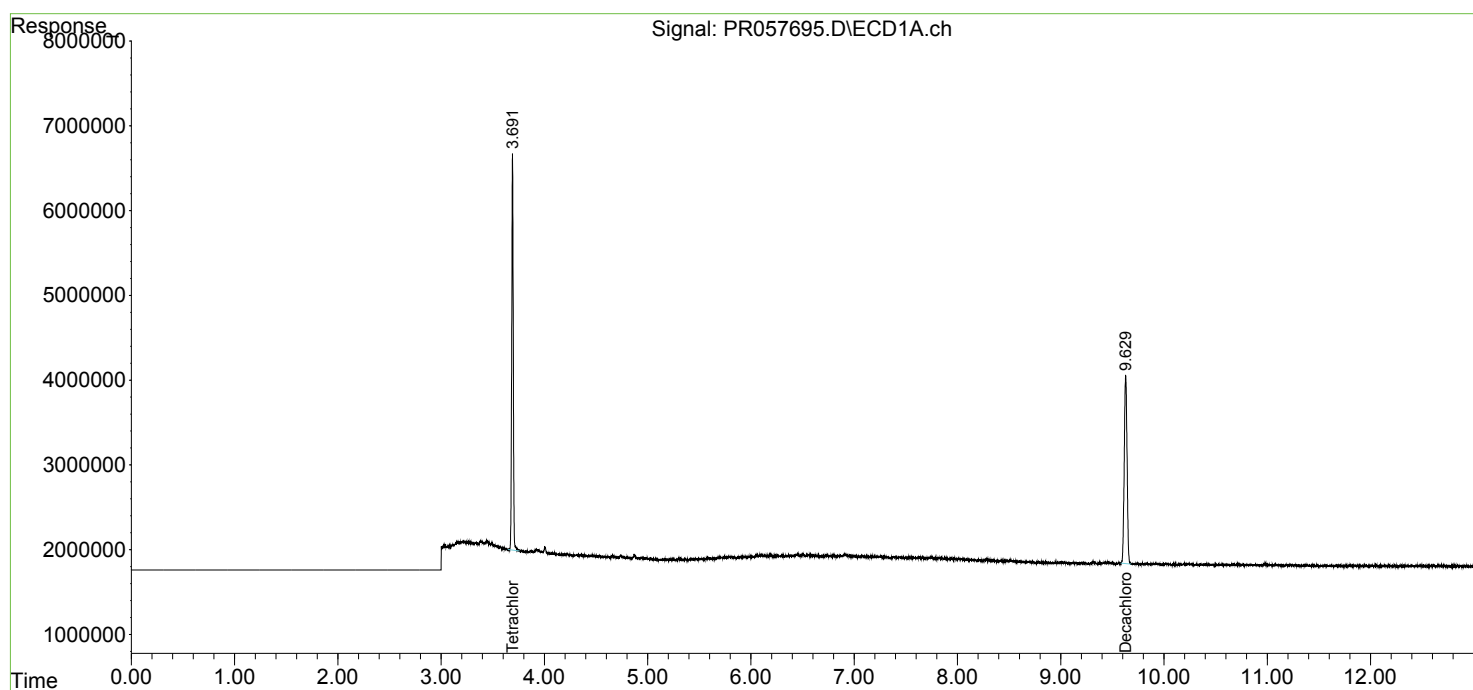


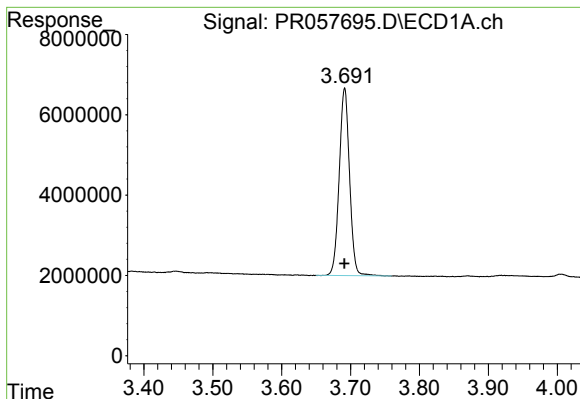

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 48573470
Conc: 23.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
20221093-198-SITE-WATER

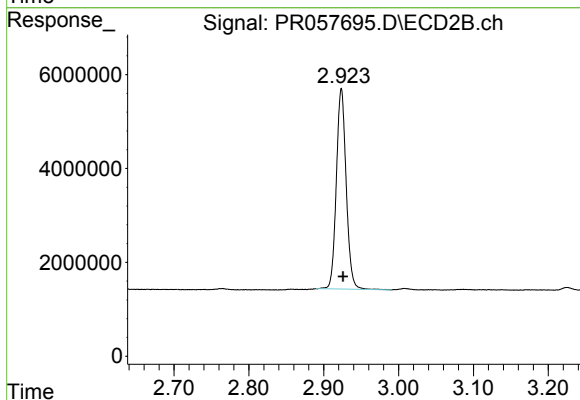


#1 Tetrachloro-m-xylene

R.T.: 2.924 min
Delta R.T.: -0.002 min
Response: 39013584
Conc: 19.39 ng/ml

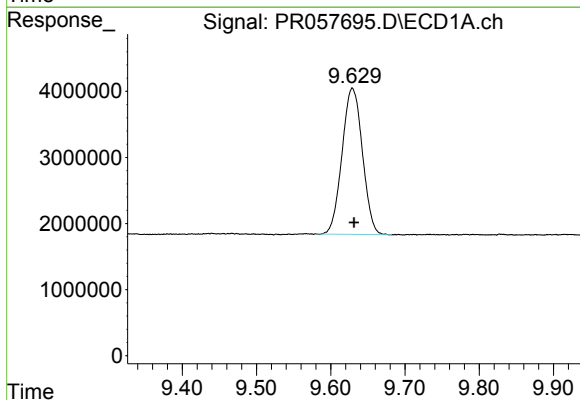

#2 Decachlorobiphenyl

R.T.: 9.629 min
Delta R.T.: -0.002 min
Response: 42104588
Conc: 19.04 ng/ml

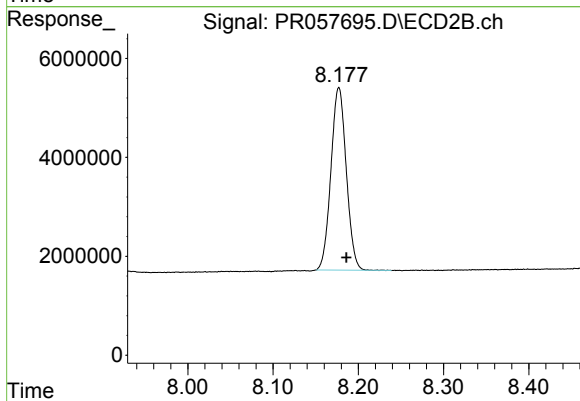

#2 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: -0.009 min
Response: 46219626
Conc: 19.58 ng/ml