

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
Data File : PR057699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 01:23
Operator : AJ\MA
Sample : N5226-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
20221098-203-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:10:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 24 18:17:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	2.925	55666850	45422196	26.502	22.574
2) SA Decachlor...	9.627	8.177	42187298	46117191	19.081	19.533

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR102522\
Data File : PR057699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 01:23
Operator : AJ\MA
Sample : N5226-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
20221098-203-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:10:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 24 18:17:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

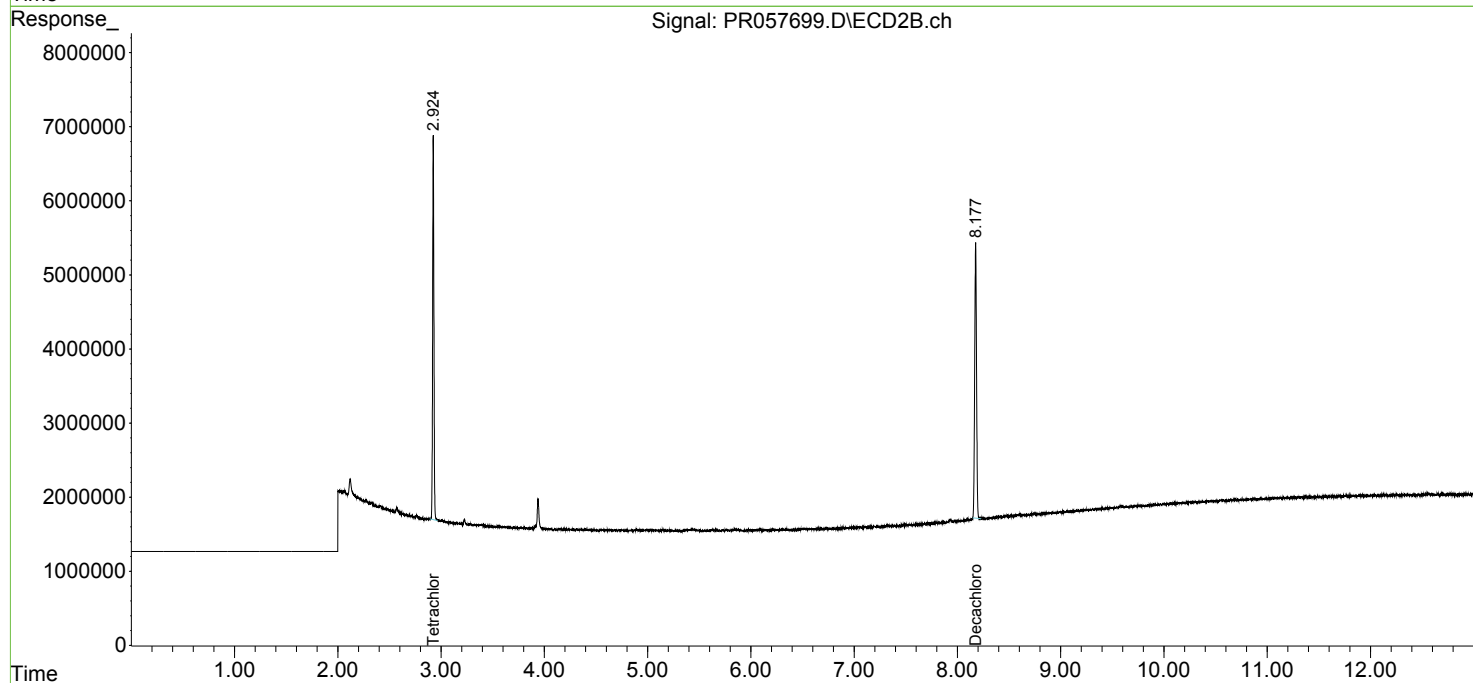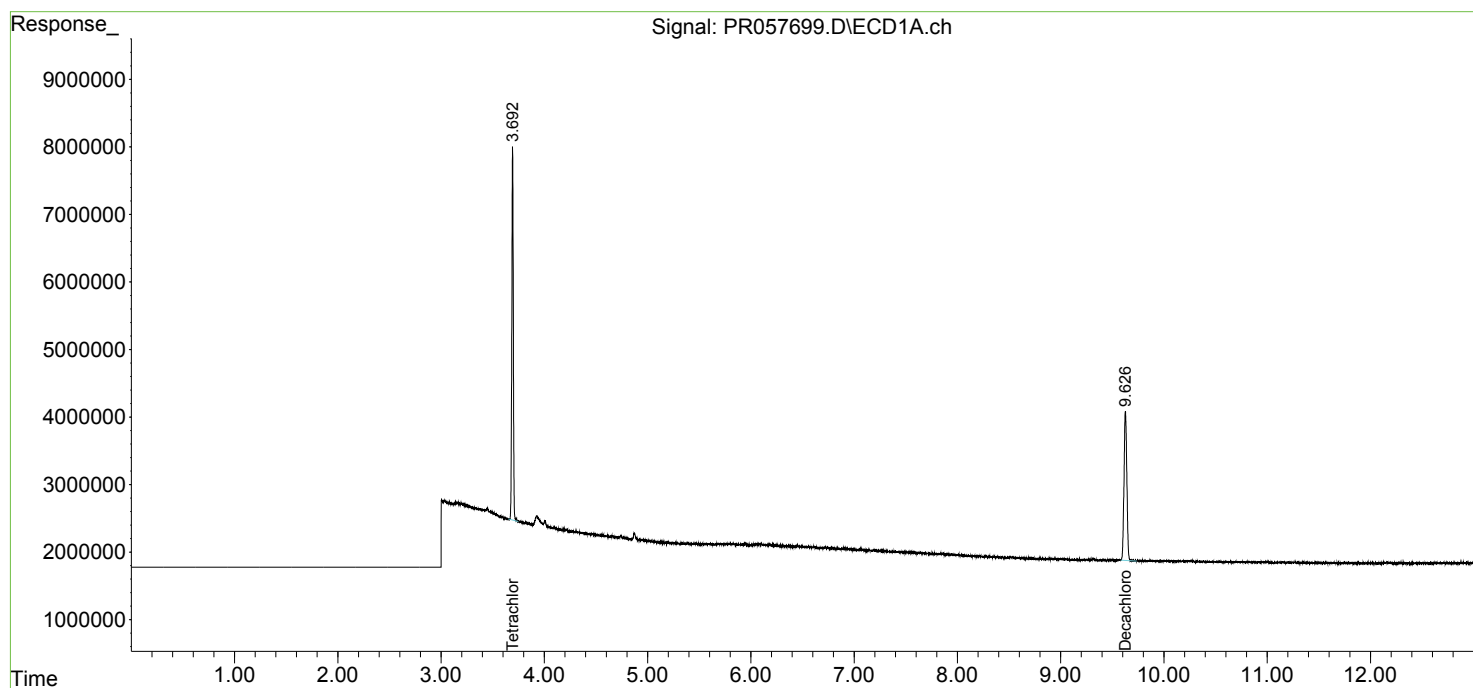


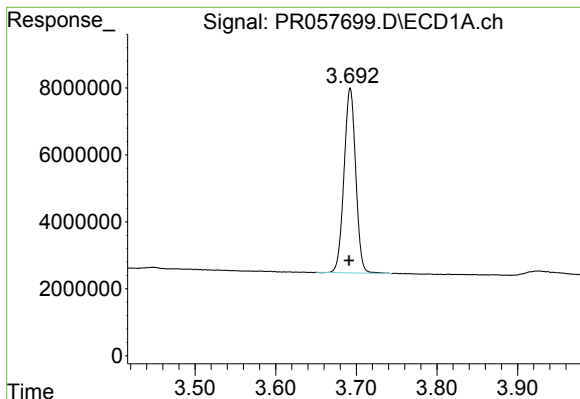

#1 Tetrachloro-m-xylene


R.T.: 3.693 min
Delta R.T.: 0.002 min
Response: 55666850
Conc: 26.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
20221098-203-SITE-WATER

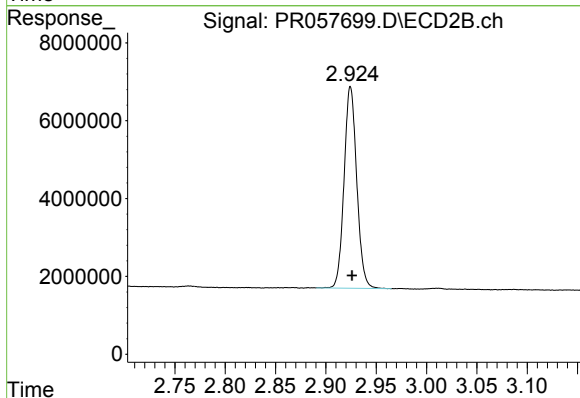


#1 Tetrachloro-m-xylene

R.T.: 2.925 min
Delta R.T.: -0.002 min
Response: 45422196
Conc: 22.57 ng/ml

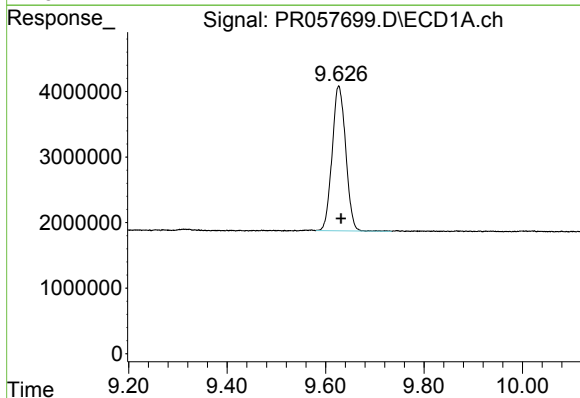

#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.005 min
Response: 42187298
Conc: 19.08 ng/ml

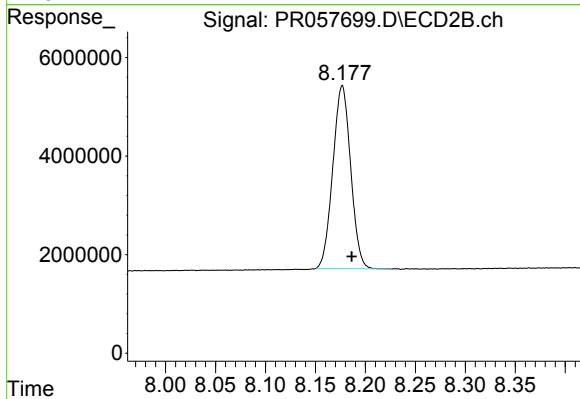

#2 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: -0.009 min
Response: 46117191
Conc: 19.53 ng/ml