

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR102620\  
Data File : PR048205.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Oct 2020 07:18  
Operator : AJ\MA  
Sample : L4505-06DL2 40X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
C0BG0DL2

Manual Integrations  
APPROVED

Ankita  
10/28/2020 3:41:05 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 27 07:42:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR102120CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 21 10:52:16 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

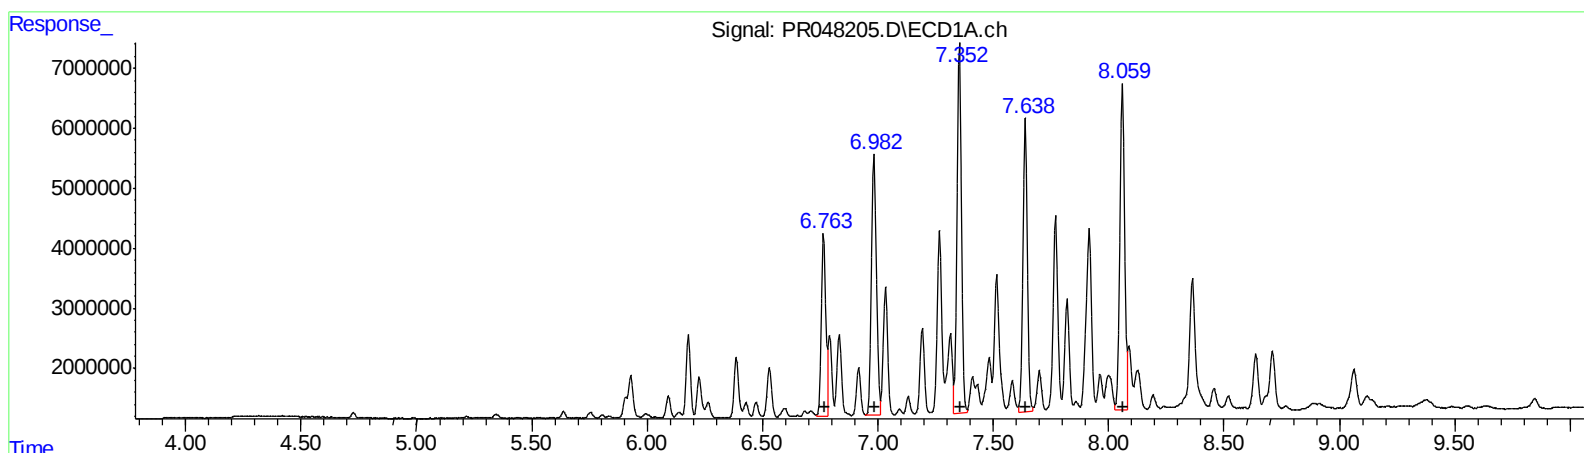

(26) AR-1254-1 (L6)  
R.T. Response Conc  
6.76 40311759 434.60  
6.98 66022062 458.22  
7.35 82064285 535.20  
7.64 64283930 542.05  
8.06 77898409 611.75  
(26) AR-1254-1 #2 (L6)  
R.T. Response Conc  
5.78 63448194 395.48  
5.93 70698241 431.42  
6.33 183052881 509.47  
6.56 283915543 591.19  
6.99 365884411 588.12

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR102620\  
Data File : PR048205.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Oct 2020 07:18  
Operator : AJ\MA  
Sample : L4505-06DL2 40X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
C0BG0DL2

Manual Integrations  
APPROVED

Ankita  
10/28/2020 3:41:05 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 27 07:42:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR102120CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 21 10:52:16 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

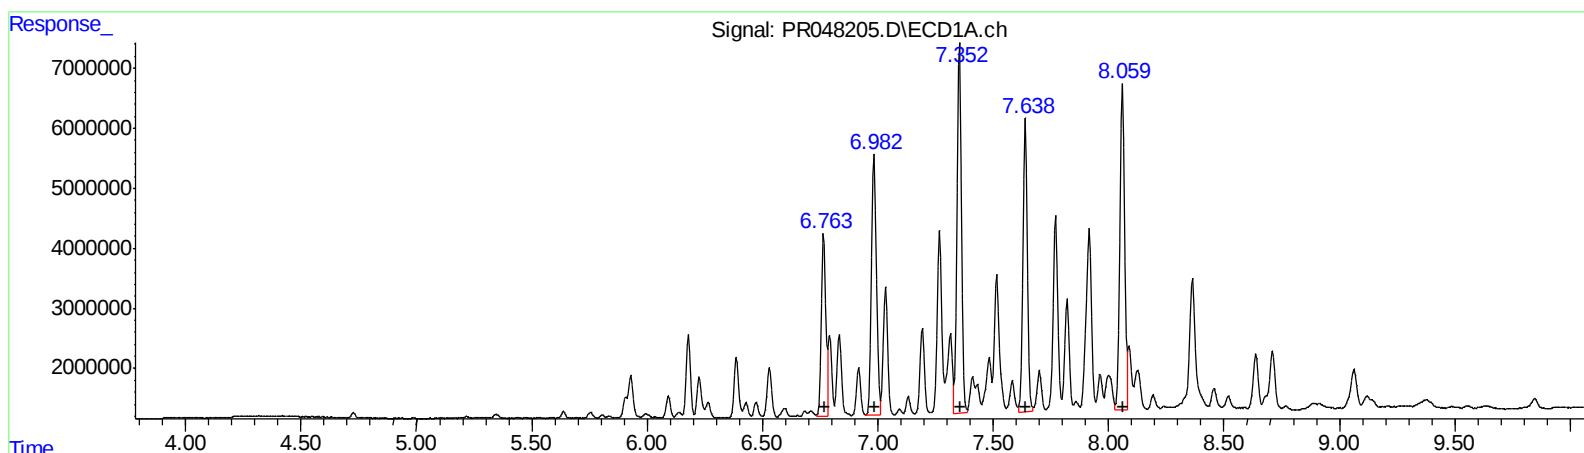

(26) AR-1254-1 #2 (L6)  
R.T. Response Conc  
6.76 40311759 434.60  
6.98 66022062 458.22  
7.35 82064285 535.20  
7.64 64283930 542.05  
8.06 77898409 611.75  
(26) AR-1254-1 #2 (L6)  
R.T. Response Conc  
5.78 63448194 395.48  
5.93 70698241 431.42  
6.33 183052881 509.47  
6.56 240206228 500.17  
6.99 365884411 588.12

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR102620\  
 Data File : PR048205.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Oct 2020 07:18  
 Operator : AJ\MA  
 Sample : L4505-06DL2 40X  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 C0BG0DL2

Manual Integrations  
 APPROVED

Ankita  
 10/28/2020 3:41:05 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 27 07:42:45 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR102120CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 21 10:52:16 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

#### Target Compounds

|     |              |       |       |          |          |         |          |
|-----|--------------|-------|-------|----------|----------|---------|----------|
| 26) | L6 AR-1254-1 | 6.764 | 5.778 | 40311759 | 63448194 | 434.599 | 395.484  |
| 27) | L6 AR-1254-2 | 6.982 | 5.926 | 66022062 | 70698241 | 458.221 | 431.424  |
| 28) | L6 AR-1254-3 | 7.352 | 6.335 | 82064285 | 183.1E6  | 535.201 | 509.474  |
| 29) | L6 AR-1254-4 | 7.638 | 6.564 | 64283930 | 240.2E6  | 542.054 | 500.172m |
| 30) | L6 AR-1254-5 | 8.059 | 6.985 | 77898409 | 365.9E6  | 611.746 | 588.116  |

AJ  
 10/30/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.