
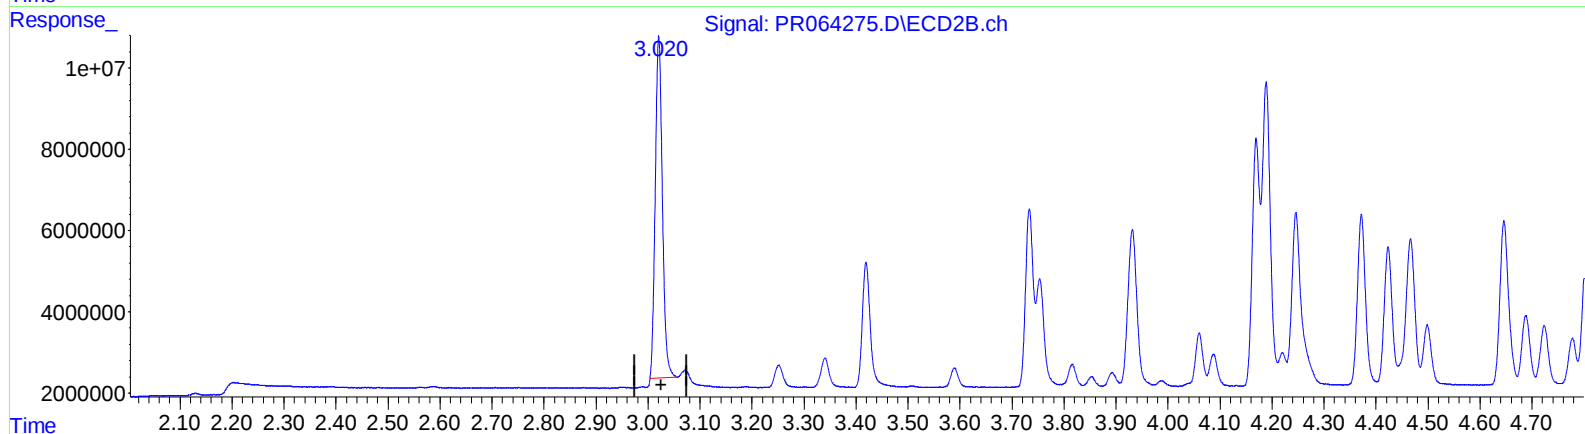


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 10:43
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:16:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

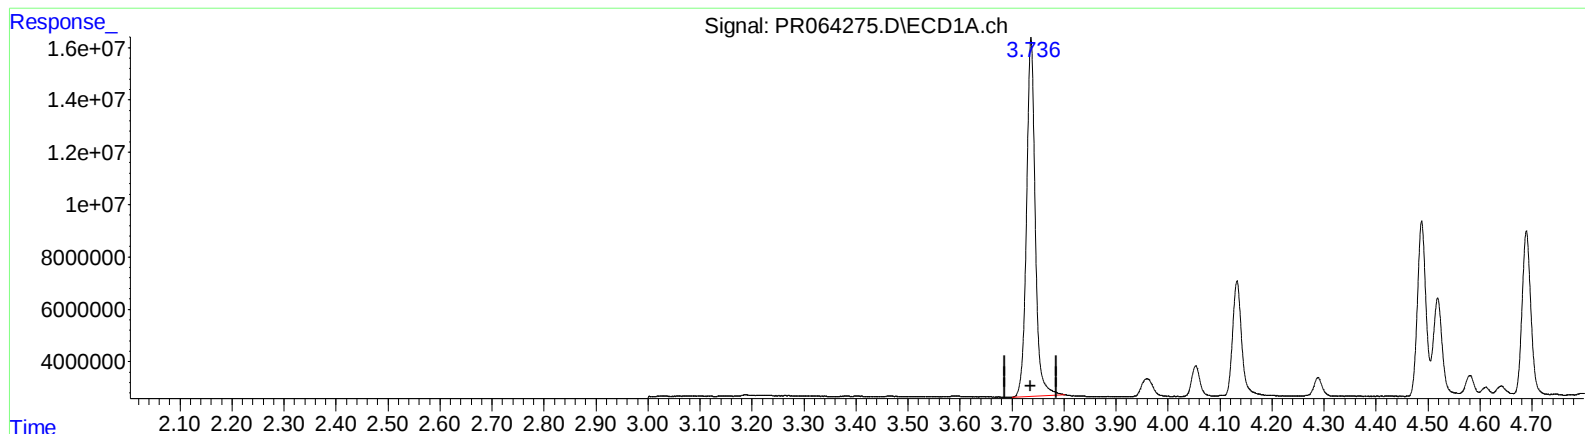

QEdit

(1) Tetrachloro-m-xylene (SA)

3.737min 22.214 ng/ml

response 159094221

(1) Tetrachloro-m-xylene #2 (SA)

3.021min 19.450 ng/ml



response 80277332

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 10:43
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:16:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

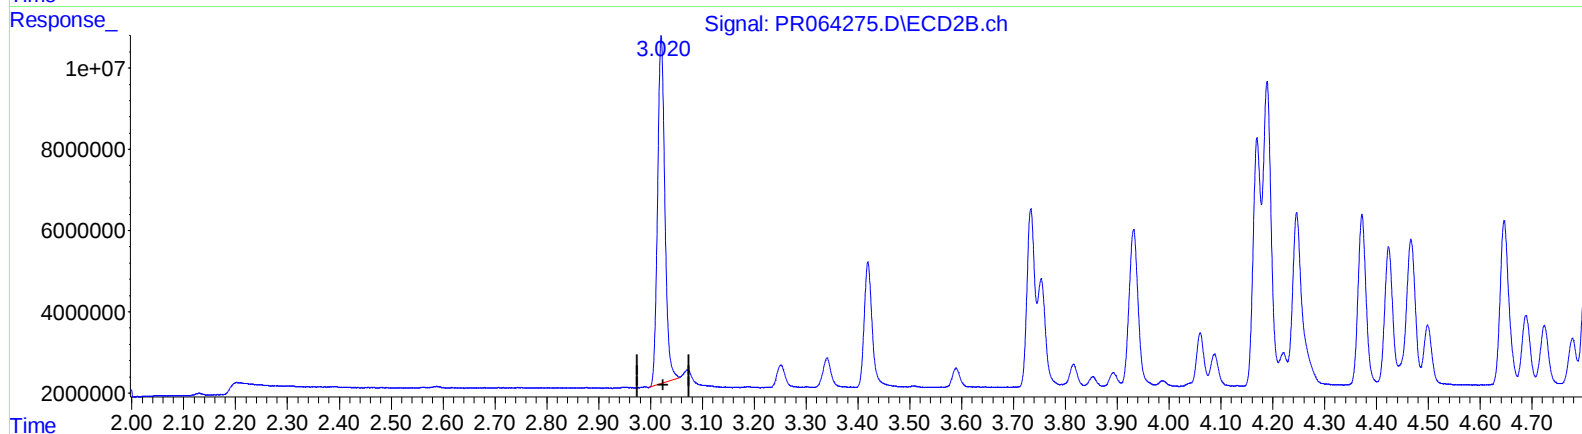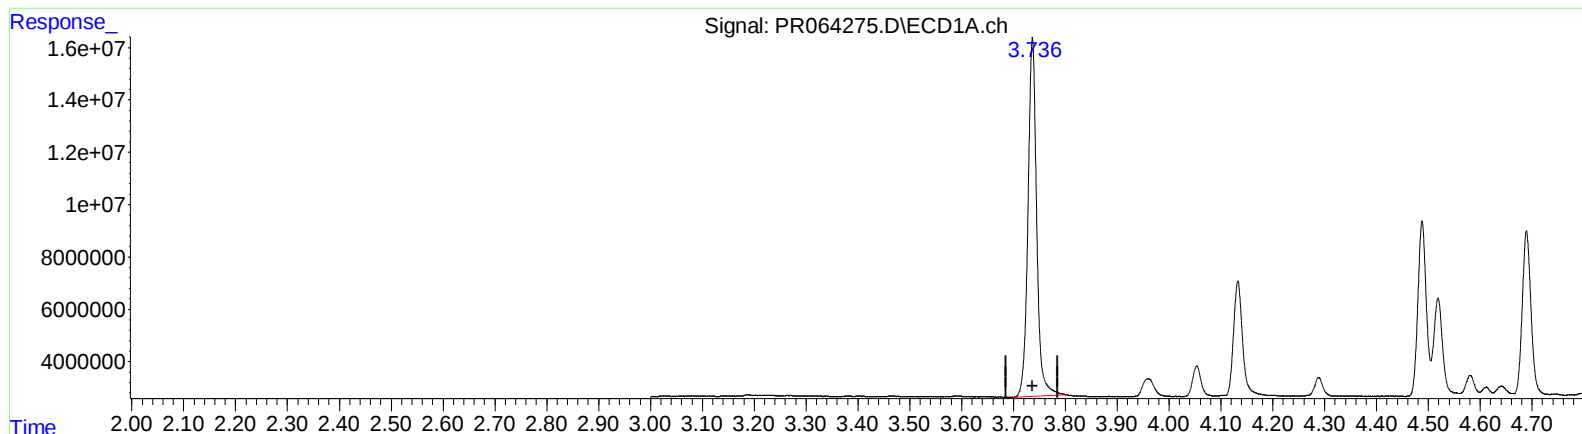

QEdit

(1) Tetrachloro-m-xylene (SA)

3.737min 22.214 ng/ml

response 159094221

(1) Tetrachloro-m-xylene #2 (SA)

3.020min 20.293 ng/ml m

response 83759530

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
 Data File : PR064275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 10:43
 Operator : AJ\MA
 Sample : AR1660CCC400
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:16:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 13 05:04:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.737	3.020	159.1E6	83759530	22.214	20.293m
2) SA Decachlor...	9.760	8.415	204.4E6	132.5E6	43.748	43.654
Target Compounds						
3) L1 AR-1016-1	4.979	4.170	92712268	58429519	430.997	401.939
4) L1 AR-1016-2	5.002	4.189	139.3E6	81638272	425.265	408.385
5) L1 AR-1016-3	5.067	4.372	88840558	45264026	429.455	410.591
6) L1 AR-1016-4	5.170	4.424	69837459	36885005	428.755	426.229
7) L1 AR-1016-5	5.489	4.646	69833231	46343199	429.598	405.640
31) L7 AR-1260-1	6.714	5.764	125.9E6	97668623	423.771	434.991
32) L7 AR-1260-2	7.000	5.973	146.0E6	113.3E6	422.039	429.474
33) L7 AR-1260-3	7.392	6.135	107.3E6	105.4E6	417.616	416.923
34) L7 AR-1260-4	7.637	6.653	120.1E6	82036579	424.867	415.836
35) L7 AR-1260-5	7.978	6.921	226.0E6	179.7E6	418.678	423.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 10:43
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:16:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

