
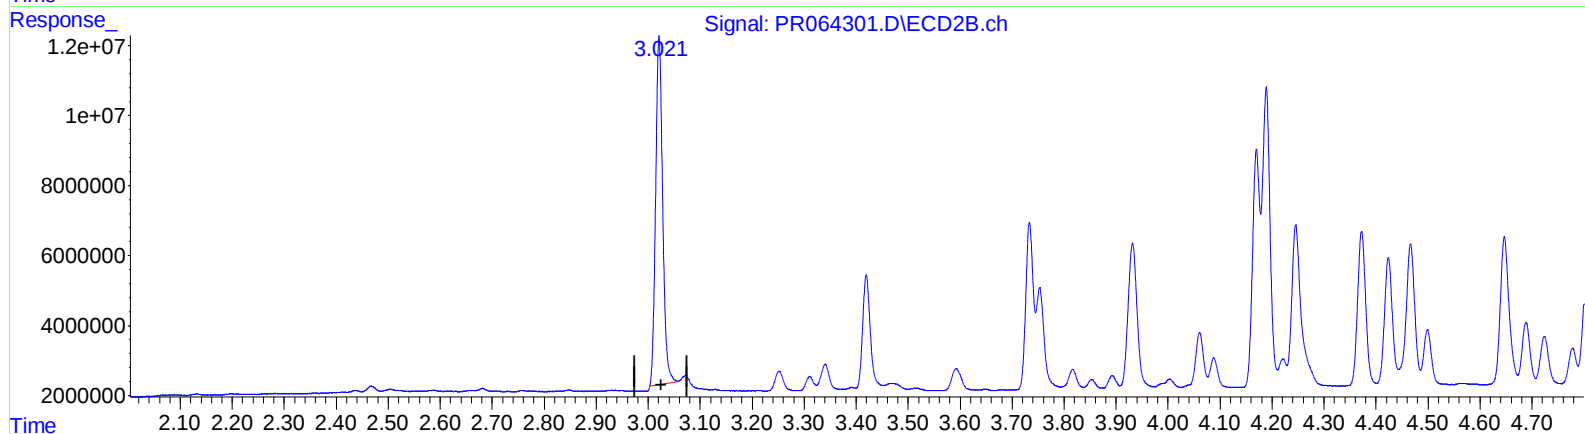


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 17:45
Operator : AJ\MA
Sample : 05104-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

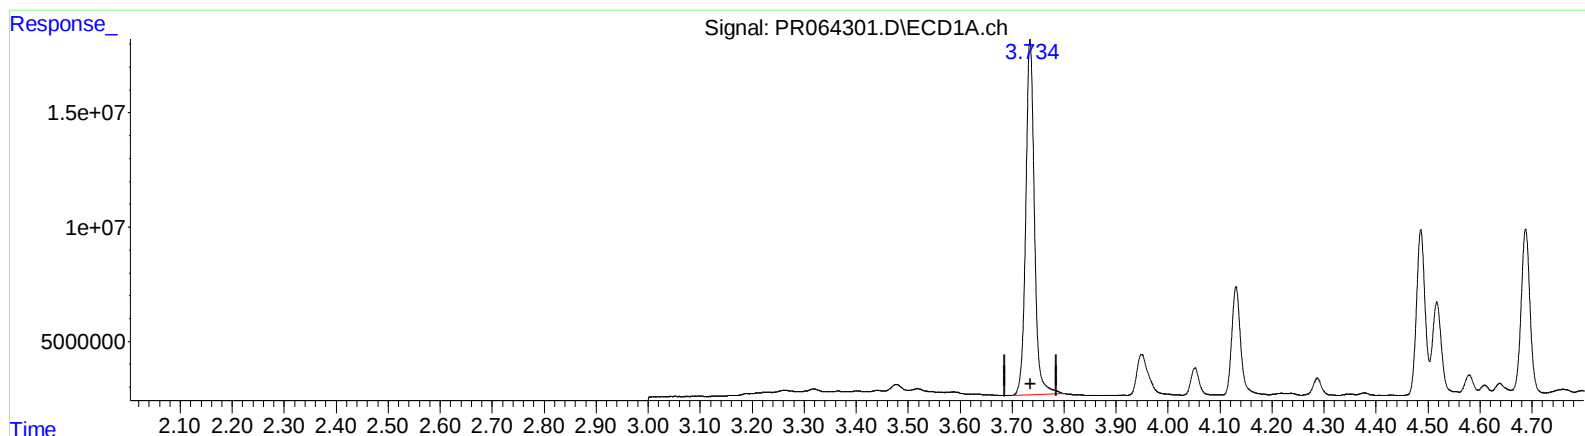

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 25.132 ng/ml

response 179993902

(1) Tetrachloro-m-xylene #2 (SA)

3.021min 22.616 ng/ml



response 93348092

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 17:45
Operator : AJ\MA
Sample : 05104-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

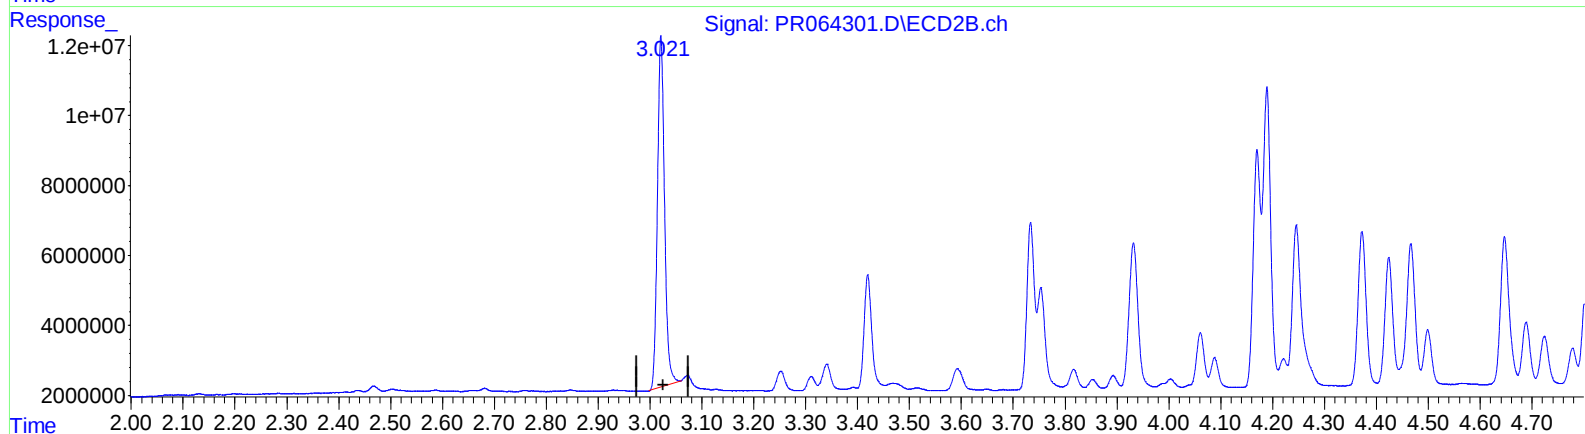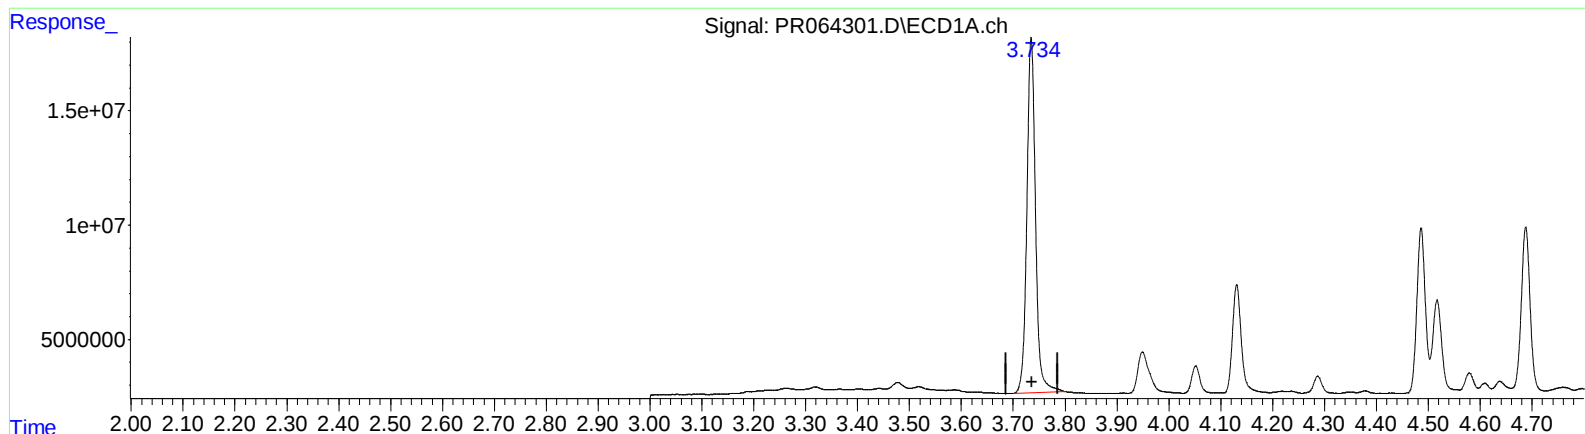

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 25.132 ng/ml

response 179993902

(1) Tetrachloro-m-xylene #2 (SA)

3.021min 23.068 ng/ml m



response 95211072

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 17:45
Operator : AJ\MA
Sample : 05104-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

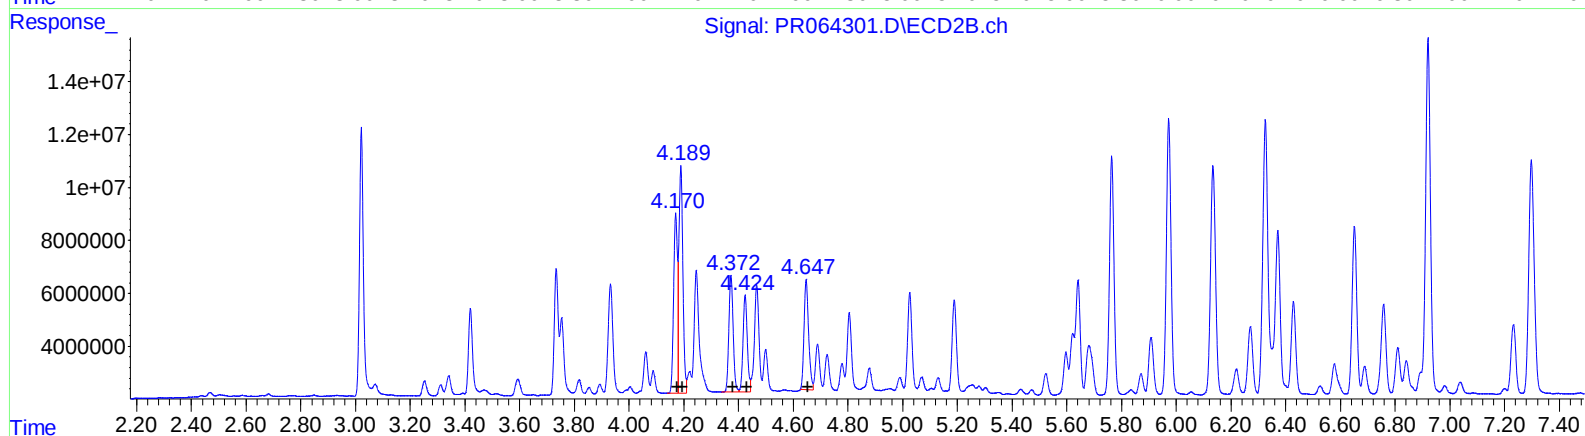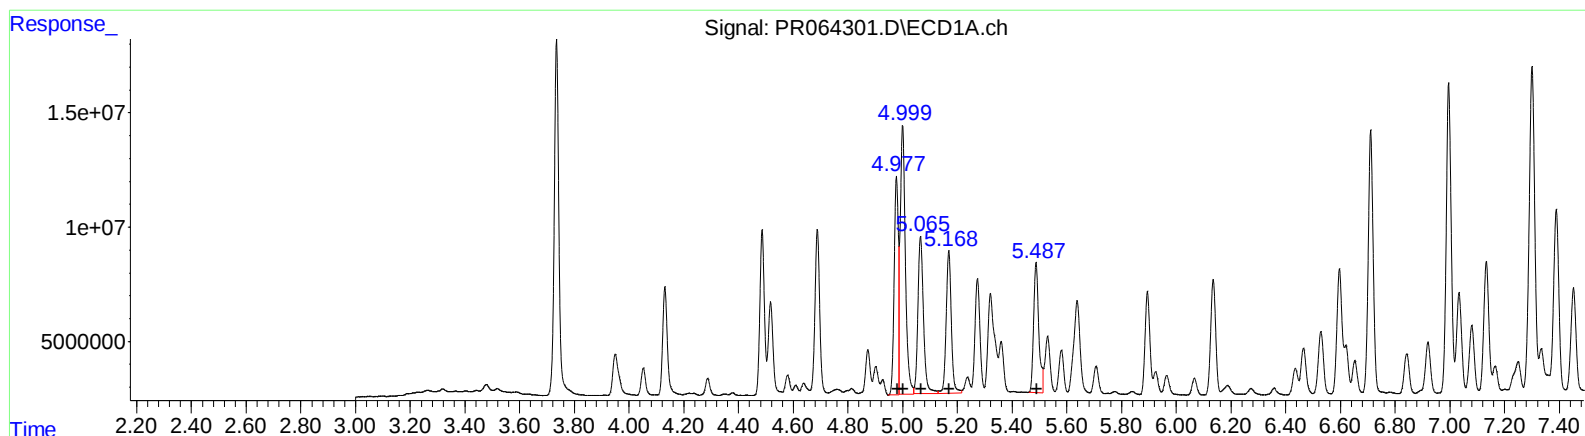

QEdit


(3) AR-1016-1 (L1)
R.T. Response Conc
4.98 103149874 479.52
5.00 153026254 467.02
5.06 98568298 476.48
5.17 81741721 501.84
5.49 75136108 462.22

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.17 63701436 438.21
4.19 88587324 443.15
4.37 48280767 437.96
4.42 39576035 457.33
4.65 48268068 422.49

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 17:45
Operator : AJ\MA
Sample : 05104-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

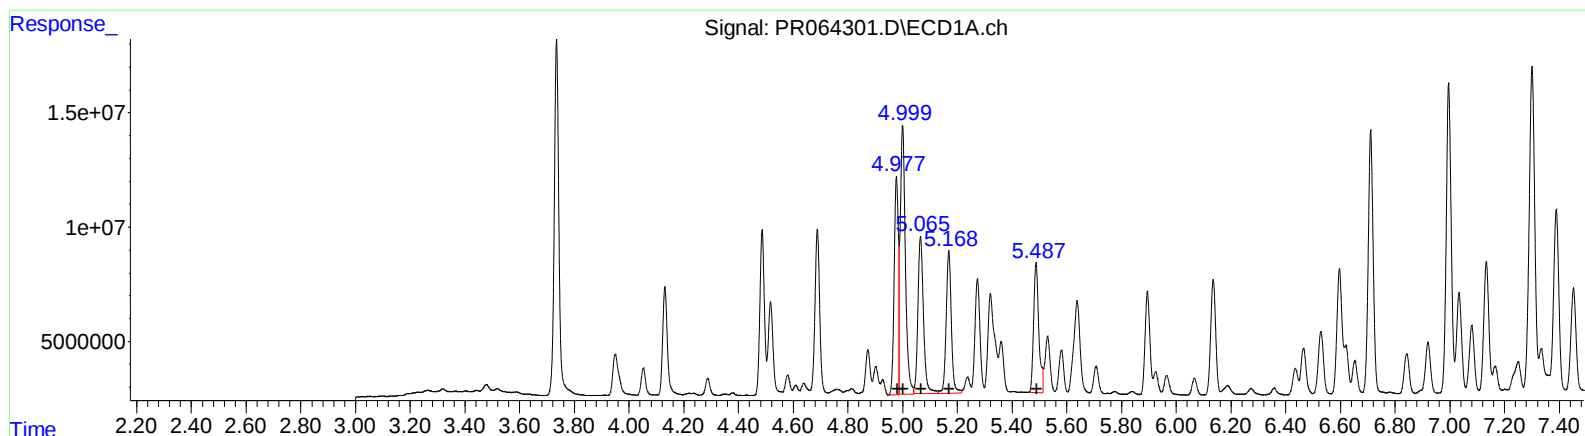

(3) AR-1016-1 (L1)
R.T. Response Conc
4.98 103149874 479.52
5.00 153026254 467.02
5.06 98568298 476.48
5.17 81741721 501.84
5.49 75136108 462.22

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.17 63701436 438.21
4.19 88587324 443.15
4.37 48280767 437.96
4.42 39576035 457.33
4.65 49345006 431.91

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
 Data File : PR064301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 17:45
 Operator : AJ\MA
 Sample : 05104-02MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:39:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 13 05:04:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.735	3.021	180.0E6	95211072	25.132	23.068m
2) SA Decachlor...	9.755	8.412	146.0E6	85255400	31.245	28.087
Target Compounds						
3) L1 AR-1016-1	4.977	4.170	103.1E6	63701436	479.518	438.205
4) L1 AR-1016-2	5.000	4.189	153.0E6	88587324	467.023	443.146
5) L1 AR-1016-3	5.065	4.372	98568298	48280767	476.479	437.956
6) L1 AR-1016-4	5.169	4.424	81741721	39576035	501.839	457.326
7) L1 AR-1016-5	5.488	4.647	75136108	49345006	462.220	431.915m
31) L7 AR-1260-1	6.711	5.764	142.3E6	103.5E6	478.785	460.777
32) L7 AR-1260-2	6.996	5.972	171.1E6	123.4E6	494.682	467.771
33) L7 AR-1260-3	7.389	6.134	107.9E6	112.2E6	419.873	443.699
34) L7 AR-1260-4	7.634	6.651	134.4E6	75473933	475.719	382.570
35) L7 AR-1260-5	7.974	6.920	244.8E6	172.5E6	453.482	406.257

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 17:45
Operator : AJ\MA
Sample : 05104-02MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:39:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

