
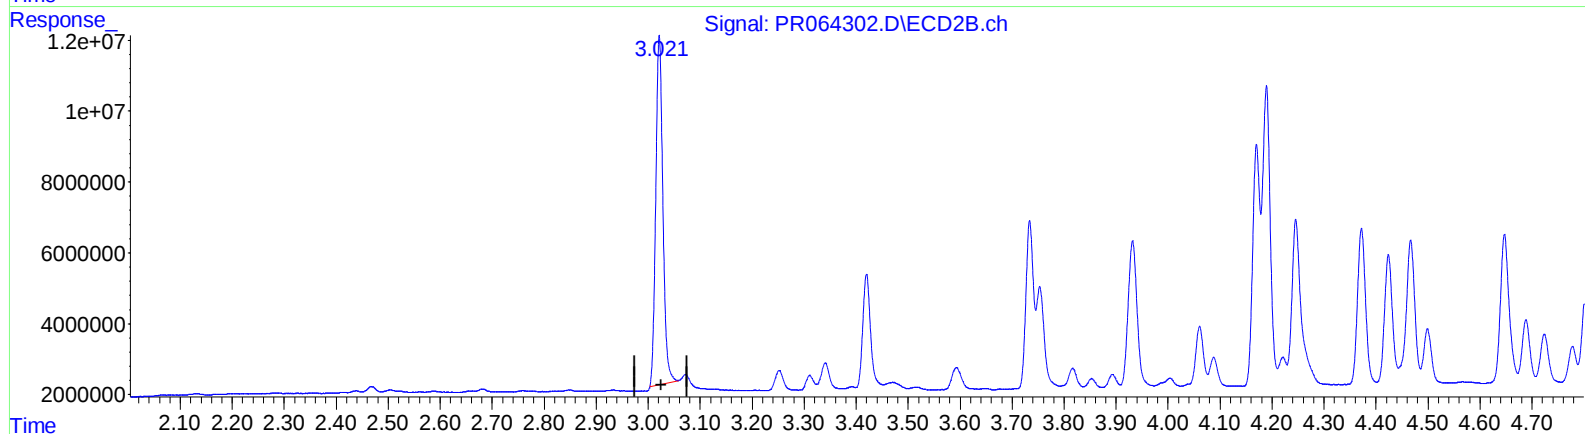


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 18:00
Operator : AJ\MA
Sample : 05104-03MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

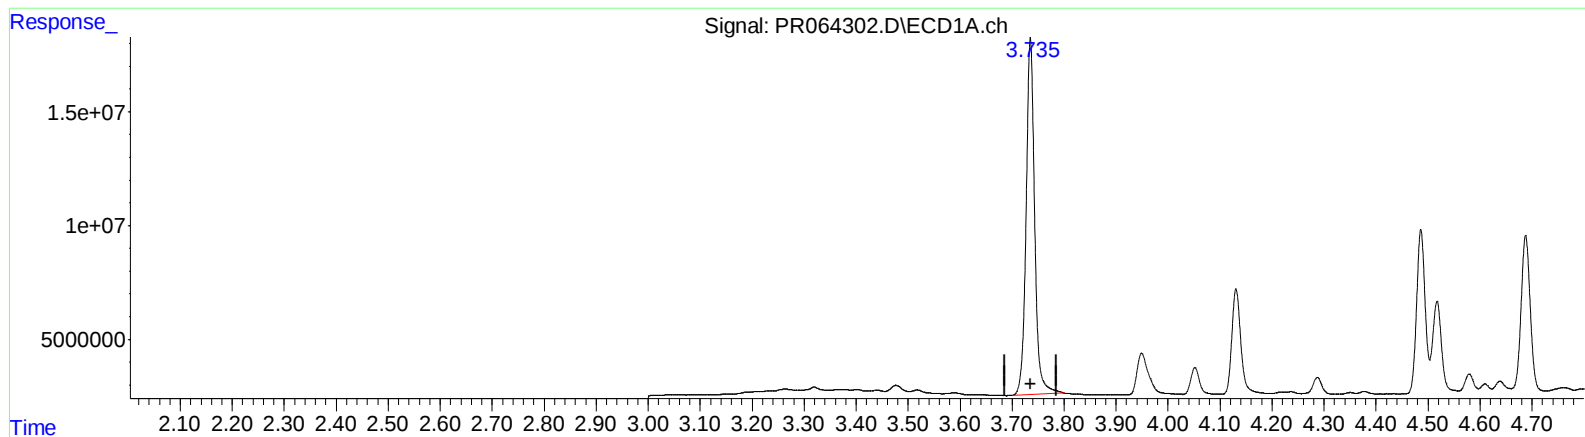

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 24.919 ng/ml

response 178472115

(1) Tetrachloro-m-xylene #2 (SA)

3.022min 22.624 ng/ml



response 93379463

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 18:00
Operator : AJ\MA
Sample : 05104-03MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

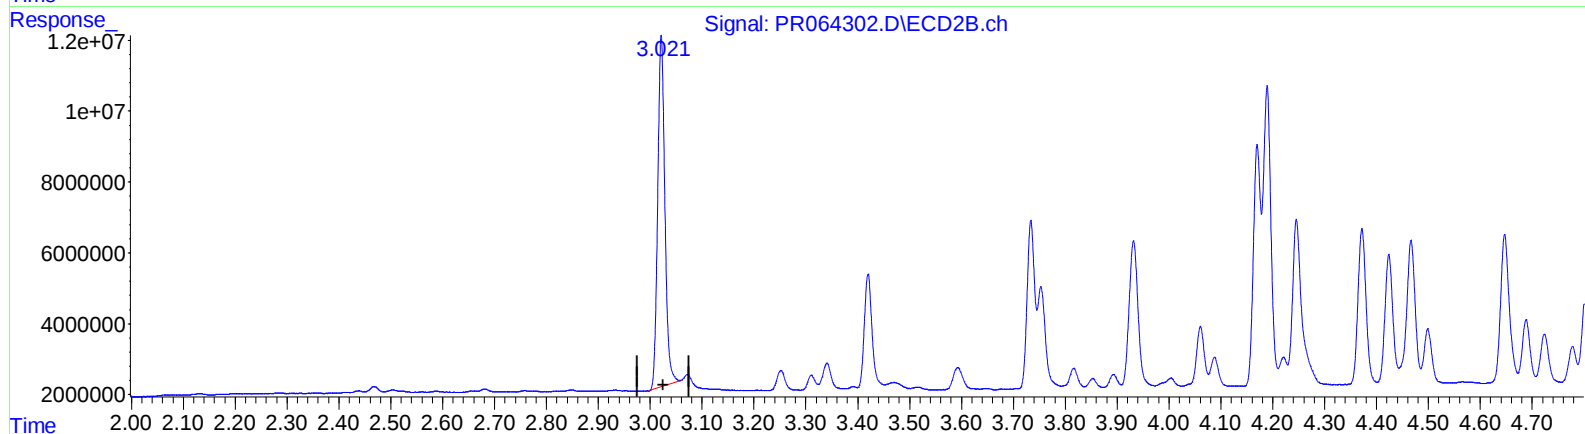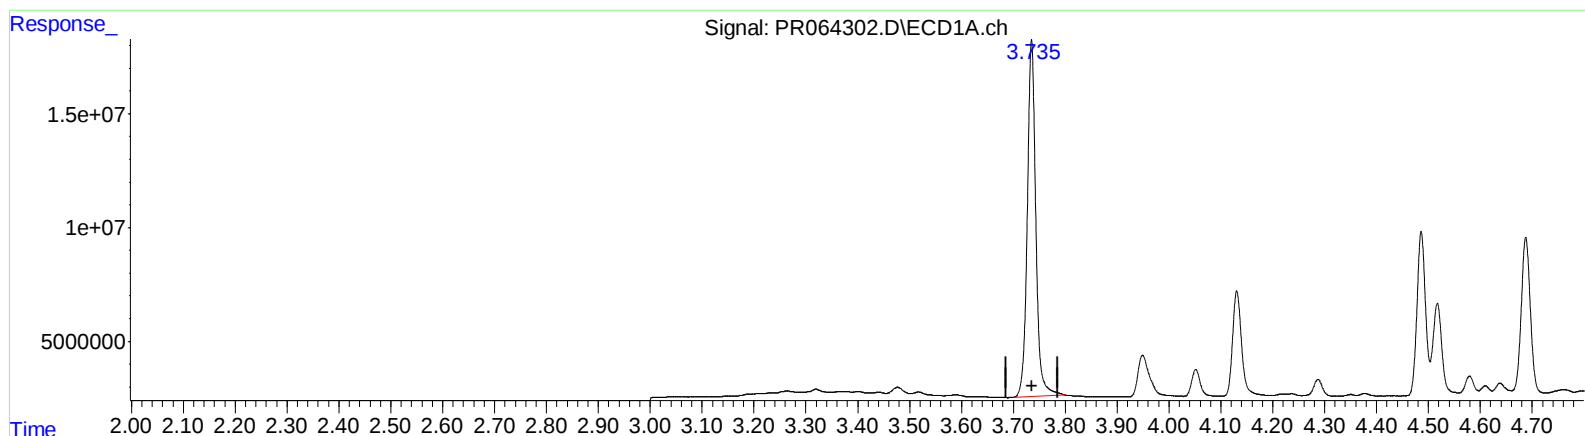

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 24.919 ng/ml

response 178472115

(1) Tetrachloro-m-xylene #2 (SA)

3.021min 23.055 ng/ml m



response 95156395

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 18:00
Operator : AJ\MA
Sample : 05104-03MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

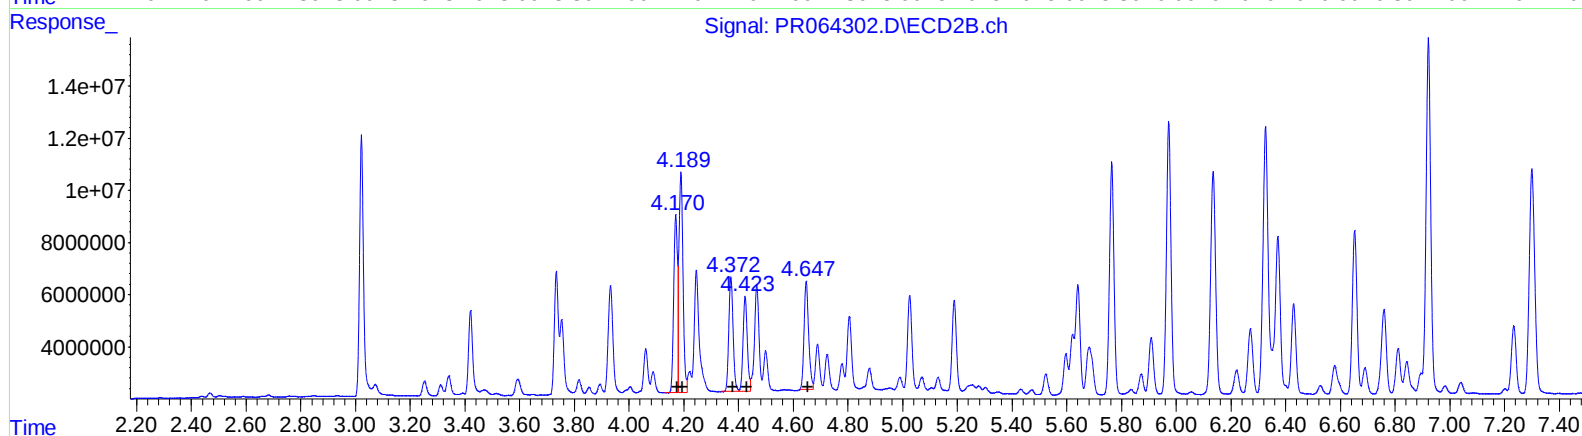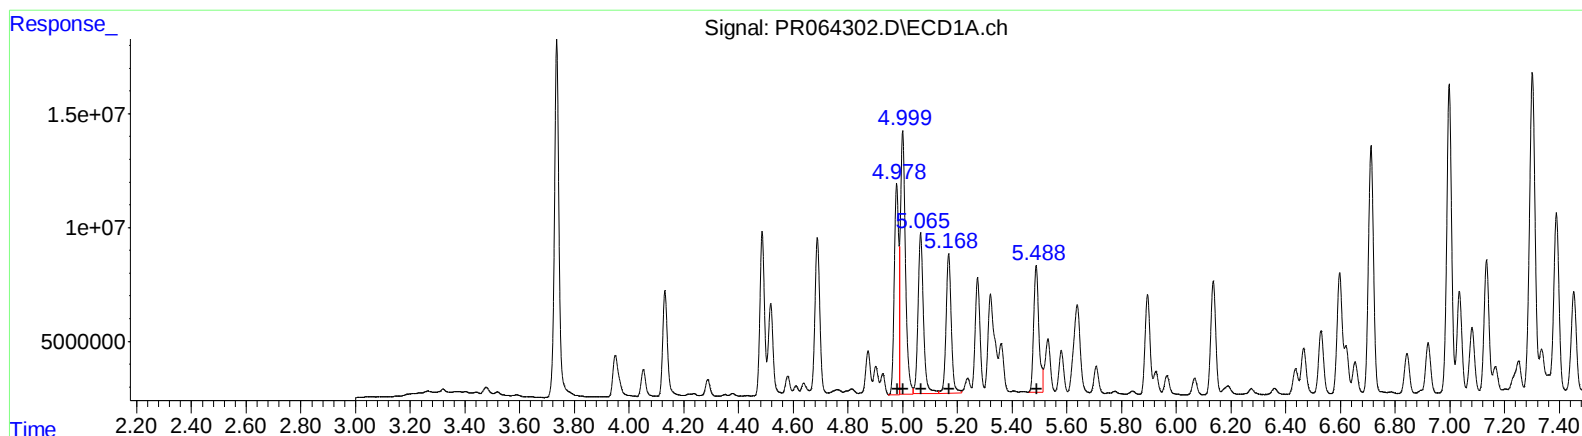

QEdit



(3) AR-1016-1 (L1)
R.T. Response Conc
4.98 101450070 471.62
5.00 149977369 457.72
5.07 97179010 469.76
5.17 79869010 490.34
5.49 73679927 453.26

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.17 63611701 437.59
4.19 87940770 439.91
4.37 47781321 433.43
4.42 39252923 453.59
4.65 47964524 419.83

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 18:00
Operator : AJ\MA
Sample : 05104-03MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

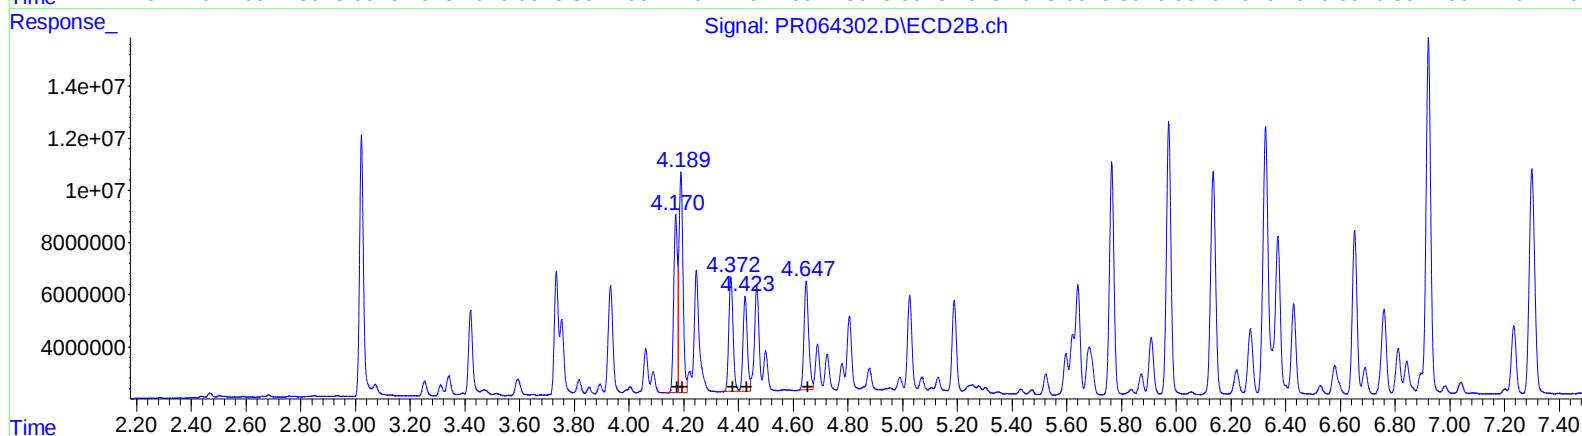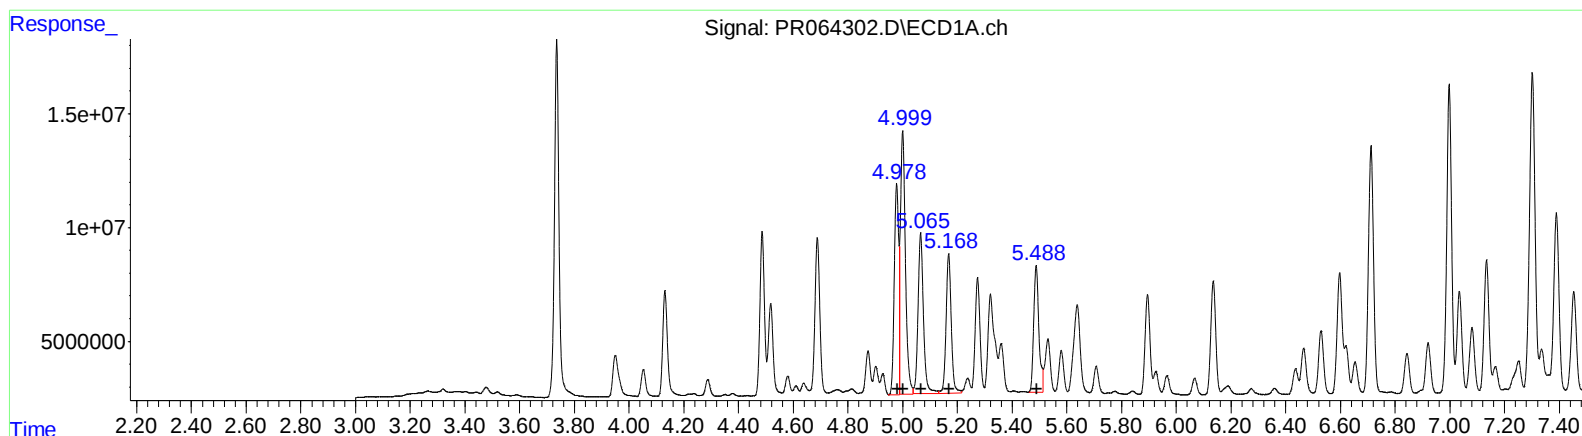

QEdit

(3) AR-1016-1 (L1)
R.T. Response Conc
4.98 101450070 471.62
5.00 149977369 457.72
5.07 97179010 469.76
5.17 79869010 490.34
5.49 73679927 453.26

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.17 63611701 437.59
4.19 87940770 439.91
4.37 47781321 433.43
4.42 39252923 453.59
4.65 48734093 426.57

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
 Data File : PR064302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 18:00
 Operator : AJ\MA
 Sample : 05104-03MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 03:36:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 13 05:04:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.735	3.021	178.5E6	95156395	24.919	23.055m
2) SA Decachlor...	9.756	8.414	142.9E6	83497194	30.590	27.508
Target Compounds						
3) L1 AR-1016-1	4.978	4.170	101.5E6	63611701	471.617	437.588
4) L1 AR-1016-2	5.000	4.189	150.0E6	87940770	457.718	439.912
5) L1 AR-1016-3	5.065	4.372	97179010	47781321	469.763	433.425
6) L1 AR-1016-4	5.168	4.424	79869010	39252923	490.342	453.592
7) L1 AR-1016-5	5.488	4.647	73679927	48734093	453.262	426.567m
31) L7 AR-1260-1	6.712	5.764	140.0E6	102.0E6	470.931	454.410
32) L7 AR-1260-2	6.998	5.972	168.1E6	121.1E6	486.003	459.319
33) L7 AR-1260-3	7.390	6.135	109.1E6	109.9E6	424.562	434.619
34) L7 AR-1260-4	7.634	6.652	133.2E6	74194934	471.347	376.087
35) L7 AR-1260-5	7.974	6.922	241.9E6	169.2E6	448.070	398.561

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 18:00
Operator : AJ\MA
Sample : 05104-03MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

