
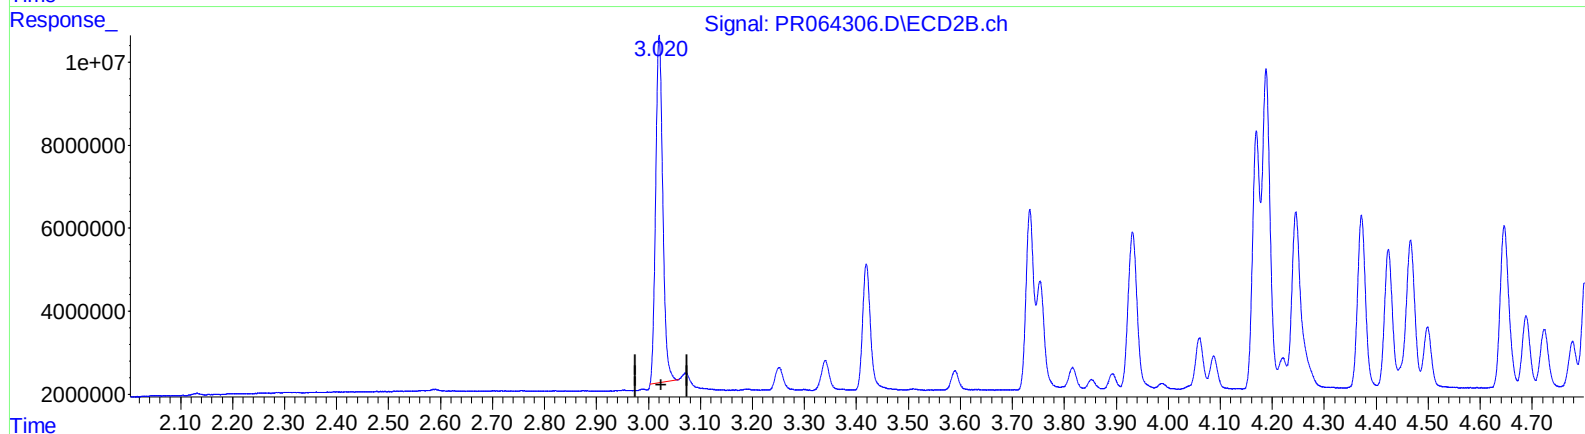


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 19:28
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:40:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

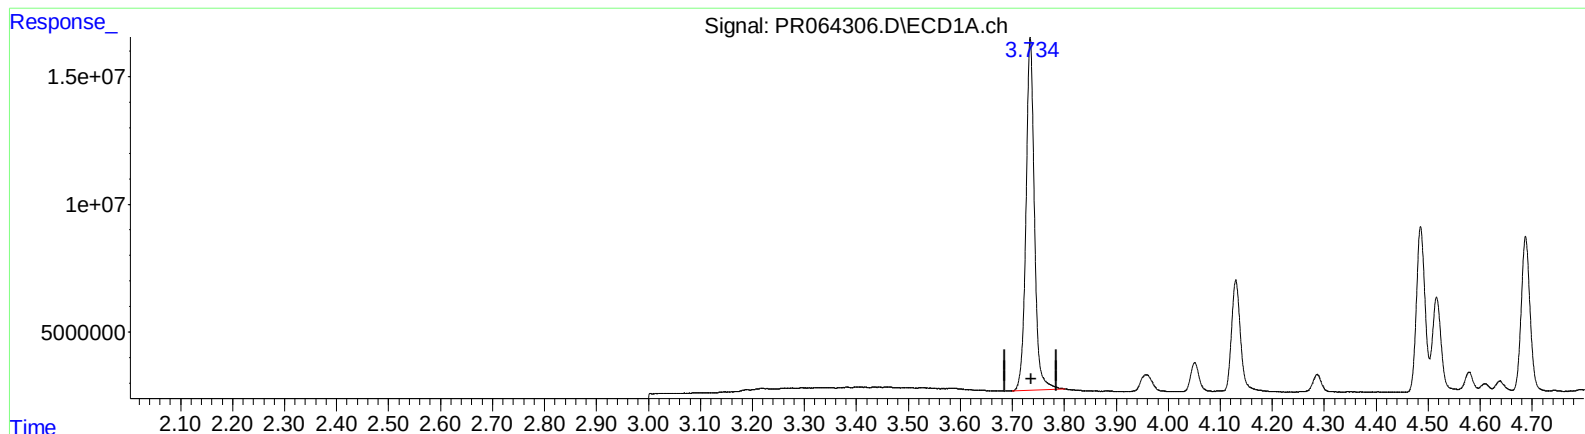

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 21.805 ng/ml

response 156169713

(1) Tetrachloro-m-xylene #2 (SA)



3.021min 19.336 ng/ml

response 79809895

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 19:28
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:40:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

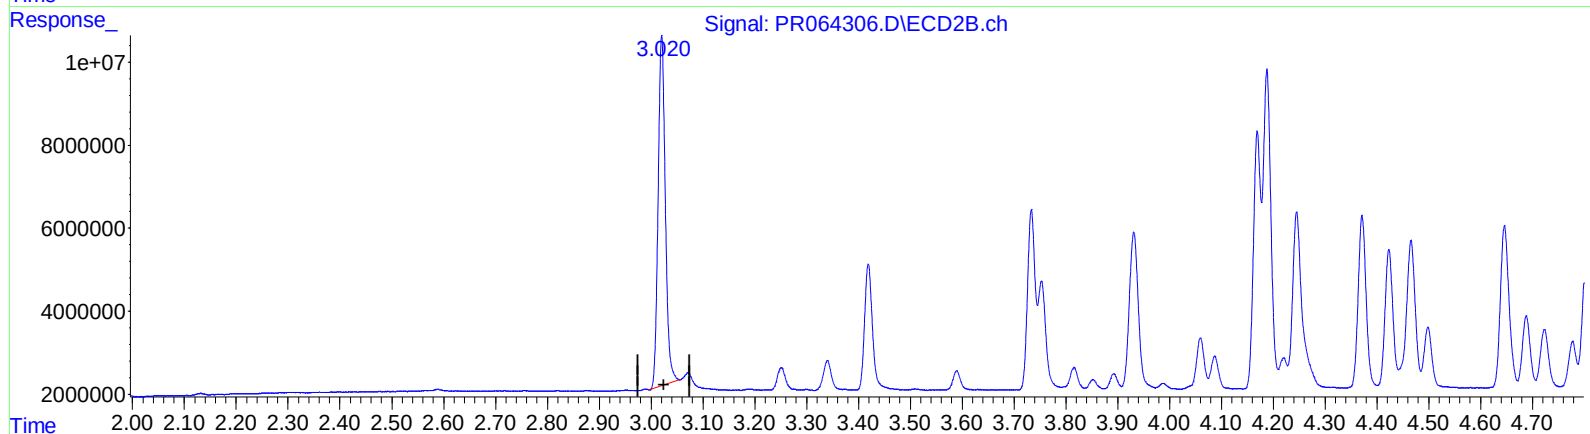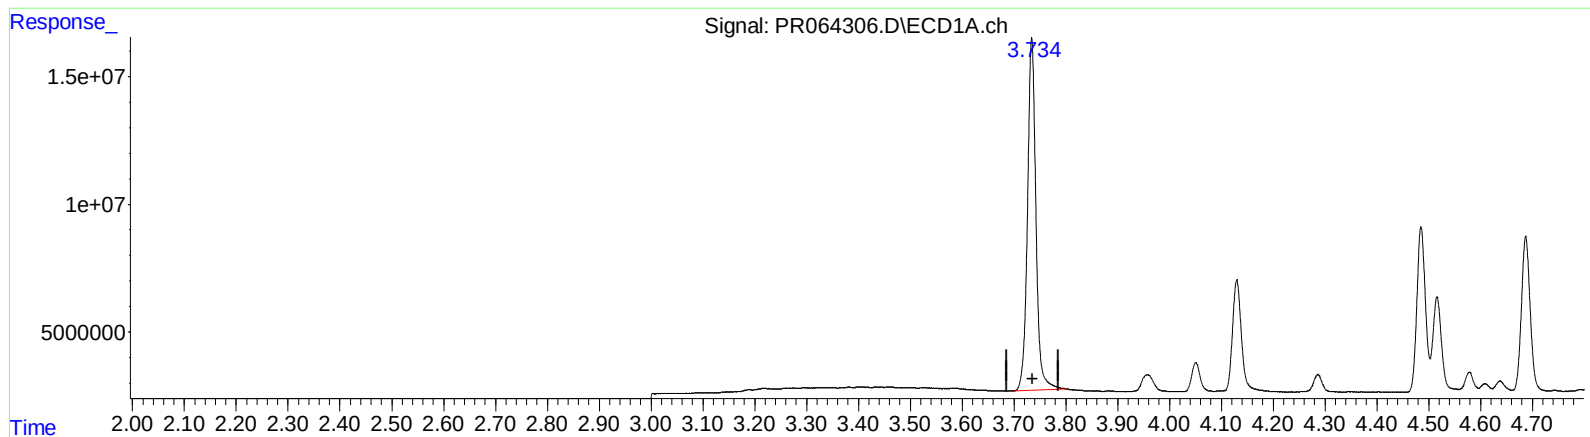

QEdit

(1) Tetrachloro-m-xylene (SA)

3.735min 21.805 ng/ml

response 156169713

(1) Tetrachloro-m-xylene #2 (SA)

3.020min 19.716 ng/ml m

response 81376998

(+) = Expected Retention Time

PR101223CLP.M Wed Nov 01 07:00:03 2023

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
 Data File : PR064306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2023 19:28
 Operator : AJ\MA
 Sample : AR1660CCC400
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 21:40:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 13 05:04:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.735	3.020	156.2E6	81376998	21.805	19.716m
2) SA Decachlor...	9.754	8.413	200.6E6	125.8E6	42.942	41.451
Target Compounds						
3) L1 AR-1016-1	4.977	4.170	91218265	57748233	424.051	397.253
4) L1 AR-1016-2	4.999	4.188	135.1E6	80541899	412.305	402.900
5) L1 AR-1016-3	5.064	4.372	85867581	44536125	415.083	403.988
6) L1 AR-1016-4	5.168	4.424	68507076	35739837	420.587	412.996
7) L1 AR-1016-5	5.487	4.646	68825882	44884075	423.401	392.868
31) L7 AR-1260-1	6.710	5.763	121.5E6	94153808	408.794	419.337
32) L7 AR-1260-2	6.996	5.972	141.9E6	108.2E6	410.380	410.477
33) L7 AR-1260-3	7.390	6.134	103.9E6	100.9E6	404.404	398.920
34) L7 AR-1260-4	7.633	6.651	114.7E6	77629616	405.739	393.497
35) L7 AR-1260-5	7.973	6.921	222.6E6	170.8E6	412.269	402.129

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR103023\
Data File : PR064306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2023 19:28
Operator : AJ\MA
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 21:40:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR101223CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 13 05:04:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

