

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110420\
 Data File : PR048545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 17:34
 Operator : DD\AJ
 Sample : PB132807BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 02:55:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.723	3.877	47353111	56231422	19.344	19.366
2)	SA Decachlor...	10.653	8.985	49029763	229.6E6	18.609	15.718
Target Compounds							
8)	L2 AR-1221-1	4.943	0.000	869092	0	32.381	N.D. #
9)	L2 AR-1221-2	5.035	4.172	546885	2707848	27.548	123.535 #
28)	L6 AR-1254-3	7.367f	0.000	986712	0	7.055	N.D. #
32)	L7 AR-1260-2	0.000	6.632f	0	1987012	N.D.	3.037 #
33)	L7 AR-1260-3	0.000	6.811	0	3742207	N.D.	8.760 #
34)	L7 AR-1260-4	8.379	0.000	2571822	0	20.701	N.D. #
43)	L9 AR-1268-3	0.000	8.096	0	15896815	N.D.	8.108 #
45)	L9 AR-1268-5	0.000	8.710	0	10740740	N.D.	1.903 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110420\
Data File : PR048545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 17:34
Operator : DD\AJ
Sample : PB132807BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 02:55:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

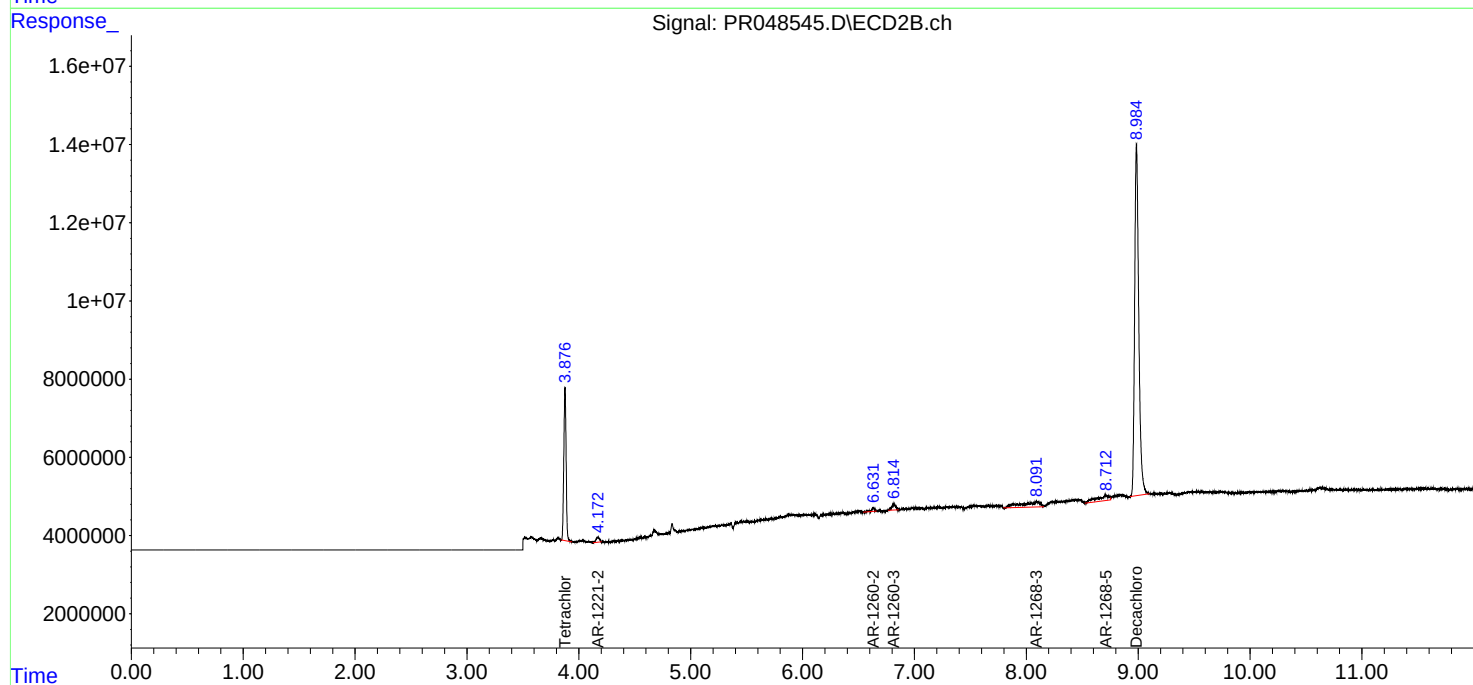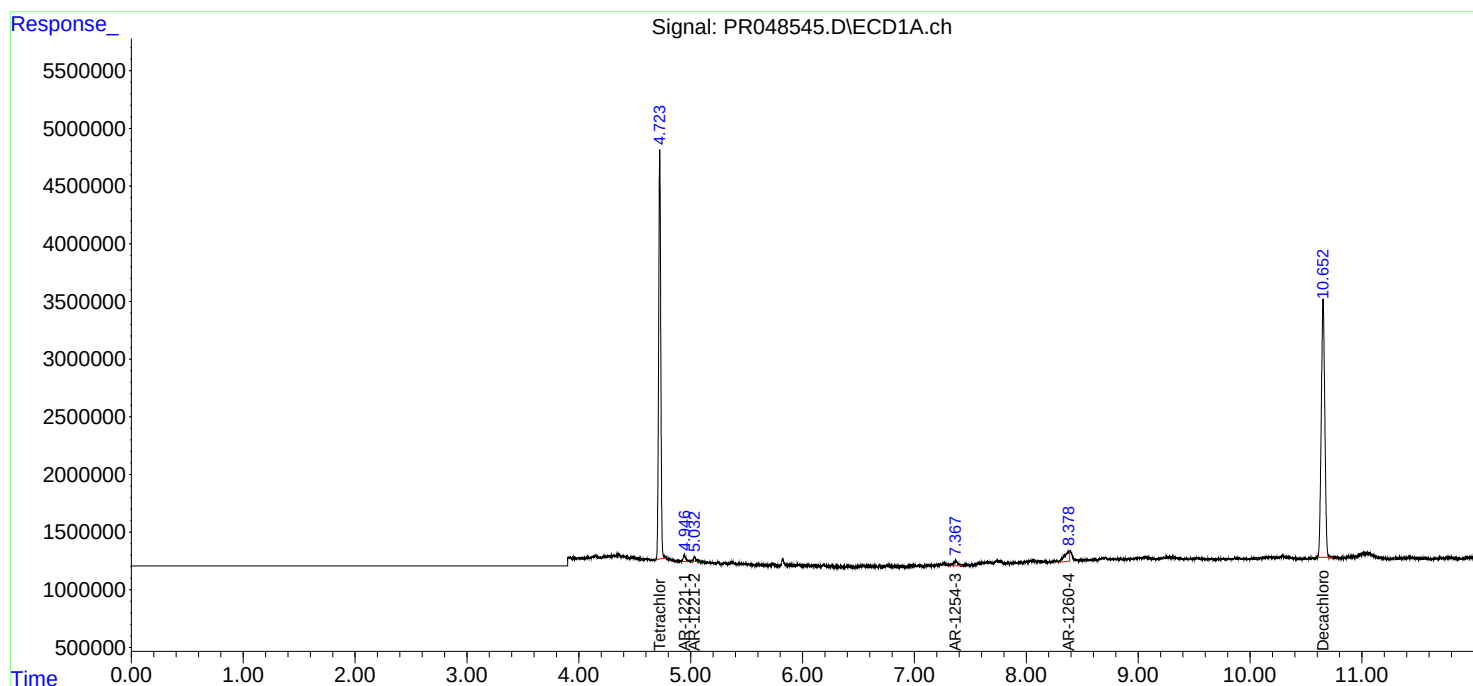


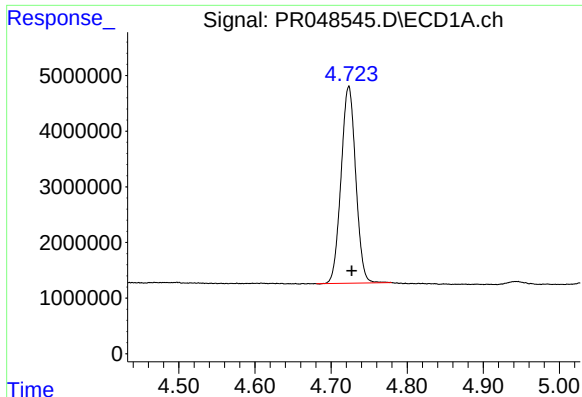

#1 Tetrachloro-m-xylene


R.T.: 4.723 min
Delta R.T.: -0.004 min
Response: 47353111
Conc: 19.34 ng/ml

Instrument :
ECD_R
ClientSampleId :

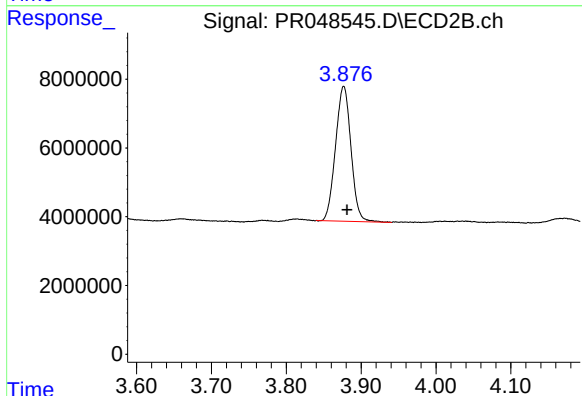


#1 Tetrachloro-m-xylene

R.T.: 3.877 min
Delta R.T.: -0.005 min
Response: 56231422
Conc: 19.37 ng/ml

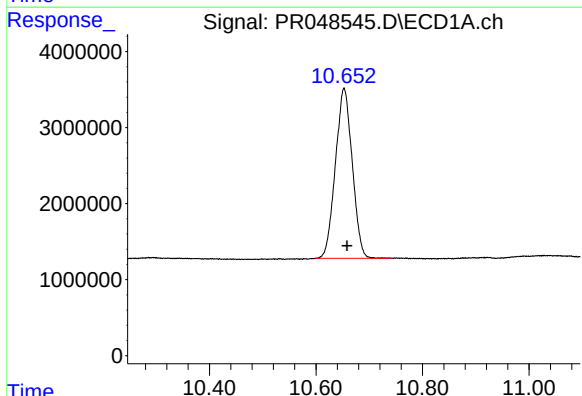


#2 Decachlorobiphenyl

R.T.: 10.653 min
Delta R.T.: -0.006 min
Response: 49029763
Conc: 18.61 ng/ml

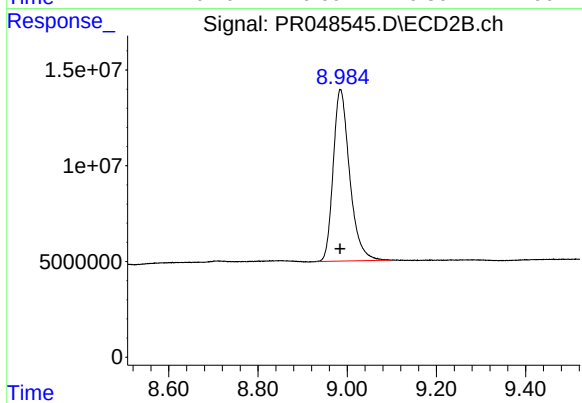

#2 Decachlorobiphenyl


R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 229574787
Conc: 15.72 ng/ml

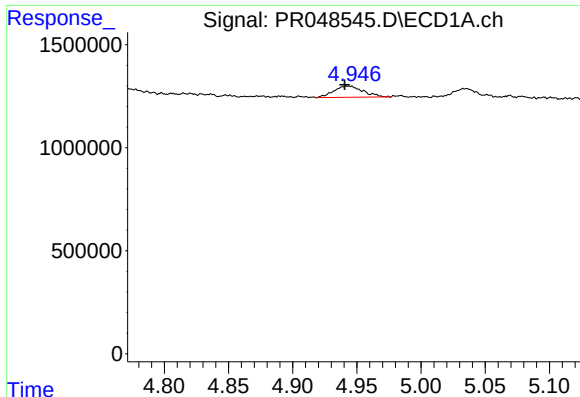

#8 AR-1221-1


R.T.: 4.943 min
Delta R.T.: 0.003 min
Response: 869092
Conc: 32.38 ng/ml

Instrument :
ECD_R
ClientSampleId :

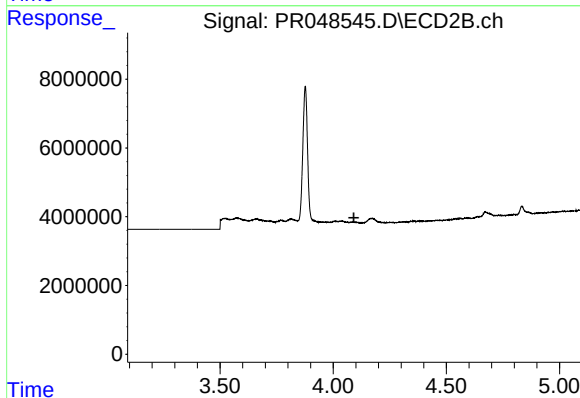


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.091 min
Response: 0
Conc: N.D.

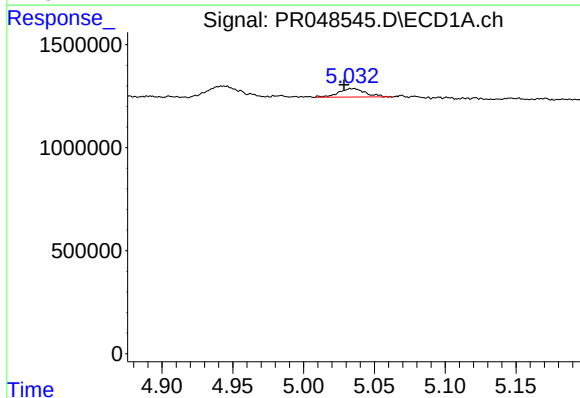


#9 AR-1221-2

R.T.: 5.035 min
Delta R.T.: 0.006 min
Response: 546885
Conc: 27.55 ng/ml

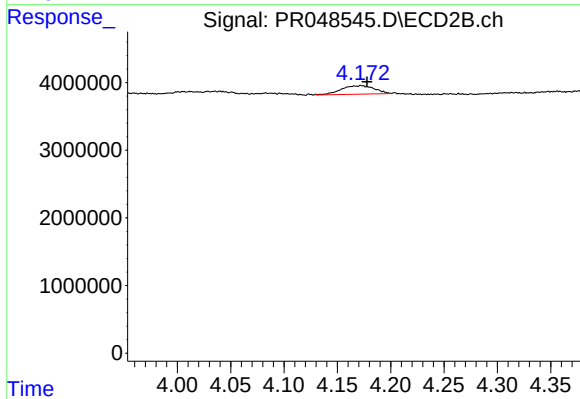

#9 AR-1221-2


R.T.: 4.172 min
Delta R.T.: -0.006 min
Response: 2707848
Conc: 123.54 ng/ml

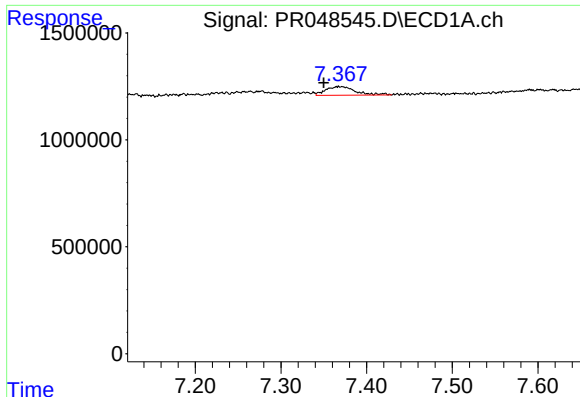

#28 AR-1254-3


R.T.: 7.367 min
Delta R.T.: 0.017 min
Response: 986712
Conc: 7.05 ng/ml

Instrument :
ECD_R
ClientSampleId :

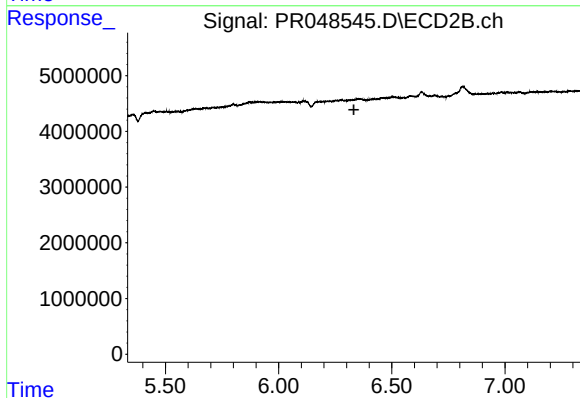


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

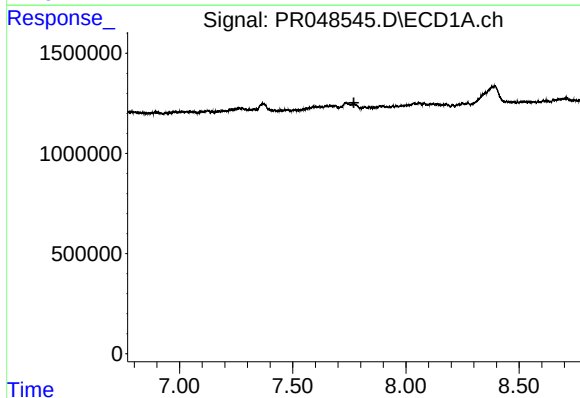


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.770 min
Response: 0
Conc: N.D.

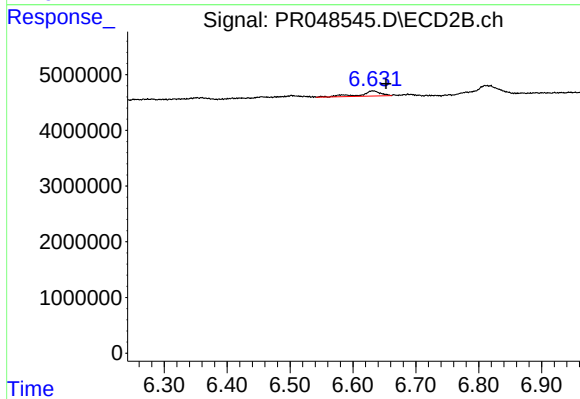

#32 AR-1260-2


R.T.: 6.632 min
Delta R.T.: -0.021 min
Response: 1987012
Conc: 3.04 ng/ml

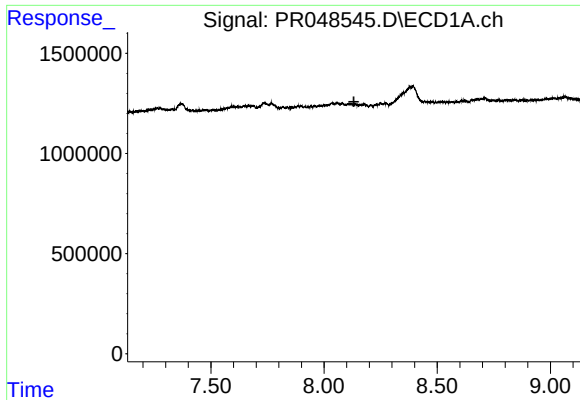

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

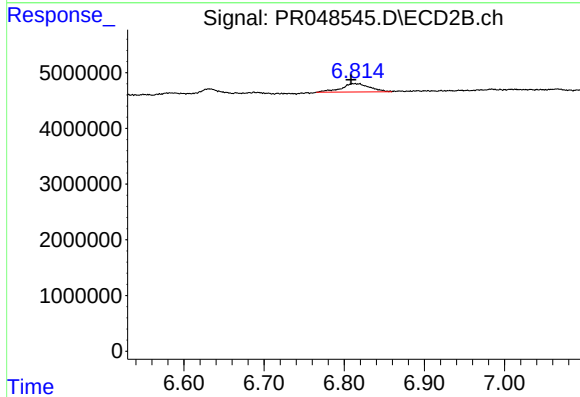


#33 AR-1260-3

R.T.: 6.811 min
Delta R.T.: 0.002 min
Response: 3742207
Conc: 8.76 ng/ml

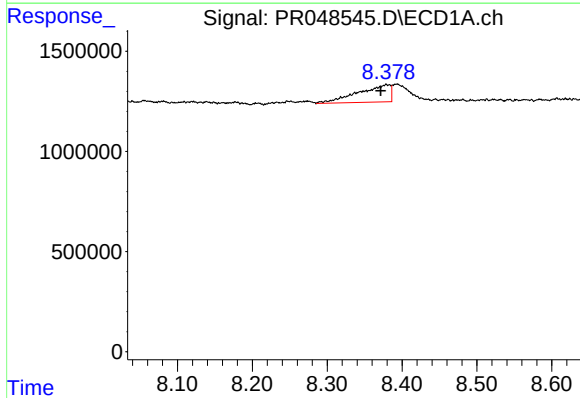


#34 AR-1260-4

R.T.: 8.379 min
Delta R.T.: 0.008 min
Response: 2571822
Conc: 20.70 ng/ml

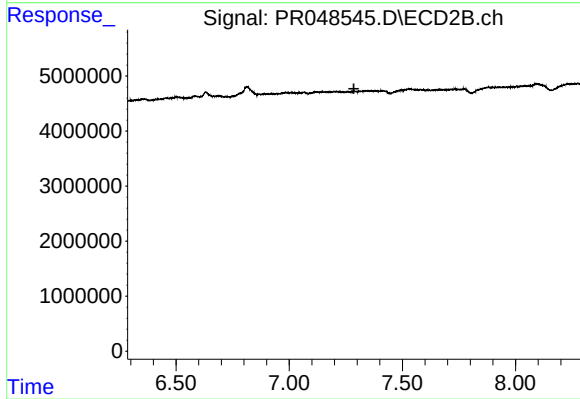

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.286 min
Response: 0
Conc: N.D.

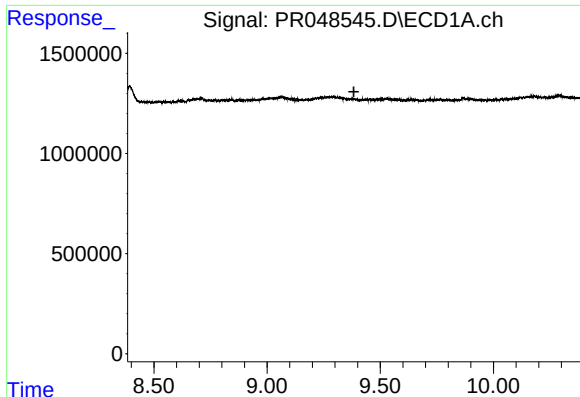

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

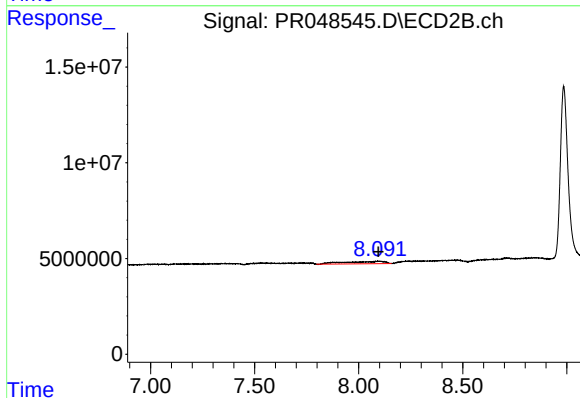


#43 AR-1268-3

R.T.: 8.096 min
Delta R.T.: 0.000 min
Response: 15896815
Conc: 8.11 ng/ml

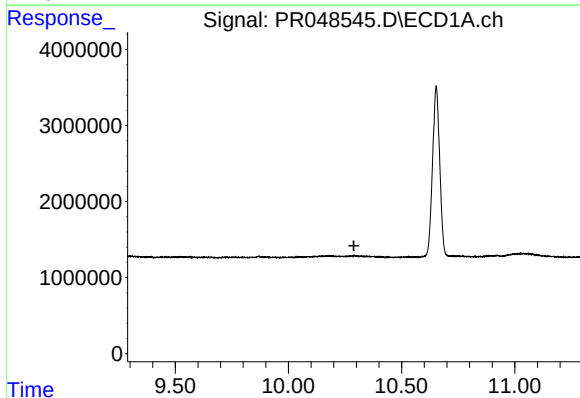

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.289 min
Response: 0
Conc: N.D.

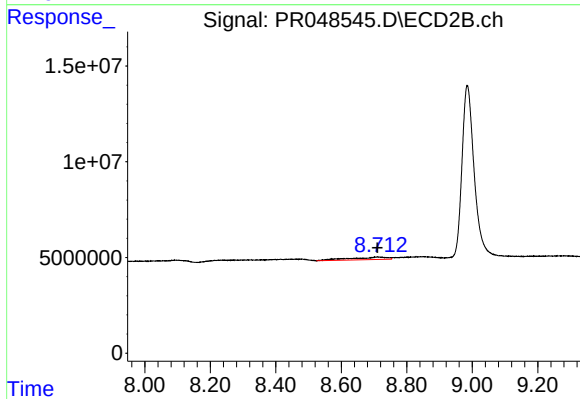

#45 AR-1268-5

R.T.: 8.710 min
Delta R.T.: 0.000 min
Response: 10740740
Conc: 1.90 ng/ml