

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110619\
 Data File : PR042845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2019 11:11
 Operator : SM\AJ
 Sample : K5658-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-30-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 12:00:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 01 09:55:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.711	3.972	90003604	336.5E6	15.269	16.783
2)	SA Decachlor...	10.623	9.070	67271462	176.3E6	16.810	14.032
Target Compounds							
9)	L2 AR-1221-2	5.022	4.277	1048491	4141636	28.186	31.317
10)	L2 AR-1221-3	5.022	0.000	1048491	0	9.077	N.D. #
11)	L3 AR-1232-1	5.022	0.000	1048491	0	6.562	N.D. #
20)	L4 AR-1242-5	6.747	0.000	2695408	0	26.964	N.D. #
24)	L5 AR-1248-4	6.747	0.000	2695408	0	15.785	N.D. #
25)	L5 AR-1248-5	6.747	0.000	2695408	0	16.621	N.D. #
26)	L6 AR-1254-1	6.747	0.000	2695408	0	14.440	N.D. #
34)	L7 AR-1260-4	8.303	0.000	20935393	0	100.317	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110619\
Data File : PR042845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2019 11:11
Operator : SM\AJ
Sample : K5658-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
TP-30-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 12:00:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 01 09:55:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

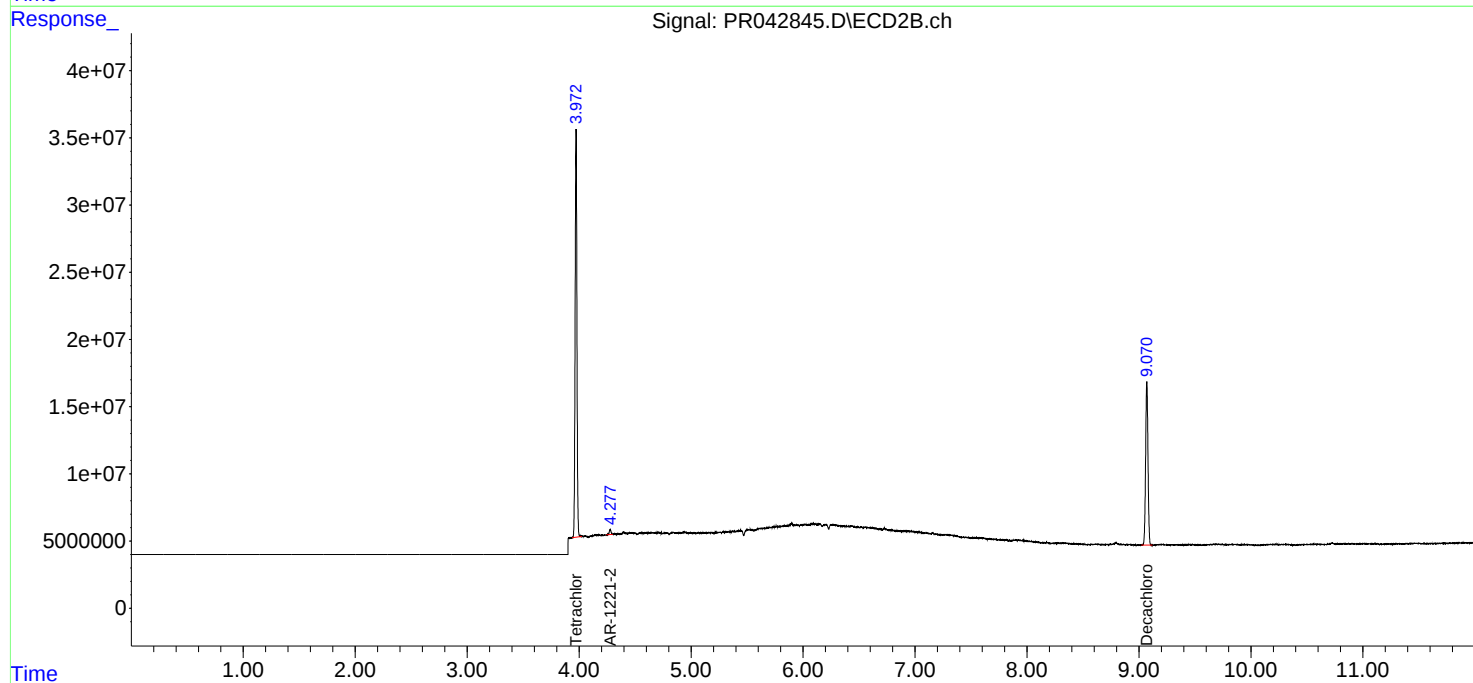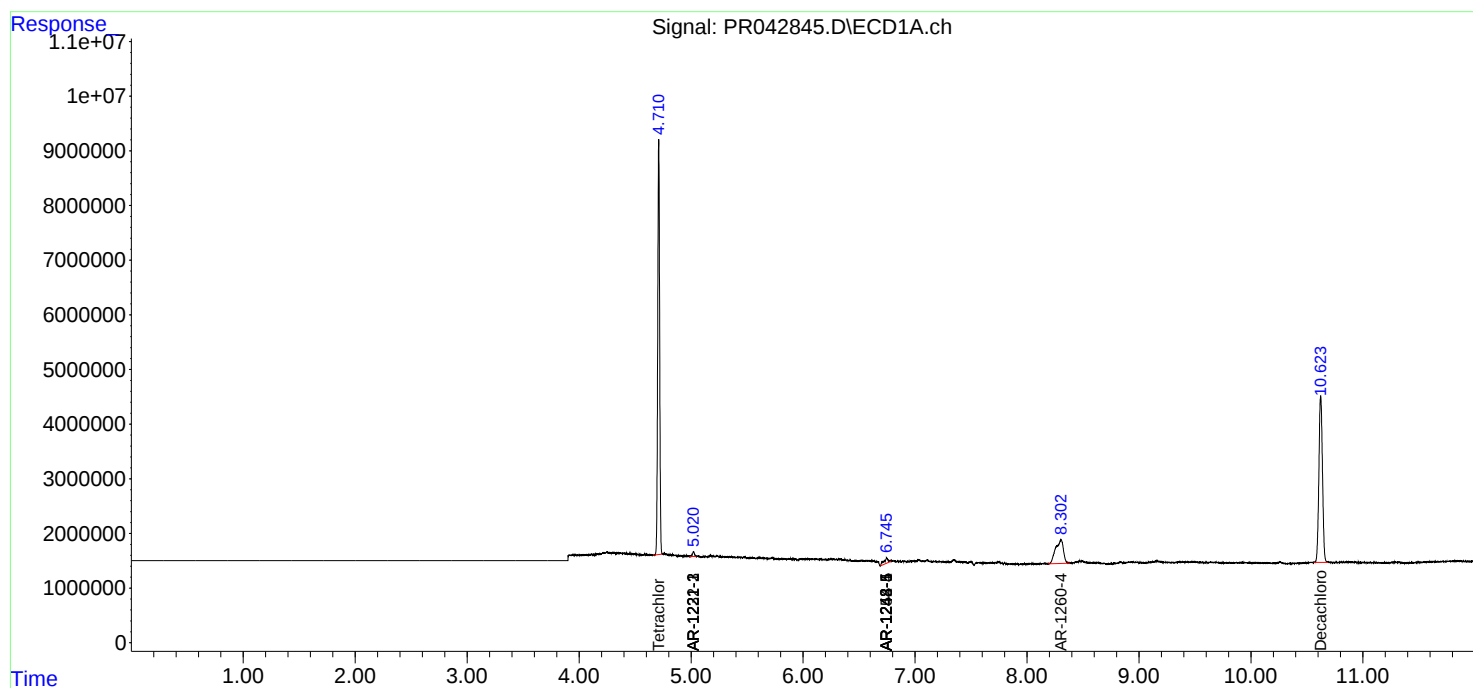


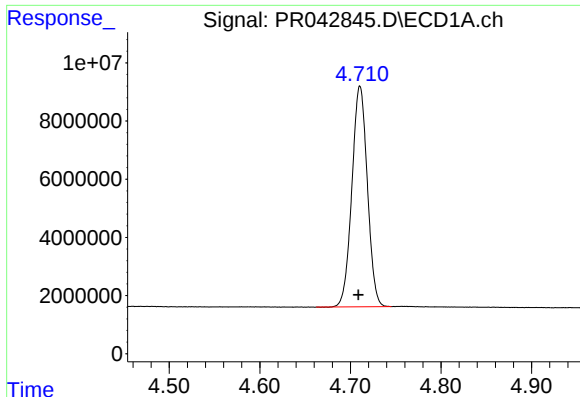

#1 Tetrachloro-m-xylene


R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 90003604
Conc: 15.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-30-D

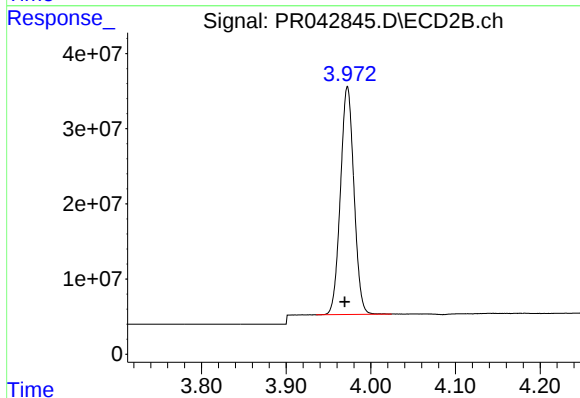


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.003 min
Response: 336523155
Conc: 16.78 ng/ml

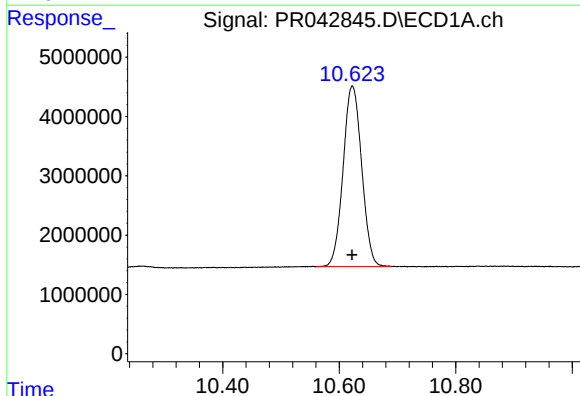


#2 Decachlorobiphenyl

R.T.: 10.623 min
Delta R.T.: 0.000 min
Response: 67271462
Conc: 16.81 ng/ml

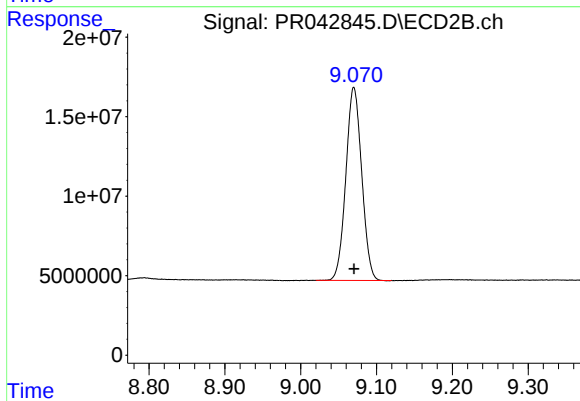

#2 Decachlorobiphenyl


R.T.: 9.070 min
Delta R.T.: 0.000 min
Response: 176320263
Conc: 14.03 ng/ml

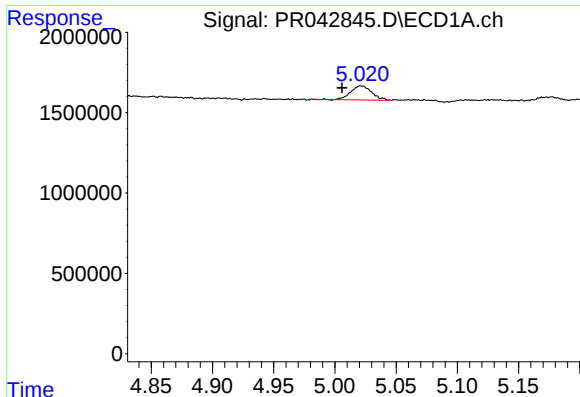

#9 AR-1221-2


R.T.: 5.022 min
Delta R.T.: 0.016 min
Response: 1048491
Conc: 28.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-30-D

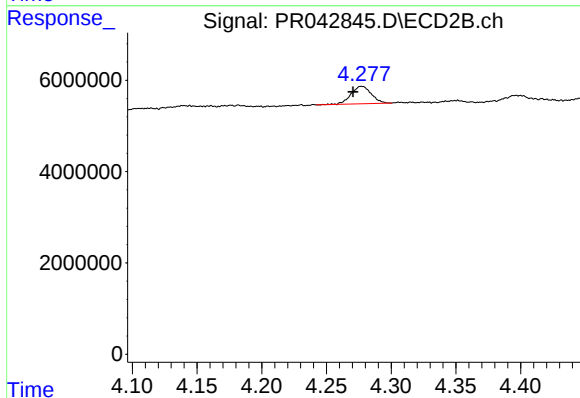


#9 AR-1221-2

R.T.: 4.277 min
Delta R.T.: 0.007 min
Response: 4141636
Conc: 31.32 ng/ml

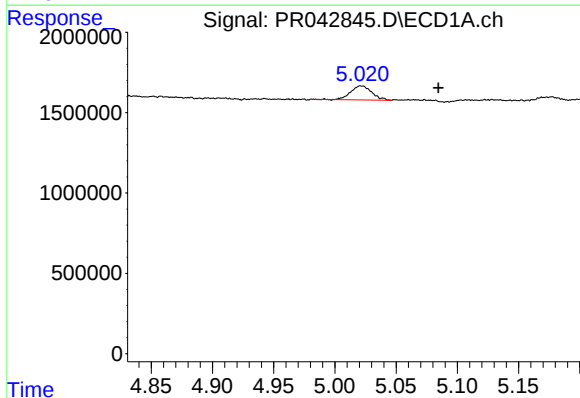


#10 AR-1221-3

R.T.: 5.022 min
Delta R.T.: -0.063 min
Response: 1048491
Conc: 9.08 ng/ml

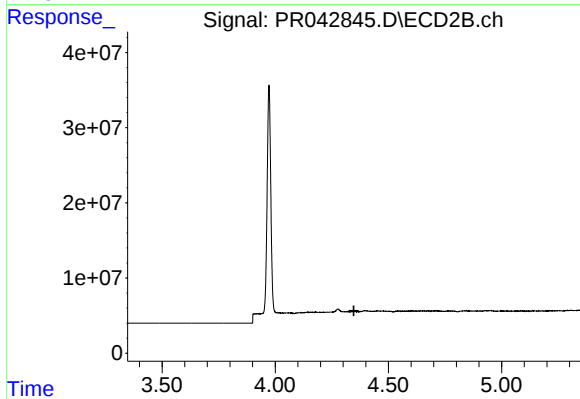

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

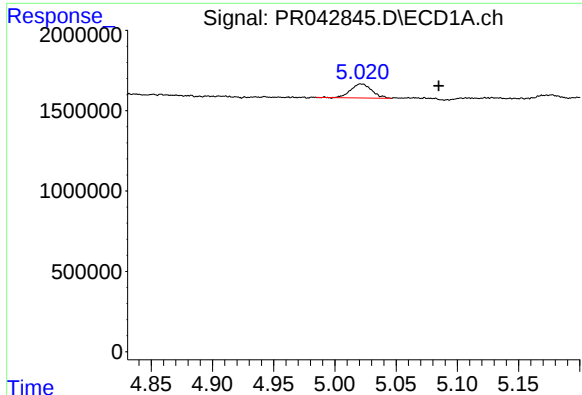

#11 AR-1232-1


R.T.: 5.022 min
Delta R.T.: -0.063 min
Response: 1048491
Conc: 6.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-30-D

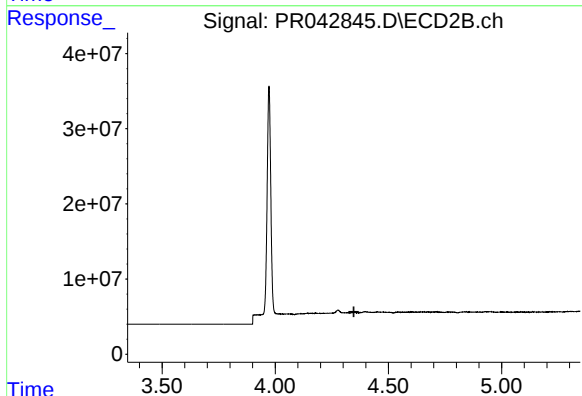


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.347 min
Response: 0
Conc: N.D.

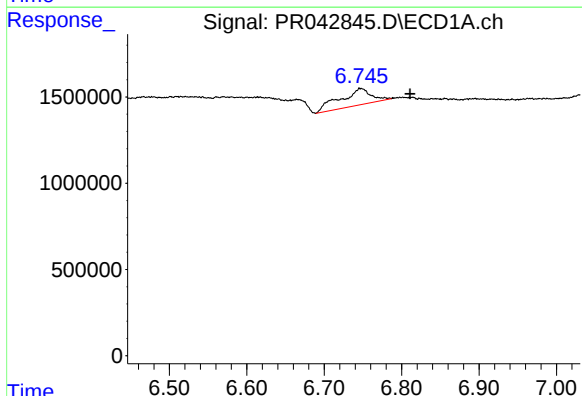


#20 AR-1242-5

R.T.: 6.747 min
Delta R.T.: -0.064 min
Response: 2695408
Conc: 26.96 ng/ml

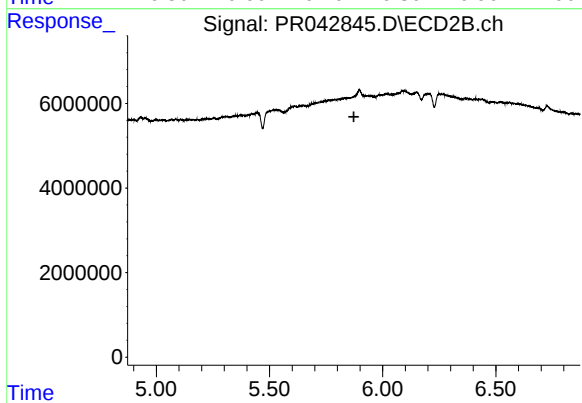

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.873 min
Response: 0
Conc: N.D.

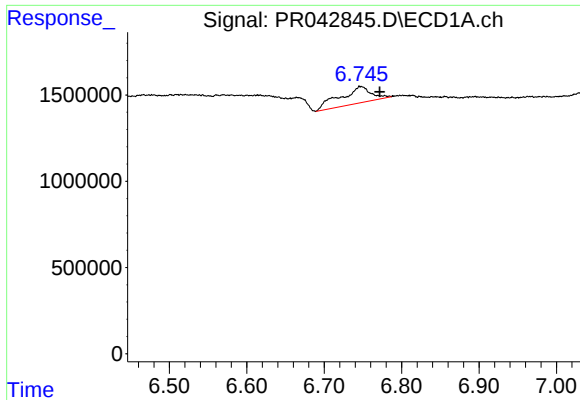

#24 AR-1248-4


R.T.: 6.747 min
Delta R.T.: -0.025 min
Response: 2695408
Conc: 15.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-30-D

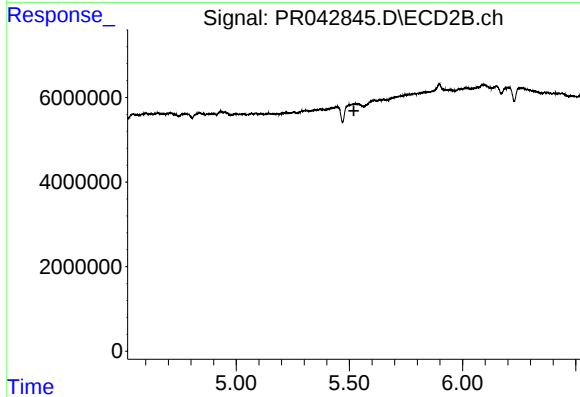


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.520 min
Response: 0
Conc: N.D.

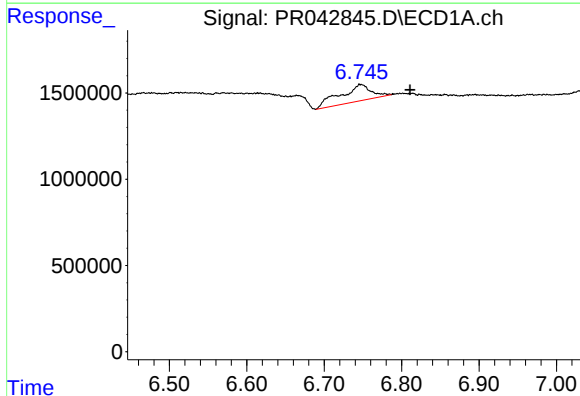


#25 AR-1248-5

R.T.: 6.747 min
Delta R.T.: -0.064 min
Response: 2695408
Conc: 16.62 ng/ml

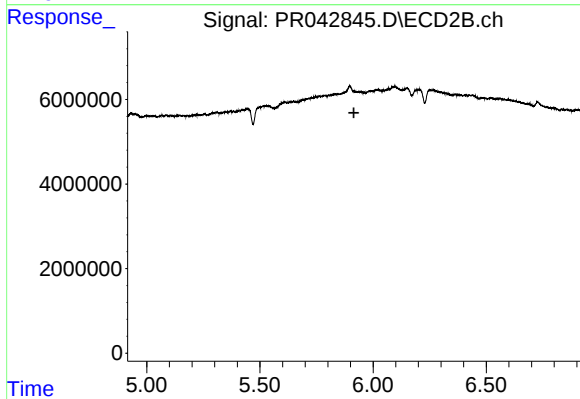

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.915 min
Response: 0
Conc: N.D.

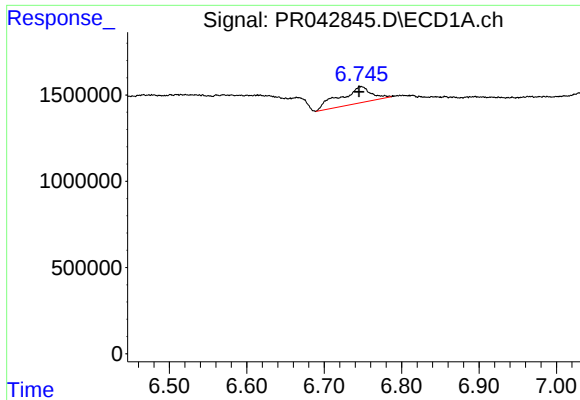

#26 AR-1254-1


R.T.: 6.747 min
Delta R.T.: 0.002 min
Response: 2695408
Conc: 14.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-30-D

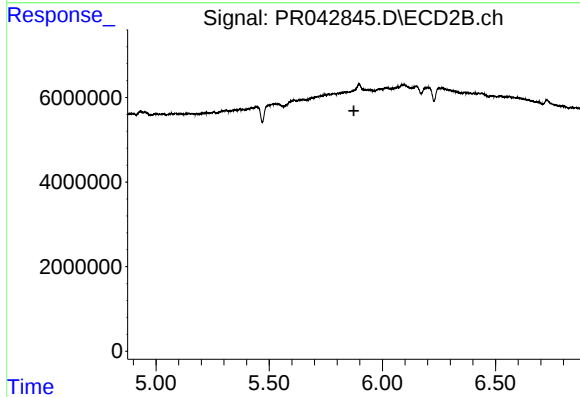


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.874 min
Response: 0
Conc: N.D.

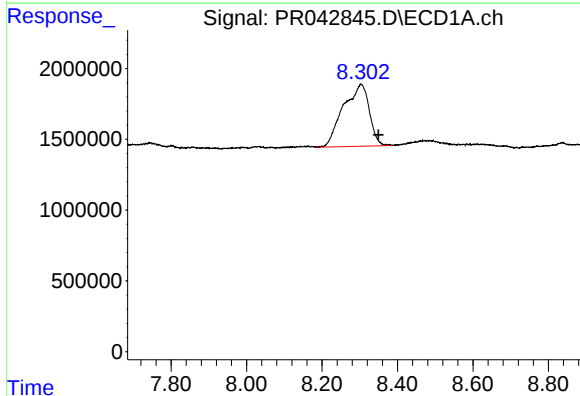

#34 AR-1260-4

R.T.: 8.303 min
Delta R.T.: -0.046 min
Response: 20935393
Conc: 100.32 ng/ml

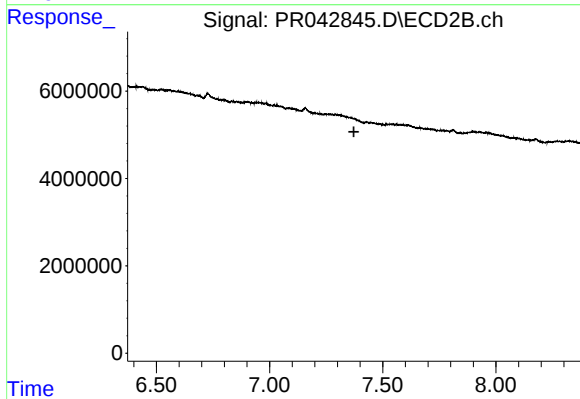

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.373 min
Response: 0
Conc: N.D.