

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110619\
Data File : PR042900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2019 02:07
Operator : SM\AJ
Sample : K5687-11
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
26B

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 07:02:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 01 09:55:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.710	3.972	107.2E6	381.0E6	18.194m	19.002
2) SA Decachlor...	10.621	9.066	49416010	137.3E6	12.348	10.923

Ankita

Target Compounds

11/6/2019 1:49:37 PM

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110619\
Data File : PR042900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2019 02:07
Operator : SM\AJ
Sample : K5687-11
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
26B

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 07:02:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 01 09:55:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

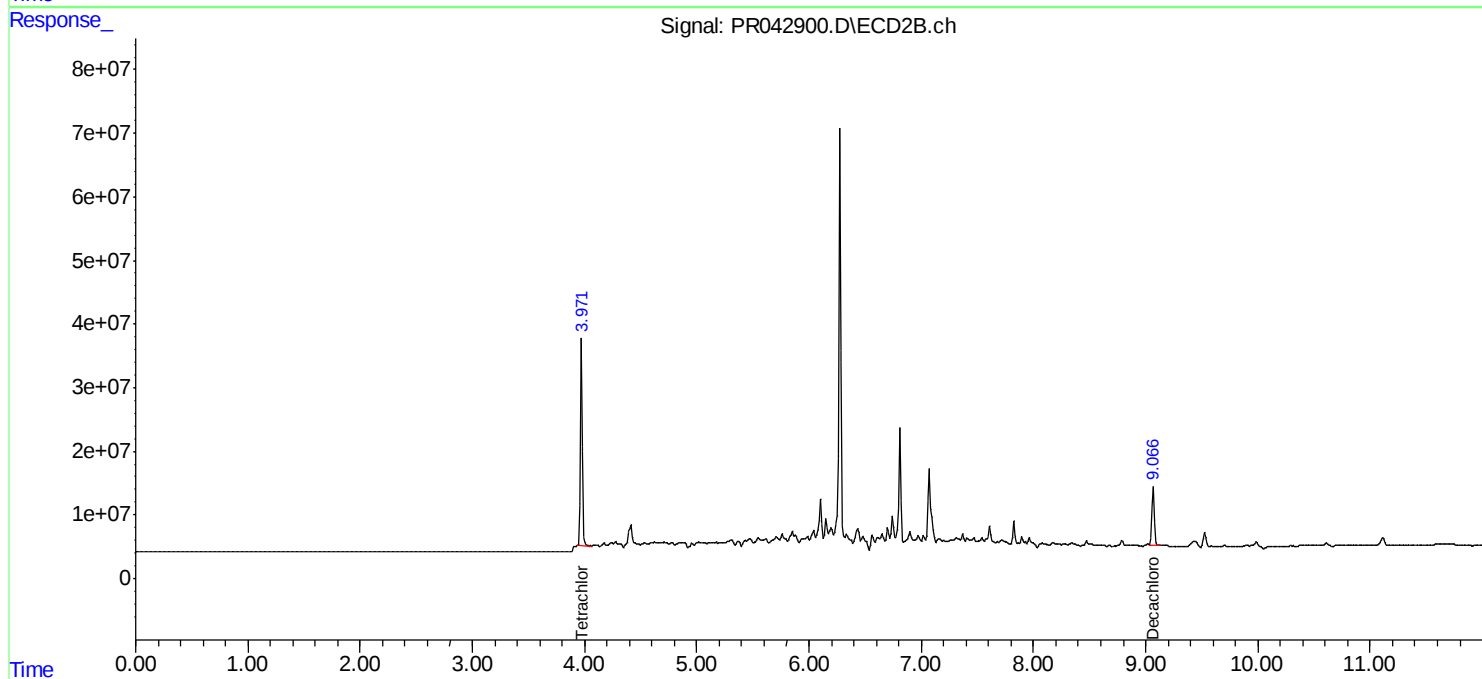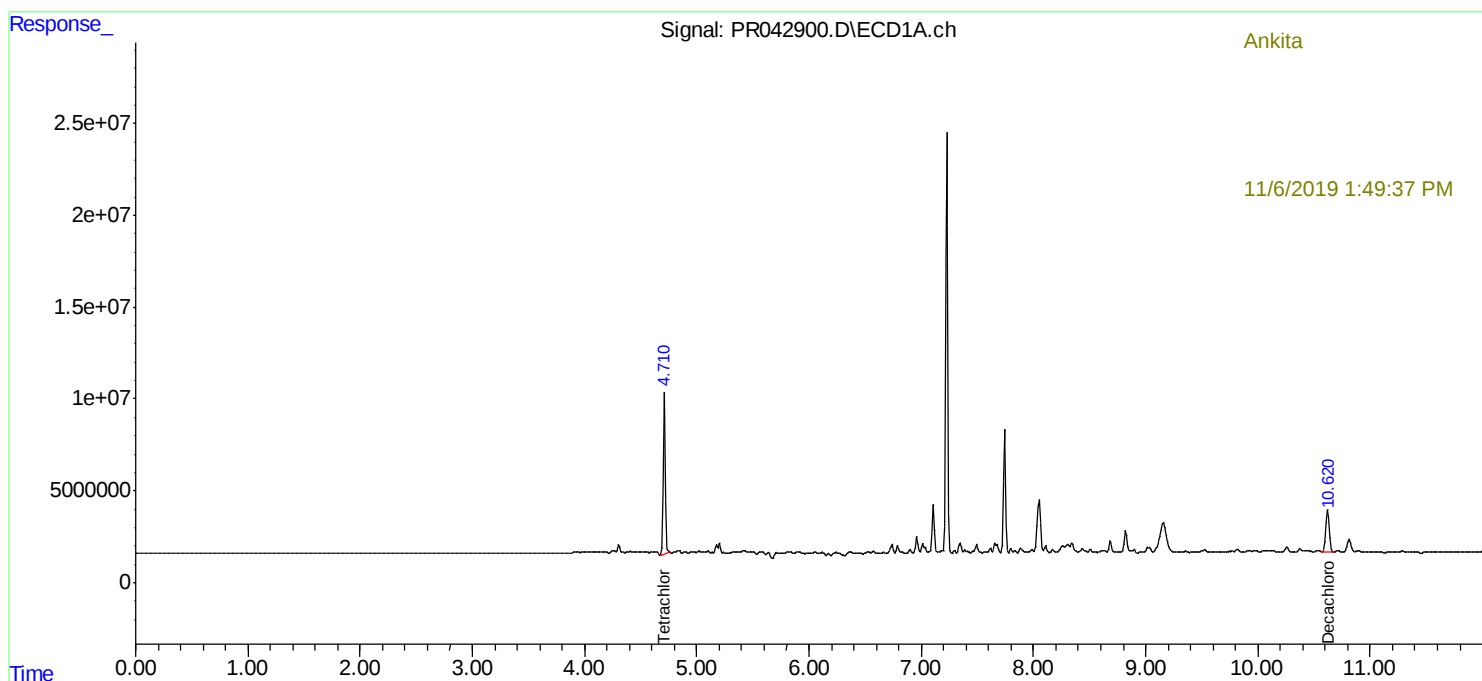

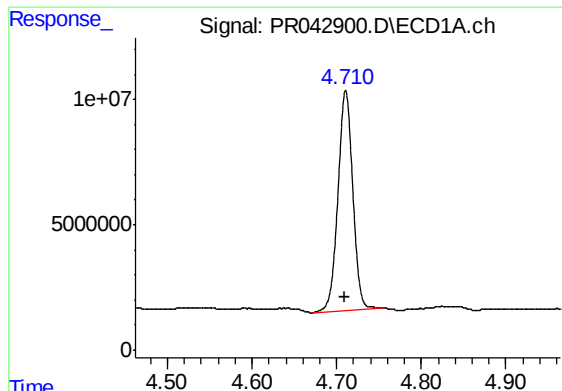


#1 Tetrachloro-m-xylene

R.T.: 4.710 min
Delta R.T.: 0.001 min
Response: 107240572
Conc: 18.19 ng/ml m

Instrument :
ECD_R
ClientSampleId :
26B


Manual Integrations
APPROVED

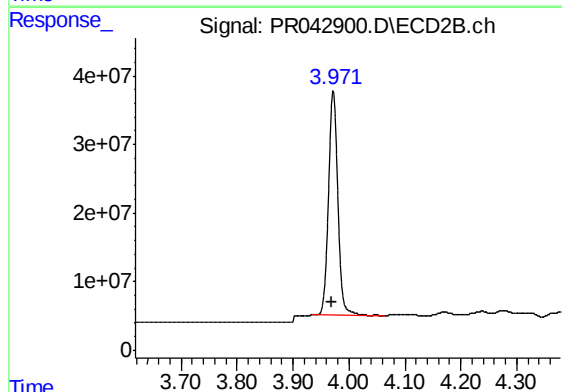

#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.003 min
Response: 381004081
Conc: 19.00 ng/ml


Ankita

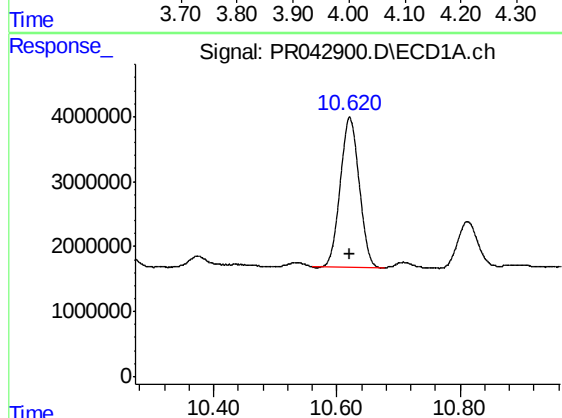

#2 Decachlorobiphenyl

R.T.: 10.621 min
Delta R.T.: -0.001 min
Response: 49416010
Conc: 12.35 ng/ml

11/6/2019 1:49:37 PM

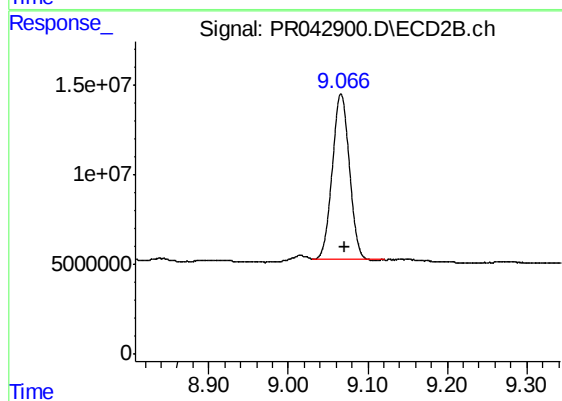

#2 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: -0.004 min
Response: 137253200
Conc: 10.92 ng/ml