

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110620\
 Data File : PR048588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2020 12:56
 Operator : DD\AJ
 Sample : L4617-06RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 DUPLICATE RE

Manual Integrations
 APPROVED

Ankita
 11/6/2020 3:11:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 14:50:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.728	3.883	38915428	42290682	15.897	14.565
2)	SA Decachlor...	10.649	8.985	25875444	127.3E6	9.821m	8.718

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR110620\
Data File : PR048588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2020 12:56
Operator : DD\AJ
Sample : L4617-06RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
DUPLICATE RE


Manual Integrations
APPROVED

Ankita
11/6/2020 3:11:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 14:50:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

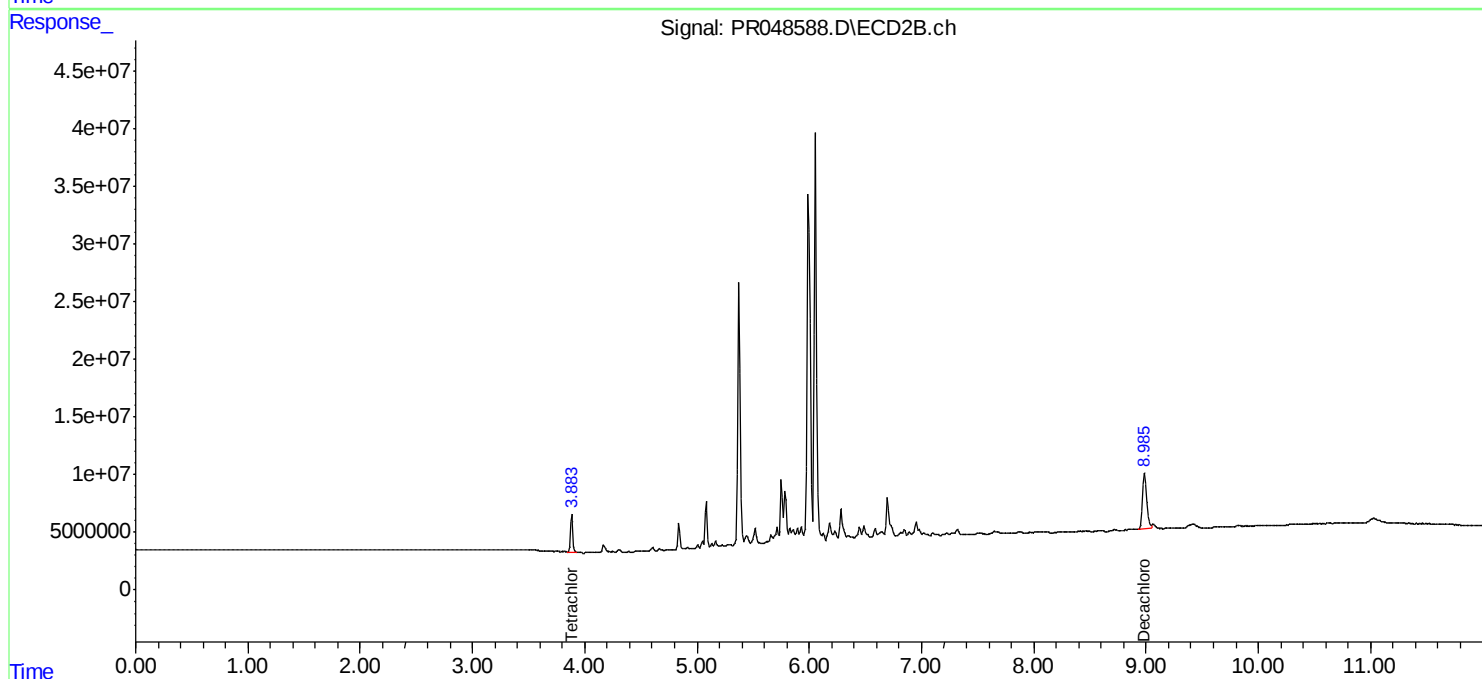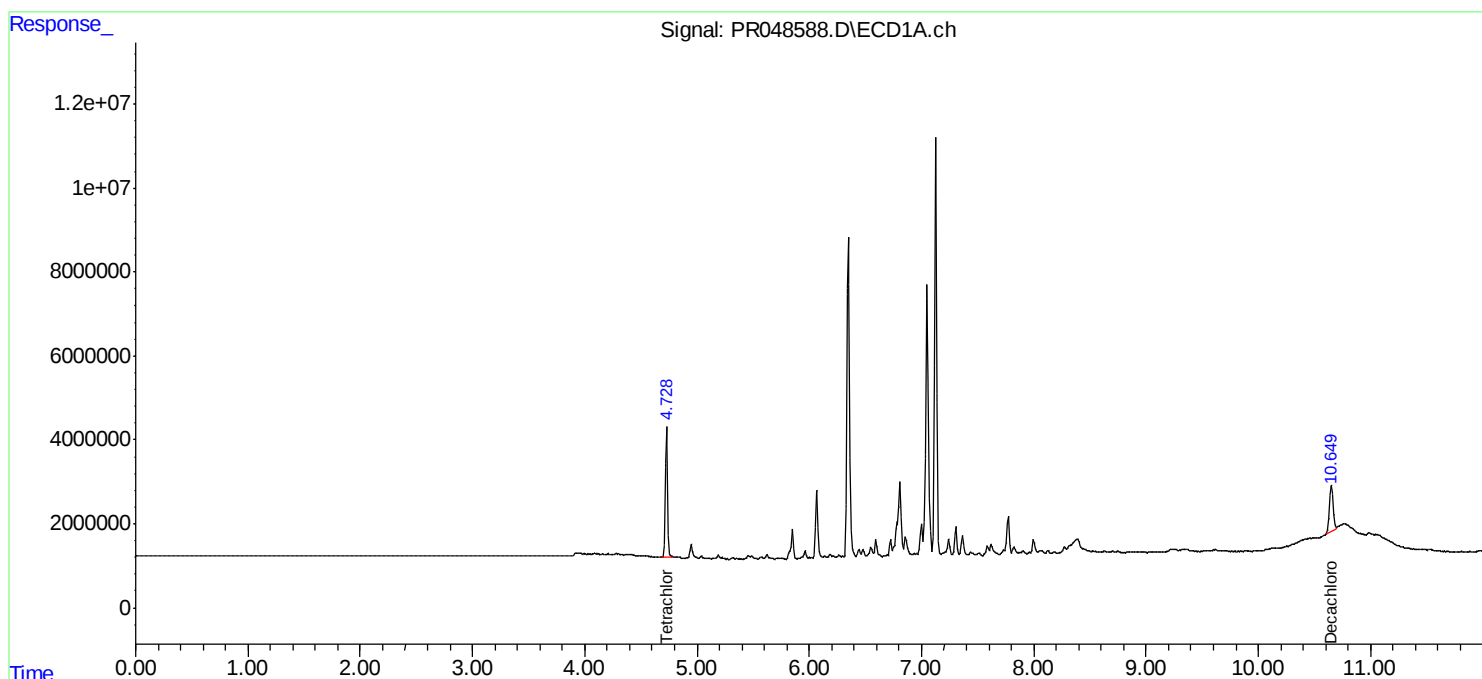

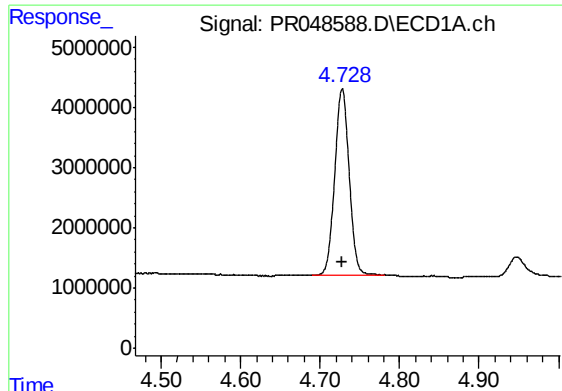


#1 Tetrachloro-m-xylene

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 38915428
Conc: 15.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
DUPLICATE RE


Manual Integrations
APPROVED

Ankita
11/6/2020 3:11:23 PM

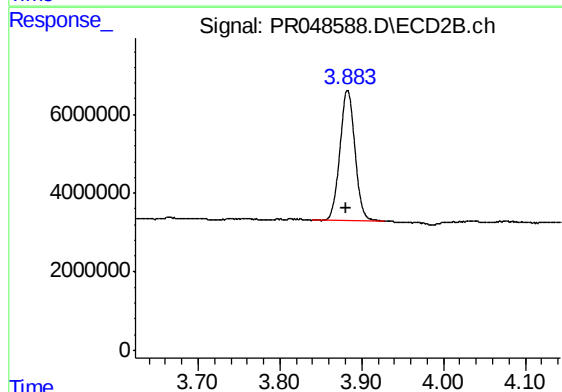


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.002 min
Response: 42290682
Conc: 14.57 ng/ml

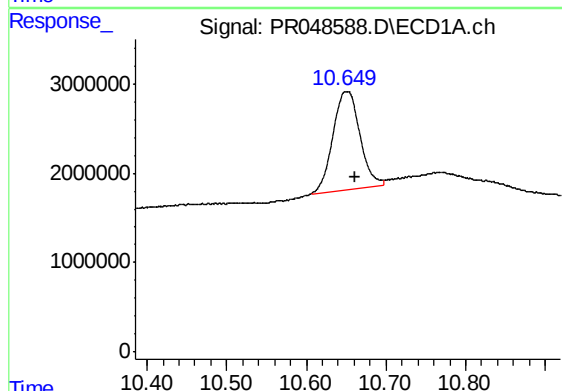

#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.012 min
Response: 25875444
Conc: 9.82 ng/ml m

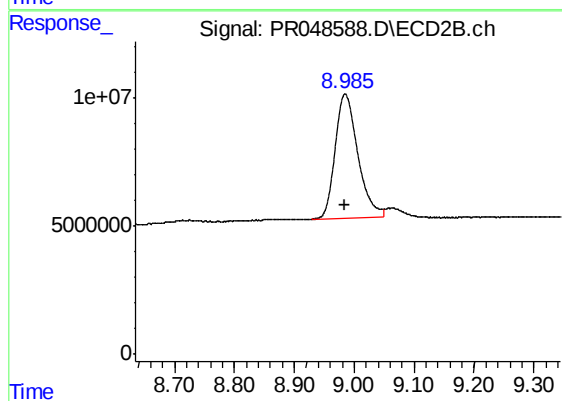

#2 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.001 min
Response: 127333947
Conc: 8.72 ng/ml