

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111419\
 Data File : PR043096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2019 14:51
 Operator : SM\AJ
 Sample : K5826-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-15-S

Manual Integrations
 APPROVED

Ankita
 11/15/2019 8:46:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 15:16:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 01 09:55:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.717	3.978	49768193	213.5E6	8.443m	10.648 #
2) SA Decachlor...	10.632	9.073	88076665	199.6E6	22.009	15.880 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111419\
Data File : PR043096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2019 14:51
Operator : SM\AJ
Sample : K5826-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/15/2019 8:46:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 15:16:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110119.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 01 09:55:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

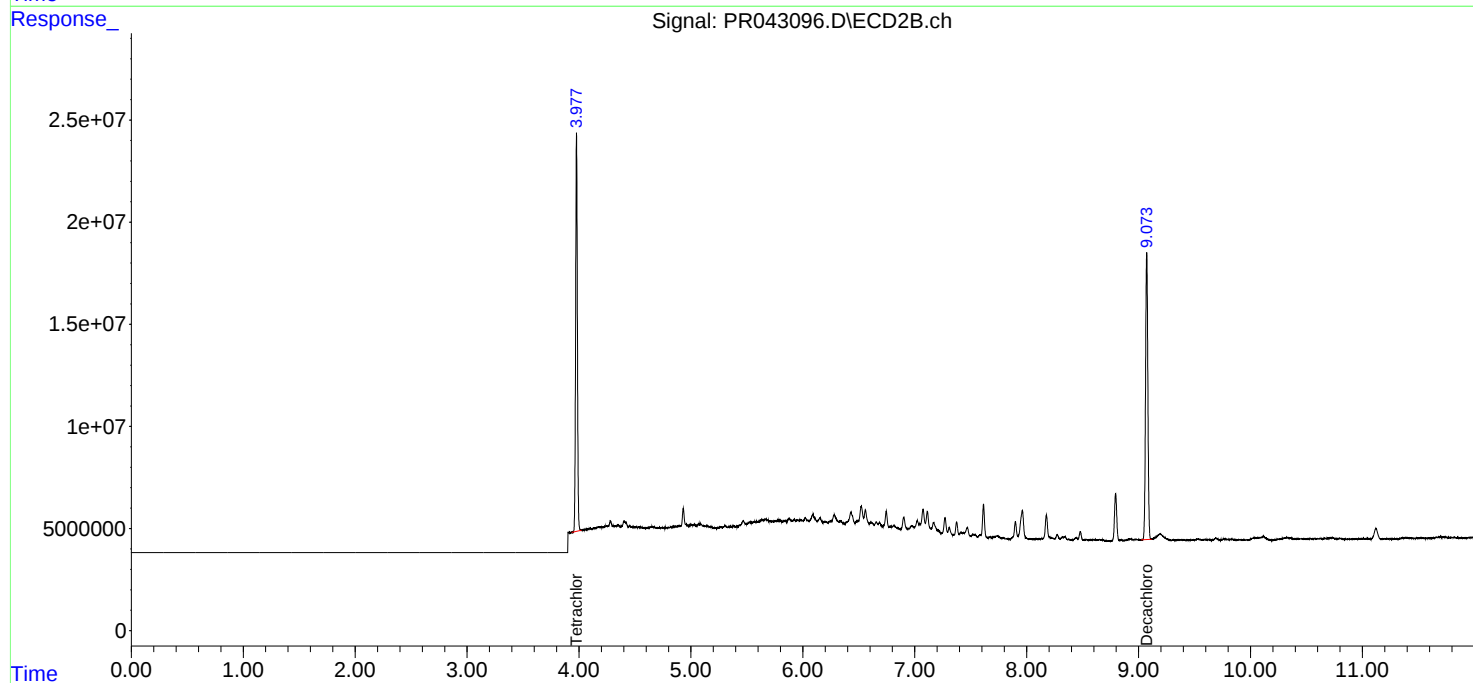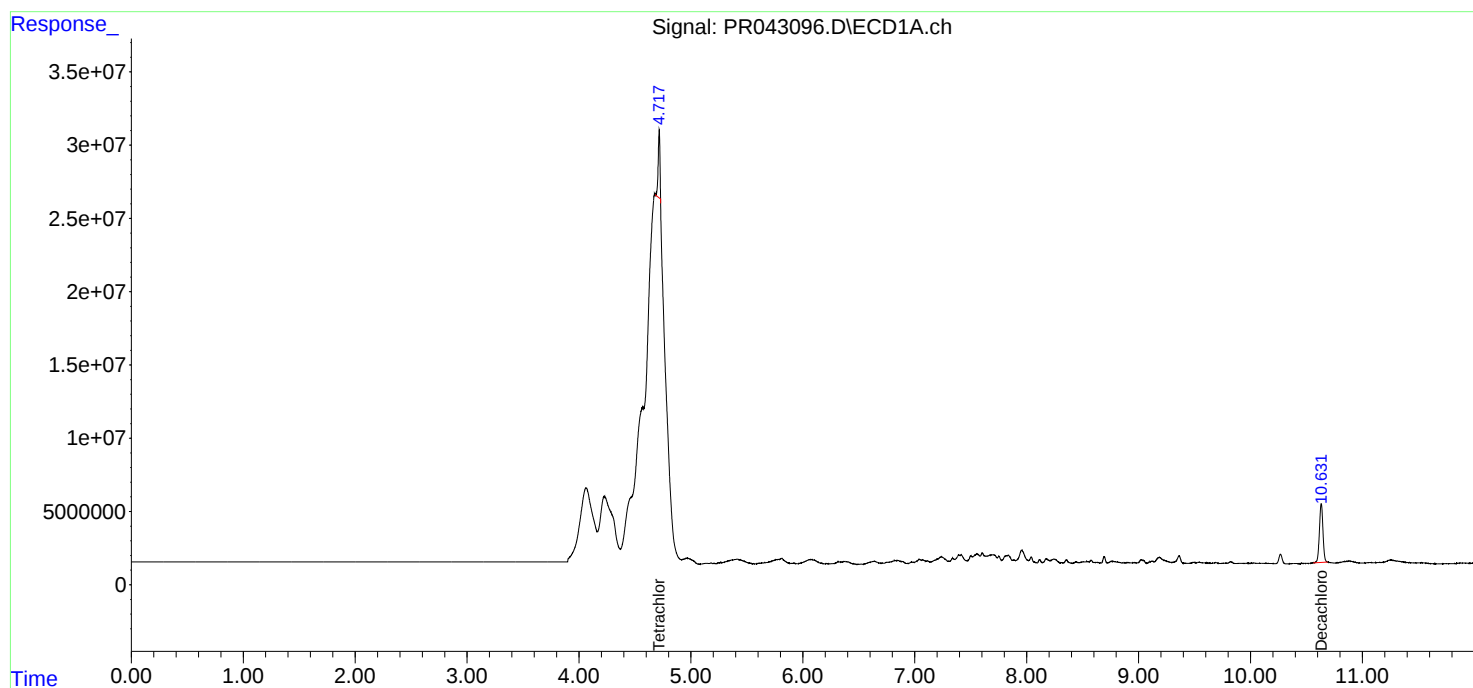

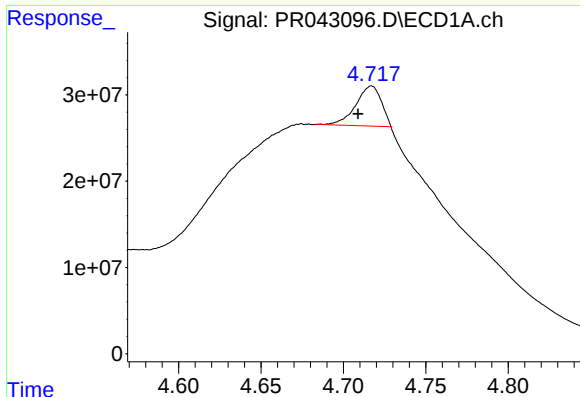


#1 Tetrachloro-m-xylene

R.T.: 4.717 min
Delta R.T.: 0.008 min
Response: 49768193
Conc: 8.44 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/15/2019 8:46:39 AM

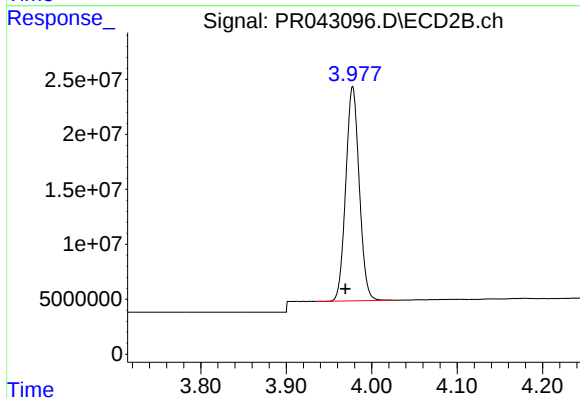


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: 0.009 min
Response: 213503834
Conc: 10.65 ng/ml

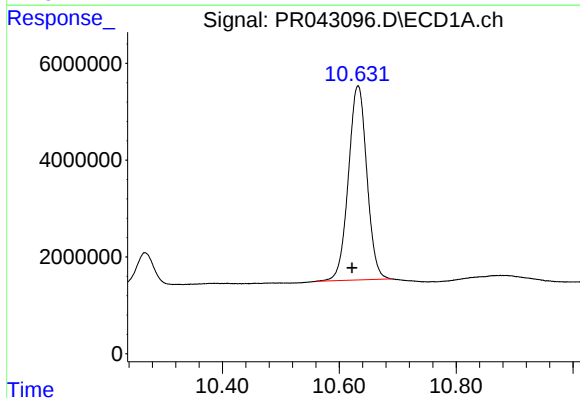

#2 Decachlorobiphenyl

R.T.: 10.632 min
Delta R.T.: 0.010 min
Response: 88076665
Conc: 22.01 ng/ml

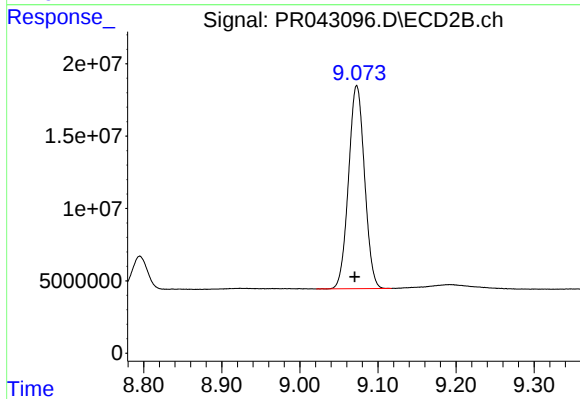

#2 Decachlorobiphenyl

R.T.: 9.073 min
Delta R.T.: 0.002 min
Response: 199552996
Conc: 15.88 ng/ml