

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
 Data File : PR048638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 14:46
 Operator : DD\AJ
 Sample : L4731-04RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TI-633-XRE

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:21:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 17:35:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.722	3.878	111.2E6	203.3E6	45.416m	70.005m#
2) SA Decachlor...	10.655	8.991	44897041	248.0E6	17.040	16.981

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
Data File : PR048638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 14:46
Operator : DD\AJ
Sample : L4731-04RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
TI-633-XRE


Manual Integrations
APPROVED

Ankita
11/18/2020 10:21:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 17:35:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

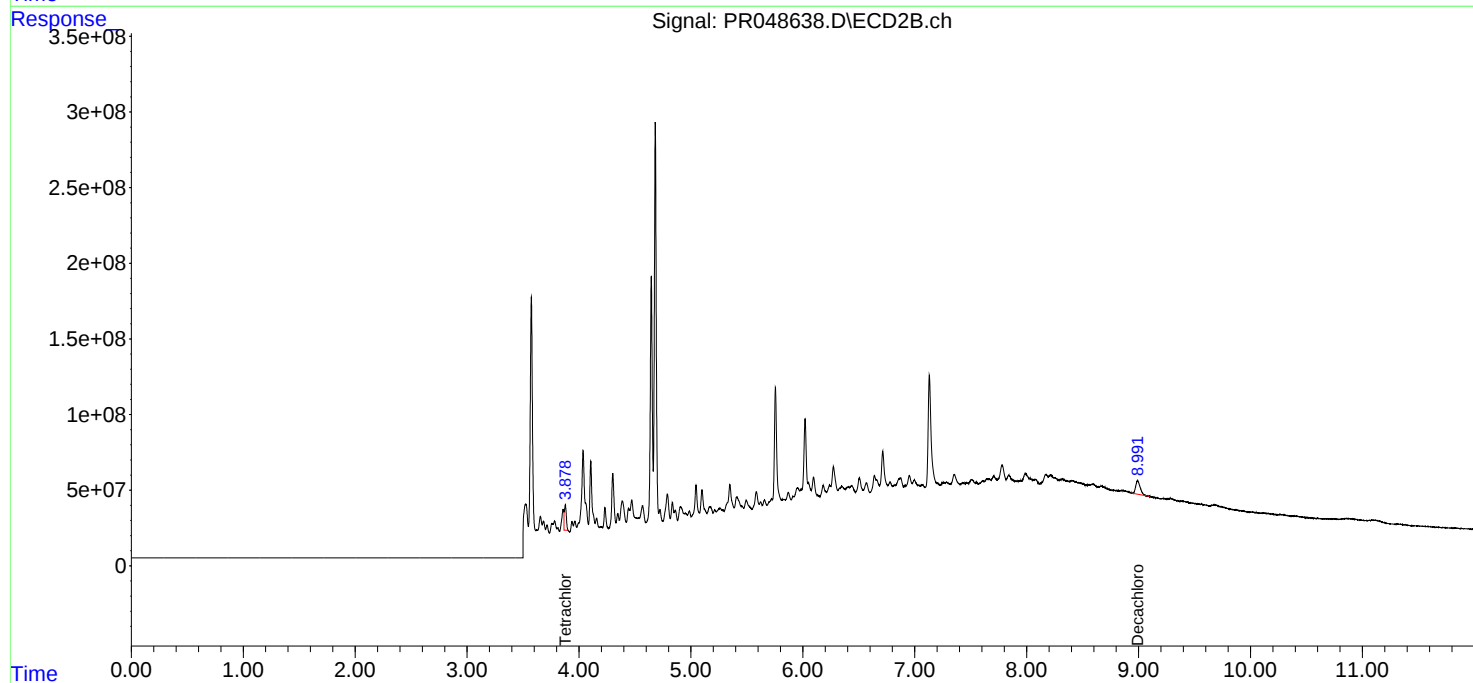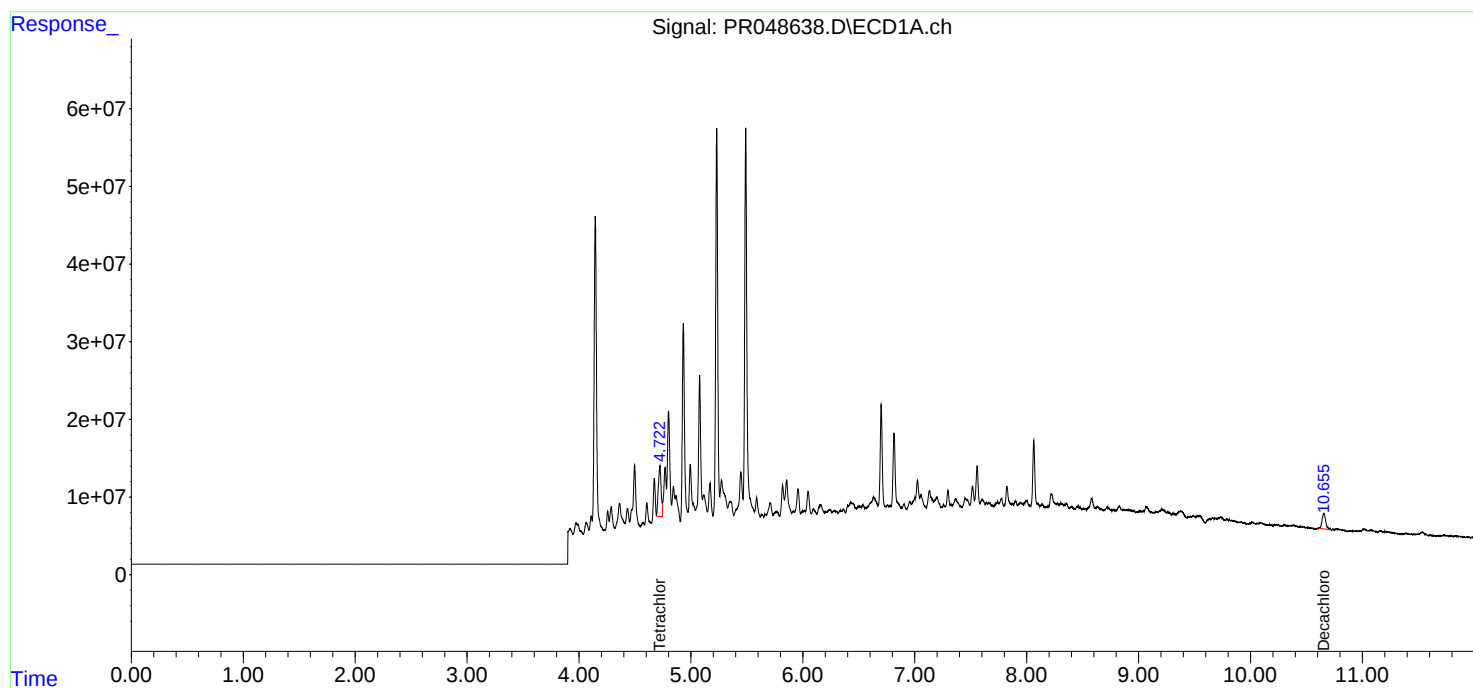

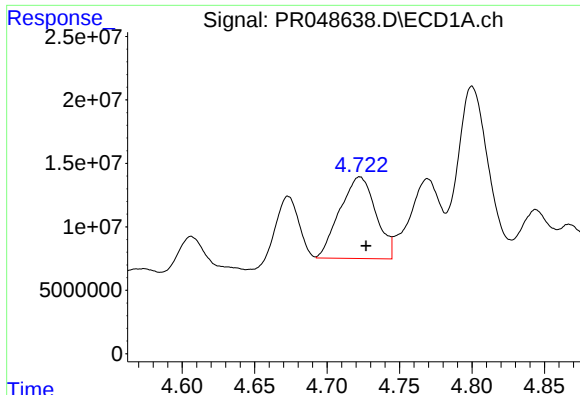


#1 Tetrachloro-m-xylene

R.T.: 4.722 min
Delta R.T.: -0.005 min
Response: 111174526
Conc: 45.42 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TI-633-XRE


Manual Integrations
APPROVED

Ankita
11/18/2020 10:21:18 AM

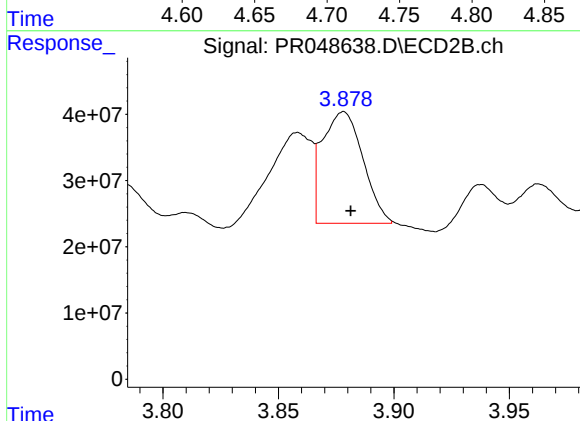


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: -0.003 min
Response: 203261593
Conc: 70.00 ng/ml m

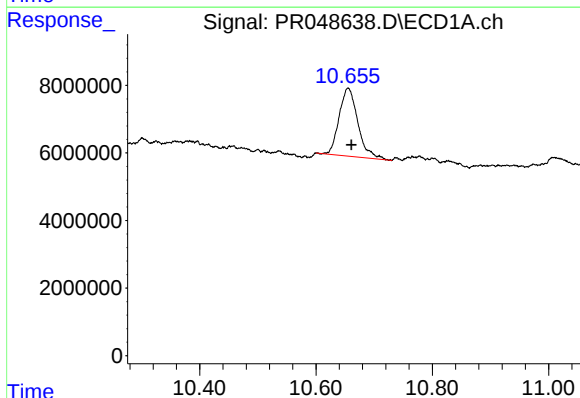

#2 Decachlorobiphenyl

R.T.: 10.655 min
Delta R.T.: -0.006 min
Response: 44897041
Conc: 17.04 ng/ml

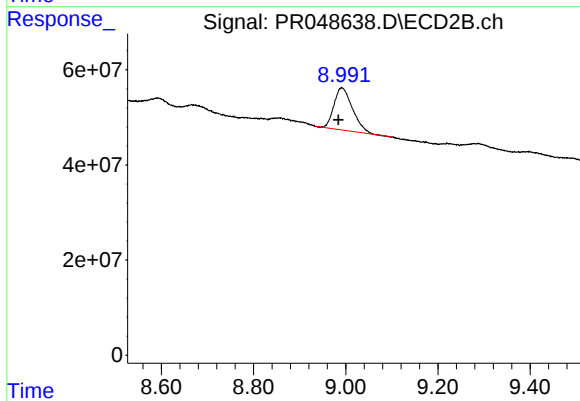

#2 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.007 min
Response: 248021872
Conc: 16.98 ng/ml