

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
 Data File : PR048657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 19:52
 Operator : DD\AJ
 Sample : L4766-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TOTE-COMP-AUD

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:22:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 02:37:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.725	3.880	39103751	52961358	15.974	18.240
2) SA Decachlor...	10.653	8.991	33292274	170.5E6	12.636m	11.671

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
Data File : PR048657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 19:52
Operator : DD\AJ
Sample : L4766-12
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
TOTE-COMP-AUD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 02:37:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

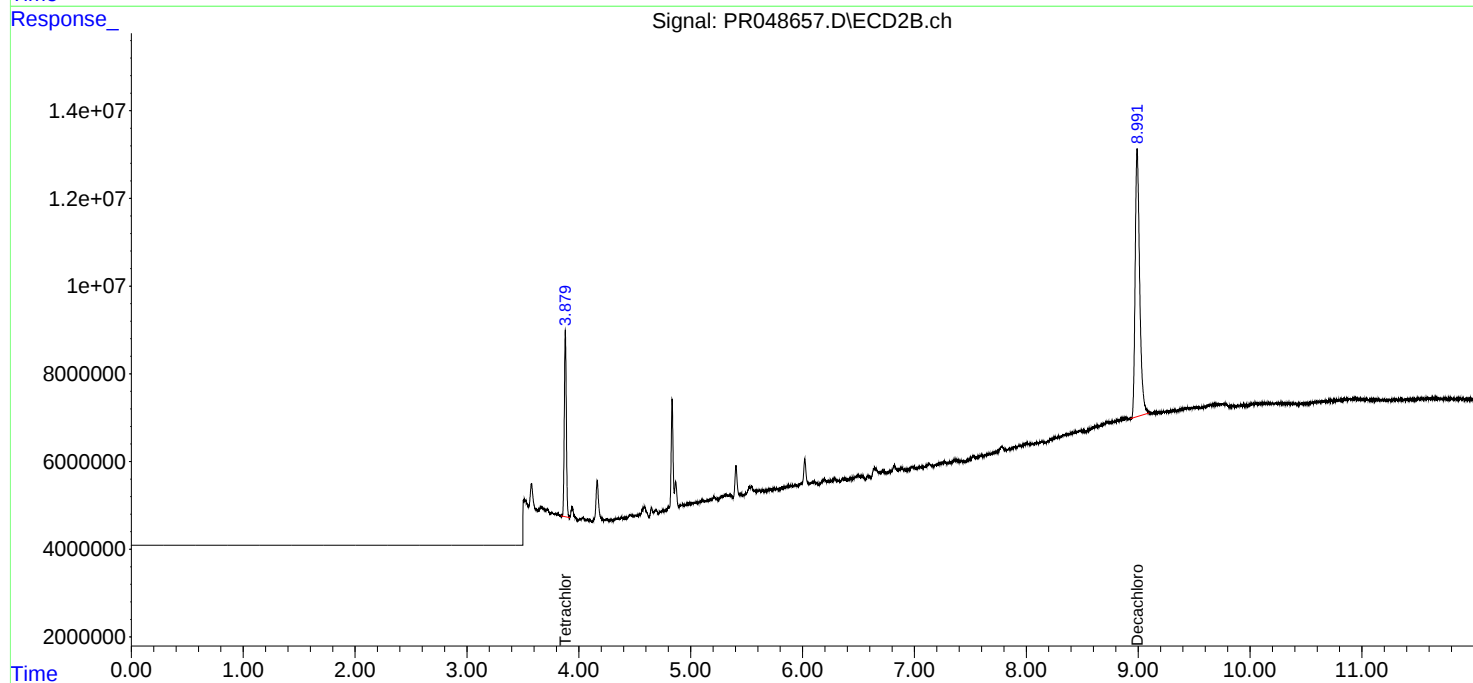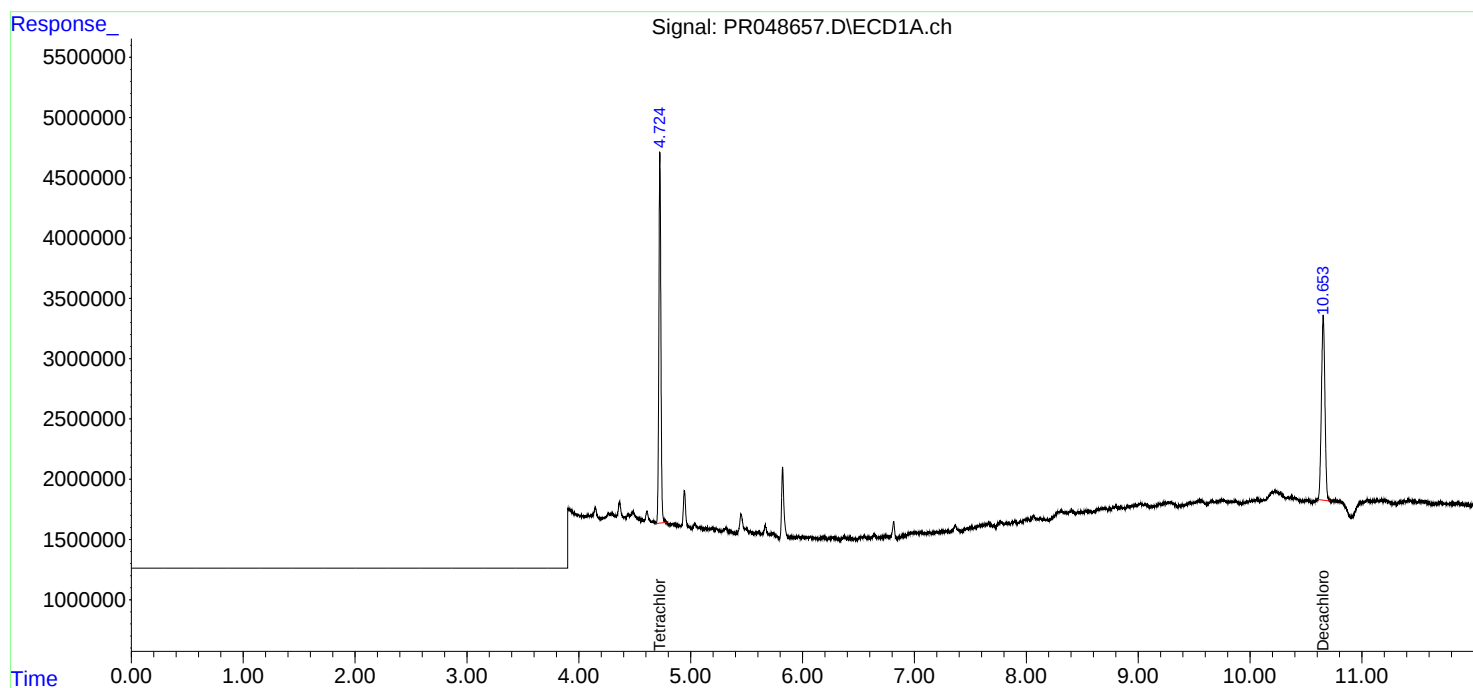

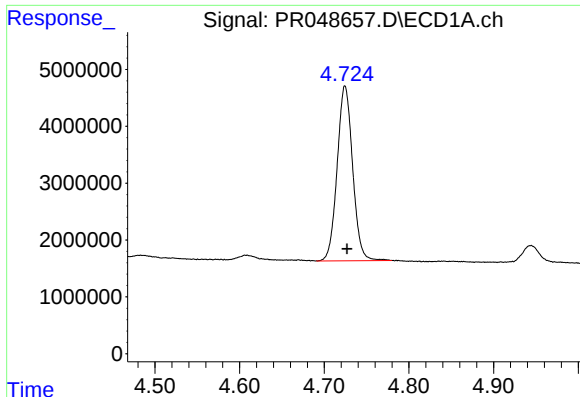


#1 Tetrachloro-m-xylene

R.T.: 4.725 min
Delta R.T.: -0.002 min
Response: 39103751
Conc: 15.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
TOTE-COMP-AUD


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:01 AM

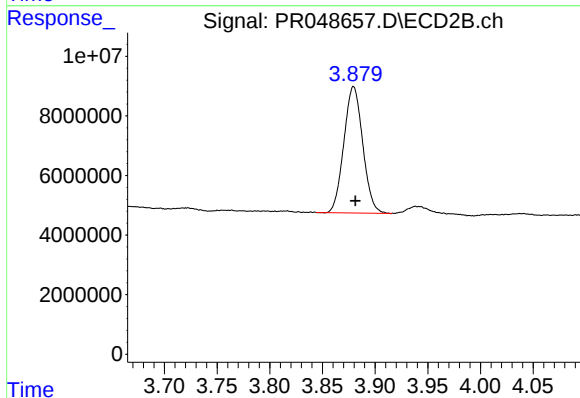


#1 Tetrachloro-m-xylene

R.T.: 3.880 min
Delta R.T.: -0.002 min
Response: 52961358
Conc: 18.24 ng/ml

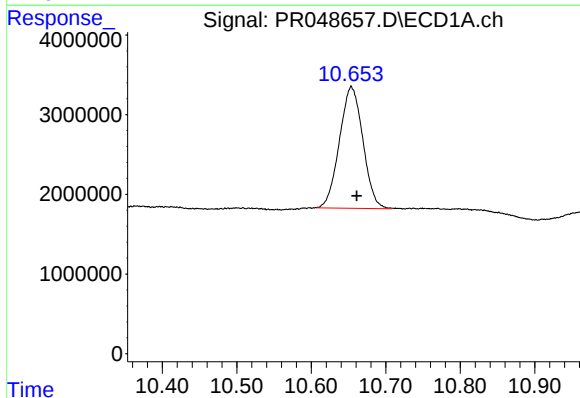

#2 Decachlorobiphenyl

R.T.: 10.653 min
Delta R.T.: -0.008 min
Response: 33292274
Conc: 12.64 ng/ml m

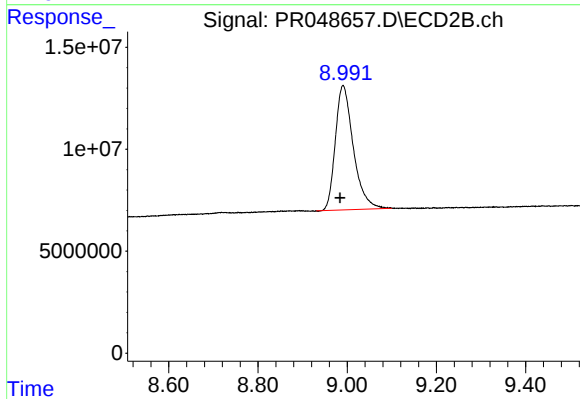

#2 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.007 min
Response: 170469052
Conc: 11.67 ng/ml