

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
 Data File : PR048661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2020 20:50
 Operator : DD\AJ
 Sample : L4769-07 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TRE-1089

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:22:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 02:41:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.723	3.874	4655212	4093327	1.902m	1.410m#
2) SA Decachlor...	10.657	8.996	5890825	24808052	2.236	1.699

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
Data File : PR048661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2020 20:50
Operator : DD\AJ
Sample : L4769-07 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
TRE-1089


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 02:41:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

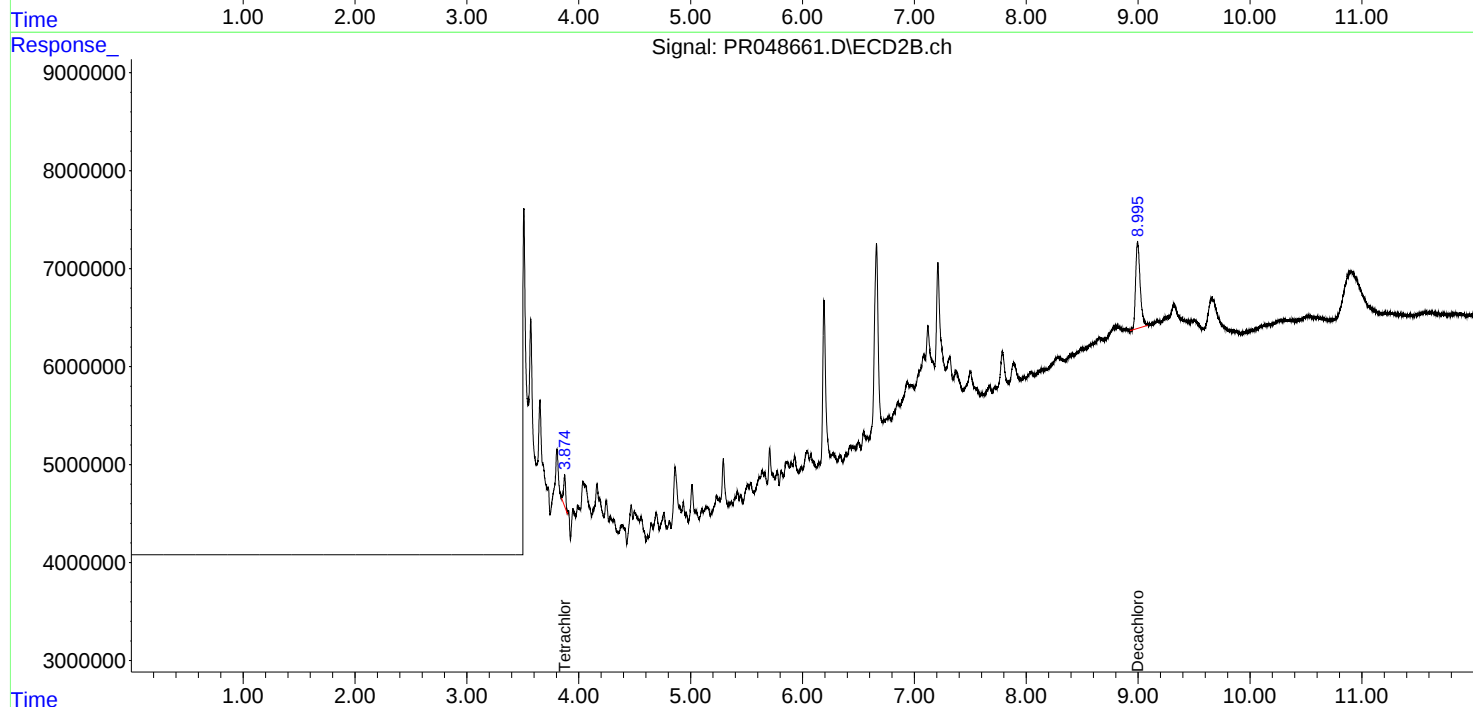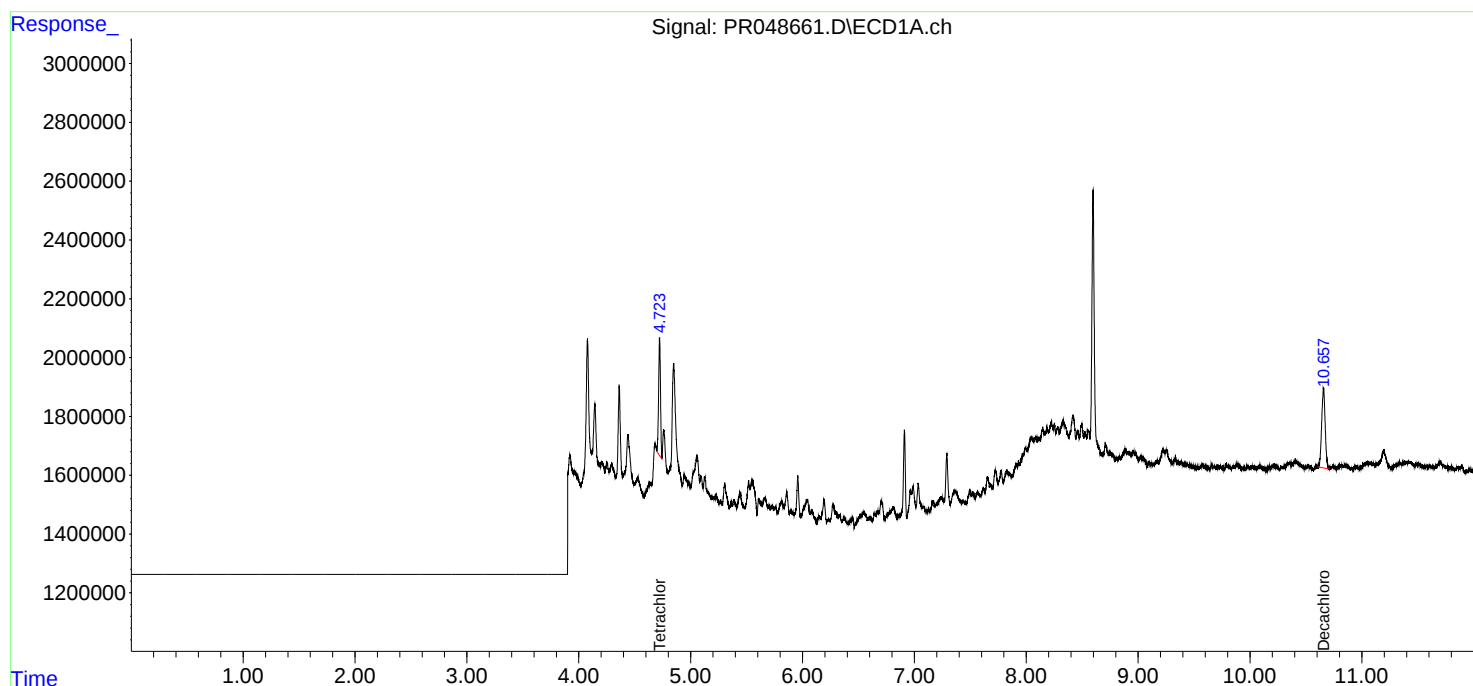

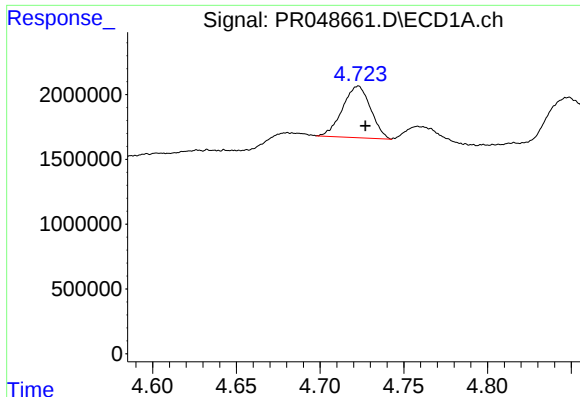


#1 Tetrachloro-m-xylene

R.T.: 4.723 min
Delta R.T.: -0.005 min
Response: 4655212
Conc: 1.90 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TRE-1089


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:06 AM

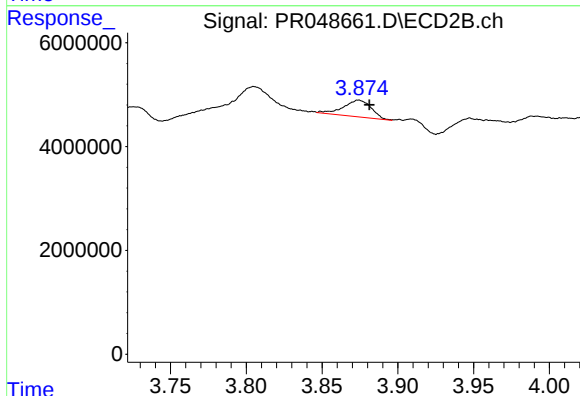


#1 Tetrachloro-m-xylene

R.T.: 3.874 min
Delta R.T.: -0.007 min
Response: 4093327
Conc: 1.41 ng/ml m

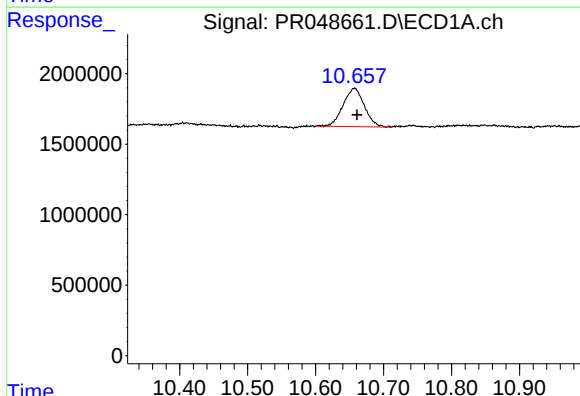

#2 Decachlorobiphenyl

R.T.: 10.657 min
Delta R.T.: -0.004 min
Response: 5890825
Conc: 2.24 ng/ml

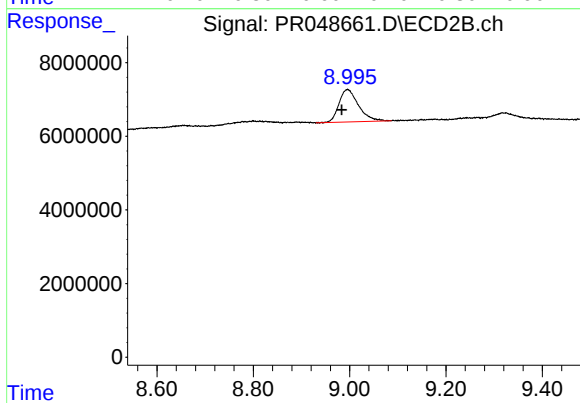

#2 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.012 min
Response: 24808052
Conc: 1.70 ng/ml