

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
 Data File : PR048674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 00:27
 Operator : DD\AJ
 Sample : L4766-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PIPE-AUD-31334

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:22:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 02:52:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.727	3.882	16852515	26775574	6.884	9.222m#
2) SA Decachlor...	10.659	9.013f	25222671	127.1E6	9.573	8.701m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
Data File : PR048674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 00:27
Operator : DD\AJ
Sample : L4766-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31334


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 02:52:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

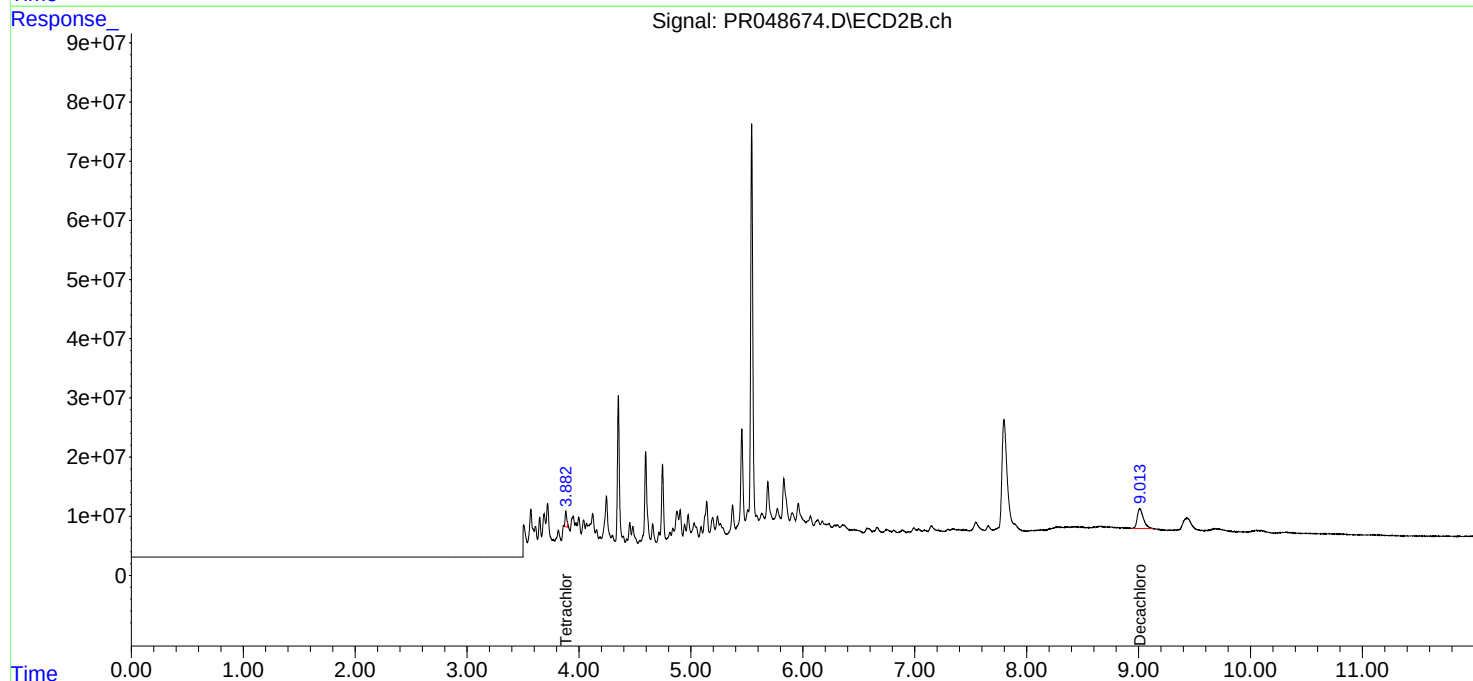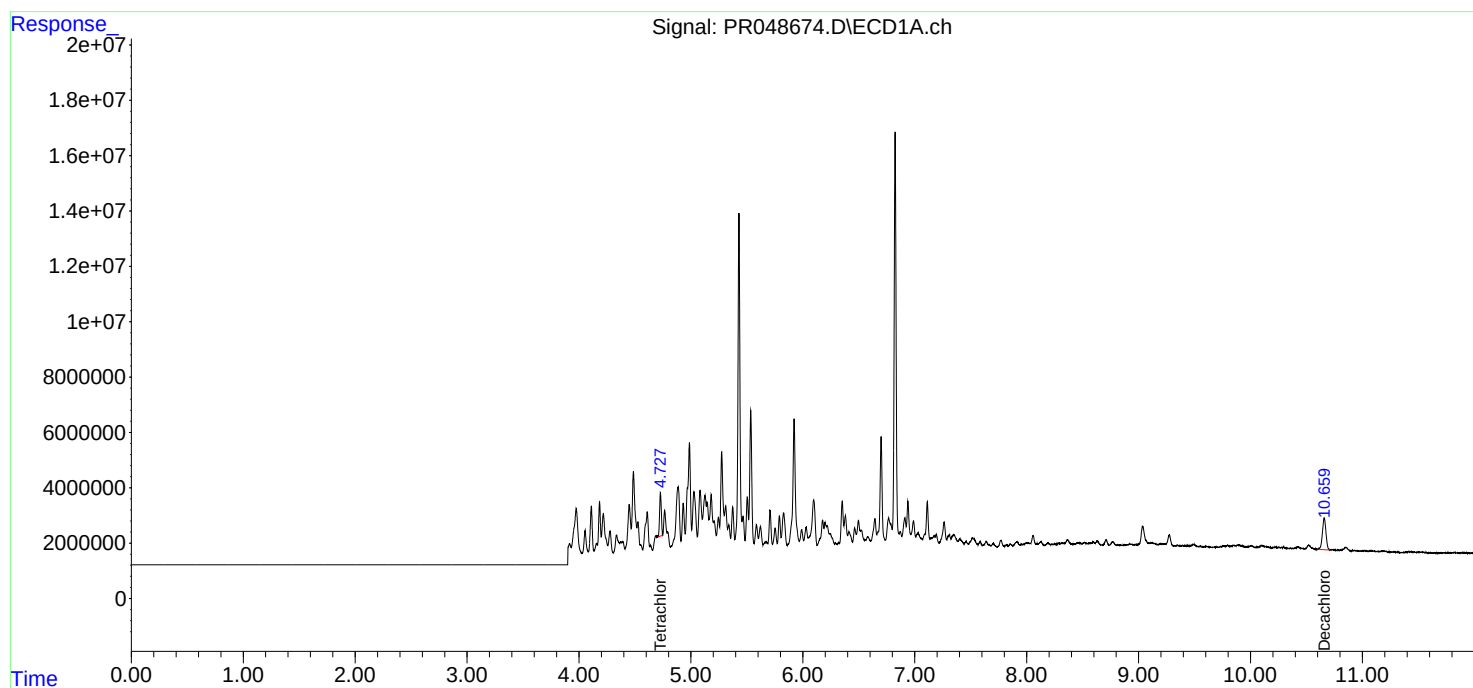

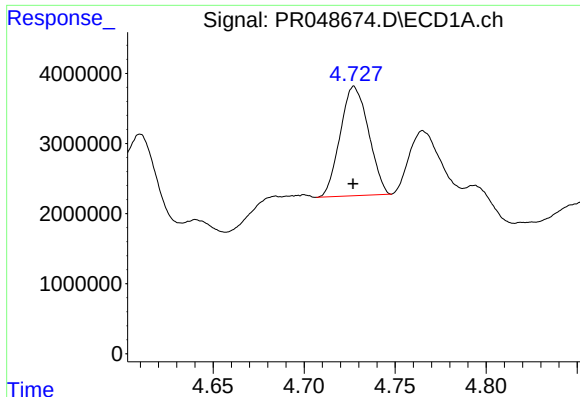


#1 Tetrachloro-m-xylene

R.T.: 4.727 min
Delta R.T.: 0.000 min
Response: 16852515
Conc: 6.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31334


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:24 AM

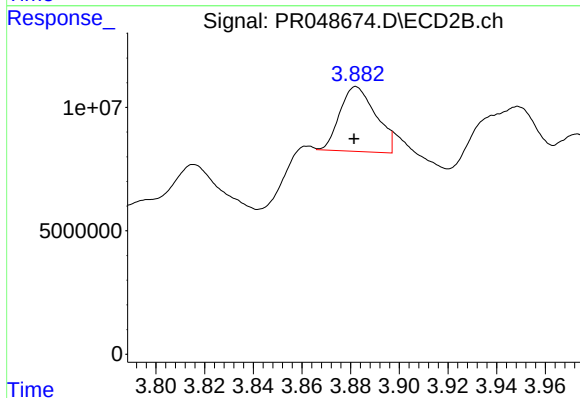


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 26775574
Conc: 9.22 ng/ml m

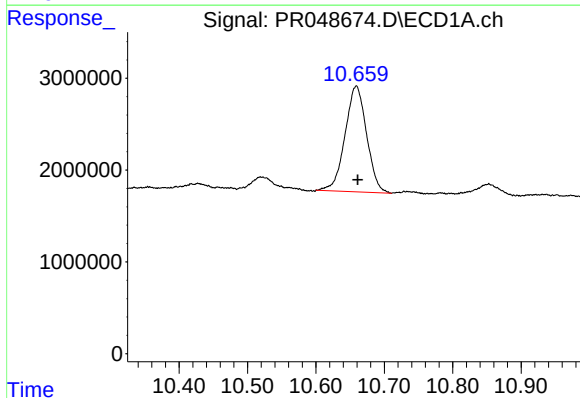

#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.002 min
Response: 25222671
Conc: 9.57 ng/ml

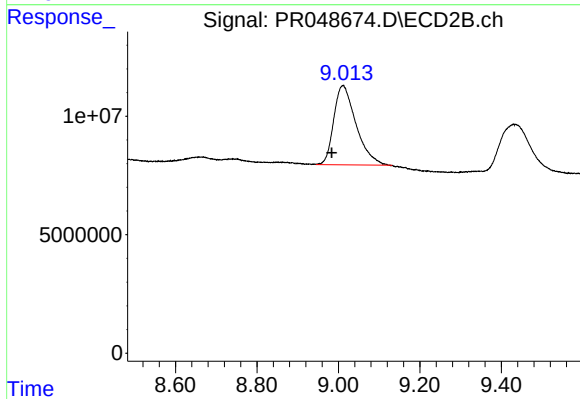

#2 Decachlorobiphenyl

R.T.: 9.013 min
Delta R.T.: 0.029 min
Response: 127080866
Conc: 8.70 ng/ml m