

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
 Data File : PR048675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 00:41
 Operator : DD\AJ
 Sample : L4766-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PIPE-AUD-31336

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:22:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 02:53:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 04 04:25:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.726	3.881	22464899	32095896	9.177	11.054
2) SA Decachlor...	10.655	9.006f	24749554	125.6E6	9.393	8.600m
Target Compounds						
26) L6 AR-1254-1	6.762	5.781	48377497	71581952	551.160	463.896
27) L6 AR-1254-2	6.980	5.931	104.5E6	102.9E6	789.810	609.104
28) L6 AR-1254-3	7.351	6.340	118.4E6	226.1E6	846.687	675.476
29) L6 AR-1254-4	7.638	6.572	138.9E6	537.4E6	1282.455	975.890
30) L6 AR-1254-5	8.058	6.995	130.0E6	538.7E6	1128.891	925.090

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR111720\
Data File : PR048675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 00:41
Operator : DD\AJ
Sample : L4766-03
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
PIPE-AUD-31336


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 02:53:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR110320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 04 04:25:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

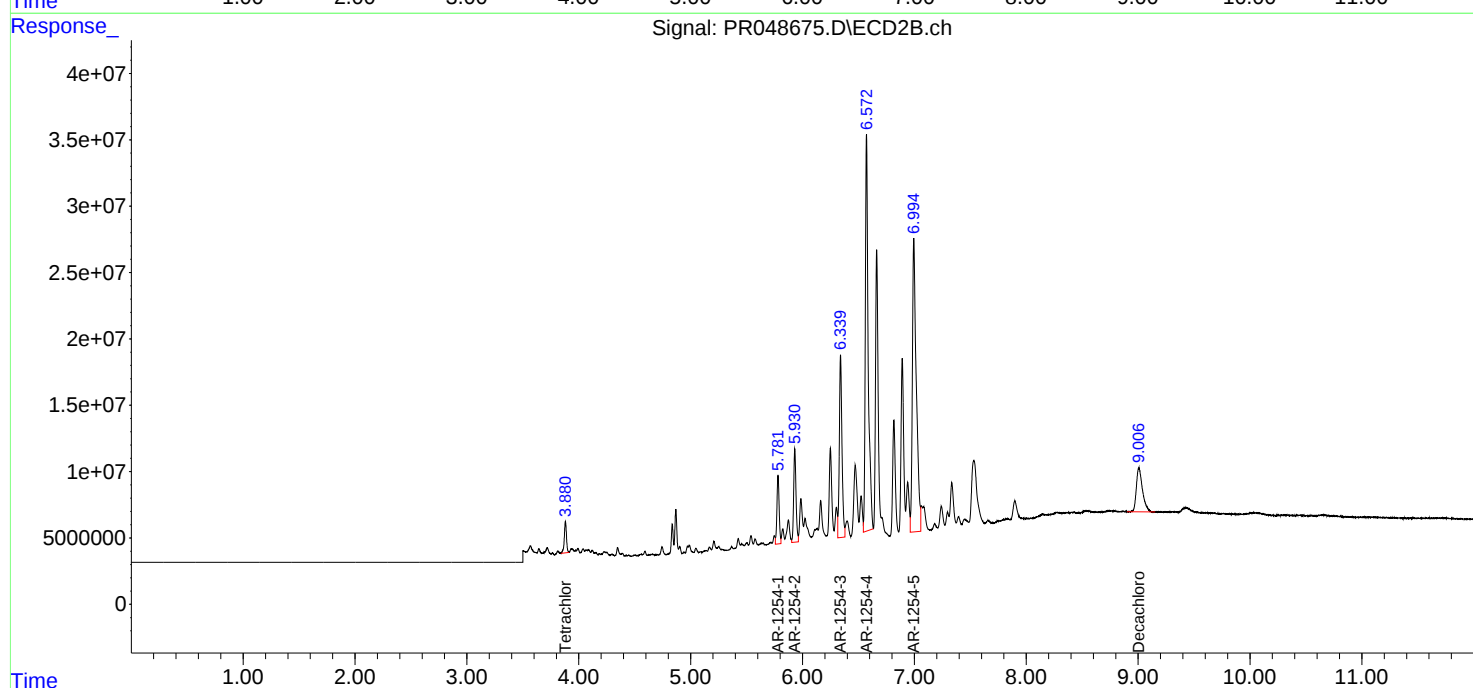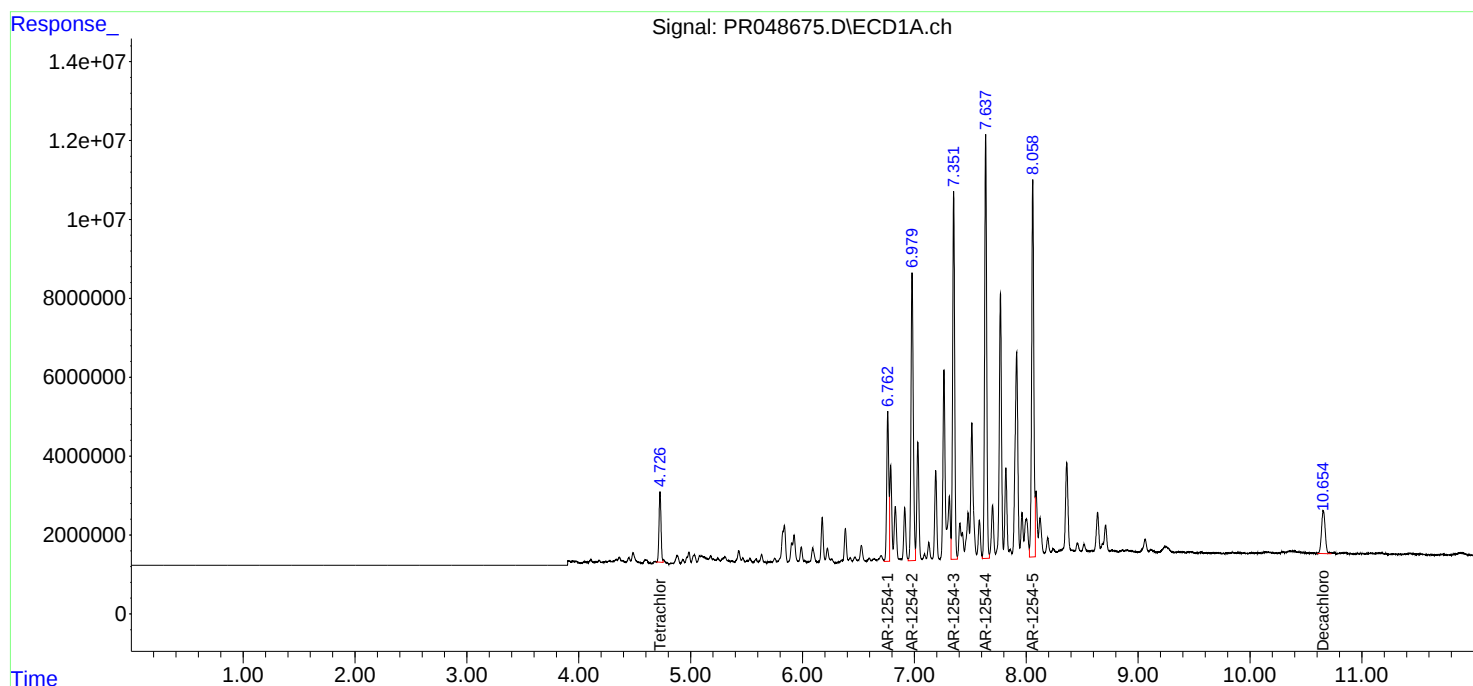

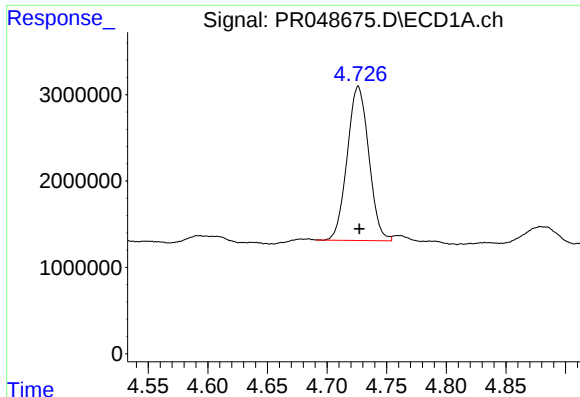


#1 Tetrachloro-m-xylene

R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 22464899
Conc: 9.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31336


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:36 AM

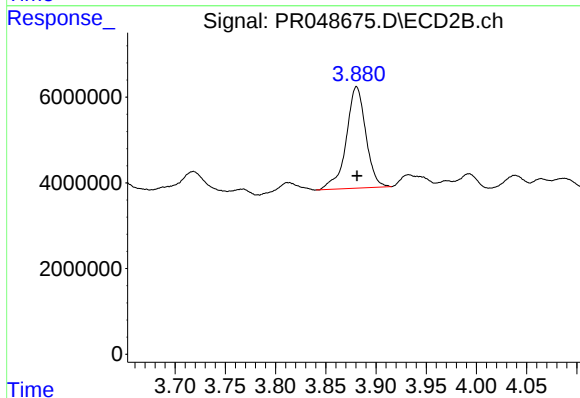


#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: 0.000 min
Response: 32095896
Conc: 11.05 ng/ml

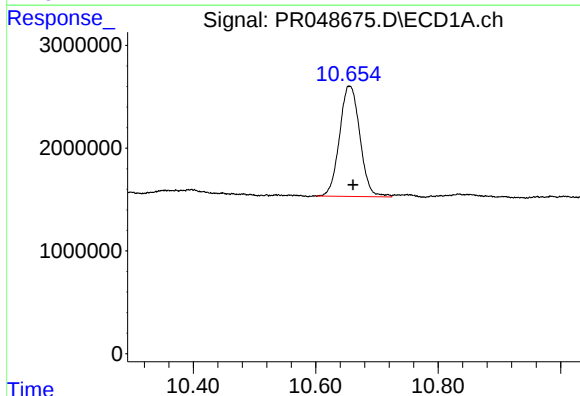


#2 Decachlorobiphenyl

R.T.: 10.655 min
Delta R.T.: -0.006 min
Response: 24749554
Conc: 9.39 ng/ml

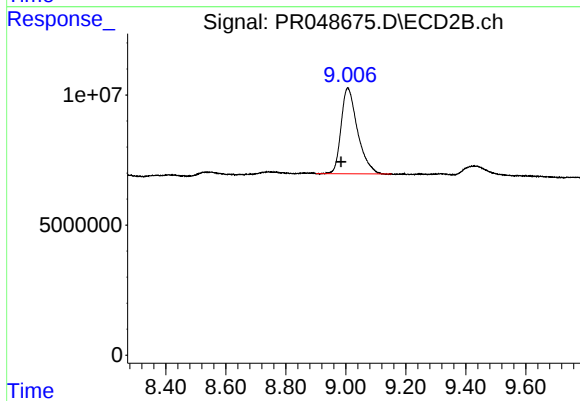

#2 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: 0.022 min
Response: 125608637
Conc: 8.60 ng/ml m

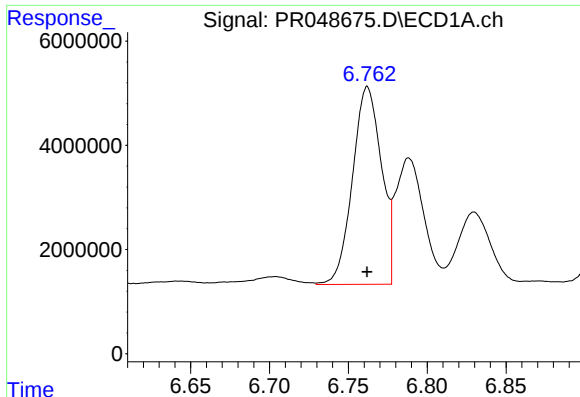


#26 AR-1254-1

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 48377497
Conc: 551.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31336


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:36 AM

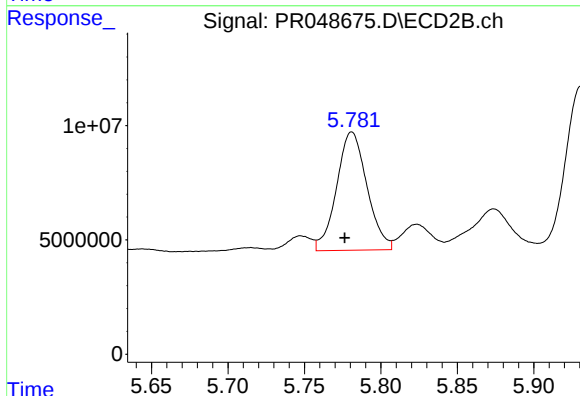


#26 AR-1254-1

R.T.: 5.781 min
Delta R.T.: 0.005 min
Response: 71581952
Conc: 463.90 ng/ml

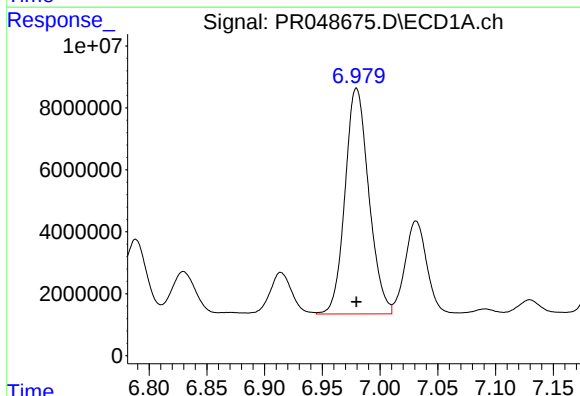


#27 AR-1254-2

R.T.: 6.980 min
Delta R.T.: 0.000 min
Response: 104481573
Conc: 789.81 ng/ml

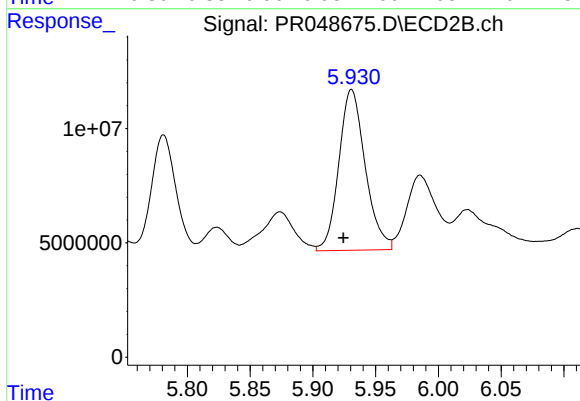

#27 AR-1254-2

R.T.: 5.931 min
Delta R.T.: 0.006 min
Response: 102935530
Conc: 609.10 ng/ml

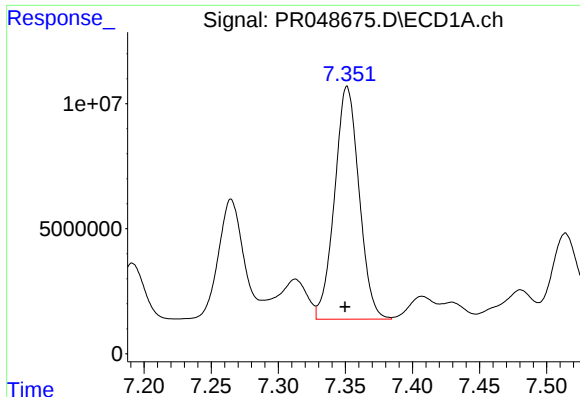


#28 AR-1254-3

R.T.: 7.351 min
Delta R.T.: 0.001 min
Response: 118424153
Conc: 846.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31336


Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:36 AM

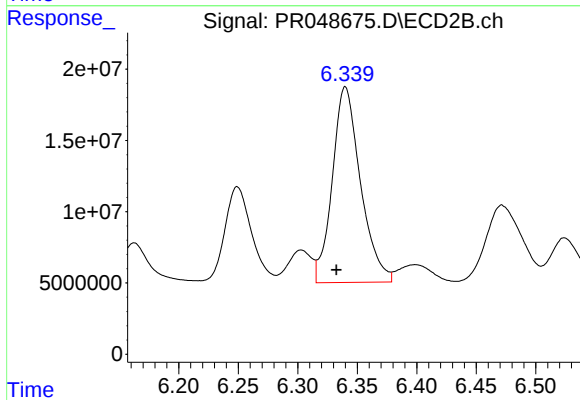


#28 AR-1254-3

R.T.: 6.340 min
Delta R.T.: 0.008 min
Response: 226070279
Conc: 675.48 ng/ml

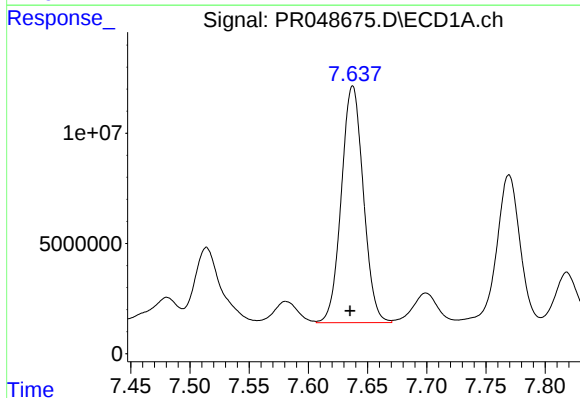


#29 AR-1254-4

R.T.: 7.638 min
Delta R.T.: 0.002 min
Response: 138929761
Conc: 1282.45 ng/ml

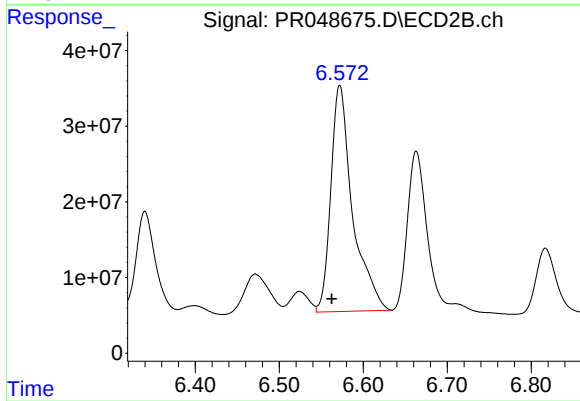

#29 AR-1254-4

R.T.: 6.572 min
Delta R.T.: 0.010 min
Response: 537408865
Conc: 975.89 ng/ml

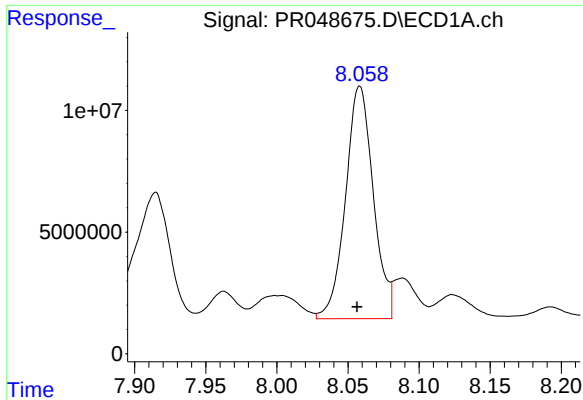


#30 AR-1254-5

R.T.: 8.058 min
Delta R.T.: 0.002 min
Response: 130033915
Conc: 1128.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
PIPE-AUD-31336

Manual Integrations
APPROVED

Ankita
11/18/2020 10:22:36 AM

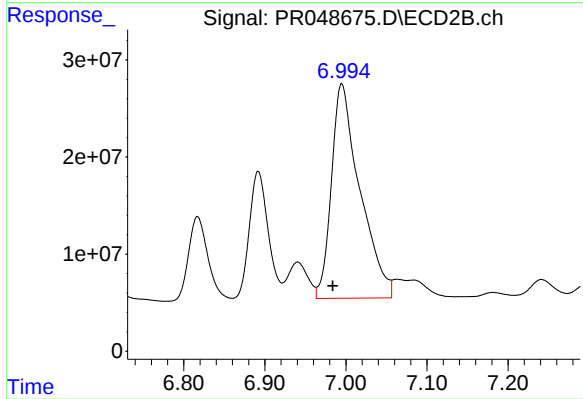

#30 AR-1254-5

R.T.: 6.995 min
Delta R.T.: 0.011 min
Response: 538653577
Conc: 925.09 ng/ml