

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR113020\
 Data File : PR048761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 17:12
 Operator : DD\AJ
 Sample : AIBLK51
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 06:14:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR113020CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 01 06:11:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.691	3.843	50521277	82087443	19.118	19.298
2)	SA Decachlor...	10.601	8.910	102.8E6	329.0E6	39.189	38.383
Target Compounds							
9)	L2 AR-1221-2	5.003	0.000	778890	0	34.848	N.D. #
10)	L2 AR-1221-3	5.003f	0.000	778890	0	10.673	N.D. #
11)	L3 AR-1232-1	5.003f	0.000	778890	0	12.880	N.D. #
28)	L6 AR-1254-3	7.330	0.000	61179	0	0.350	N.D. #
32)	L7 AR-1260-2	7.719	0.000	24793	0	0.165	N.D. #
38)	L8 AR-1262-3	0.000	7.767	0	773650	N.D.	1.210 #
39)	L8 AR-1262-4	0.000	7.767f	0	773650	N.D.	0.731 #
41)	L9 AR-1268-1	0.000	7.767	0	773650	N.D.	0.396 #
42)	L9 AR-1268-2	0.000	7.767f	0	773650	N.D.	0.453 #
45)	L9 AR-1268-5	10.246	8.644	910344	979259	0.900	0.247 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR113020\
Data File : PR048761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 17:12
Operator : DD\AJ
Sample : AIBLK51
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 06:14:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR113020CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 01 06:11:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

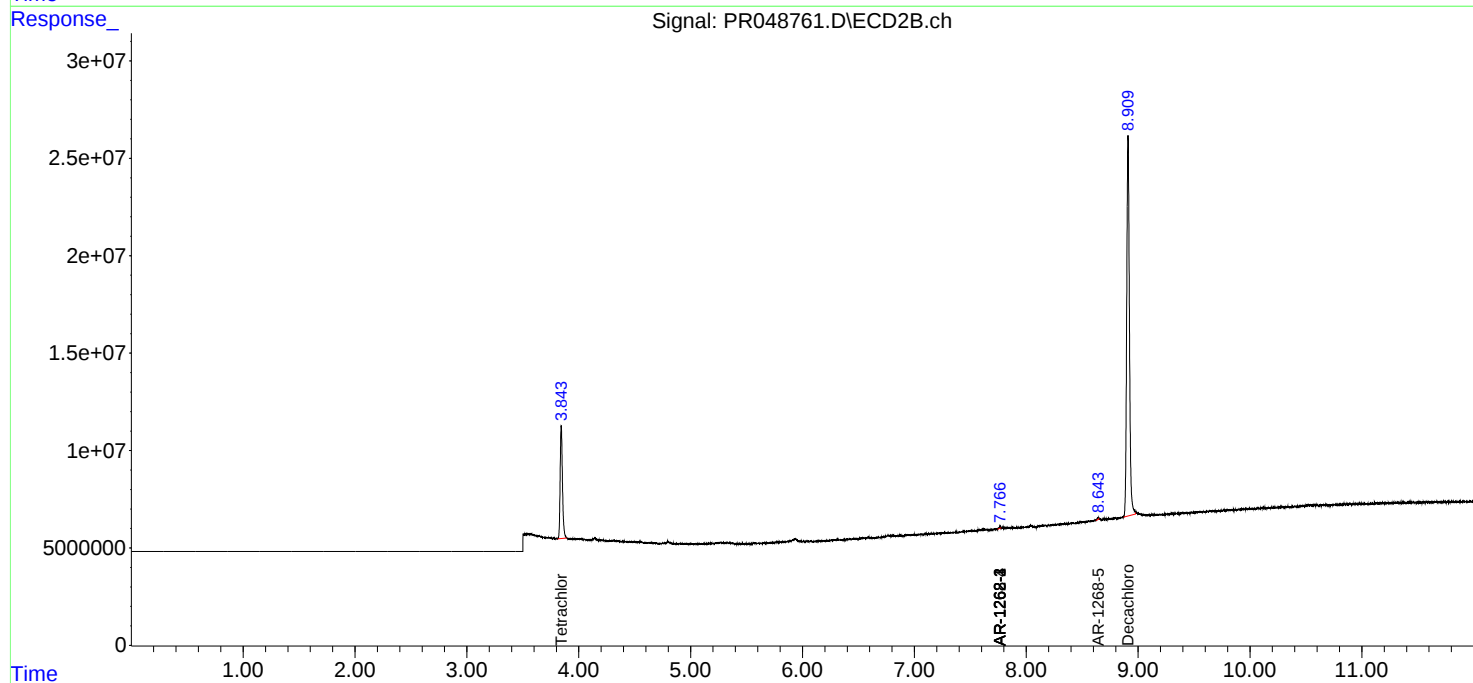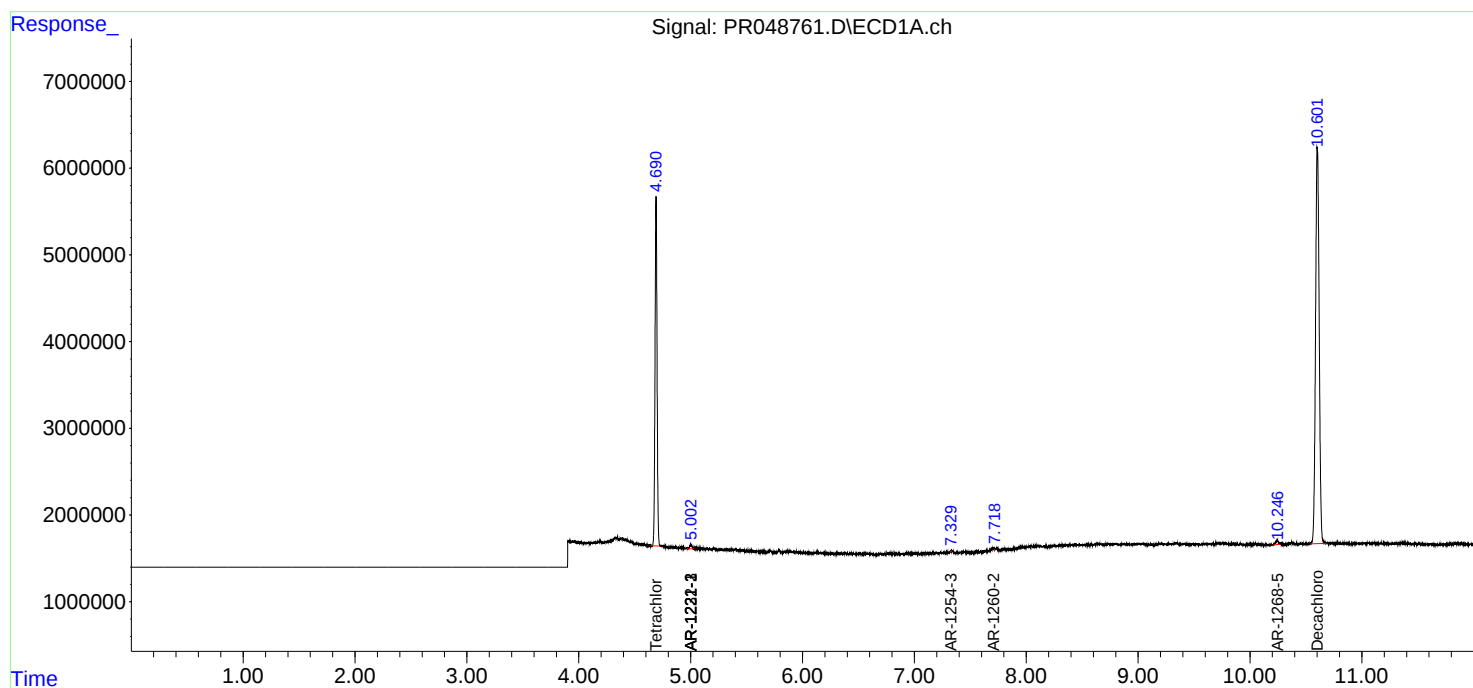


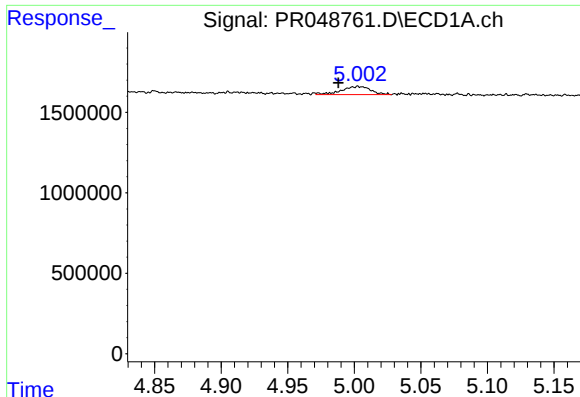

#9 AR-1221-2


R.T.: 5.003 min
Delta R.T.: 0.015 min
Response: 778890
Conc: 34.85 ng/ml

Instrument :
ECD_R
ClientSampleId :

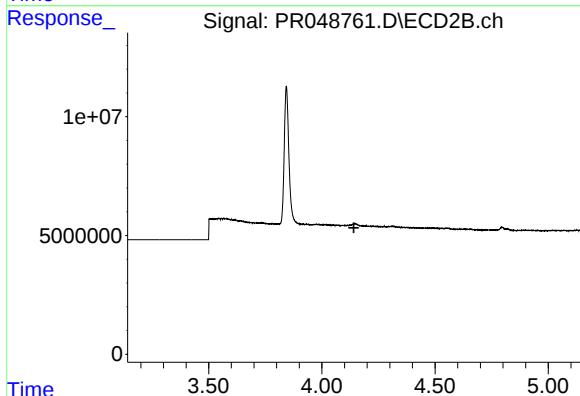


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.141 min
Response: 0
Conc: N.D.

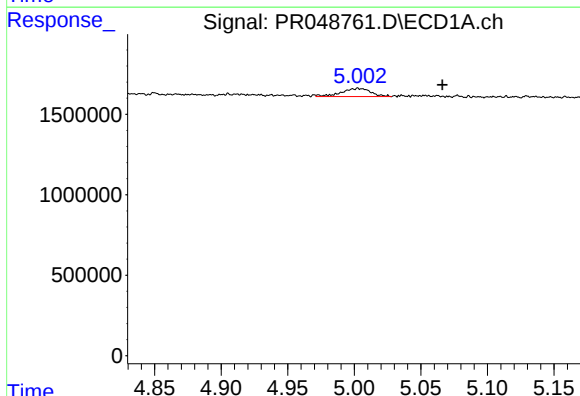


#10 AR-1221-3

R.T.: 5.003 min
Delta R.T.: -0.063 min
Response: 778890
Conc: 10.67 ng/ml

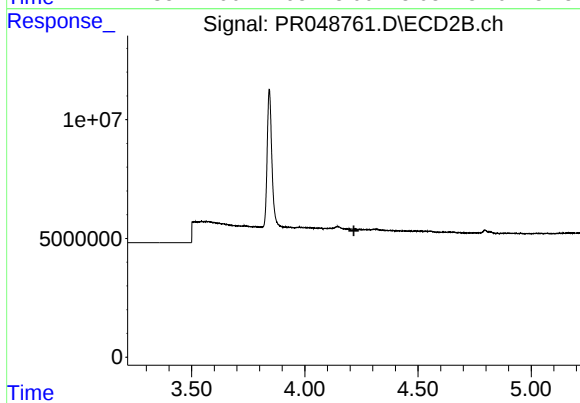

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

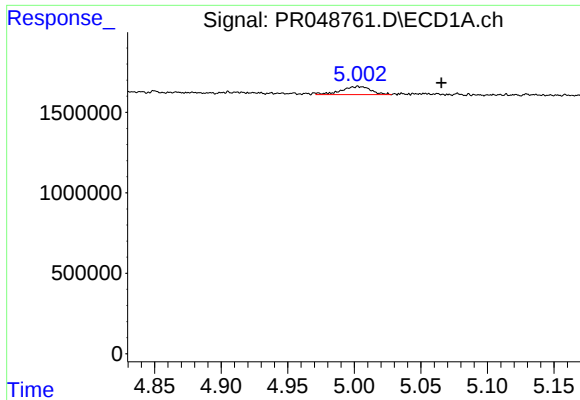

#11 AR-1232-1


R.T.: 5.003 min
Delta R.T.: -0.063 min
Response: 778890
Conc: 12.88 ng/ml

Instrument :
ECD_R
ClientSampleId :

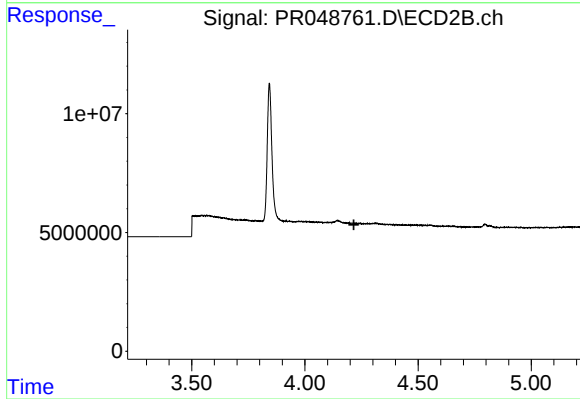


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

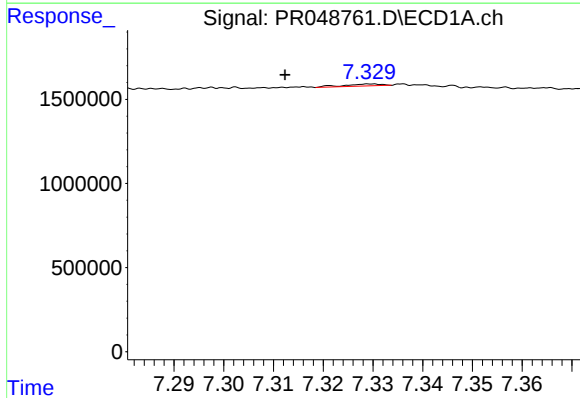


#28 AR-1254-3

R.T.: 7.330 min
Delta R.T.: 0.017 min
Response: 61179
Conc: 0.35 ng/ml

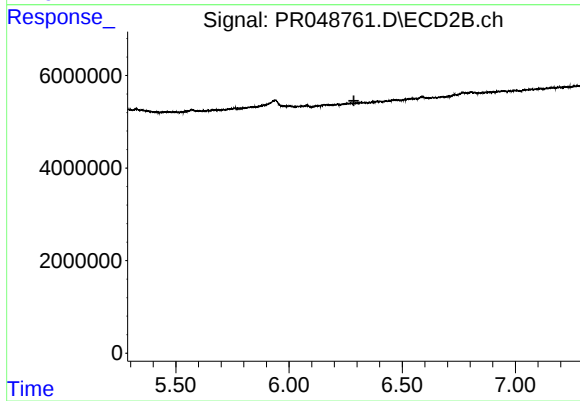

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.286 min
Response: 0
Conc: N.D.

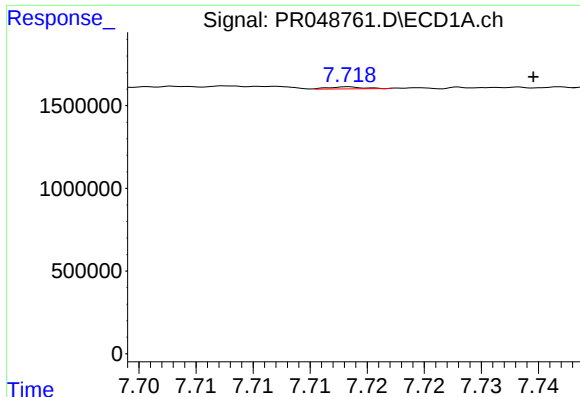

#32 AR-1260-2


R.T.: 7.719 min
Delta R.T.: -0.016 min
Response: 24793
Conc: 0.17 ng/ml

Instrument :
ECD_R
ClientSampleId :

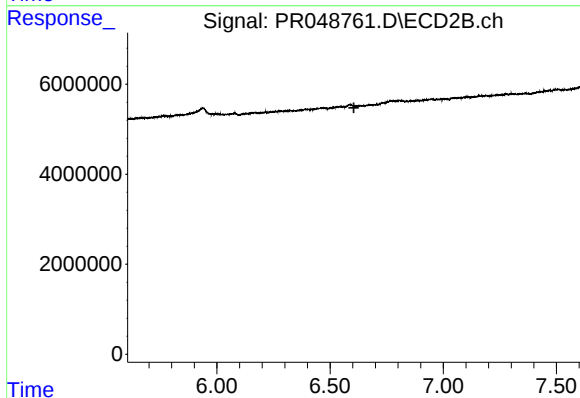


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.605 min
Response: 0
Conc: N.D.

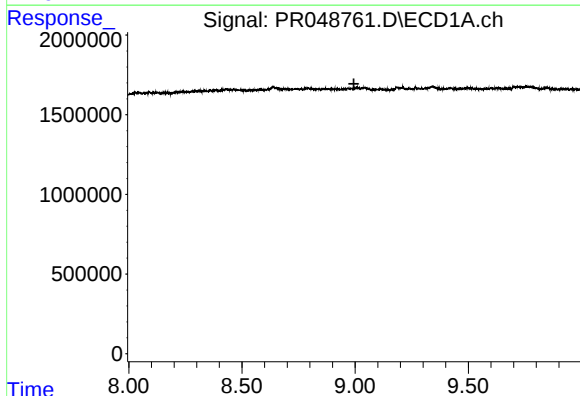


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.994 min
Response: 0
Conc: N.D.

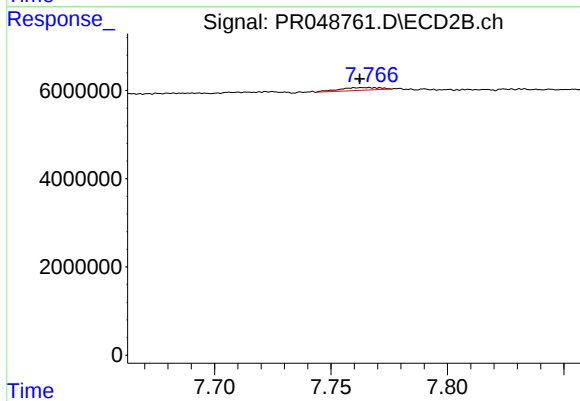

#38 AR-1262-3


R.T.: 7.767 min
Delta R.T.: 0.004 min
Response: 773650
Conc: 1.21 ng/ml

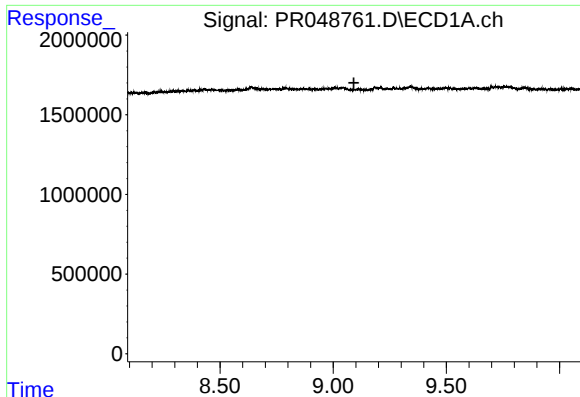

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

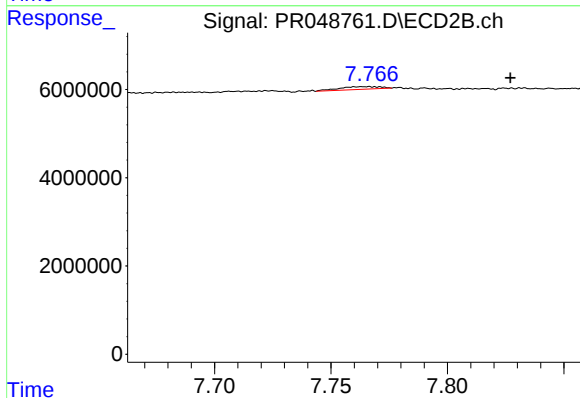


#39 AR-1262-4

R.T.: 7.767 min
Delta R.T.: -0.060 min
Response: 773650
Conc: 0.73 ng/ml

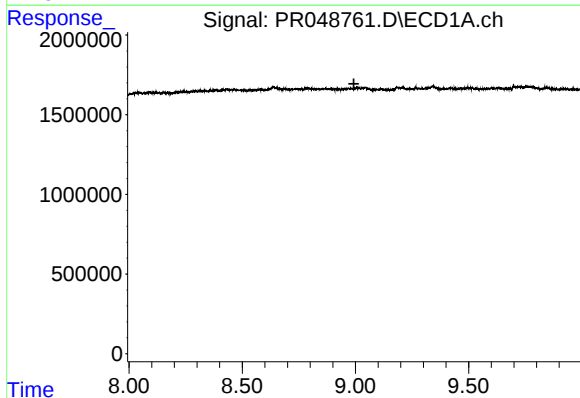


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.993 min
Response: 0
Conc: N.D.

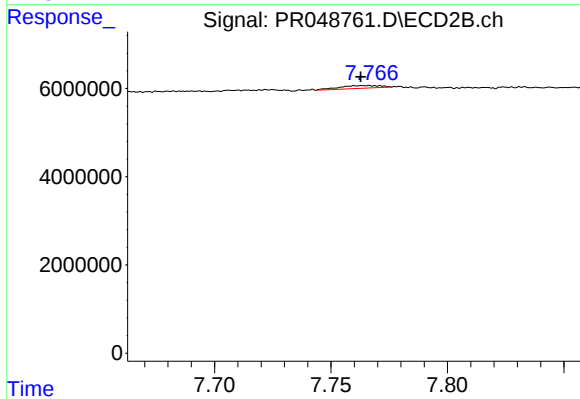

#41 AR-1268-1


R.T.: 7.767 min
Delta R.T.: 0.004 min
Response: 773650
Conc: 0.40 ng/ml

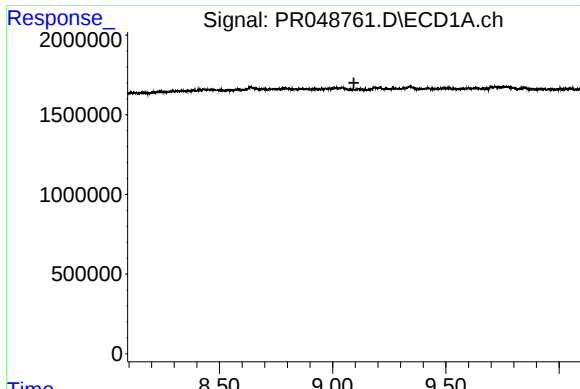

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

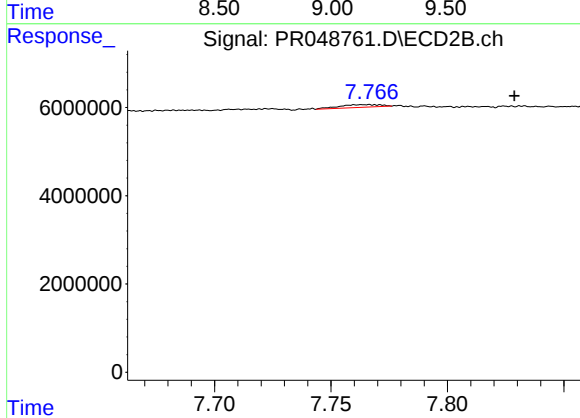


#42 AR-1268-2

R.T.: 7.767 min
Delta R.T.: -0.062 min
Response: 773650
Conc: 0.45 ng/ml

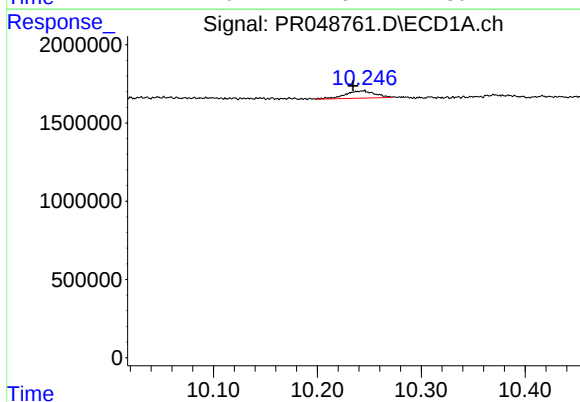

#45 AR-1268-5

R.T.: 10.246 min
Delta R.T.: 0.011 min
Response: 910344
Conc: 0.90 ng/ml

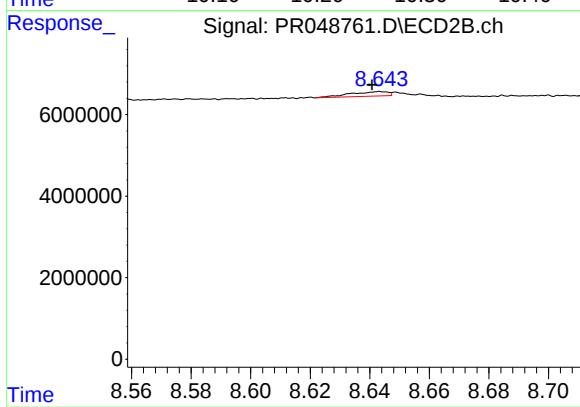

#45 AR-1268-5

R.T.: 8.644 min
Delta R.T.: 0.003 min
Response: 979259
Conc: 0.25 ng/ml