

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR113021\
 Data File : PR052790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2021 05:03
 Operator : AJ\MA
 Sample : M4068-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 08:26:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR112921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 29 22:45:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.685	3.854	55276825	40367407	16.770	14.784
2) SA Decachlor...	10.615	8.854	60291869	52666739	18.603	16.293
Target Compounds						
26) L6 AR-1254-1	6.729	5.727	3111113	3165815	23.704	20.881
27) L6 AR-1254-2	6.944	5.873	4517595	2747428	22.329	20.951
28) L6 AR-1254-3	7.319	6.274	4745895	4300807	22.386	19.483
29) L6 AR-1254-4	7.603	6.499	4324282	2430644	27.382	17.844 #
30) L6 AR-1254-5	8.024	6.914	4077333	3361474	23.135	16.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR113021\
Data File : PR052790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2021 05:03
Operator : AJ\MA
Sample : M4068-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 08:26:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR112921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 29 22:45:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

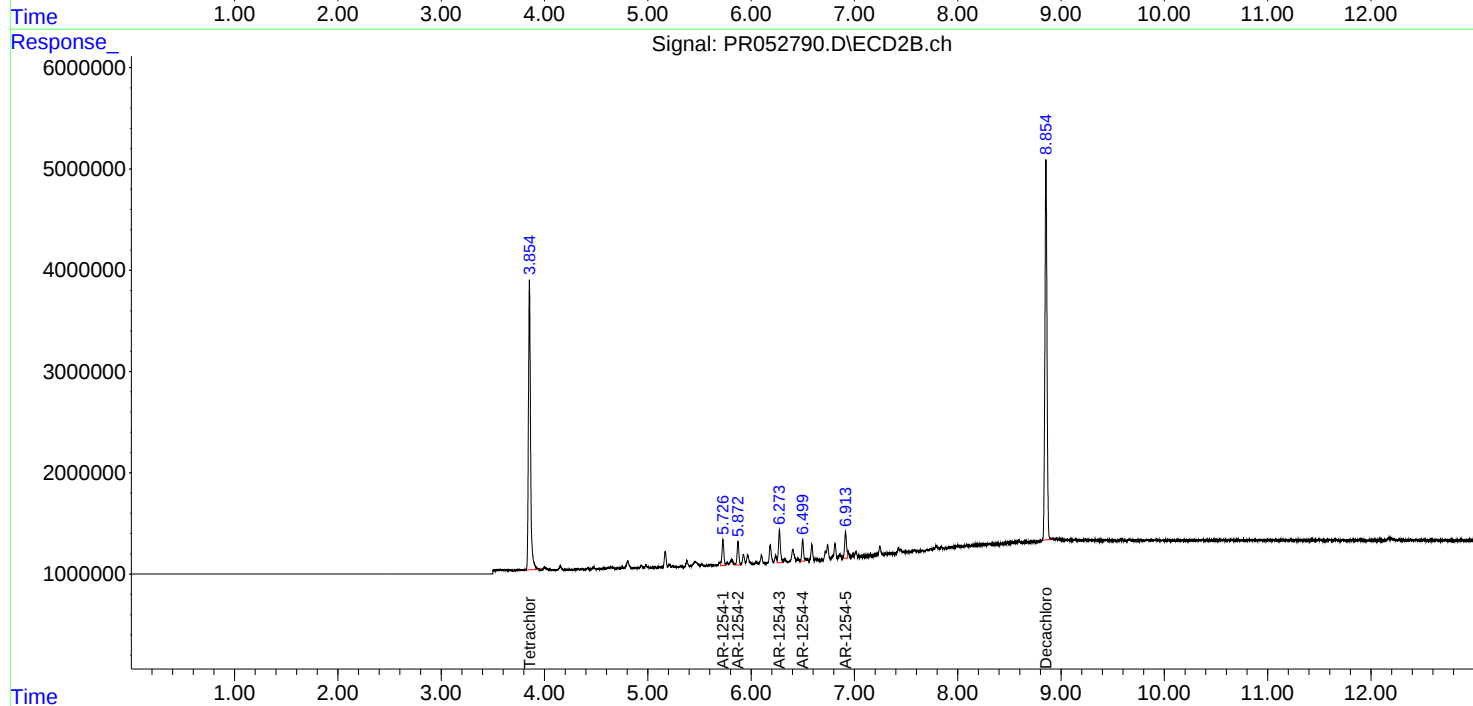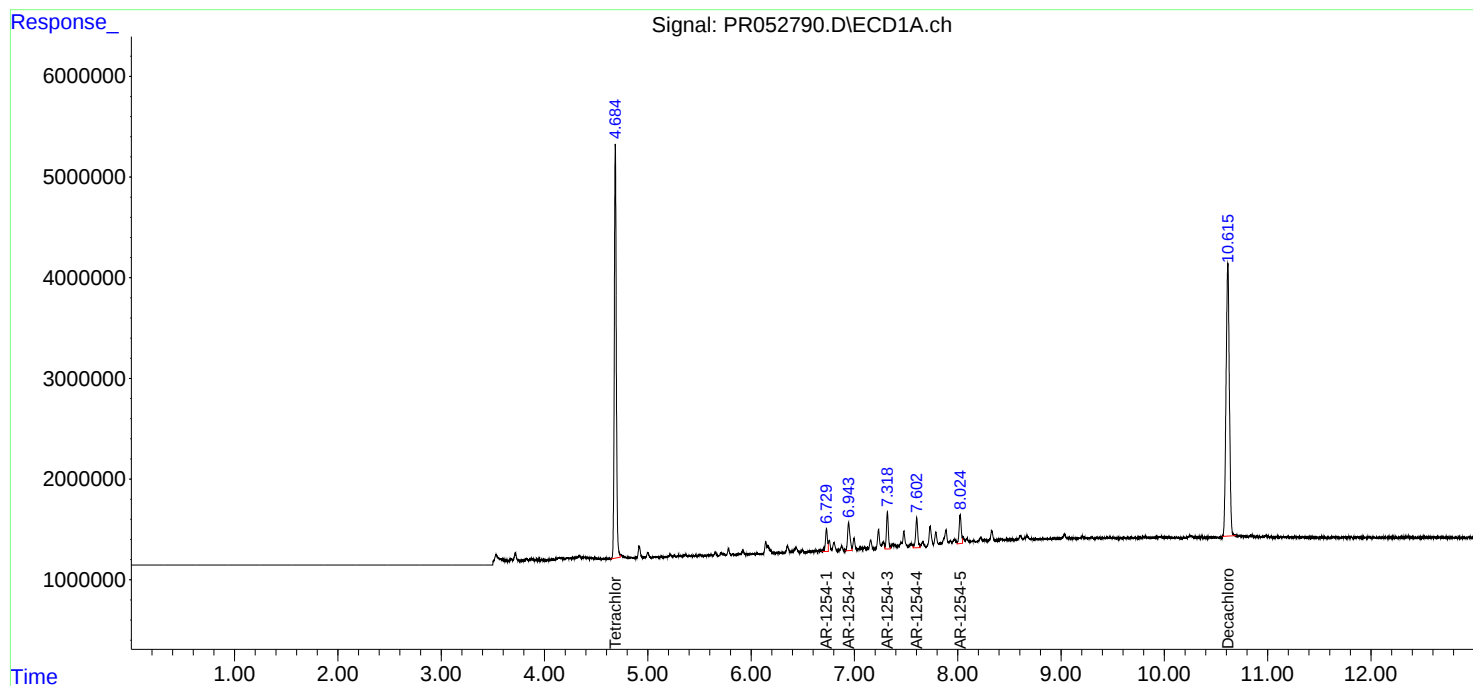


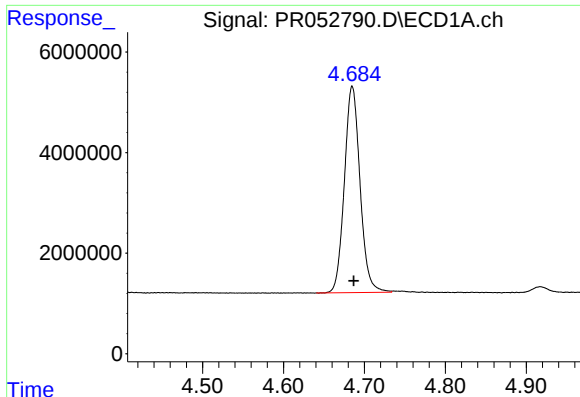

#1 Tetrachloro-m-xylene


R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 55276825
Conc: 16.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2021

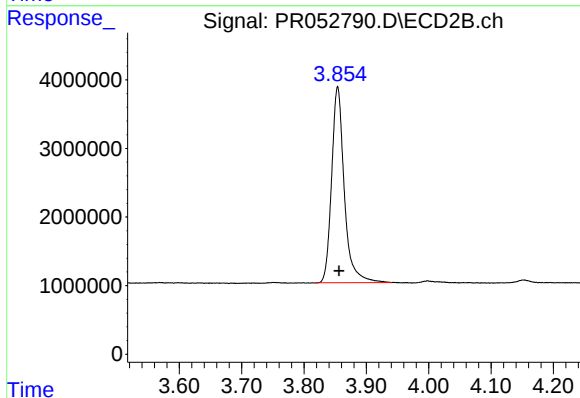


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.002 min
Response: 40367407
Conc: 14.78 ng/ml

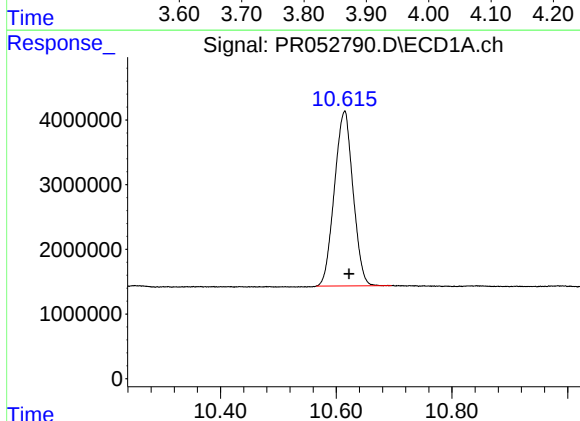


#2 Decachlorobiphenyl

R.T.: 10.615 min
Delta R.T.: -0.007 min
Response: 60291869
Conc: 18.60 ng/ml

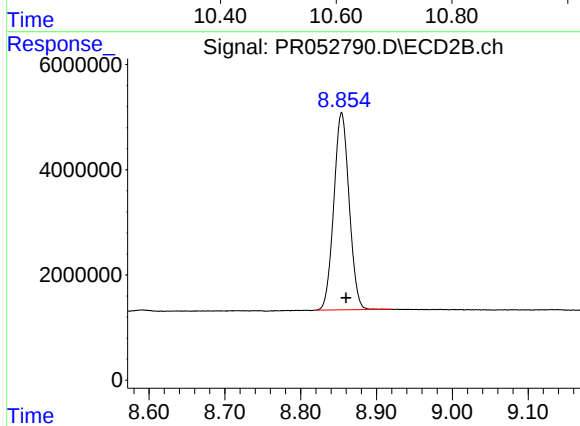

#2 Decachlorobiphenyl


R.T.: 8.854 min
Delta R.T.: -0.006 min
Response: 52666739
Conc: 16.29 ng/ml

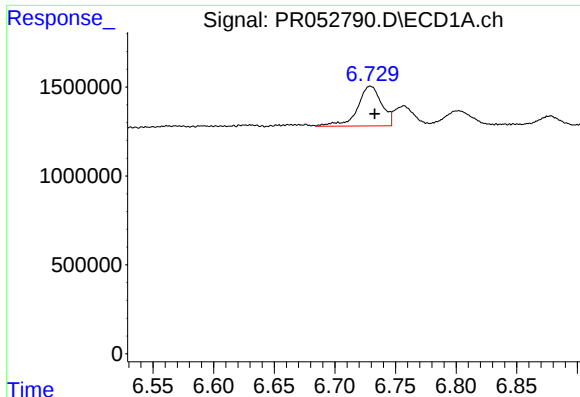

#26 AR-1254-1


R.T.: 6.729 min
Delta R.T.: -0.004 min
Response: 3111113
Conc: 23.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2021

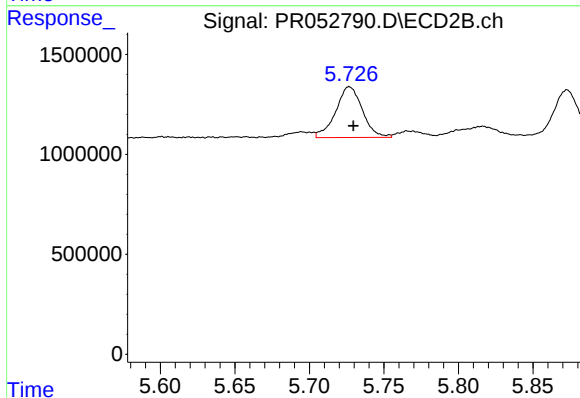


#26 AR-1254-1

R.T.: 5.727 min
Delta R.T.: -0.003 min
Response: 3165815
Conc: 20.88 ng/ml

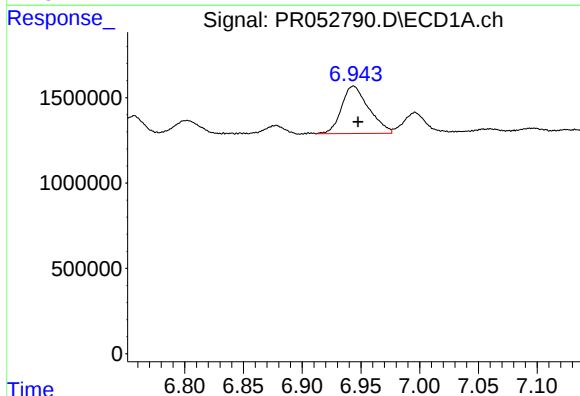


#27 AR-1254-2

R.T.: 6.944 min
Delta R.T.: -0.004 min
Response: 4517595
Conc: 22.33 ng/ml

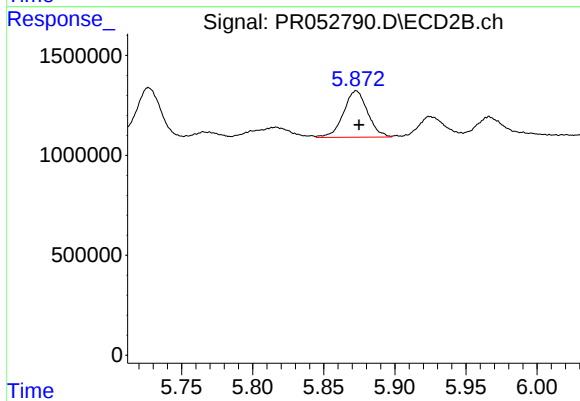

#27 AR-1254-2


R.T.: 5.873 min
Delta R.T.: -0.002 min
Response: 2747428
Conc: 20.95 ng/ml

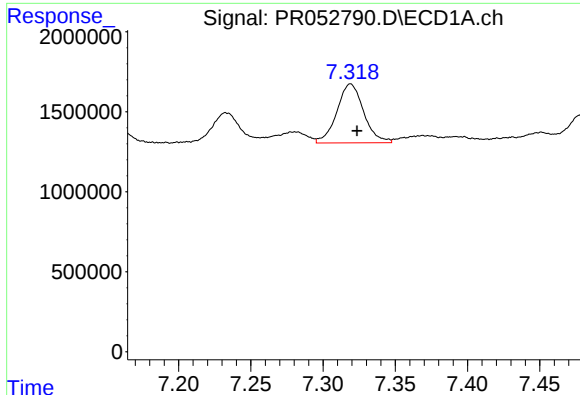

#28 AR-1254-3


R.T.: 7.319 min
Delta R.T.: -0.004 min
Response: 4745895
Conc: 22.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2021

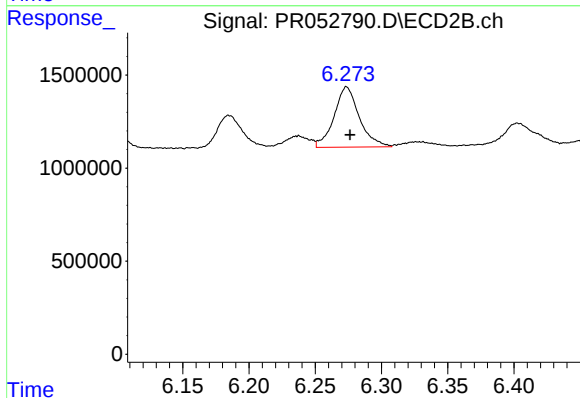


#28 AR-1254-3

R.T.: 6.274 min
Delta R.T.: -0.003 min
Response: 4300807
Conc: 19.48 ng/ml

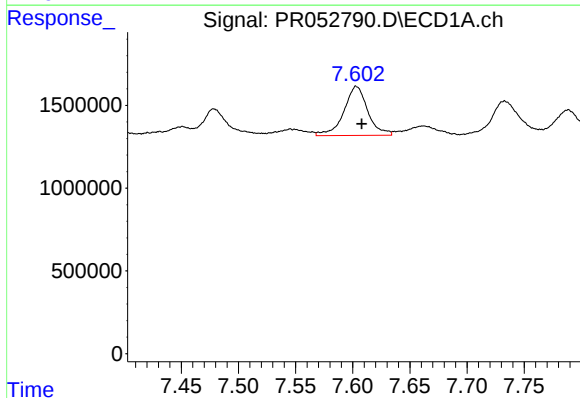


#29 AR-1254-4

R.T.: 7.603 min
Delta R.T.: -0.005 min
Response: 4324282
Conc: 27.38 ng/ml

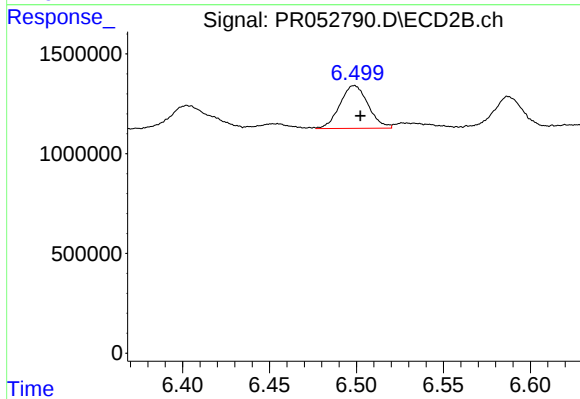

#29 AR-1254-4


R.T.: 6.499 min
Delta R.T.: -0.003 min
Response: 2430644
Conc: 17.84 ng/ml

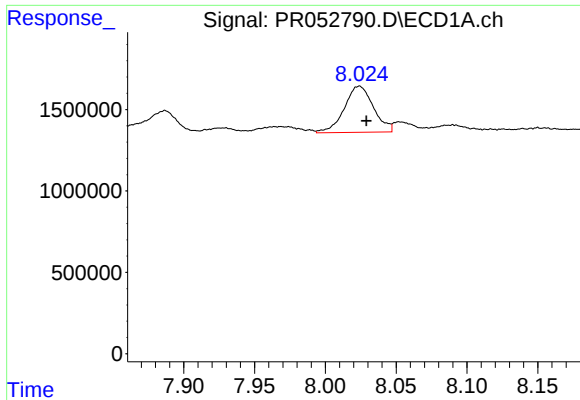

#30 AR-1254-5

R.T.: 8.024 min
Delta R.T.: -0.005 min
Response: 4077333
Conc: 23.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT4-2021

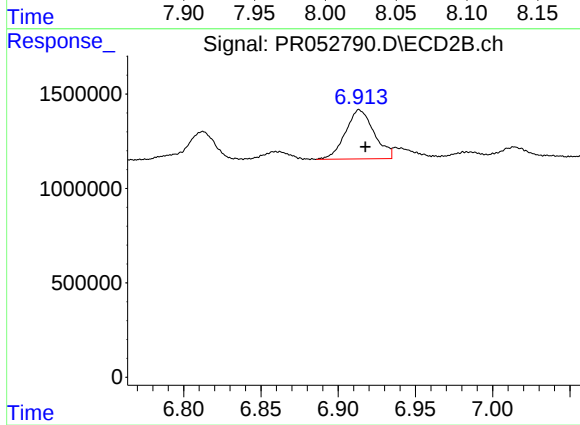

#30 AR-1254-5

R.T.: 6.914 min
Delta R.T.: -0.004 min
Response: 3361474
Conc: 16.18 ng/ml