

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR120518\
 Data File : PR034285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 17:51
 Operator : SM\SJ
 Sample : J6135-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20180972-MANASQUAN-H2O

Manual Integrations
 APPROVED

mohammad
 12/5/2018 12:51:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 01:13:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR120518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 13:48:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.519	31054246	64719318	18.451	19.049m
2) SA Decachlor...	10.120	8.422	27291142	57834299	15.953	15.739

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR120518\
Data File : PR034285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 17:51
Operator : SM\SJ
Sample : J6135-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
20180972-MANASQUAN-H2O


Manual Integrations
APPROVED

mohammad
12/5/2018 12:51:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 01:13:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR120518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 13:48:33 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

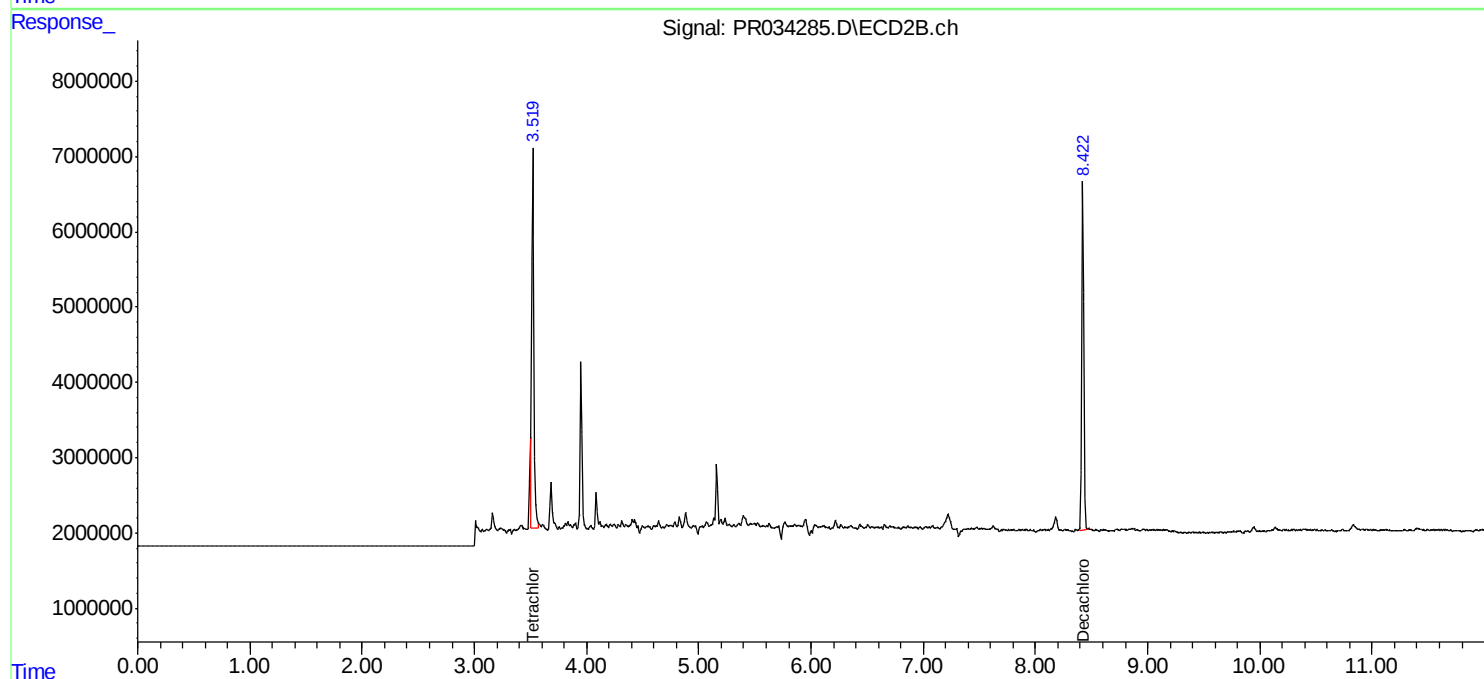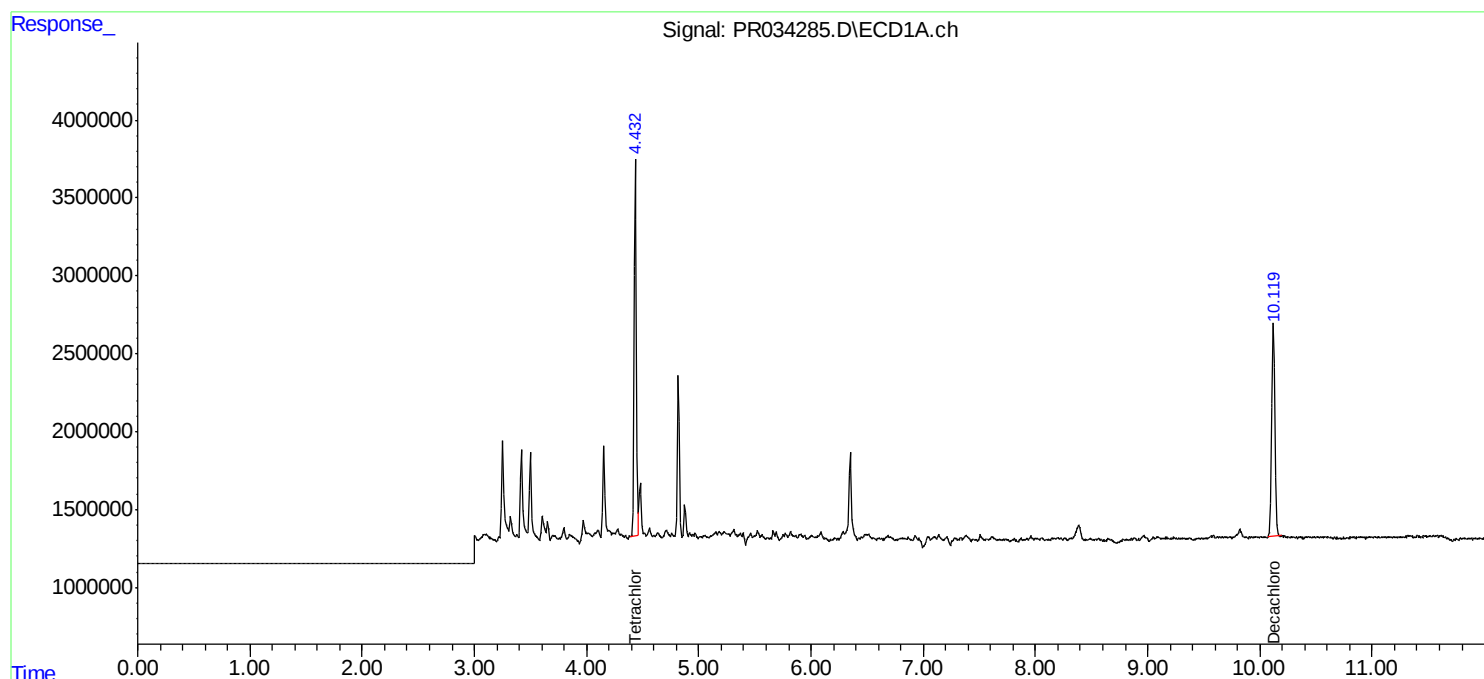

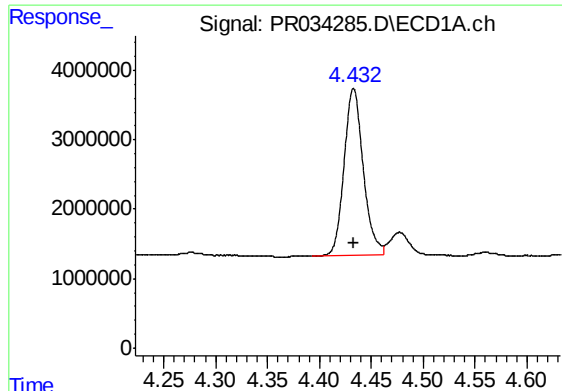


#1 Tetrachloro-m-xylene

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 31054246
Conc: 18.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
20180972-MANASQUAN-H2O


Manual Integrations
APPROVED

mohammad
12/5/2018 12:51:20 PM

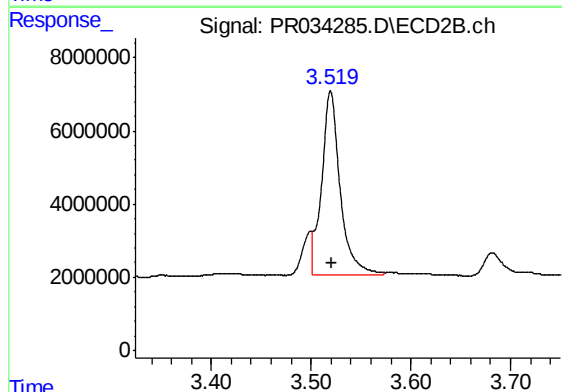


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.001 min
Response: 64719318
Conc: 19.05 ng/ml m

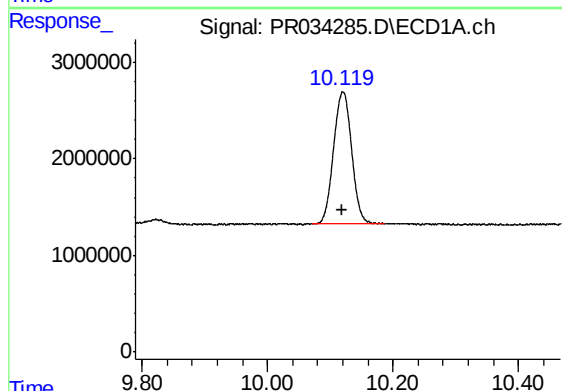

#2 Decachlorobiphenyl

R.T.: 10.120 min
Delta R.T.: 0.000 min
Response: 27291142
Conc: 15.95 ng/ml

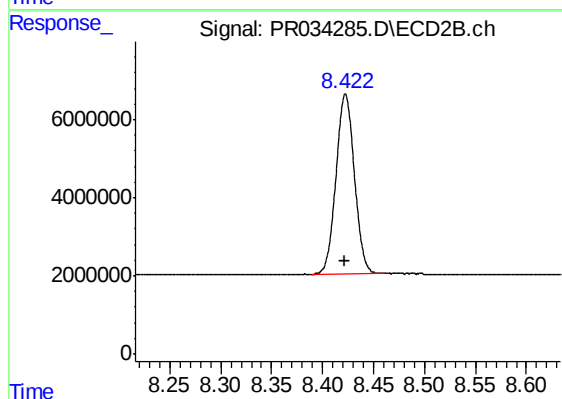

#2 Decachlorobiphenyl

R.T.: 8.422 min
Delta R.T.: 0.000 min
Response: 57834299
Conc: 15.74 ng/ml