

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR121220\  
Data File : PR048934.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Dec 2020 10:30  
Operator : DD\AJ  
Sample : L5063-04  
Misc :  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
C0AD6

Manual Integrations  
APPROVED

Ankita  
12/14/2020 3:21:26 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 14 00:36:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR113020CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Dec 01 06:11:17 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

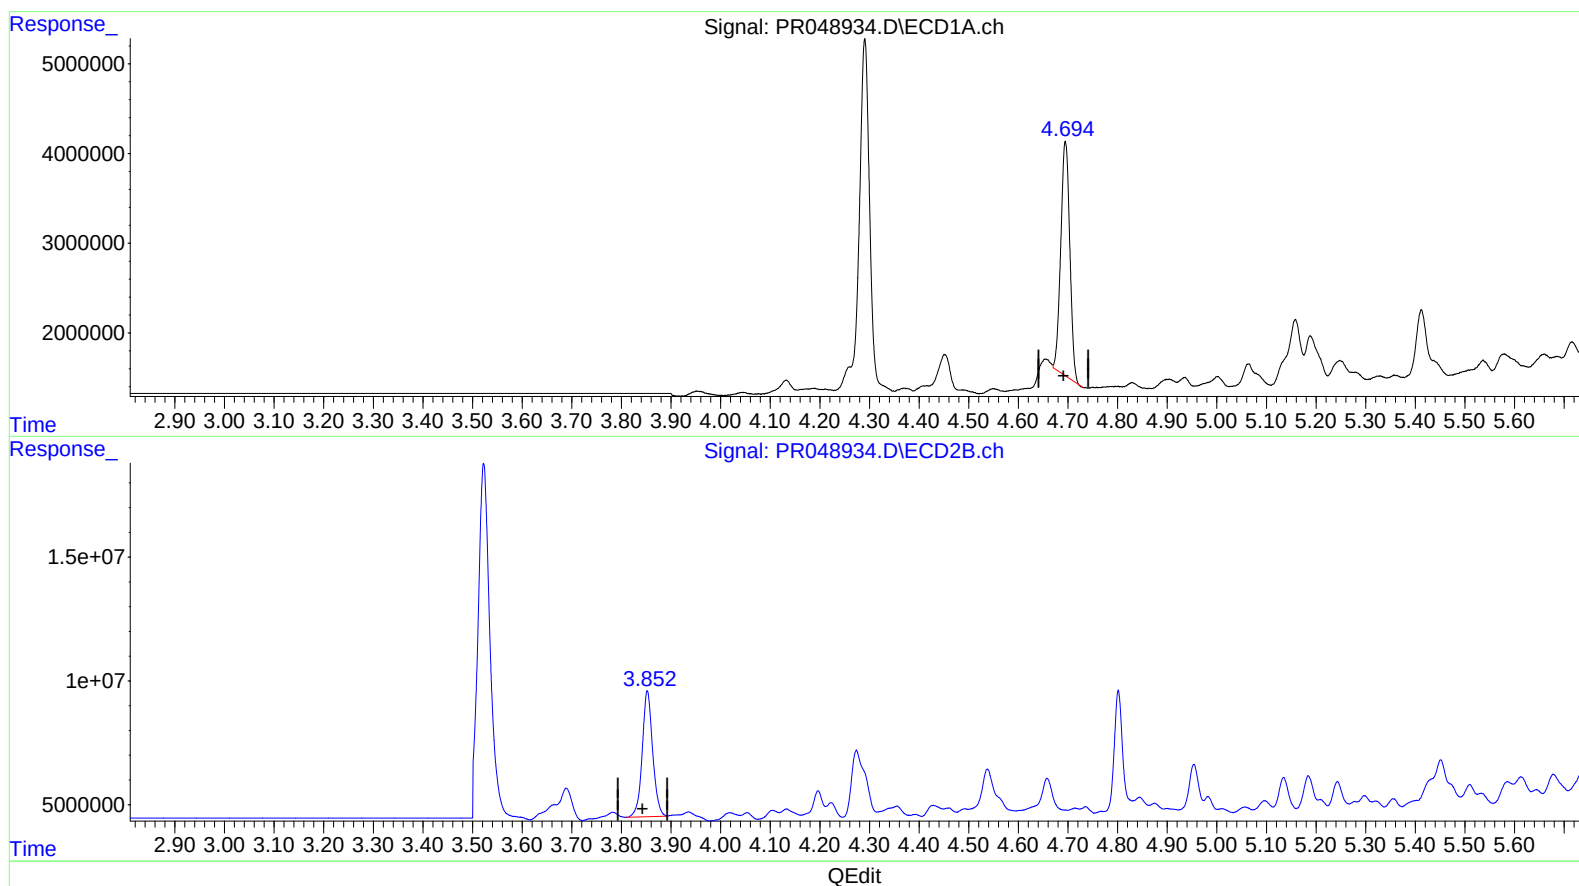

(1) Tetrachloro-m-xylene (SA)

4.695min 12.494 ng/ml

response 33017773

(1) Tetrachloro-m-xylene #2 (SA)

3.852min 17.476 ng/ml

response 74338660

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR121220\  
Data File : PR048934.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Dec 2020 10:30  
Operator : DD\AJ  
Sample : L5063-04  
Misc :  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
C0AD6

Manual Integrations  
APPROVED

Ankita  
12/14/2020 3:21:26 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 14 00:36:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR113020CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Dec 01 06:11:17 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

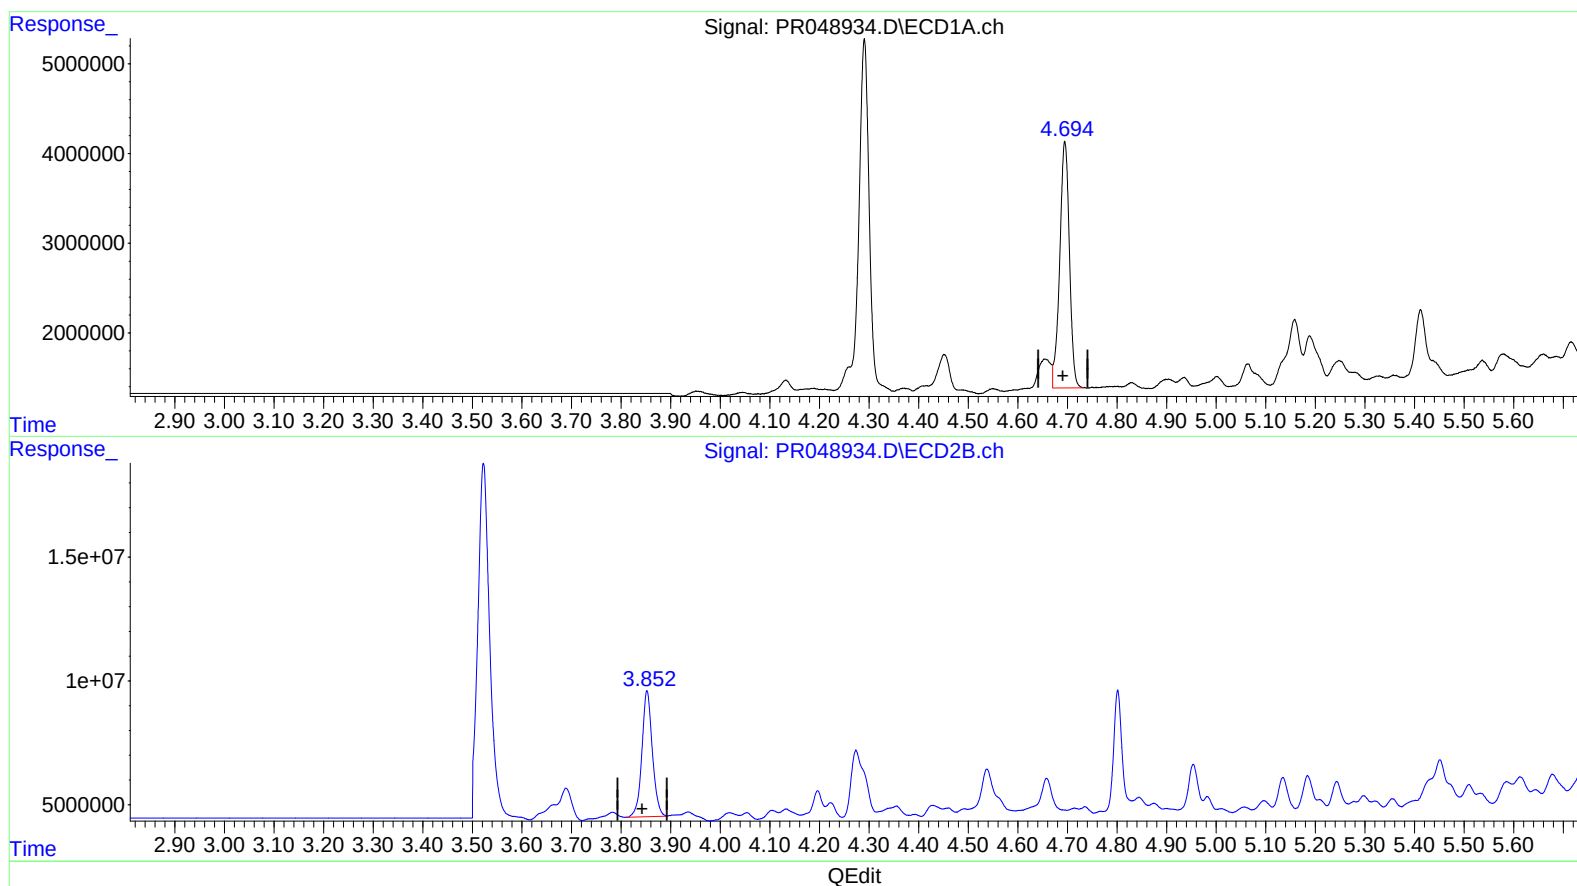

(1) Tetrachloro-m-xylene (SA)

4.694min 14.078 ng/ml m

response 37201765

(1) Tetrachloro-m-xylene #2 (SA)

3.852min 17.476 ng/ml

response 74338660

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR121220\  
 Data File : PR048934.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 12 Dec 2020 10:30  
 Operator : DD\AJ  
 Sample : L5063-04  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Ankita  
 12/14/2020 3:21:26 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 14 00:36:37 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR113020CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Dec 01 06:11:17 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------|-------|----------|----------|---------|-----------|
| -----                       |        |       |          |          |         |           |
| System Monitoring Compounds |        |       |          |          |         |           |
| 1) SA Tetrachlo...          | 4.694  | 3.852 | 37201765 | 74338660 | 14.078m | 17.476    |
| 2) SA Decachlor...          | 10.603 | 8.934 | 75460122 | 255.4E6  | 28.757  | 29.798    |
| Target Compounds            |        |       |          |          |         |           |
| 31) L7 AR-1260-1            | 7.478  | 6.426 | 61080986 | 87833990 | 504.613 | 687.230 # |
| 32) L7 AR-1260-2            | 7.733  | 6.616 | 75137958 | 288.9E6  | 500.297 | 624.257   |
| 33) L7 AR-1260-3            | 8.095  | 6.771 | 54317523 | 163.3E6  | 471.161 | 580.773   |
| 34) L7 AR-1260-4            | 8.334  | 7.247 | 64909815 | 193.7E6  | 489.358 | 569.050   |
| 35) L7 AR-1260-5            | 8.671  | 7.493 | 135.5E6  | 813.7E6  | 507.918 | 574.381   |
| -----                       |        |       |          |          |         |           |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AS  
 12/22/20