

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR121523\
Data File : PR064743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 19:45
Operator : AJ\MA
Sample : 05794-21DL 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
BGRG2DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 05:12:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121423CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 15 04:19:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

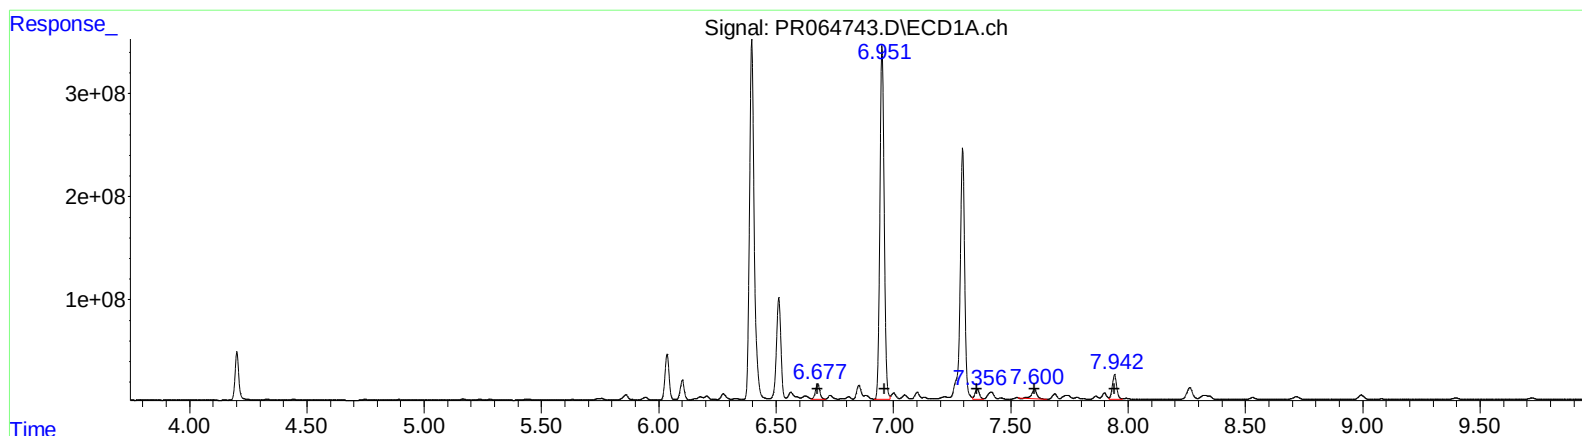

(31) AR-1260-1 (L7)
R.T. Response Conc
6.68 189103231 756.75
6.95 4354169461 15232.42
7.36 129619394 611.32
7.60 134791483 586.43
7.94 312528320 728.36

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.75 197041211 681.86
5.96 345802386 995.31
6.12 221944782 674.29
6.63 144038016 534.02
6.90 368236104 589.26

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR121523\
Data File : PR064743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 19:45
Operator : AJ\MA
Sample : 05794-21DL 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BGRG2DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 05:12:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121423CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 15 04:19:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

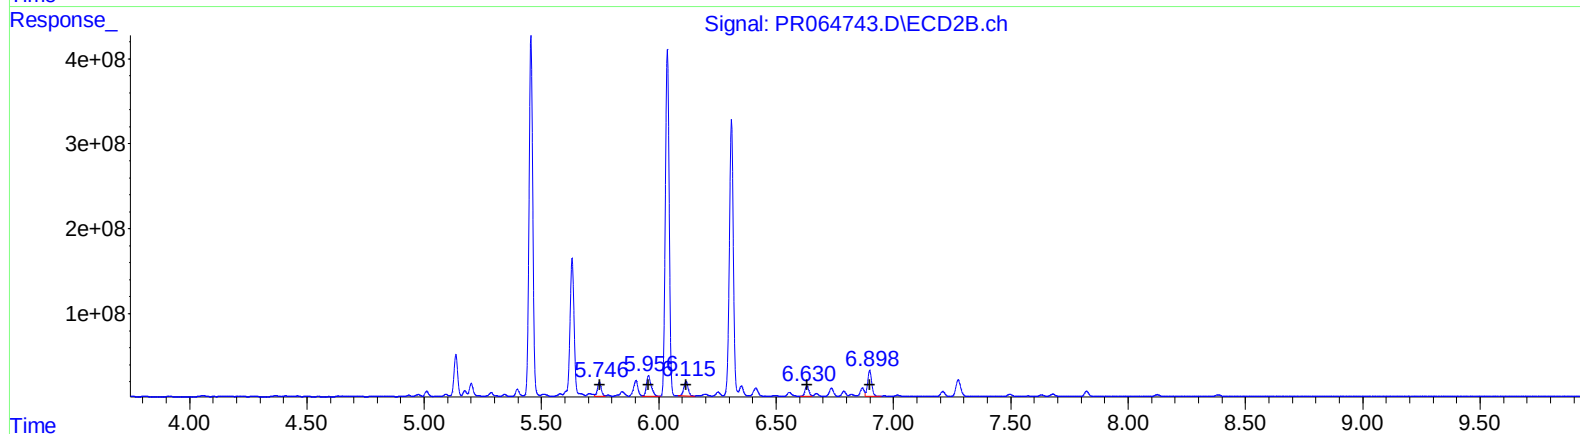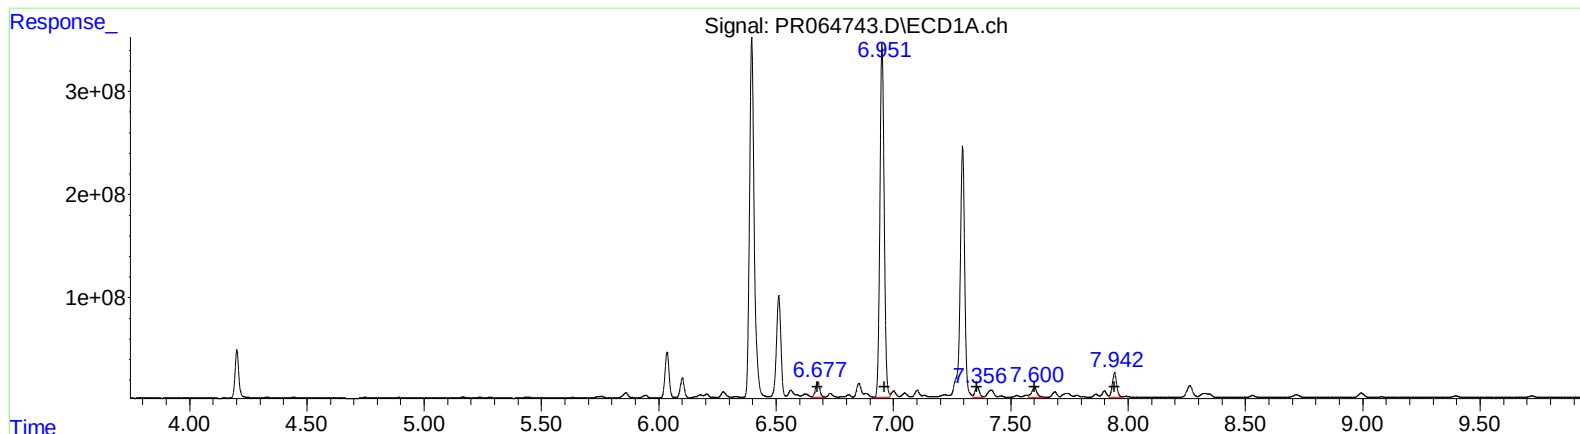

QEdit

(31) AR-1260-1 (L7)
R.T. Response Conc
6.68 189103231 756.75
6.95 4354169461 15232.42
7.36 129619394 611.32
7.60 144846019 630.17
7.94 312528320 728.36

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.75 197041211 681.86
5.96 345802386 995.31
6.12 221944782 674.29
6.63 144038016 534.02
6.90 368236104 589.26

(+) = Expected Retention Time

PR121423CLP.M Sun Dec 17 11:56:44 2023

Page: 1