

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122120\
 Data File : P0074007.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 2:04
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:00:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.997	2019356	1215888	22.087	22.669
2) SA Decachlor...	10.967	9.263	1741716	995118	21.076	21.267
Target Compounds						
9) L2 AR-1221-2	5.291	0.000	25425	0	32.367	N.D. #
24) L5 AR-1248-4	7.182f	0.000	93347	0	23.342	N.D. #
26) L6 AR-1254-1	7.182	0.000	93347	0	24.592	N.D. #
28) L6 AR-1254-3	7.808f	0.000	20698	0	3.378	N.D. #
29) L6 AR-1254-4	8.082	0.000	11493	0	2.191	N.D. #
30) L6 AR-1254-5	8.508	0.000	3114	0	0.605	N.D. #
34) L7 AR-1260-4	8.827	0.000	5119	0	1.081	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122120\
Data File : PO074007.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 2:04
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:00:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

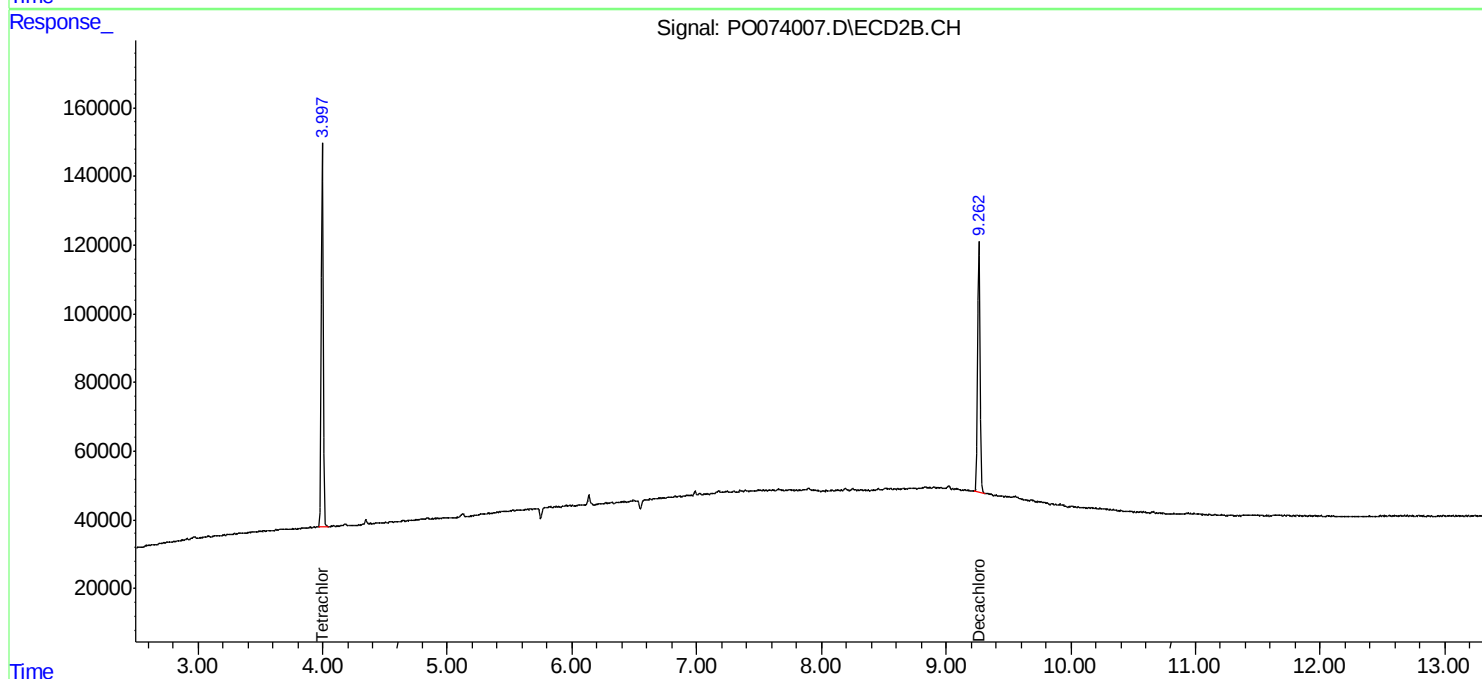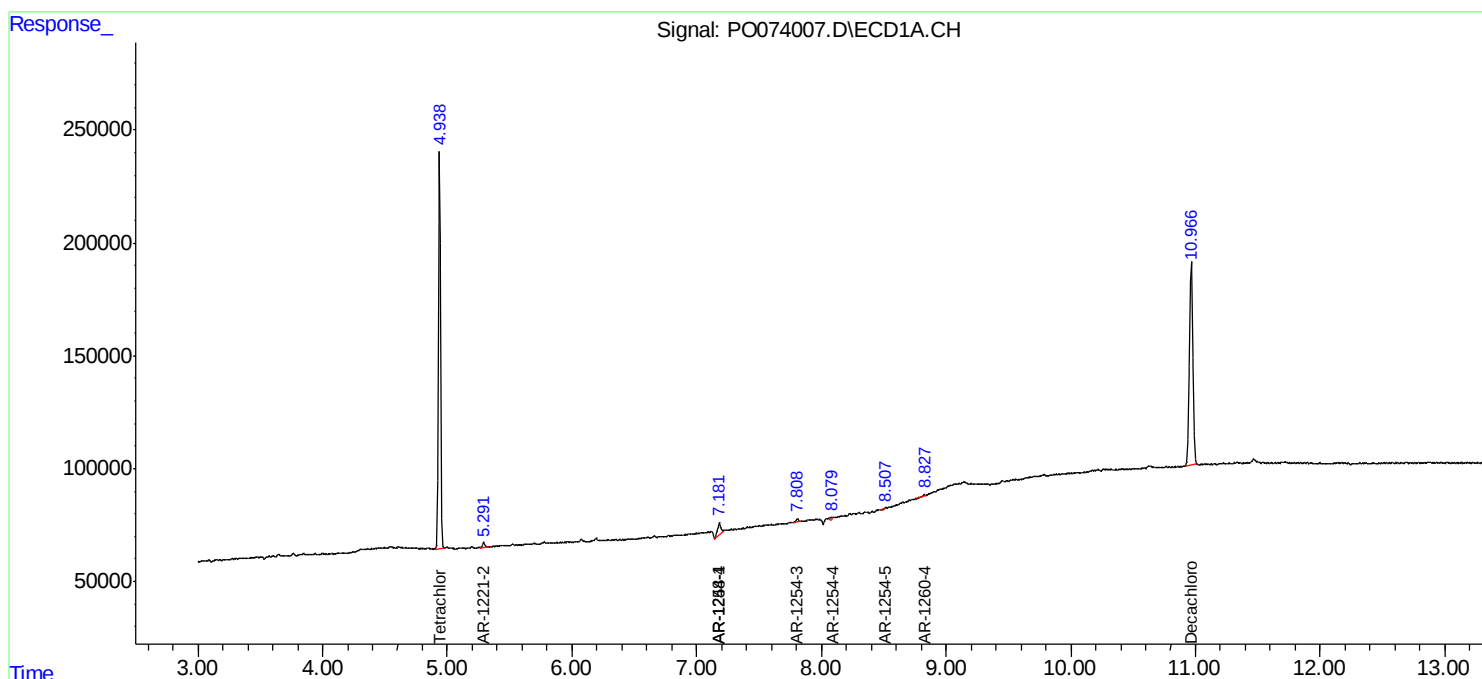


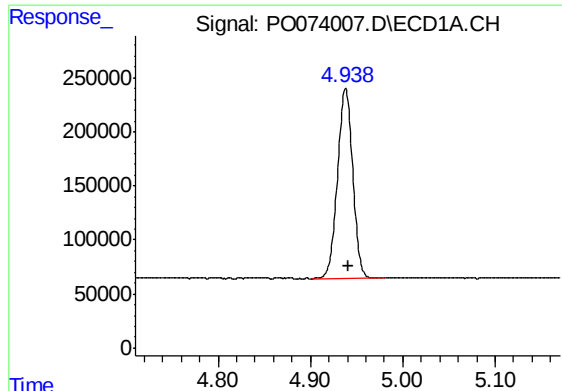

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 2019356
Conc: 22.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

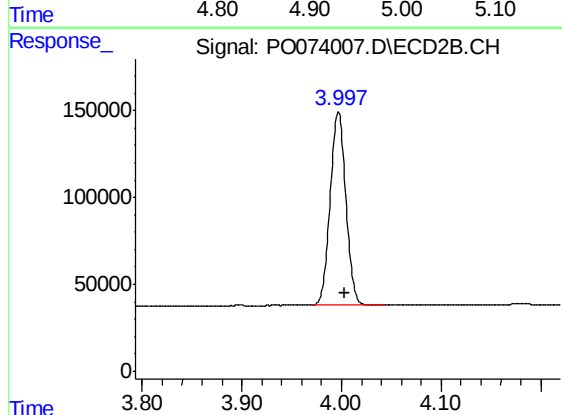


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 1215888
Conc: 22.67 ng/ml

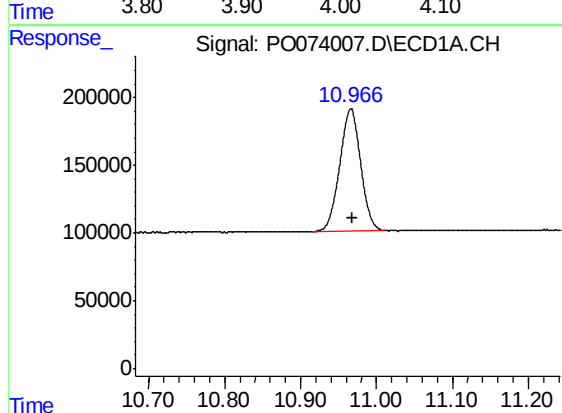


#2 Decachlorobiphenyl

R.T.: 10.967 min
Delta R.T.: -0.002 min
Response: 1741716
Conc: 21.08 ng/ml

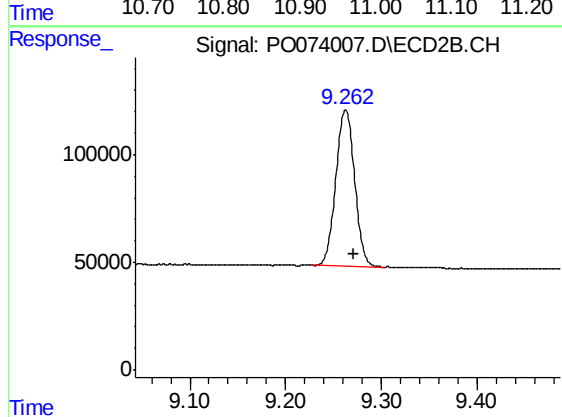

#2 Decachlorobiphenyl


R.T.: 9.263 min
Delta R.T.: -0.009 min
Response: 995118
Conc: 21.27 ng/ml

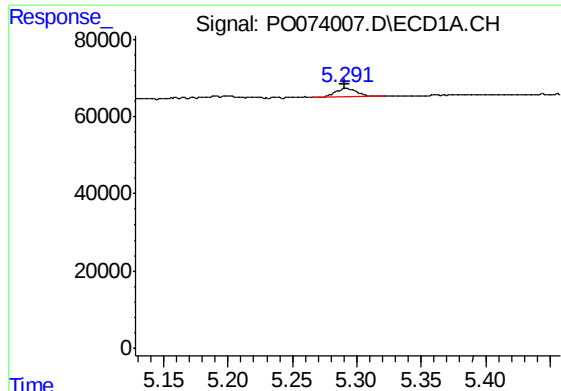

#9 AR-1221-2


R.T.: 5.291 min
Delta R.T.: 0.000 min
Response: 25425
Conc: 32.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

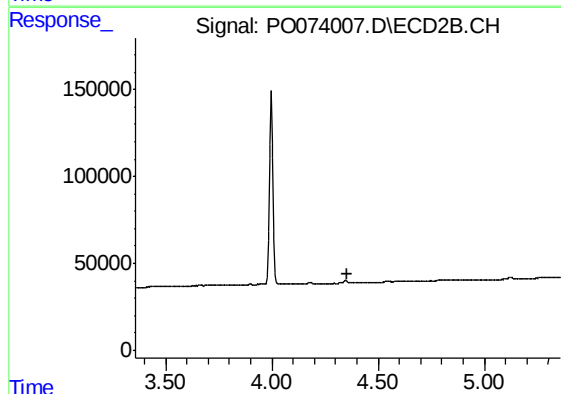


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

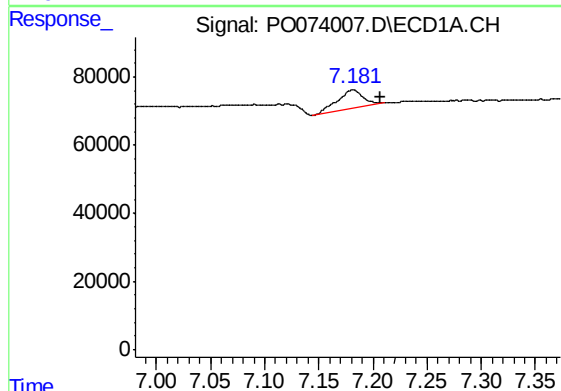


#24 AR-1248-4

R.T.: 7.182 min
Delta R.T.: -0.025 min
Response: 93347
Conc: 23.34 ng/ml

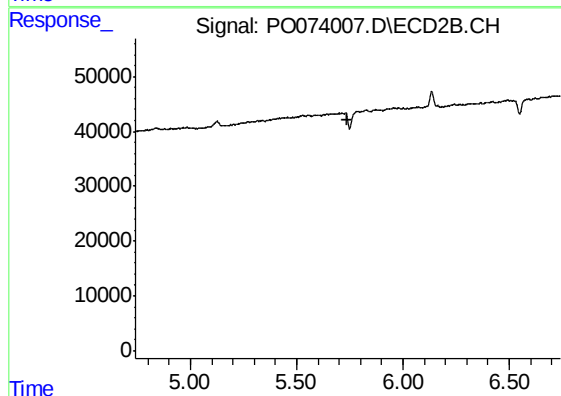

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.741 min
Response: 0
Conc: N.D.

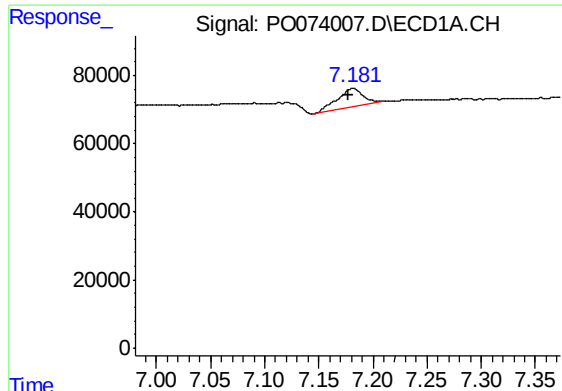

#26 AR-1254-1


R.T.: 7.182 min
Delta R.T.: 0.005 min
Response: 93347
Conc: 24.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

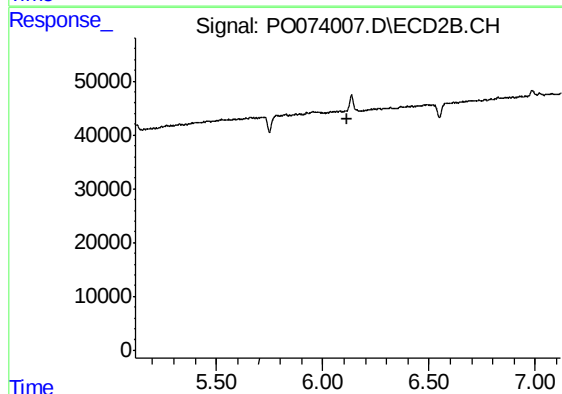


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

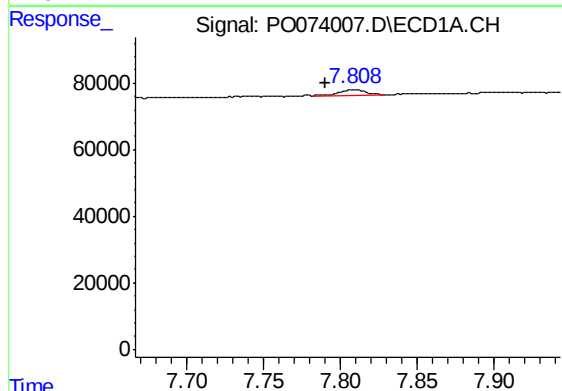


#28 AR-1254-3

R.T.: 7.808 min
Delta R.T.: 0.018 min
Response: 20698
Conc: 3.38 ng/ml

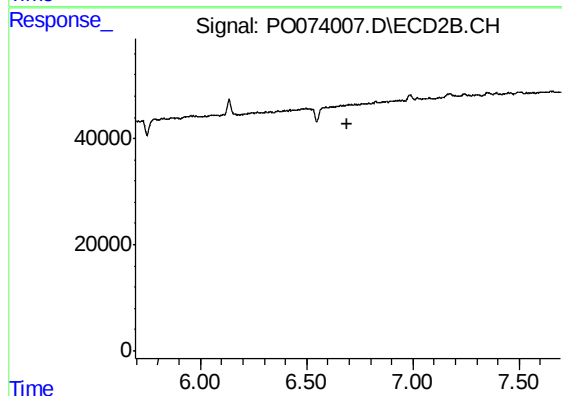

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

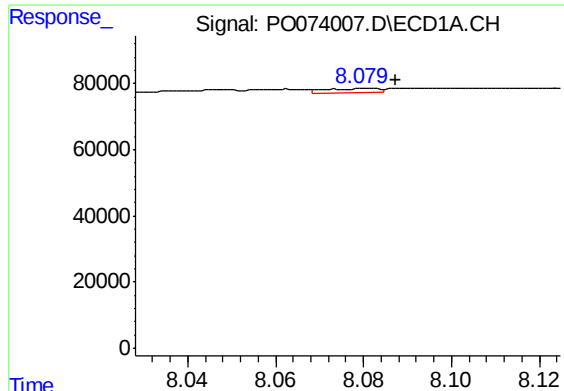

#29 AR-1254-4


R.T.: 8.082 min
Delta R.T.: -0.005 min
Response: 11493
Conc: 2.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

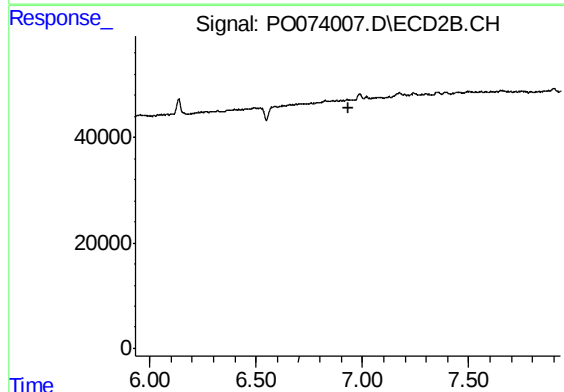


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

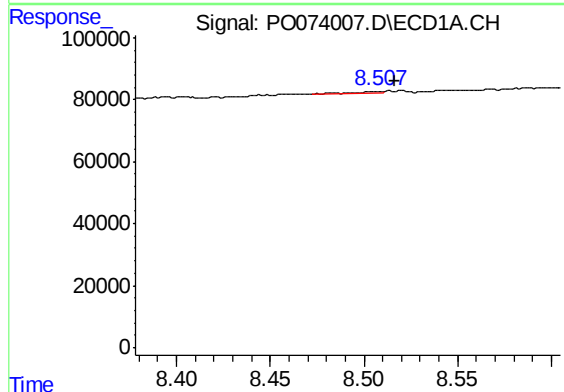


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: -0.009 min
Response: 3114
Conc: 0.60 ng/ml

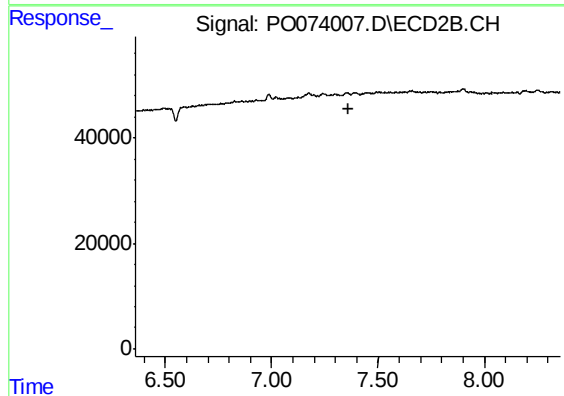

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

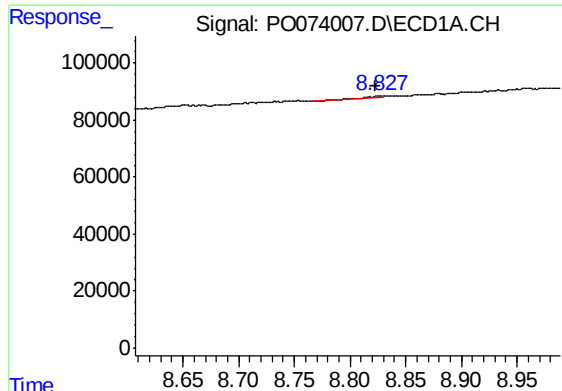

#34 AR-1260-4

R.T.: 8.827 min
Delta R.T.: 0.005 min
Response: 5119
Conc: 1.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

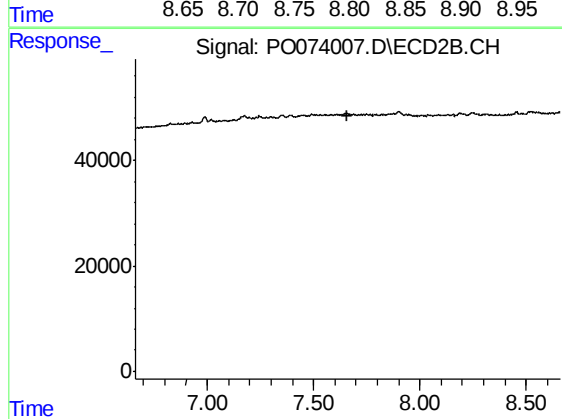

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.