

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR122419\
 Data File : PR044146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Dec 2019 07:40
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:32:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121519CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 16 06:15:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4)	L1	AR-1016-2	0.000	5.134f	0 129312	N.D. 0.269 #
12)	L3	AR-1232-2	0.000	5.134f	0 129312	N.D. 0.594 #
16)	L4	AR-1242-1	0.000	5.134f	0 129312	N.D. 0.449 #
17)	L4	AR-1242-2	0.000	5.134f	0 129312	N.D. 0.327 #
27)	L6	AR-1254-2	0.000	6.072f	0 12316113	N.D. 22.696 #
28)	L6	AR-1254-3	0.000	6.418	0 32004521	N.D. 33.569 #
29)	L6	AR-1254-4	0.000	6.612	0 6031328	N.D. 9.093 #
31)	L7	AR-1260-1	0.000	6.503f	0 6512922	N.D. 11.918 #
32)	L7	AR-1260-2	0.000	6.710	0 1888180	N.D. 2.353 #
45)	L9	AR-1268-5	0.000	8.835f	0 12680814	N.D. 2.598 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR122419\
Data File : PR044146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Dec 2019 07:40
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:32:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121519CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 16 06:15:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

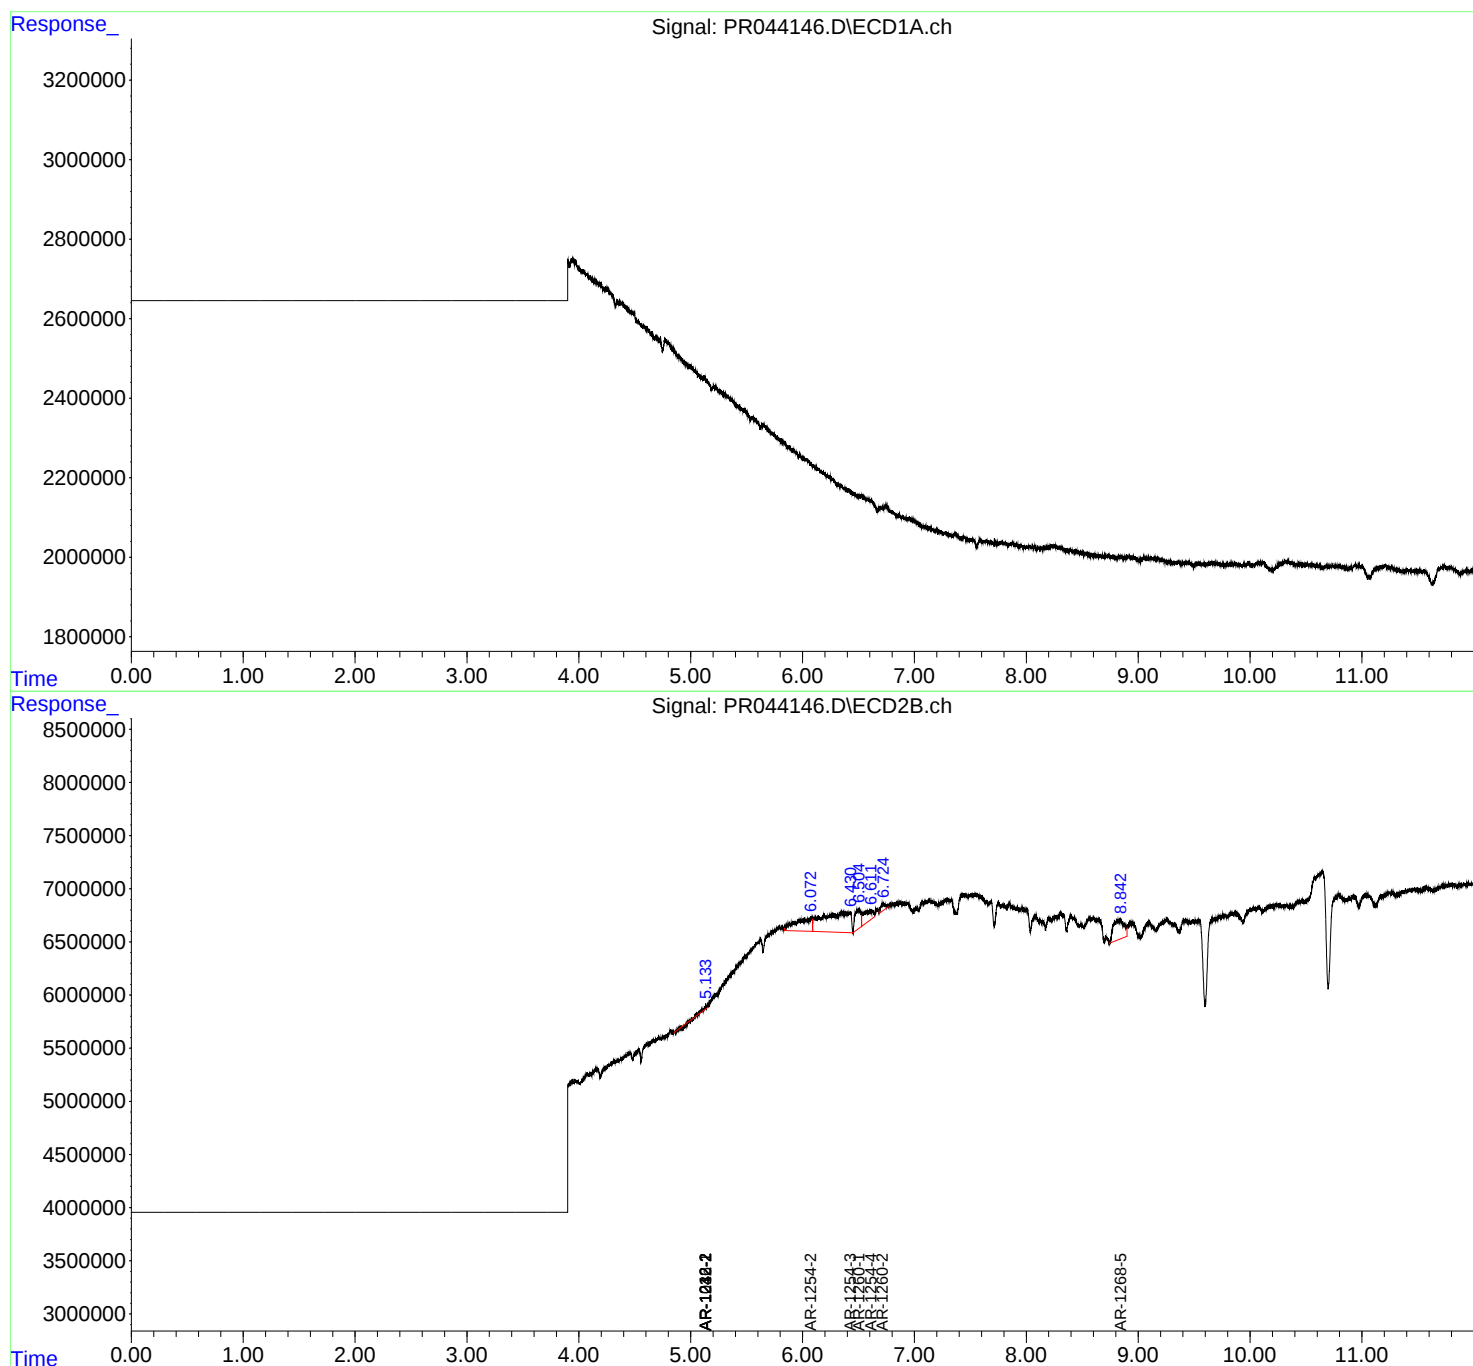


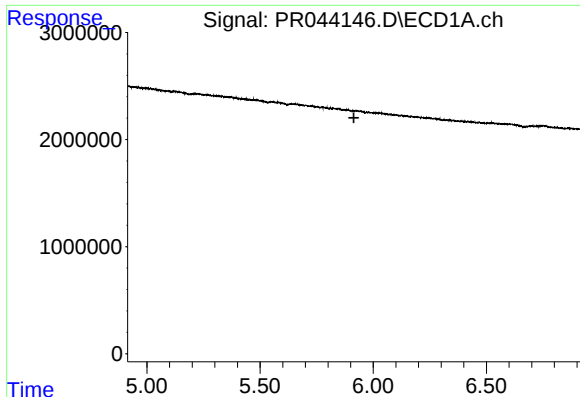

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

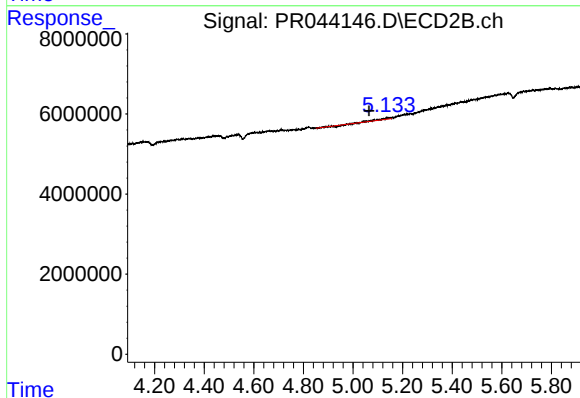


#4 AR-1016-2

R.T.: 5.134 min
Delta R.T.: 0.069 min
Response: 129312
Conc: 0.27 ng/ml

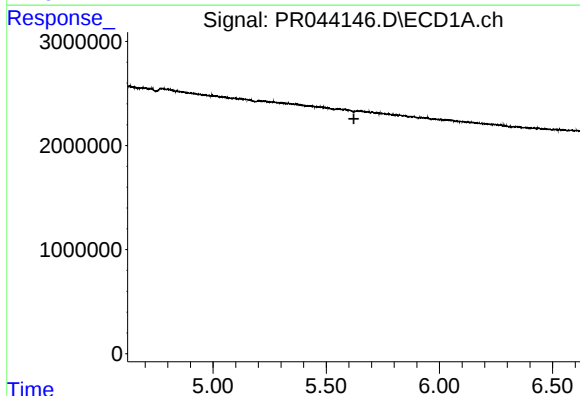


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.622 min
Response: 0
Conc: N.D.

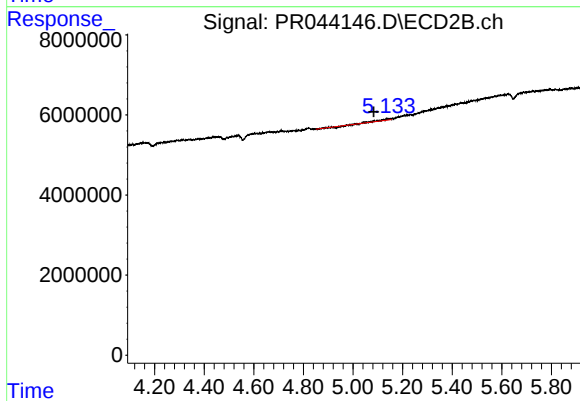

#12 AR-1232-2


R.T.: 5.134 min
Delta R.T.: 0.050 min
Response: 129312
Conc: 0.59 ng/ml

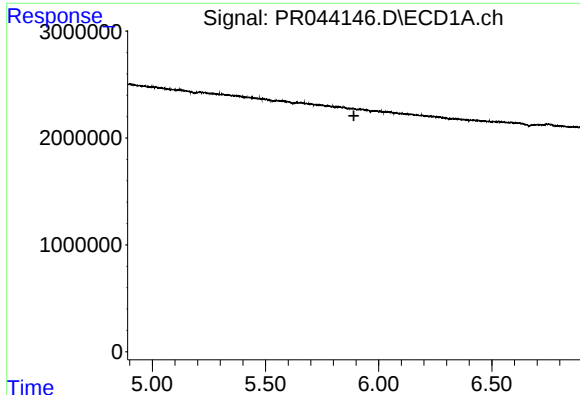

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 5.891 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

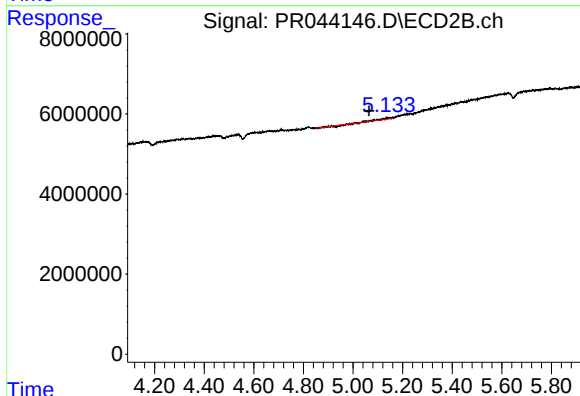


#16 AR-1242-1

R.T.: 5.134 min
Delta R.T.: 0.070 min
Response: 129312
Conc: 0.45 ng/ml

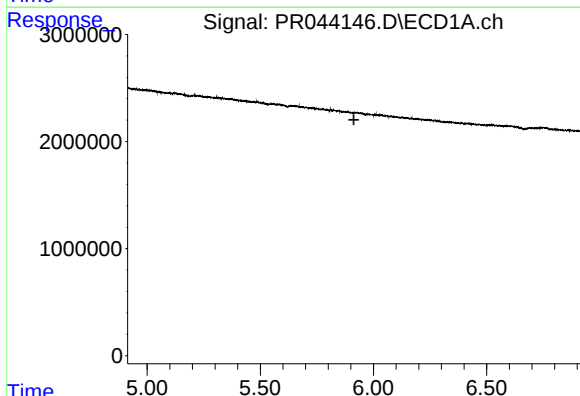


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 5.913 min
Response: 0
Conc: N.D.

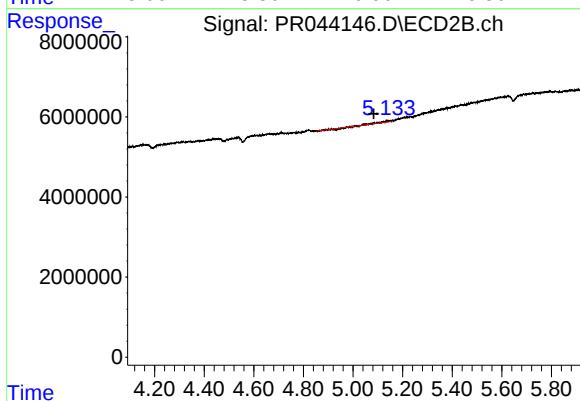

#17 AR-1242-2


R.T.: 5.134 min
Delta R.T.: 0.050 min
Response: 129312
Conc: 0.33 ng/ml

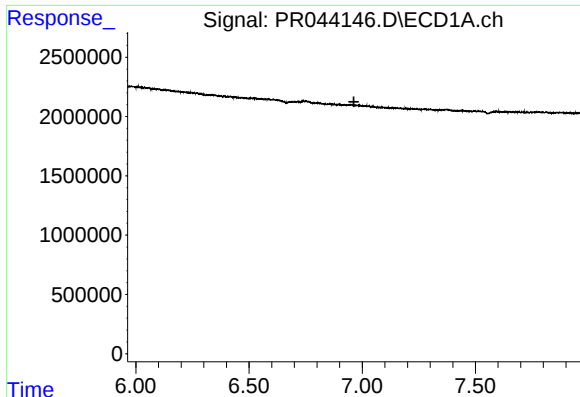

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.963 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

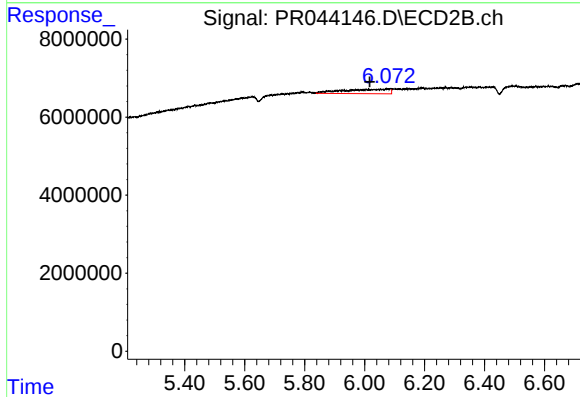


#27 AR-1254-2

R.T.: 6.072 min
Delta R.T.: 0.054 min
Response: 12316113
Conc: 22.70 ng/ml

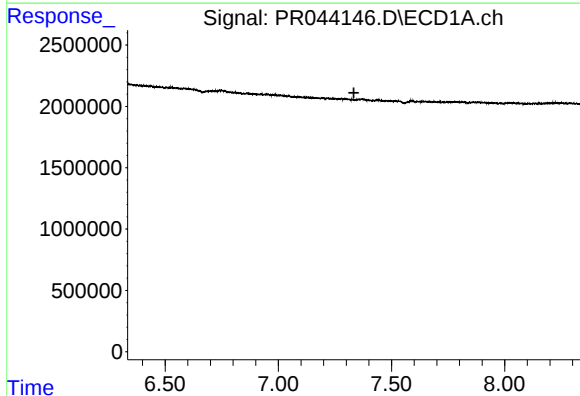


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.334 min
Response: 0
Conc: N.D.

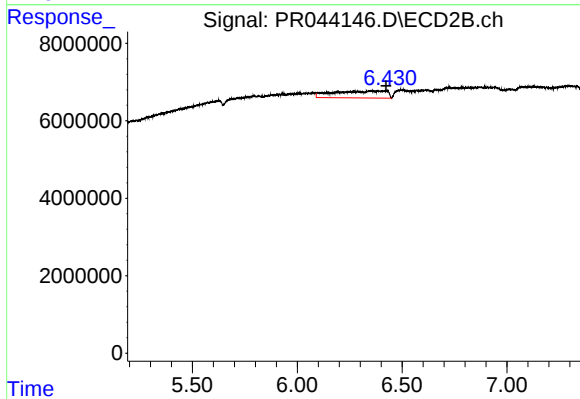

#28 AR-1254-3


R.T.: 6.418 min
Delta R.T.: -0.005 min
Response: 32004521
Conc: 33.57 ng/ml

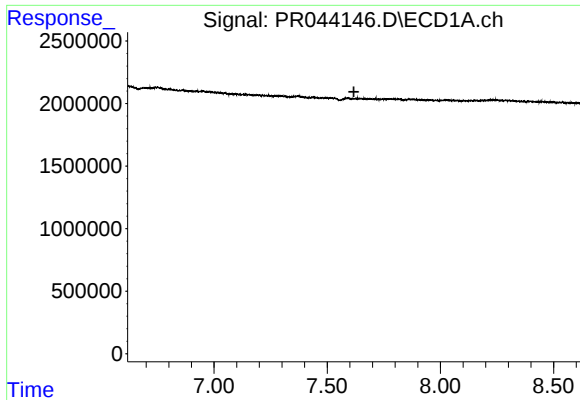

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.618 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

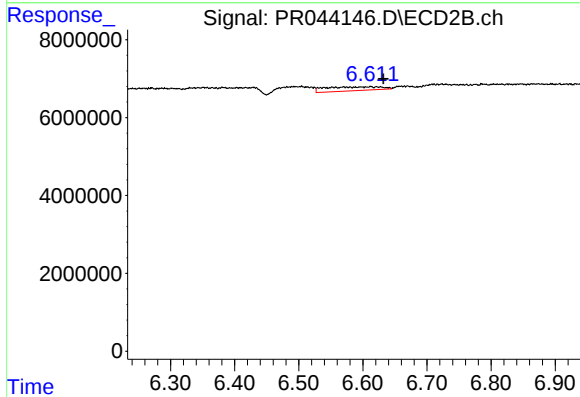


#29 AR-1254-4

R.T.: 6.612 min
Delta R.T.: -0.020 min
Response: 6031328
Conc: 9.09 ng/ml

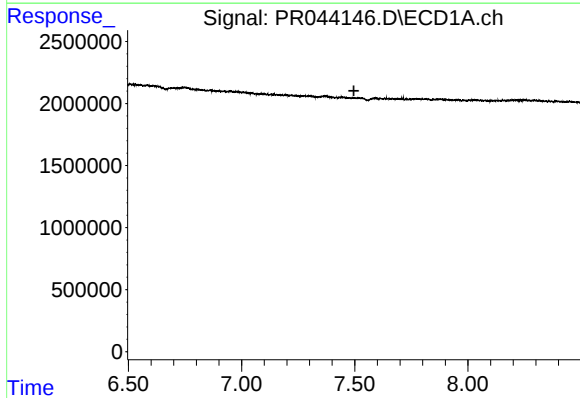


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.496 min
Response: 0
Conc: N.D.

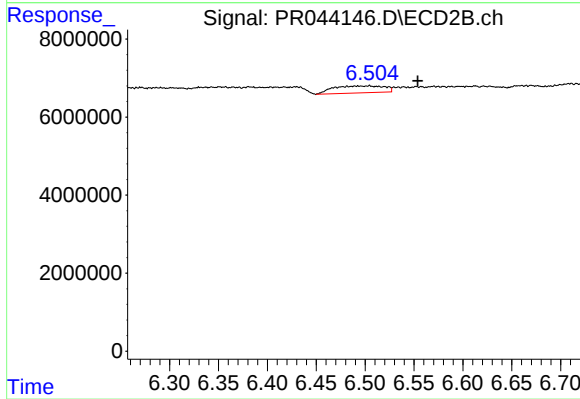

#31 AR-1260-1


R.T.: 6.503 min
Delta R.T.: -0.051 min
Response: 6512922
Conc: 11.92 ng/ml

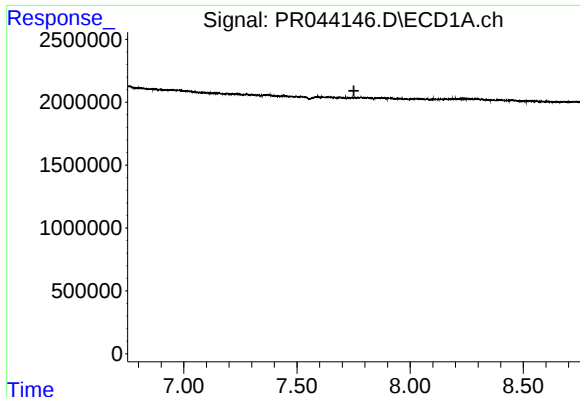

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

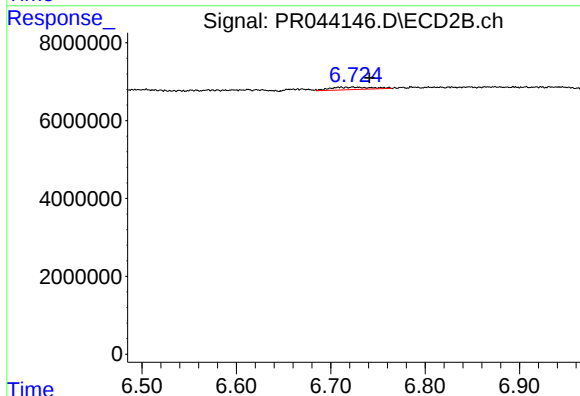


#32 AR-1260-2

R.T.: 6.710 min
Delta R.T.: -0.031 min
Response: 1888180
Conc: 2.35 ng/ml

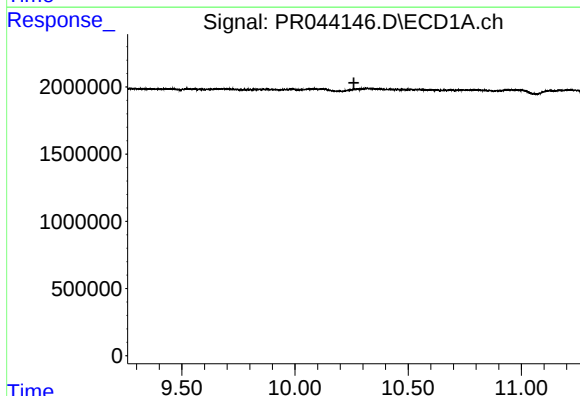

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.260 min
Response: 0
Conc: N.D.

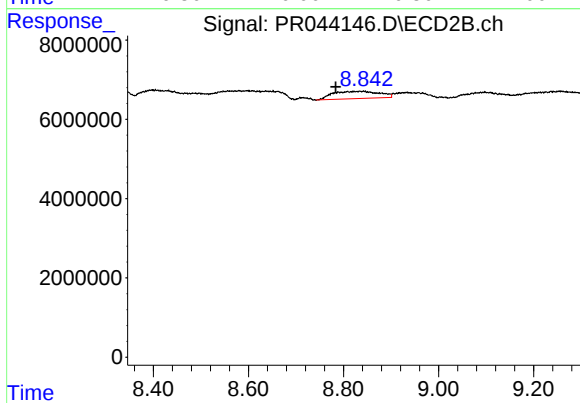

#45 AR-1268-5

R.T.: 8.835 min
Delta R.T.: 0.052 min
Response: 12680814
Conc: 2.60 ng/ml