

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 12:59
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1221 LOD 55PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:54:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.363	3.410	21450967	83195953	17.147	17.349
2)	SA Decachlor...	9.991	8.246	24751275	118.7E6	18.714	20.384
Target Compounds							
3)	L1 AR-1016-1	0.000	4.456	0	605338	N.D.	3.325 #
4)	L1 AR-1016-2	0.000	4.468	0	550239	N.D.	1.950 #
5)	L1 AR-1016-3	0.000	4.638	0	368984	N.D.	2.566 #
6)	L1 AR-1016-4	0.000	4.688	0	403620	N.D.	3.648 #
7)	L1 AR-1016-5	0.000	4.881	0	285664	N.D.	1.879 #
8)	L2 AR-1221-1	4.571	3.615	817906	2610770	65.416	51.273
9)	L2 AR-1221-2	4.660	3.697	781748	2784361	86.439	74.978
10)	L2 AR-1221-3	4.733	3.769	1479850	5726071	48.284	46.763
11)	L3 AR-1232-1	4.733	3.769	1479850	5726071	50.591	48.944
12)	L3 AR-1232-2	0.000	4.468	0	550239	N.D.	3.981 #
13)	L3 AR-1232-3	0.000	4.638	0	368984	N.D.	5.256 #
14)	L3 AR-1232-4	0.000	4.718	0	227210	N.D.	3.808 #
15)	L3 AR-1232-5	0.000	4.881	0	285664	N.D.	4.186 #
16)	L4 AR-1242-1	0.000	4.456	0	605338	N.D.	4.131 #
17)	L4 AR-1242-2	0.000	4.468	0	550239	N.D.	2.412 #
18)	L4 AR-1242-3	0.000	4.638	0	368984	N.D.	3.191 #
19)	L4 AR-1242-4	0.000	4.718	0	227210	N.D.	2.067 #
20)	L4 AR-1242-5	6.370	5.226	775396	686635	24.096	4.144 #
21)	L5 AR-1248-1	0.000	4.456	0	605338	N.D.	6.013 #
22)	L5 AR-1248-2	0.000	4.688	0	403620	N.D.	2.957 #
23)	L5 AR-1248-3	0.000	4.718	0	227210	N.D.	1.623 #
24)	L5 AR-1248-4	6.370	4.881	775396	285664	15.839	1.605 #
25)	L5 AR-1248-5	6.370	5.269	775396	799701	16.415	4.088 #
26)	L6 AR-1254-1	6.370	5.226	775396	686635	14.193	1.993 #
27)	L6 AR-1254-2	0.000	5.388	0	1607580	N.D.	5.368 #
28)	L6 AR-1254-3	6.965	5.769	573415	2353964	6.304	4.970
29)	L6 AR-1254-4	0.000	5.975	0	492730	N.D.	1.405 #
30)	L6 AR-1254-5	0.000	6.379	0	2885566	N.D.	6.516 #
31)	L7 AR-1260-1	0.000	5.895	0	93892	N.D.	0.321 #
32)	L7 AR-1260-2	7.393	6.066	1487543	3112056	18.663	6.757 #
33)	L7 AR-1260-3	0.000	6.284	0	3179276	N.D.	8.918 #
34)	L7 AR-1260-4	0.000	6.737	0	3476780	N.D.	11.408 #
35)	L7 AR-1260-5	0.000	6.929	0	209856	N.D.	0.242 #
36)	L8 AR-1262-1	0.000	6.493	0	3543939	N.D.	14.141 #
37)	L8 AR-1262-2	0.000	6.929	0	209856	N.D.	0.167 #
38)	L8 AR-1262-3	0.000	7.219	0	10250774	N.D.	18.697 #
39)	L8 AR-1262-4	0.000	7.300	0	15386293	N.D.	17.141 #
40)	L8 AR-1262-5	0.000	7.779	0	845412	N.D.	2.210 #
41)	L9 AR-1268-1	0.000	7.219	0	10250774	N.D.	8.327 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 12:59
Operator : SM\SJ
Sample : K2241-07
Misc : AR1221 LOD 55PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:54:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.300	0	15386293	N.D.	14.530 #
43)	L9 AR-1268-3	0.000	7.464	0	4682216	N.D.	5.283 #
44)	L9 AR-1268-4	0.000	7.779	0	845412	N.D.	2.330 #
45)	L9 AR-1268-5	0.000	8.028	0	6404600	N.D.	2.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 12:59
Operator : SM\SJ
Sample : K2241-07
Misc : AR1221 LOD 55PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:54:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

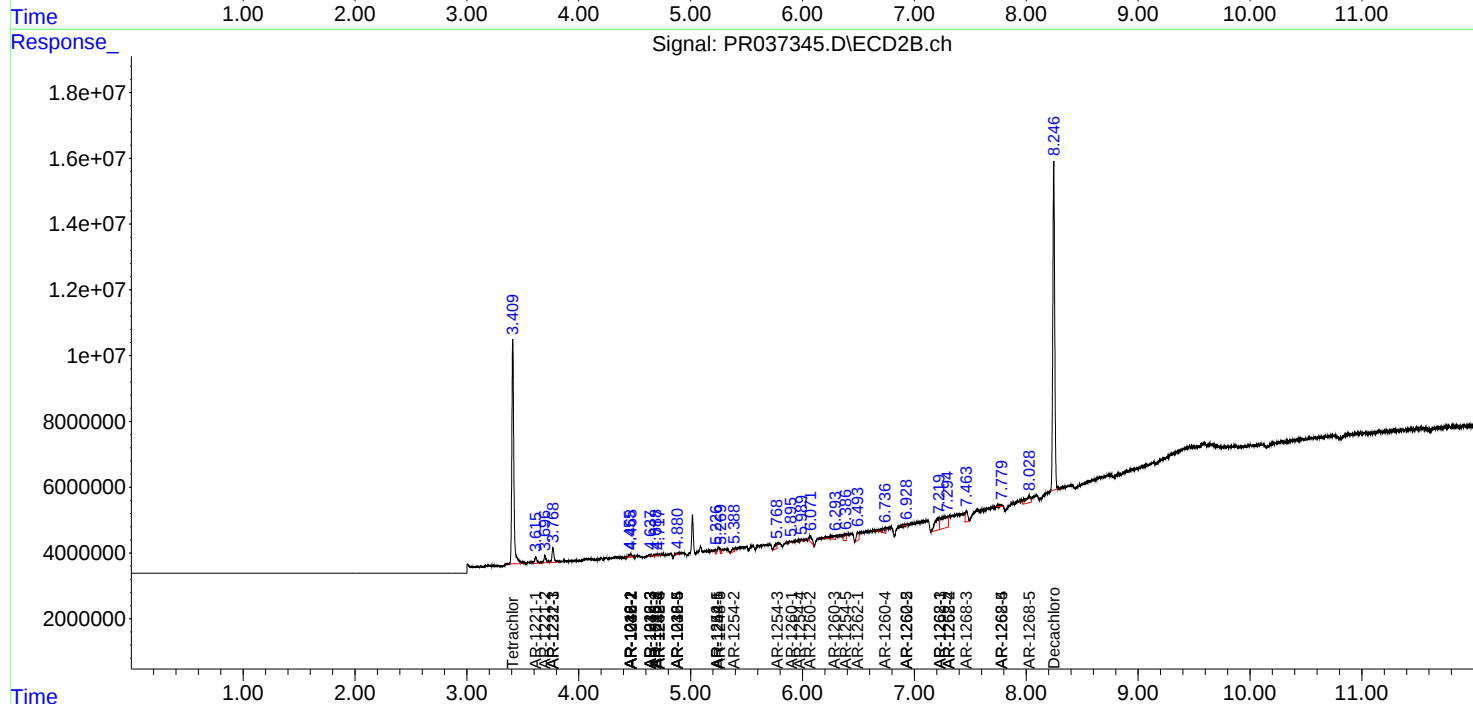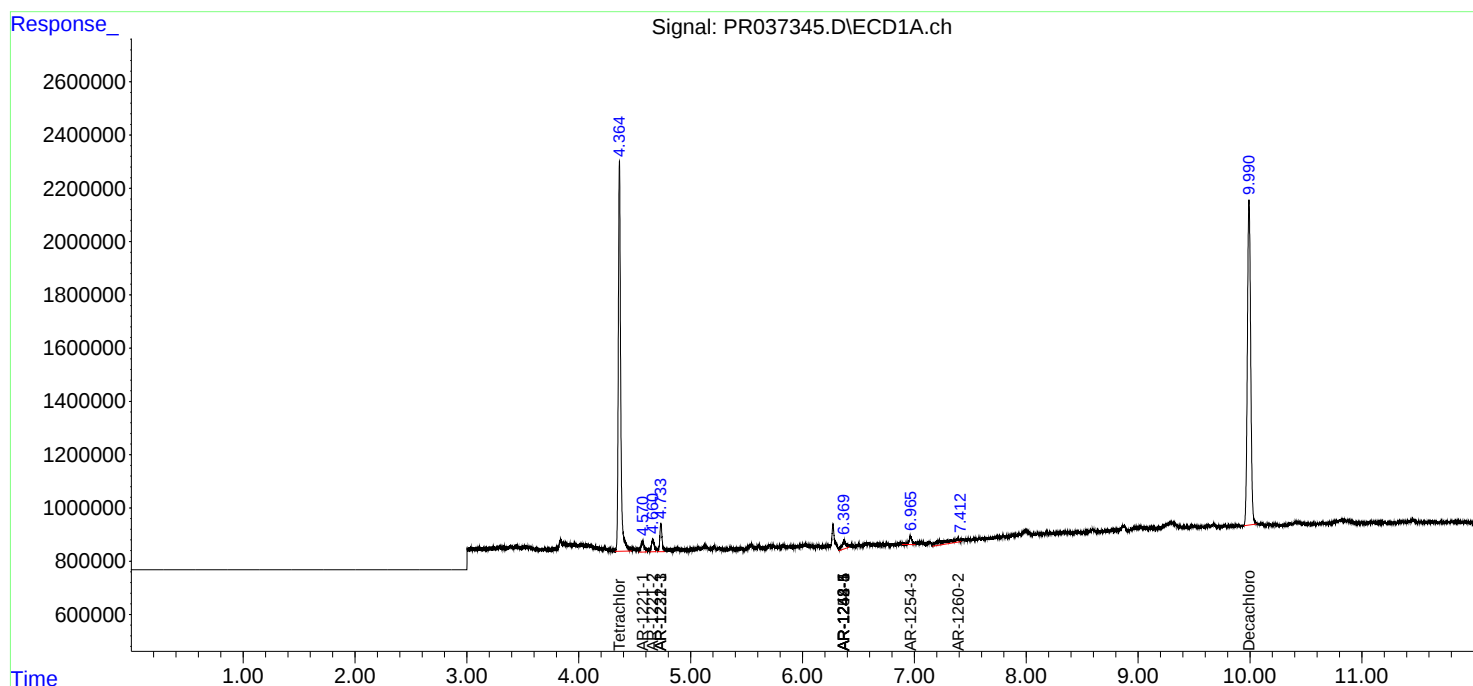


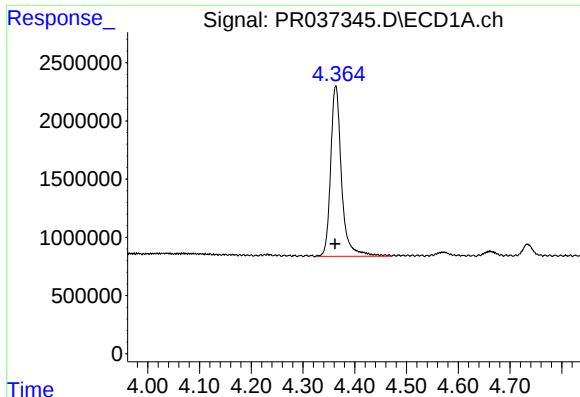

#1 Tetrachloro-m-xylene


R.T.: 4.363 min
Delta R.T.: 0.001 min
Response: 21450967
Conc: 17.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

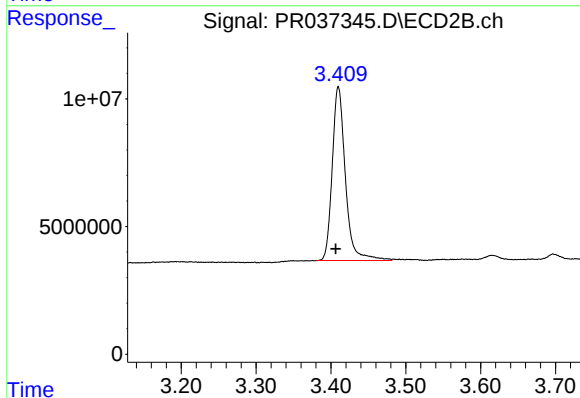


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.003 min
Response: 83195953
Conc: 17.35 ng/ml

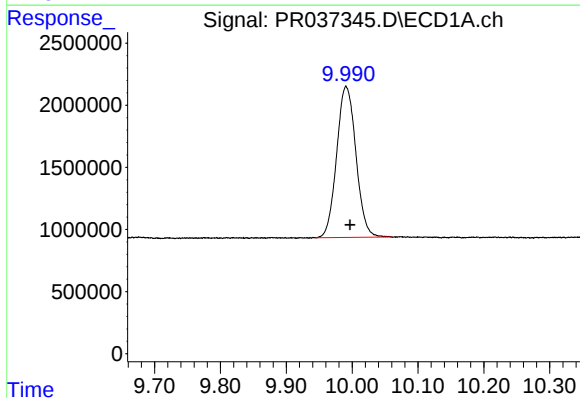


#2 Decachlorobiphenyl

R.T.: 9.991 min
Delta R.T.: -0.006 min
Response: 24751275
Conc: 18.71 ng/ml

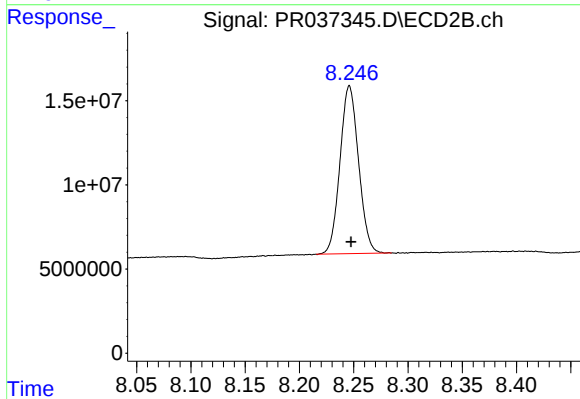

#2 Decachlorobiphenyl


R.T.: 8.246 min
Delta R.T.: -0.001 min
Response: 118719952
Conc: 20.38 ng/ml

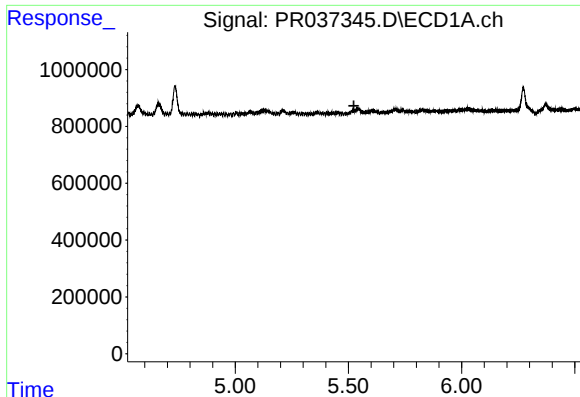

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

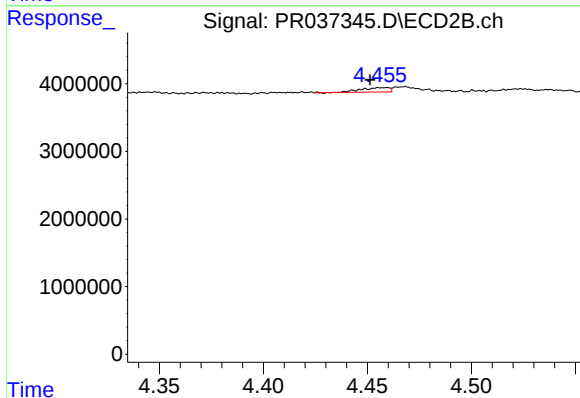


#3 AR-1016-1

R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 605338
Conc: 3.32 ng/ml

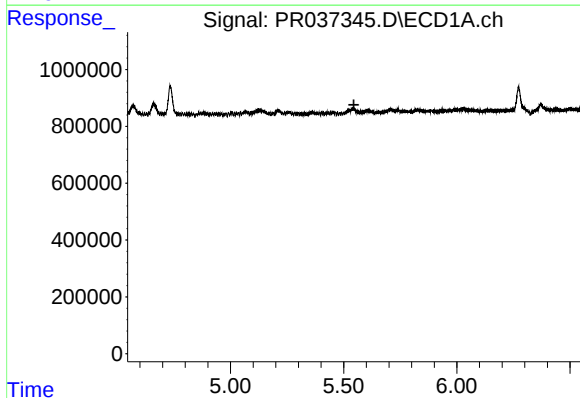


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

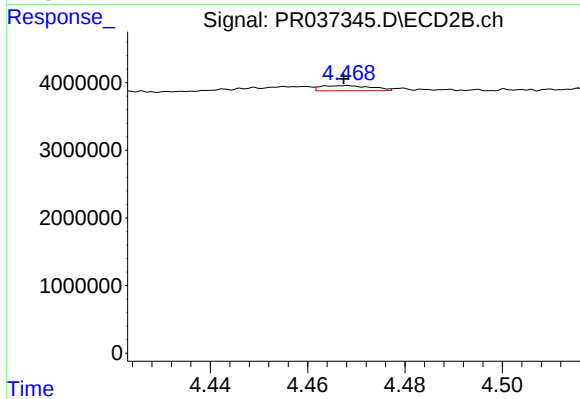

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 550239
Conc: 1.95 ng/ml

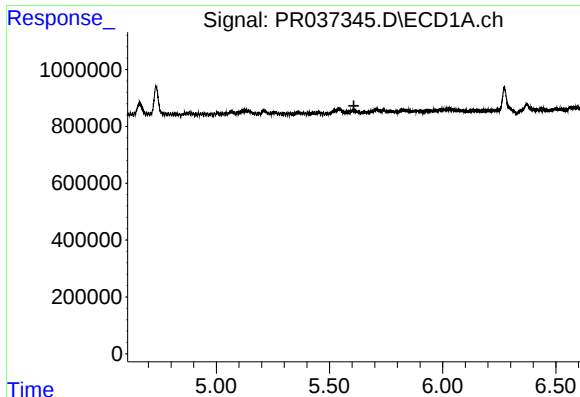

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

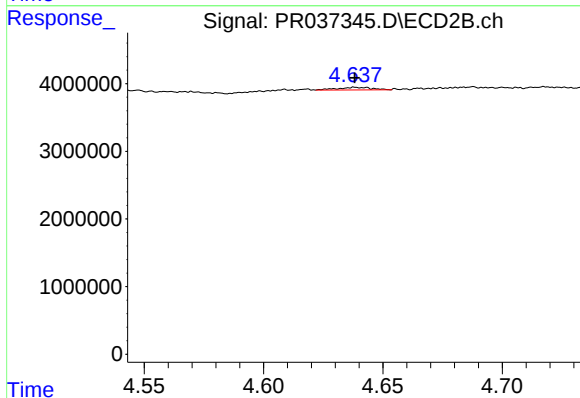


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 368984
Conc: 2.57 ng/ml

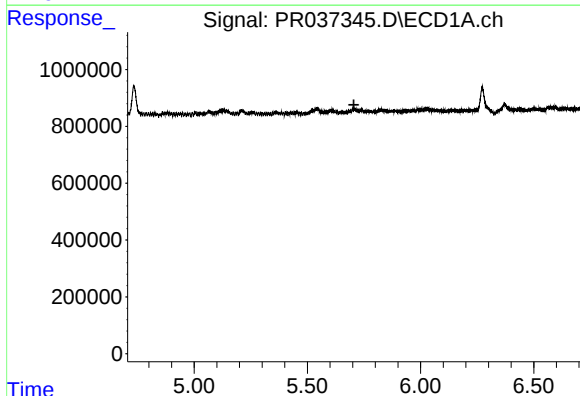


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

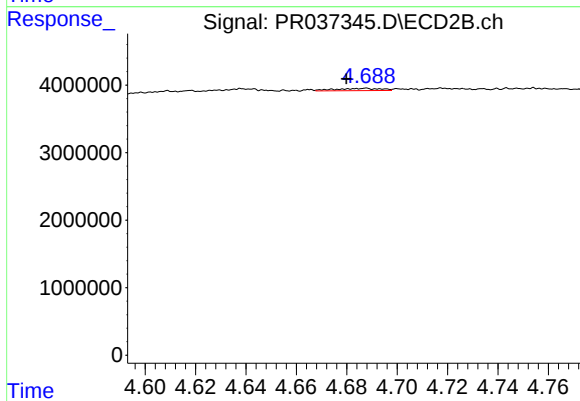

#6 AR-1016-4


R.T.: 4.688 min
Delta R.T.: 0.008 min
Response: 403620
Conc: 3.65 ng/ml

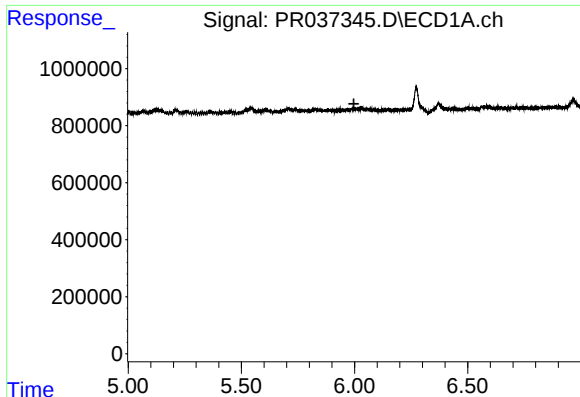

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

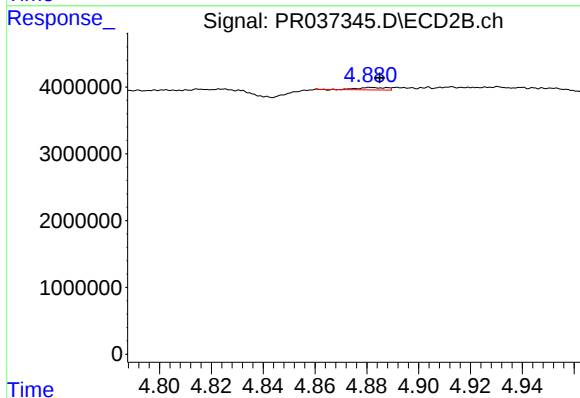


#7 AR-1016-5

R.T.: 4.881 min
Delta R.T.: -0.004 min
Response: 285664
Conc: 1.88 ng/ml

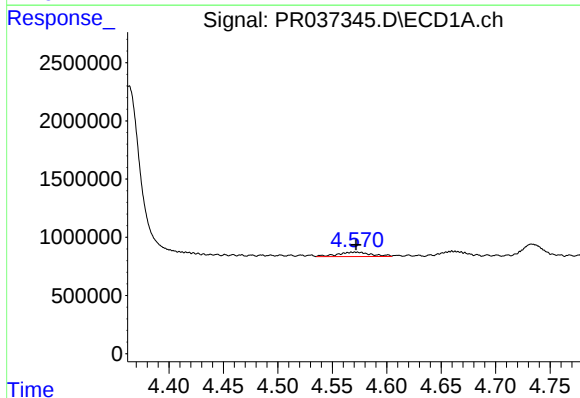


#8 AR-1221-1

R.T.: 4.571 min
Delta R.T.: 0.000 min
Response: 817906
Conc: 65.42 ng/ml

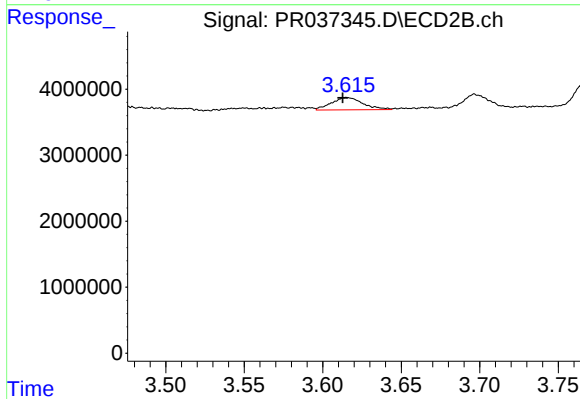

#8 AR-1221-1


R.T.: 3.615 min
Delta R.T.: 0.002 min
Response: 2610770
Conc: 51.27 ng/ml

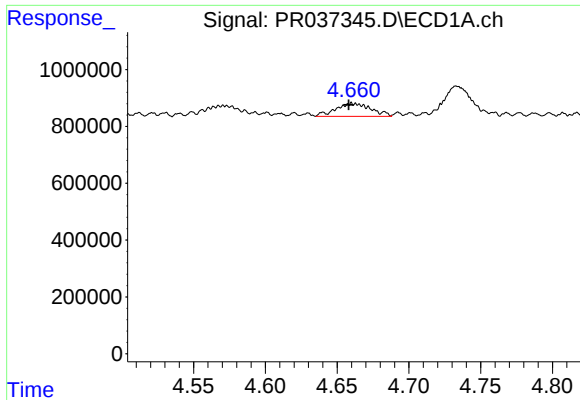

#9 AR-1221-2


R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 781748
Conc: 86.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

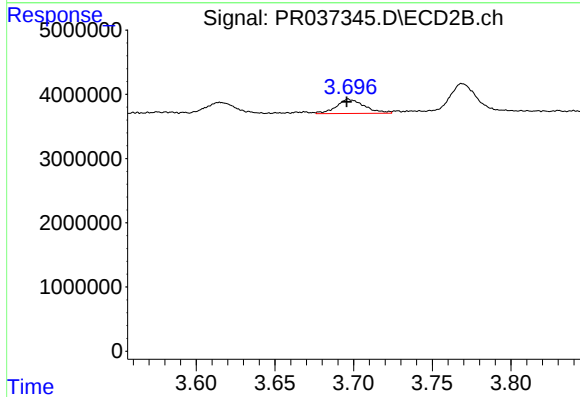


#9 AR-1221-2

R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 2784361
Conc: 74.98 ng/ml

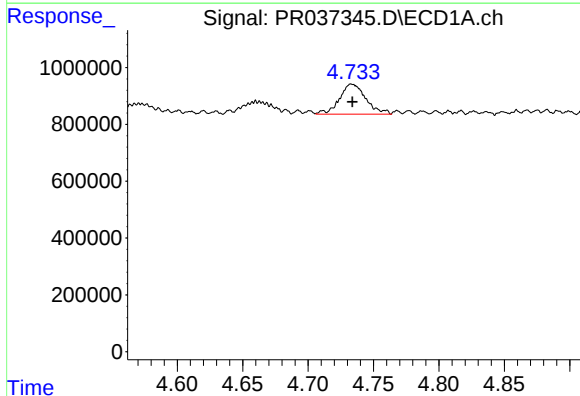


#10 AR-1221-3

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 1479850
Conc: 48.28 ng/ml

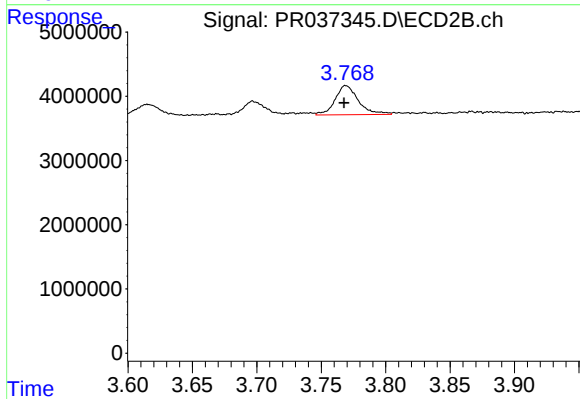

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.001 min
Response: 5726071
Conc: 46.76 ng/ml

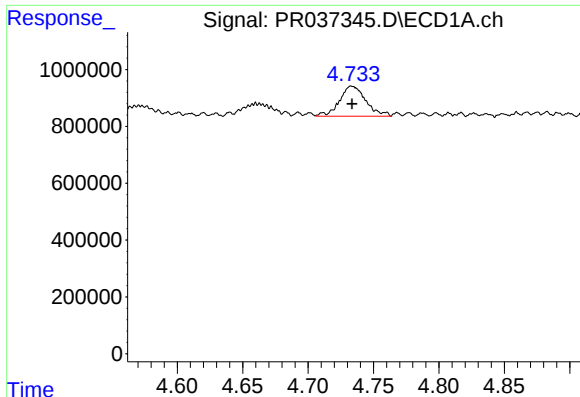

#11 AR-1232-1


R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 1479850
Conc: 50.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

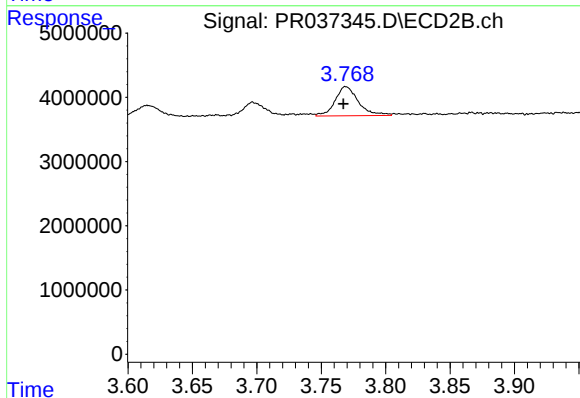


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 5726071
Conc: 48.94 ng/ml

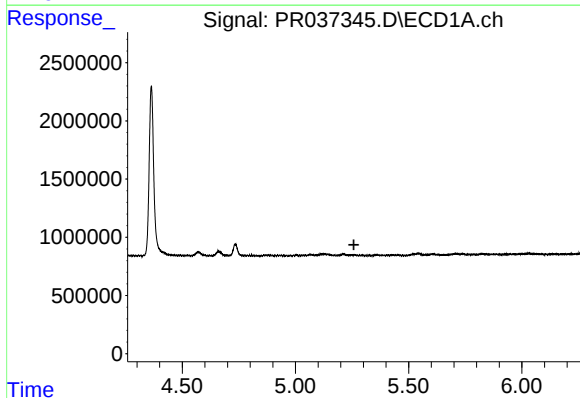


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

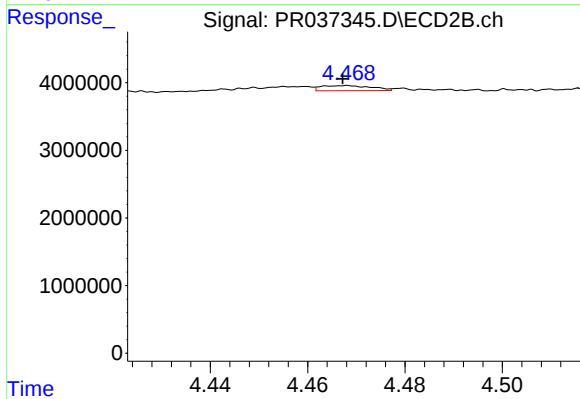

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.001 min
Response: 550239
Conc: 3.98 ng/ml

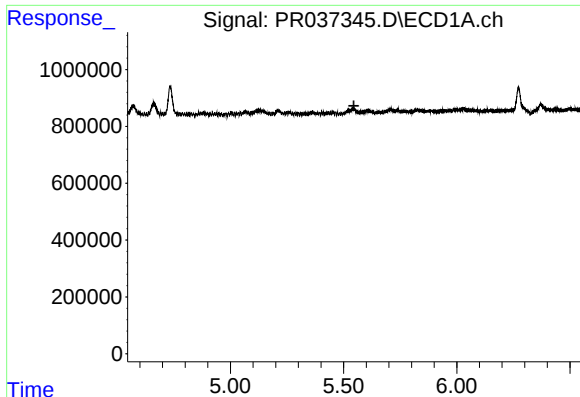

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

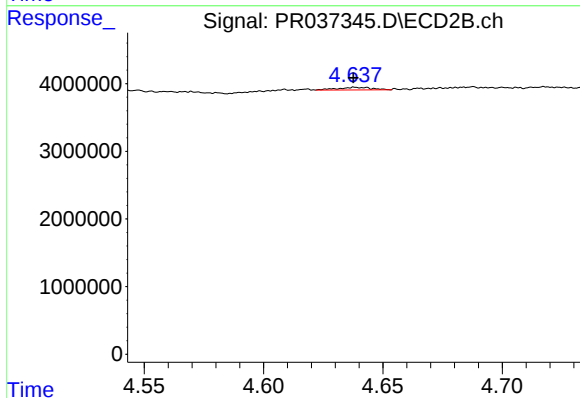


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 368984
Conc: 5.26 ng/ml

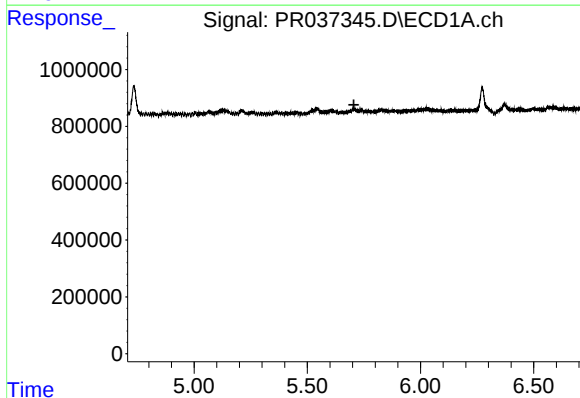


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

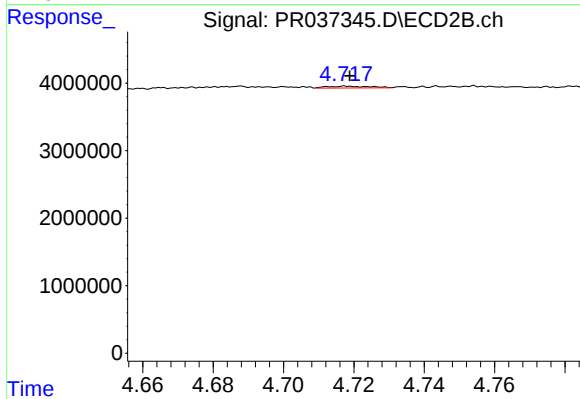

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 227210
Conc: 3.81 ng/ml

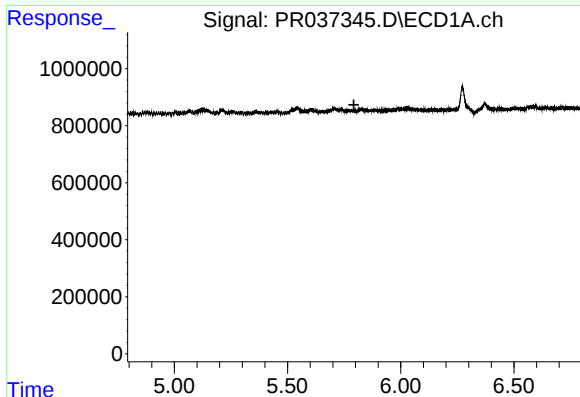

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

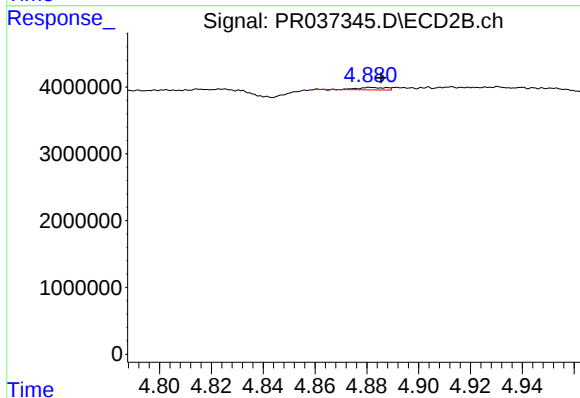


#15 AR-1232-5

R.T.: 4.881 min
Delta R.T.: -0.004 min
Response: 285664
Conc: 4.19 ng/ml

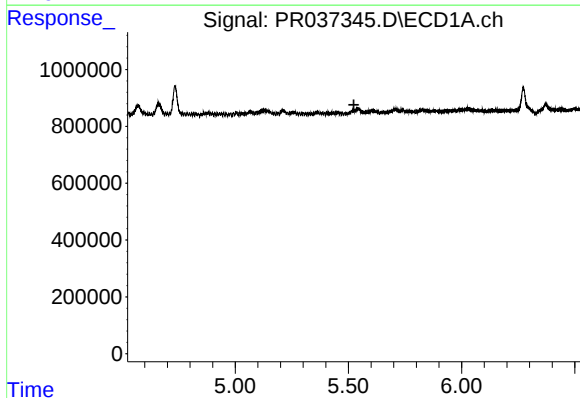


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

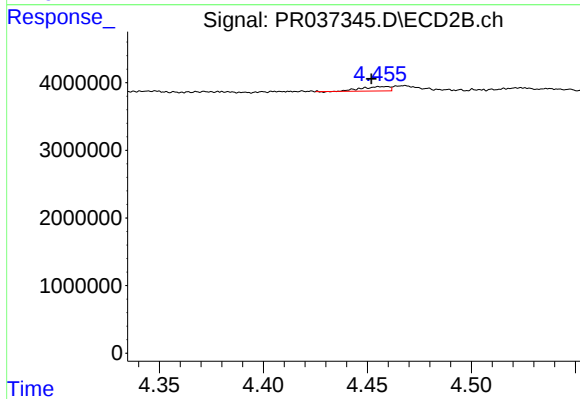

#16 AR-1242-1


R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 605338
Conc: 4.13 ng/ml

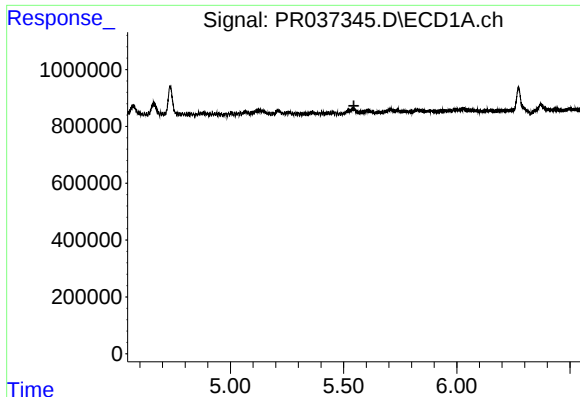

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

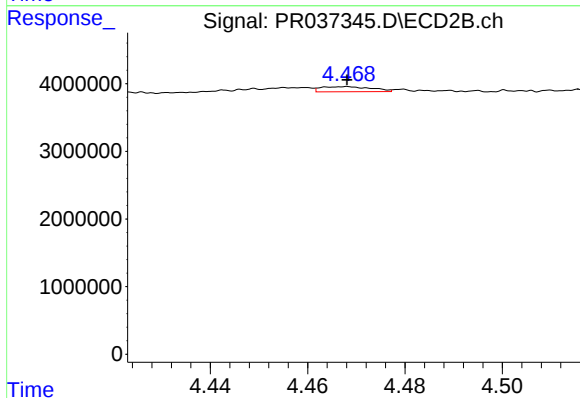


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 550239
Conc: 2.41 ng/ml

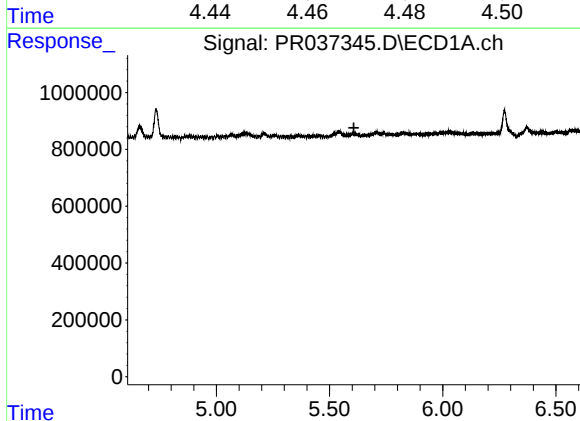


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

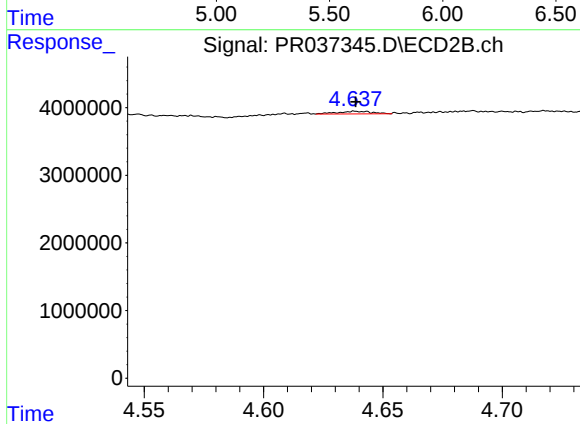

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 368984
Conc: 3.19 ng/ml

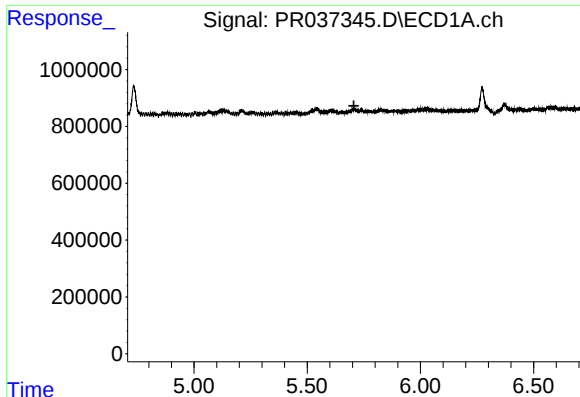

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

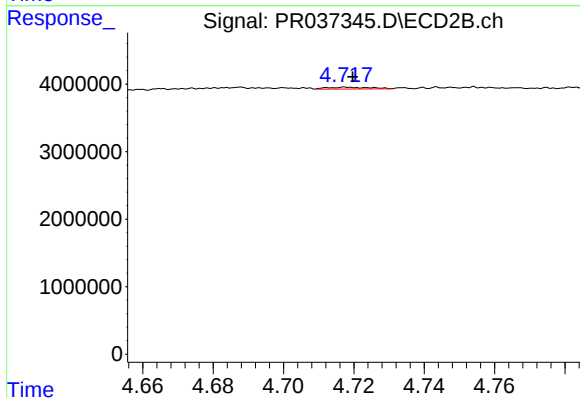


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 227210
Conc: 2.07 ng/ml

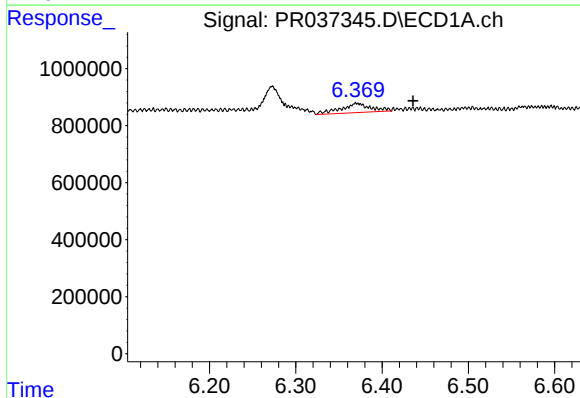


#20 AR-1242-5

R.T.: 6.370 min
Delta R.T.: -0.066 min
Response: 775396
Conc: 24.10 ng/ml

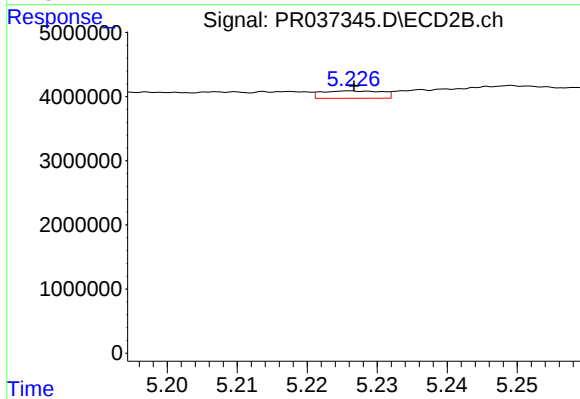

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 686635
Conc: 4.14 ng/ml

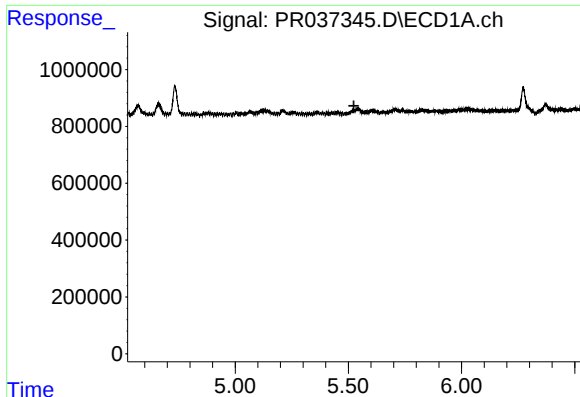

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

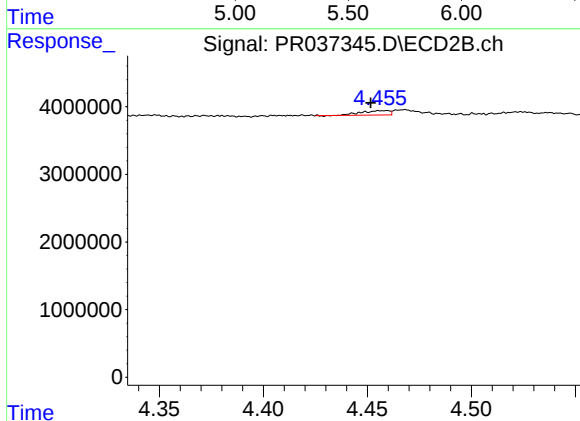


#21 AR-1248-1

R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 605338
Conc: 6.01 ng/ml

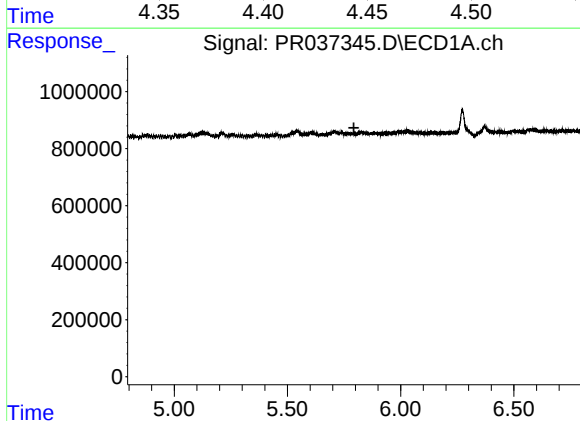


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

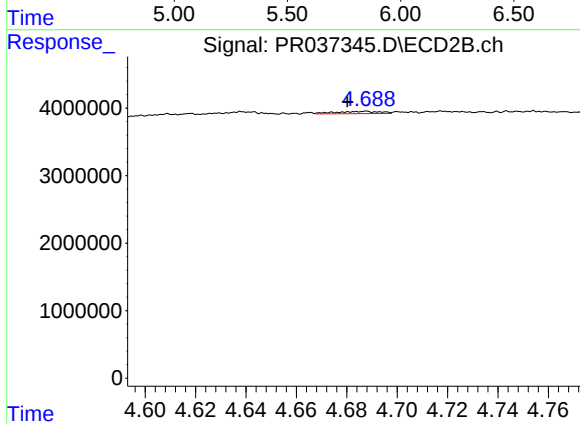

#22 AR-1248-2


R.T.: 4.688 min
Delta R.T.: 0.008 min
Response: 403620
Conc: 2.96 ng/ml

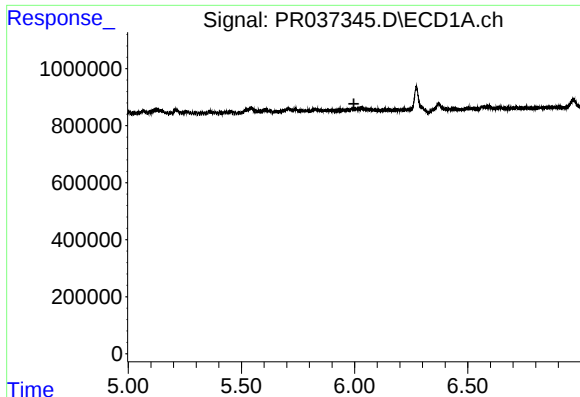

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

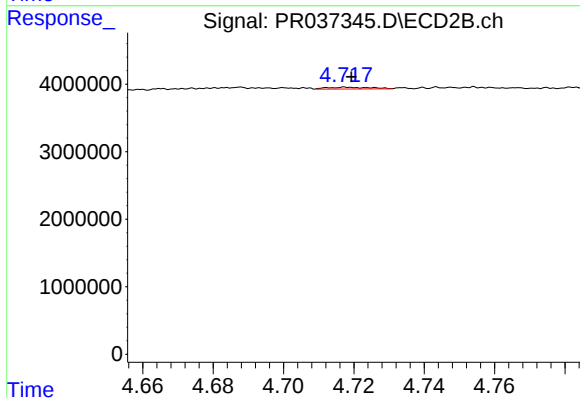


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 227210
Conc: 1.62 ng/ml

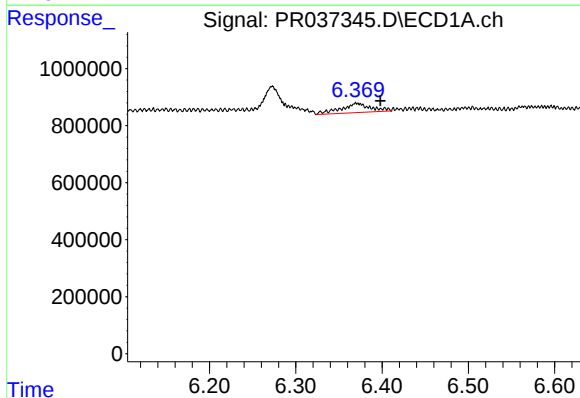


#24 AR-1248-4

R.T.: 6.370 min
Delta R.T.: -0.028 min
Response: 775396
Conc: 15.84 ng/ml

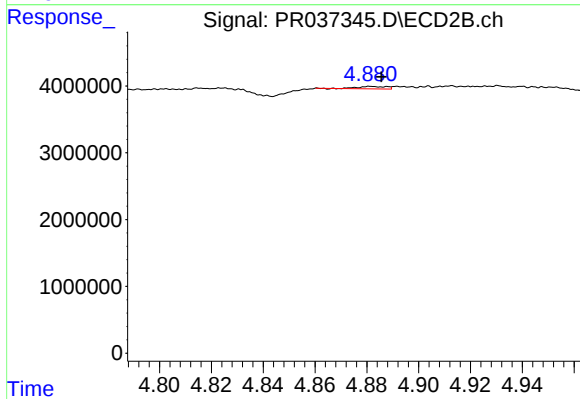

#24 AR-1248-4


R.T.: 4.881 min
Delta R.T.: -0.004 min
Response: 285664
Conc: 1.61 ng/ml

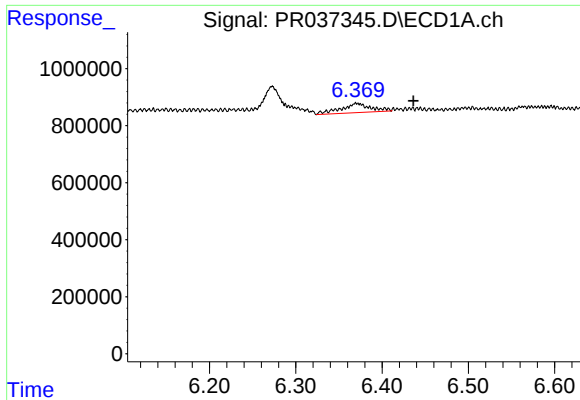

#25 AR-1248-5


R.T.: 6.370 min
Delta R.T.: -0.067 min
Response: 775396
Conc: 16.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

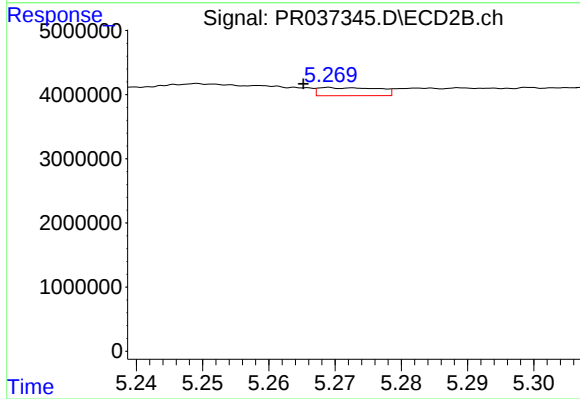


#25 AR-1248-5

R.T.: 5.269 min
Delta R.T.: 0.004 min
Response: 799701
Conc: 4.09 ng/ml

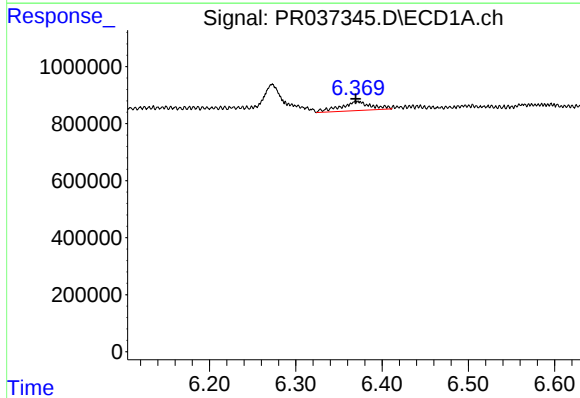


#26 AR-1254-1

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 775396
Conc: 14.19 ng/ml

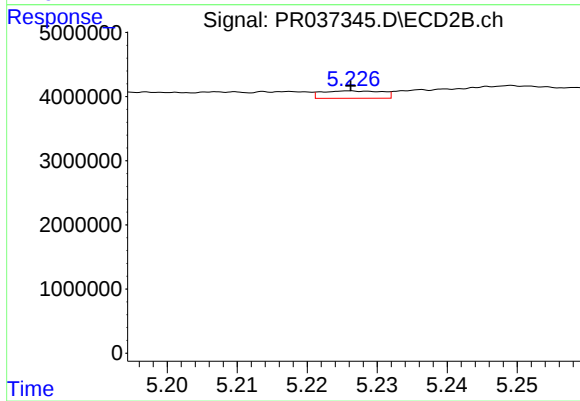

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 686635
Conc: 1.99 ng/ml

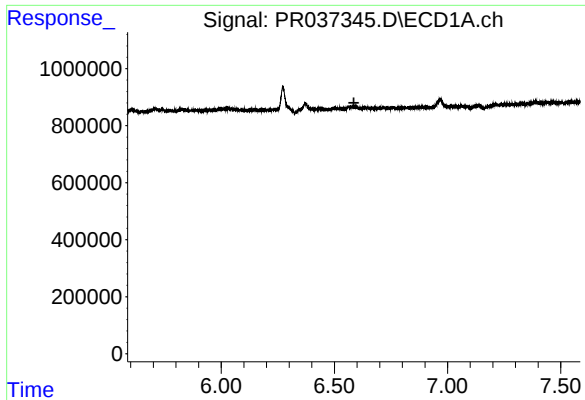

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

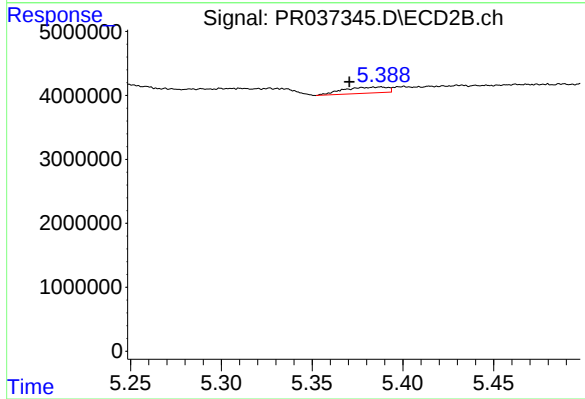


#27 AR-1254-2

R.T.: 5.388 min
Delta R.T.: 0.017 min
Response: 1607580
Conc: 5.37 ng/ml

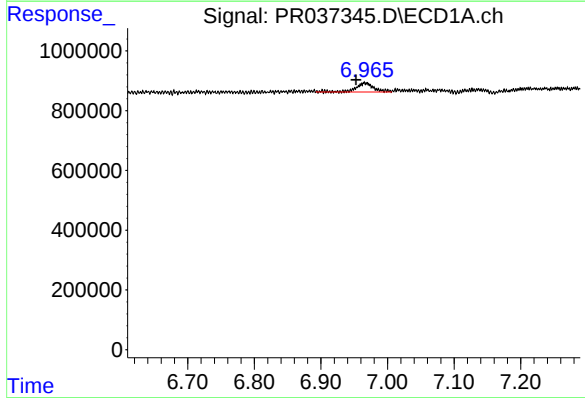


#28 AR-1254-3

R.T.: 6.965 min
Delta R.T.: 0.013 min
Response: 573415
Conc: 6.30 ng/ml

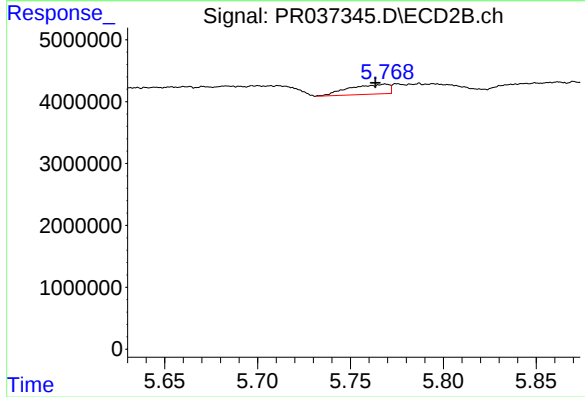

#28 AR-1254-3


R.T.: 5.769 min
Delta R.T.: 0.005 min
Response: 2353964
Conc: 4.97 ng/ml

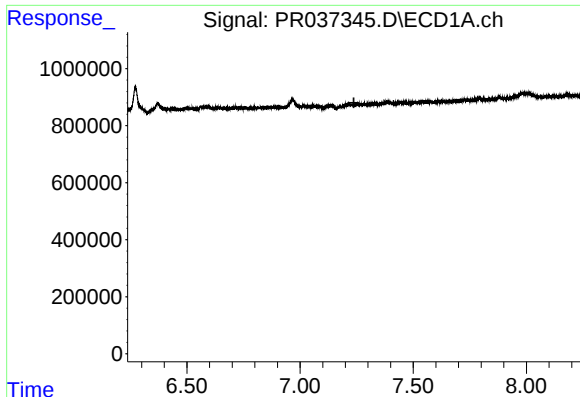

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

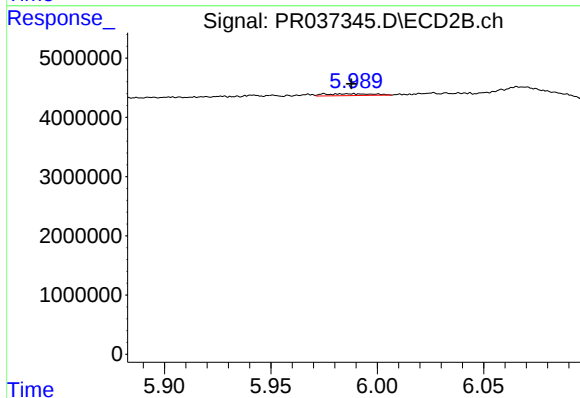


#29 AR-1254-4

R.T.: 5.975 min
Delta R.T.: -0.013 min
Response: 492730
Conc: 1.41 ng/ml

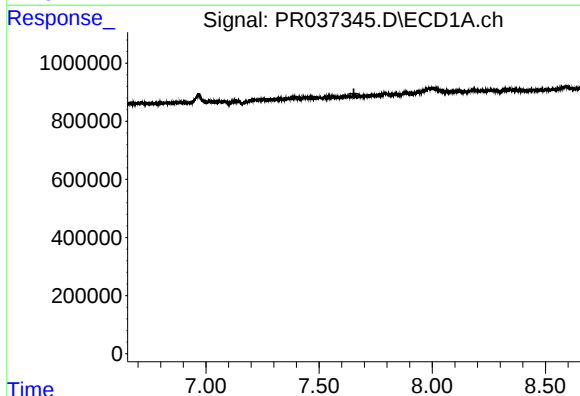


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

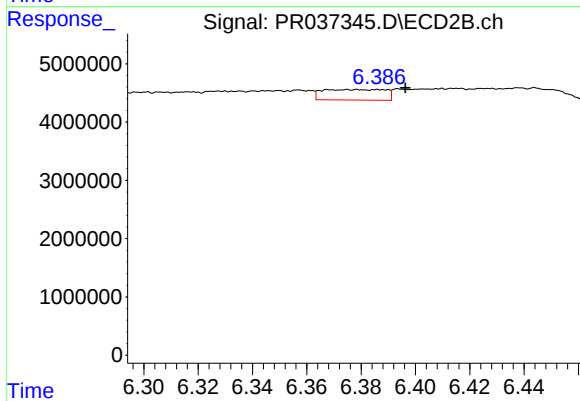

#30 AR-1254-5


R.T.: 6.379 min
Delta R.T.: -0.018 min
Response: 2885566
Conc: 6.52 ng/ml

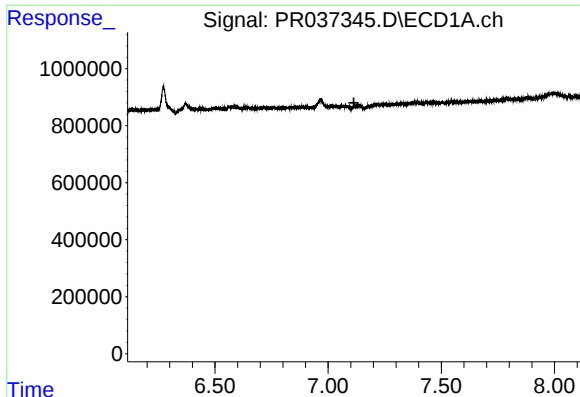

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

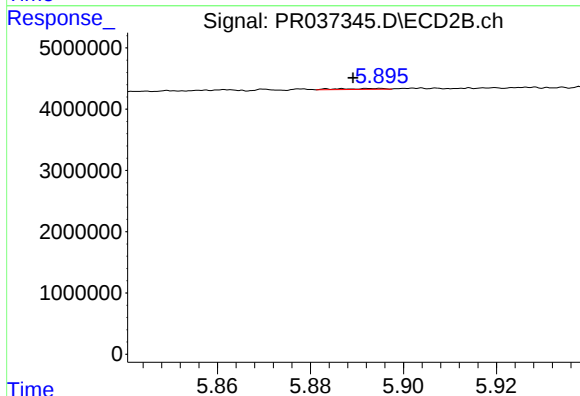


#31 AR-1260-1

R.T.: 5.895 min
Delta R.T.: 0.006 min
Response: 93892
Conc: 0.32 ng/ml

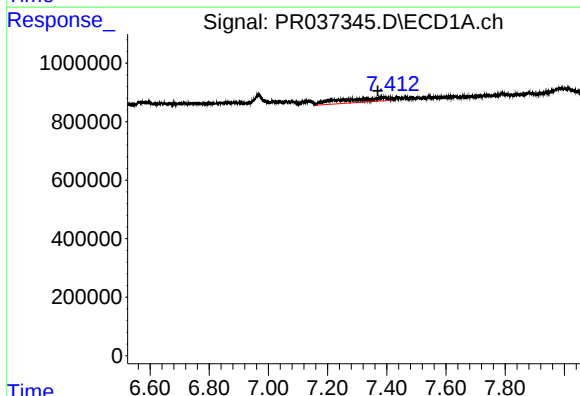


#32 AR-1260-2

R.T.: 7.393 min
Delta R.T.: 0.023 min
Response: 1487543
Conc: 18.66 ng/ml

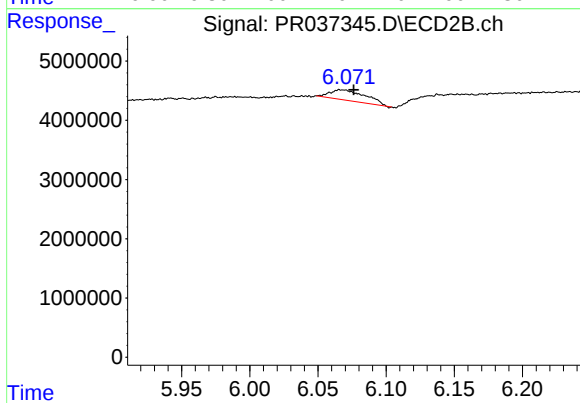

#32 AR-1260-2


R.T.: 6.066 min
Delta R.T.: -0.010 min
Response: 3112056
Conc: 6.76 ng/ml

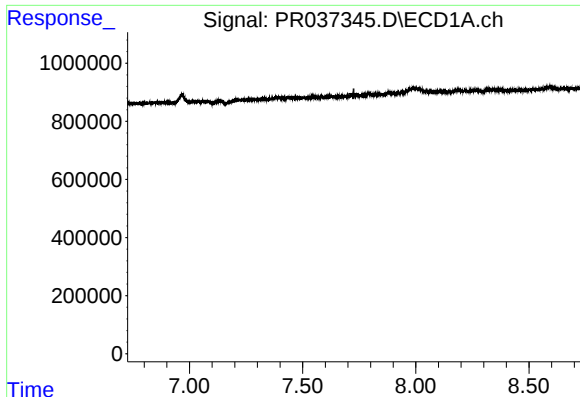

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

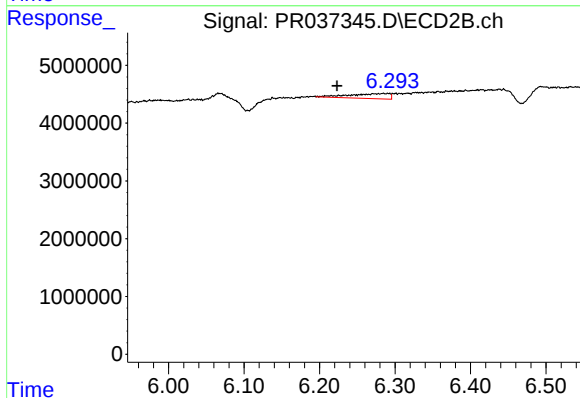


#33 AR-1260-3

R.T.: 6.284 min
Delta R.T.: 0.061 min
Response: 3179276
Conc: 8.92 ng/ml

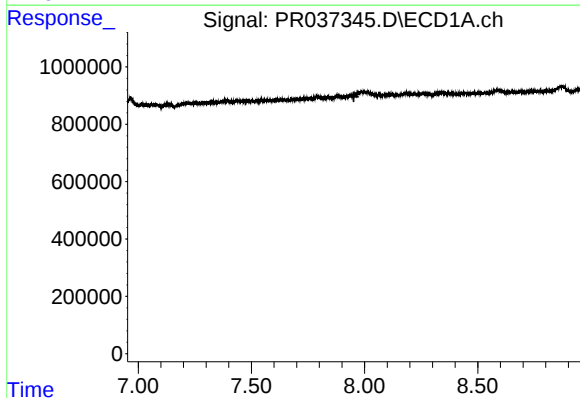


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

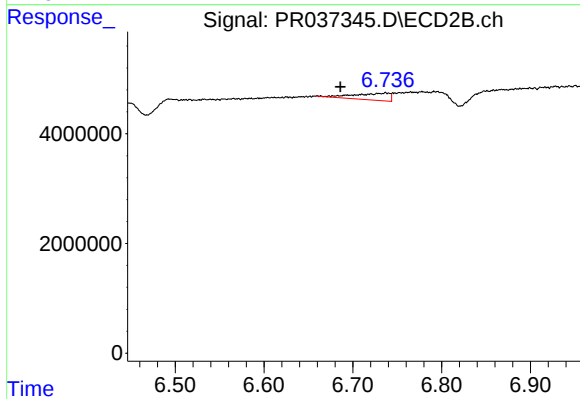

#34 AR-1260-4


R.T.: 6.737 min
Delta R.T.: 0.051 min
Response: 3476780
Conc: 11.41 ng/ml

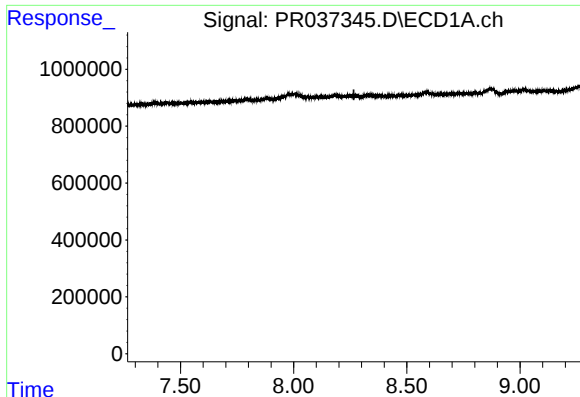

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

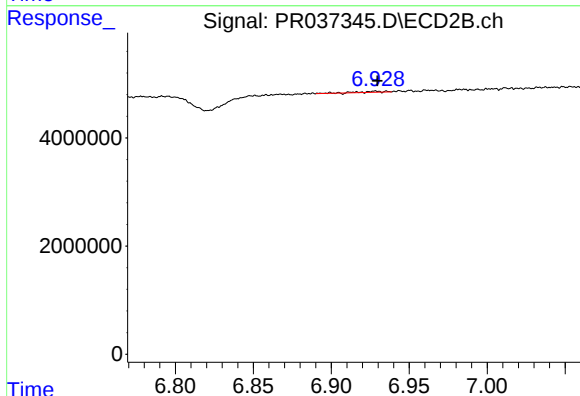


#35 AR-1260-5

R.T.: 6.929 min
Delta R.T.: -0.001 min
Response: 209856
Conc: 0.24 ng/ml

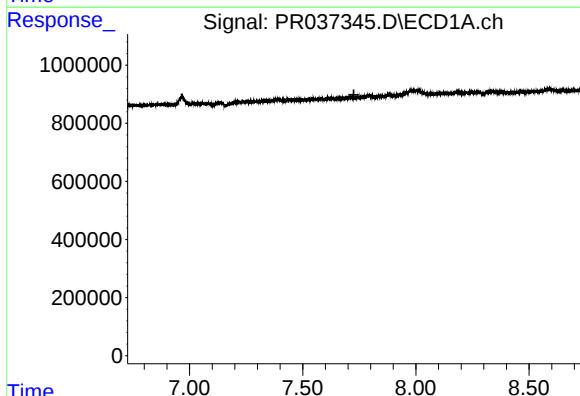


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

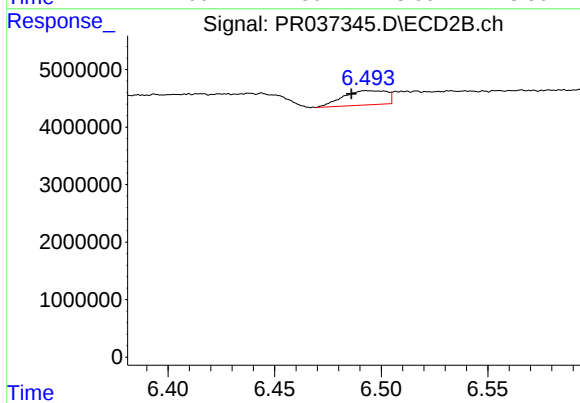

#36 AR-1262-1


R.T.: 6.493 min
Delta R.T.: 0.007 min
Response: 3543939
Conc: 14.14 ng/ml

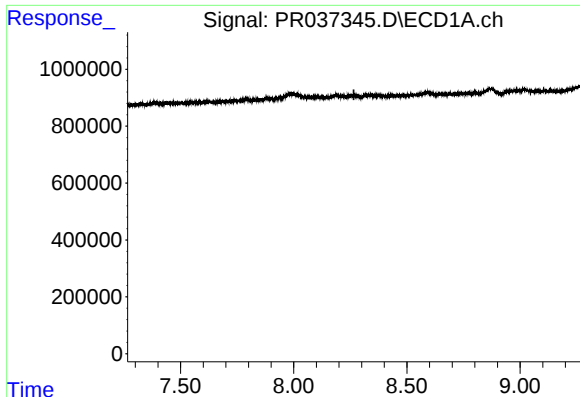

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

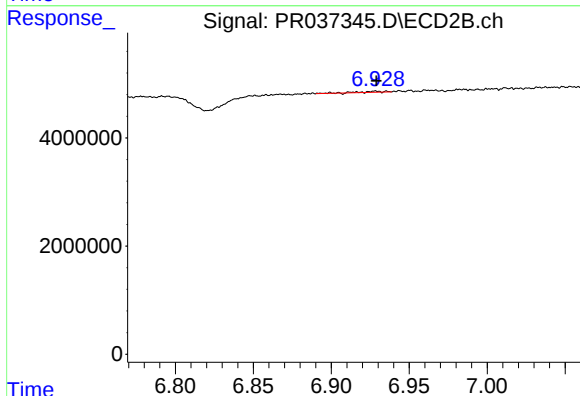


#37 AR-1262-2

R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 209856
Conc: 0.17 ng/ml

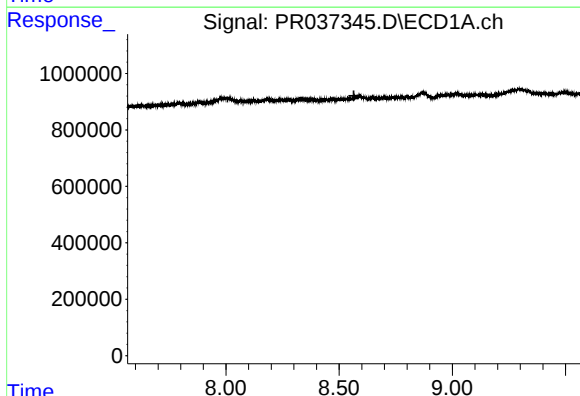


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

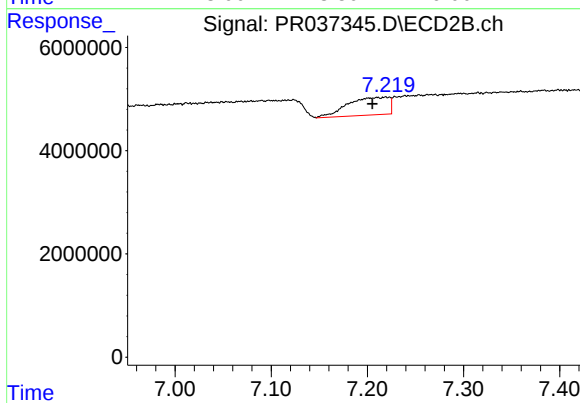

#38 AR-1262-3


R.T.: 7.219 min
Delta R.T.: 0.014 min
Response: 10250774
Conc: 18.70 ng/ml

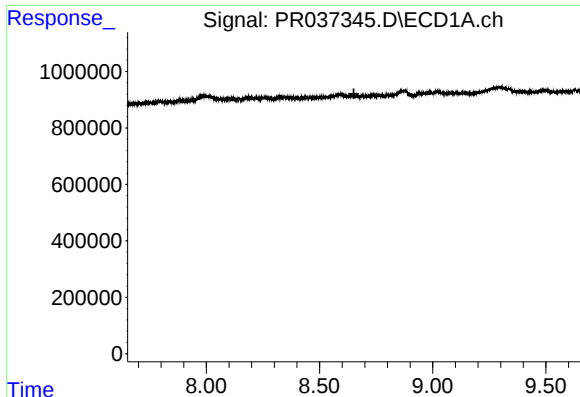

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

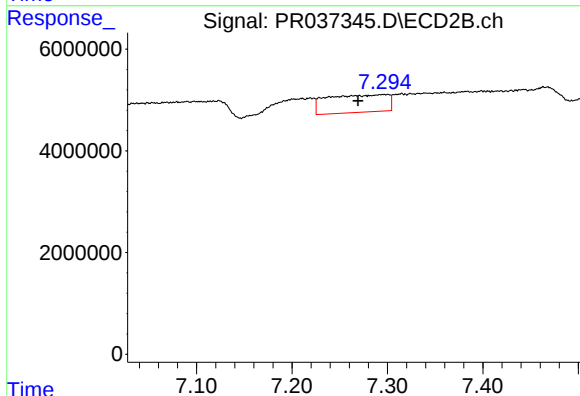


#39 AR-1262-4

R.T.: 7.300 min
Delta R.T.: 0.031 min
Response: 15386293
Conc: 17.14 ng/ml

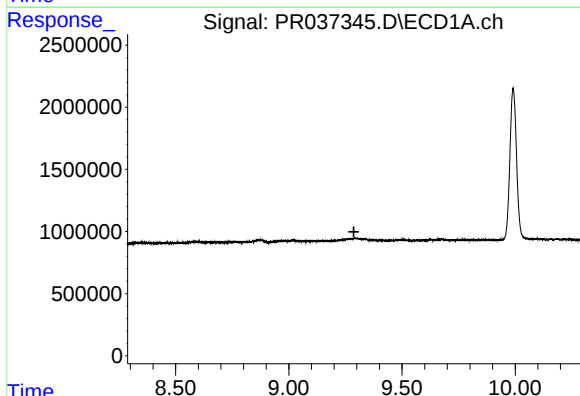


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

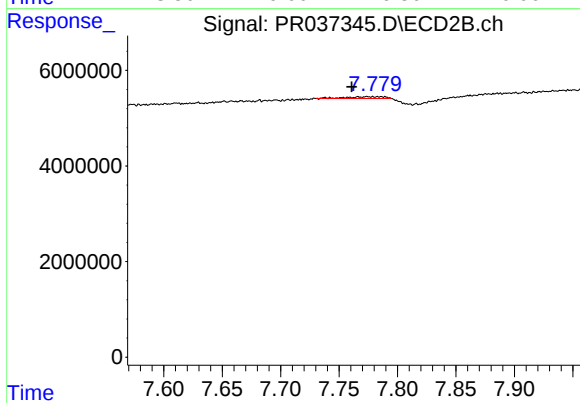

#40 AR-1262-5


R.T.: 7.779 min
Delta R.T.: 0.018 min
Response: 845412
Conc: 2.21 ng/ml

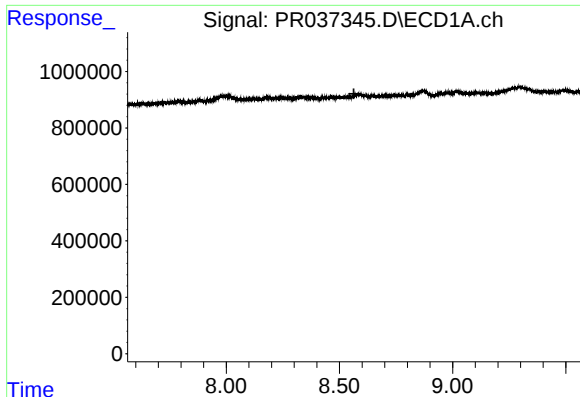

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

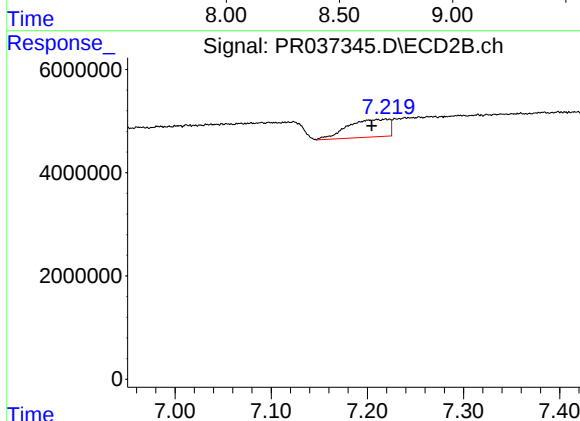


#41 AR-1268-1

R.T.: 7.219 min
Delta R.T.: 0.014 min
Response: 10250774
Conc: 8.33 ng/ml

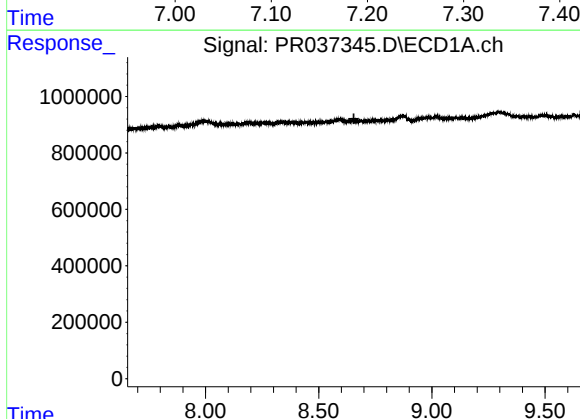


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

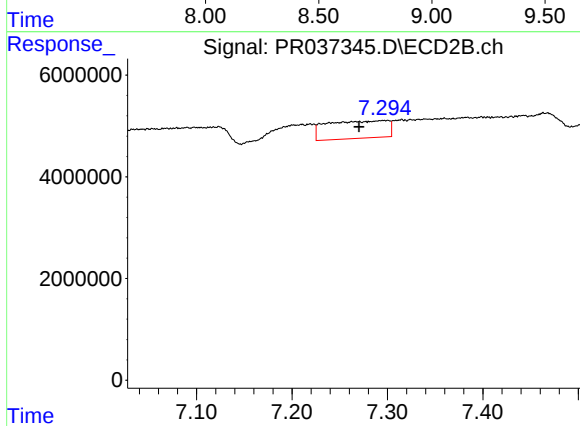

#42 AR-1268-2


R.T.: 7.300 min
Delta R.T.: 0.030 min
Response: 15386293
Conc: 14.53 ng/ml

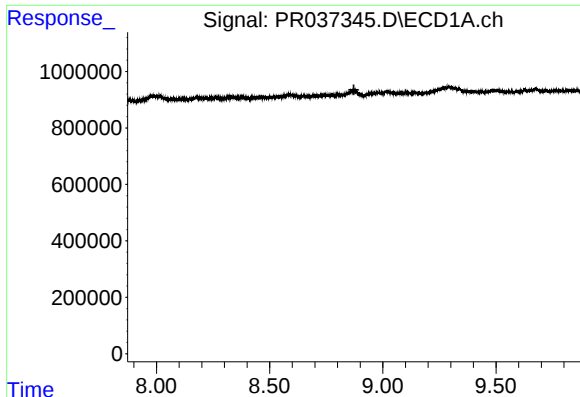

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

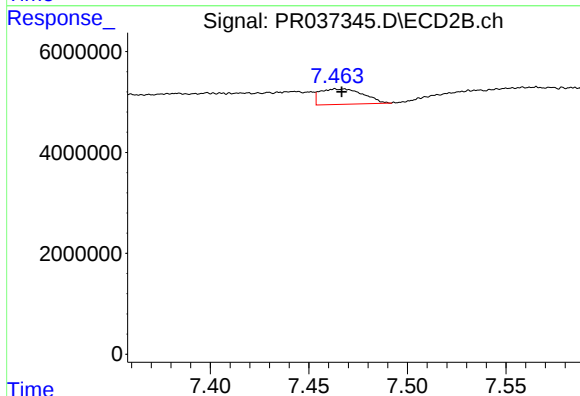


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 4682216
Conc: 5.28 ng/ml

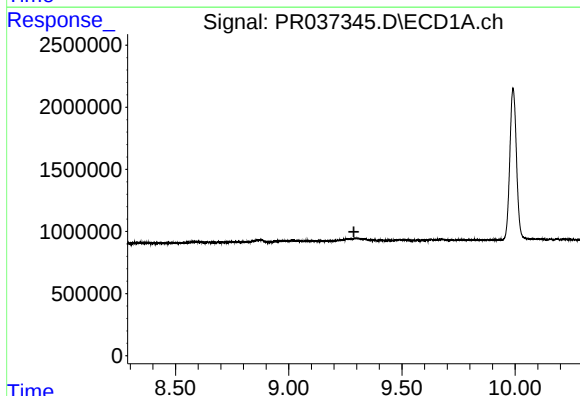


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

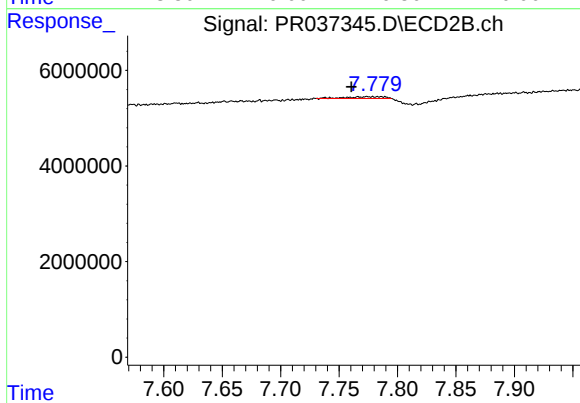

#44 AR-1268-4


R.T.: 7.779 min
Delta R.T.: 0.018 min
Response: 845412
Conc: 2.33 ng/ml

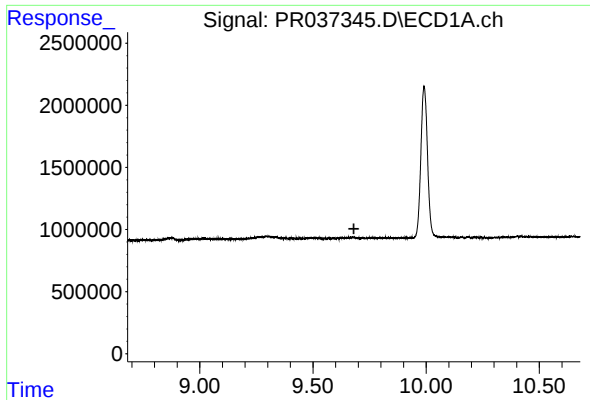

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

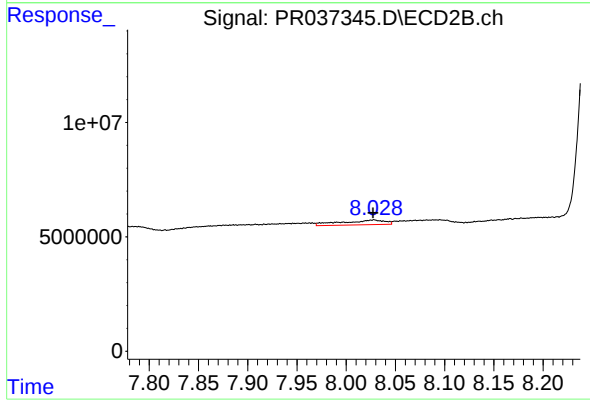

#45 AR-1268-5

R.T.: 8.028 min
Delta R.T.: 0.000 min
Response: 6404600
Conc: 2.52 ng/ml