

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 13:44
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1221 LOD 55PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:56:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.410	18431954	73747004	14.734	15.378
2)	SA Decachlor...	9.992	8.245	23095076	108.3E6	17.462	18.598
Target Compounds							
3)	L1 AR-1016-1	0.000	4.456	0	488495	N.D.	2.683 #
4)	L1 AR-1016-2	0.000	4.467	0	383049	N.D.	1.358 #
5)	L1 AR-1016-3	0.000	4.639	0	360405	N.D.	2.507 #
6)	L1 AR-1016-4	0.000	4.676	0	112375	N.D.	1.016 #
7)	L1 AR-1016-5	0.000	4.882	0	374073	N.D.	2.461 #
8)	L2 AR-1221-1	4.576	3.613	620156	2271374	49.600	44.608
9)	L2 AR-1221-2	4.664	3.698	721963	2277414	79.828	61.327
10)	L2 AR-1221-3	4.737	3.768	1339767	4623916	43.713	37.762
11)	L3 AR-1232-1	4.737	3.768	1339767	4623916	45.802	39.524
12)	L3 AR-1232-2	0.000	4.467	0	383049	N.D.	2.771 #
13)	L3 AR-1232-3	0.000	4.639	0	360405	N.D.	5.134 #
14)	L3 AR-1232-4	0.000	4.720	0	243307	N.D.	4.077 #
15)	L3 AR-1232-5	0.000	4.888	0	289967	N.D.	4.249 #
16)	L4 AR-1242-1	0.000	4.456	0	488495	N.D.	3.334 #
17)	L4 AR-1242-2	0.000	4.467	0	383049	N.D.	1.679 #
18)	L4 AR-1242-3	0.000	4.639	0	360405	N.D.	3.117 #
19)	L4 AR-1242-4	0.000	4.720	0	243307	N.D.	2.214 #
20)	L4 AR-1242-5	6.374	5.250	1097934	4162466	34.120	25.121 #
21)	L5 AR-1248-1	0.000	4.456	0	488495	N.D.	4.853 #
22)	L5 AR-1248-2	0.000	4.676	0	112375	N.D.	0.823 #
23)	L5 AR-1248-3	0.000	4.720	0	243307	N.D.	1.738 #
24)	L5 AR-1248-4	6.374	4.888	1097934	289967	22.428	1.629 #
25)	L5 AR-1248-5	6.374	5.250	1097934	4162466	23.243	21.279
26)	L6 AR-1254-1	6.374	5.250	1097934	4162466	20.097	12.084 #
27)	L6 AR-1254-2	0.000	5.385	0	4463131	N.D.	14.902 #
28)	L6 AR-1254-3	6.969	5.774	897166	6015024	9.863	12.700 #
29)	L6 AR-1254-4	7.297	5.996	1358616	135970	20.275	0.388 #
30)	L6 AR-1254-5	0.000	6.401	0	7684889	N.D.	17.354 #
31)	L7 AR-1260-1	0.000	5.903	0	137525	N.D.	0.471 #
32)	L7 AR-1260-2	7.387	6.071	671584	6352593	8.426	13.792 #
33)	L7 AR-1260-3	7.796	6.213	377930	455224	6.040	1.277 #
34)	L7 AR-1260-4	0.000	6.654	0	712080	N.D.	2.336 #
35)	L7 AR-1260-5	0.000	6.886	0	5834302	N.D.	6.727 #
36)	L8 AR-1262-1	7.796	6.511	377930	13812814	3.618	55.115 #
37)	L8 AR-1262-2	0.000	6.886	0	5834302	N.D.	4.645 #
38)	L8 AR-1262-3	8.589	7.249	628872	26627052	4.782	48.566 #
39)	L8 AR-1262-4	8.589	7.286	628872	16931700	6.402	18.862 #
40)	L8 AR-1262-5	0.000	7.784	0	1354336	N.D.	3.540 #
41)	L9 AR-1268-1	8.589	7.249	628872	26627052	3.511	21.630 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 13:44
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1221 LOD 55PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:56:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.589	7.286	628872	16931700	3.823	15.990 #
43) L9	AR-1268-3	0.000	7.464	0	48656077	N.D.	54.902 #
44) L9	AR-1268-4	0.000	7.784	0	1354336	N.D.	3.733 #
45) L9	AR-1268-5	0.000	8.030	0	38511871	N.D.	15.137 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 13:44
Operator : SM\SJ
Sample : K2241-07
Misc : AR1221 LOD 55PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:56:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

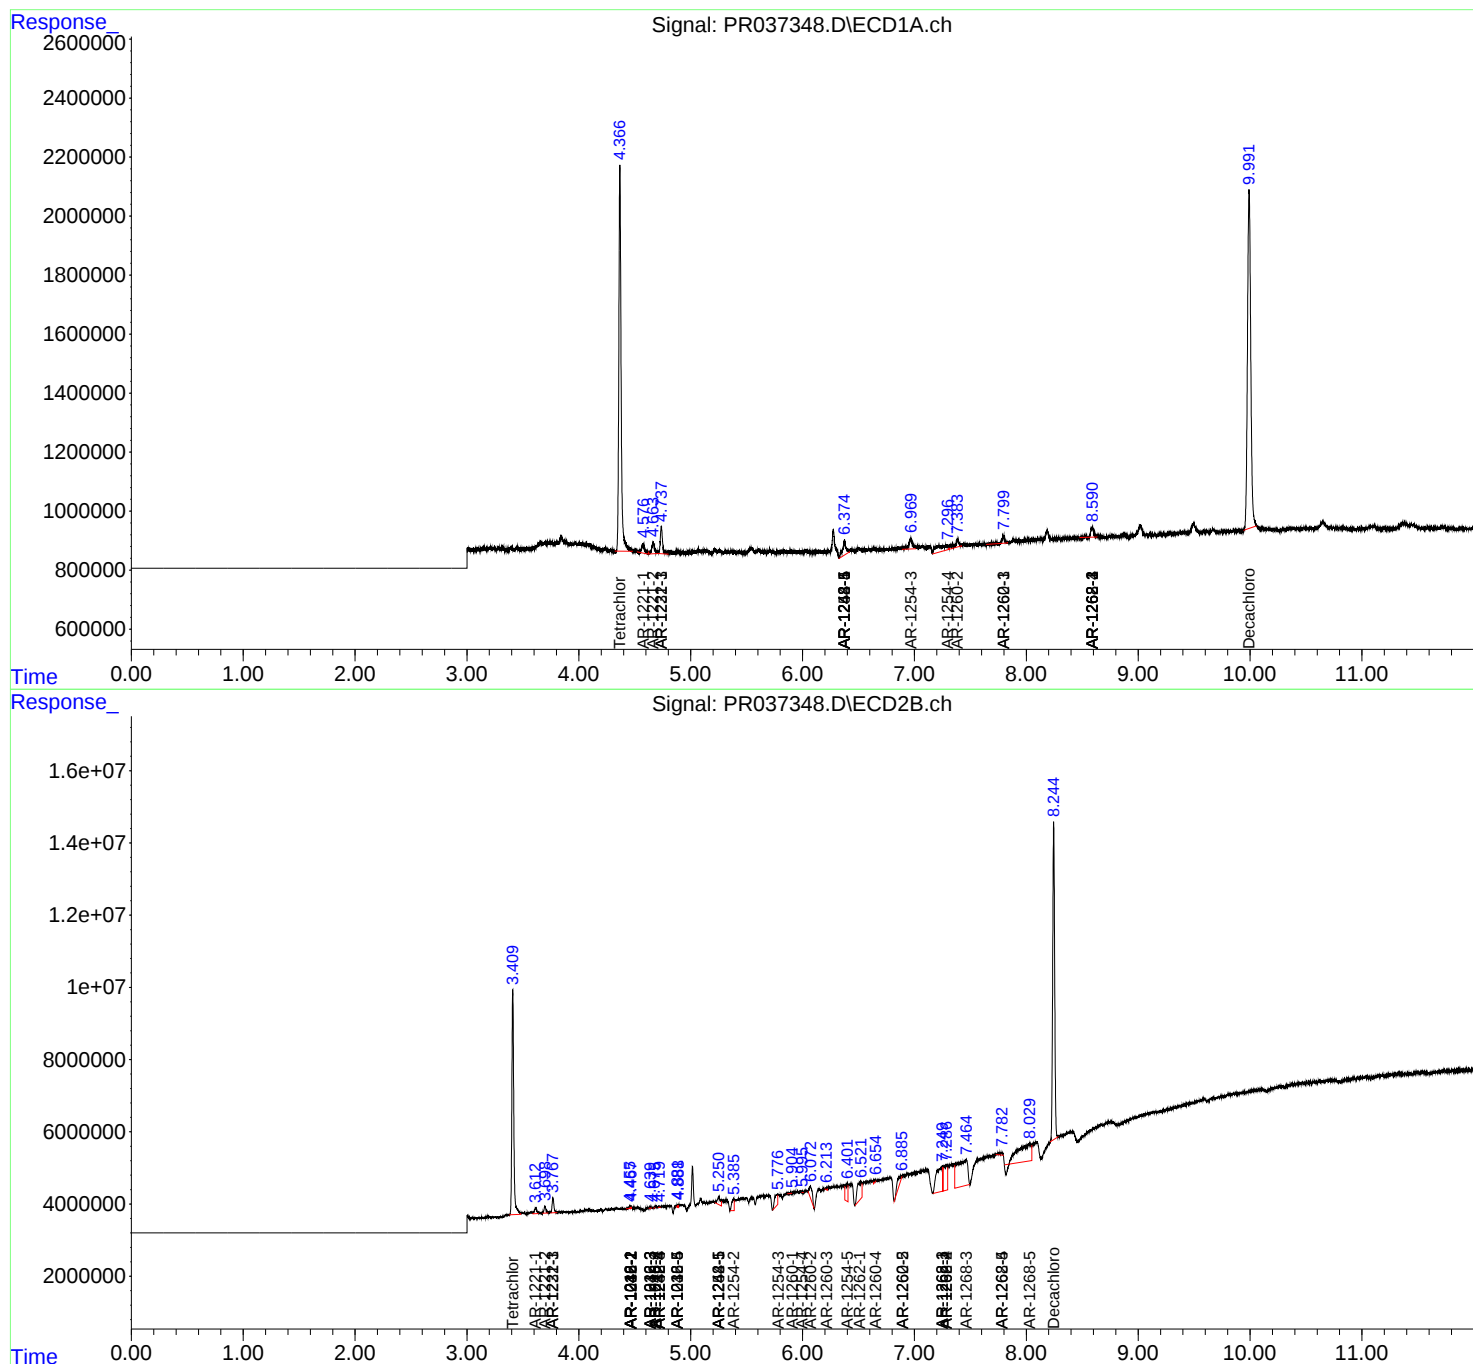


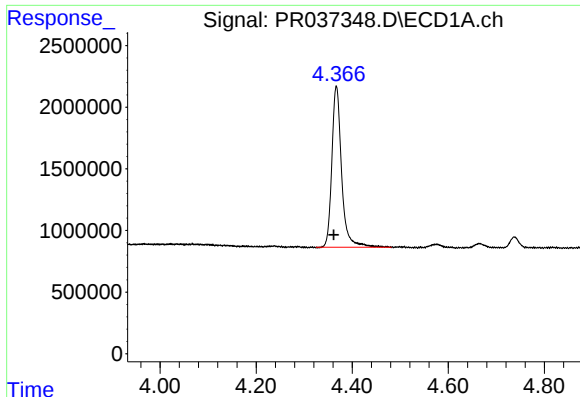

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: 0.005 min
Response: 18431954
Conc: 14.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

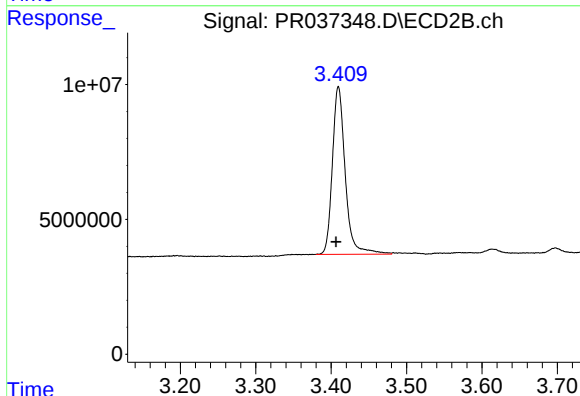


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.003 min
Response: 73747004
Conc: 15.38 ng/ml

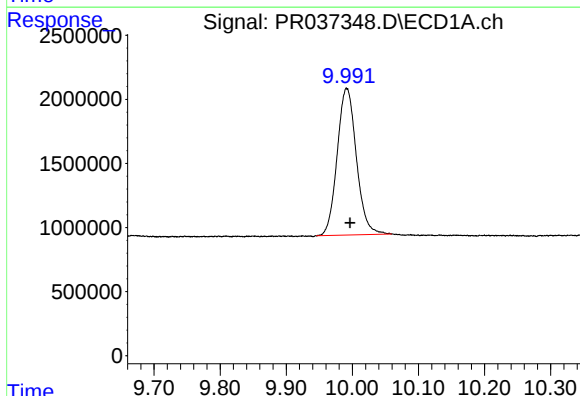


#2 Decachlorobiphenyl

R.T.: 9.992 min
Delta R.T.: -0.005 min
Response: 23095076
Conc: 17.46 ng/ml

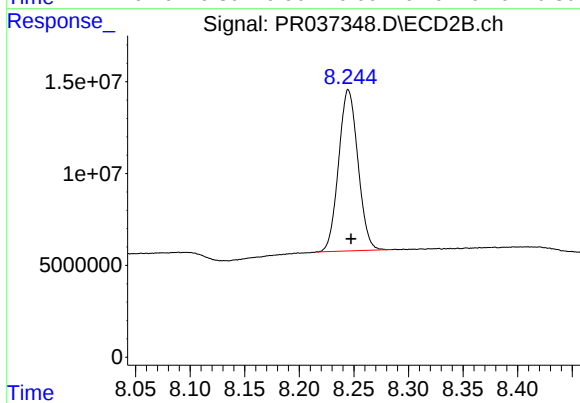

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.002 min
Response: 108320199
Conc: 18.60 ng/ml

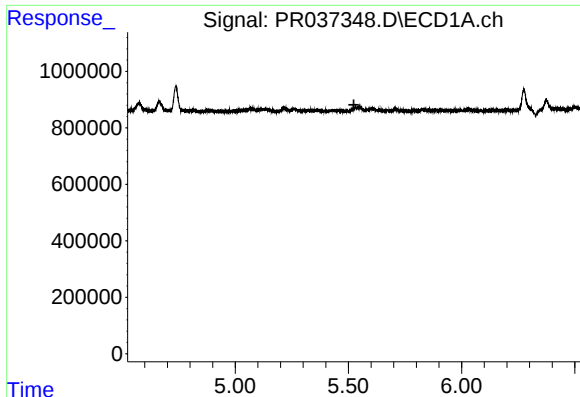

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

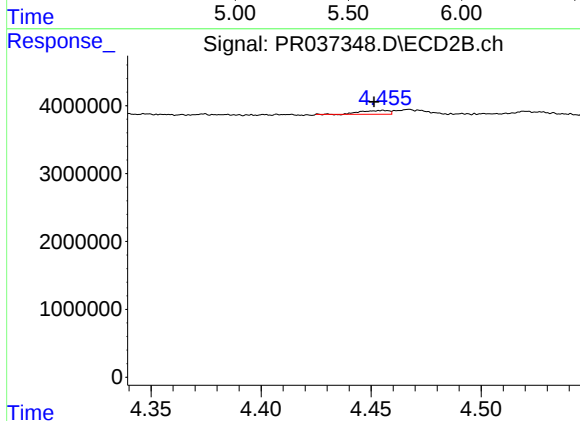


#3 AR-1016-1

R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 488495
Conc: 2.68 ng/ml

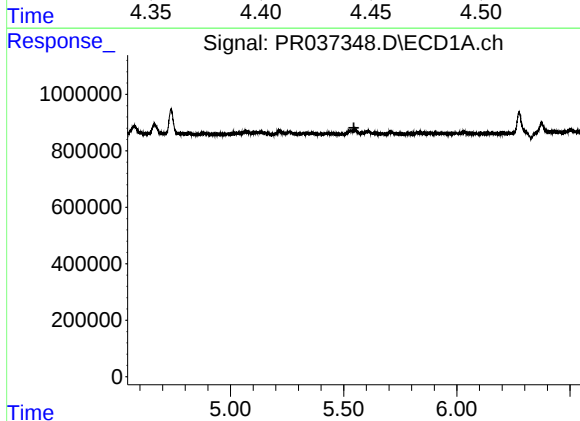


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

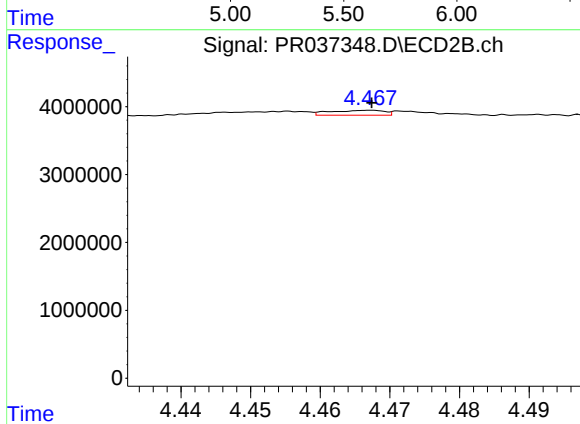

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 383049
Conc: 1.36 ng/ml

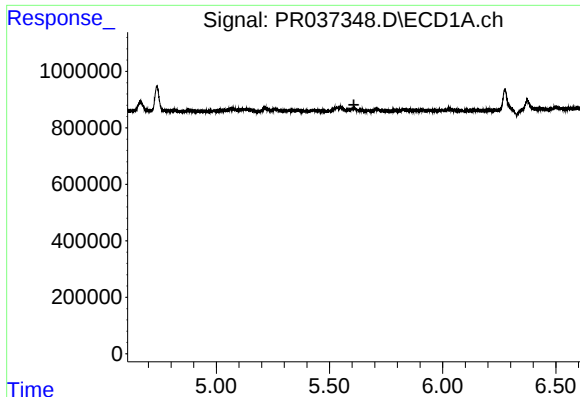

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

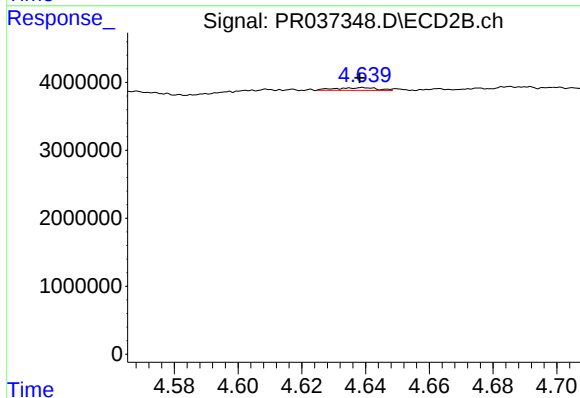


#5 AR-1016-3

R.T.: 4.639 min
Delta R.T.: 0.001 min
Response: 360405
Conc: 2.51 ng/ml

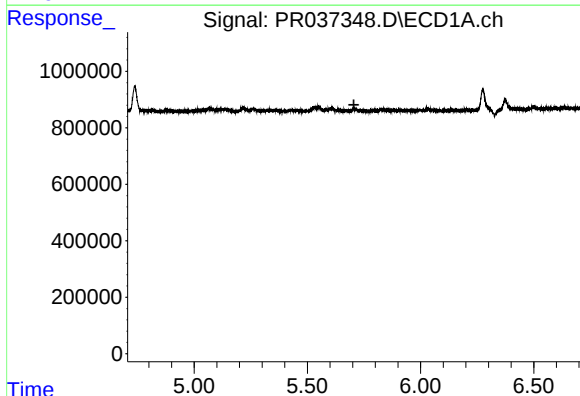


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

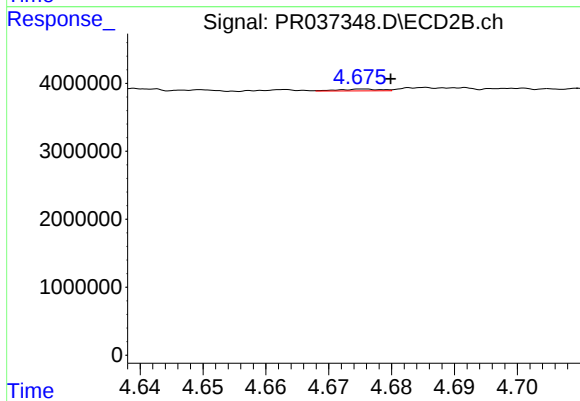

#6 AR-1016-4


R.T.: 4.676 min
Delta R.T.: -0.004 min
Response: 112375
Conc: 1.02 ng/ml

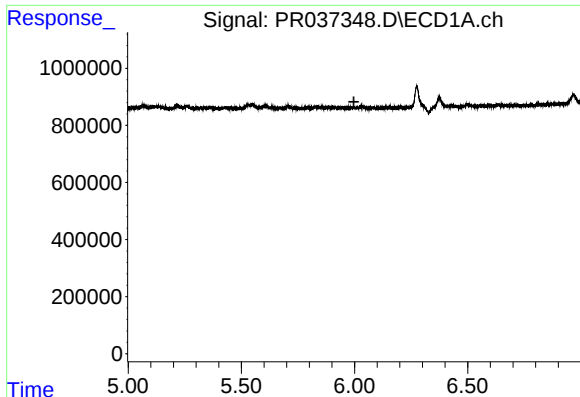

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

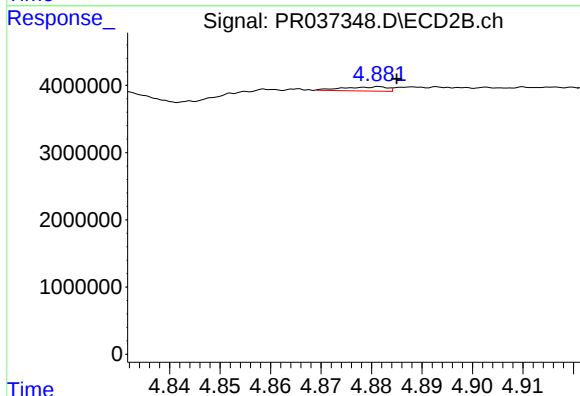


#7 AR-1016-5

R.T.: 4.882 min
Delta R.T.: -0.003 min
Response: 374073
Conc: 2.46 ng/ml

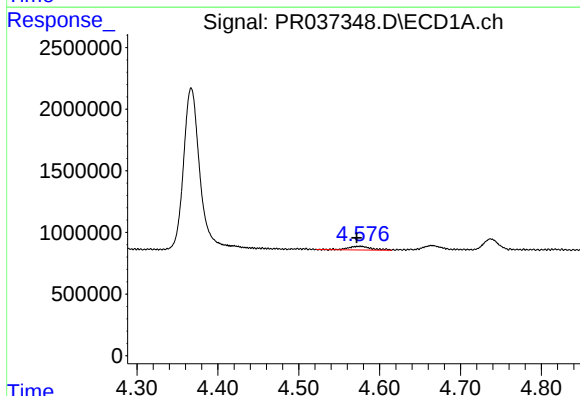


#8 AR-1221-1

R.T.: 4.576 min
Delta R.T.: 0.005 min
Response: 620156
Conc: 49.60 ng/ml

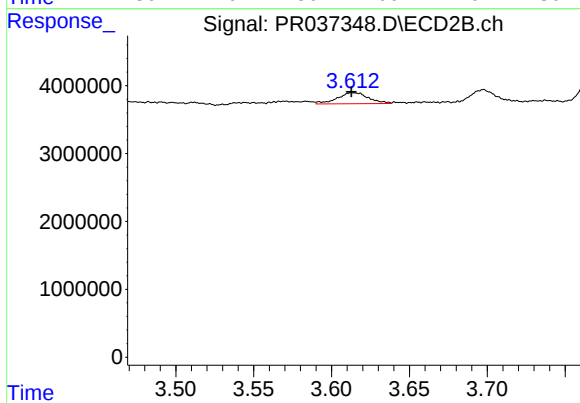

#8 AR-1221-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 2271374
Conc: 44.61 ng/ml

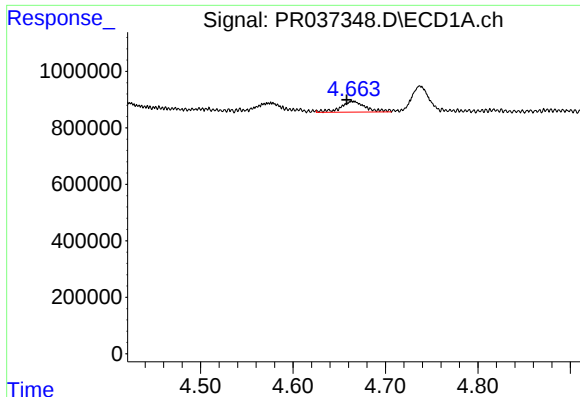

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 721963
Conc: 79.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

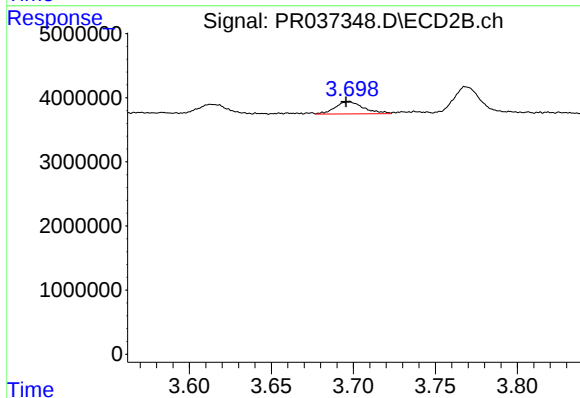


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 2277414
Conc: 61.33 ng/ml

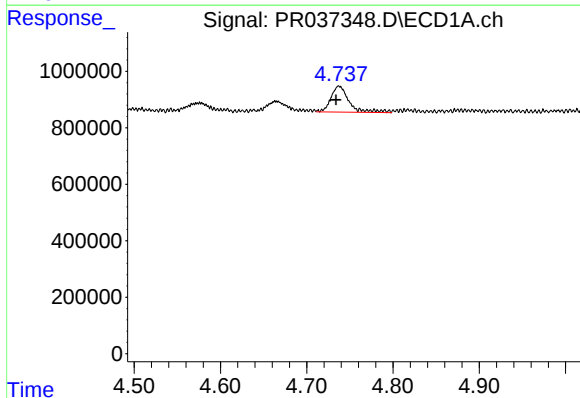


#10 AR-1221-3

R.T.: 4.737 min
Delta R.T.: 0.003 min
Response: 1339767
Conc: 43.71 ng/ml

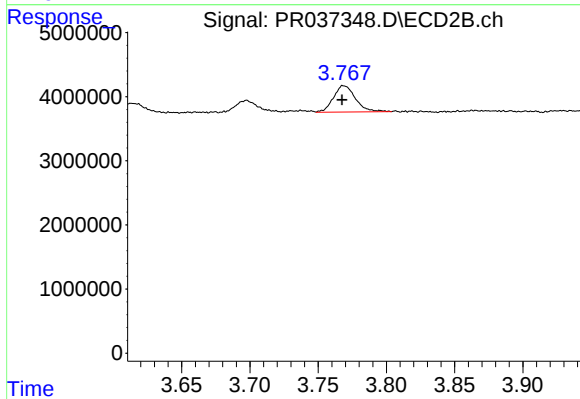

#10 AR-1221-3


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 4623916
Conc: 37.76 ng/ml

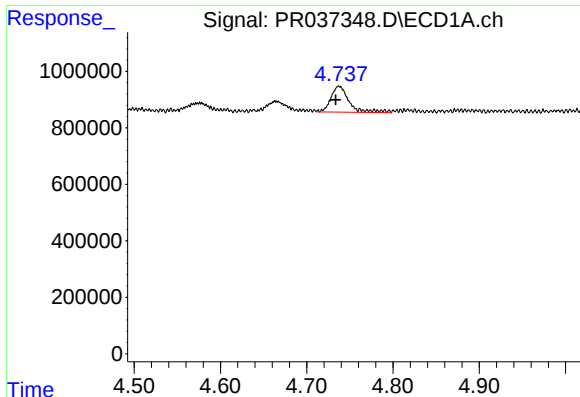

#11 AR-1232-1


R.T.: 4.737 min
Delta R.T.: 0.004 min
Response: 1339767
Conc: 45.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

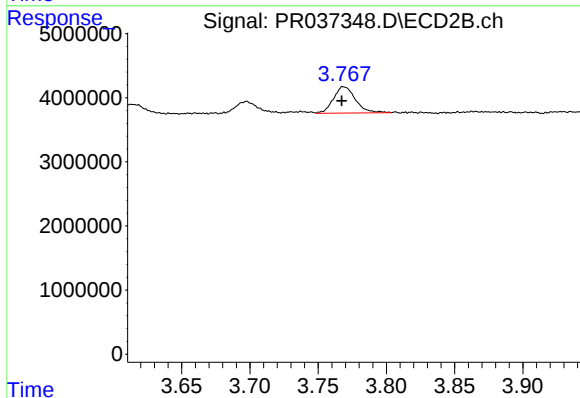


#11 AR-1232-1

R.T.: 3.768 min
Delta R.T.: 0.001 min
Response: 4623916
Conc: 39.52 ng/ml

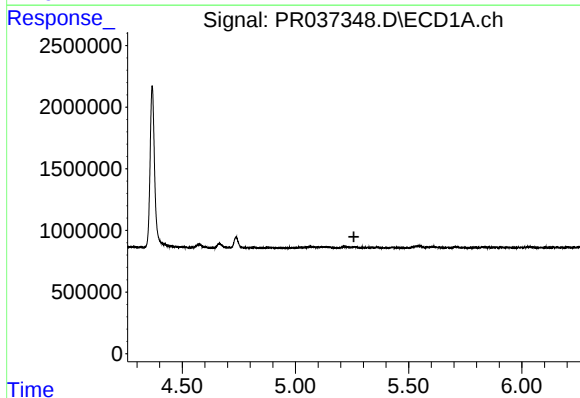


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

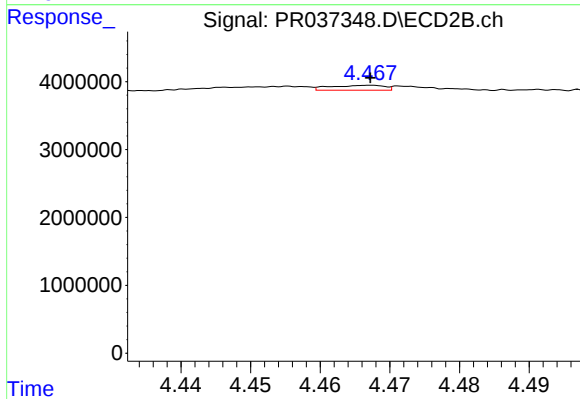

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 383049
Conc: 2.77 ng/ml

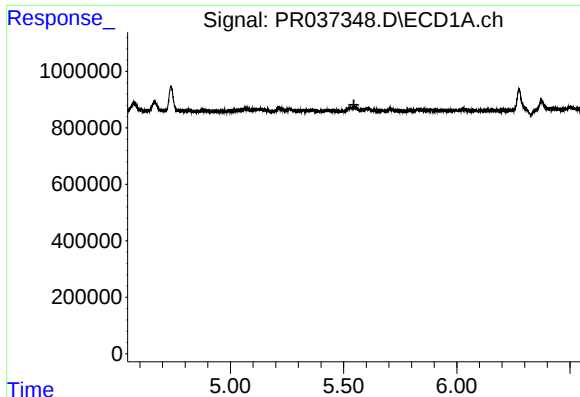

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

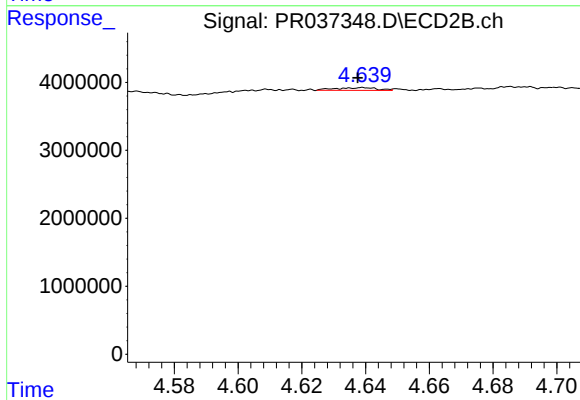


#13 AR-1232-3

R.T.: 4.639 min
Delta R.T.: 0.002 min
Response: 360405
Conc: 5.13 ng/ml

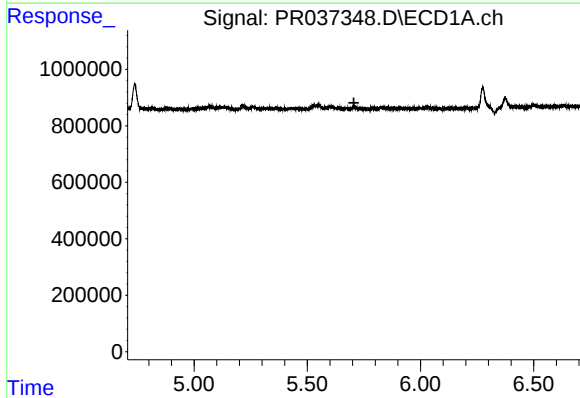


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

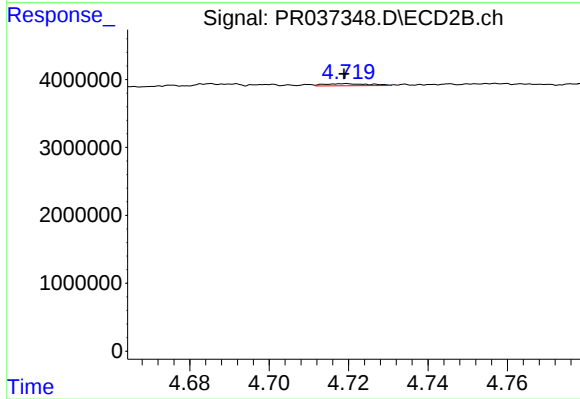

#14 AR-1232-4


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 243307
Conc: 4.08 ng/ml

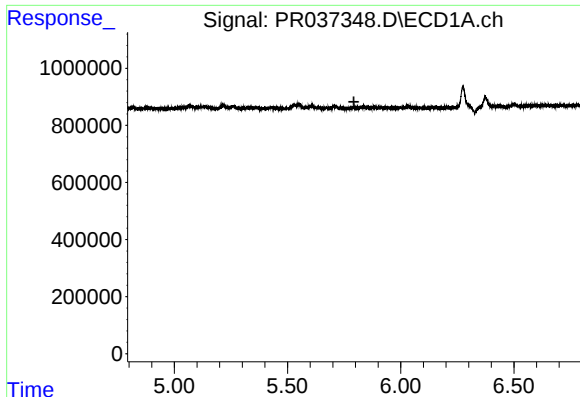

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

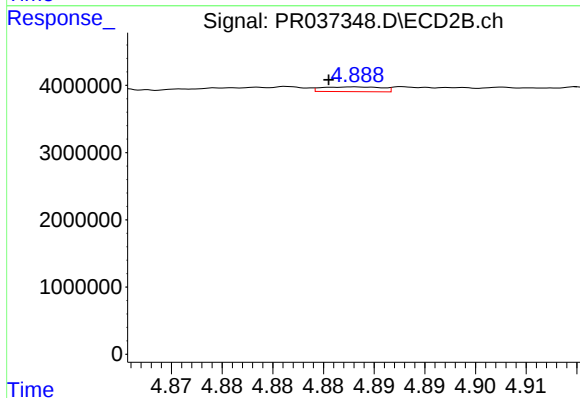


#15 AR-1232-5

R.T.: 4.888 min
Delta R.T.: 0.003 min
Response: 289967
Conc: 4.25 ng/ml

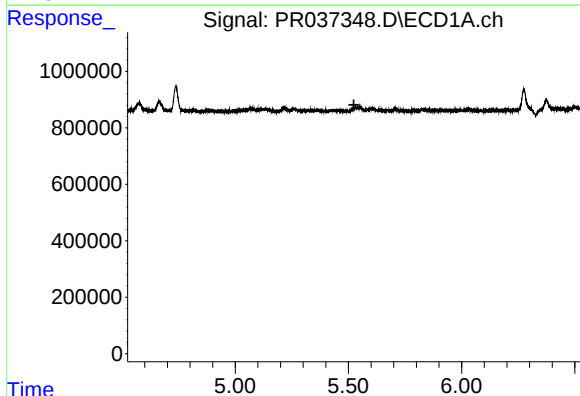


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

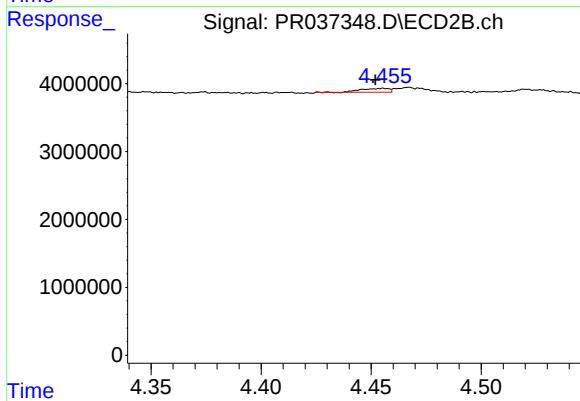

#16 AR-1242-1


R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 488495
Conc: 3.33 ng/ml

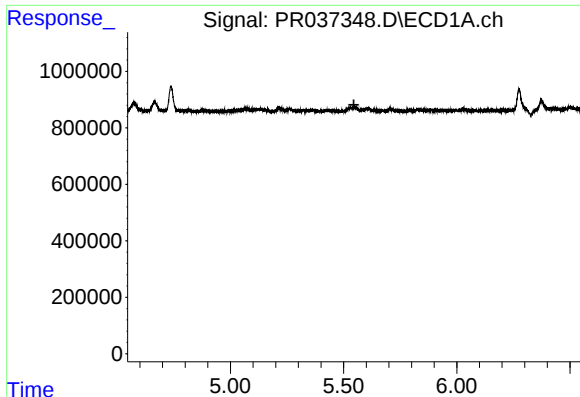

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

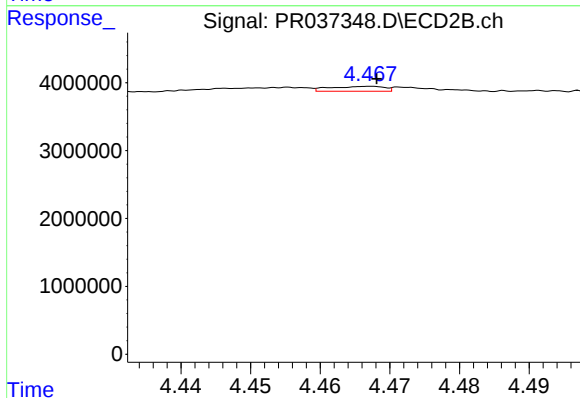


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 383049
Conc: 1.68 ng/ml

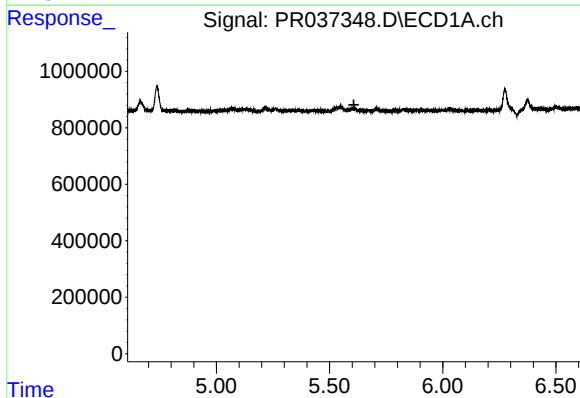


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

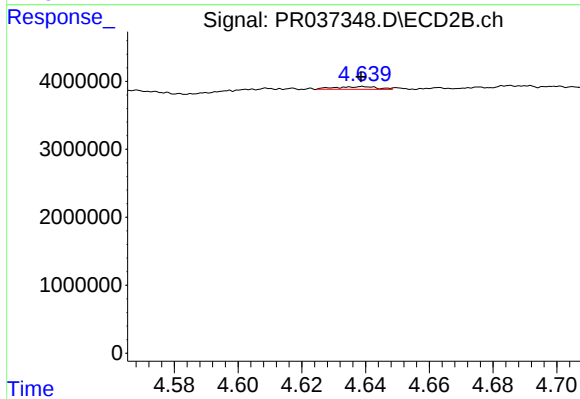

#18 AR-1242-3


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 360405
Conc: 3.12 ng/ml

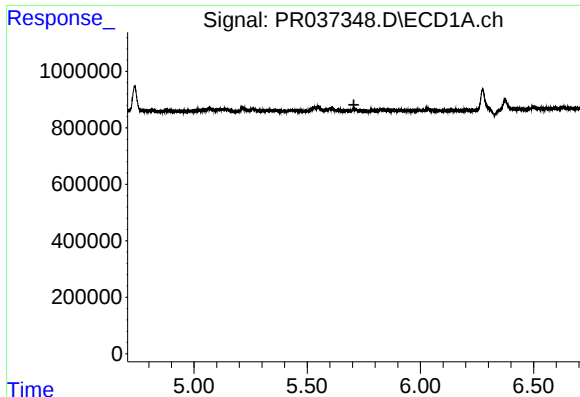

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

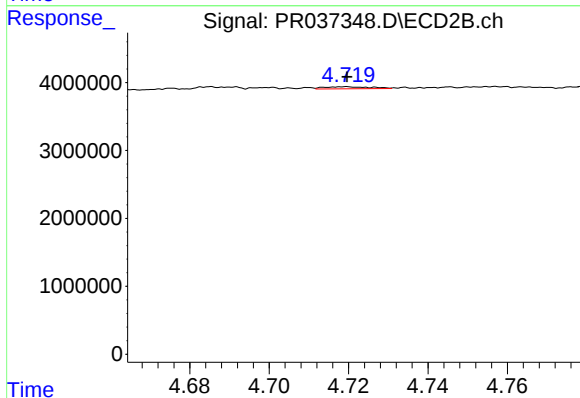


#19 AR-1242-4

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 243307
Conc: 2.21 ng/ml

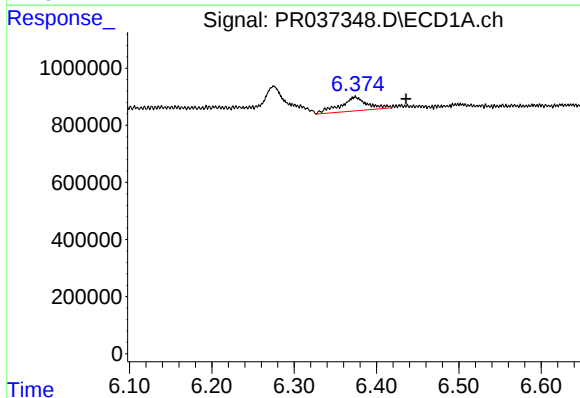


#20 AR-1242-5

R.T.: 6.374 min
Delta R.T.: -0.062 min
Response: 1097934
Conc: 34.12 ng/ml

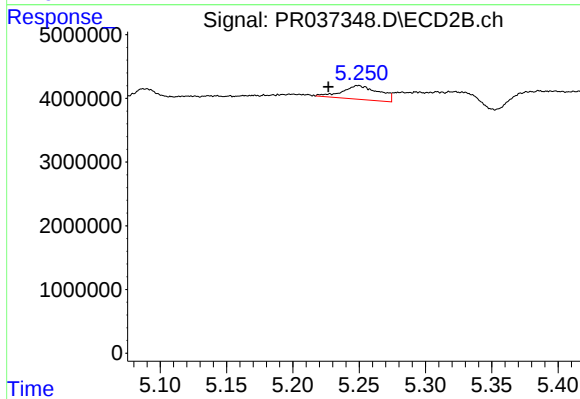

#20 AR-1242-5


R.T.: 5.250 min
Delta R.T.: 0.023 min
Response: 4162466
Conc: 25.12 ng/ml

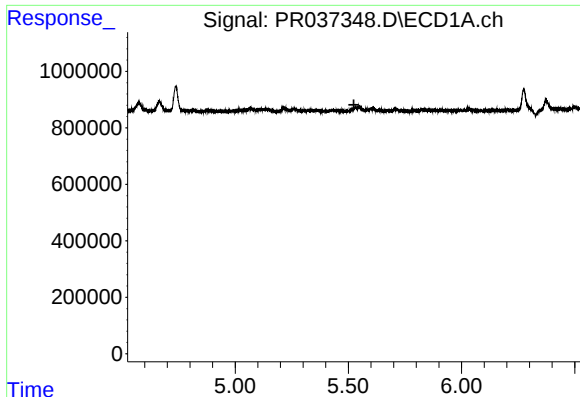

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

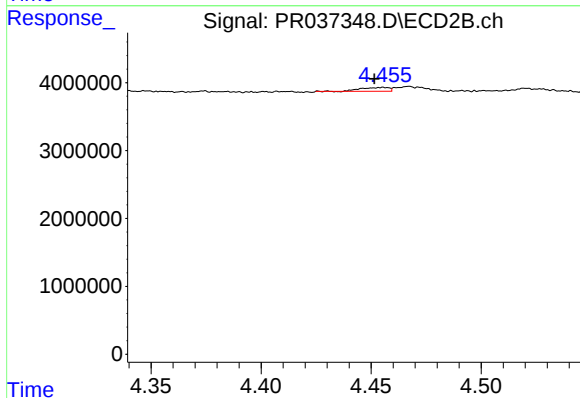


#21 AR-1248-1

R.T.: 4.456 min
Delta R.T.: 0.004 min
Response: 488495
Conc: 4.85 ng/ml

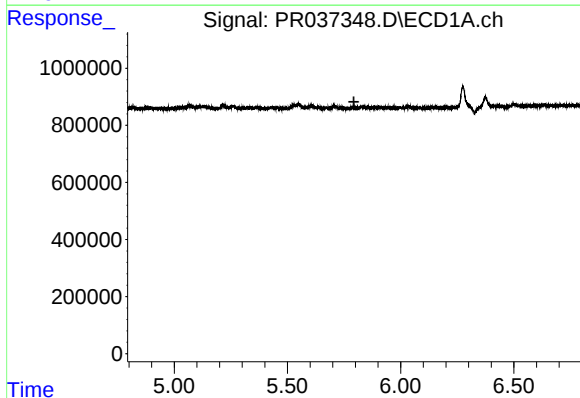


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

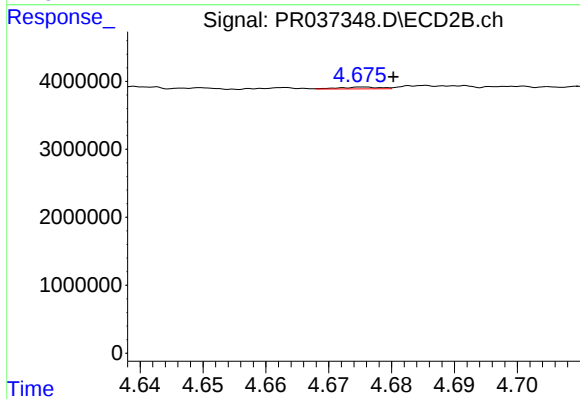

#22 AR-1248-2


R.T.: 4.676 min
Delta R.T.: -0.005 min
Response: 112375
Conc: 0.82 ng/ml

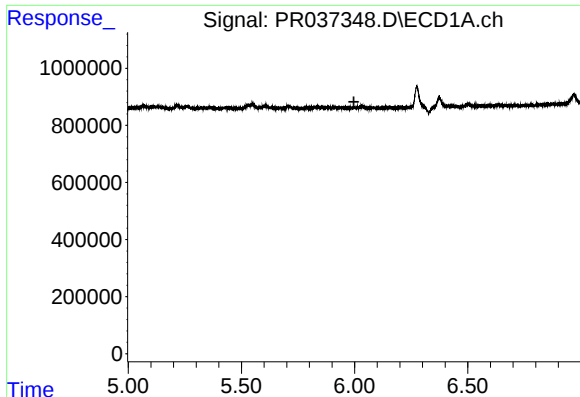

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

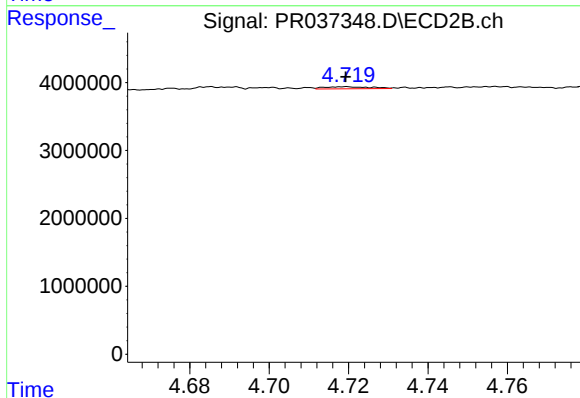


#23 AR-1248-3

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 243307
Conc: 1.74 ng/ml

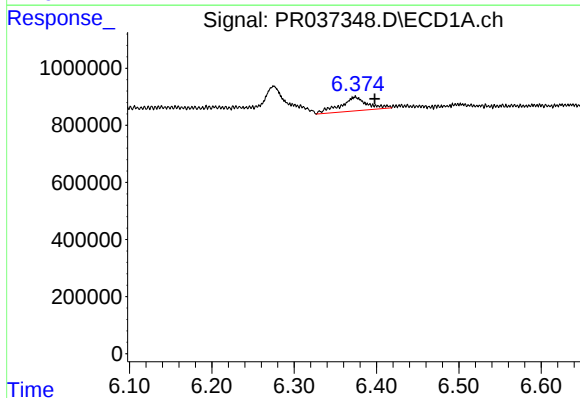


#24 AR-1248-4

R.T.: 6.374 min
Delta R.T.: -0.024 min
Response: 1097934
Conc: 22.43 ng/ml

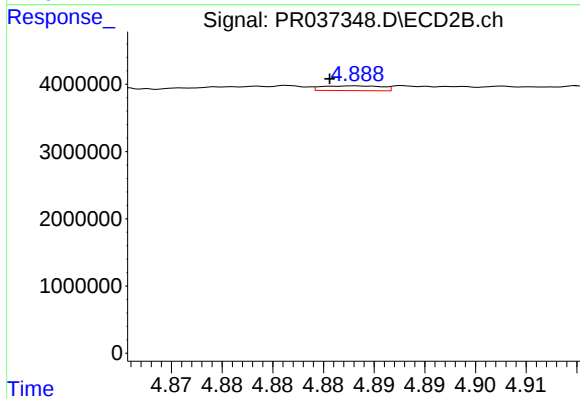

#24 AR-1248-4


R.T.: 4.888 min
Delta R.T.: 0.003 min
Response: 289967
Conc: 1.63 ng/ml

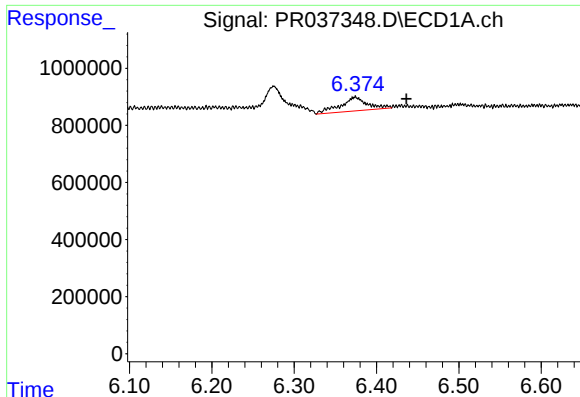

#25 AR-1248-5


R.T.: 6.374 min
Delta R.T.: -0.062 min
Response: 1097934
Conc: 23.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

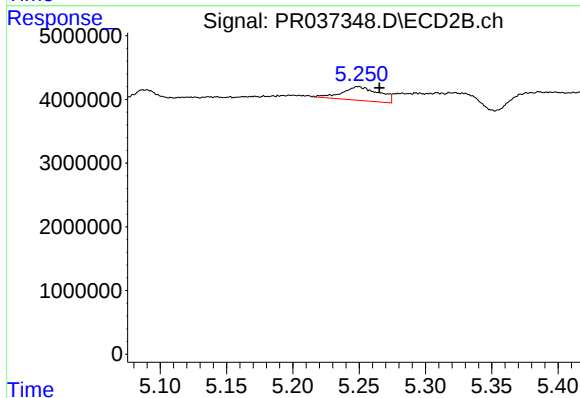


#25 AR-1248-5

R.T.: 5.250 min
Delta R.T.: -0.015 min
Response: 4162466
Conc: 21.28 ng/ml

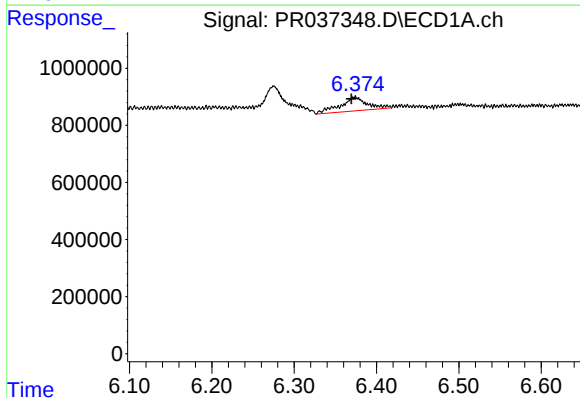


#26 AR-1254-1

R.T.: 6.374 min
Delta R.T.: 0.005 min
Response: 1097934
Conc: 20.10 ng/ml

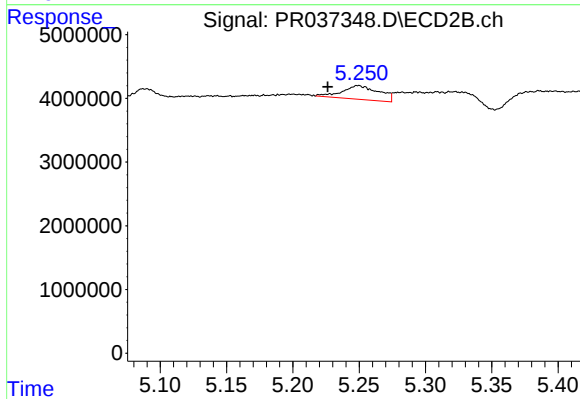

#26 AR-1254-1


R.T.: 5.250 min
Delta R.T.: 0.024 min
Response: 4162466
Conc: 12.08 ng/ml

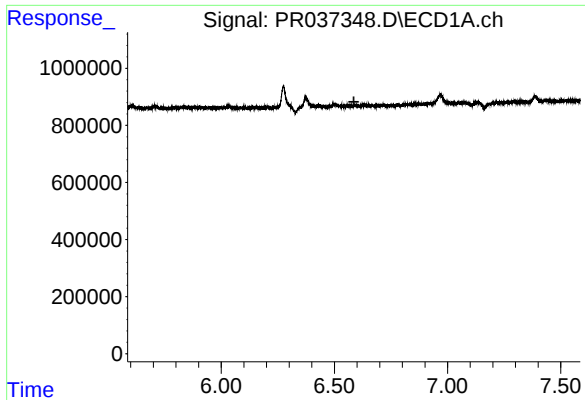

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

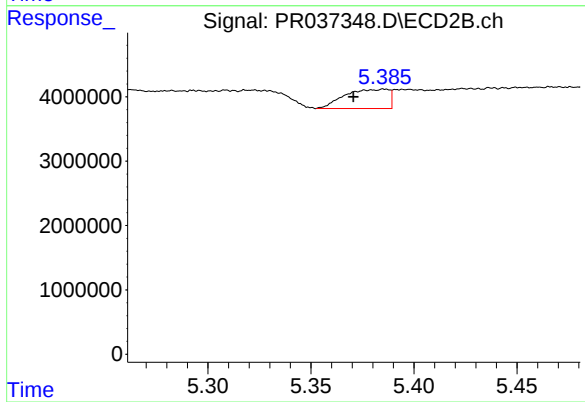


#27 AR-1254-2

R.T.: 5.385 min
Delta R.T.: 0.015 min
Response: 4463131
Conc: 14.90 ng/ml

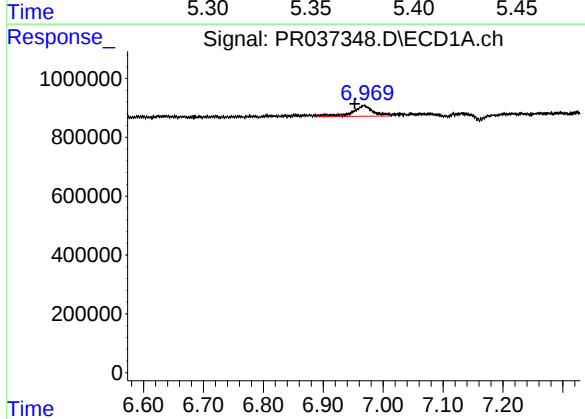


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.016 min
Response: 897166
Conc: 9.86 ng/ml

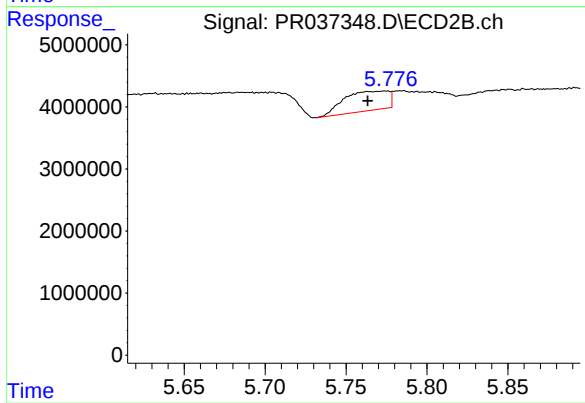

#28 AR-1254-3


R.T.: 5.774 min
Delta R.T.: 0.011 min
Response: 6015024
Conc: 12.70 ng/ml

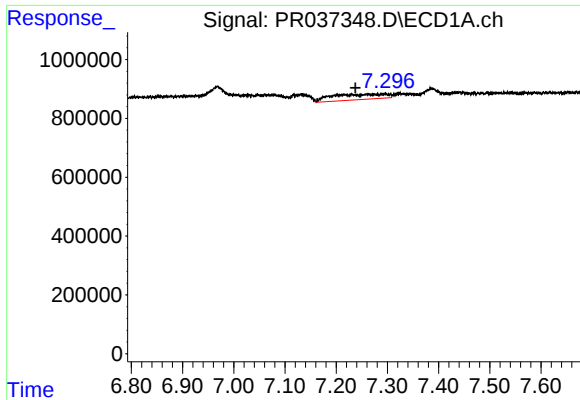

#29 AR-1254-4


R.T.: 7.297 min
Delta R.T.: 0.059 min
Response: 1358616
Conc: 20.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

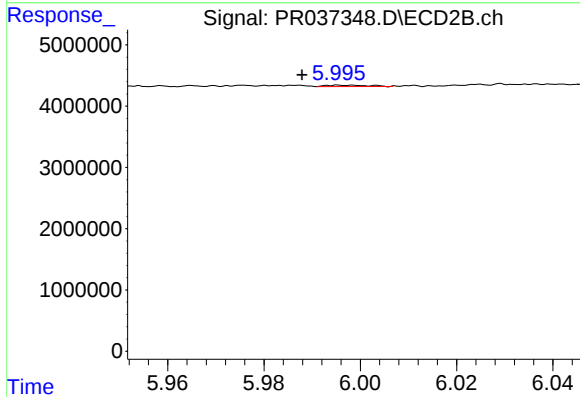


#29 AR-1254-4

R.T.: 5.996 min
Delta R.T.: 0.008 min
Response: 135970
Conc: 0.39 ng/ml

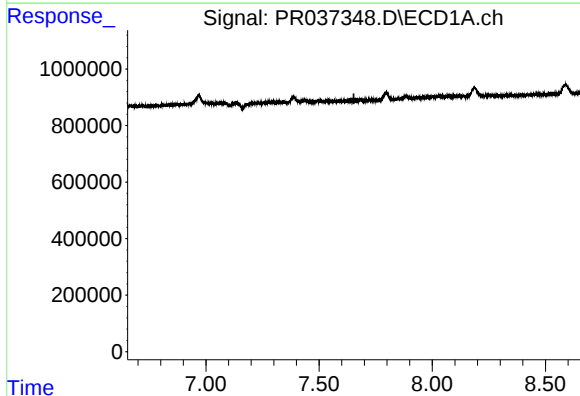


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

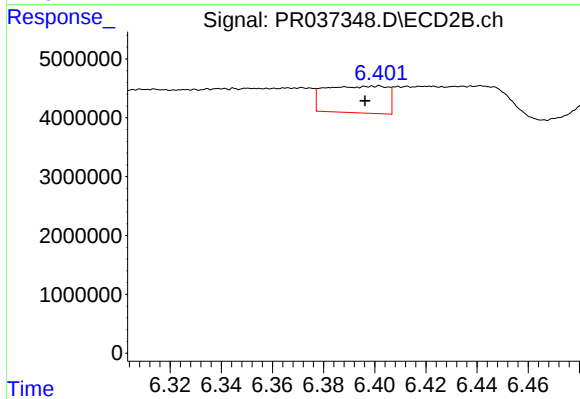

#30 AR-1254-5


R.T.: 6.401 min
Delta R.T.: 0.005 min
Response: 7684889
Conc: 17.35 ng/ml

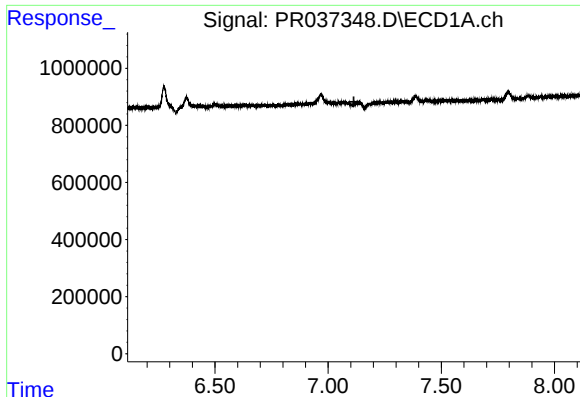

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

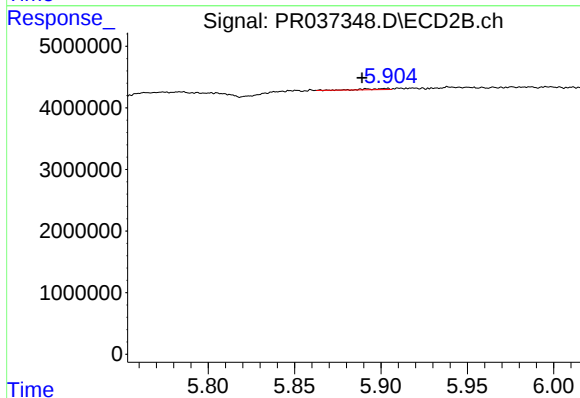


#31 AR-1260-1

R.T.: 5.903 min
Delta R.T.: 0.014 min
Response: 137525
Conc: 0.47 ng/ml

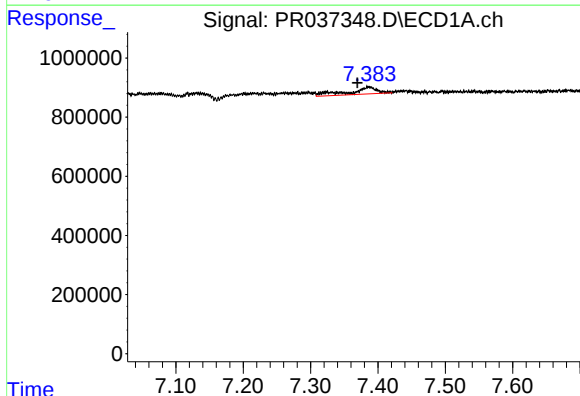


#32 AR-1260-2

R.T.: 7.387 min
Delta R.T.: 0.018 min
Response: 671584
Conc: 8.43 ng/ml

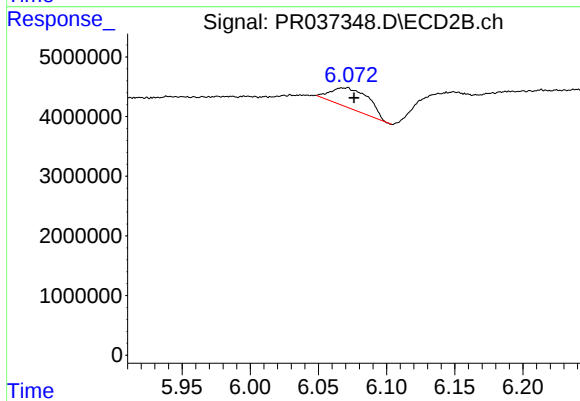

#32 AR-1260-2


R.T.: 6.071 min
Delta R.T.: -0.005 min
Response: 6352593
Conc: 13.79 ng/ml

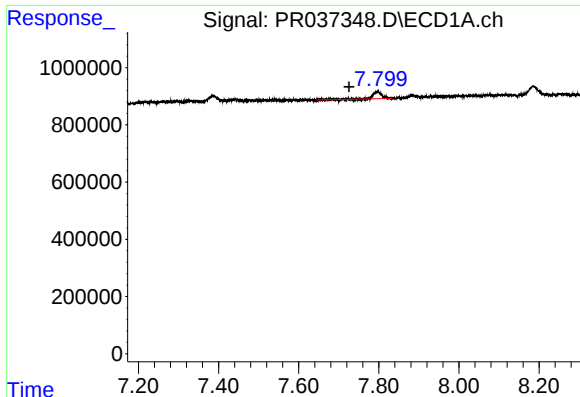

#33 AR-1260-3


R.T.: 7.796 min
Delta R.T.: 0.070 min
Response: 377930
Conc: 6.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

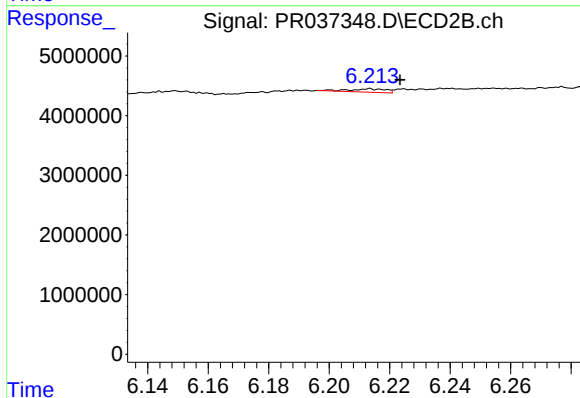


#33 AR-1260-3

R.T.: 6.213 min
Delta R.T.: -0.010 min
Response: 455224
Conc: 1.28 ng/ml

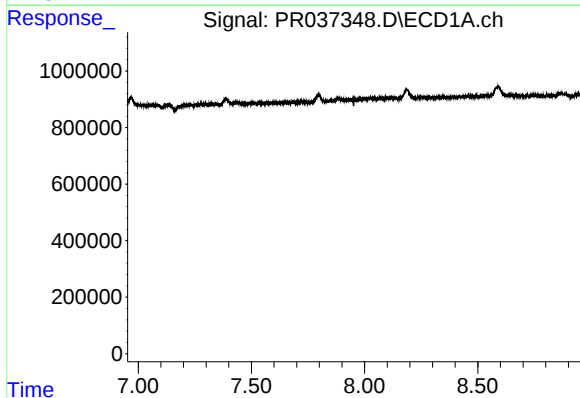


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.953 min
Response: 0
Conc: N.D.

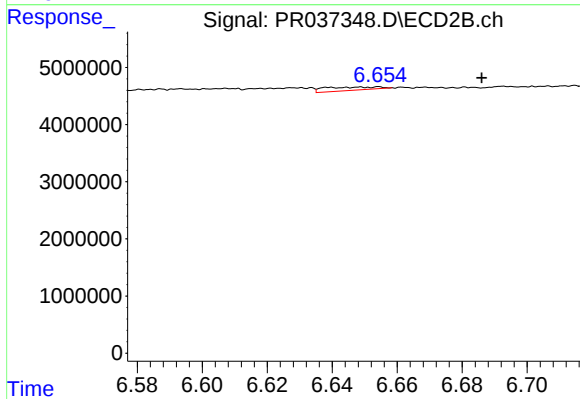

#34 AR-1260-4


R.T.: 6.654 min
Delta R.T.: -0.032 min
Response: 712080
Conc: 2.34 ng/ml

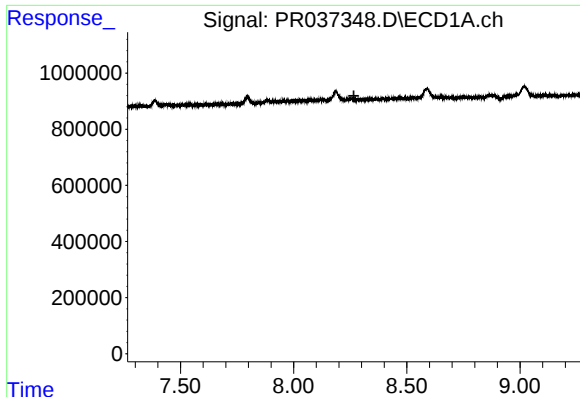

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

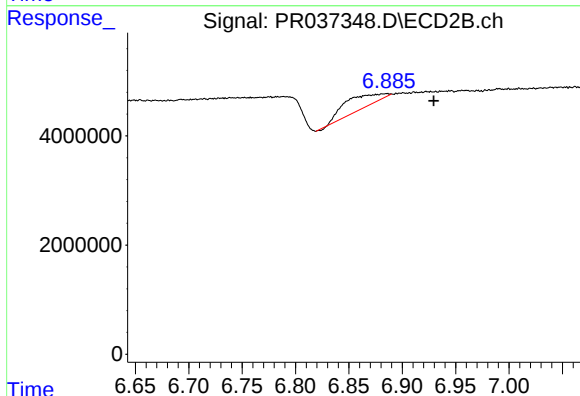


#35 AR-1260-5

R.T.: 6.886 min
Delta R.T.: -0.044 min
Response: 5834302
Conc: 6.73 ng/ml

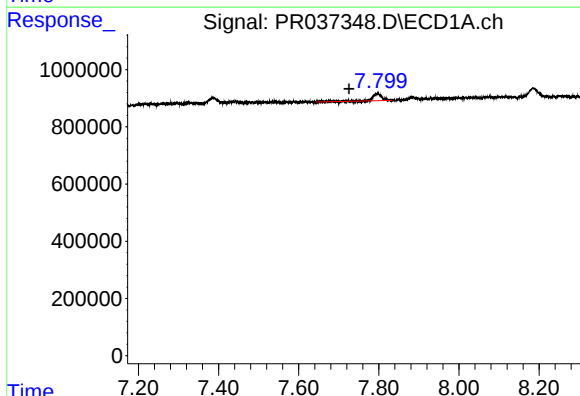


#36 AR-1262-1

R.T.: 7.796 min
Delta R.T.: 0.070 min
Response: 377930
Conc: 3.62 ng/ml

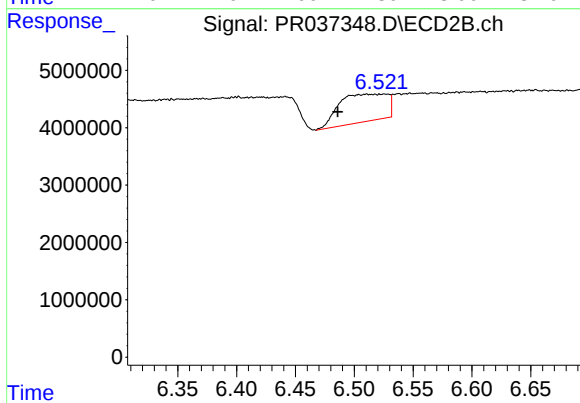

#36 AR-1262-1


R.T.: 6.511 min
Delta R.T.: 0.025 min
Response: 13812814
Conc: 55.11 ng/ml

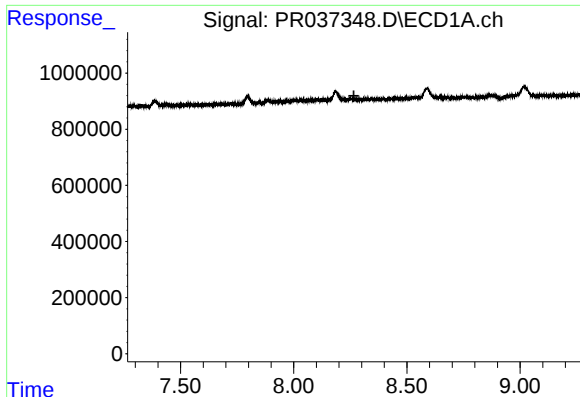

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

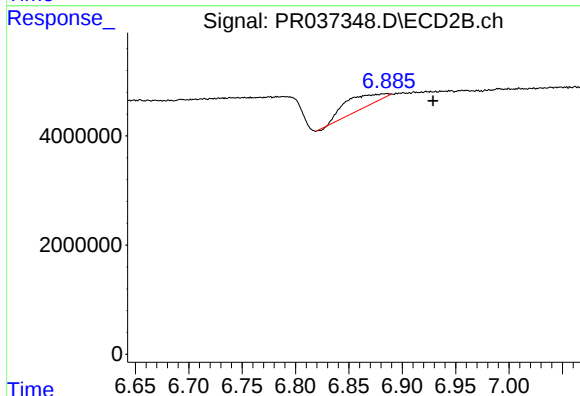


#37 AR-1262-2

R.T.: 6.886 min
Delta R.T.: -0.043 min
Response: 5834302
Conc: 4.65 ng/ml

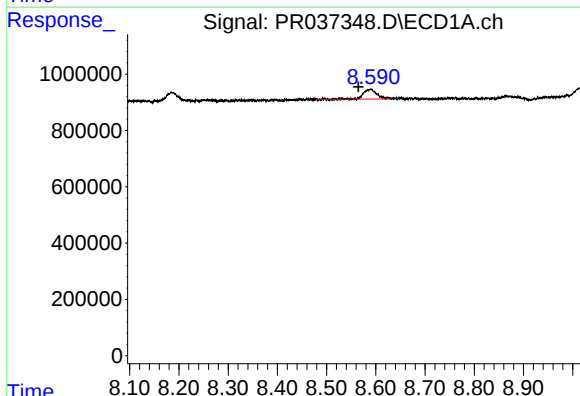


#38 AR-1262-3

R.T.: 8.589 min
Delta R.T.: 0.024 min
Response: 628872
Conc: 4.78 ng/ml

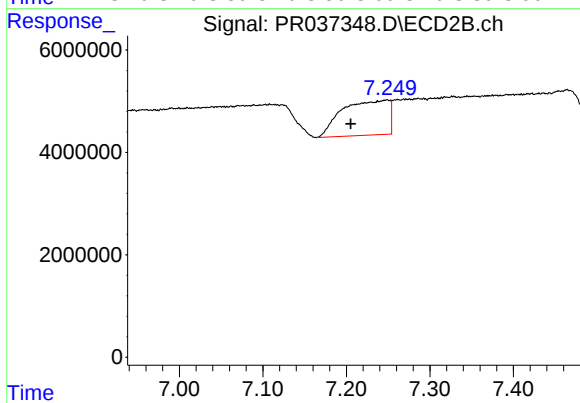

#38 AR-1262-3


R.T.: 7.249 min
Delta R.T.: 0.043 min
Response: 26627052
Conc: 48.57 ng/ml

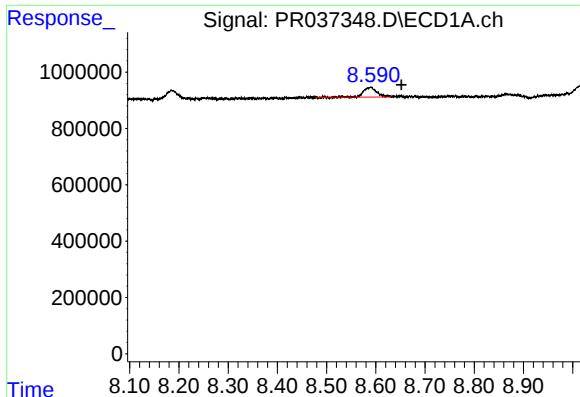

#39 AR-1262-4


R.T.: 8.589 min
Delta R.T.: -0.063 min
Response: 628872
Conc: 6.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

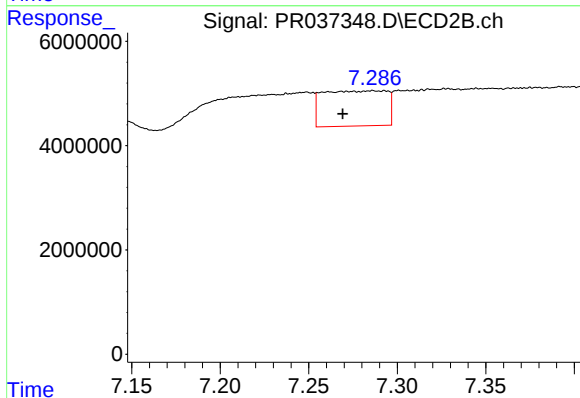


#39 AR-1262-4

R.T.: 7.286 min
Delta R.T.: 0.017 min
Response: 16931700
Conc: 18.86 ng/ml

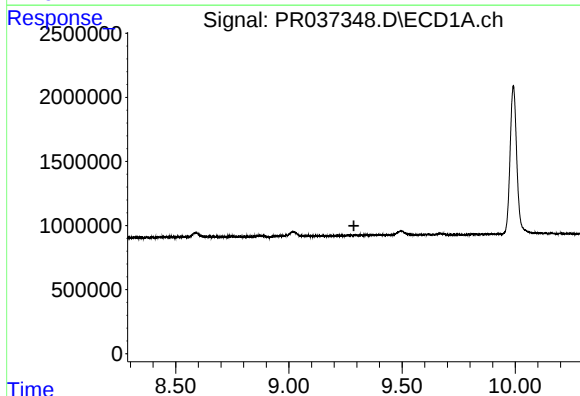


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.287 min
Response: 0
Conc: N.D.

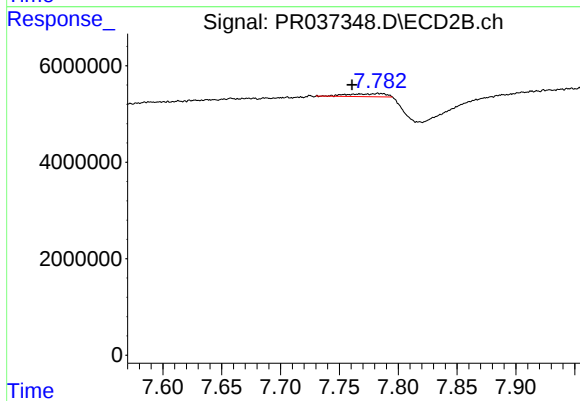

#40 AR-1262-5


R.T.: 7.784 min
Delta R.T.: 0.023 min
Response: 1354336
Conc: 3.54 ng/ml

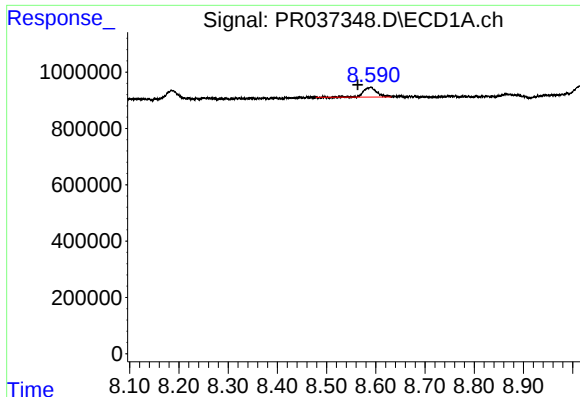

#41 AR-1268-1


R.T.: 8.589 min
Delta R.T.: 0.025 min
Response: 628872
Conc: 3.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

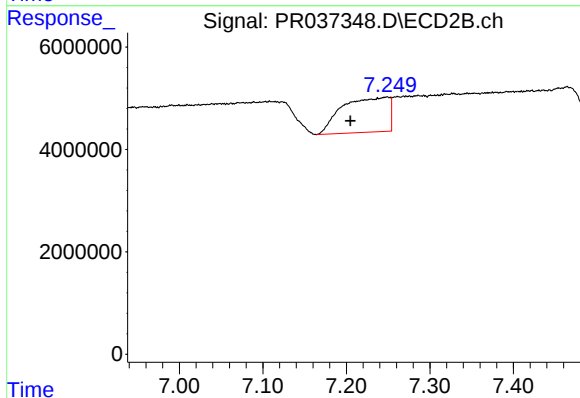


#41 AR-1268-1

R.T.: 7.249 min
Delta R.T.: 0.044 min
Response: 26627052
Conc: 21.63 ng/ml

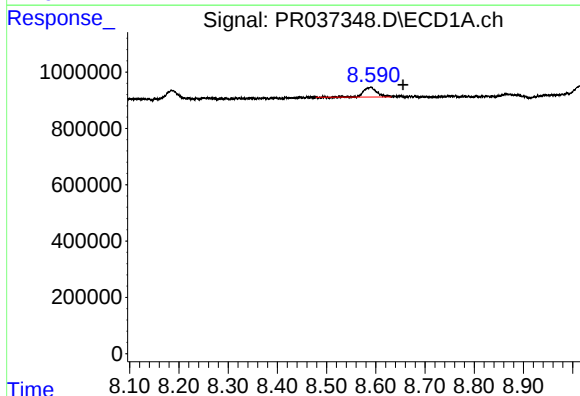


#42 AR-1268-2

R.T.: 8.589 min
Delta R.T.: -0.066 min
Response: 628872
Conc: 3.82 ng/ml

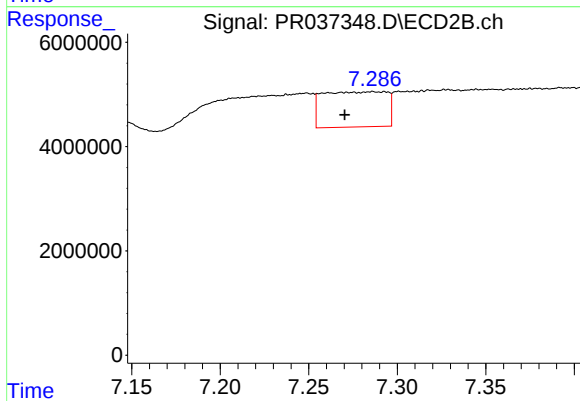

#42 AR-1268-2


R.T.: 7.286 min
Delta R.T.: 0.016 min
Response: 16931700
Conc: 15.99 ng/ml

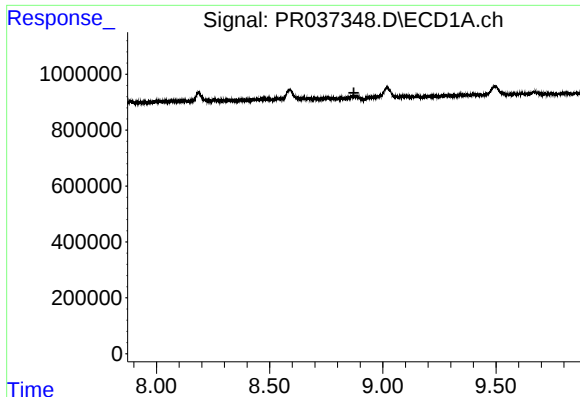

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

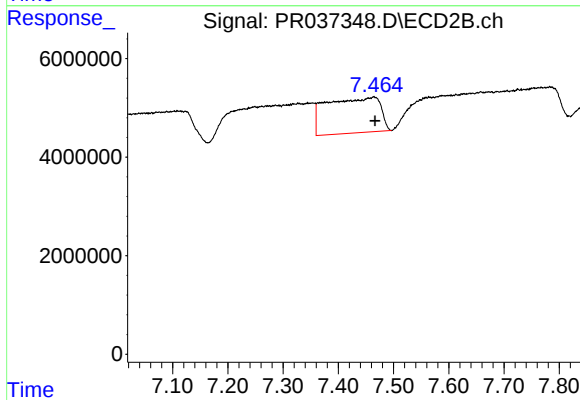


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 48656077
Conc: 54.90 ng/ml

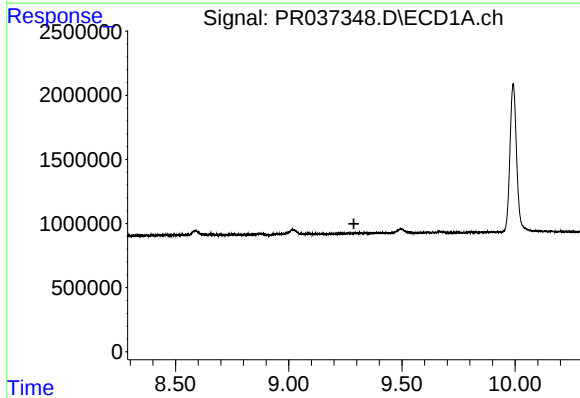


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

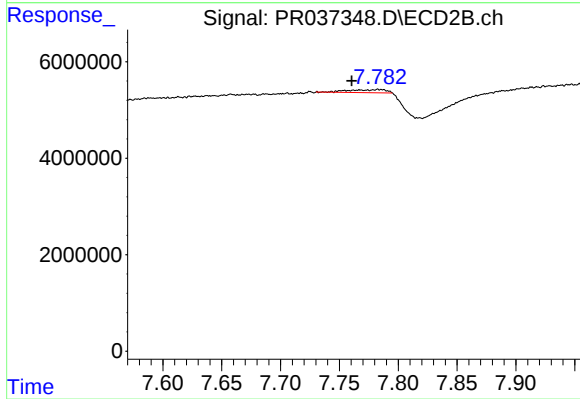

#44 AR-1268-4


R.T.: 7.784 min
Delta R.T.: 0.023 min
Response: 1354336
Conc: 3.73 ng/ml

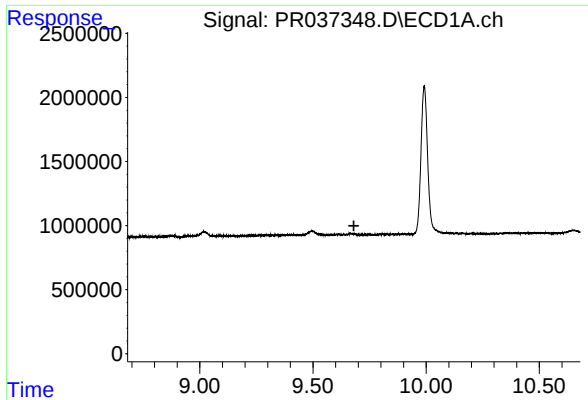

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

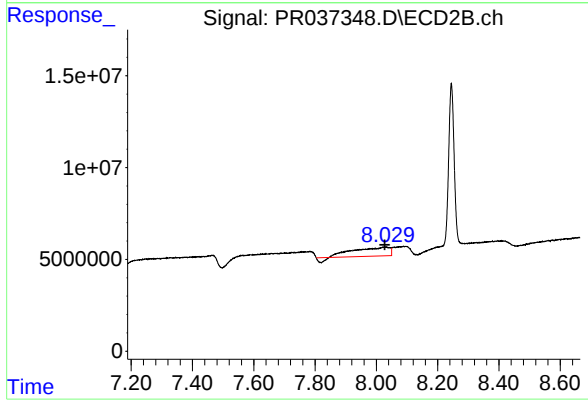

#45 AR-1268-5

R.T.: 8.030 min
Delta R.T.: 0.003 min
Response: 38511871
Conc: 15.14 ng/ml