

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 13:58
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1232 LOD 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.411	24567246	98787342	19.638	20.600
2)	SA Decachlor...	9.985	8.243	28860743	138.9E6	21.821	23.855
Target Compounds							
3)	L1 AR-1016-1	5.521	4.452	516294	2348118	11.982	12.896
4)	L1 AR-1016-2	5.542	4.467	899006	3141372	12.983	11.135
5)	L1 AR-1016-3	5.603	4.640	629649	1158600	15.613	8.058 #
6)	L1 AR-1016-4	0.000	4.681	0	995364	N.D.	8.997 #
7)	L1 AR-1016-5	5.991	4.886	202229	2086058	5.898	13.723 #
8)	L2 AR-1221-1	0.000	3.615	0	1443119	N.D.	28.342 #
9)	L2 AR-1221-2	4.661	3.700	684943	2380467	75.735	64.102
10)	L2 AR-1221-3	4.733	3.771	887606	3297486	28.960	26.930
11)	L3 AR-1232-1	4.733	3.771	887606	3297486	30.344	28.186
12)	L3 AR-1232-2	5.254	4.467	418221	3141372	24.750	22.727
13)	L3 AR-1232-3	5.542	4.640	899006	1158600	26.594	16.504 #
14)	L3 AR-1232-4	0.000	4.718	0	1378557	N.D.	23.102 #
15)	L3 AR-1232-5	0.000	4.886	0	2086058	N.D.	30.568 #
16)	L4 AR-1242-1	5.521	4.452	516294	2348118	15.090	16.024
17)	L4 AR-1242-2	5.542	4.467	899006	3141372	16.207	13.768
18)	L4 AR-1242-3	5.603	4.640	629649	1158600	19.130	10.020 #
19)	L4 AR-1242-4	0.000	4.718	0	1378557	N.D.	12.543 #
20)	L4 AR-1242-5	6.430	5.226	499616	5435680	15.526	32.804 #
21)	L5 AR-1248-1	5.521	4.452	516294	2348118	22.538	23.326
22)	L5 AR-1248-2	0.000	4.681	0	995364	N.D.	7.293 #
23)	L5 AR-1248-3	5.991	4.718	202229	1378557	4.943	9.849 #
24)	L5 AR-1248-4	6.393	4.886	456771	2086058	9.331	11.722 #
25)	L5 AR-1248-5	6.430	5.264	499616	6357553	10.577	32.501 #
26)	L6 AR-1254-1	6.362	5.226	341749	5435680	6.256	15.780 #
27)	L6 AR-1254-2	0.000	5.379	0	2919847	N.D.	9.749 #
28)	L6 AR-1254-3	0.000	5.763	0	7202844	N.D.	15.208 #
29)	L6 AR-1254-4	0.000	5.988	0	828387	N.D.	2.362 #
30)	L6 AR-1254-5	0.000	6.372	0	5394892	N.D.	12.183 #
31)	L7 AR-1260-1	0.000	5.899	0	456059	N.D.	1.560 #
32)	L7 AR-1260-2	0.000	6.069	0	3995059	N.D.	8.674 #
33)	L7 AR-1260-3	0.000	6.223	0	1129875	N.D.	3.169 #
34)	L7 AR-1260-4	0.000	6.733	0	4733102	N.D.	15.530 #
35)	L7 AR-1260-5	0.000	6.927	0	593548	N.D.	0.684 #
36)	L8 AR-1262-1	0.000	6.495	0	4861898	N.D.	19.399 #
37)	L8 AR-1262-2	0.000	6.927	0	593548	N.D.	0.473 #
38)	L8 AR-1262-3	0.000	7.268	0	24466991	N.D.	44.626 #
39)	L8 AR-1262-4	0.000	7.268	0	24466991	N.D.	27.257 #
40)	L8 AR-1262-5	0.000	7.766	0	1001572	N.D.	2.618 #
41)	L9 AR-1268-1	0.000	7.268	0	24466991	N.D.	19.875 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 13:58
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1232 LOD 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.268	0	24466991	N.D.	23.106 #
43) L9	AR-1268-3	0.000	7.463	0	15963309	N.D.	18.012 #
44) L9	AR-1268-4	0.000	7.766	0	1001572	N.D.	2.761 #
45) L9	AR-1268-5	0.000	8.023	0	13225453	N.D.	5.198 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 13:58
Operator : SM\SJ
Sample : K2241-07
Misc : AR1232 LOD 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:57:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

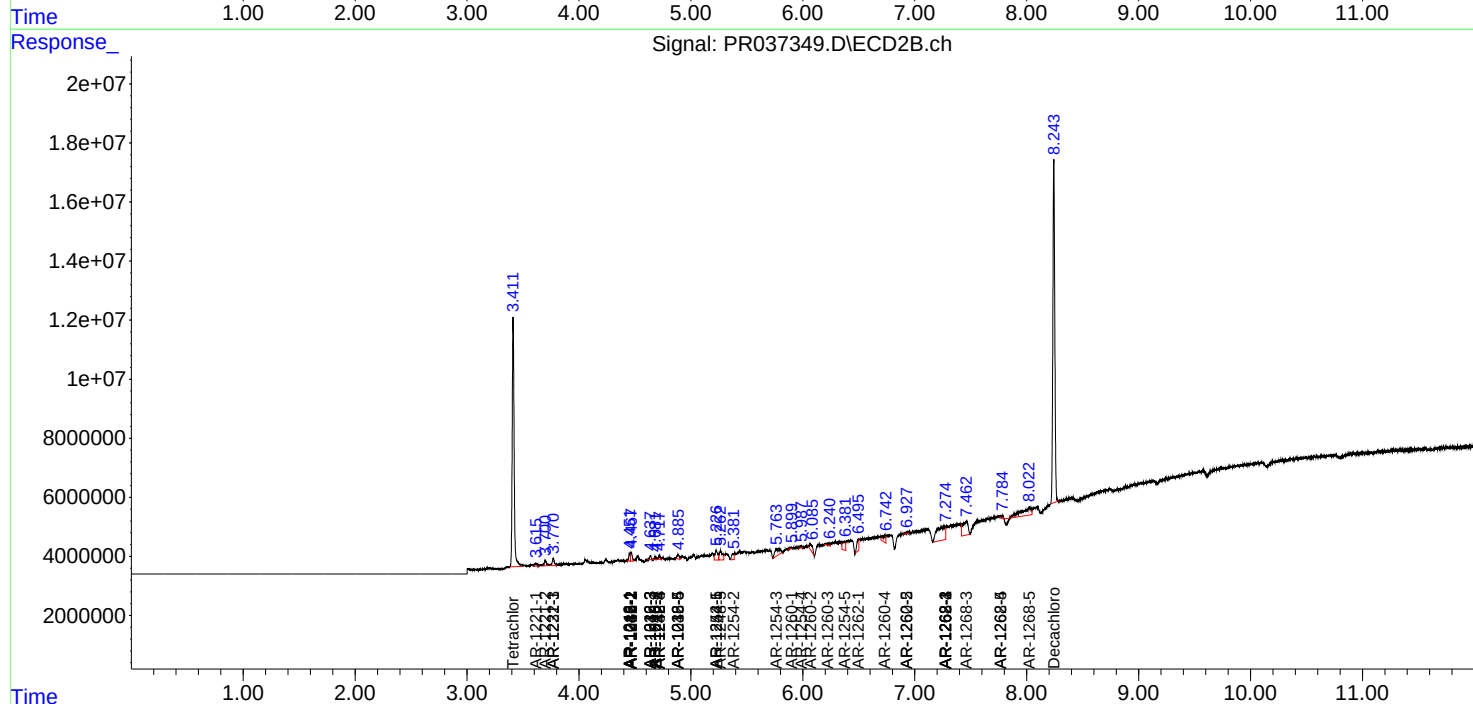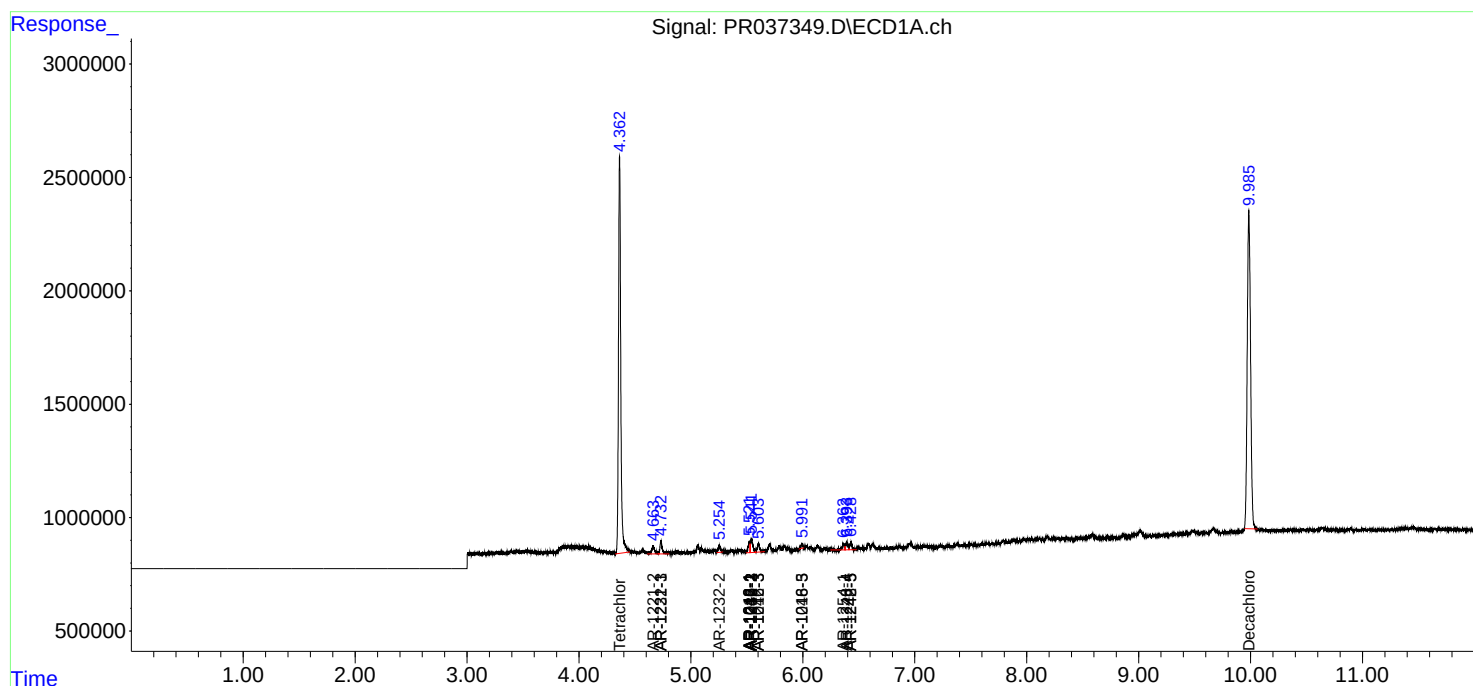


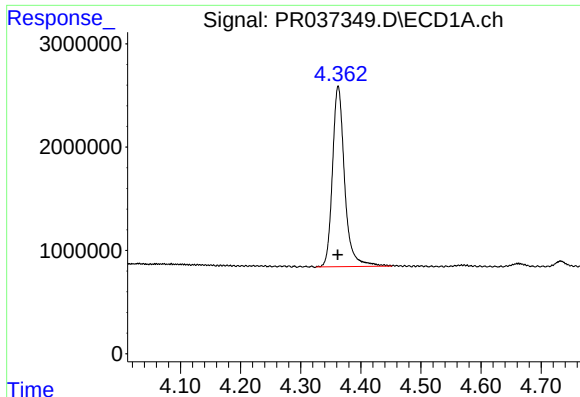

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 24567246
Conc: 19.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

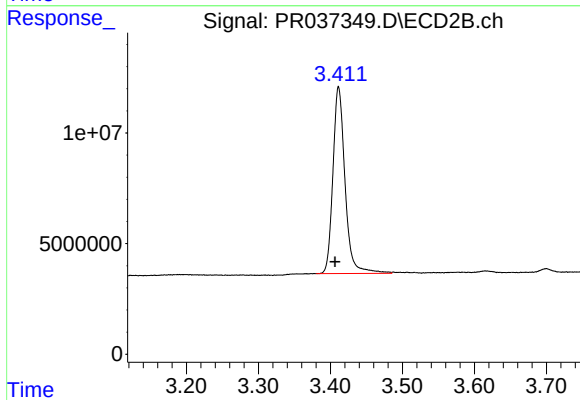


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.005 min
Response: 98787342
Conc: 20.60 ng/ml

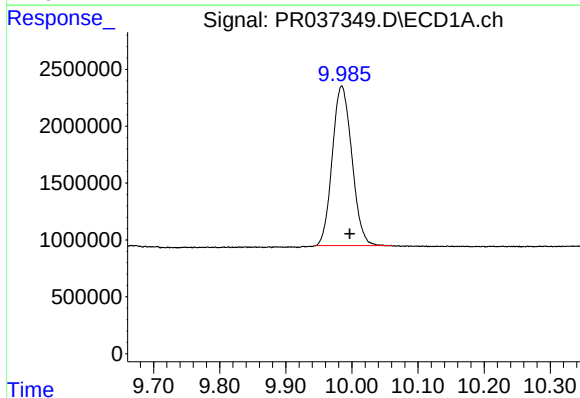


#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.012 min
Response: 28860743
Conc: 21.82 ng/ml

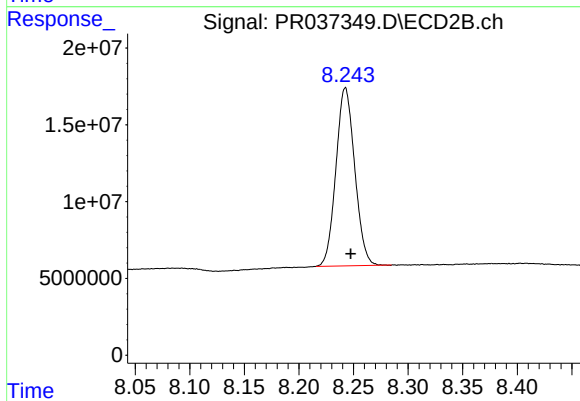

#2 Decachlorobiphenyl


R.T.: 8.243 min
Delta R.T.: -0.005 min
Response: 138938568
Conc: 23.86 ng/ml

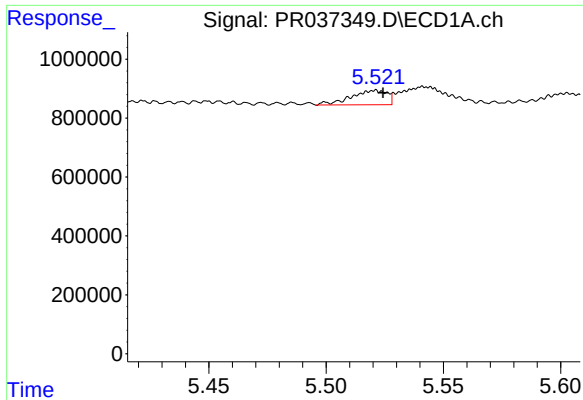

#3 AR-1016-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 516294
Conc: 11.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

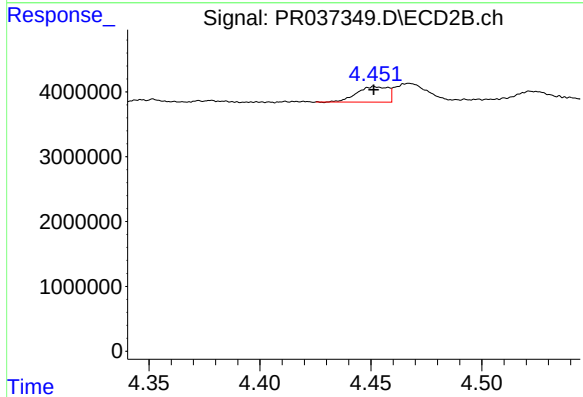


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2348118
Conc: 12.90 ng/ml

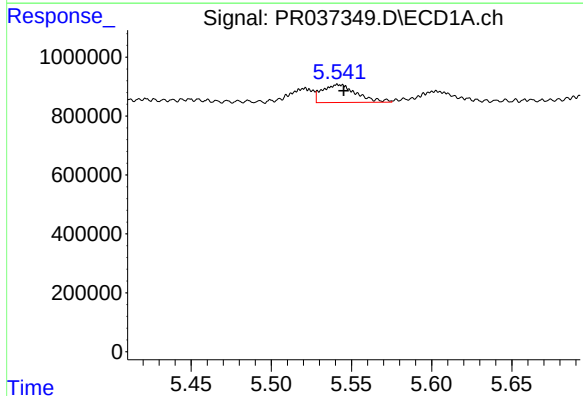


#4 AR-1016-2

R.T.: 5.542 min
Delta R.T.: -0.003 min
Response: 899006
Conc: 12.98 ng/ml

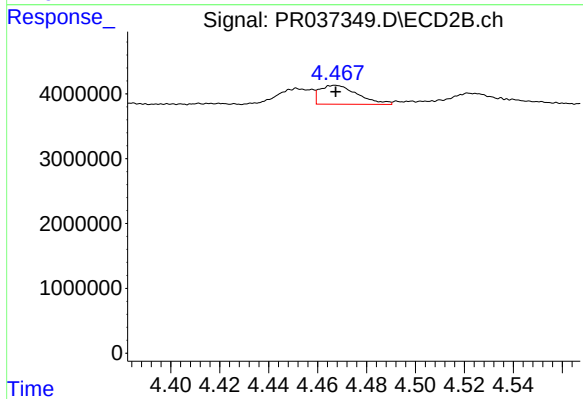

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3141372
Conc: 11.13 ng/ml

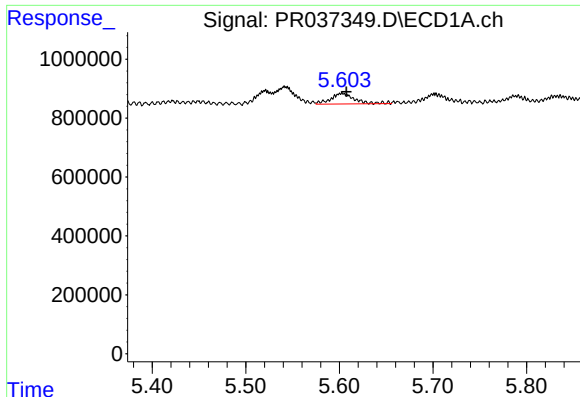

#5 AR-1016-3


R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 629649
Conc: 15.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

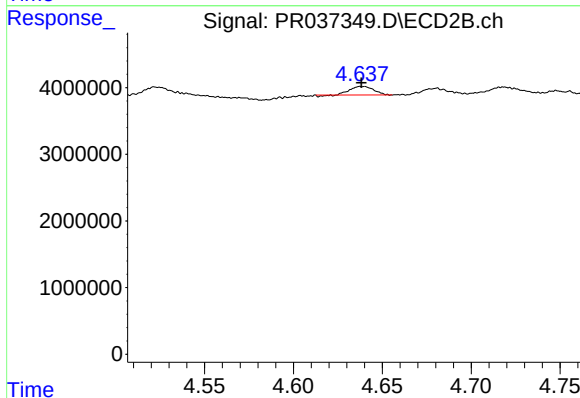


#5 AR-1016-3

R.T.: 4.640 min
Delta R.T.: 0.002 min
Response: 1158600
Conc: 8.06 ng/ml

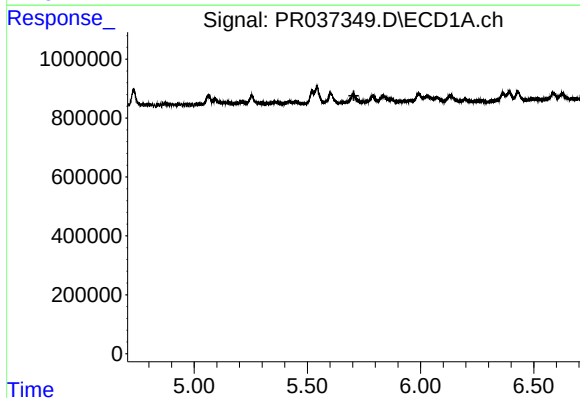


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

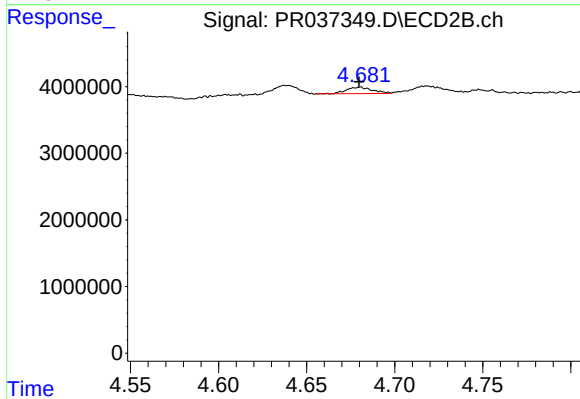

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.001 min
Response: 995364
Conc: 9.00 ng/ml

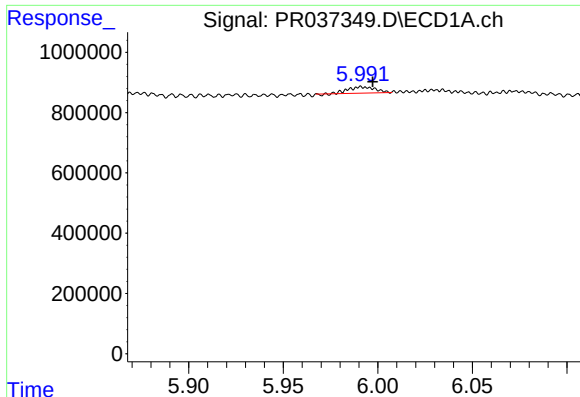

#7 AR-1016-5


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 202229
Conc: 5.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

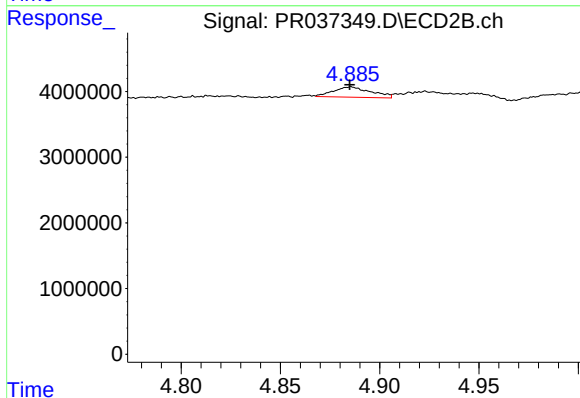


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 2086058
Conc: 13.72 ng/ml

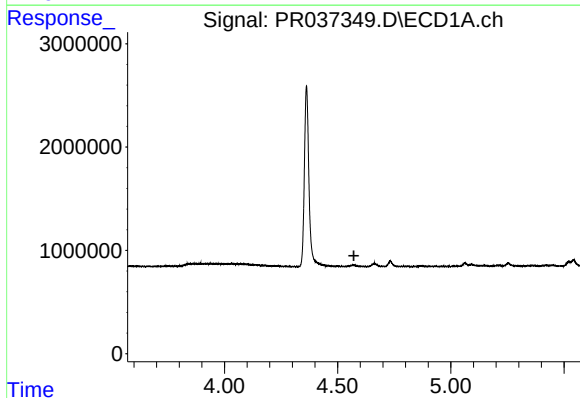


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

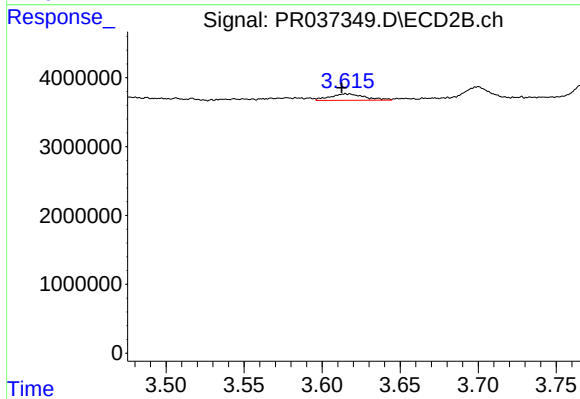

#8 AR-1221-1


R.T.: 3.615 min
Delta R.T.: 0.002 min
Response: 1443119
Conc: 28.34 ng/ml

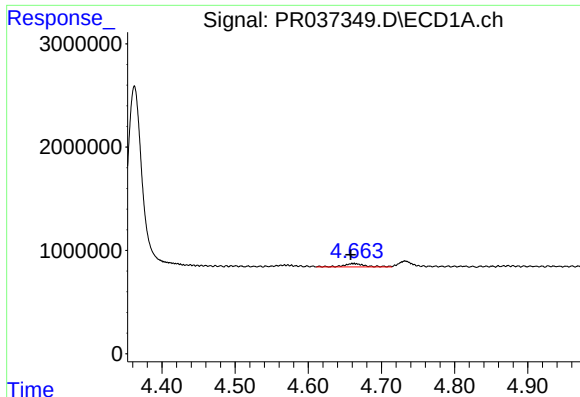

#9 AR-1221-2


R.T.: 4.661 min
Delta R.T.: 0.003 min
Response: 684943
Conc: 75.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

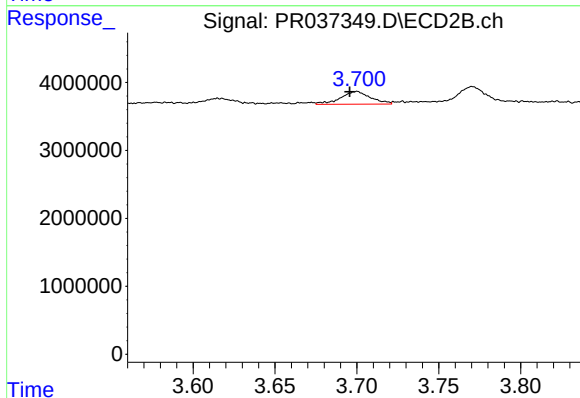


#9 AR-1221-2

R.T.: 3.700 min
Delta R.T.: 0.005 min
Response: 2380467
Conc: 64.10 ng/ml

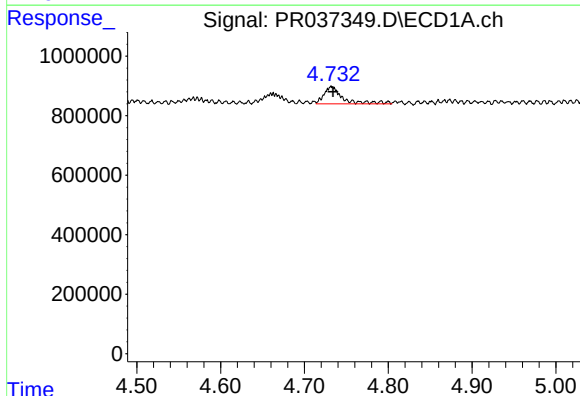


#10 AR-1221-3

R.T.: 4.733 min
Delta R.T.: -0.001 min
Response: 887606
Conc: 28.96 ng/ml

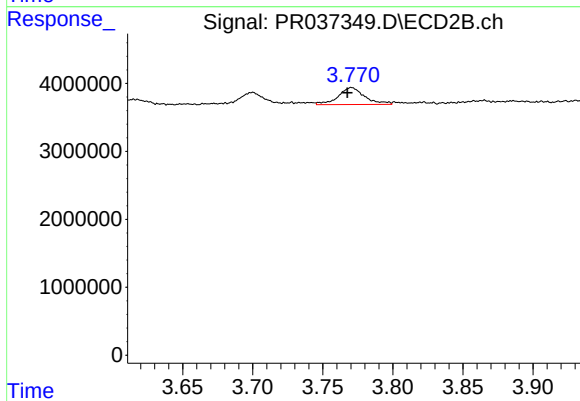

#10 AR-1221-3


R.T.: 3.771 min
Delta R.T.: 0.003 min
Response: 3297486
Conc: 26.93 ng/ml

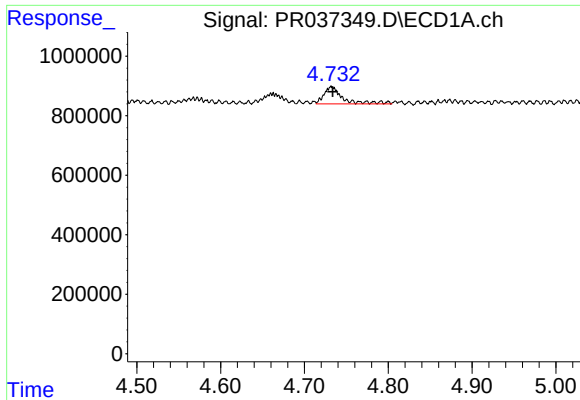

#11 AR-1232-1


R.T.: 4.733 min
Delta R.T.: -0.001 min
Response: 887606
Conc: 30.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

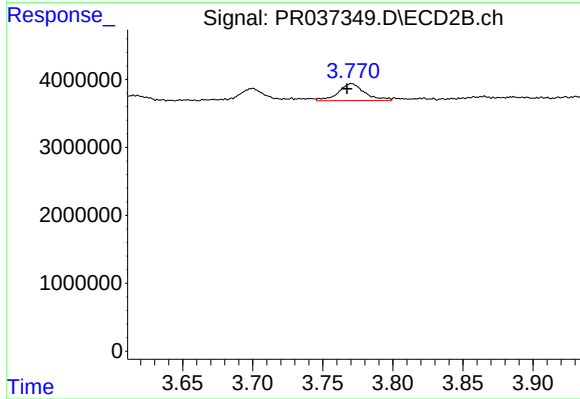


#11 AR-1232-1

R.T.: 3.771 min
Delta R.T.: 0.003 min
Response: 3297486
Conc: 28.19 ng/ml

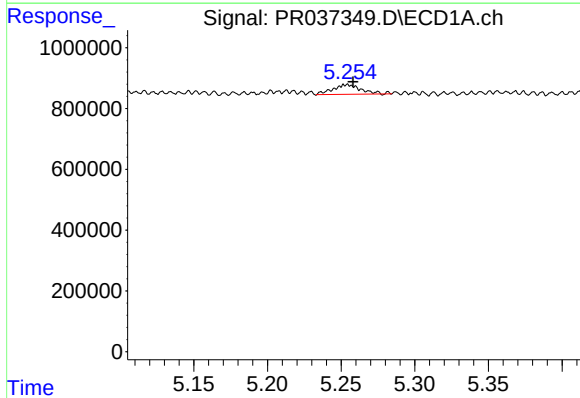


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 418221
Conc: 24.75 ng/ml

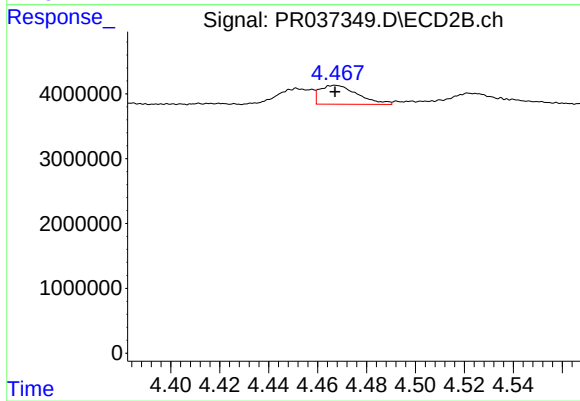

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3141372
Conc: 22.73 ng/ml

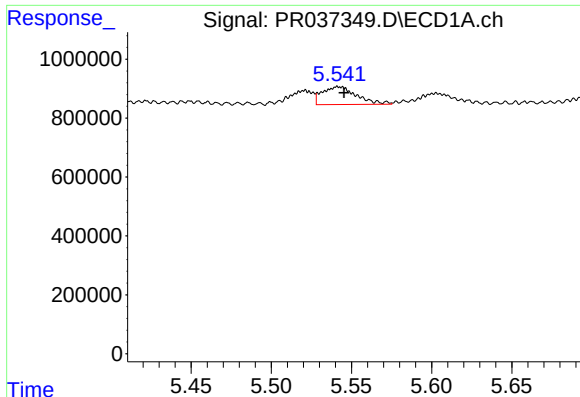

#13 AR-1232-3


R.T.: 5.542 min
Delta R.T.: -0.003 min
Response: 899006
Conc: 26.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

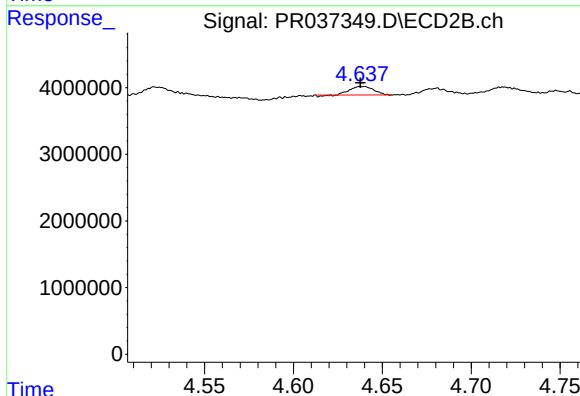


#13 AR-1232-3

R.T.: 4.640 min
Delta R.T.: 0.003 min
Response: 1158600
Conc: 16.50 ng/ml

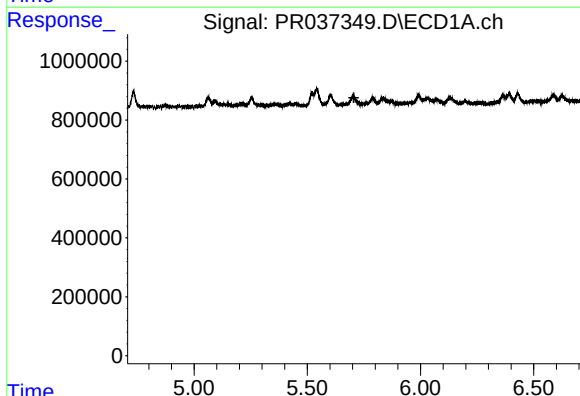


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.706 min
Response: 0
Conc: N.D.

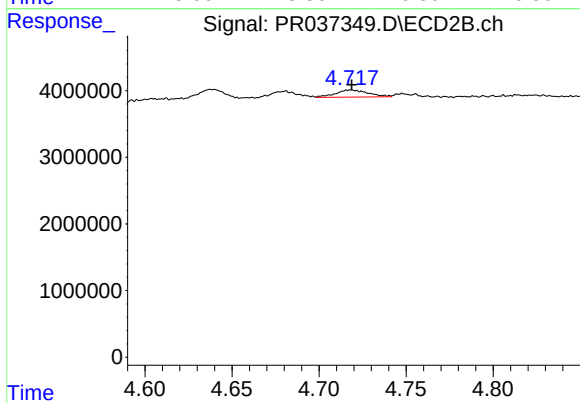

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 1378557
Conc: 23.10 ng/ml

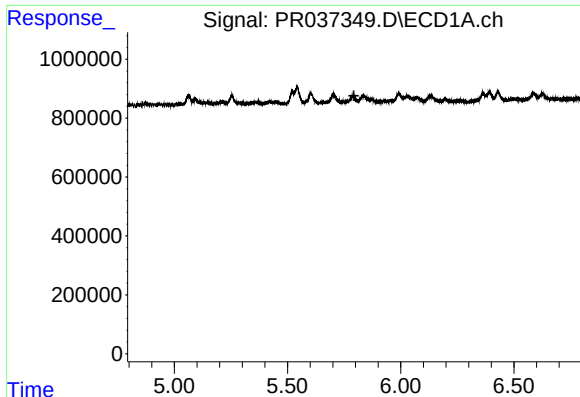

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

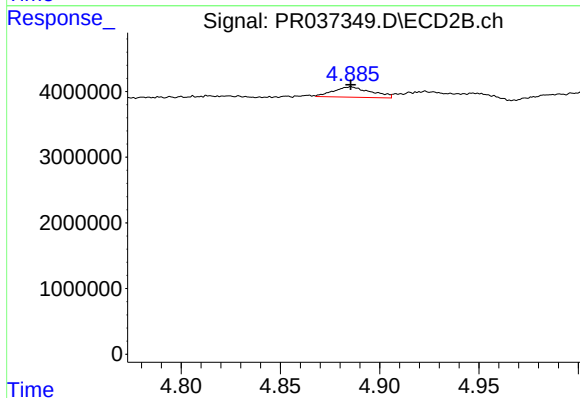


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 2086058
Conc: 30.57 ng/ml

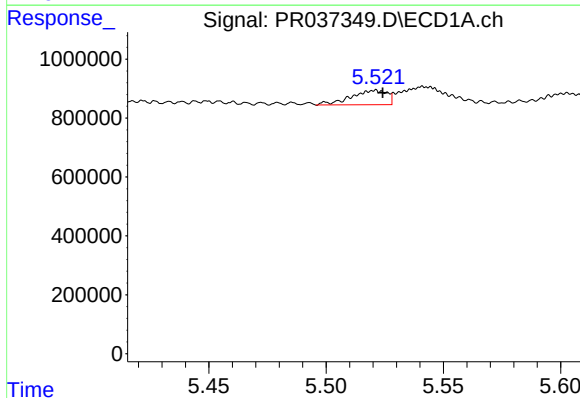


#16 AR-1242-1

R.T.: 5.521 min
Delta R.T.: -0.003 min
Response: 516294
Conc: 15.09 ng/ml

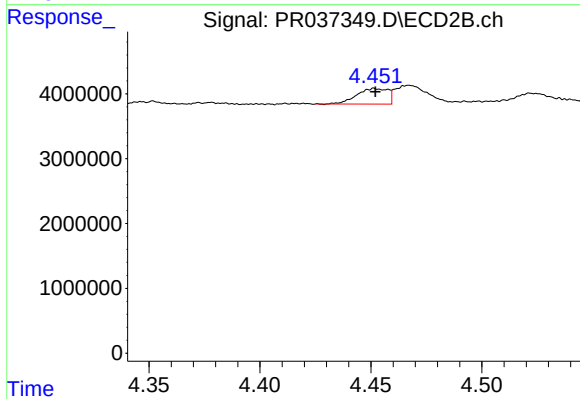

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2348118
Conc: 16.02 ng/ml

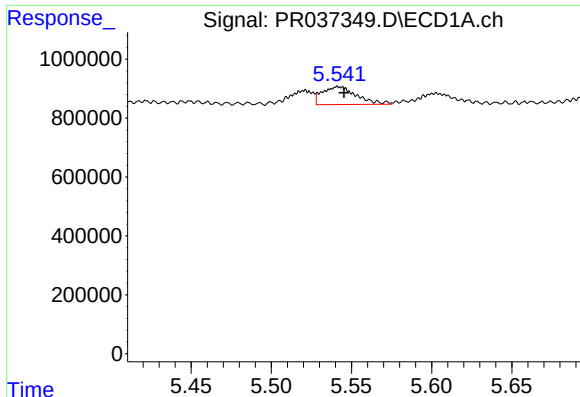

#17 AR-1242-2


R.T.: 5.542 min
Delta R.T.: -0.003 min
Response: 899006
Conc: 16.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

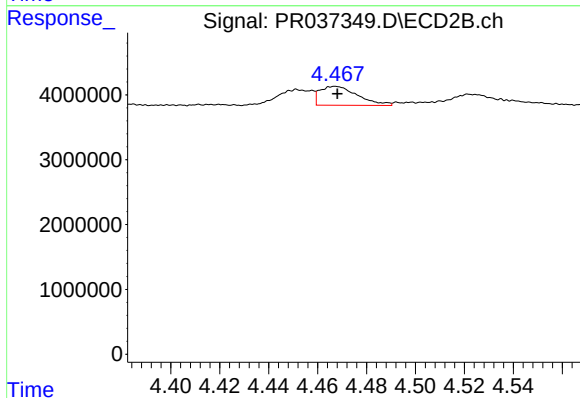


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3141372
Conc: 13.77 ng/ml

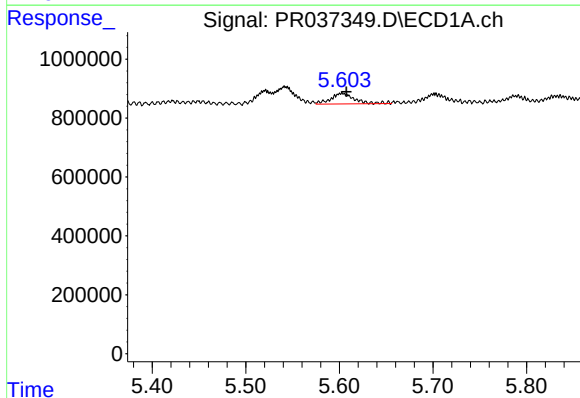


#18 AR-1242-3

R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 629649
Conc: 19.13 ng/ml

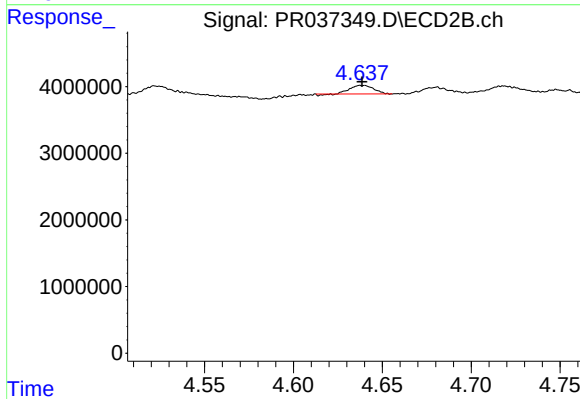

#18 AR-1242-3


R.T.: 4.640 min
Delta R.T.: 0.002 min
Response: 1158600
Conc: 10.02 ng/ml

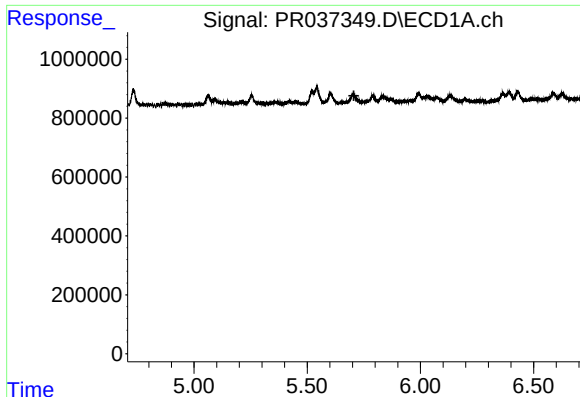

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

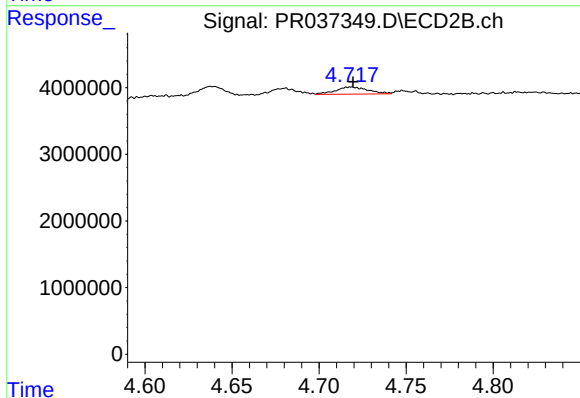


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 1378557
Conc: 12.54 ng/ml

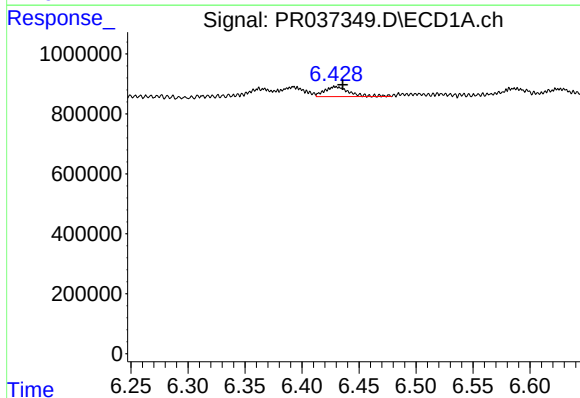


#20 AR-1242-5

R.T.: 6.430 min
Delta R.T.: -0.006 min
Response: 499616
Conc: 15.53 ng/ml

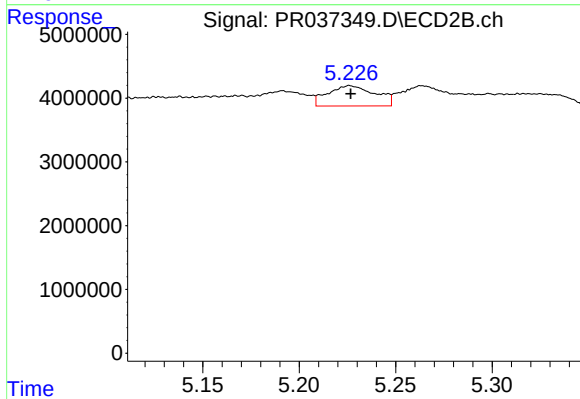

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 5435680
Conc: 32.80 ng/ml

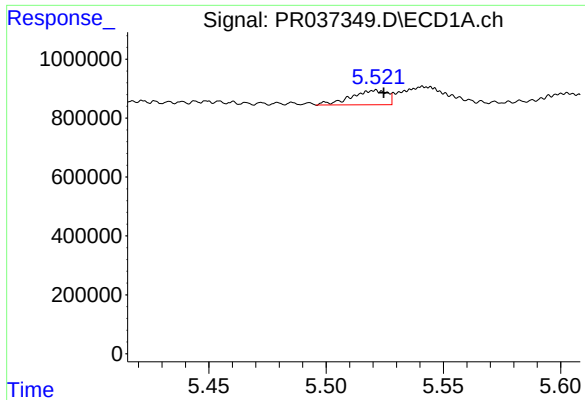

#21 AR-1248-1


R.T.: 5.521 min
Delta R.T.: -0.004 min
Response: 516294
Conc: 22.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

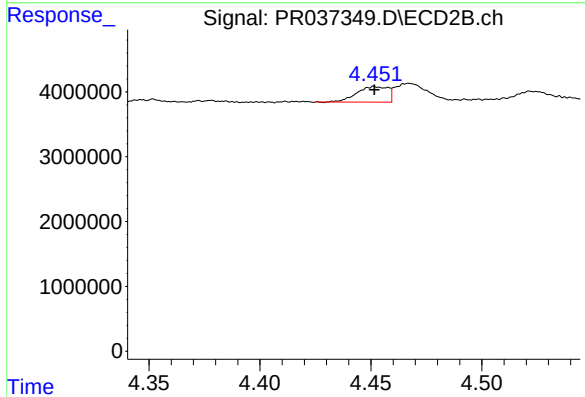


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 2348118
Conc: 23.33 ng/ml

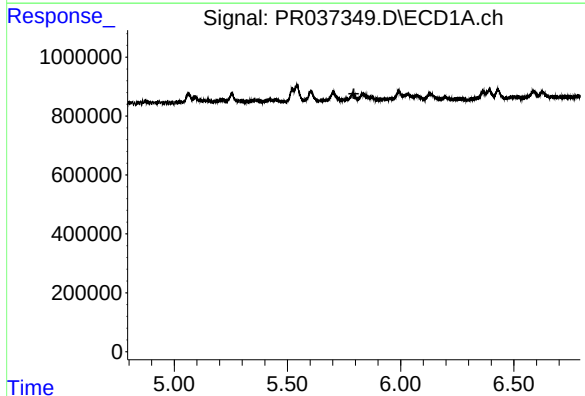


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

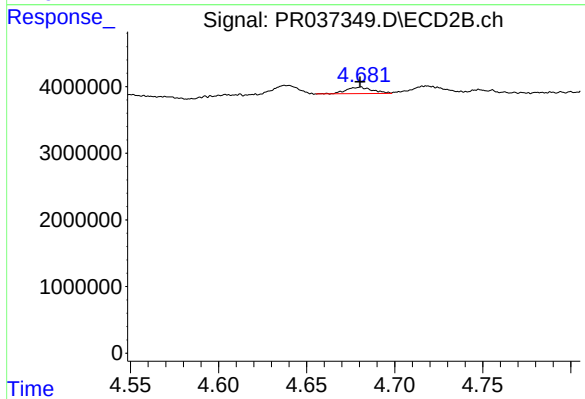

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 995364
Conc: 7.29 ng/ml

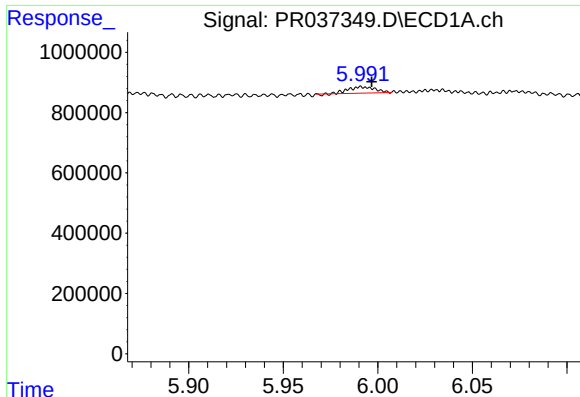

#23 AR-1248-3


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 202229
Conc: 4.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

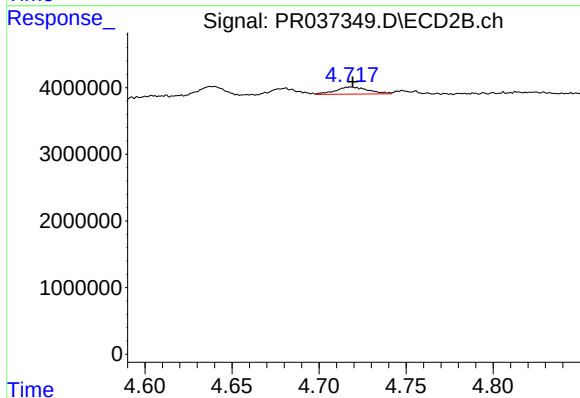


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 1378557
Conc: 9.85 ng/ml

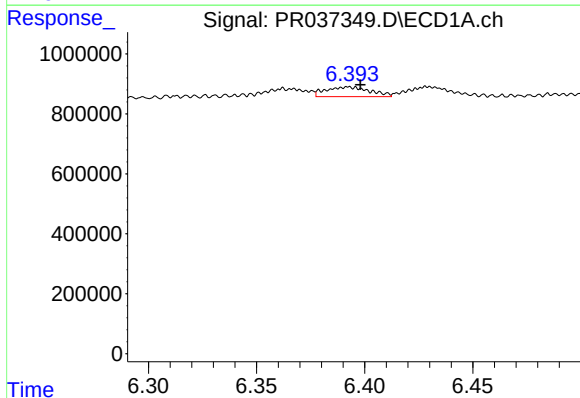


#24 AR-1248-4

R.T.: 6.393 min
Delta R.T.: -0.005 min
Response: 456771
Conc: 9.33 ng/ml

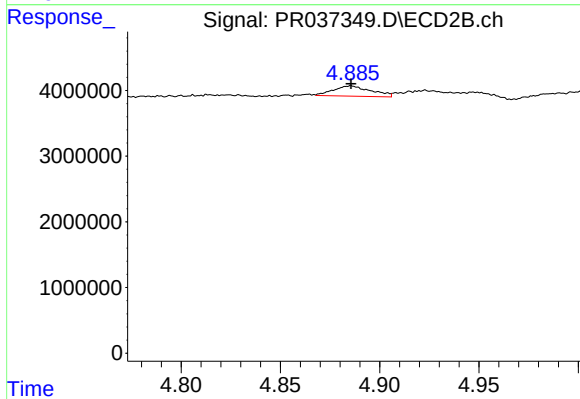

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 2086058
Conc: 11.72 ng/ml

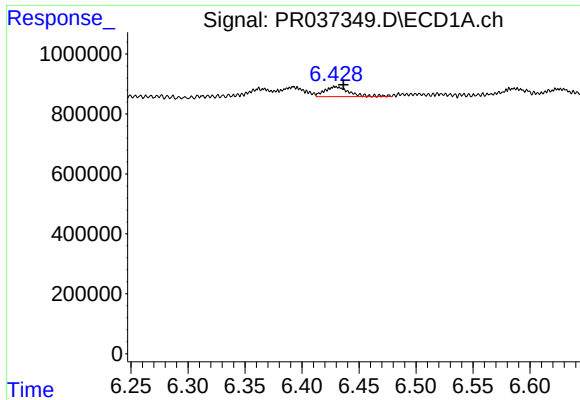

#25 AR-1248-5


R.T.: 6.430 min
Delta R.T.: -0.007 min
Response: 499616
Conc: 10.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

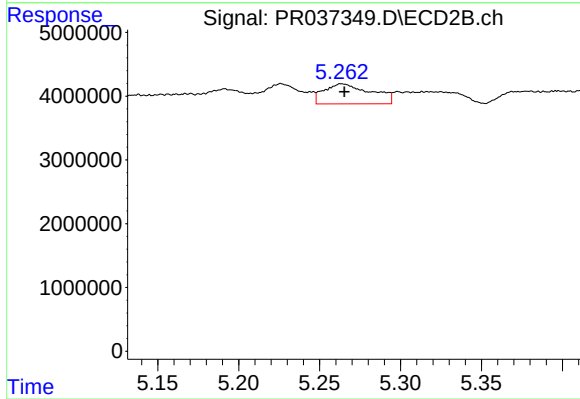


#25 AR-1248-5

R.T.: 5.264 min
Delta R.T.: -0.001 min
Response: 6357553
Conc: 32.50 ng/ml

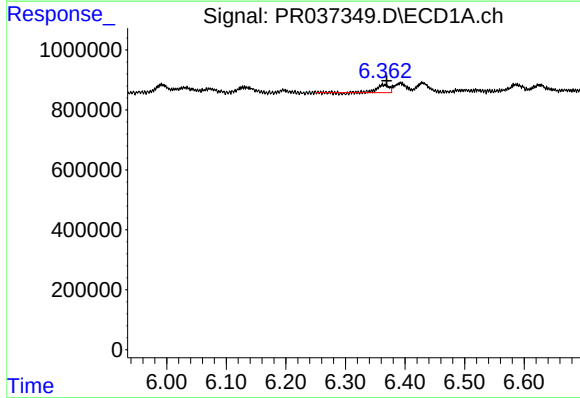


#26 AR-1254-1

R.T.: 6.362 min
Delta R.T.: -0.007 min
Response: 341749
Conc: 6.26 ng/ml

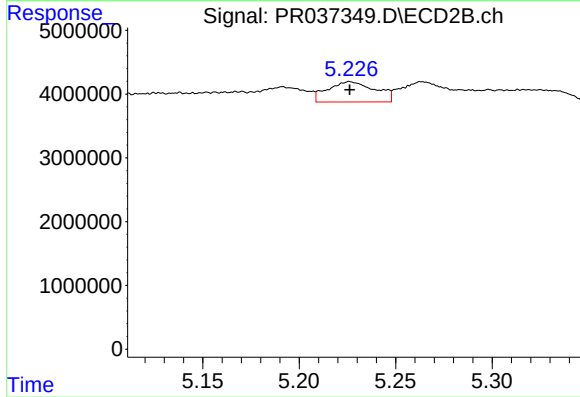

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 5435680
Conc: 15.78 ng/ml

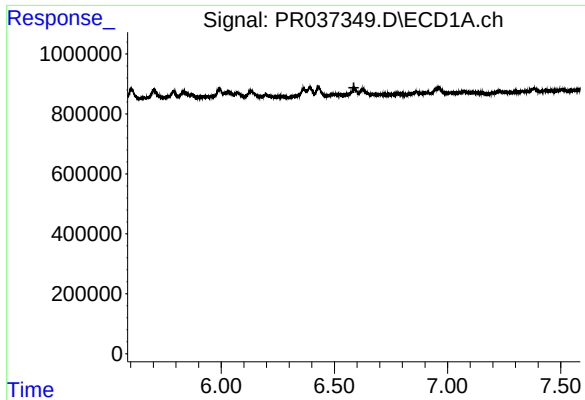

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

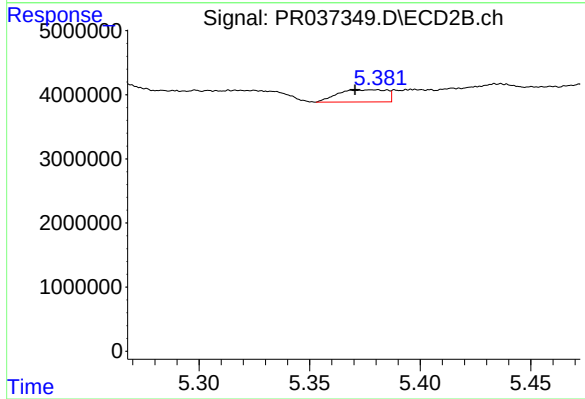


#27 AR-1254-2

R.T.: 5.379 min
Delta R.T.: 0.009 min
Response: 2919847
Conc: 9.75 ng/ml

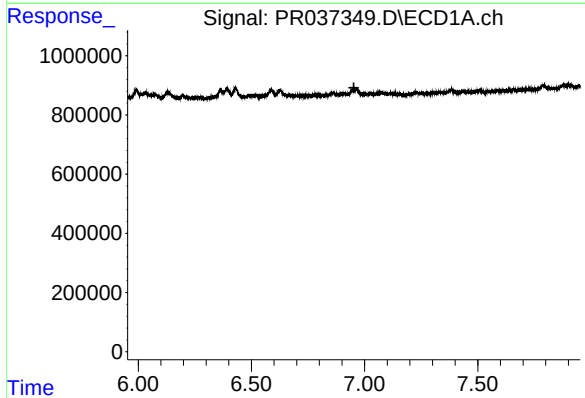


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.953 min
Response: 0
Conc: N.D.

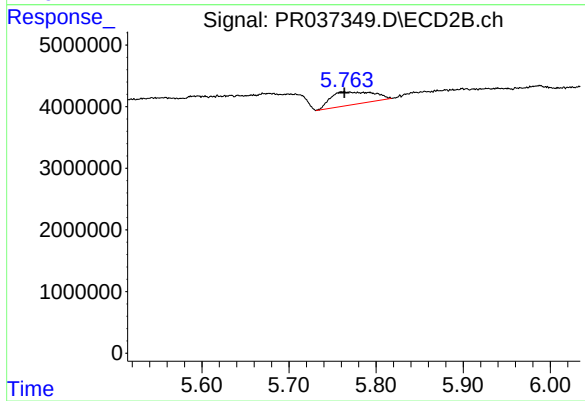

#28 AR-1254-3


R.T.: 5.763 min
Delta R.T.: 0.000 min
Response: 7202844
Conc: 15.21 ng/ml

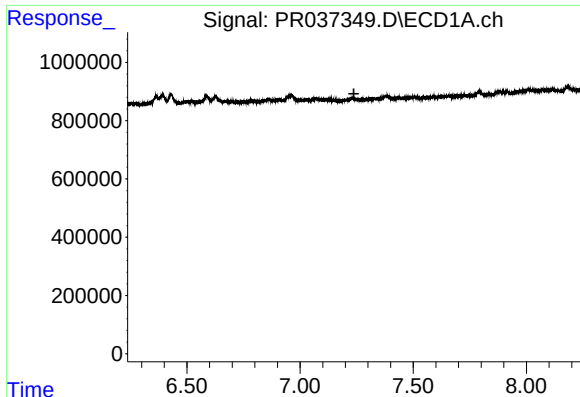

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

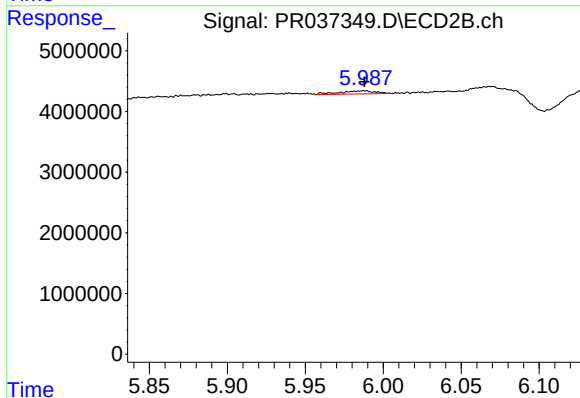


#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 828387
Conc: 2.36 ng/ml

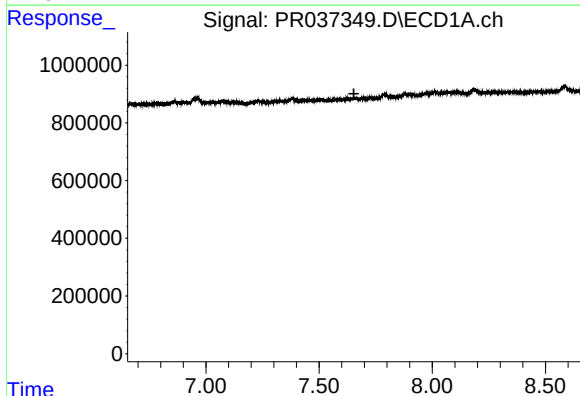


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

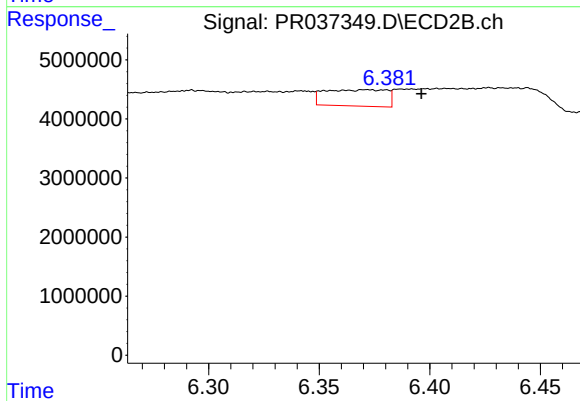

#30 AR-1254-5


R.T.: 6.372 min
Delta R.T.: -0.025 min
Response: 5394892
Conc: 12.18 ng/ml

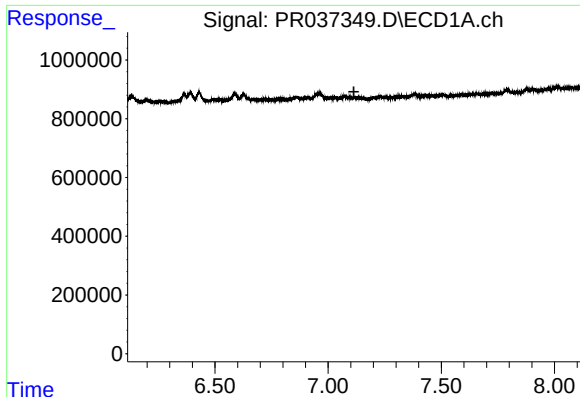

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

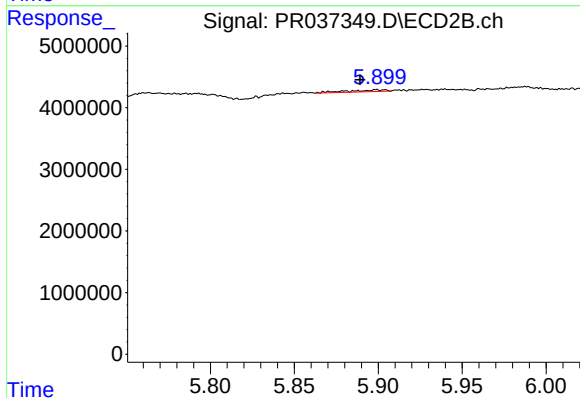


#31 AR-1260-1

R.T.: 5.899 min
Delta R.T.: 0.010 min
Response: 456059
Conc: 1.56 ng/ml

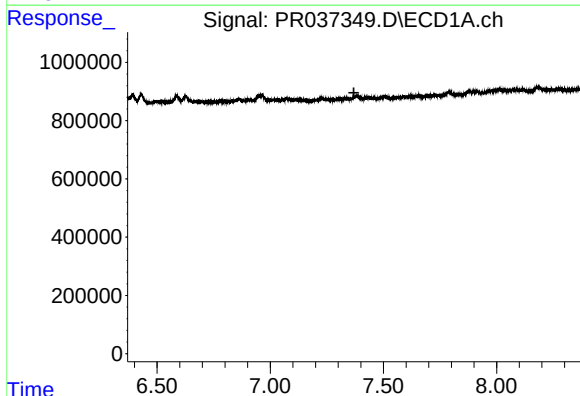


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

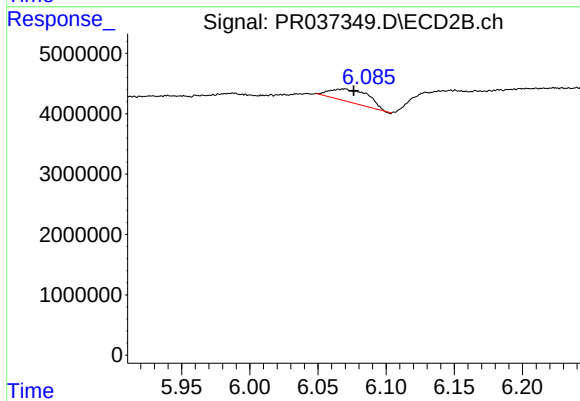

#32 AR-1260-2


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 3995059
Conc: 8.67 ng/ml

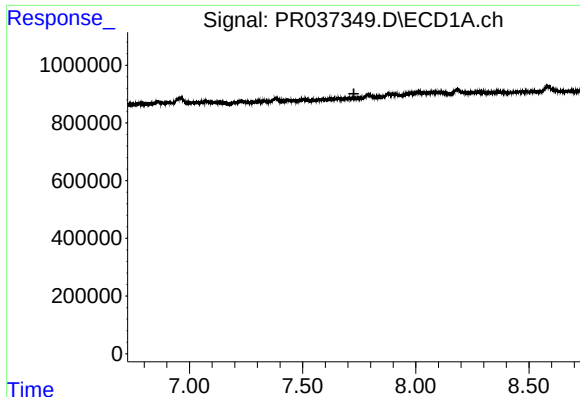

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

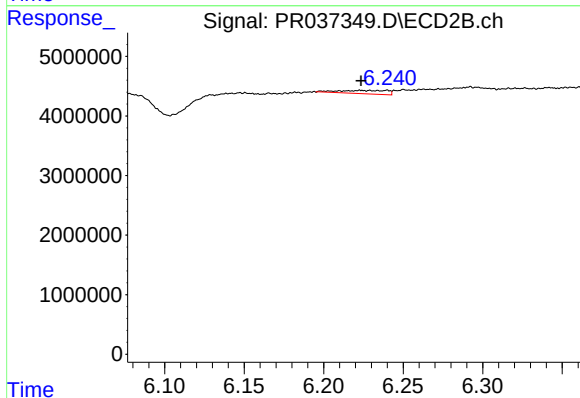


#33 AR-1260-3

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 1129875
Conc: 3.17 ng/ml

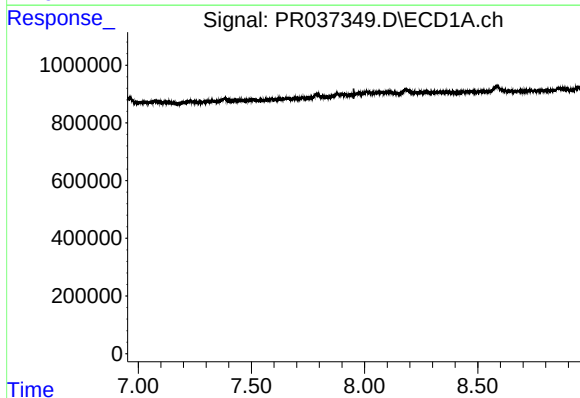


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

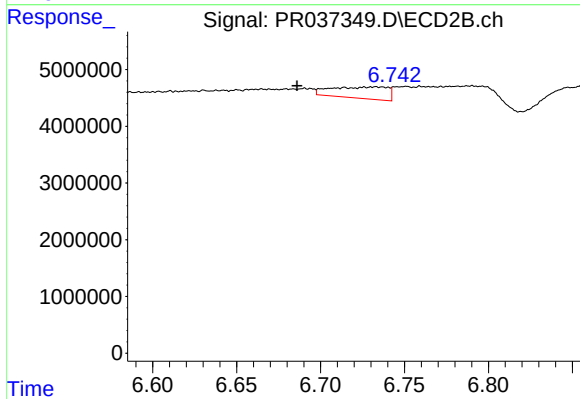

#34 AR-1260-4


R.T.: 6.733 min
Delta R.T.: 0.047 min
Response: 4733102
Conc: 15.53 ng/ml

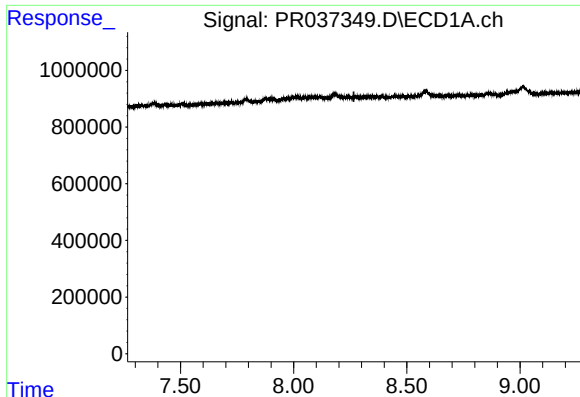

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

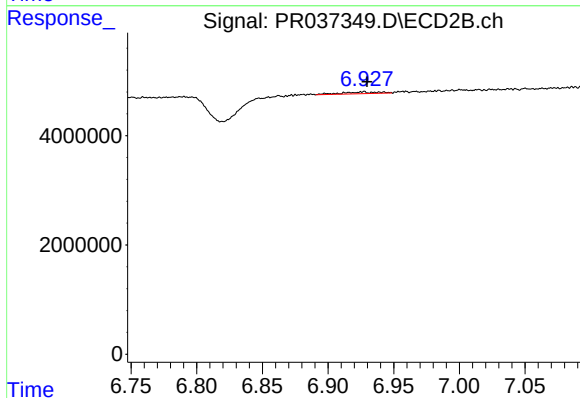


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.003 min
Response: 593548
Conc: 0.68 ng/ml

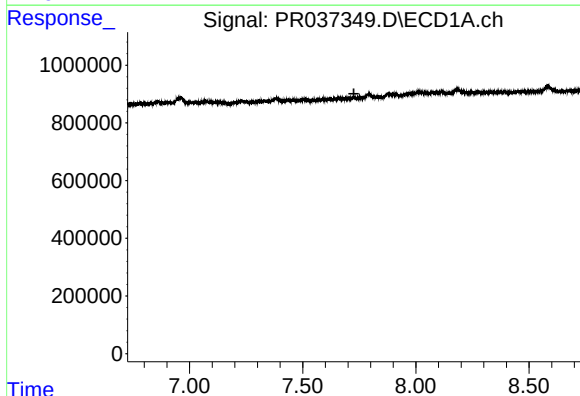


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

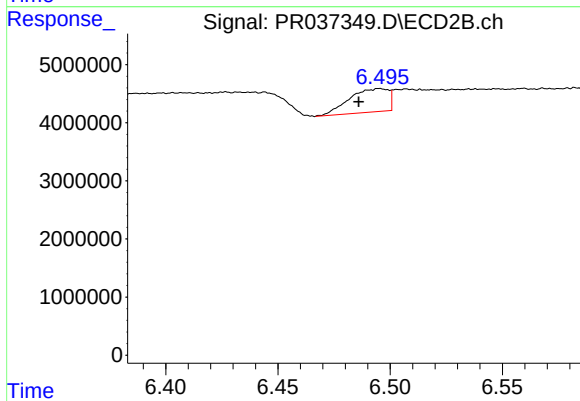

#36 AR-1262-1


R.T.: 6.495 min
Delta R.T.: 0.010 min
Response: 4861898
Conc: 19.40 ng/ml

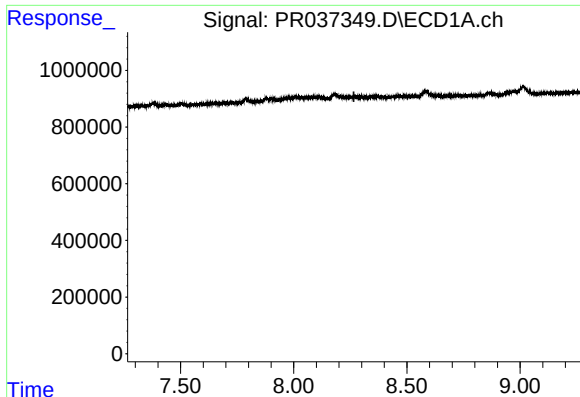

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

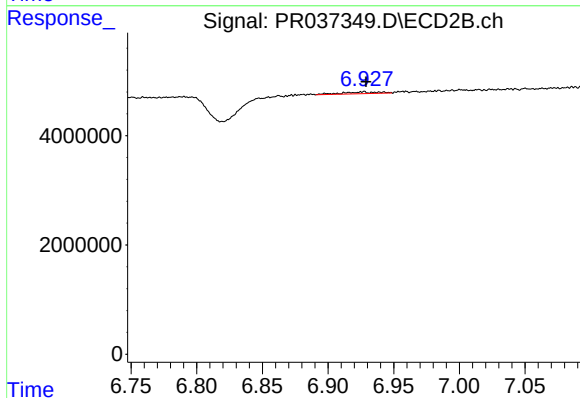


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 593548
Conc: 0.47 ng/ml

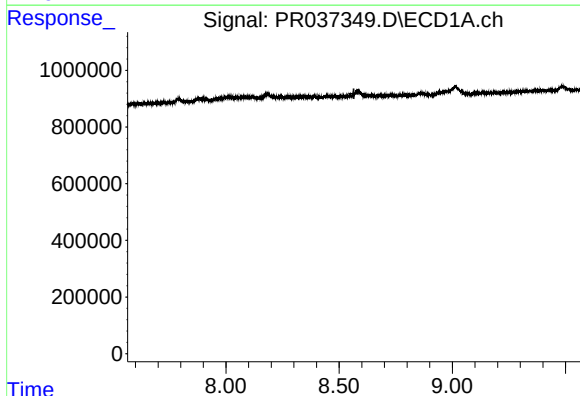


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

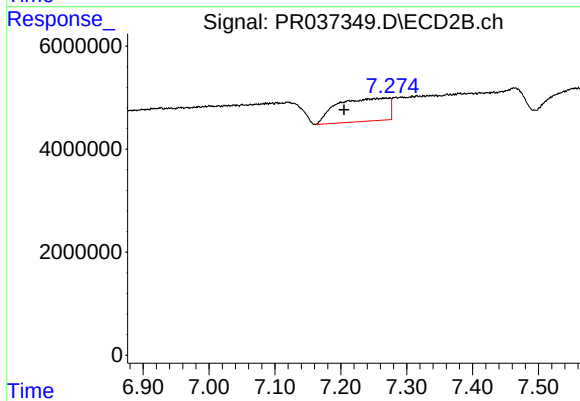

#38 AR-1262-3


R.T.: 7.268 min
Delta R.T.: 0.063 min
Response: 24466991
Conc: 44.63 ng/ml

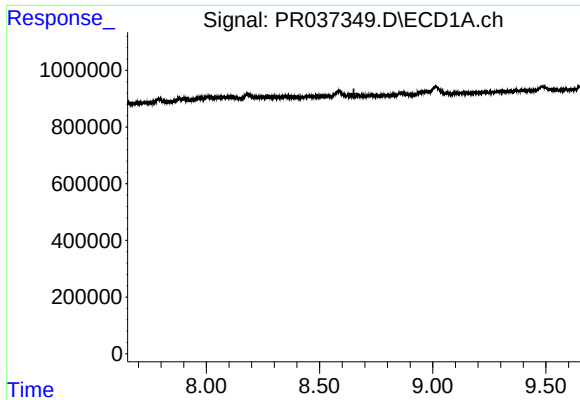

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

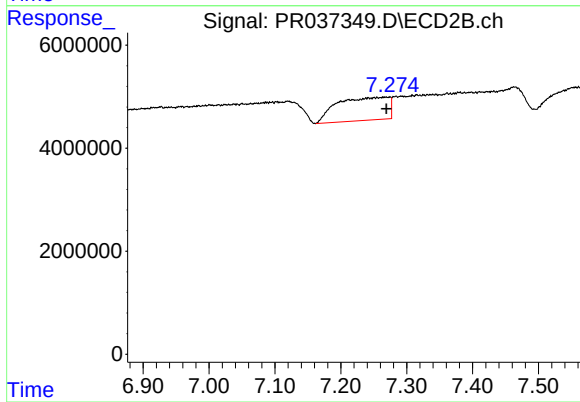


#39 AR-1262-4

R.T.: 7.268 min
Delta R.T.: 0.000 min
Response: 24466991
Conc: 27.26 ng/ml

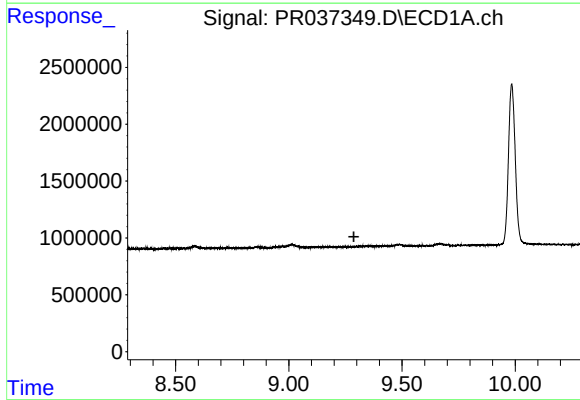


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

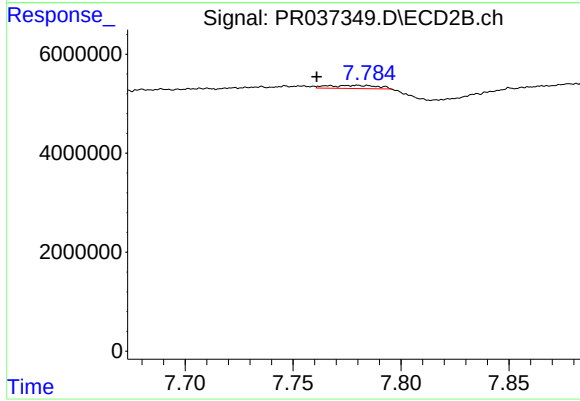

#40 AR-1262-5


R.T.: 7.766 min
Delta R.T.: 0.006 min
Response: 1001572
Conc: 2.62 ng/ml

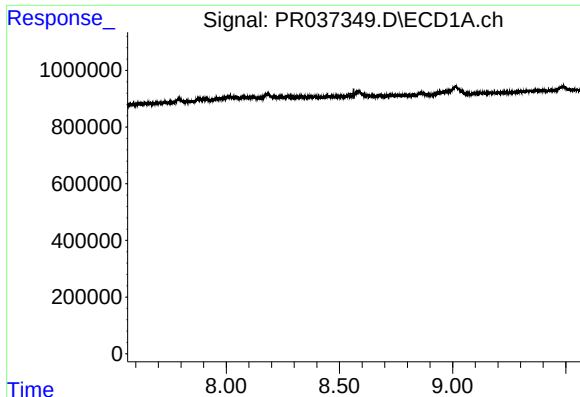

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

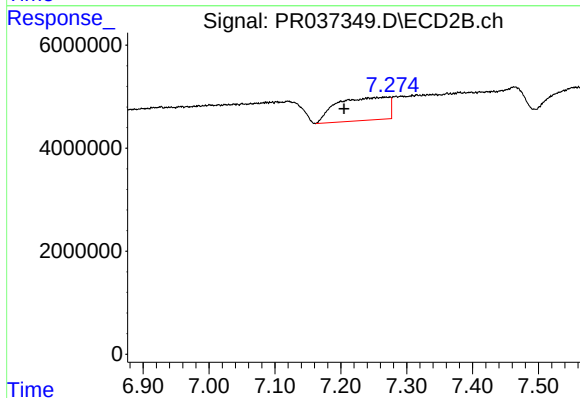


#41 AR-1268-1

R.T.: 7.268 min
Delta R.T.: 0.064 min
Response: 24466991
Conc: 19.88 ng/ml

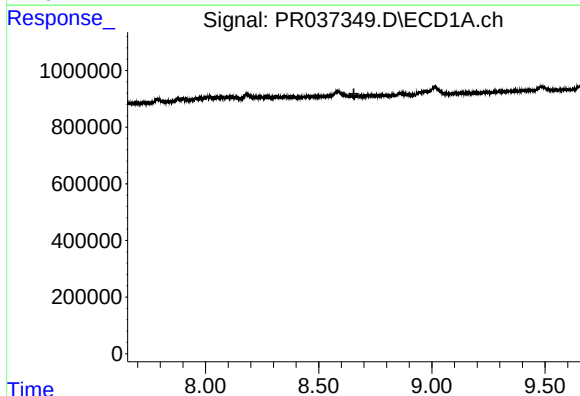


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

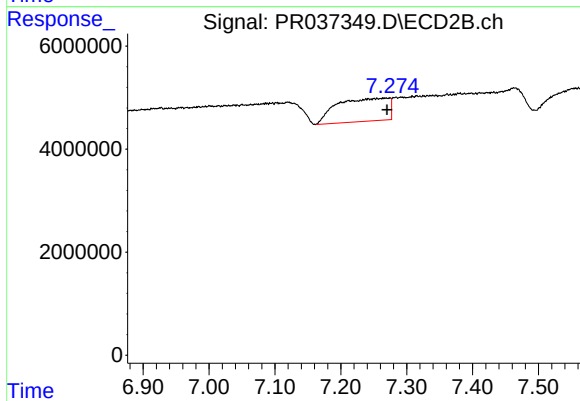

#42 AR-1268-2


R.T.: 7.268 min
Delta R.T.: -0.002 min
Response: 24466991
Conc: 23.11 ng/ml

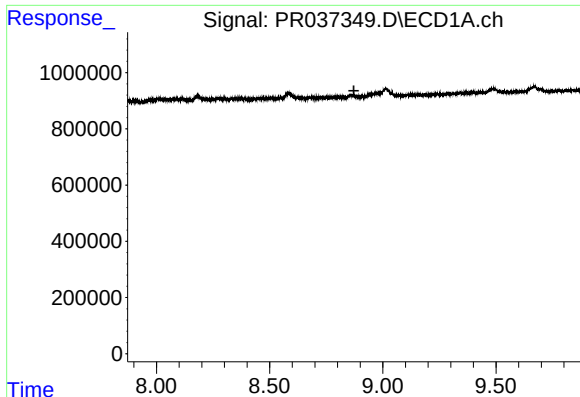

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

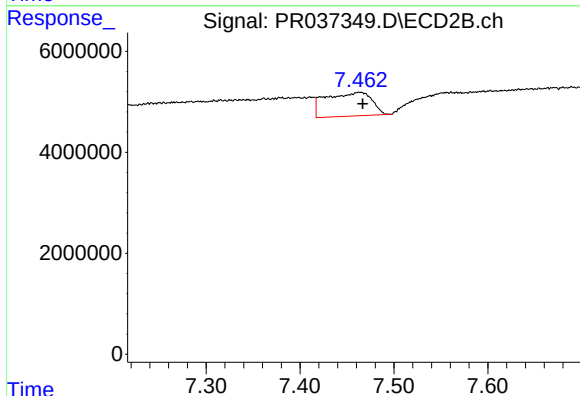


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.003 min
Response: 15963309
Conc: 18.01 ng/ml

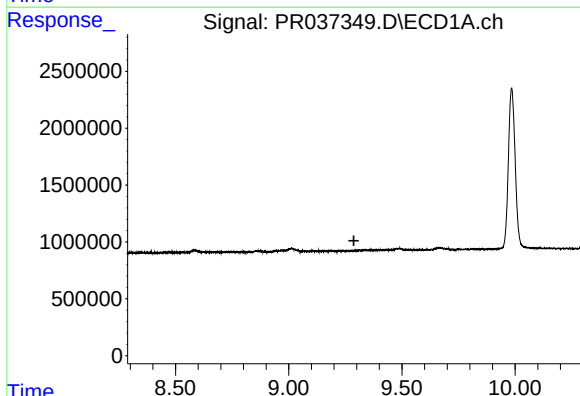


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

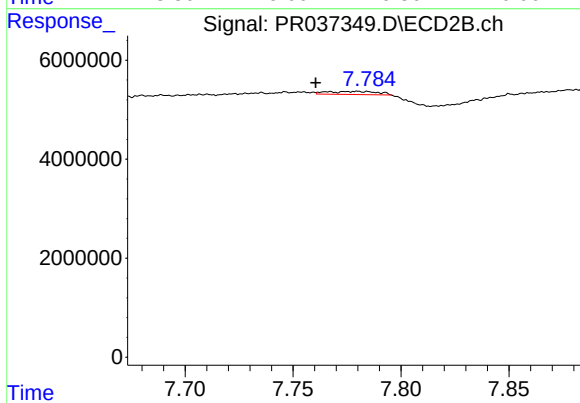

#44 AR-1268-4


R.T.: 7.766 min
Delta R.T.: 0.006 min
Response: 1001572
Conc: 2.76 ng/ml

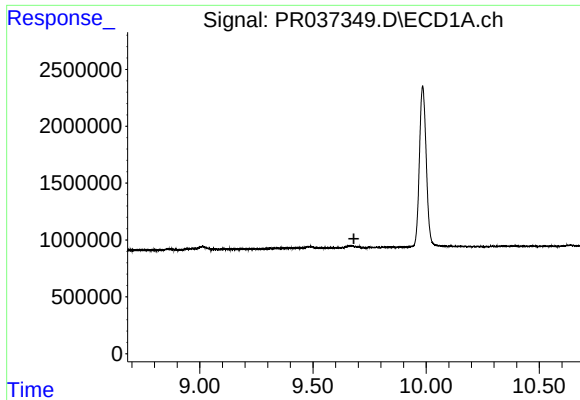

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

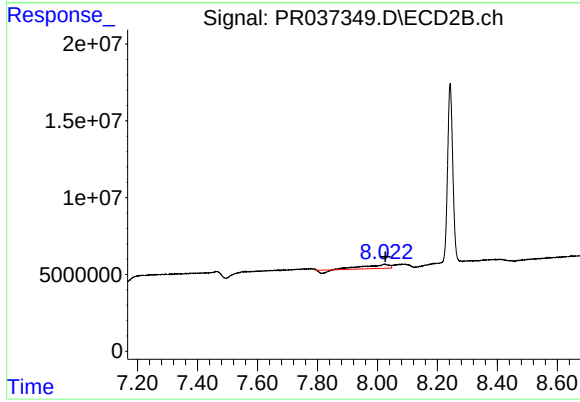

#45 AR-1268-5

R.T.: 8.023 min
Delta R.T.: -0.005 min
Response: 13225453
Conc: 5.20 ng/ml