

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 14:13
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1232 LOD 40PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.361	3.410	23410266	95683992	18.713	19.953
2)	SA Decachlor...	9.984	8.244	26888261	134.4E6	20.330	23.080
Target Compounds							
3)	L1 AR-1016-1	5.541	4.452	2035898	3519770	47.249	19.331 #
4)	L1 AR-1016-2	5.541	4.468	2035898	5836394	29.400	20.687 #
5)	L1 AR-1016-3	5.603	4.637	734276	2731601	18.207	18.998
6)	L1 AR-1016-4	5.701	4.680	603774	2054980	18.385	18.574
7)	L1 AR-1016-5	5.991	4.884	600686	2768695	17.518	18.214
8)	L2 AR-1221-1	0.000	3.613	0	2090177	N.D.	41.049 #
9)	L2 AR-1221-2	4.660	3.697	768264	2934854	84.948	79.030
10)	L2 AR-1221-3	4.732	3.769	1399080	5209726	45.648	42.546
11)	L3 AR-1232-1	4.732	3.769	1399080	5209726	47.830	44.531
12)	L3 AR-1232-2	5.254	4.468	699134	5836394	41.375	42.224
13)	L3 AR-1232-3	5.541	4.637	2035898	2731601	60.226	38.911 #
14)	L3 AR-1232-4	5.701	4.719	603774	2485737	38.465	41.657
15)	L3 AR-1232-5	5.789	4.884	485676	2768695	41.526	40.571
16)	L4 AR-1242-1	5.541	4.452	2035898	3519770	59.504	24.020 #
17)	L4 AR-1242-2	5.541	4.468	2035898	5836394	36.703	25.580 #
18)	L4 AR-1242-3	5.603	4.637	734276	2731601	22.308	23.624
19)	L4 AR-1242-4	5.701	4.719	603774	2485737	22.890	22.616
20)	L4 AR-1242-5	6.429	5.226	804987	4663742	25.016	28.146
21)	L5 AR-1248-1	5.541	4.452	2035898	3519770	88.875	34.966 #
22)	L5 AR-1248-2	5.789	4.680	485676	2054980	13.871	15.058
23)	L5 AR-1248-3	5.991	4.719	600686	2485737	14.683	17.759
24)	L5 AR-1248-4	6.392	4.884	744621	2768695	15.211	15.558
25)	L5 AR-1248-5	6.429	5.264	804987	5025195	17.041	25.690 #
26)	L6 AR-1254-1	6.364	5.226	615052	4663742	11.258	13.539
27)	L6 AR-1254-2	6.586	5.374	1023954	1645133	11.949	5.493 #
28)	L6 AR-1254-3	0.000	5.762	0	4518844	N.D.	9.541 #
29)	L6 AR-1254-4	0.000	5.988	0	1028756	N.D.	2.934 #
30)	L6 AR-1254-5	0.000	6.399	0	5776951	N.D.	13.046 #
31)	L7 AR-1260-1	0.000	5.885	0	366391	N.D.	1.254 #
32)	L7 AR-1260-2	0.000	6.069	0	2045442	N.D.	4.441 #
33)	L7 AR-1260-3	0.000	6.218	0	429275	N.D.	1.204 #
36)	L8 AR-1262-1	0.000	6.438	0	3284638	N.D.	13.106 #
38)	L8 AR-1262-3	0.000	7.274	0	11059791	N.D.	20.172 #
39)	L8 AR-1262-4	0.000	7.274	0	11059791	N.D.	12.321 #
40)	L8 AR-1262-5	0.000	7.780	0	660544	N.D.	1.726 #
41)	L9 AR-1268-1	0.000	7.274	0	11059791	N.D.	8.984 #
42)	L9 AR-1268-2	0.000	7.274	0	11059791	N.D.	10.444 #
43)	L9 AR-1268-3	0.000	7.464	0	6416200	N.D.	7.240 #
44)	L9 AR-1268-4	0.000	7.780	0	660544	N.D.	1.821 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 14:13
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1232 LOD 40PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.025	0	5855832	N.D.	2.302 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 14:13
Operator : SM\SJ
Sample : K2241-07
Misc : AR1232 LOD 40PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:57:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

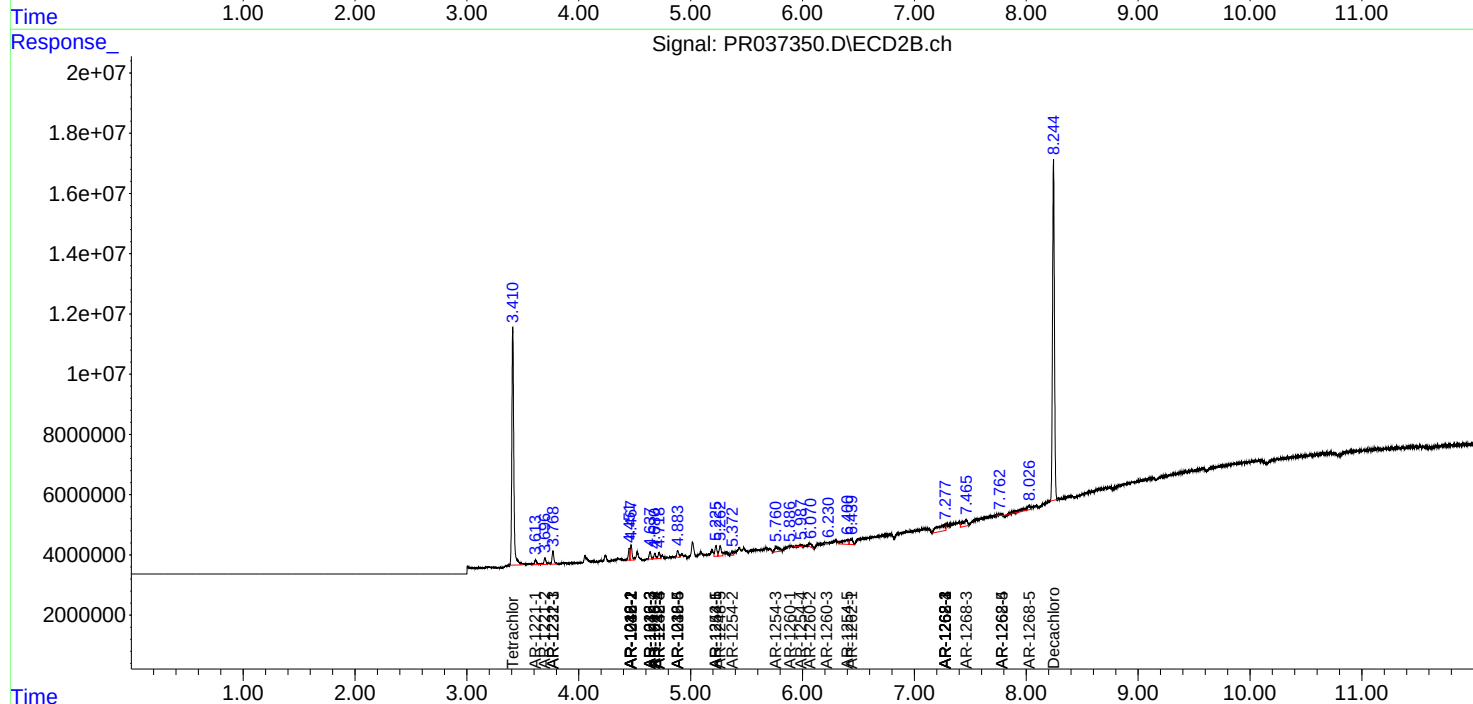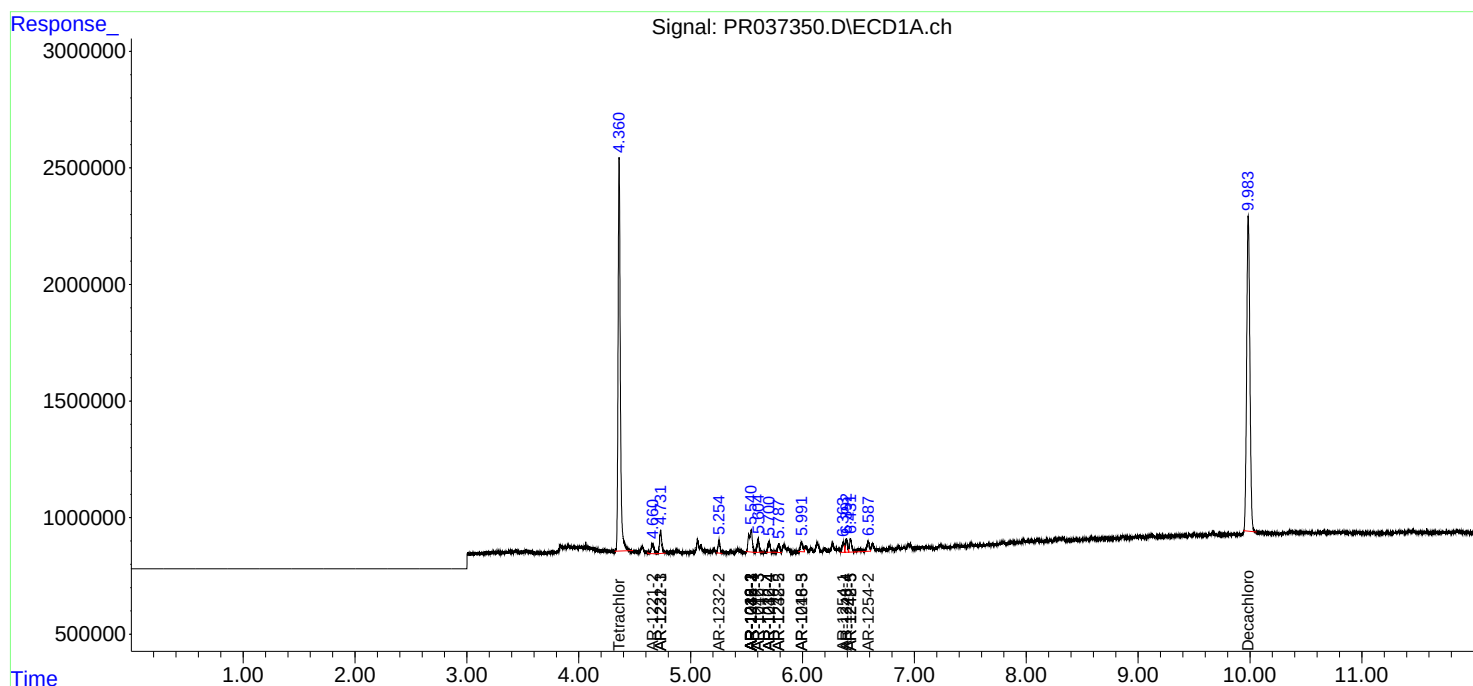


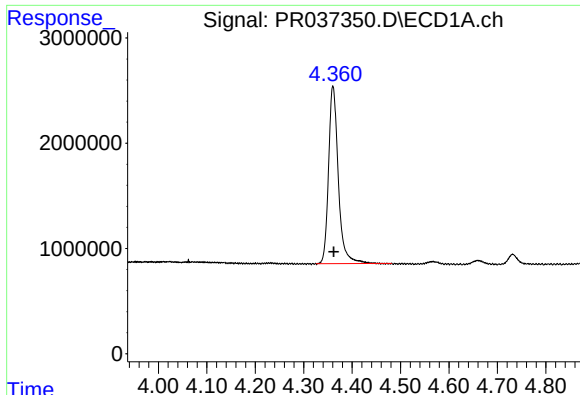

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: -0.001 min
Response: 23410266
Conc: 18.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

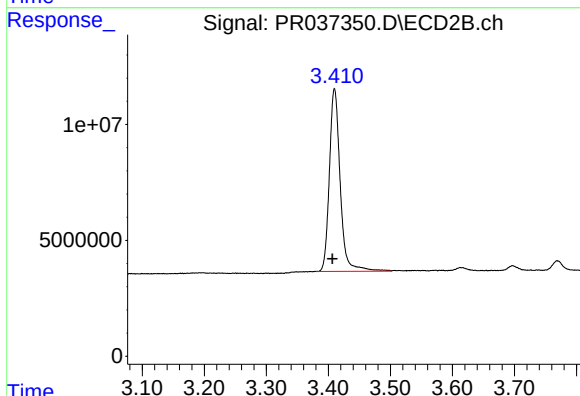


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.004 min
Response: 95683992
Conc: 19.95 ng/ml

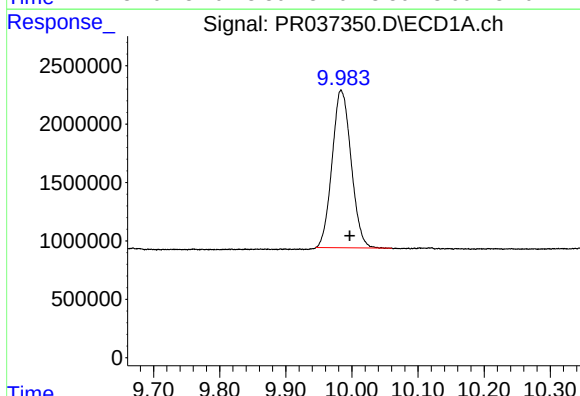


#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: -0.013 min
Response: 26888261
Conc: 20.33 ng/ml

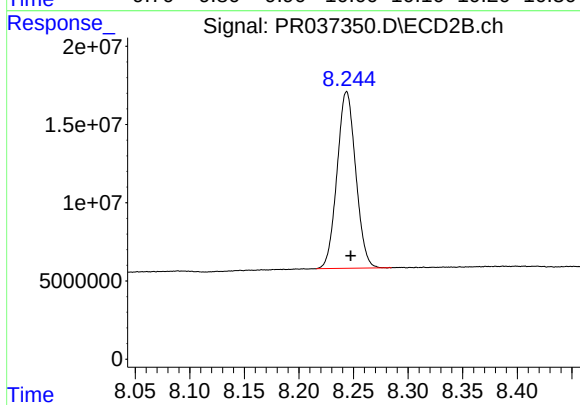

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 134422095
Conc: 23.08 ng/ml

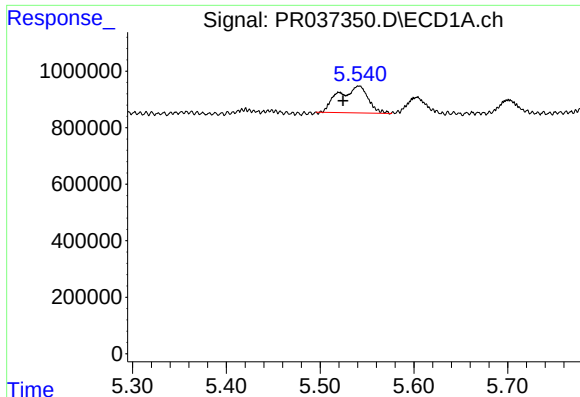

#3 AR-1016-1


R.T.: 5.541 min
Delta R.T.: 0.017 min
Response: 2035898
Conc: 47.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

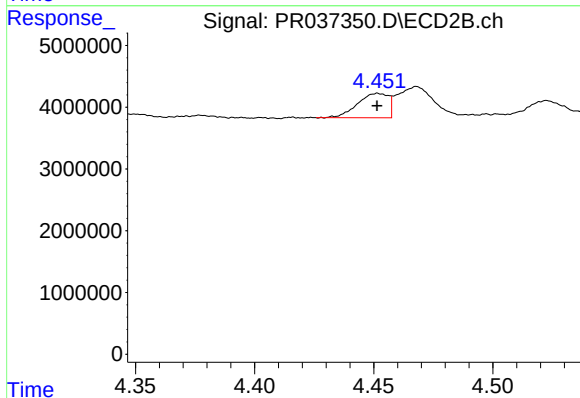


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 3519770
Conc: 19.33 ng/ml

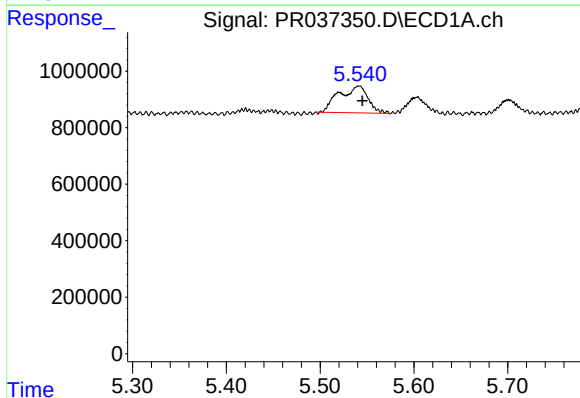


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2035898
Conc: 29.40 ng/ml

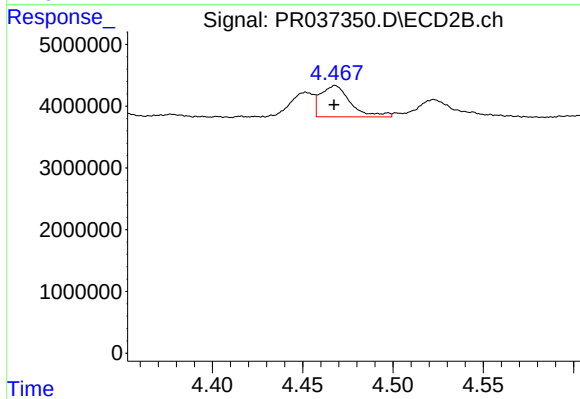

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 5836394
Conc: 20.69 ng/ml

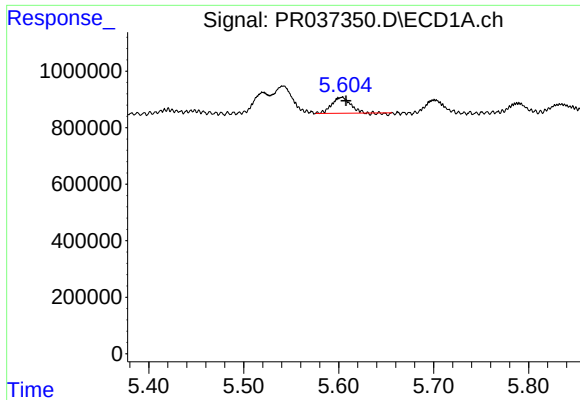

#5 AR-1016-3


R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 734276
Conc: 18.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

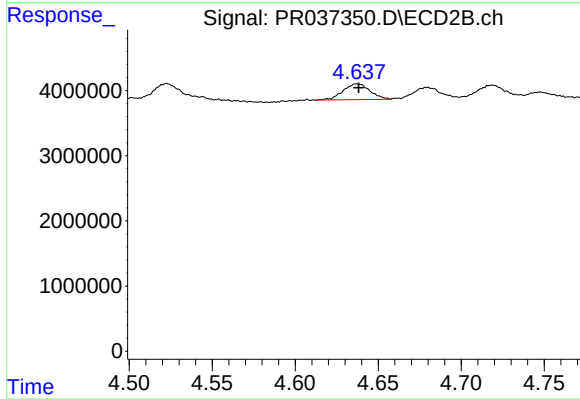


#5 AR-1016-3

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 2731601
Conc: 19.00 ng/ml

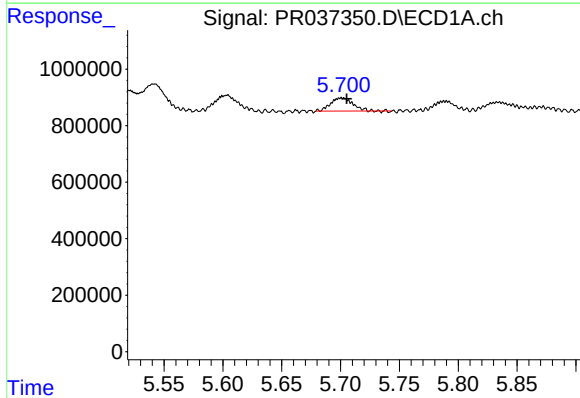


#6 AR-1016-4

R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 603774
Conc: 18.39 ng/ml

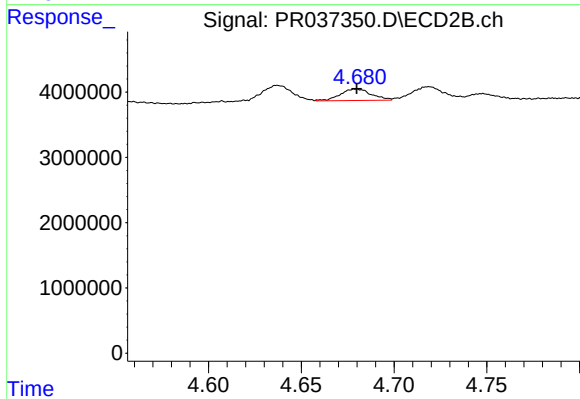

#6 AR-1016-4


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 2054980
Conc: 18.57 ng/ml

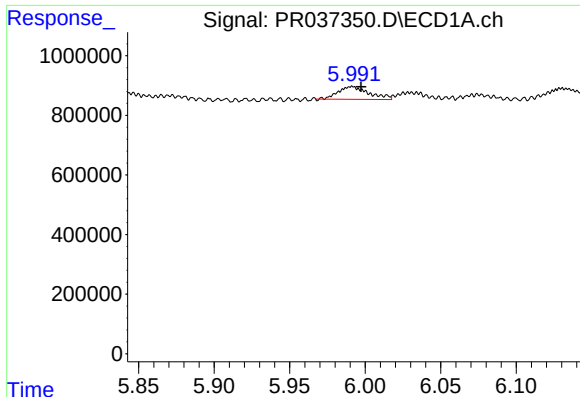

#7 AR-1016-5


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 600686
Conc: 17.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

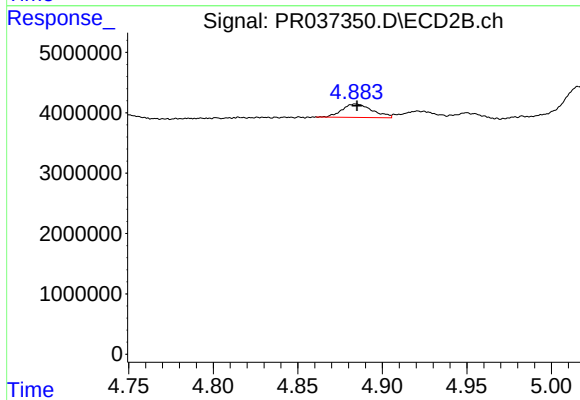


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 2768695
Conc: 18.21 ng/ml

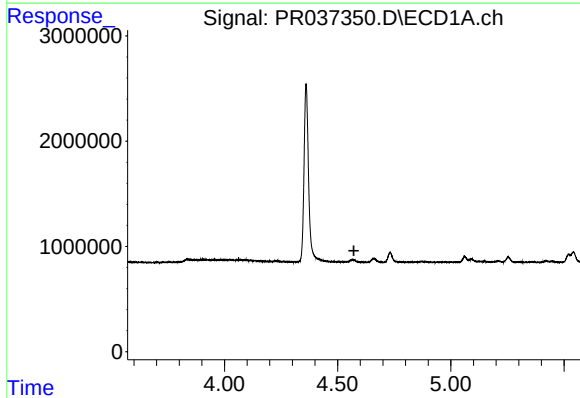


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

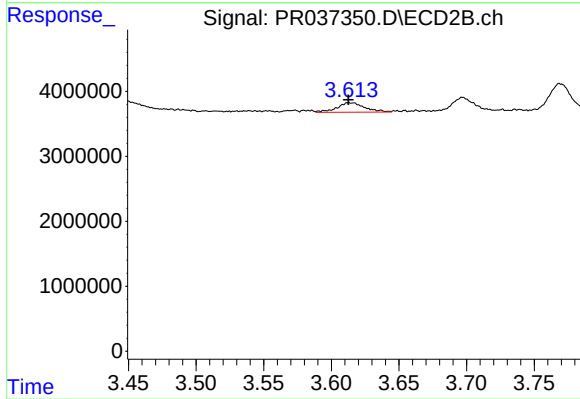

#8 AR-1221-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 2090177
Conc: 41.05 ng/ml

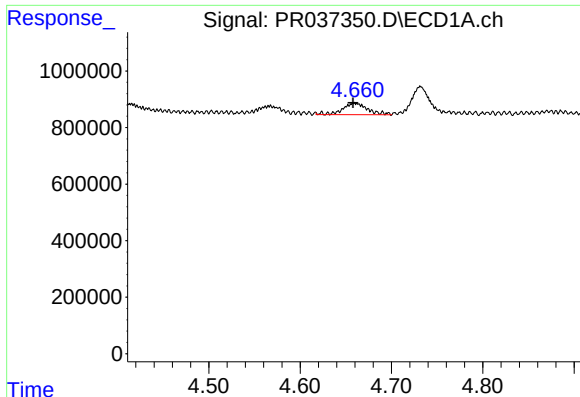

#9 AR-1221-2


R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 768264
Conc: 84.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

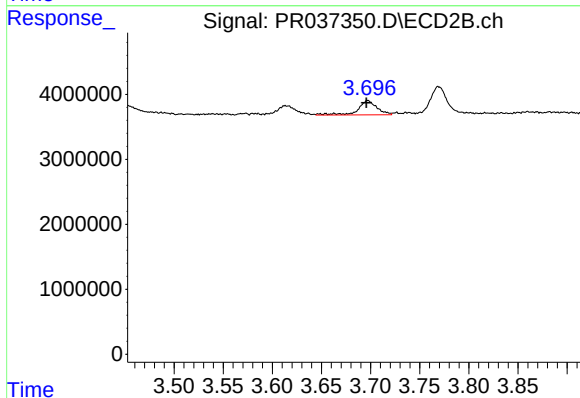


#9 AR-1221-2

R.T.: 3.697 min
Delta R.T.: 0.001 min
Response: 2934854
Conc: 79.03 ng/ml

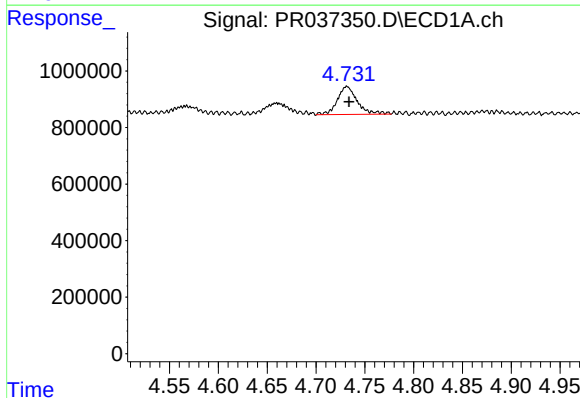


#10 AR-1221-3

R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 1399080
Conc: 45.65 ng/ml

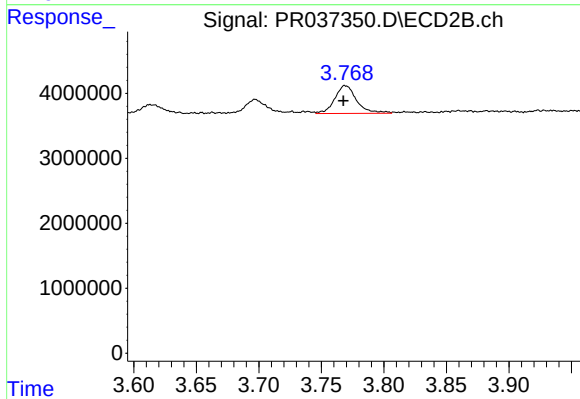

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 5209726
Conc: 42.55 ng/ml

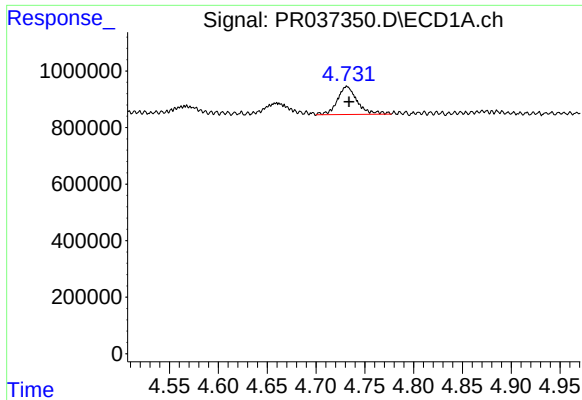

#11 AR-1232-1


R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 1399080
Conc: 47.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

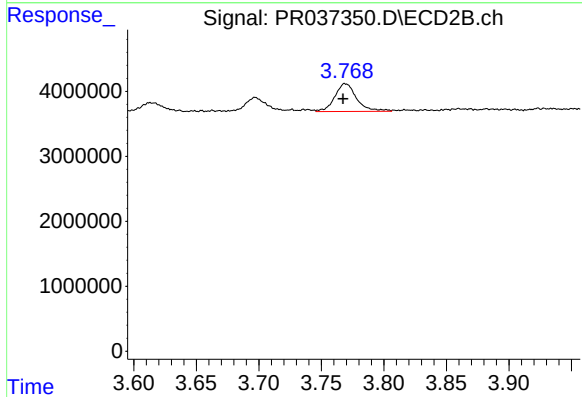


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 5209726
Conc: 44.53 ng/ml

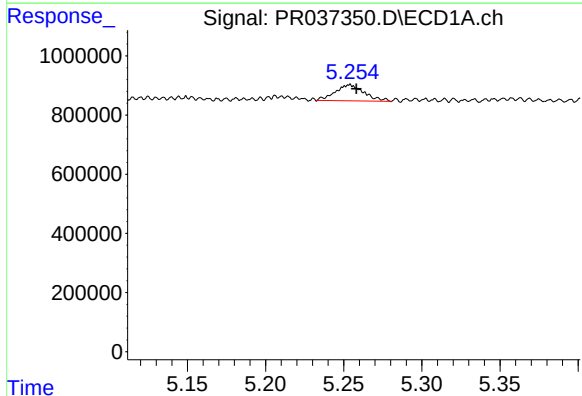


#12 AR-1232-2

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 699134
Conc: 41.38 ng/ml

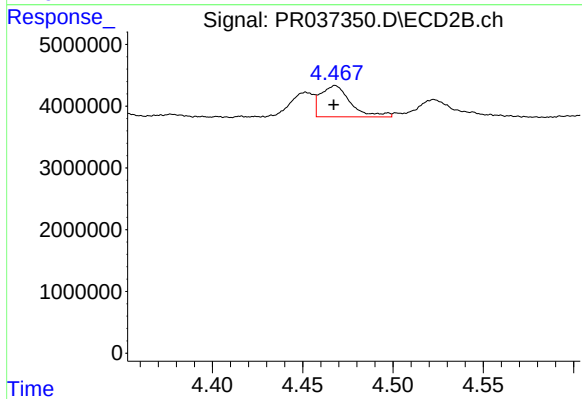

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 5836394
Conc: 42.22 ng/ml

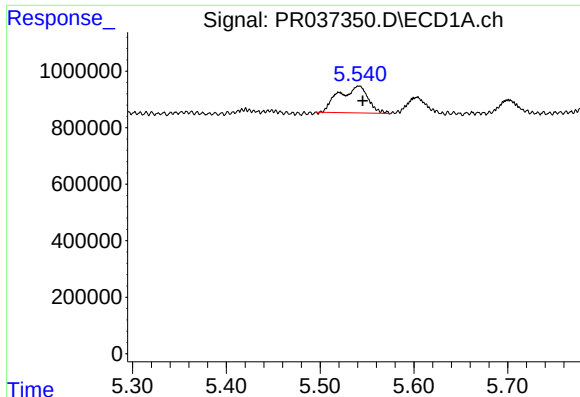

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2035898
Conc: 60.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

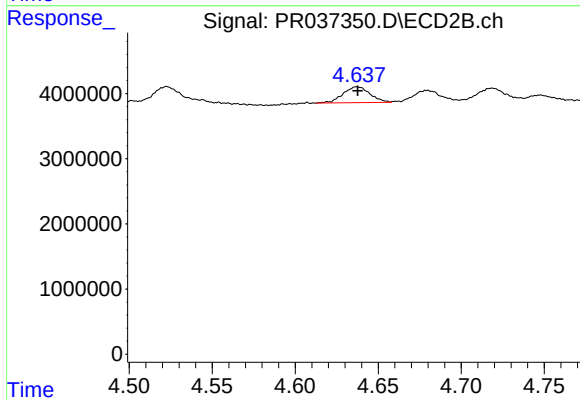


#13 AR-1232-3

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 2731601
Conc: 38.91 ng/ml

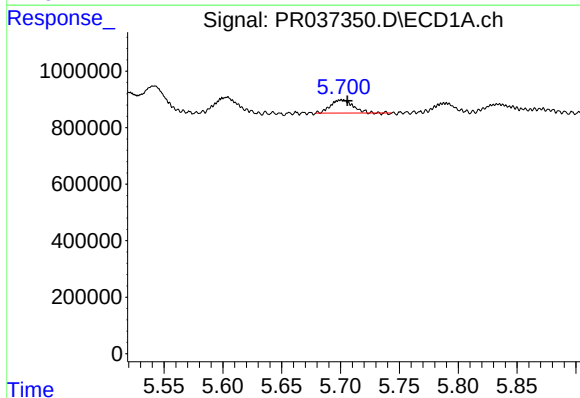


#14 AR-1232-4

R.T.: 5.701 min
Delta R.T.: -0.005 min
Response: 603774
Conc: 38.46 ng/ml

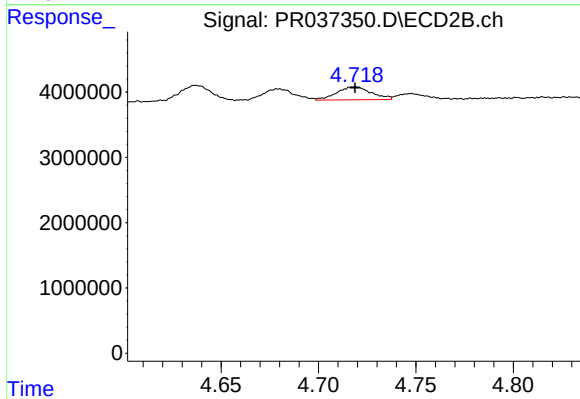

#14 AR-1232-4


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 2485737
Conc: 41.66 ng/ml

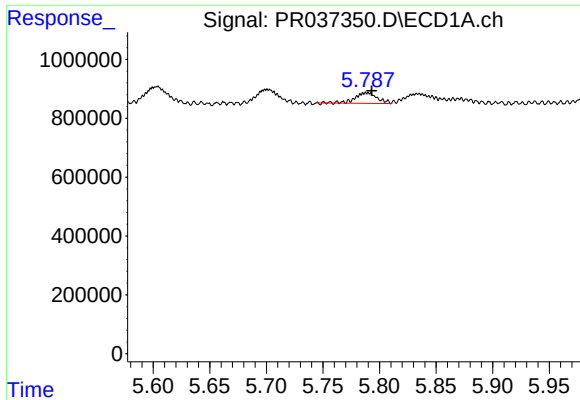

#15 AR-1232-5


R.T.: 5.789 min
Delta R.T.: -0.005 min
Response: 485676
Conc: 41.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

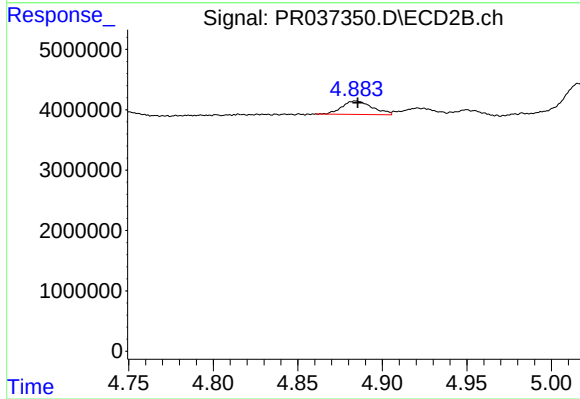


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 2768695
Conc: 40.57 ng/ml

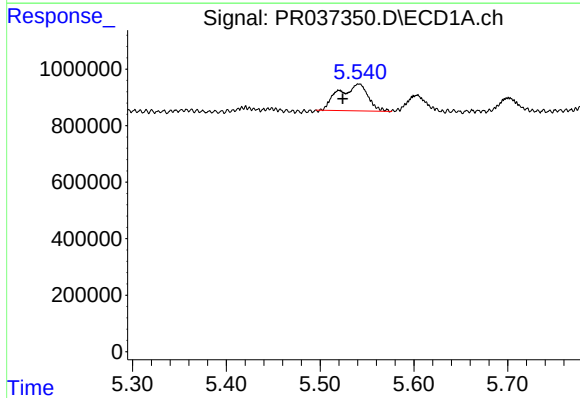


#16 AR-1242-1

R.T.: 5.541 min
Delta R.T.: 0.017 min
Response: 2035898
Conc: 59.50 ng/ml

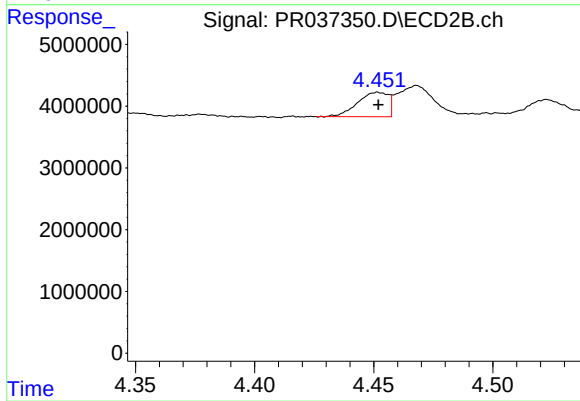

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 3519770
Conc: 24.02 ng/ml

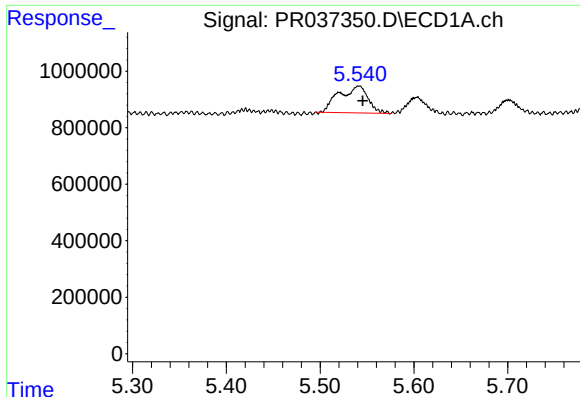

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 2035898
Conc: 36.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

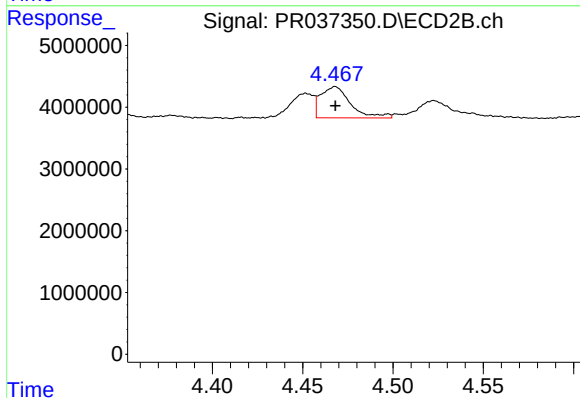


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 5836394
Conc: 25.58 ng/ml

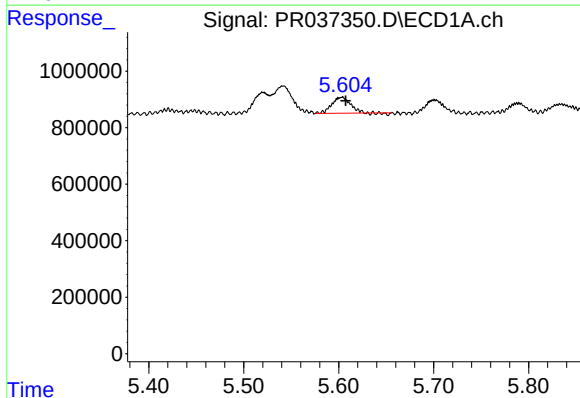


#18 AR-1242-3

R.T.: 5.603 min
Delta R.T.: -0.005 min
Response: 734276
Conc: 22.31 ng/ml

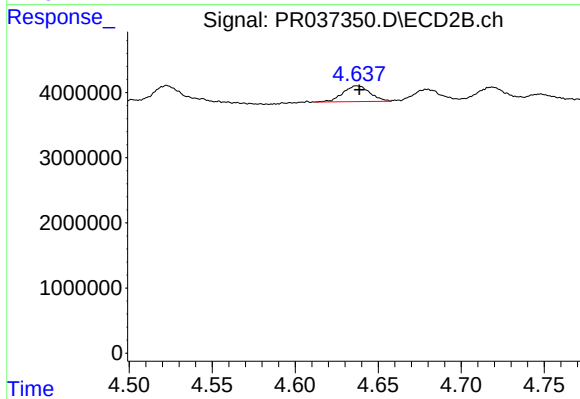

#18 AR-1242-3


R.T.: 4.637 min
Delta R.T.: -0.001 min
Response: 2731601
Conc: 23.62 ng/ml

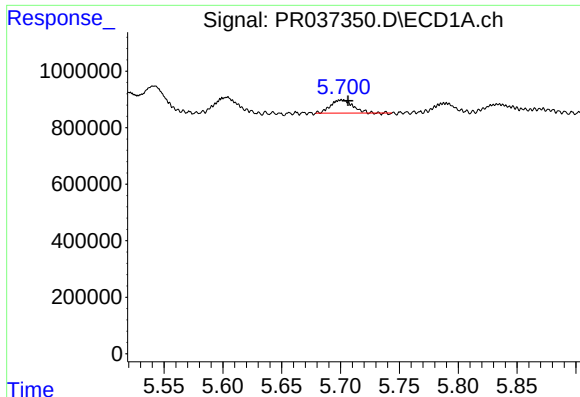

#19 AR-1242-4


R.T.: 5.701 min
Delta R.T.: -0.006 min
Response: 603774
Conc: 22.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

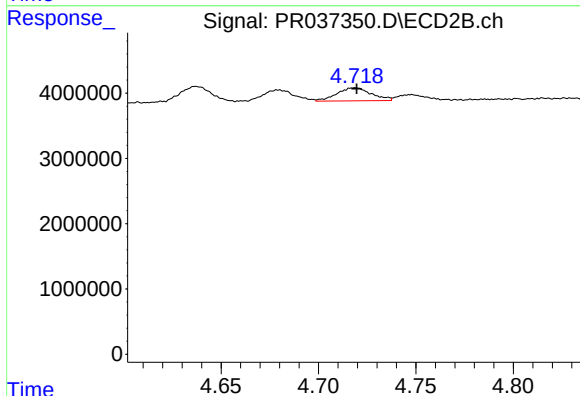


#19 AR-1242-4

R.T.: 4.719 min
Delta R.T.: -0.001 min
Response: 2485737
Conc: 22.62 ng/ml

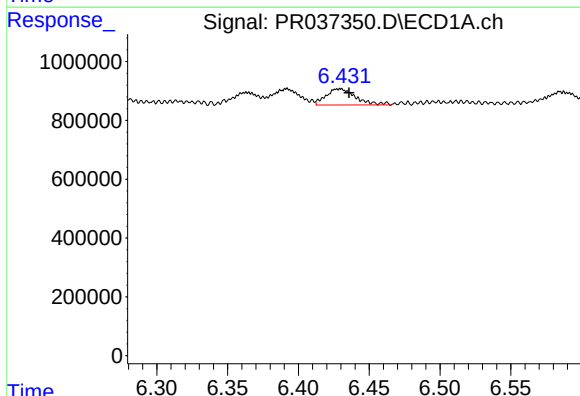


#20 AR-1242-5

R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 804987
Conc: 25.02 ng/ml

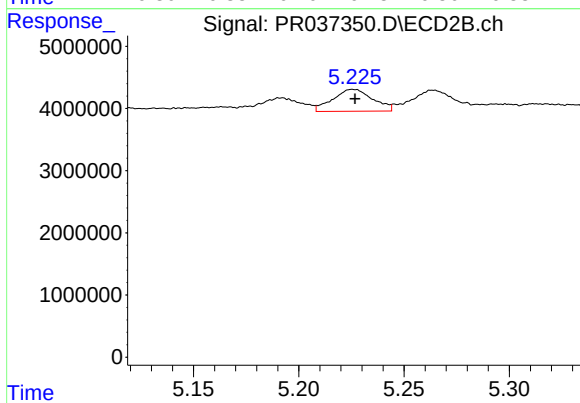

#20 AR-1242-5


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 4663742
Conc: 28.15 ng/ml

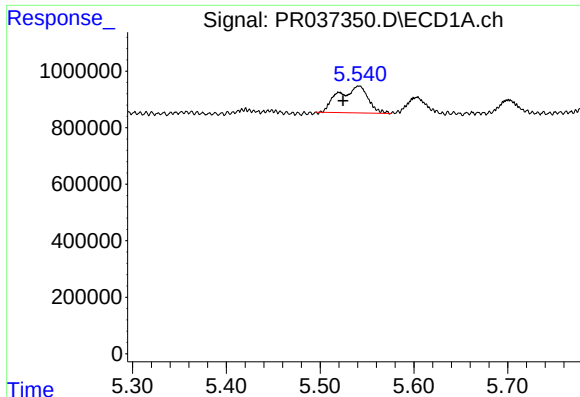

#21 AR-1248-1


R.T.: 5.541 min
Delta R.T.: 0.017 min
Response: 2035898
Conc: 88.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

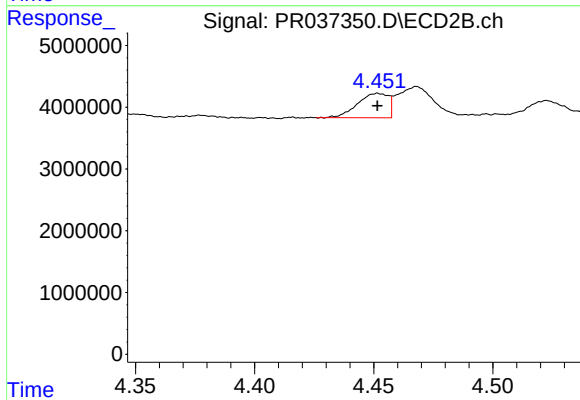


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 3519770
Conc: 34.97 ng/ml

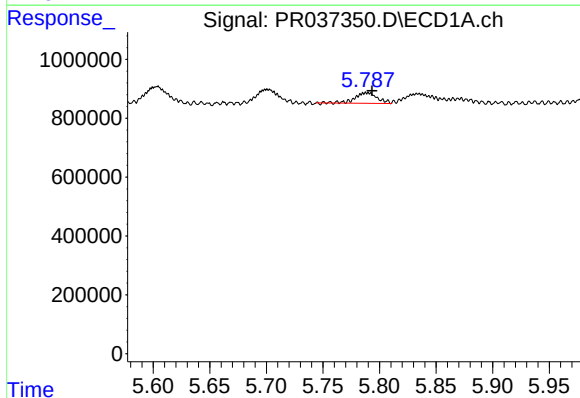


#22 AR-1248-2

R.T.: 5.789 min
Delta R.T.: -0.005 min
Response: 485676
Conc: 13.87 ng/ml

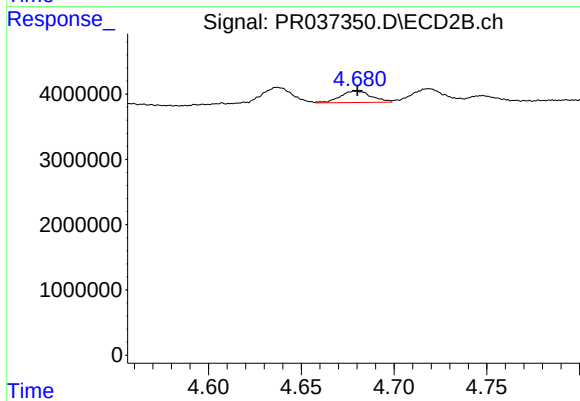

#22 AR-1248-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 2054980
Conc: 15.06 ng/ml

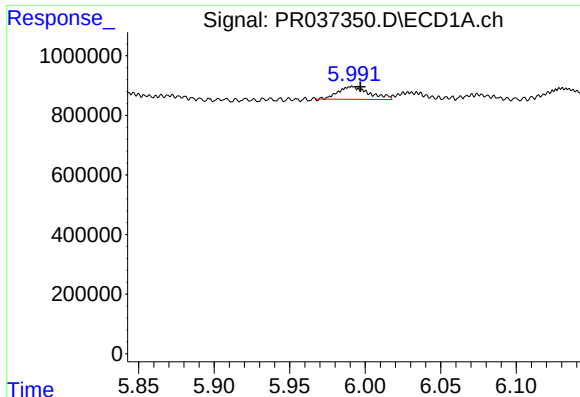

#23 AR-1248-3


R.T.: 5.991 min
Delta R.T.: -0.006 min
Response: 600686
Conc: 14.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

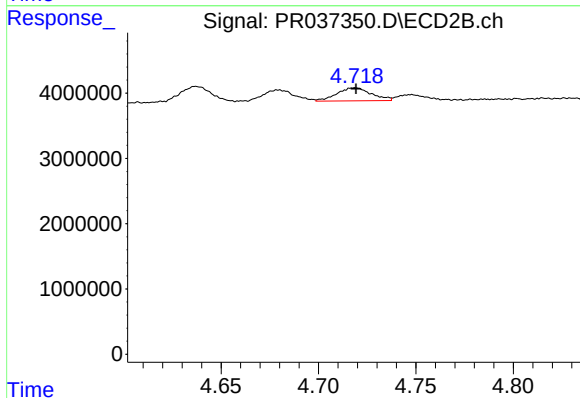


#23 AR-1248-3

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 2485737
Conc: 17.76 ng/ml

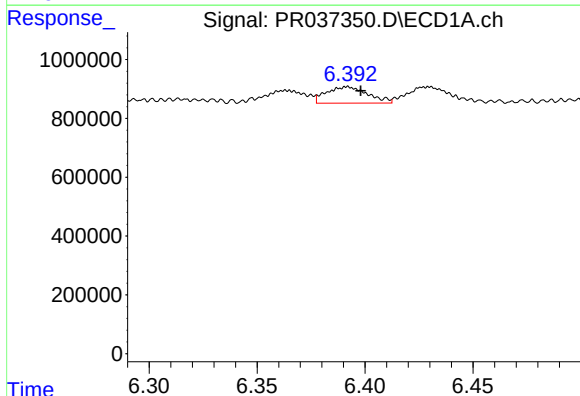


#24 AR-1248-4

R.T.: 6.392 min
Delta R.T.: -0.006 min
Response: 744621
Conc: 15.21 ng/ml

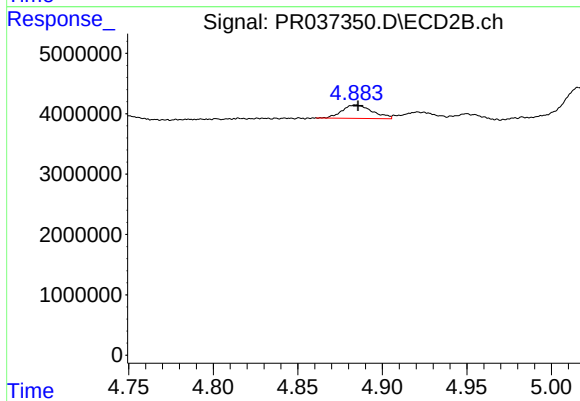

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 2768695
Conc: 15.56 ng/ml

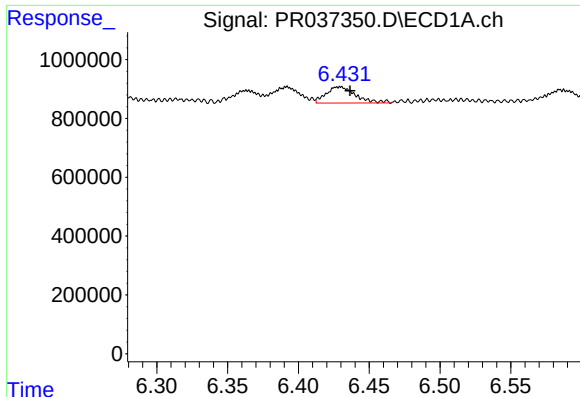

#25 AR-1248-5


R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 804987
Conc: 17.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

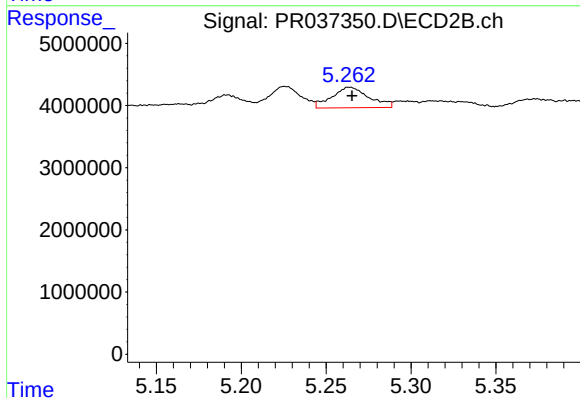


#25 AR-1248-5

R.T.: 5.264 min
Delta R.T.: -0.001 min
Response: 5025195
Conc: 25.69 ng/ml

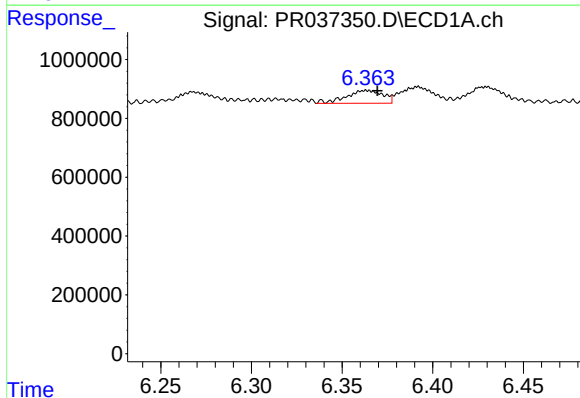


#26 AR-1254-1

R.T.: 6.364 min
Delta R.T.: -0.006 min
Response: 615052
Conc: 11.26 ng/ml

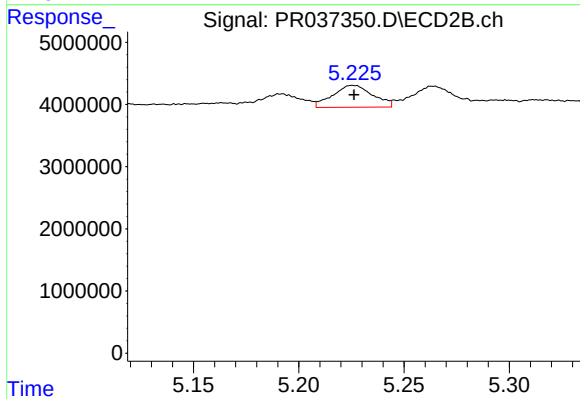

#26 AR-1254-1


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 4663742
Conc: 13.54 ng/ml

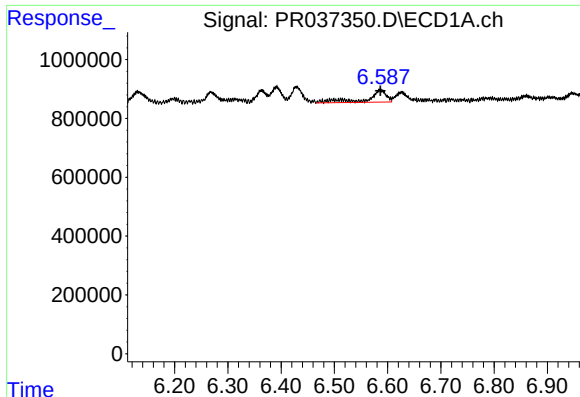

#27 AR-1254-2


R.T.: 6.586 min
Delta R.T.: 0.000 min
Response: 1023954
Conc: 11.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

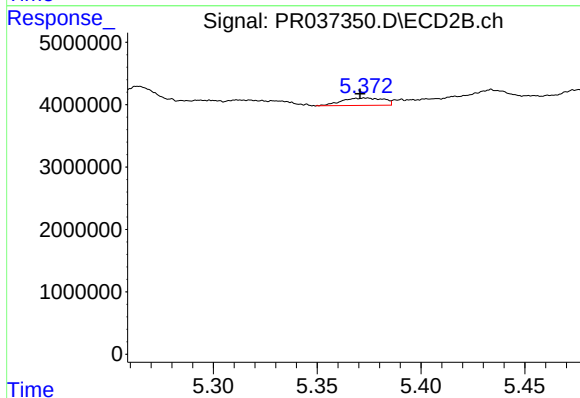


#27 AR-1254-2

R.T.: 5.374 min
Delta R.T.: 0.003 min
Response: 1645133
Conc: 5.49 ng/ml

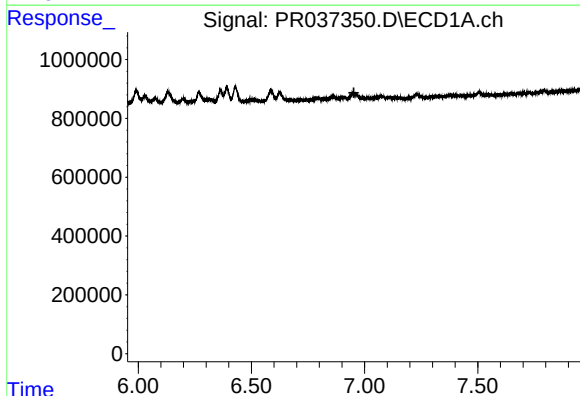


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

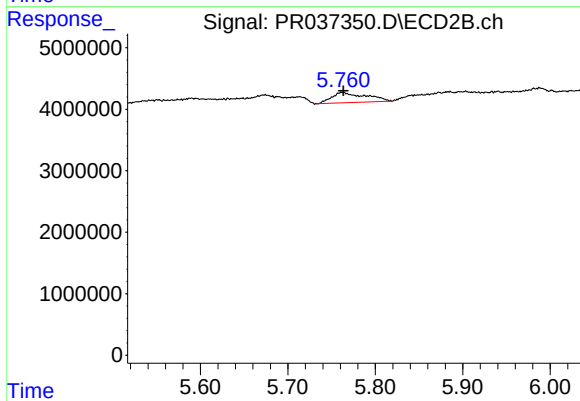

#28 AR-1254-3


R.T.: 5.762 min
Delta R.T.: 0.000 min
Response: 4518844
Conc: 9.54 ng/ml

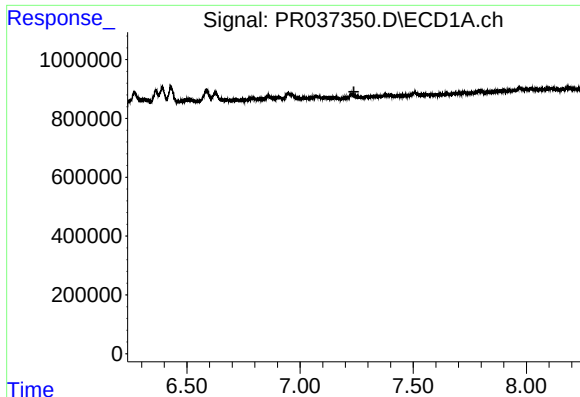

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

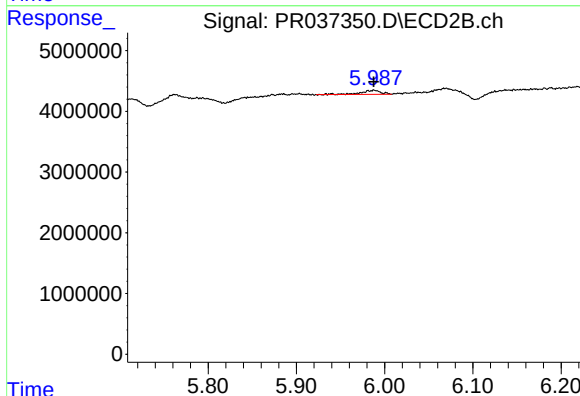


#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 1028756
Conc: 2.93 ng/ml

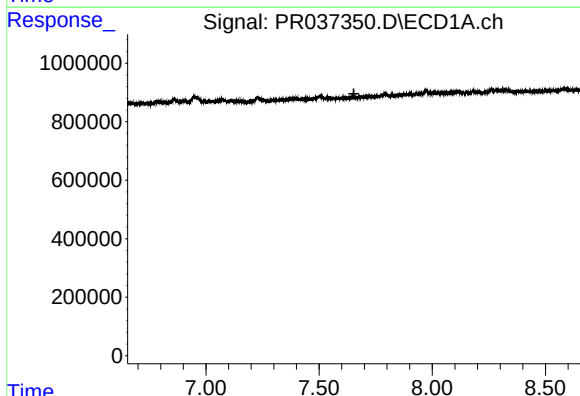


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

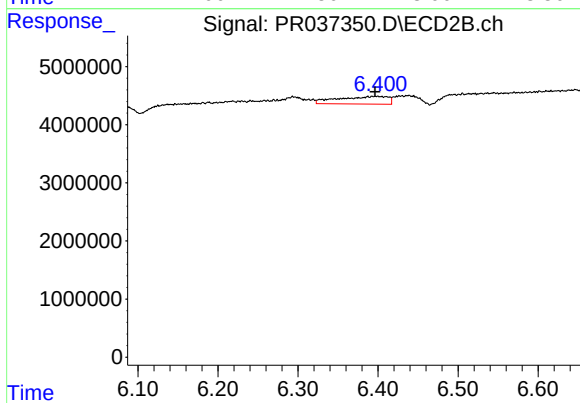

#30 AR-1254-5


R.T.: 6.399 min
Delta R.T.: 0.003 min
Response: 5776951
Conc: 13.05 ng/ml

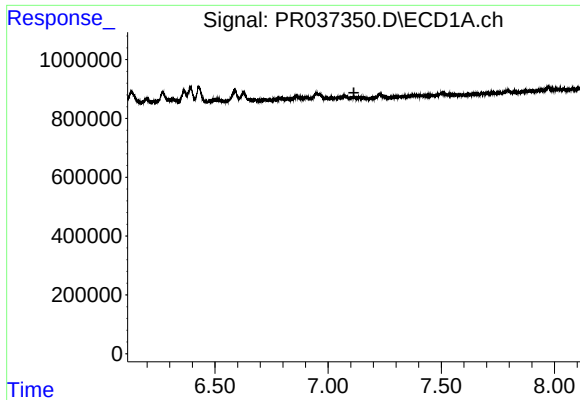

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

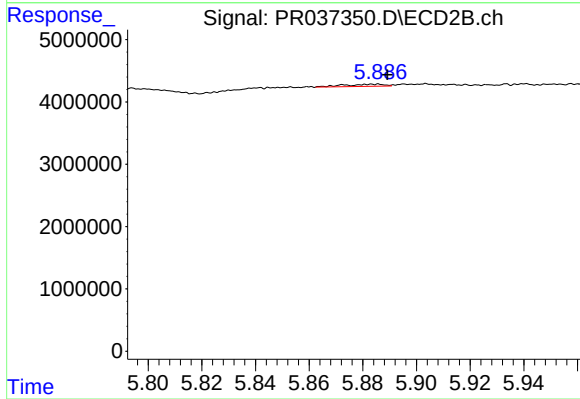


#31 AR-1260-1

R.T.: 5.885 min
Delta R.T.: -0.004 min
Response: 366391
Conc: 1.25 ng/ml

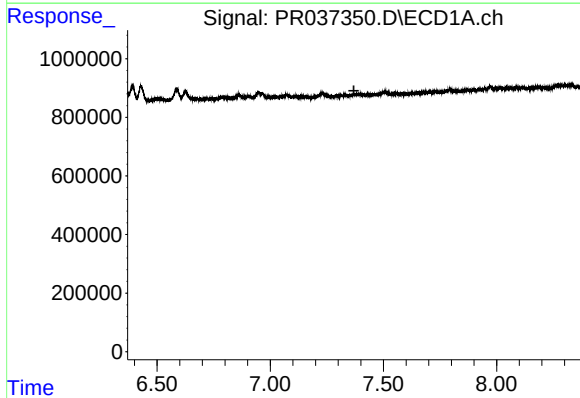


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

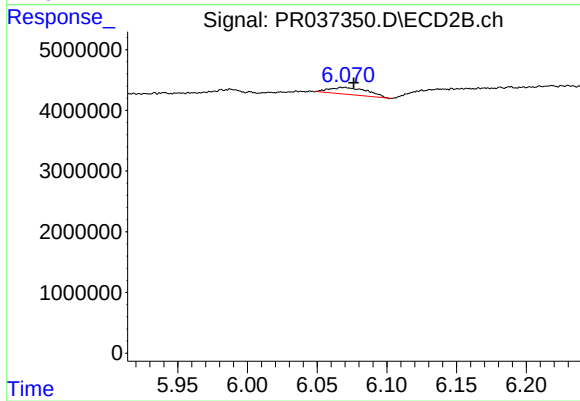

#32 AR-1260-2


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 2045442
Conc: 4.44 ng/ml

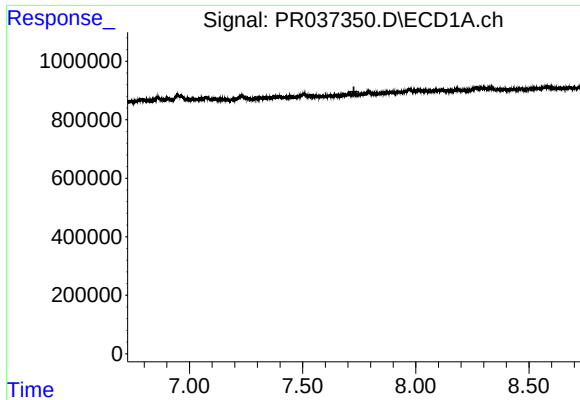

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

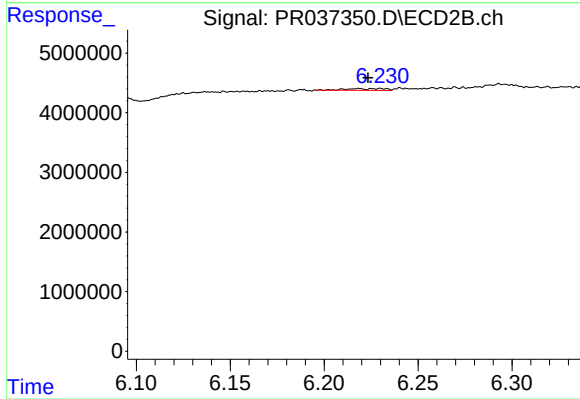


#33 AR-1260-3

R.T.: 6.218 min
Delta R.T.: -0.005 min
Response: 429275
Conc: 1.20 ng/ml

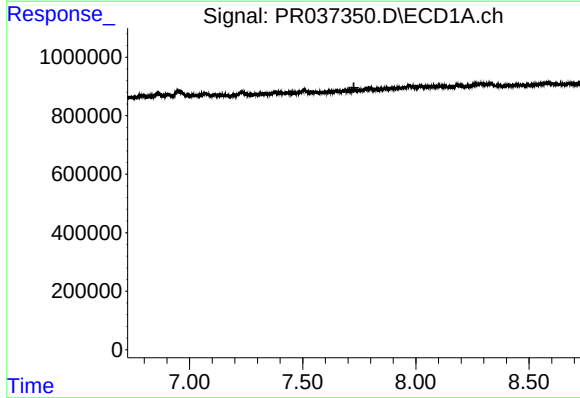


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

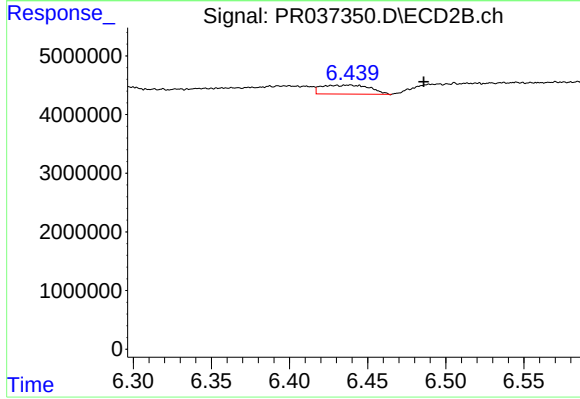

#36 AR-1262-1


R.T.: 6.438 min
Delta R.T.: -0.048 min
Response: 3284638
Conc: 13.11 ng/ml

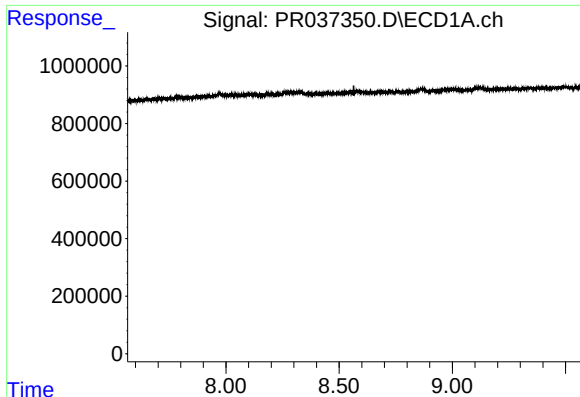

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

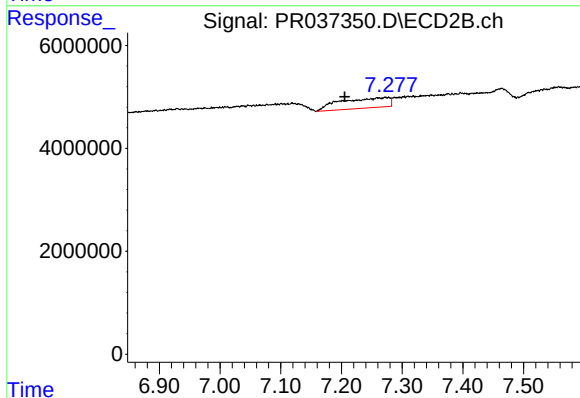


#38 AR-1262-3

R.T.: 7.274 min
Delta R.T.: 0.069 min
Response: 11059791
Conc: 20.17 ng/ml

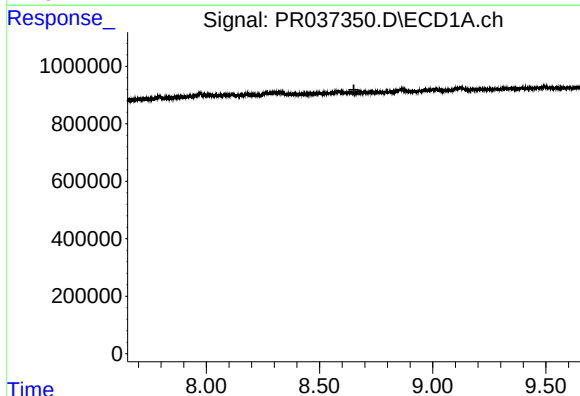


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

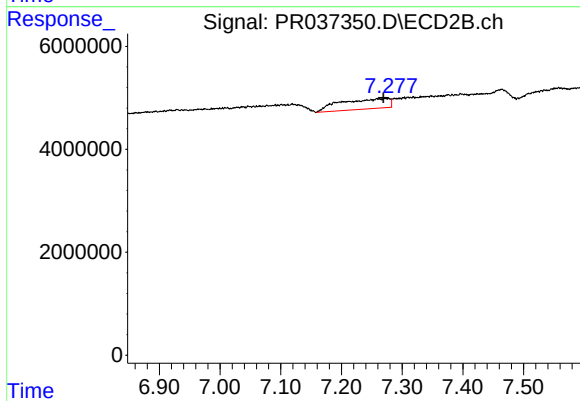

#39 AR-1262-4


R.T.: 7.274 min
Delta R.T.: 0.005 min
Response: 11059791
Conc: 12.32 ng/ml

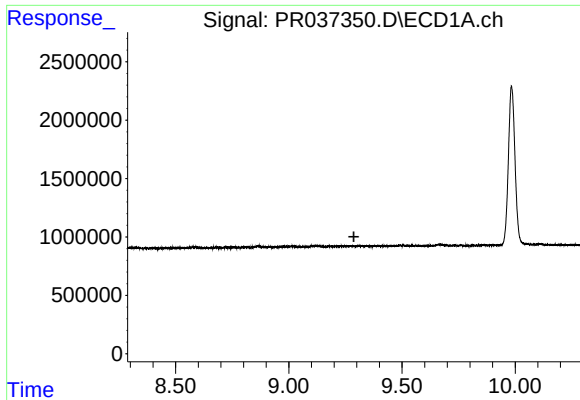

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

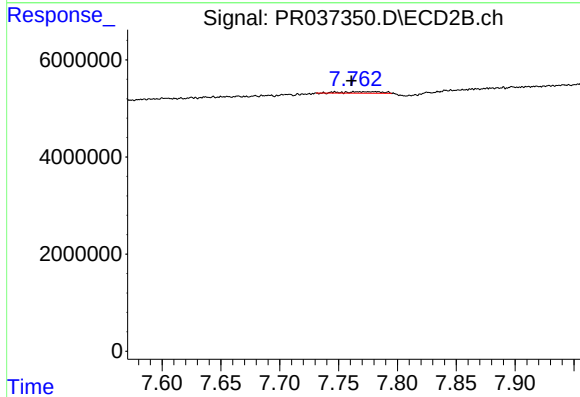


#40 AR-1262-5

R.T.: 7.780 min
Delta R.T.: 0.019 min
Response: 660544
Conc: 1.73 ng/ml

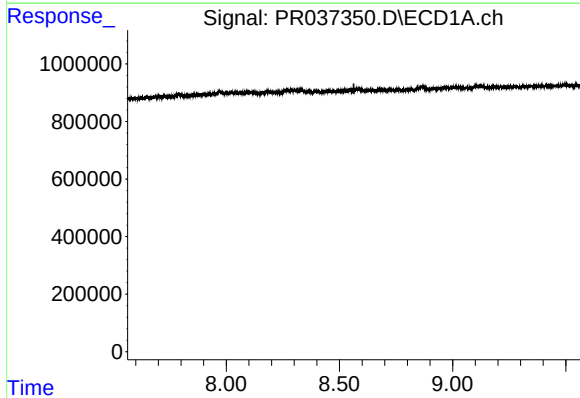


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

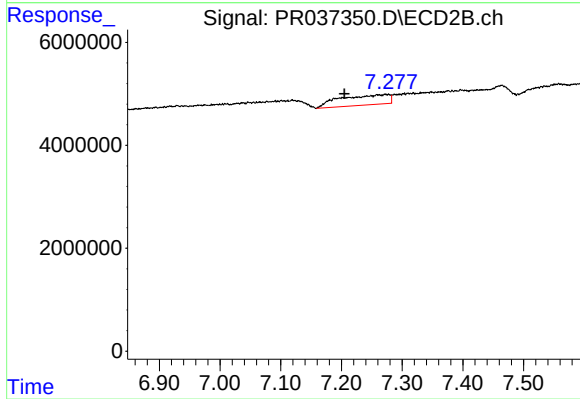

#41 AR-1268-1


R.T.: 7.274 min
Delta R.T.: 0.070 min
Response: 11059791
Conc: 8.98 ng/ml

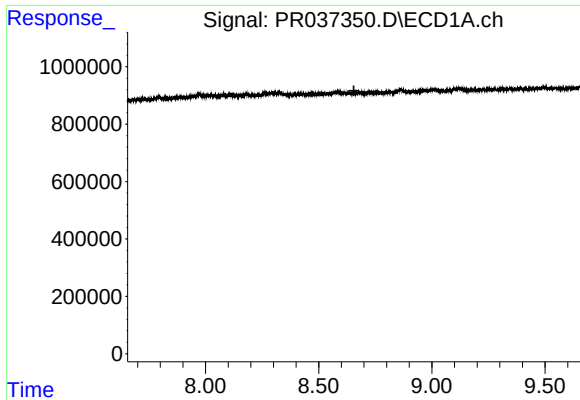

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

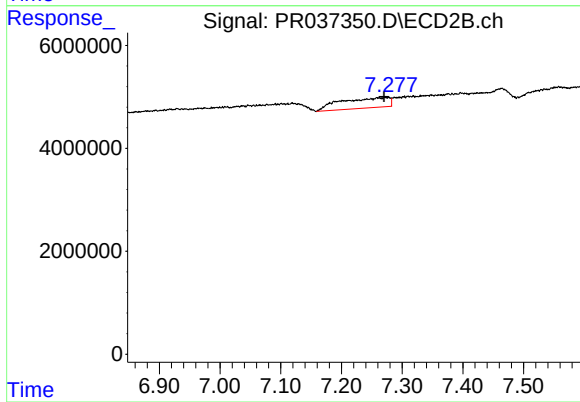


#42 AR-1268-2

R.T.: 7.274 min
Delta R.T.: 0.004 min
Response: 11059791
Conc: 10.44 ng/ml

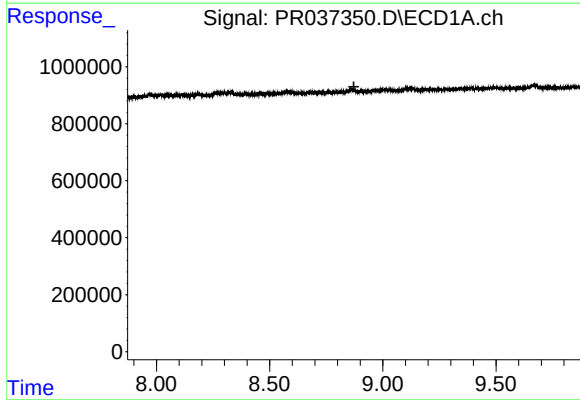


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

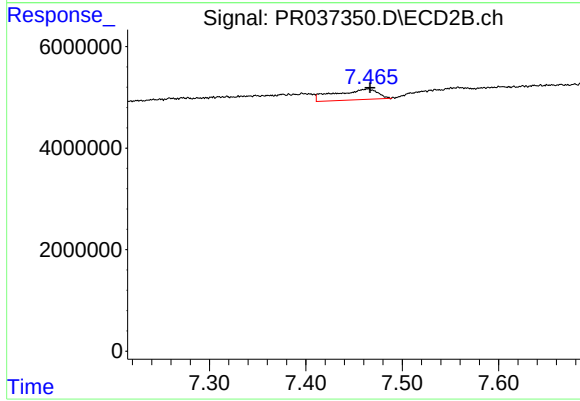

#43 AR-1268-3


R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 6416200
Conc: 7.24 ng/ml

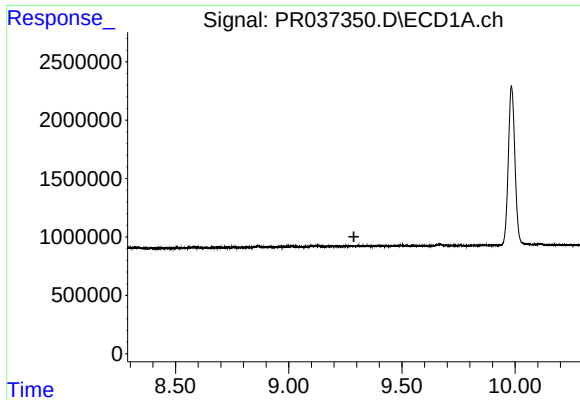

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

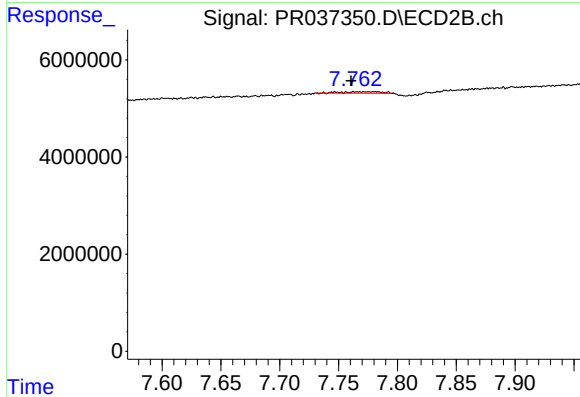


#44 AR-1268-4

R.T.: 7.780 min
Delta R.T.: 0.019 min
Response: 660544
Conc: 1.82 ng/ml

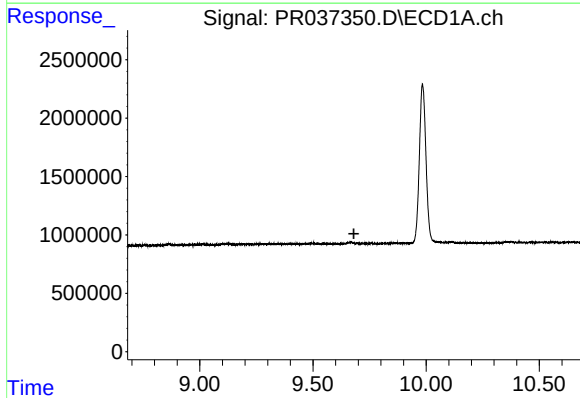

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

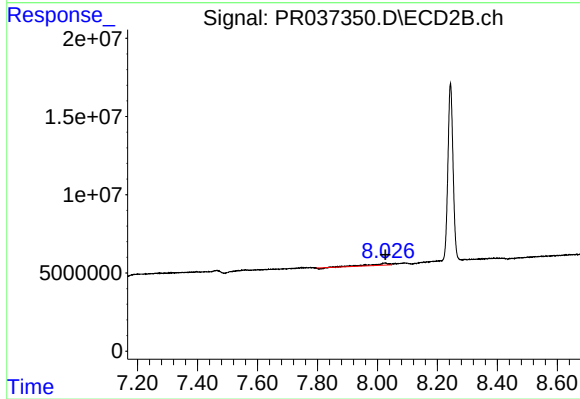

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.002 min
Response: 5855832
Conc: 2.30 ng/ml