

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 17:20
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1248 LOD 25PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:04:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.361	3.410	30108792	121.9E6	24.068	25.417
2)	SA Decachlor...	9.980	8.241	29545365	153.3E6	22.339	26.317
Target Compounds							
3)	L1 AR-1016-1	5.519	4.451	693178	3113686	16.087	17.101
4)	L1 AR-1016-2	5.541	4.467	913087	3422426	13.186	12.131
5)	L1 AR-1016-3	5.601	4.638	668371	2000149	16.573	13.911
6)	L1 AR-1016-4	5.700	4.679	353775	4387847	10.773	39.661 #
7)	L1 AR-1016-5	5.990	4.884	1233520	5534446	35.973	36.409
8)	L2 AR-1221-1	0.000	3.607	0	113259	N.D.	2.224 #
9)	L2 AR-1221-2	4.665	3.698	778272	2021057	86.054	54.423 #
10)	L2 AR-1221-3	4.665	3.771	778272	510274	25.393	4.167 #
11)	L3 AR-1232-1	4.665	3.771	778272	510274	26.607	4.362 #
12)	L3 AR-1232-2	5.253	4.467	785817	3422426	46.505	24.760 #
13)	L3 AR-1232-3	5.541	4.638	913087	2000149	27.011	28.491
14)	L3 AR-1232-4	5.700	4.718	353775	4208219	22.538	70.523 #
15)	L3 AR-1232-5	5.787	4.884	1010843	5534446	86.429	81.098
16)	L4 AR-1242-1	5.519	4.451	693178	3113686	20.260	21.248
17)	L4 AR-1242-2	5.541	4.467	913087	3422426	16.461	15.000
18)	L4 AR-1242-3	5.601	4.638	668371	2000149	20.306	17.298
19)	L4 AR-1242-4	5.700	4.718	353775	4208219	13.412	38.288 #
20)	L4 AR-1242-5	6.428	5.225	1520007	9736352	47.236	58.759
21)	L5 AR-1248-1	5.519	4.451	693178	3113686	30.260	30.931
22)	L5 AR-1248-2	5.787	4.679	1010843	4387847	28.869	32.152
23)	L5 AR-1248-3	5.990	4.718	1233520	4208219	30.152	30.064
24)	L5 AR-1248-4	6.390	4.884	1604155	5534446	32.768	31.099
25)	L5 AR-1248-5	6.428	5.263	1520007	7315356	32.178	37.397
26)	L6 AR-1254-1	6.362	5.225	1248896	9736352	22.861	28.264
27)	L6 AR-1254-2	6.584	5.370	1863161	3573575	21.741	11.932 #
28)	L6 AR-1254-3	6.945	5.760	1174312	5710042	12.910	12.056
29)	L6 AR-1254-4	7.228	5.985	780516	2754011	11.648	7.854 #
30)	L6 AR-1254-5	0.000	6.393	0	4310049	N.D.	9.733 #
31)	L7 AR-1260-1	0.000	5.902	0	1735431	N.D.	5.938 #
32)	L7 AR-1260-2	0.000	6.068	0	2375904	N.D.	5.158 #
33)	L7 AR-1260-3	0.000	6.222	0	414764	N.D.	1.163 #
34)	L7 AR-1260-4	0.000	6.687	0	415981	N.D.	1.365 #
35)	L7 AR-1260-5	0.000	6.925	0	433241	N.D.	0.500 #
36)	L8 AR-1262-1	0.000	6.490	0	3104403	N.D.	12.387 #
37)	L8 AR-1262-2	0.000	6.925	0	433241	N.D.	0.345 #
38)	L8 AR-1262-3	0.000	7.204	0	3831310	N.D.	6.988 #
39)	L8 AR-1262-4	0.000	7.279	0	6826928	N.D.	7.605 #
40)	L8 AR-1262-5	0.000	7.758	0	253420	N.D.	0.662 #
41)	L9 AR-1268-1	0.000	7.204	0	3831310	N.D.	3.112 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 17:20
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1248 LOD 25PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:04:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.279	0	6826928	N.D.	6.447 #
43) L9	AR-1268-3	0.000	7.463	0	9776303	N.D.	11.031 #
44) L9	AR-1268-4	0.000	7.758	0	253420	N.D.	0.699 #
45) L9	AR-1268-5	0.000	8.024	0	3127704	N.D.	1.229 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 17:20
Operator : SM\SJ
Sample : K2241-07
Misc : AR1248 LOD 25PPB
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:04:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

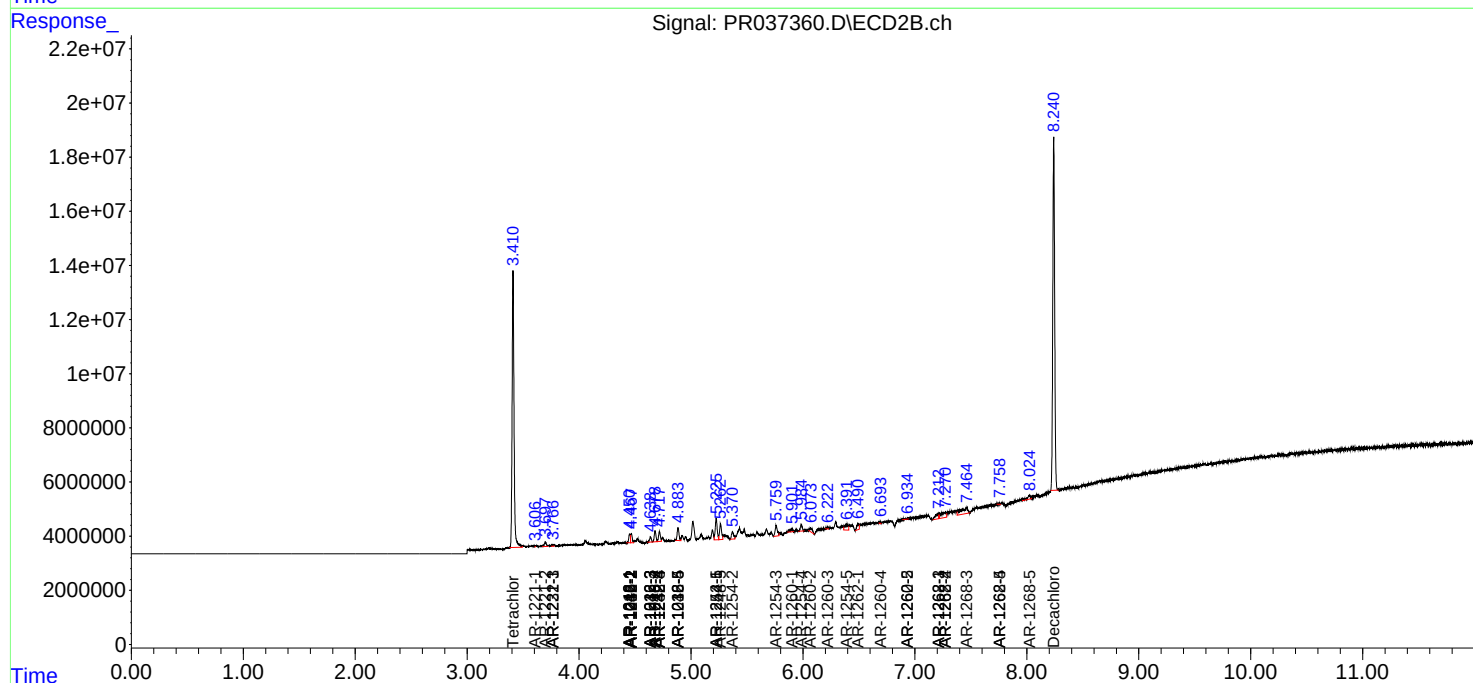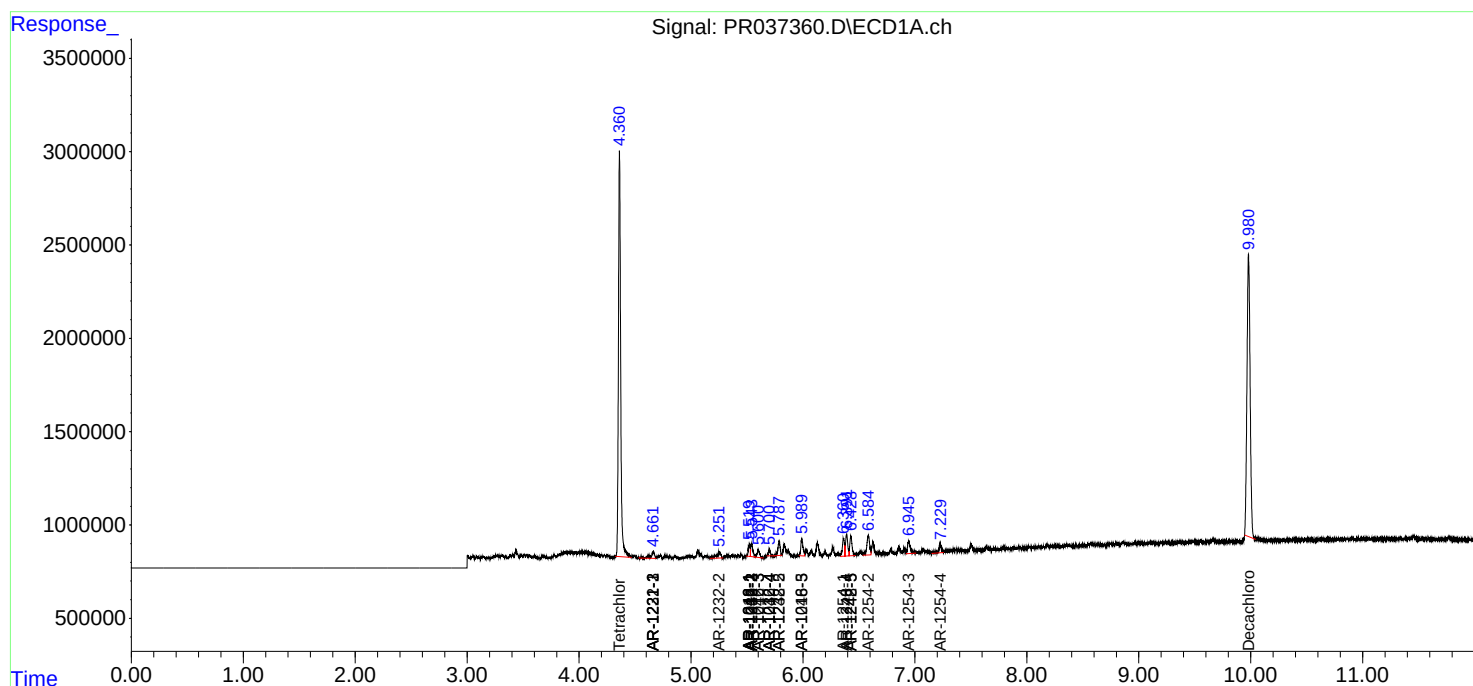


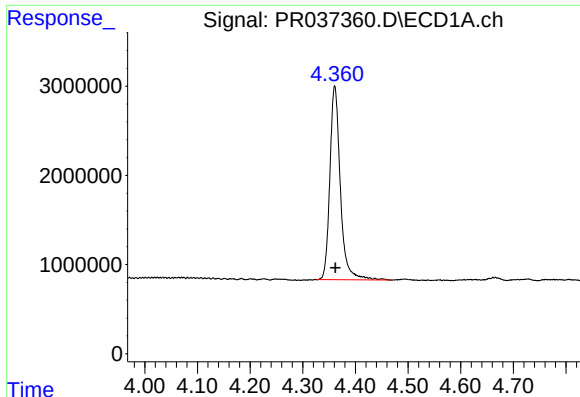

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: -0.001 min
Response: 30108792
Conc: 24.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

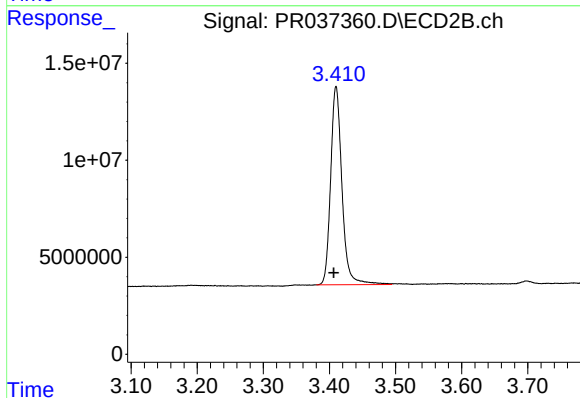


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.004 min
Response: 121887316
Conc: 25.42 ng/ml

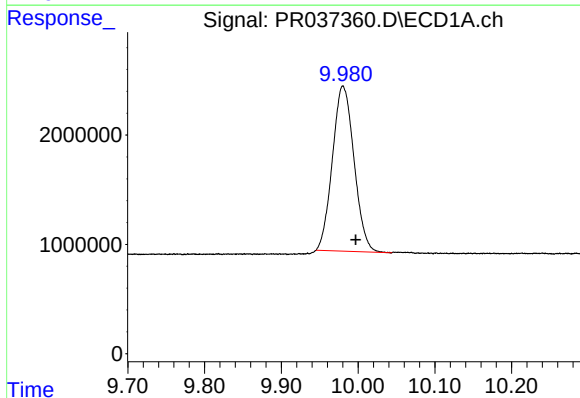


#2 Decachlorobiphenyl

R.T.: 9.980 min
Delta R.T.: -0.016 min
Response: 29545365
Conc: 22.34 ng/ml

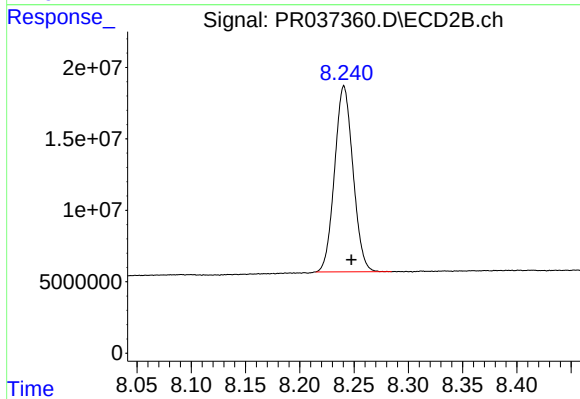

#2 Decachlorobiphenyl


R.T.: 8.241 min
Delta R.T.: -0.007 min
Response: 153275732
Conc: 26.32 ng/ml

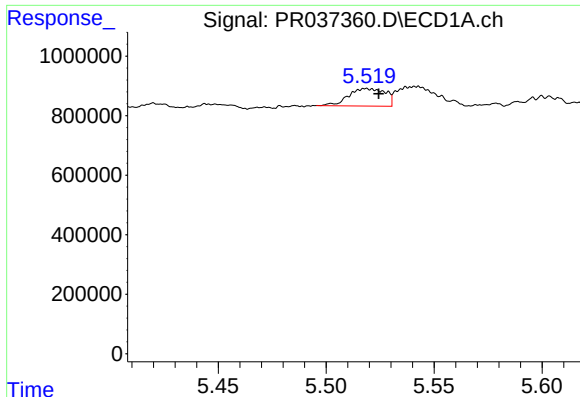

#3 AR-1016-1


R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 693178
Conc: 16.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

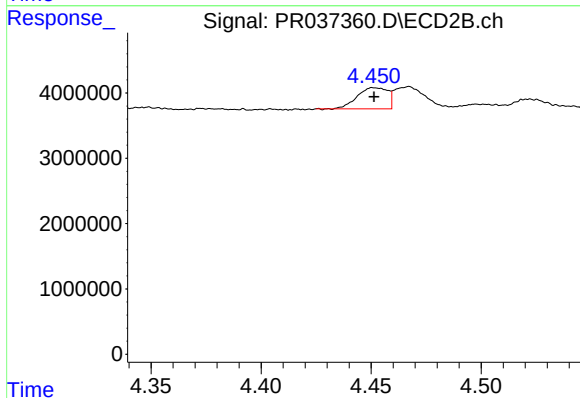


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3113686
Conc: 17.10 ng/ml

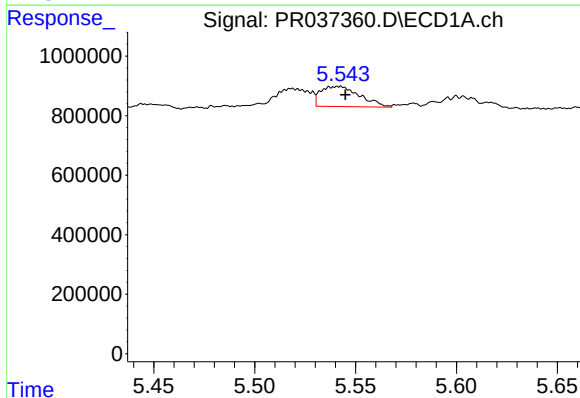


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 913087
Conc: 13.19 ng/ml

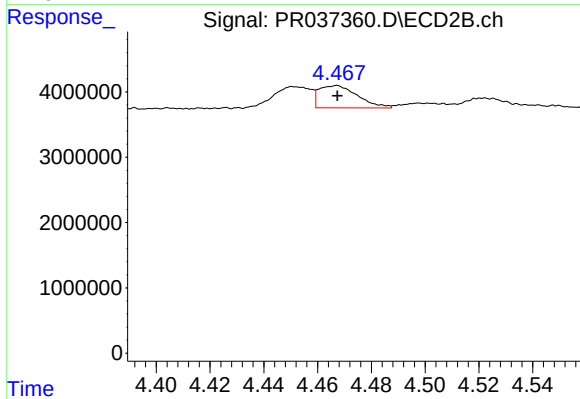

#4 AR-1016-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3422426
Conc: 12.13 ng/ml

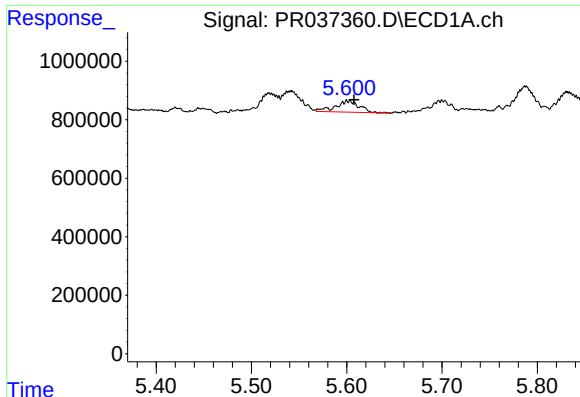

#5 AR-1016-3


R.T.: 5.601 min
Delta R.T.: -0.007 min
Response: 668371
Conc: 16.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

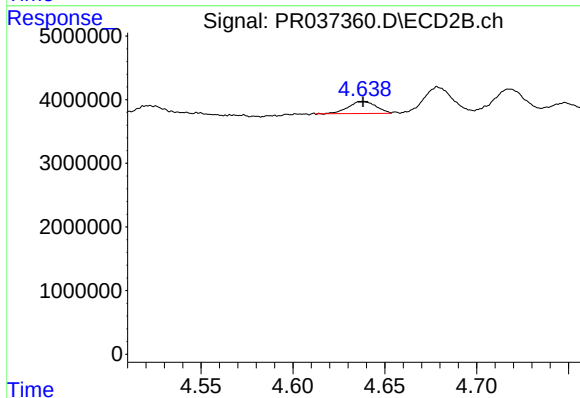


#5 AR-1016-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 2000149
Conc: 13.91 ng/ml

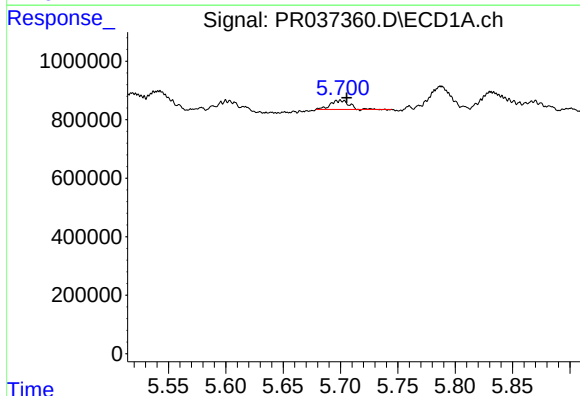


#6 AR-1016-4

R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 353775
Conc: 10.77 ng/ml

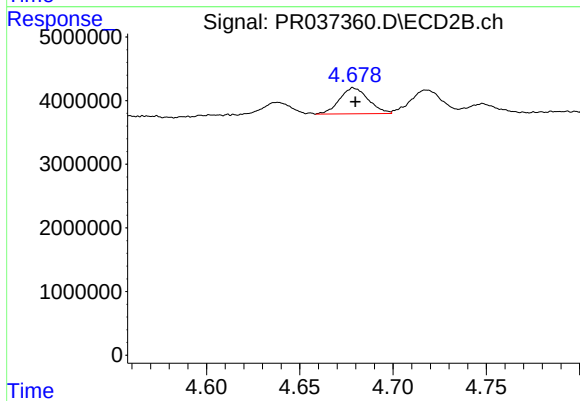

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: -0.001 min
Response: 4387847
Conc: 39.66 ng/ml

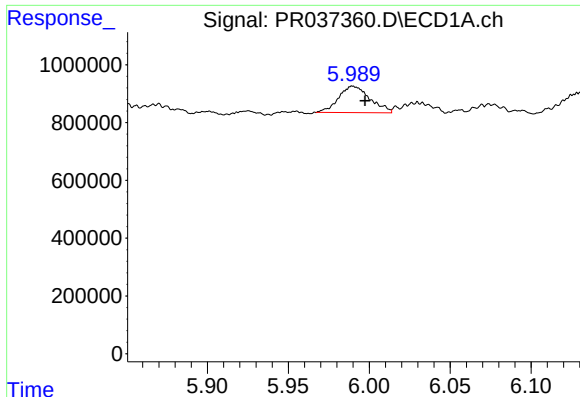

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1233520
Conc: 35.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

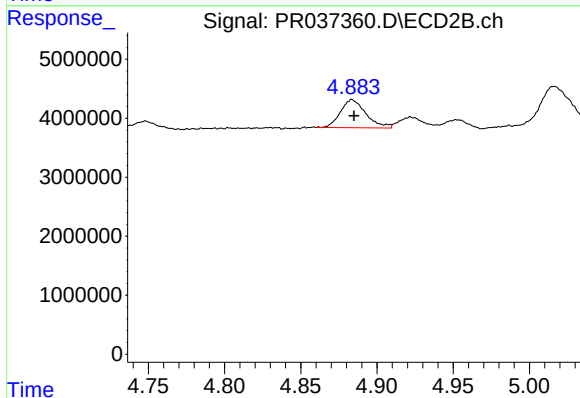


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 5534446
Conc: 36.41 ng/ml

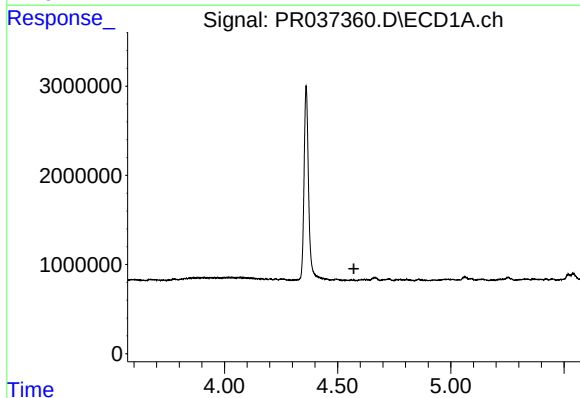


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

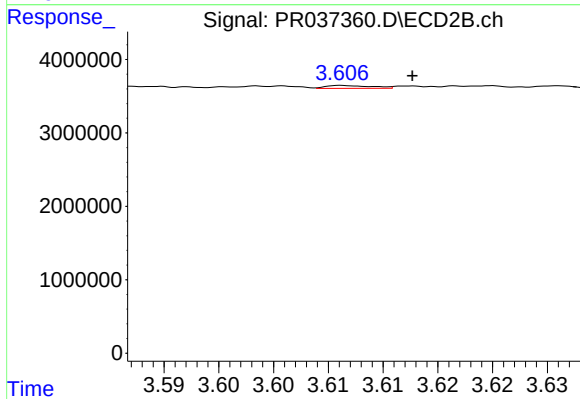

#8 AR-1221-1


R.T.: 3.607 min
Delta R.T.: -0.006 min
Response: 113259
Conc: 2.22 ng/ml

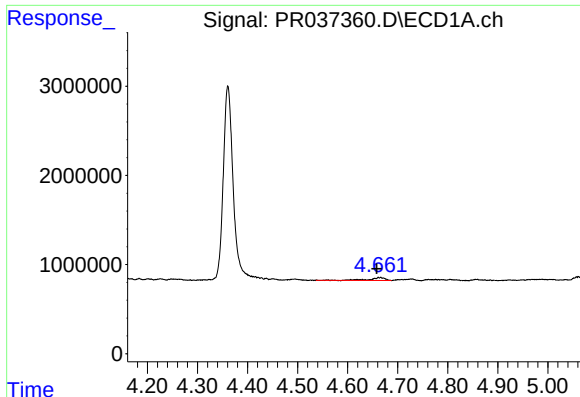

#9 AR-1221-2


R.T.: 4.665 min
Delta R.T.: 0.007 min
Response: 778272
Conc: 86.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

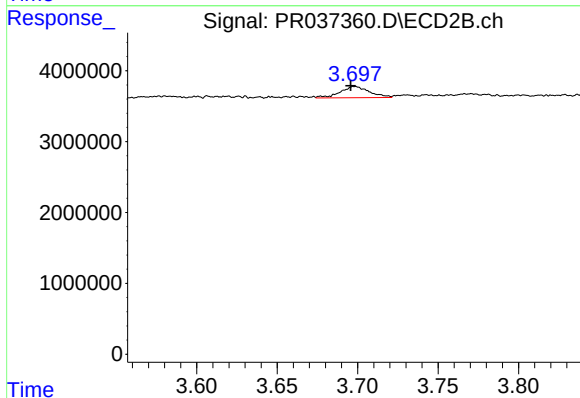


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 2021057
Conc: 54.42 ng/ml

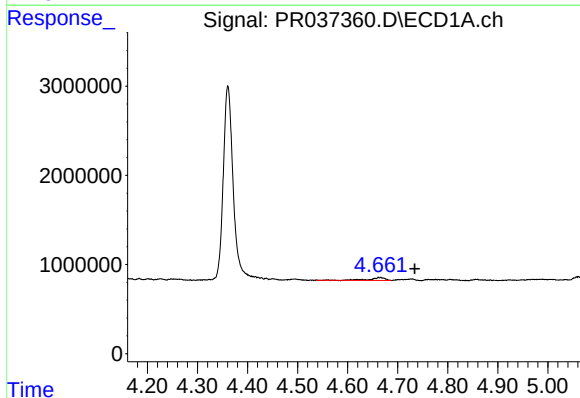


#10 AR-1221-3

R.T.: 4.665 min
Delta R.T.: -0.069 min
Response: 778272
Conc: 25.39 ng/ml

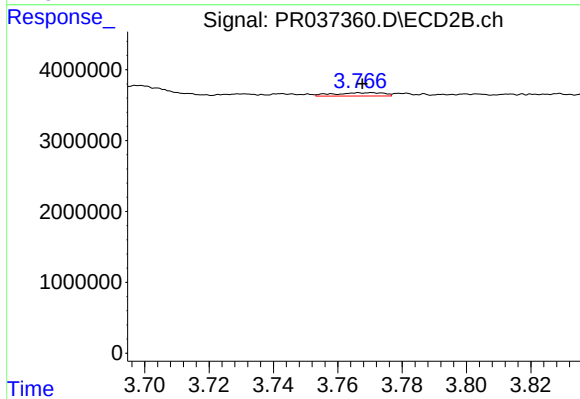

#10 AR-1221-3


R.T.: 3.771 min
Delta R.T.: 0.003 min
Response: 510274
Conc: 4.17 ng/ml

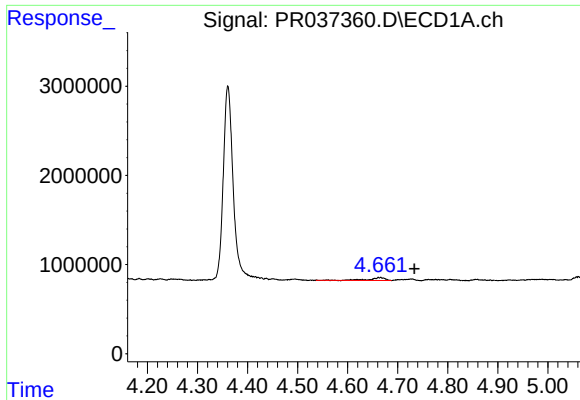

#11 AR-1232-1


R.T.: 4.665 min
Delta R.T.: -0.069 min
Response: 778272
Conc: 26.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

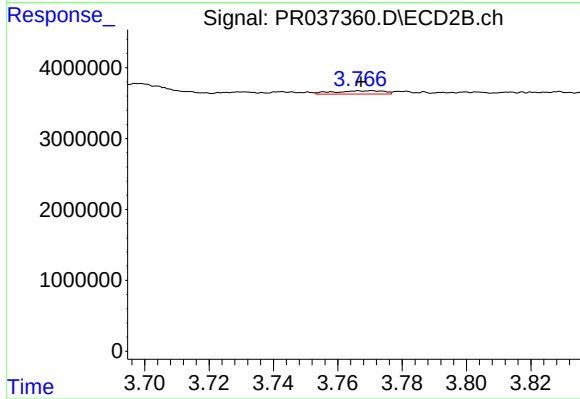


#11 AR-1232-1

R.T.: 3.771 min
Delta R.T.: 0.003 min
Response: 510274
Conc: 4.36 ng/ml

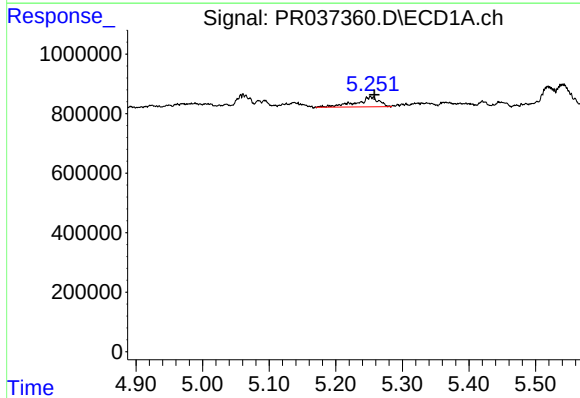


#12 AR-1232-2

R.T.: 5.253 min
Delta R.T.: -0.005 min
Response: 785817
Conc: 46.50 ng/ml

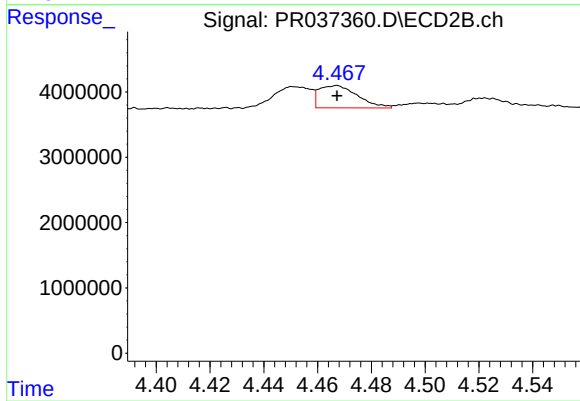

#12 AR-1232-2


R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3422426
Conc: 24.76 ng/ml

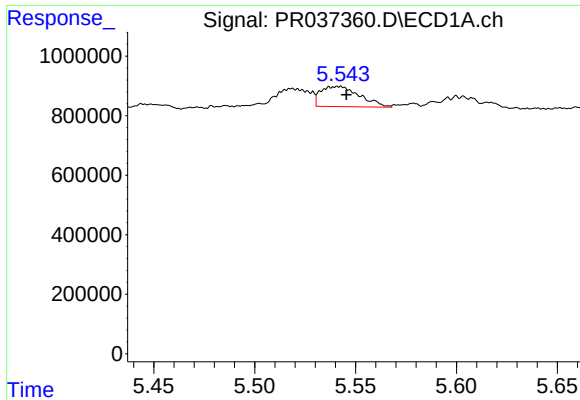

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.005 min
Response: 913087
Conc: 27.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

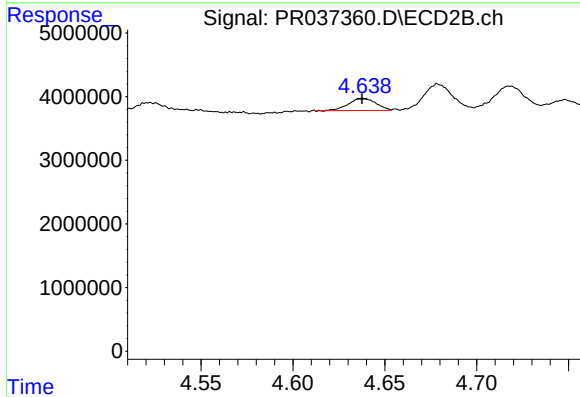


#13 AR-1232-3

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 2000149
Conc: 28.49 ng/ml

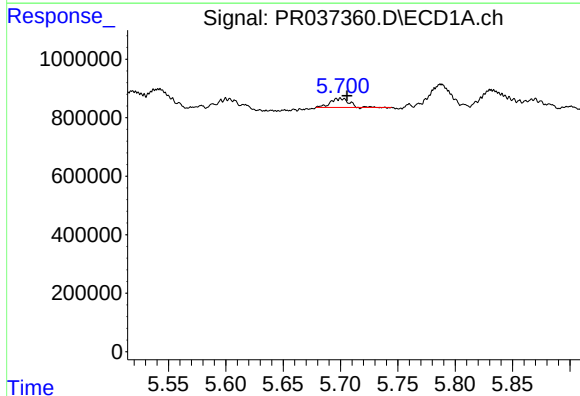


#14 AR-1232-4

R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 353775
Conc: 22.54 ng/ml

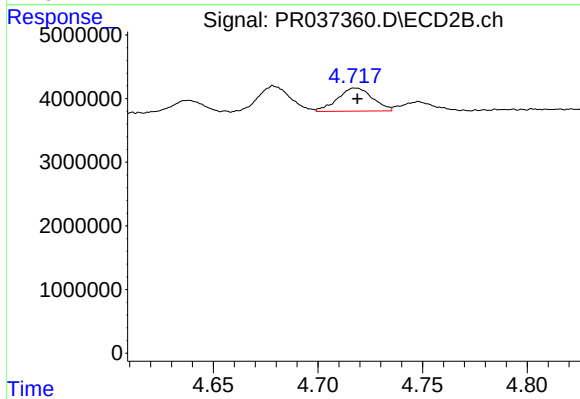

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 4208219
Conc: 70.52 ng/ml

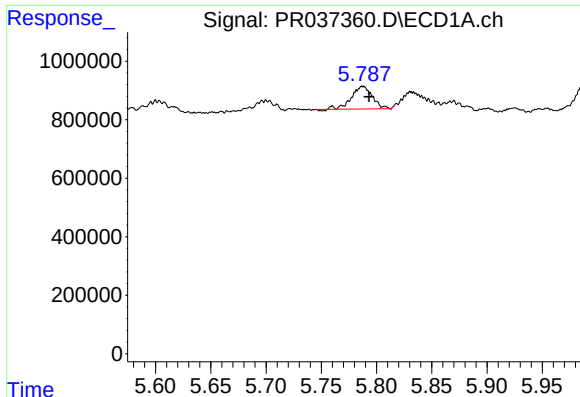

#15 AR-1232-5


R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 1010843
Conc: 86.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

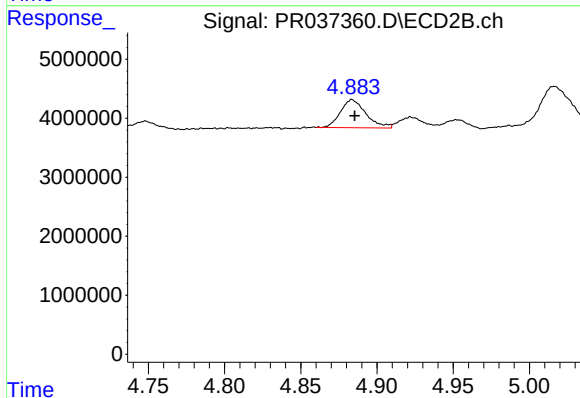


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 5534446
Conc: 81.10 ng/ml

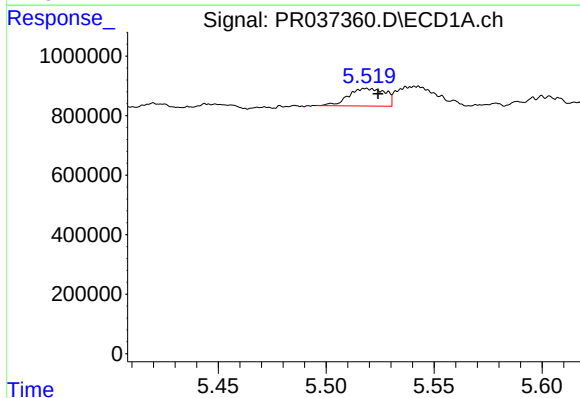


#16 AR-1242-1

R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 693178
Conc: 20.26 ng/ml

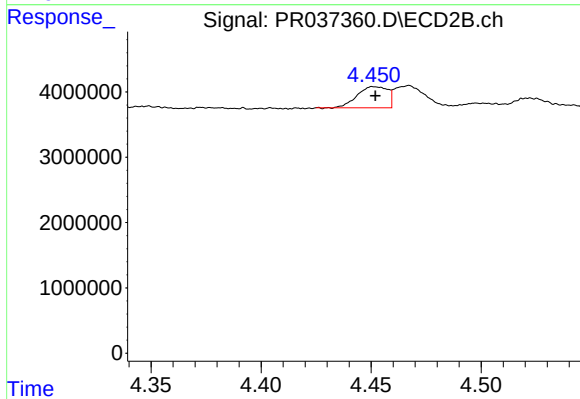

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 3113686
Conc: 21.25 ng/ml

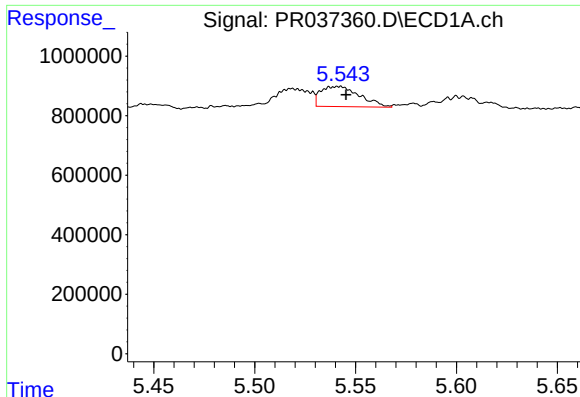

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.005 min
Response: 913087
Conc: 16.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

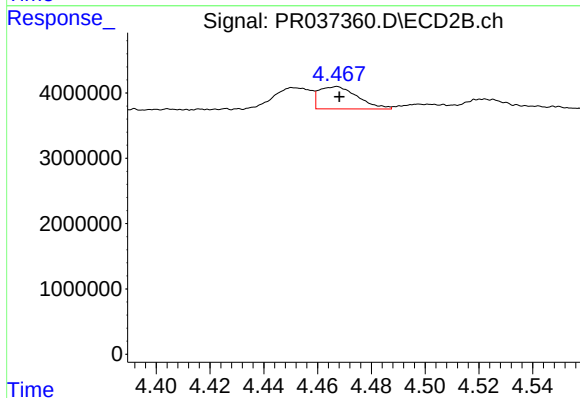


#17 AR-1242-2

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 3422426
Conc: 15.00 ng/ml

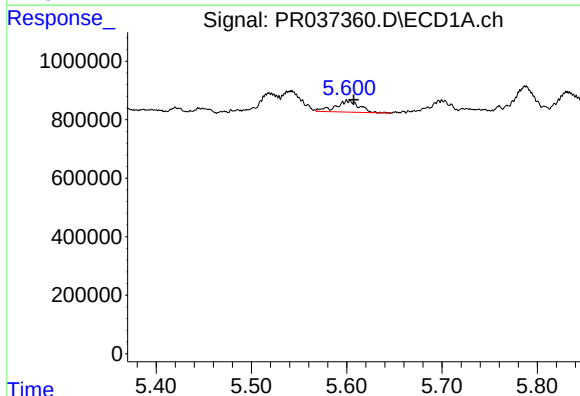


#18 AR-1242-3

R.T.: 5.601 min
Delta R.T.: -0.006 min
Response: 668371
Conc: 20.31 ng/ml

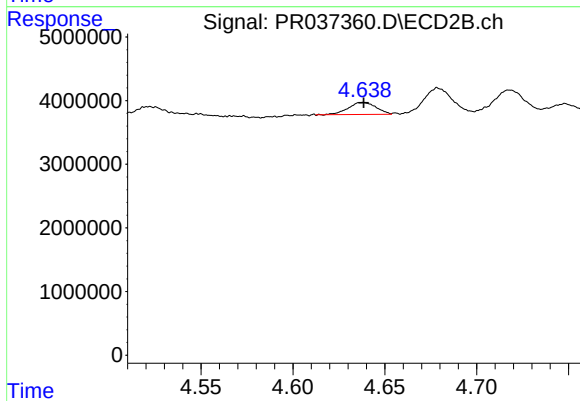

#18 AR-1242-3


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 2000149
Conc: 17.30 ng/ml

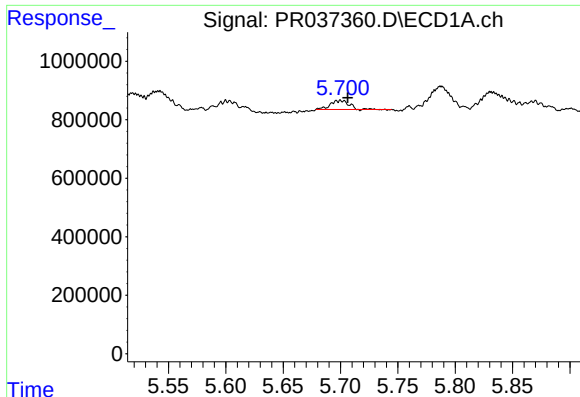

#19 AR-1242-4


R.T.: 5.700 min
Delta R.T.: -0.006 min
Response: 353775
Conc: 13.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

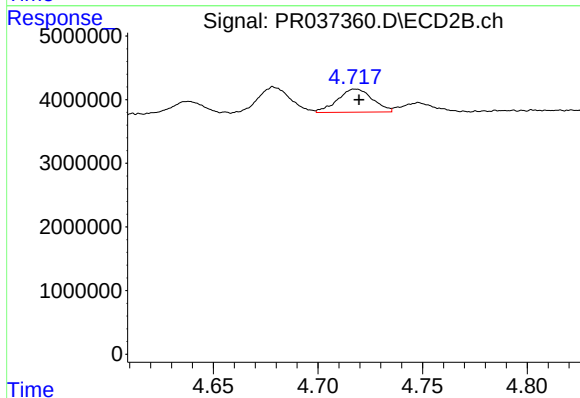


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 4208219
Conc: 38.29 ng/ml

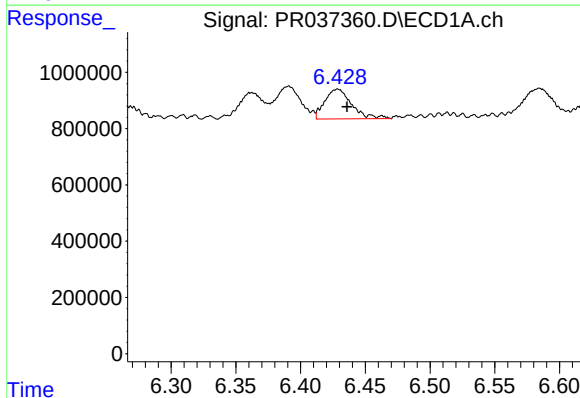


#20 AR-1242-5

R.T.: 6.428 min
Delta R.T.: -0.007 min
Response: 1520007
Conc: 47.24 ng/ml

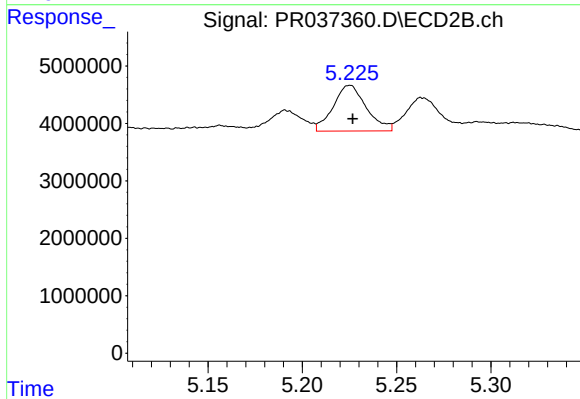

#20 AR-1242-5


R.T.: 5.225 min
Delta R.T.: -0.001 min
Response: 9736352
Conc: 58.76 ng/ml

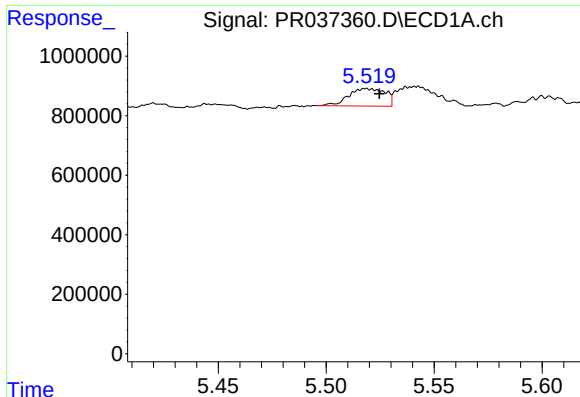

#21 AR-1248-1


R.T.: 5.519 min
Delta R.T.: -0.005 min
Response: 693178
Conc: 30.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

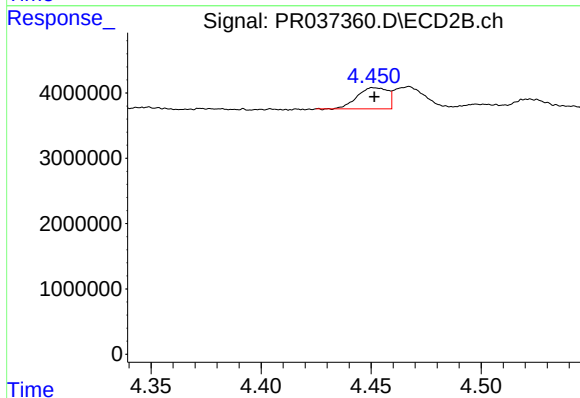


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 3113686
Conc: 30.93 ng/ml

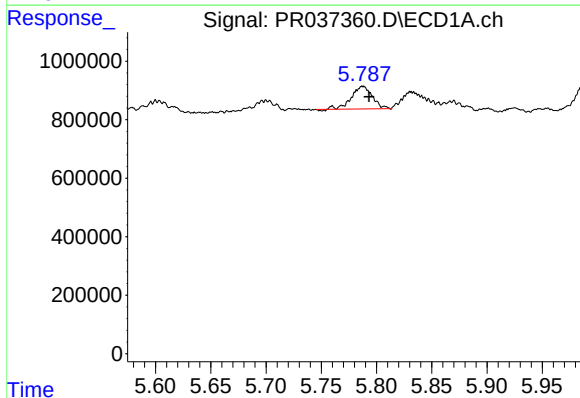


#22 AR-1248-2

R.T.: 5.787 min
Delta R.T.: -0.006 min
Response: 1010843
Conc: 28.87 ng/ml

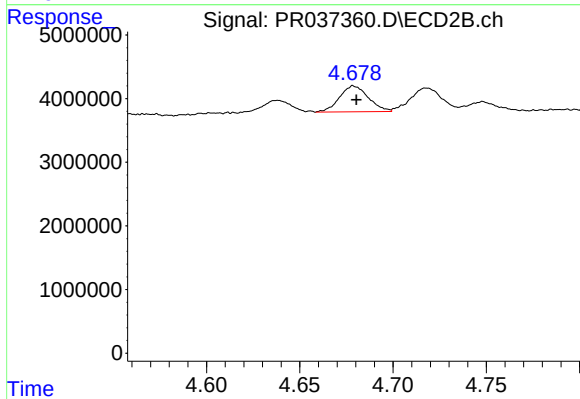

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: -0.002 min
Response: 4387847
Conc: 32.15 ng/ml

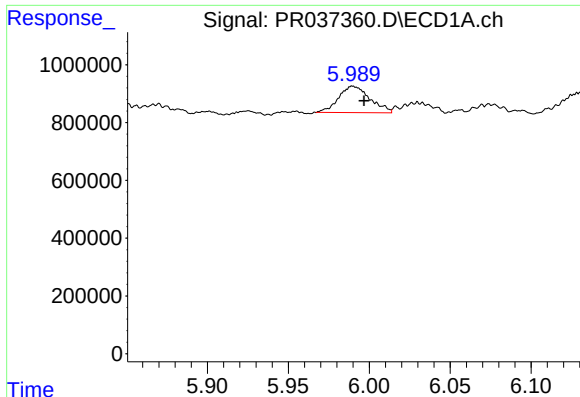

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.006 min
Response: 1233520
Conc: 30.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

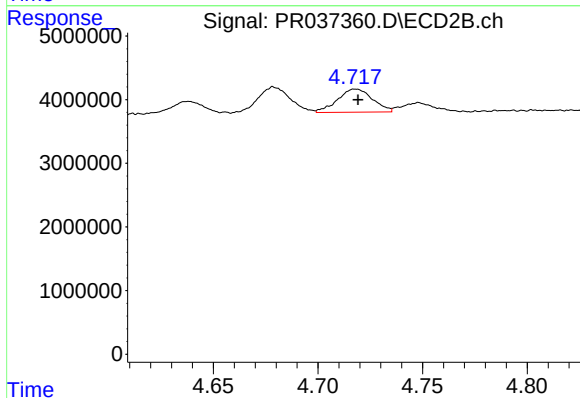


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 4208219
Conc: 30.06 ng/ml

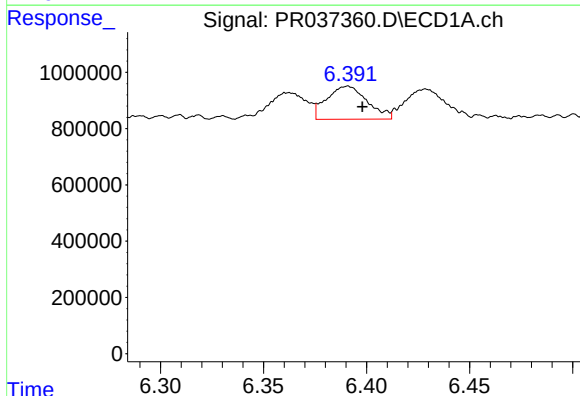


#24 AR-1248-4

R.T.: 6.390 min
Delta R.T.: -0.007 min
Response: 1604155
Conc: 32.77 ng/ml

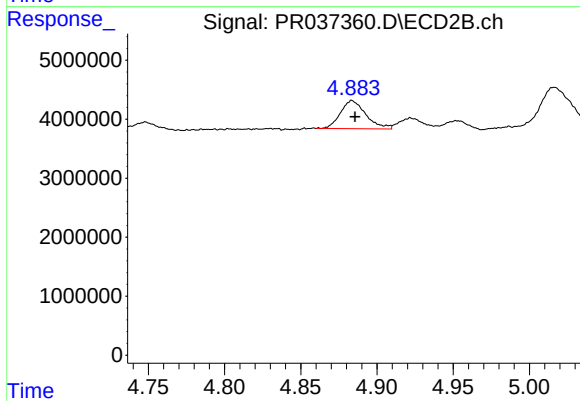

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 5534446
Conc: 31.10 ng/ml

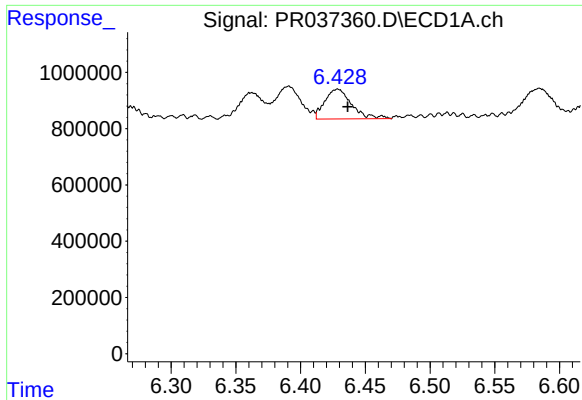

#25 AR-1248-5


R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 1520007
Conc: 32.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

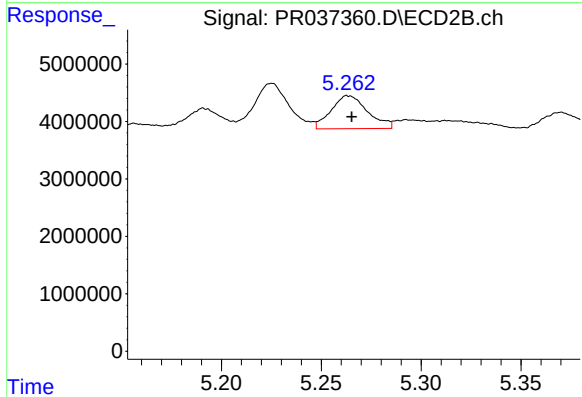


#25 AR-1248-5

R.T.: 5.263 min
Delta R.T.: -0.002 min
Response: 7315356
Conc: 37.40 ng/ml

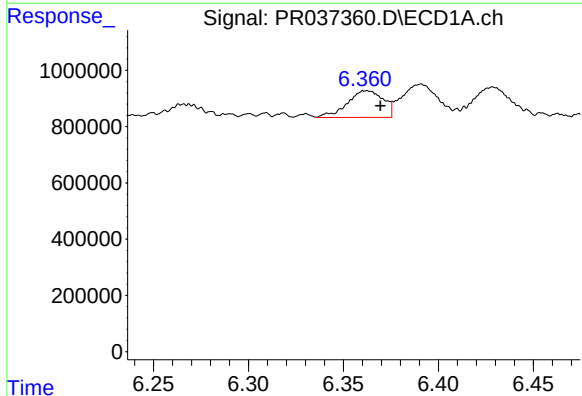


#26 AR-1254-1

R.T.: 6.362 min
Delta R.T.: -0.007 min
Response: 1248896
Conc: 22.86 ng/ml

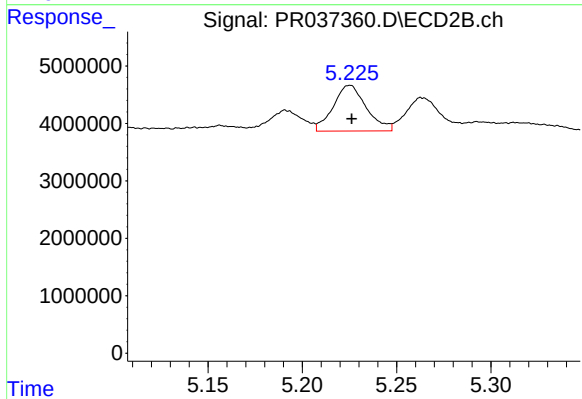

#26 AR-1254-1


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 9736352
Conc: 28.26 ng/ml

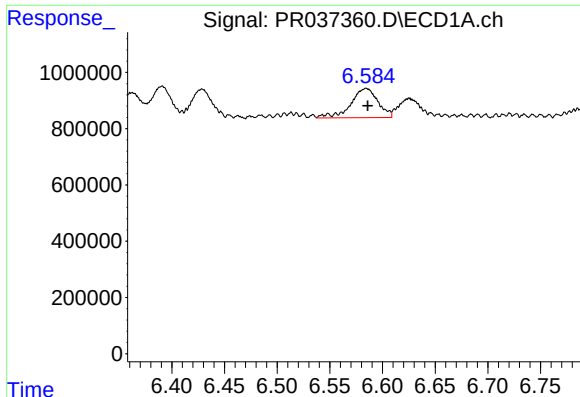

#27 AR-1254-2


R.T.: 6.584 min
Delta R.T.: -0.002 min
Response: 1863161
Conc: 21.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

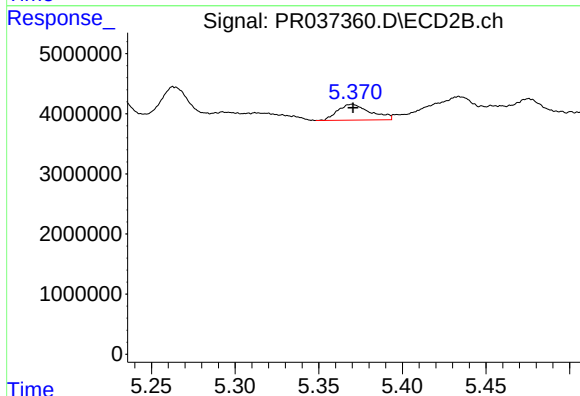


#27 AR-1254-2

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 3573575
Conc: 11.93 ng/ml

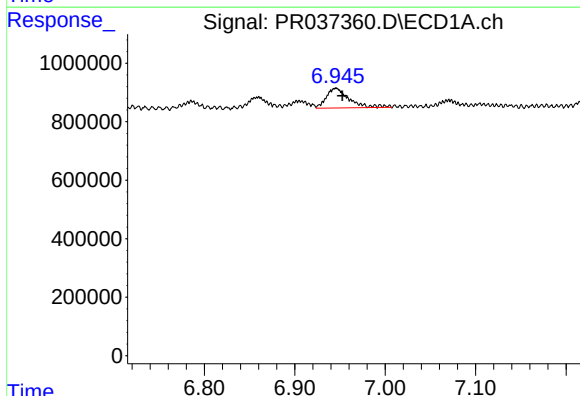


#28 AR-1254-3

R.T.: 6.945 min
Delta R.T.: -0.007 min
Response: 1174312
Conc: 12.91 ng/ml

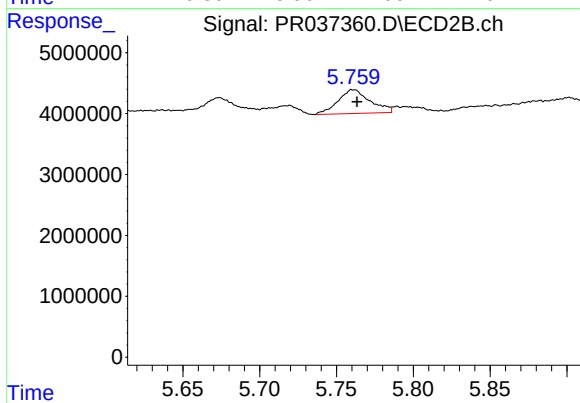

#28 AR-1254-3


R.T.: 5.760 min
Delta R.T.: -0.003 min
Response: 5710042
Conc: 12.06 ng/ml

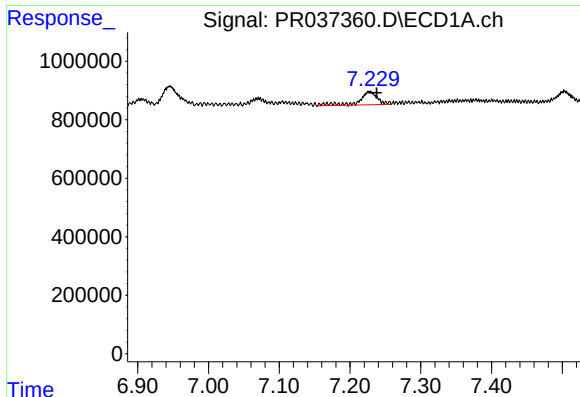

#29 AR-1254-4


R.T.: 7.228 min
Delta R.T.: -0.010 min
Response: 780516
Conc: 11.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

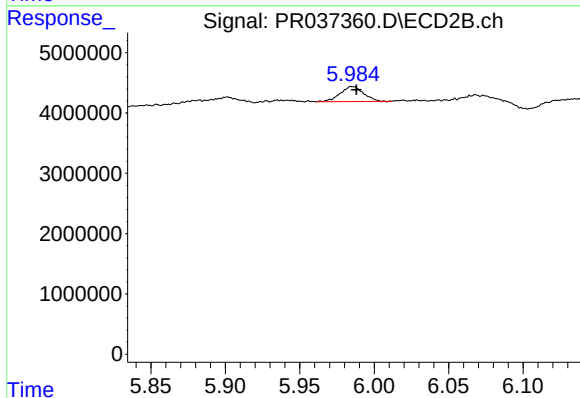


#29 AR-1254-4

R.T.: 5.985 min
Delta R.T.: -0.003 min
Response: 2754011
Conc: 7.85 ng/ml

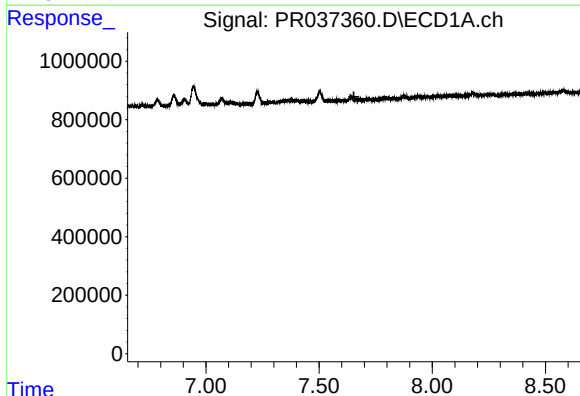


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

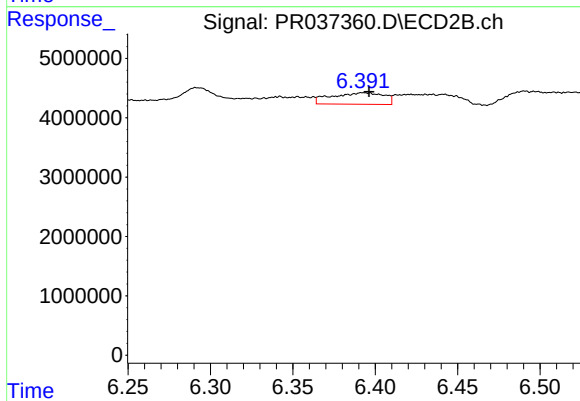

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 4310049
Conc: 9.73 ng/ml

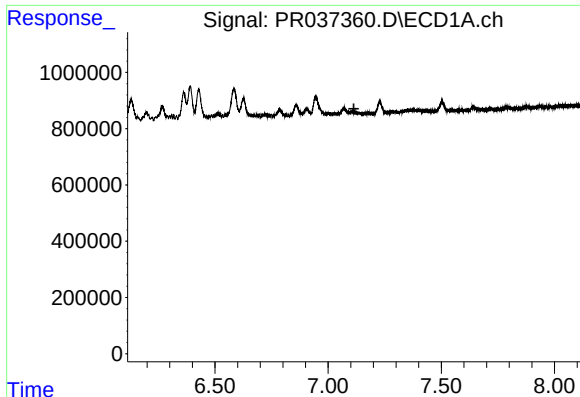

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

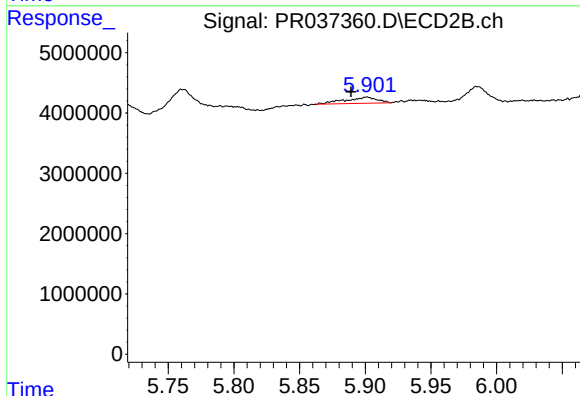


#31 AR-1260-1

R.T.: 5.902 min
Delta R.T.: 0.012 min
Response: 1735431
Conc: 5.94 ng/ml

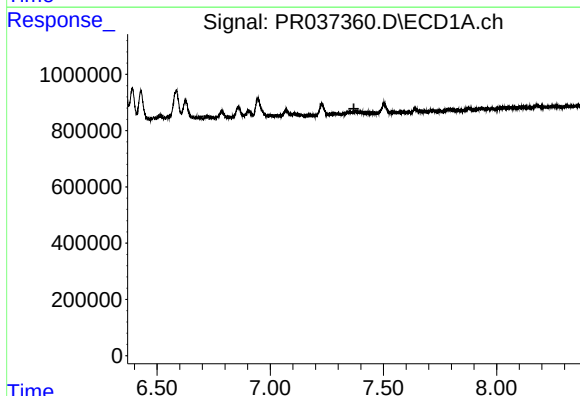


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

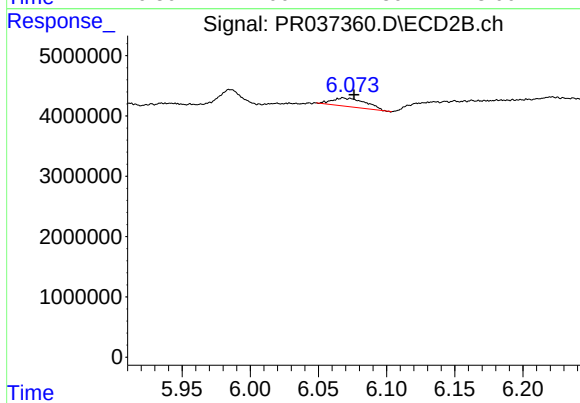

#32 AR-1260-2


R.T.: 6.068 min
Delta R.T.: -0.008 min
Response: 2375904
Conc: 5.16 ng/ml

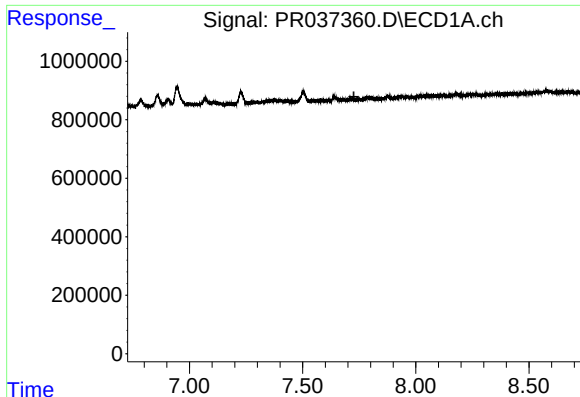

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

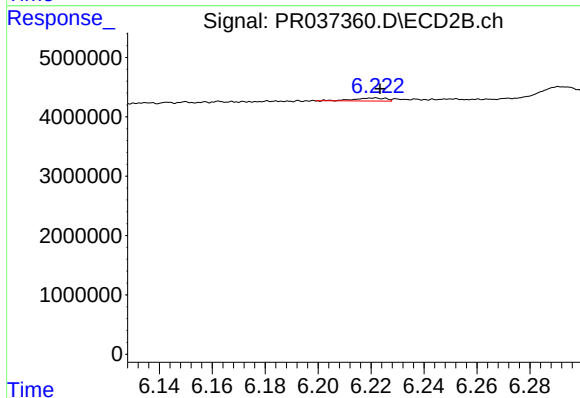


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 414764
Conc: 1.16 ng/ml

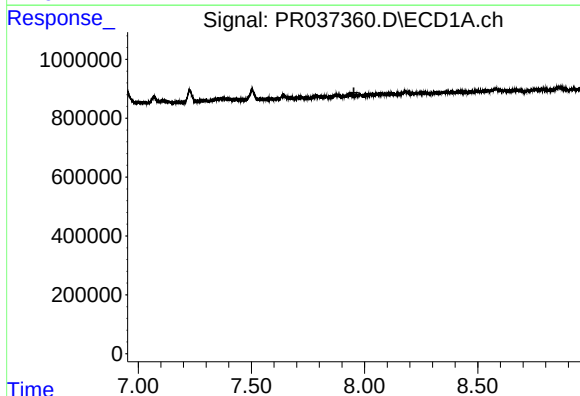


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

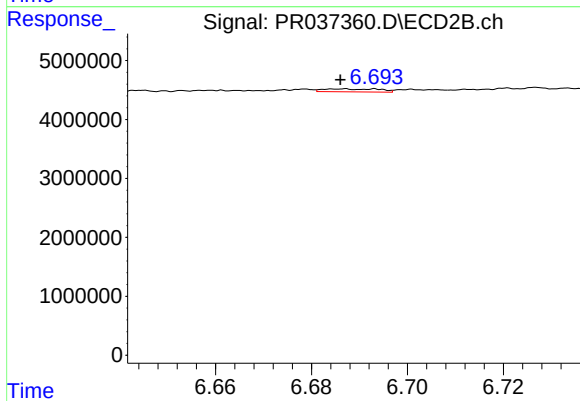

#34 AR-1260-4


R.T.: 6.687 min
Delta R.T.: 0.001 min
Response: 415981
Conc: 1.36 ng/ml

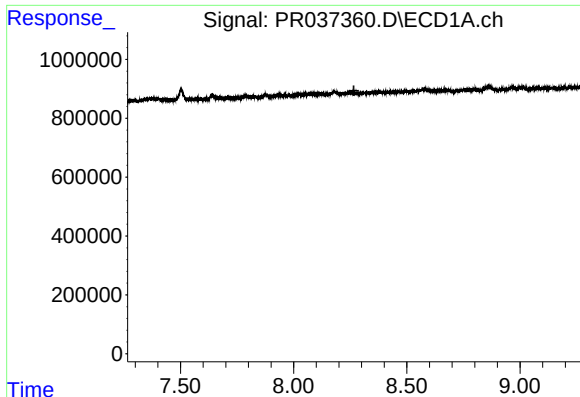

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

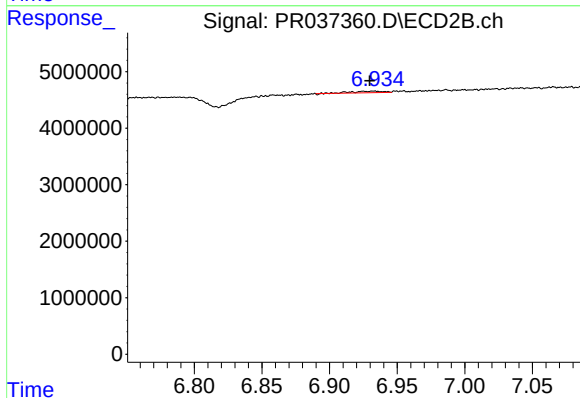


#35 AR-1260-5

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 433241
Conc: 0.50 ng/ml

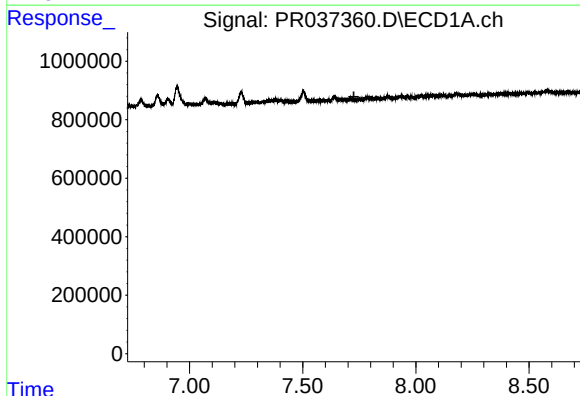


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

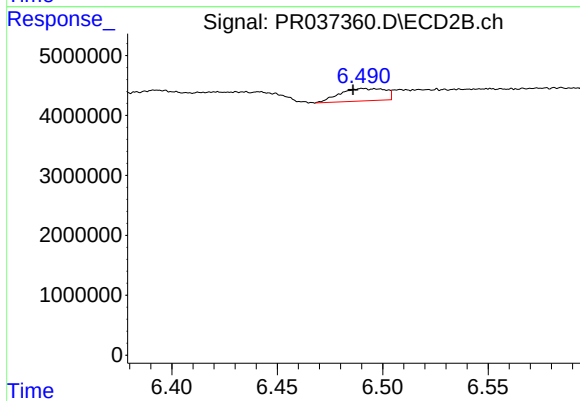

#36 AR-1262-1


R.T.: 6.490 min
Delta R.T.: 0.004 min
Response: 3104403
Conc: 12.39 ng/ml

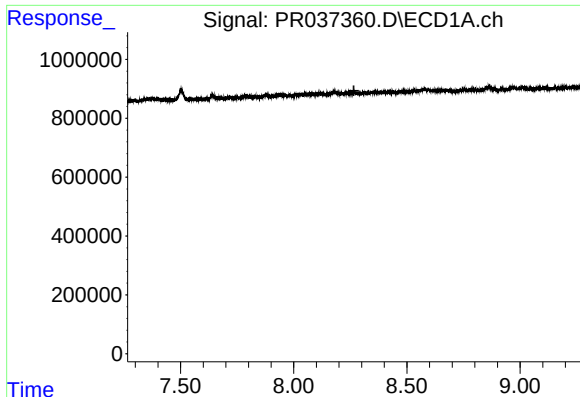

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

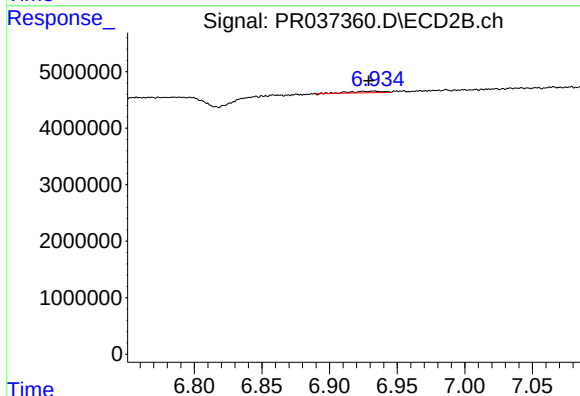


#37 AR-1262-2

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 433241
Conc: 0.34 ng/ml

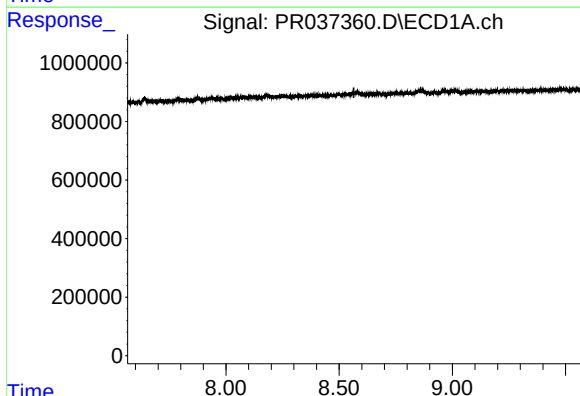


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

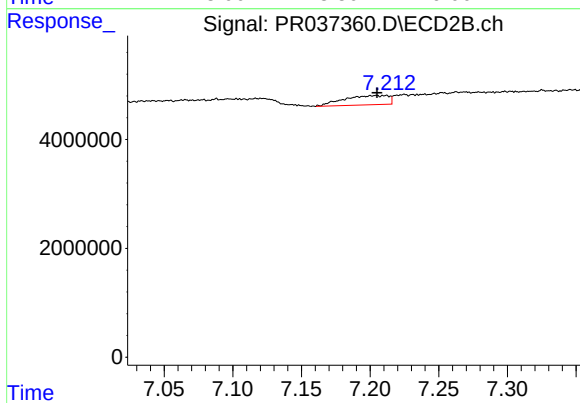

#38 AR-1262-3


R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 3831310
Conc: 6.99 ng/ml

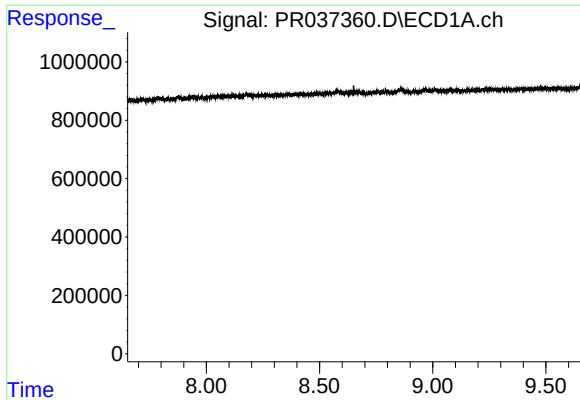

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

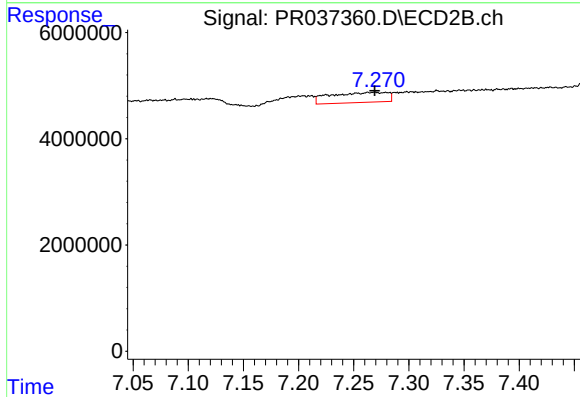


#39 AR-1262-4

R.T.: 7.279 min
Delta R.T.: 0.010 min
Response: 6826928
Conc: 7.61 ng/ml

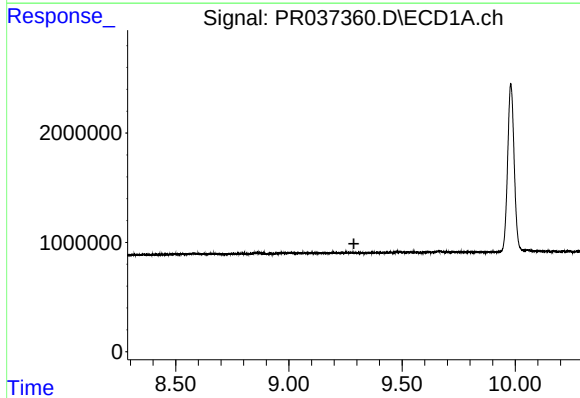


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

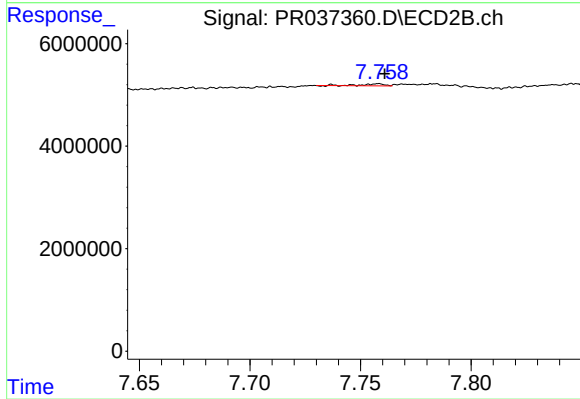

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 253420
Conc: 0.66 ng/ml

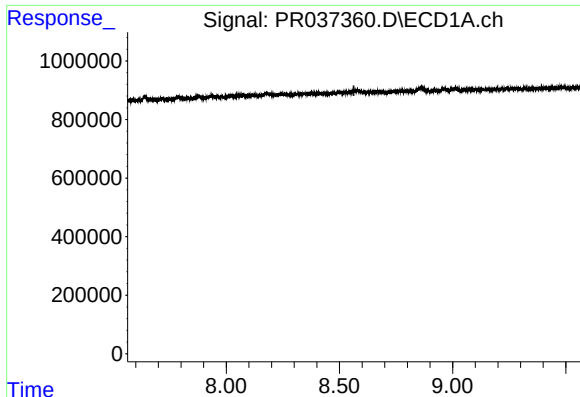

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

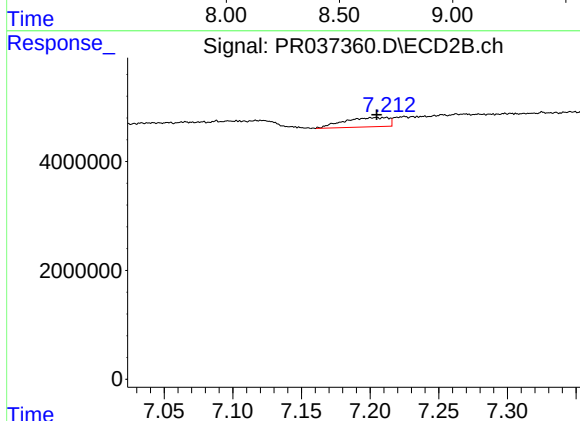


#41 AR-1268-1

R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 3831310
Conc: 3.11 ng/ml

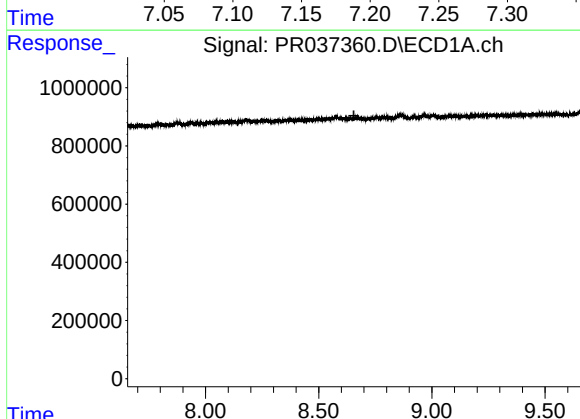


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

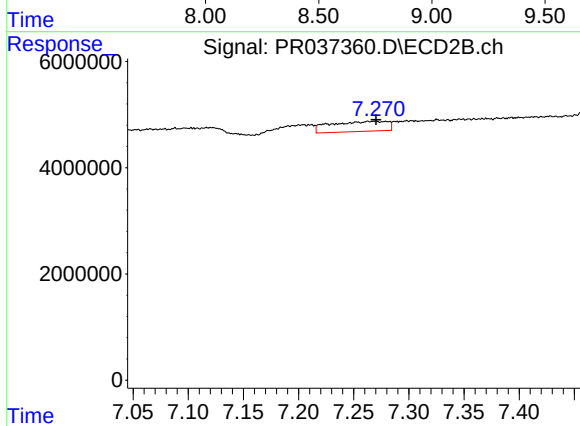

#42 AR-1268-2


R.T.: 7.279 min
Delta R.T.: 0.009 min
Response: 6826928
Conc: 6.45 ng/ml

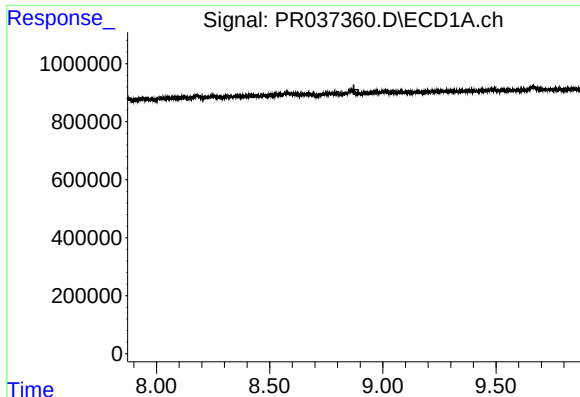

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

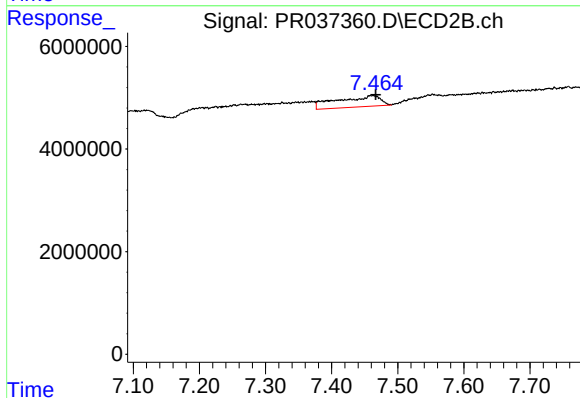


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.004 min
Response: 9776303
Conc: 11.03 ng/ml

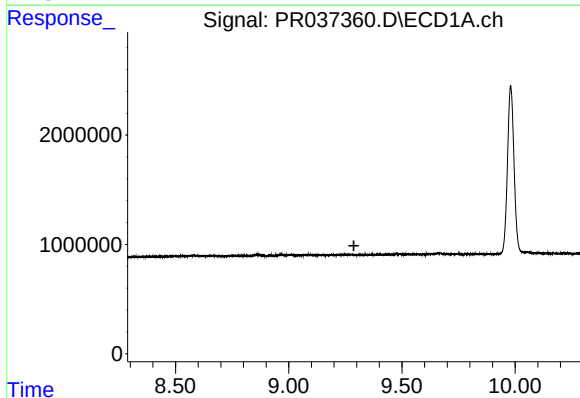


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

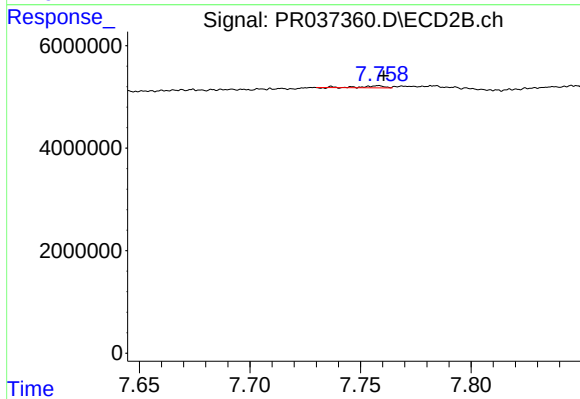

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 253420
Conc: 0.70 ng/ml

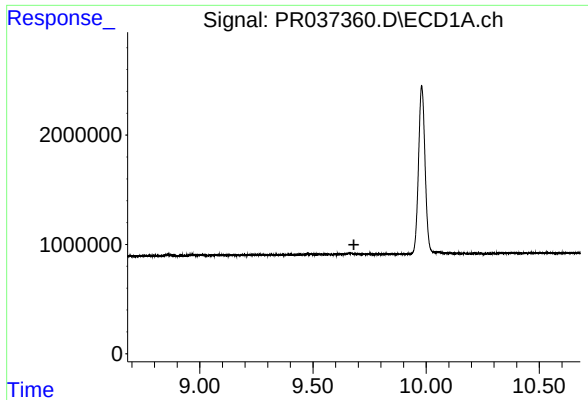

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

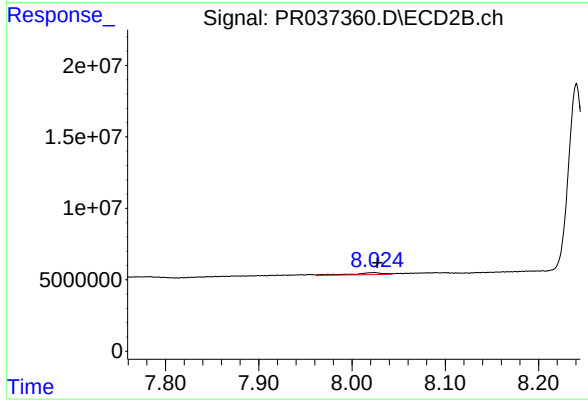

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.003 min
Response: 3127704
Conc: 1.23 ng/ml