

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 17:35
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1248 LOD 40PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:04:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	24731753	101.2E6	19.770	21.095
2)	SA Decachlor...	9.982	8.241	25923198	133.7E6	19.600	22.963
Target Compounds							
3)	L1 AR-1016-1	5.518	4.451	974809	4777060	22.623	26.236
4)	L1 AR-1016-2	5.541	4.466	1411494	5618418	20.383	19.915
5)	L1 AR-1016-3	5.601	4.639	614812	3170676	15.245	22.052 #
6)	L1 AR-1016-4	5.699	4.678	729474	6537367	22.213	59.089 #
7)	L1 AR-1016-5	5.990	4.885	1810175	8119530	52.790	53.415
8)	L2 AR-1221-1	0.000	3.616	0	460844	N.D.	9.051 #
9)	L2 AR-1221-2	4.662	3.699	480969	1865424	53.181	50.233
10)	L2 AR-1221-3	0.000	3.769	0	546155	N.D.	4.460 #
11)	L3 AR-1232-1	0.000	3.769	0	546155	N.D.	4.668 #
12)	L3 AR-1232-2	5.253	4.466	1022885	5618418	60.535	40.647 #
13)	L3 AR-1232-3	5.541	4.639	1411494	3170676	41.755	45.165
14)	L3 AR-1232-4	5.699	4.718	729474	6354596	46.473	106.492 #
15)	L3 AR-1232-5	5.787	4.885	1668838	8119530	142.689	118.978
16)	L4 AR-1242-1	5.518	4.451	974809	4777060	28.491	32.599
17)	L4 AR-1242-2	5.541	4.466	1411494	5618418	25.446	24.625
18)	L4 AR-1242-3	5.601	4.639	614812	3170676	18.679	27.421 #
19)	L4 AR-1242-4	5.699	4.718	729474	6354596	27.655	57.816 #
20)	L4 AR-1242-5	6.428	5.225	2244948	13515538	69.765	81.567
21)	L5 AR-1248-1	5.518	4.451	974809	4777060	42.554	47.456
22)	L5 AR-1248-2	5.787	4.678	1668838	6537367	47.661	47.902
23)	L5 AR-1248-3	5.990	4.718	1810175	6354596	44.248	45.399
24)	L5 AR-1248-4	6.390	4.885	2307292	8119530	47.132	45.624
25)	L5 AR-1248-5	6.428	5.264	2244948	10056868	47.525	51.412
26)	L6 AR-1254-1	6.362	5.225	1752302	13515538	32.075	39.235
27)	L6 AR-1254-2	6.583	5.369	2379769	4753546	27.769	15.871 #
28)	L6 AR-1254-3	6.944	5.761	1744029	7864038	19.173	16.604
29)	L6 AR-1254-4	7.227	5.984	994645	4164103	14.844	11.876
30)	L6 AR-1254-5	0.000	6.394	0	3942053	N.D.	8.902 #
31)	L7 AR-1260-1	7.070	5.885	897197	709628	13.597	2.428 #
32)	L7 AR-1260-2	0.000	6.069	0	2211996	N.D.	4.803 #
33)	L7 AR-1260-3	0.000	6.219	0	996974	N.D.	2.797 #
34)	L7 AR-1260-4	0.000	6.684	0	284542	N.D.	0.934 #
35)	L7 AR-1260-5	0.000	6.926	0	623437	N.D.	0.719 #
36)	L8 AR-1262-1	0.000	6.490	0	1626433	N.D.	6.490 #
37)	L8 AR-1262-2	0.000	6.926	0	623437	N.D.	0.496 #
38)	L8 AR-1262-3	0.000	7.207	0	320435	N.D.	0.584 #
39)	L8 AR-1262-4	0.000	7.263	0	4775494	N.D.	5.320 #
40)	L8 AR-1262-5	0.000	7.753	0	32045	N.D.	0.084 #
41)	L9 AR-1268-1	0.000	7.207	0	320435	N.D.	0.260 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 17:35
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1248 LOD 40PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:04:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.263	0	4775494	N.D.	4.510 #
43) L9	AR-1268-3	0.000	7.460	0	8213347	N.D.	9.268 #
44) L9	AR-1268-4	0.000	7.753	0	32045	N.D.	0.088 #
45) L9	AR-1268-5	0.000	8.022	0	5872201	N.D.	2.308 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 17:35
Operator : SM\SJ
Sample : K2241-07
Misc : AR1248 LOD 40PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:04:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

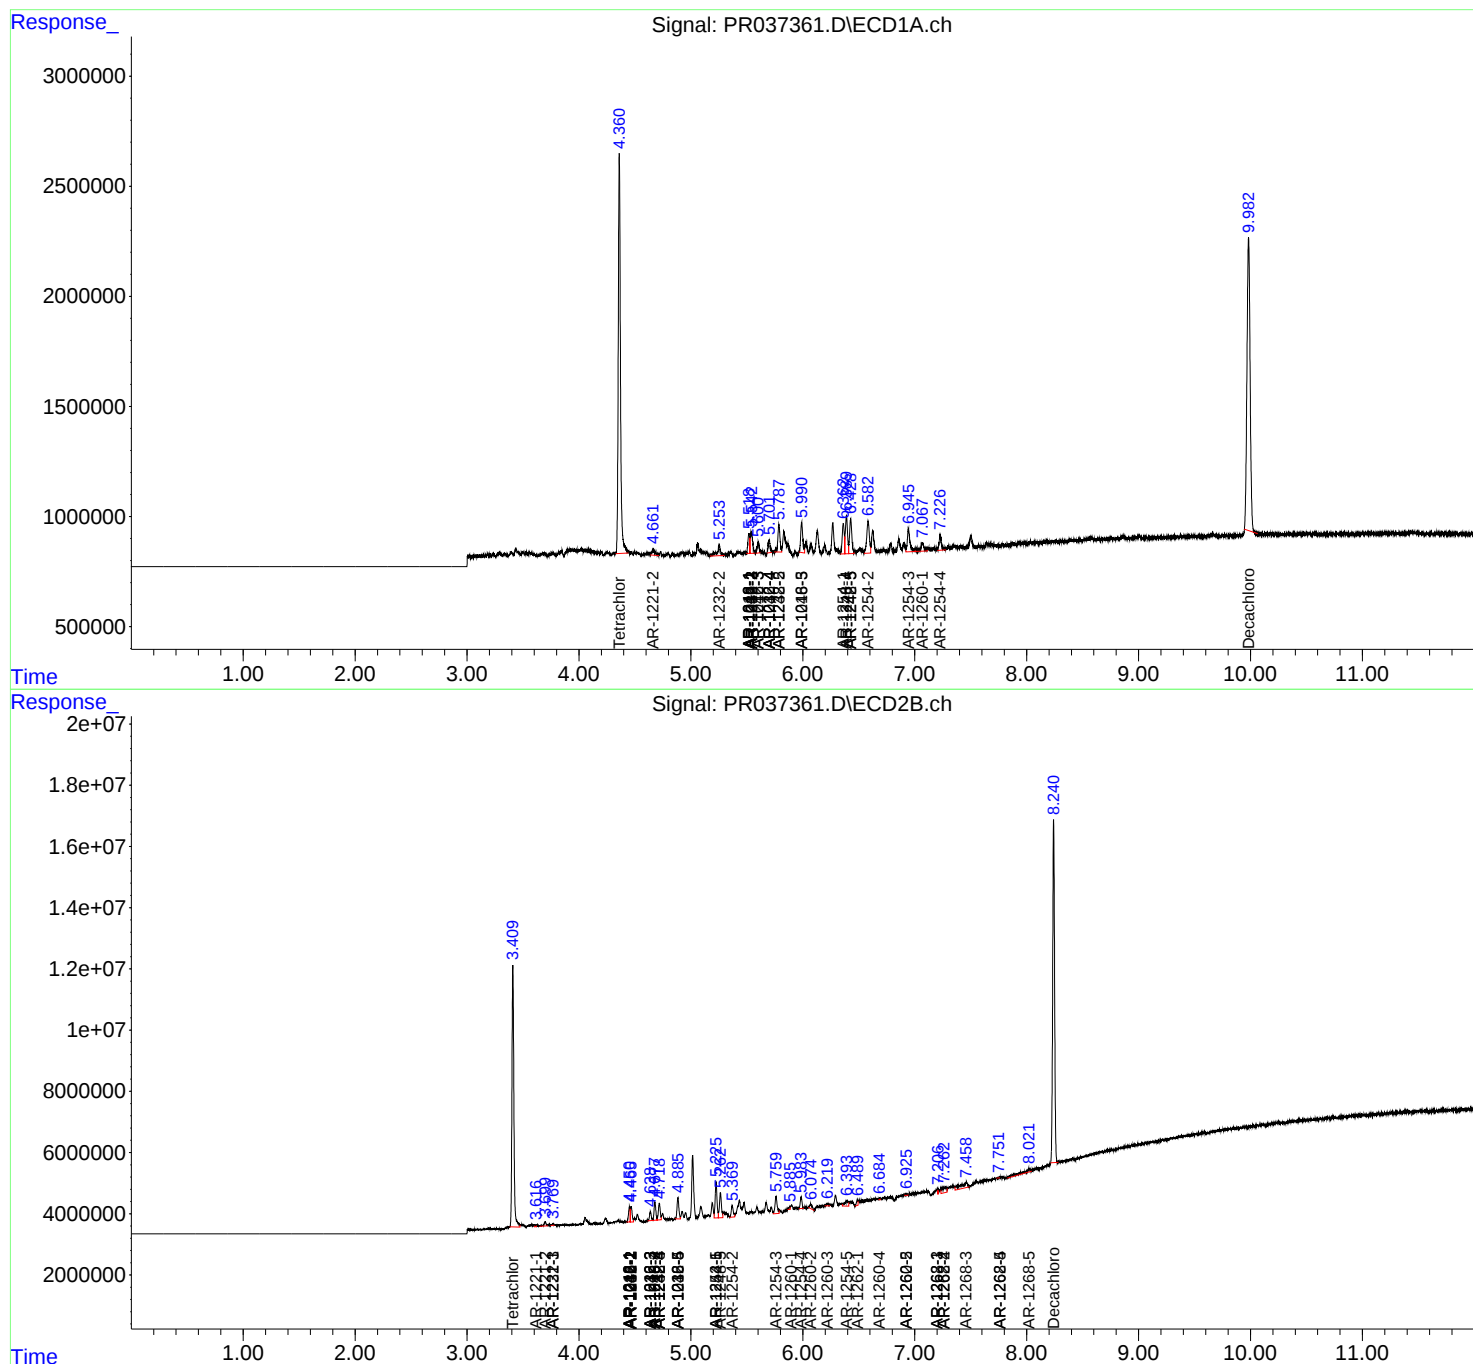


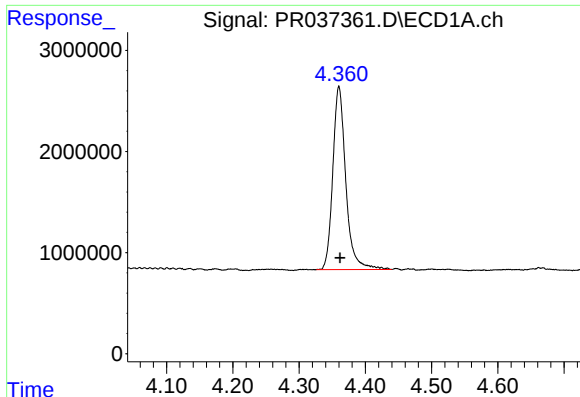

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 24731753
Conc: 19.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

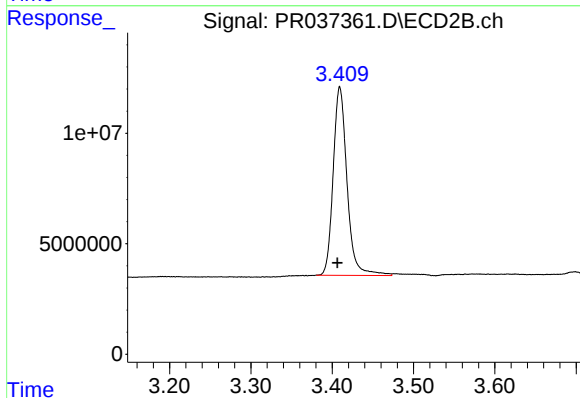


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.003 min
Response: 101162717
Conc: 21.10 ng/ml

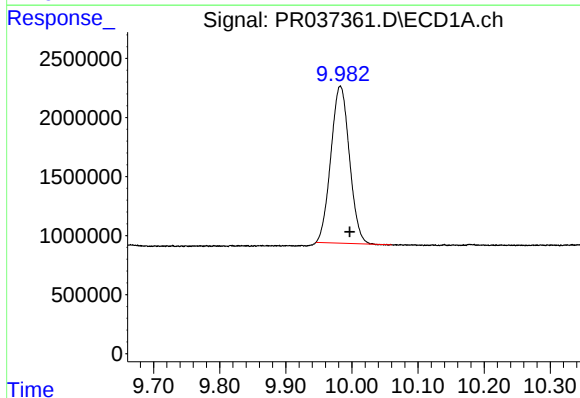


#2 Decachlorobiphenyl

R.T.: 9.982 min
Delta R.T.: -0.014 min
Response: 25923198
Conc: 19.60 ng/ml

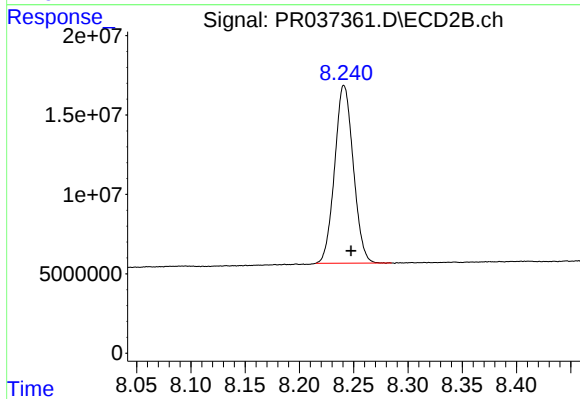

#2 Decachlorobiphenyl


R.T.: 8.241 min
Delta R.T.: -0.006 min
Response: 133740311
Conc: 22.96 ng/ml

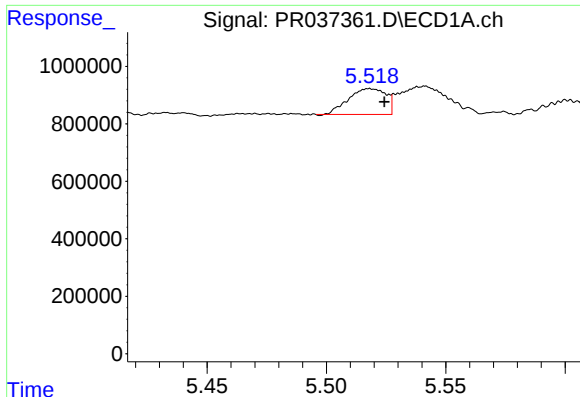

#3 AR-1016-1


R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 974809
Conc: 22.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

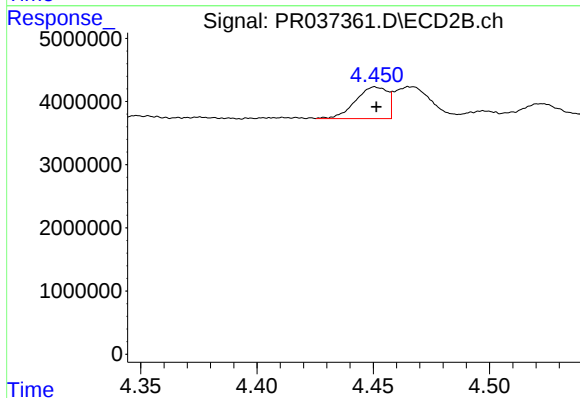


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 4777060
Conc: 26.24 ng/ml

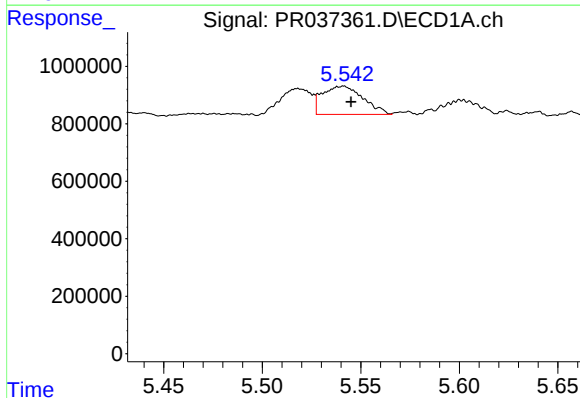


#4 AR-1016-2

R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 1411494
Conc: 20.38 ng/ml

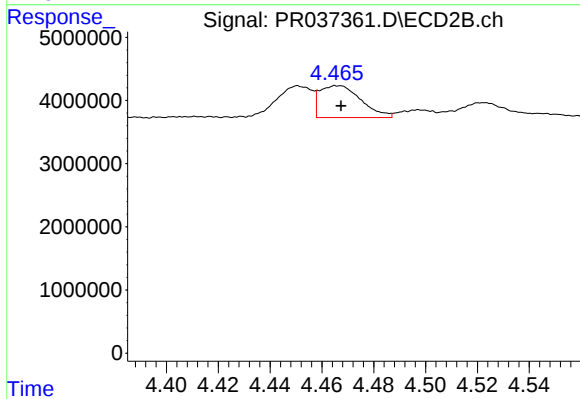

#4 AR-1016-2


R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 5618418
Conc: 19.91 ng/ml

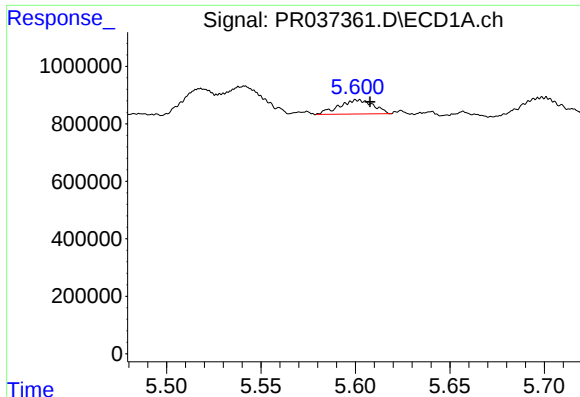

#5 AR-1016-3


R.T.: 5.601 min
Delta R.T.: -0.006 min
Response: 614812
Conc: 15.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

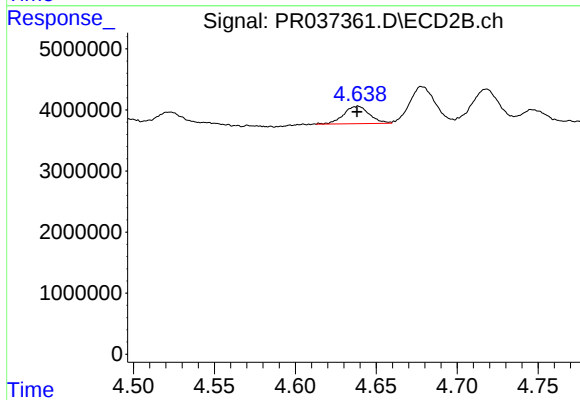


#5 AR-1016-3

R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 3170676
Conc: 22.05 ng/ml

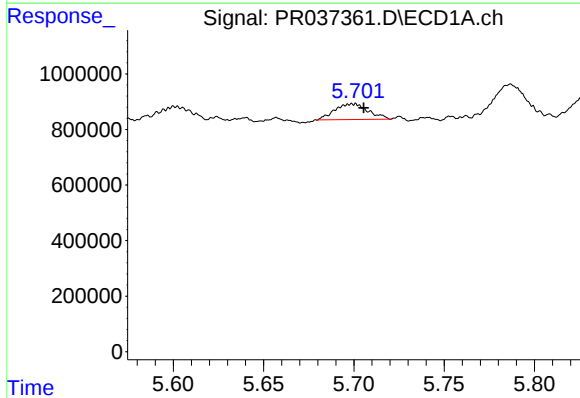


#6 AR-1016-4

R.T.: 5.699 min
Delta R.T.: -0.006 min
Response: 729474
Conc: 22.21 ng/ml

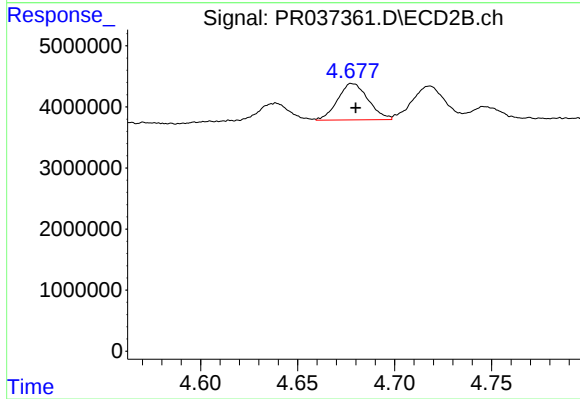

#6 AR-1016-4


R.T.: 4.678 min
Delta R.T.: -0.002 min
Response: 6537367
Conc: 59.09 ng/ml

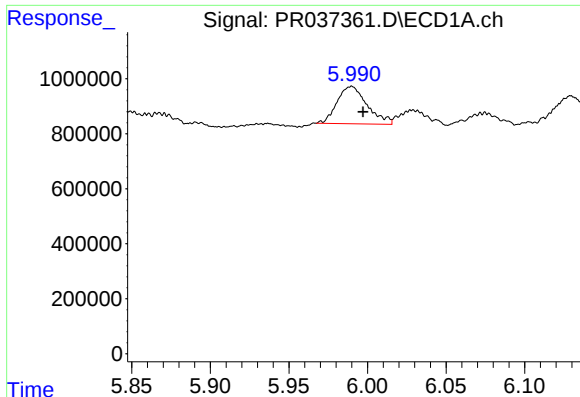

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1810175
Conc: 52.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

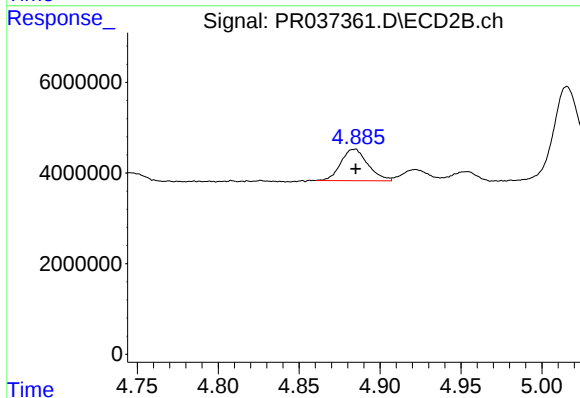


#7 AR-1016-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 8119530
Conc: 53.41 ng/ml

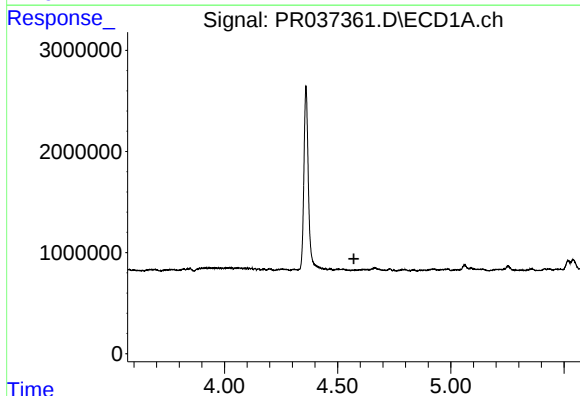


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

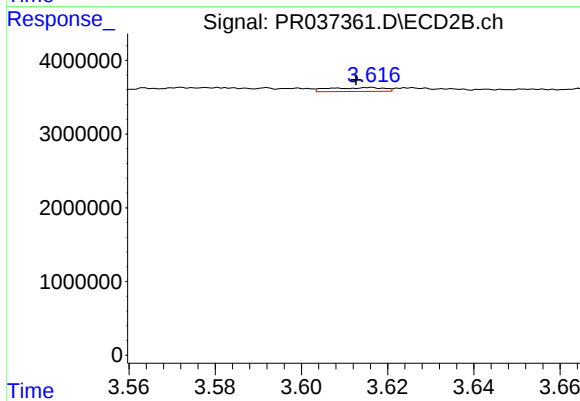

#8 AR-1221-1


R.T.: 3.616 min
Delta R.T.: 0.003 min
Response: 460844
Conc: 9.05 ng/ml

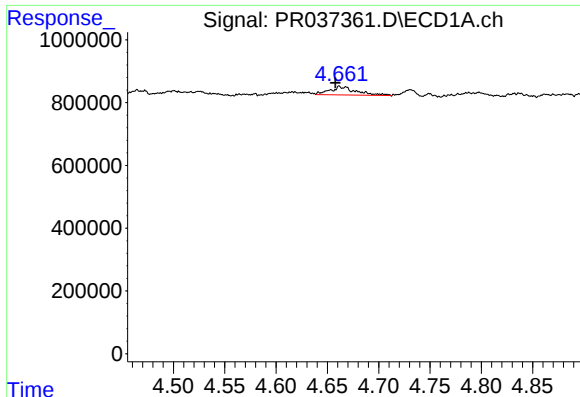

#9 AR-1221-2


R.T.: 4.662 min
Delta R.T.: 0.004 min
Response: 480969
Conc: 53.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

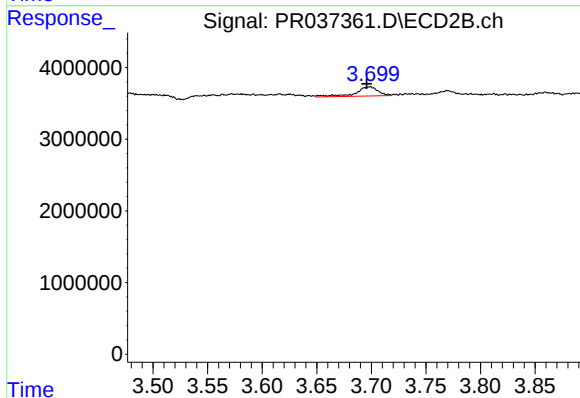


#9 AR-1221-2

R.T.: 3.699 min
Delta R.T.: 0.004 min
Response: 1865424
Conc: 50.23 ng/ml

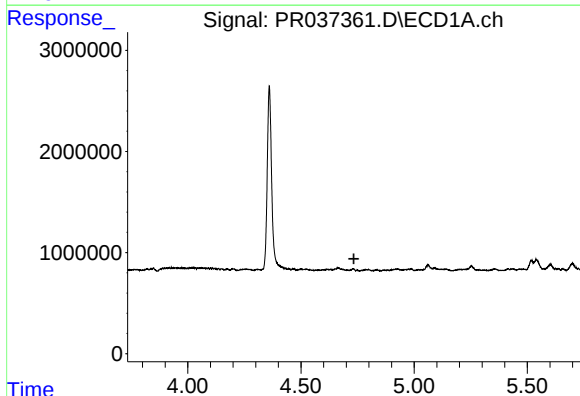


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

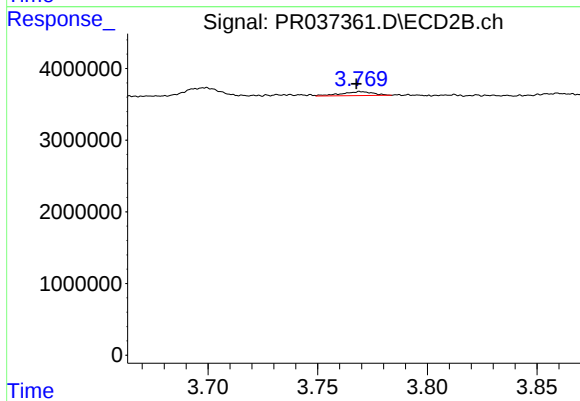

#10 AR-1221-3


R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 546155
Conc: 4.46 ng/ml

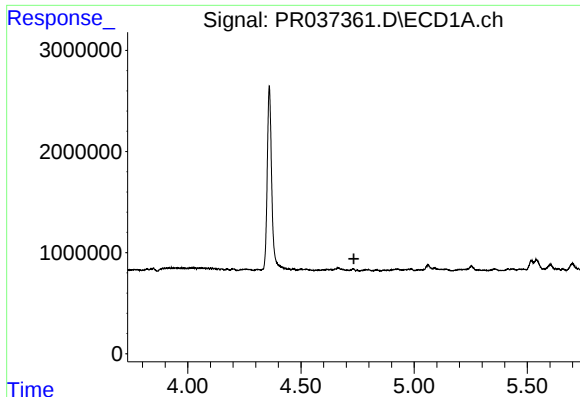

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

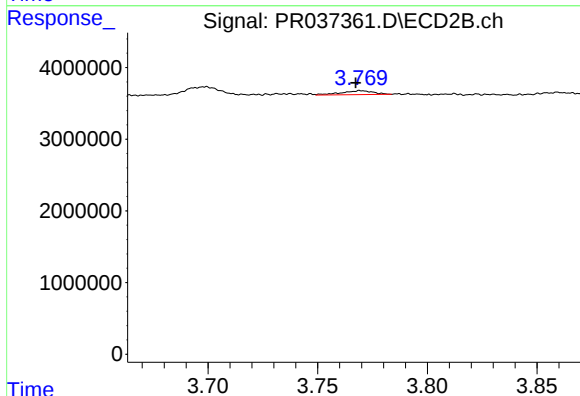


#11 AR-1232-1

R.T.: 3.769 min
Delta R.T.: 0.002 min
Response: 546155
Conc: 4.67 ng/ml

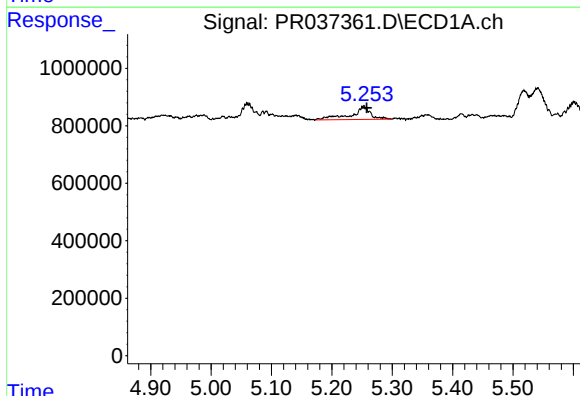


#12 AR-1232-2

R.T.: 5.253 min
Delta R.T.: -0.005 min
Response: 1022885
Conc: 60.53 ng/ml

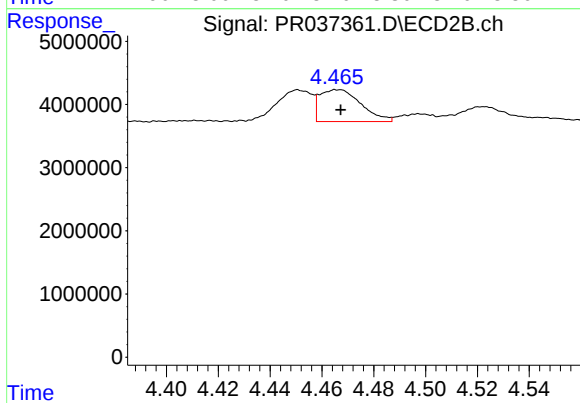

#12 AR-1232-2


R.T.: 4.466 min
Delta R.T.: -0.002 min
Response: 5618418
Conc: 40.65 ng/ml

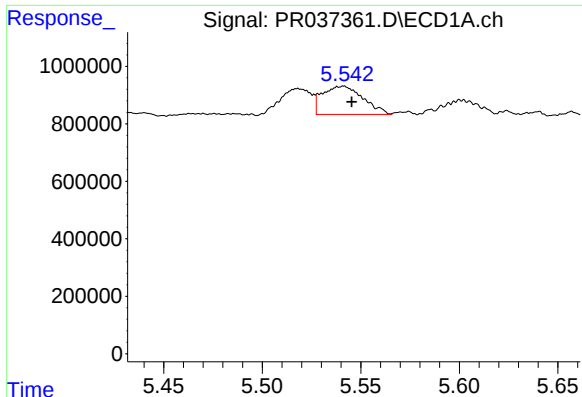

#13 AR-1232-3


R.T.: 5.541 min
Delta R.T.: -0.005 min
Response: 1411494
Conc: 41.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

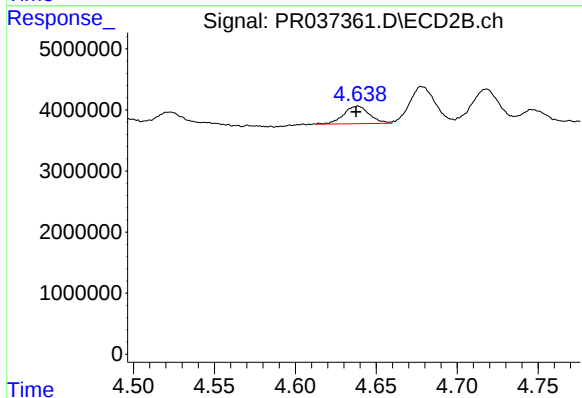


#13 AR-1232-3

R.T.: 4.639 min
Delta R.T.: 0.001 min
Response: 3170676
Conc: 45.17 ng/ml

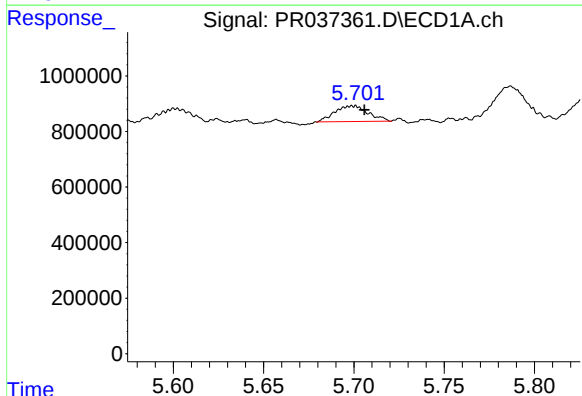


#14 AR-1232-4

R.T.: 5.699 min
Delta R.T.: -0.006 min
Response: 729474
Conc: 46.47 ng/ml

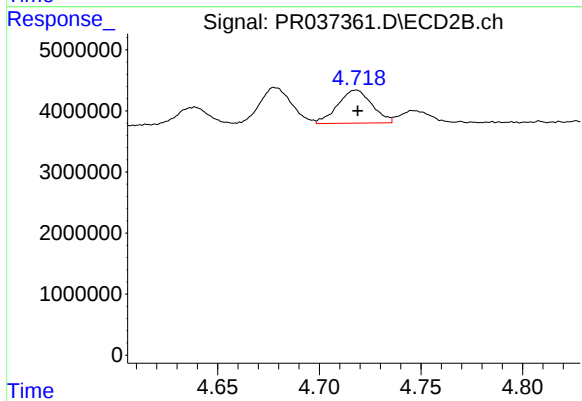

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 6354596
Conc: 106.49 ng/ml

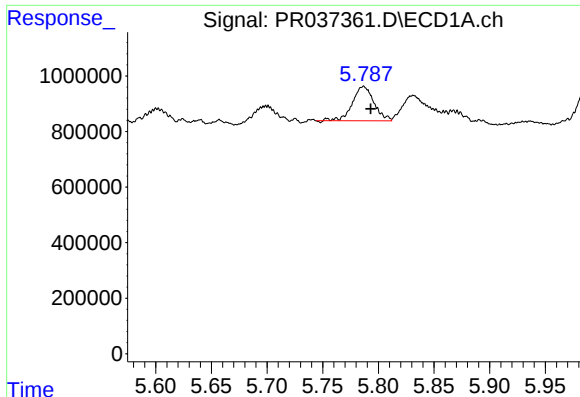

#15 AR-1232-5


R.T.: 5.787 min
Delta R.T.: -0.007 min
Response: 1668838
Conc: 142.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

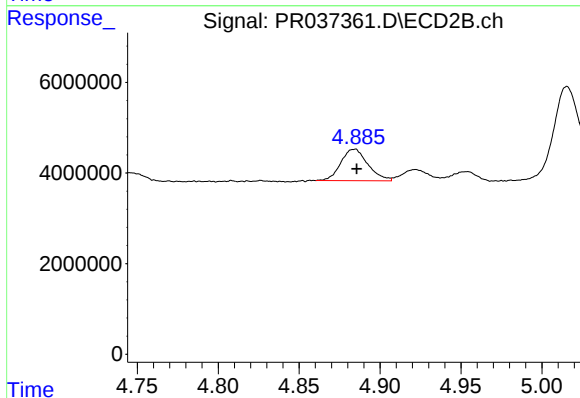


#15 AR-1232-5

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 8119530
Conc: 118.98 ng/ml

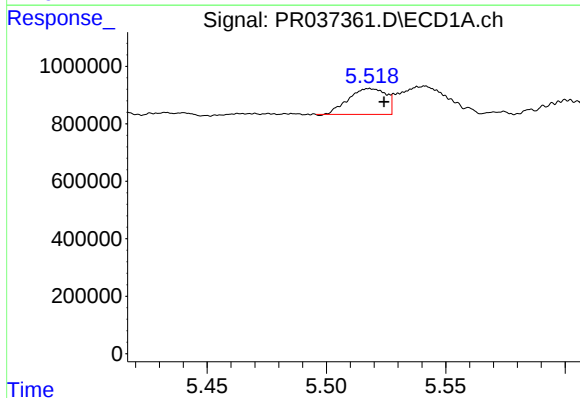


#16 AR-1242-1

R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 974809
Conc: 28.49 ng/ml

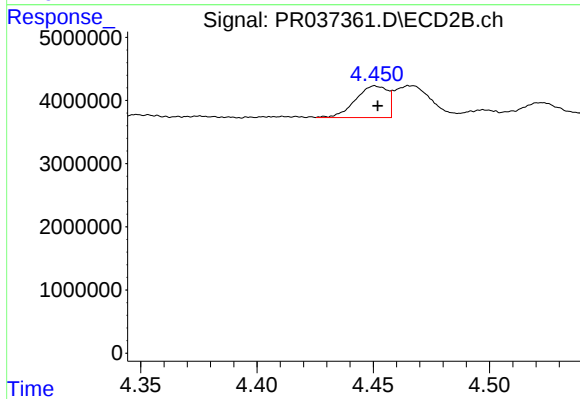

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 4777060
Conc: 32.60 ng/ml

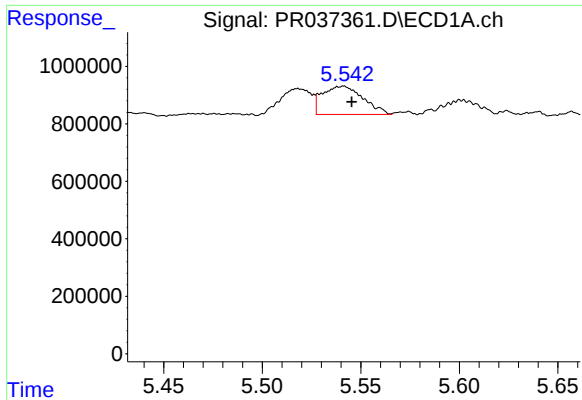

#17 AR-1242-2


R.T.: 5.541 min
Delta R.T.: -0.004 min
Response: 1411494
Conc: 25.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

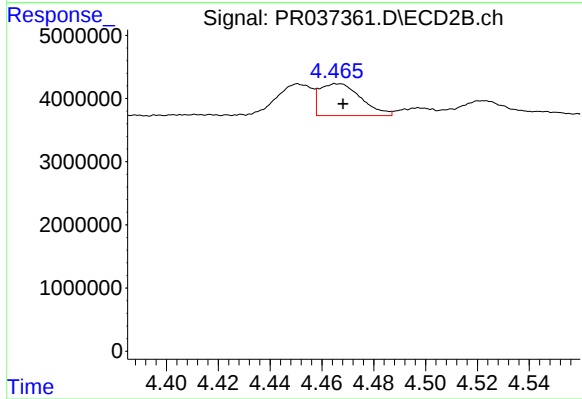


#17 AR-1242-2

R.T.: 4.466 min
Delta R.T.: -0.003 min
Response: 5618418
Conc: 24.62 ng/ml

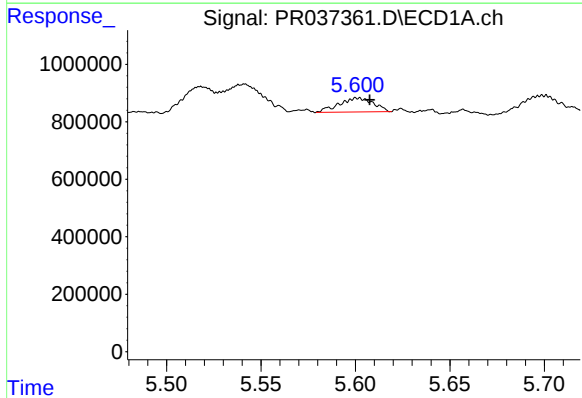


#18 AR-1242-3

R.T.: 5.601 min
Delta R.T.: -0.006 min
Response: 614812
Conc: 18.68 ng/ml

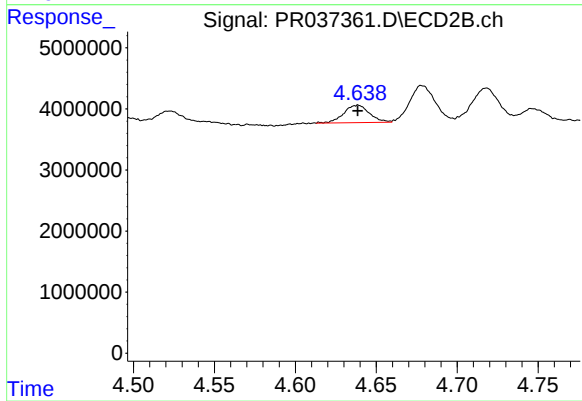

#18 AR-1242-3


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 3170676
Conc: 27.42 ng/ml

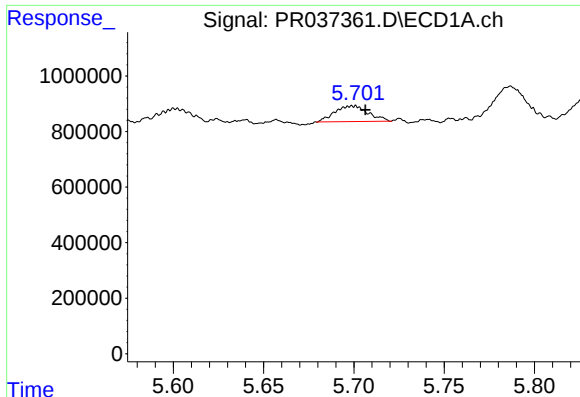

#19 AR-1242-4


R.T.: 5.699 min
Delta R.T.: -0.007 min
Response: 729474
Conc: 27.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

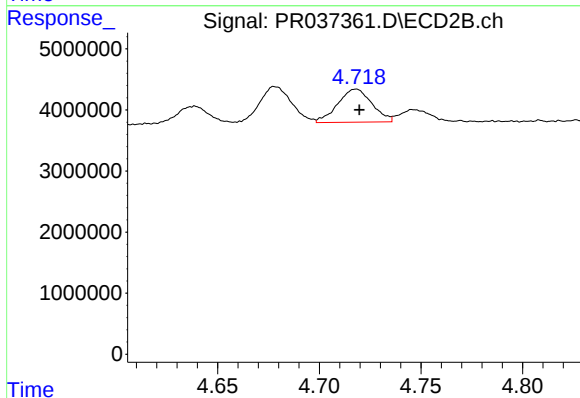


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 6354596
Conc: 57.82 ng/ml

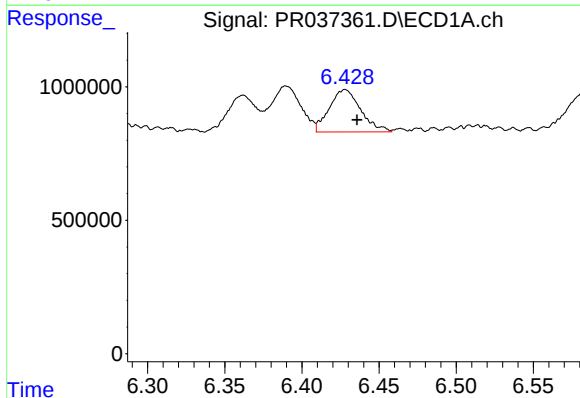


#20 AR-1242-5

R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 2244948
Conc: 69.76 ng/ml

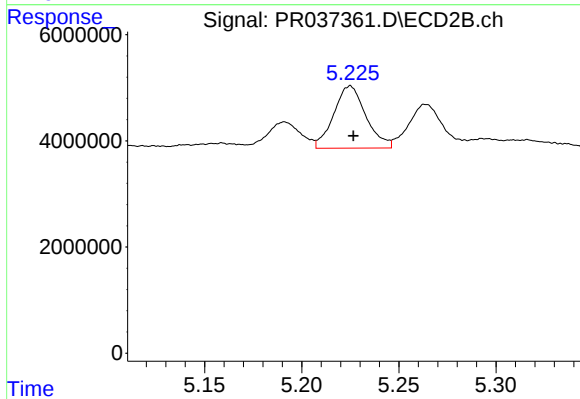

#20 AR-1242-5


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 13515538
Conc: 81.57 ng/ml

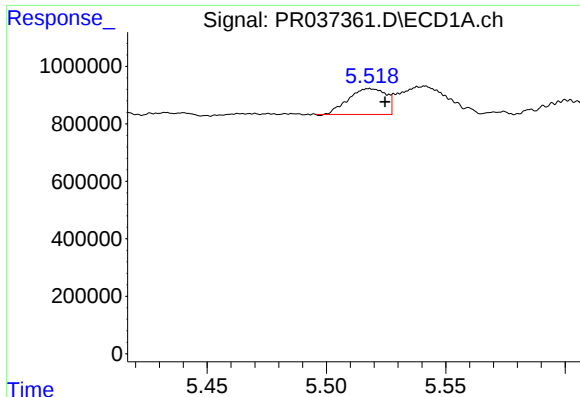

#21 AR-1248-1


R.T.: 5.518 min
Delta R.T.: -0.006 min
Response: 974809
Conc: 42.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

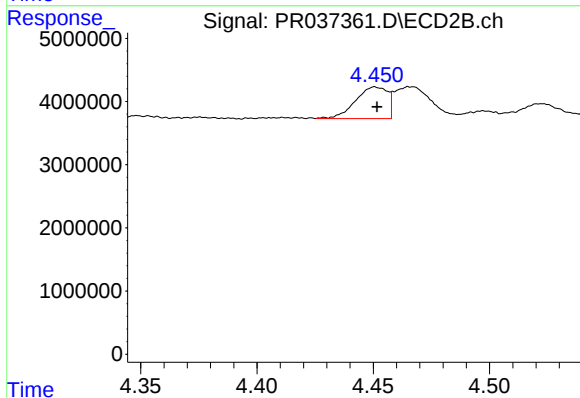


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 4777060
Conc: 47.46 ng/ml

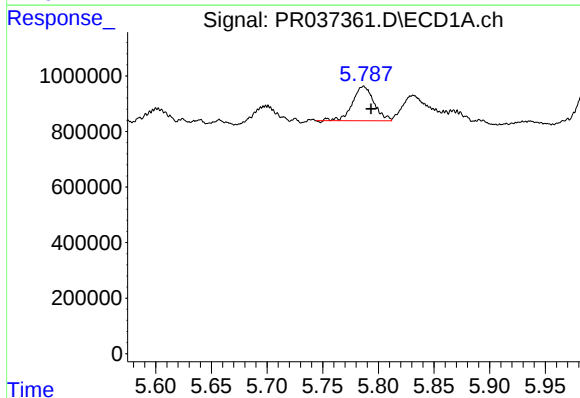


#22 AR-1248-2

R.T.: 5.787 min
Delta R.T.: -0.007 min
Response: 1668838
Conc: 47.66 ng/ml

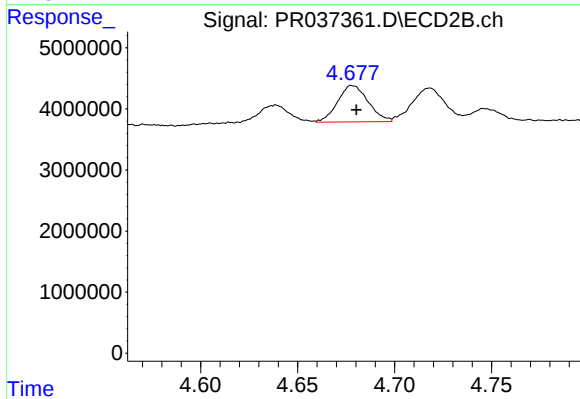

#22 AR-1248-2


R.T.: 4.678 min
Delta R.T.: -0.002 min
Response: 6537367
Conc: 47.90 ng/ml

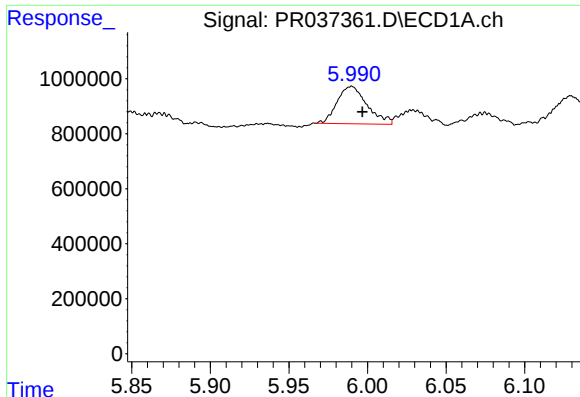

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1810175
Conc: 44.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

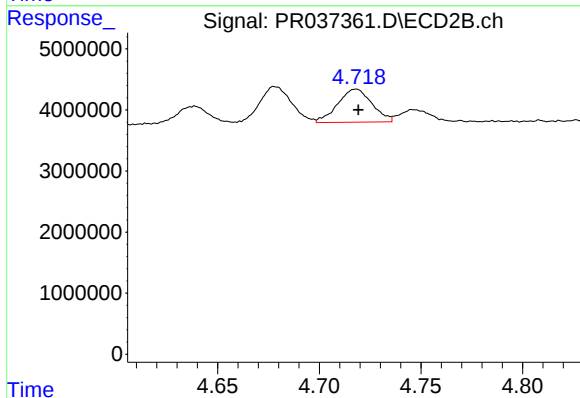


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 6354596
Conc: 45.40 ng/ml

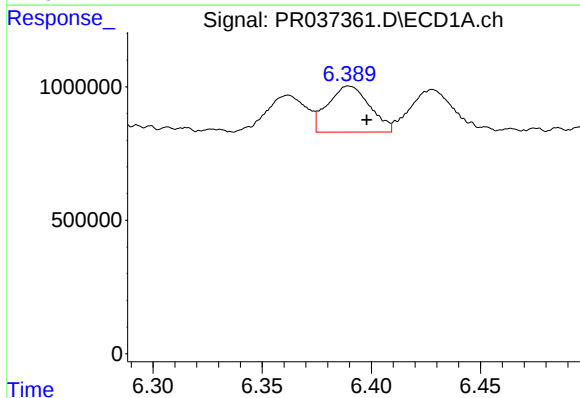


#24 AR-1248-4

R.T.: 6.390 min
Delta R.T.: -0.008 min
Response: 2307292
Conc: 47.13 ng/ml

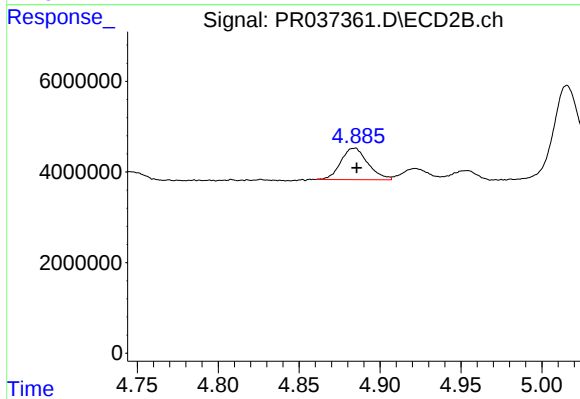

#24 AR-1248-4


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 8119530
Conc: 45.62 ng/ml

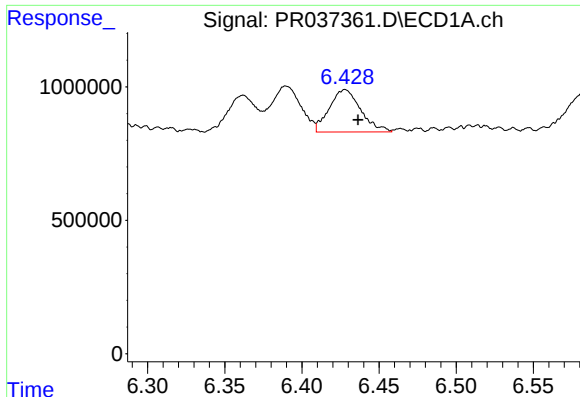

#25 AR-1248-5


R.T.: 6.428 min
Delta R.T.: -0.008 min
Response: 2244948
Conc: 47.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

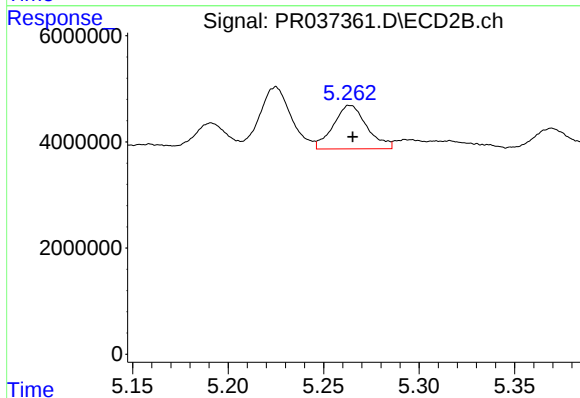


#25 AR-1248-5

R.T.: 5.264 min
Delta R.T.: -0.002 min
Response: 10056868
Conc: 51.41 ng/ml

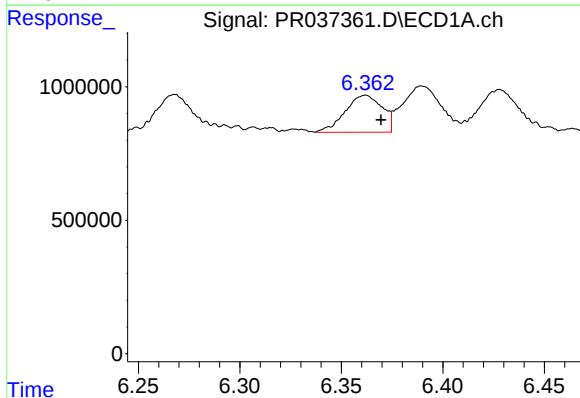


#26 AR-1254-1

R.T.: 6.362 min
Delta R.T.: -0.008 min
Response: 1752302
Conc: 32.08 ng/ml

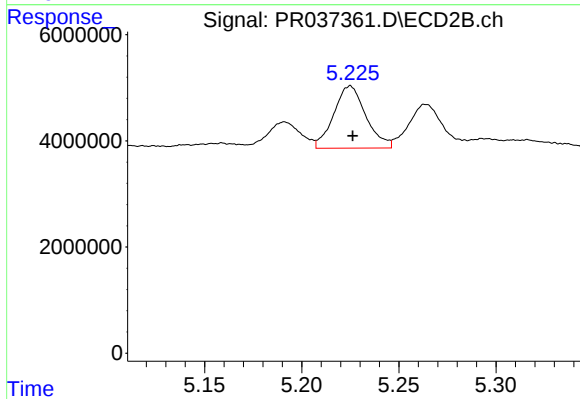

#26 AR-1254-1


R.T.: 5.225 min
Delta R.T.: -0.001 min
Response: 13515538
Conc: 39.24 ng/ml

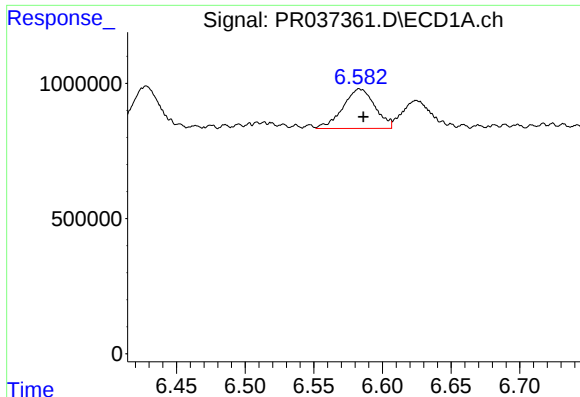

#27 AR-1254-2


R.T.: 6.583 min
Delta R.T.: -0.003 min
Response: 2379769
Conc: 27.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

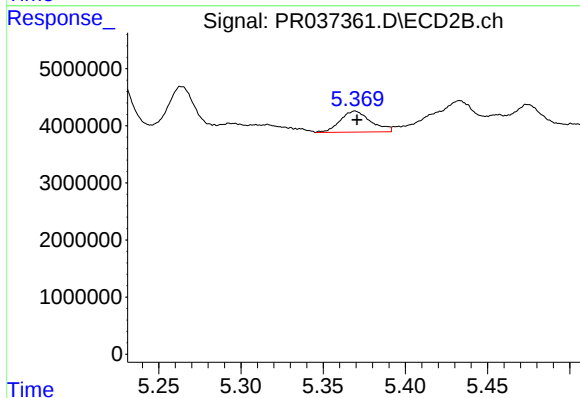


#27 AR-1254-2

R.T.: 5.369 min
Delta R.T.: -0.001 min
Response: 4753546
Conc: 15.87 ng/ml

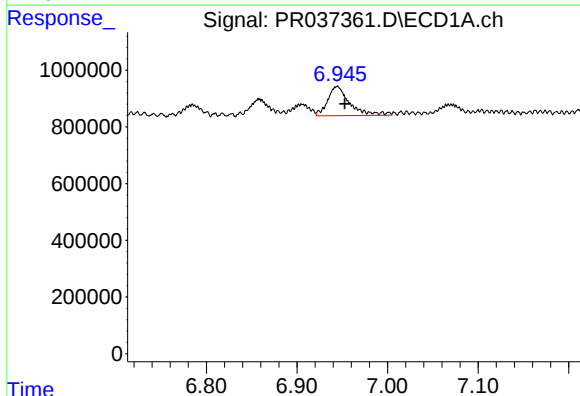


#28 AR-1254-3

R.T.: 6.944 min
Delta R.T.: -0.008 min
Response: 1744029
Conc: 19.17 ng/ml

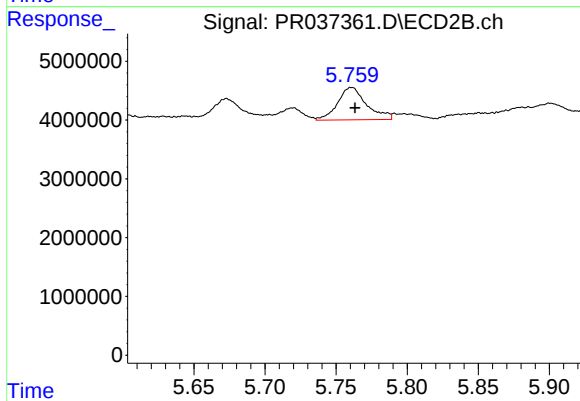

#28 AR-1254-3


R.T.: 5.761 min
Delta R.T.: -0.003 min
Response: 7864038
Conc: 16.60 ng/ml

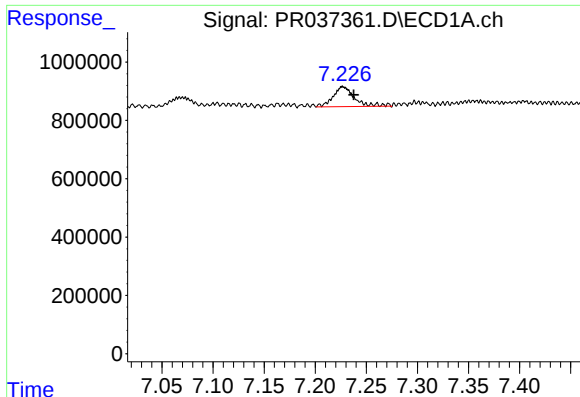

#29 AR-1254-4


R.T.: 7.227 min
Delta R.T.: -0.011 min
Response: 994645
Conc: 14.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

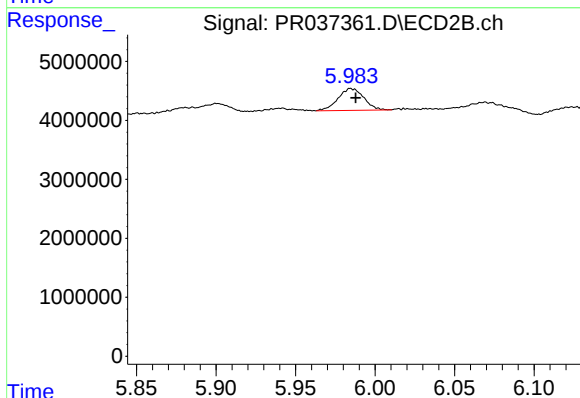


#29 AR-1254-4

R.T.: 5.984 min
Delta R.T.: -0.003 min
Response: 4164103
Conc: 11.88 ng/ml

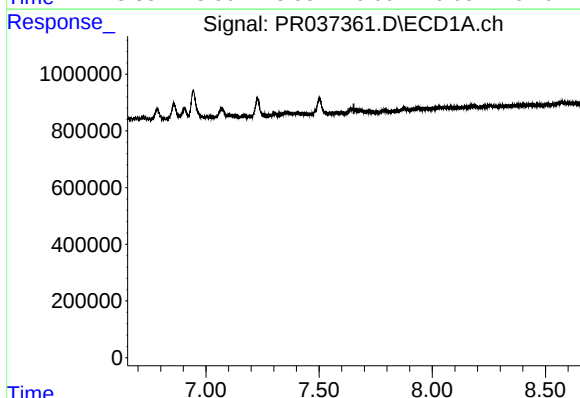


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

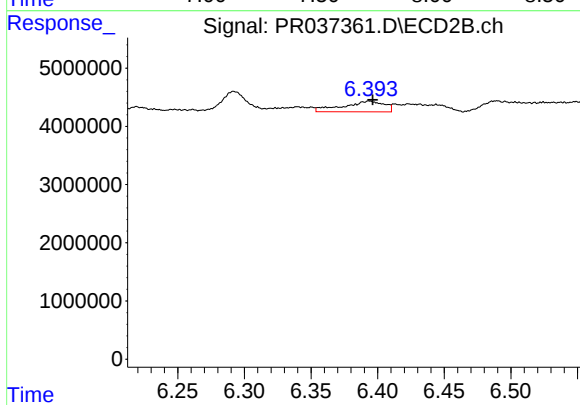

#30 AR-1254-5


R.T.: 6.394 min
Delta R.T.: -0.003 min
Response: 3942053
Conc: 8.90 ng/ml

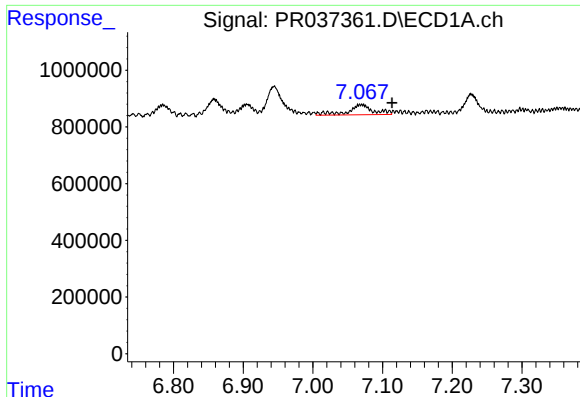

#31 AR-1260-1


R.T.: 7.070 min
Delta R.T.: -0.044 min
Response: 897197
Conc: 13.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

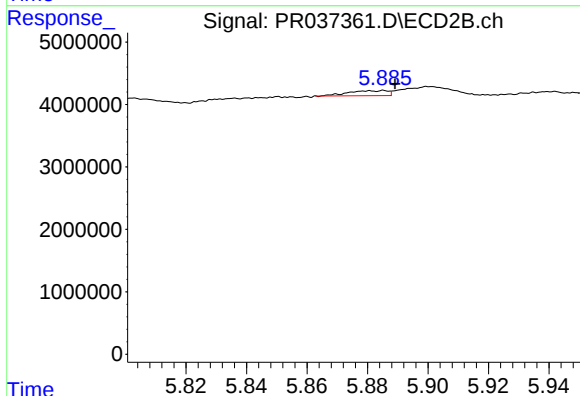


#31 AR-1260-1

R.T.: 5.885 min
Delta R.T.: -0.004 min
Response: 709628
Conc: 2.43 ng/ml

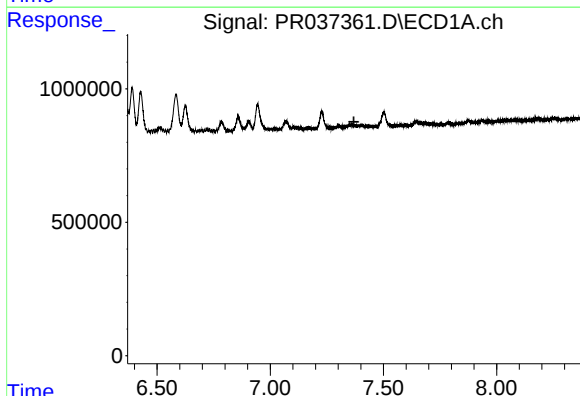


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

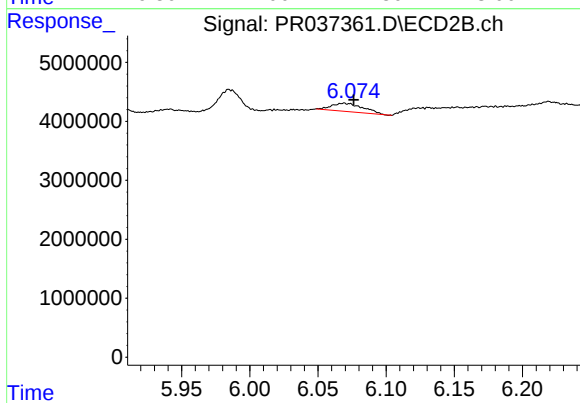

#32 AR-1260-2


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 2211996
Conc: 4.80 ng/ml

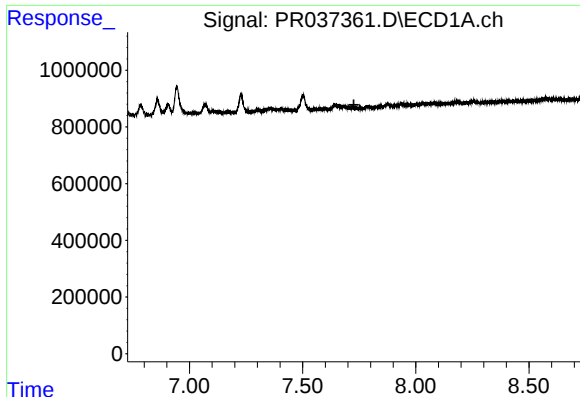

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

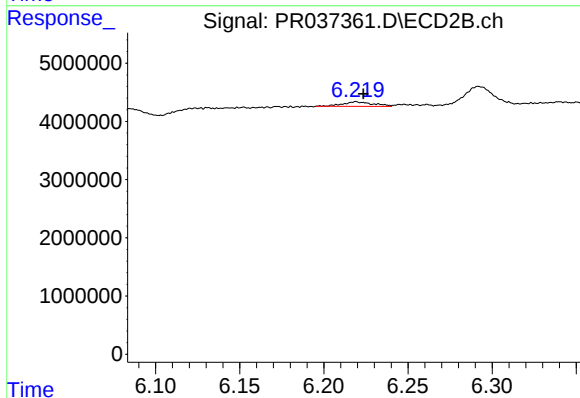


#33 AR-1260-3

R.T.: 6.219 min
Delta R.T.: -0.004 min
Response: 996974
Conc: 2.80 ng/ml

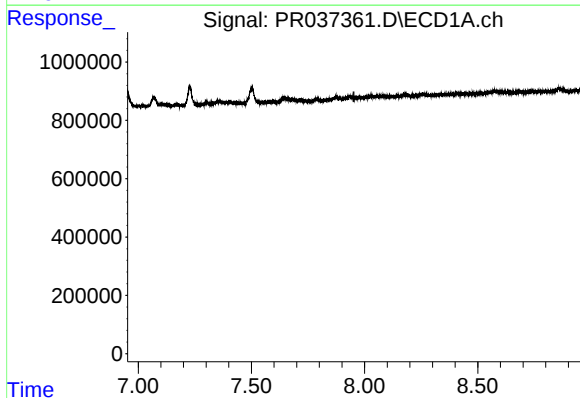


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

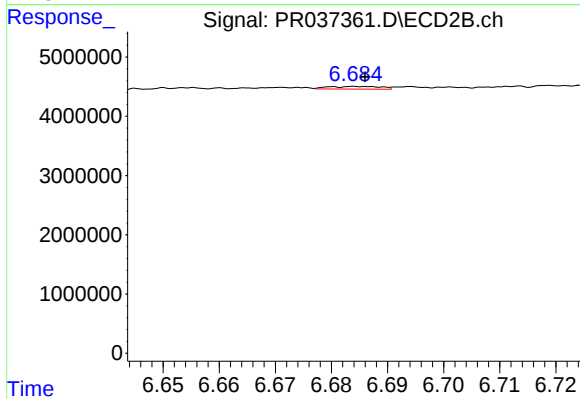

#34 AR-1260-4


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 284542
Conc: 0.93 ng/ml

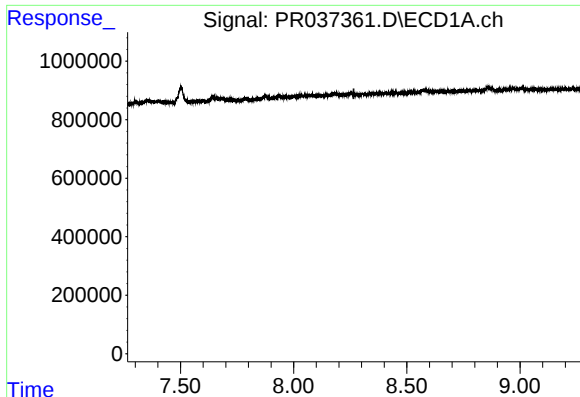

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

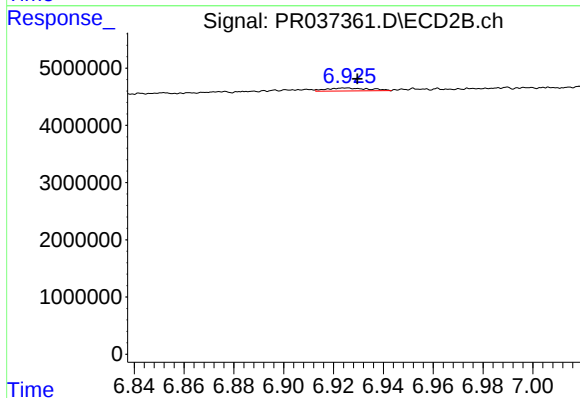


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 623437
Conc: 0.72 ng/ml

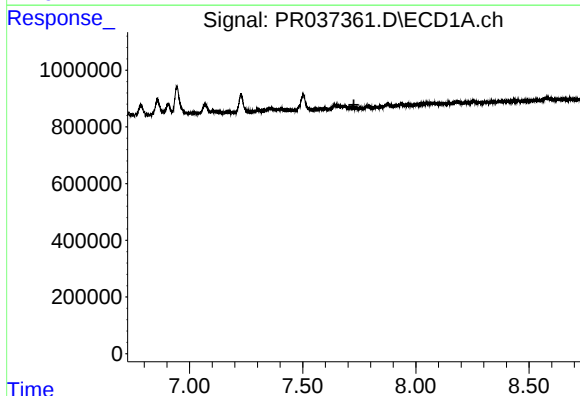


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

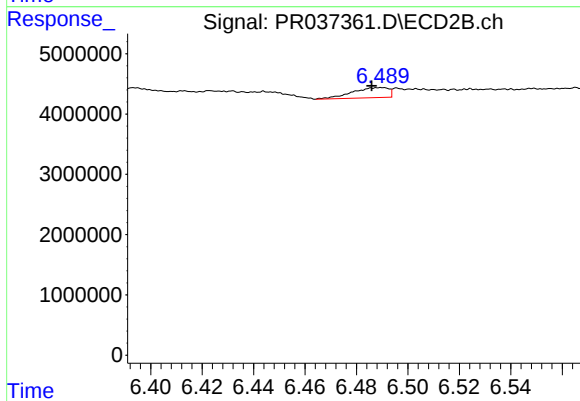

#36 AR-1262-1


R.T.: 6.490 min
Delta R.T.: 0.004 min
Response: 1626433
Conc: 6.49 ng/ml

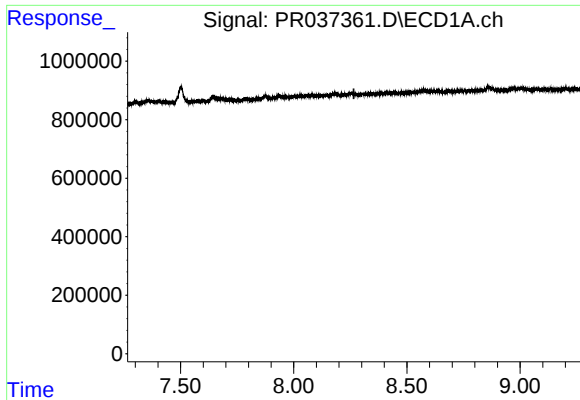

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

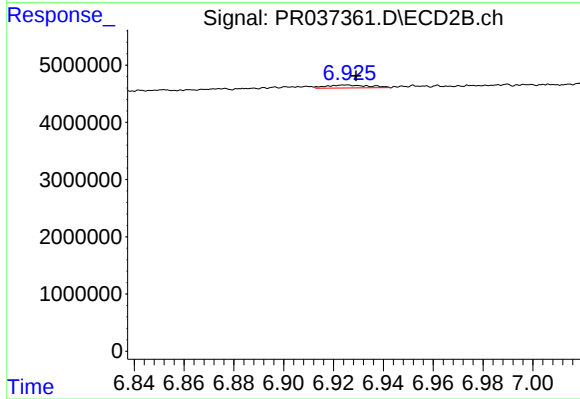


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 623437
Conc: 0.50 ng/ml

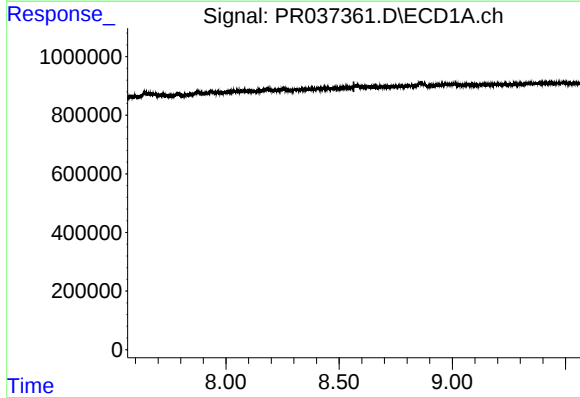


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

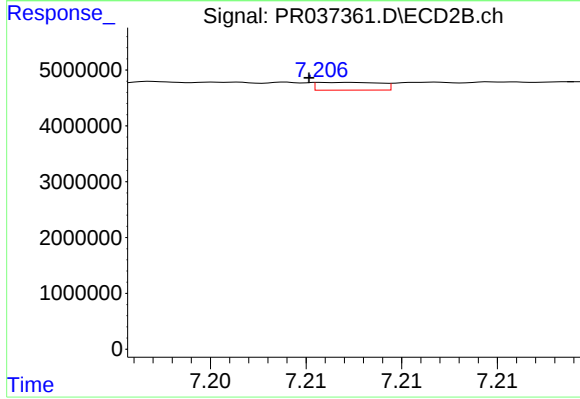

#38 AR-1262-3


R.T.: 7.207 min
Delta R.T.: 0.002 min
Response: 320435
Conc: 0.58 ng/ml

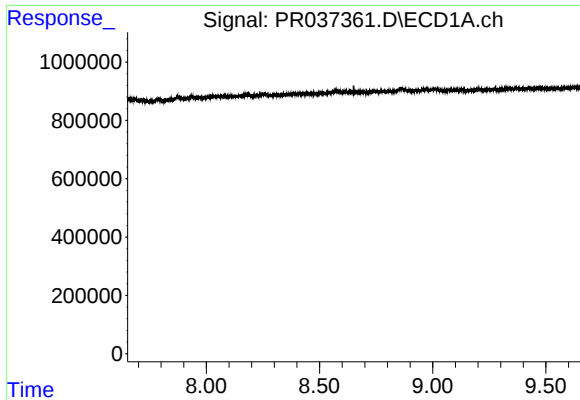

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

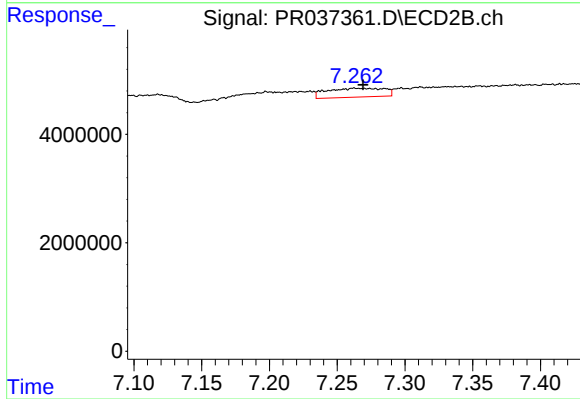


#39 AR-1262-4

R.T.: 7.263 min
Delta R.T.: -0.007 min
Response: 4775494
Conc: 5.32 ng/ml

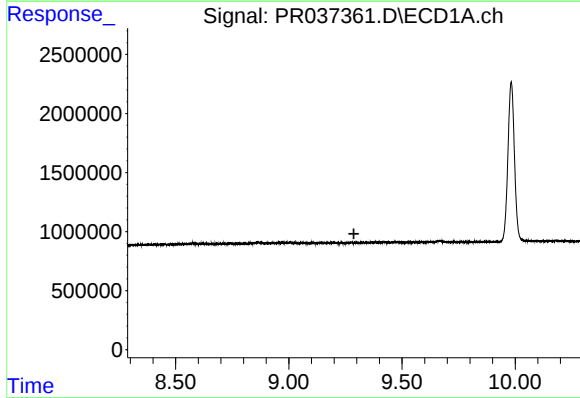


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

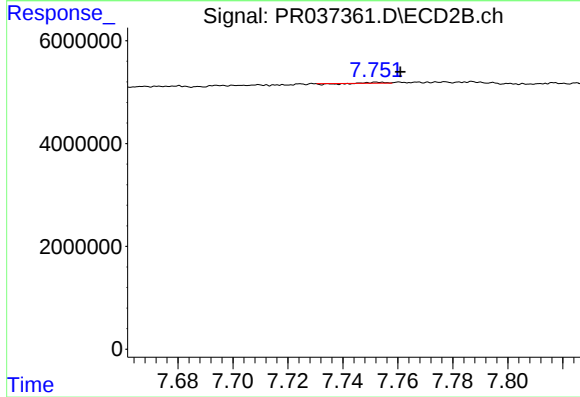

#40 AR-1262-5


R.T.: 7.753 min
Delta R.T.: -0.008 min
Response: 32045
Conc: 0.08 ng/ml

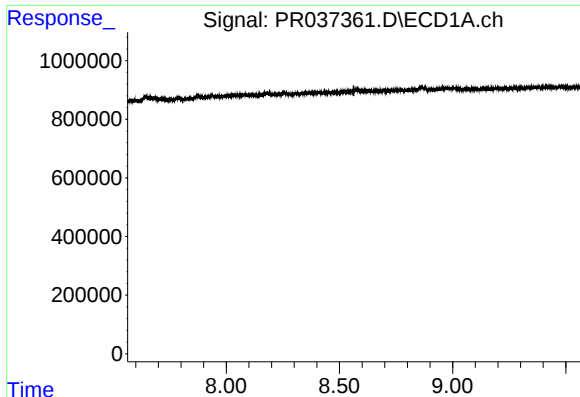

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

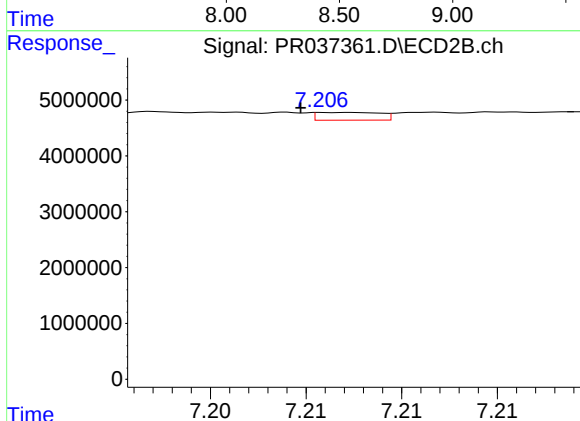


#41 AR-1268-1

R.T.: 7.207 min
Delta R.T.: 0.002 min
Response: 320435
Conc: 0.26 ng/ml

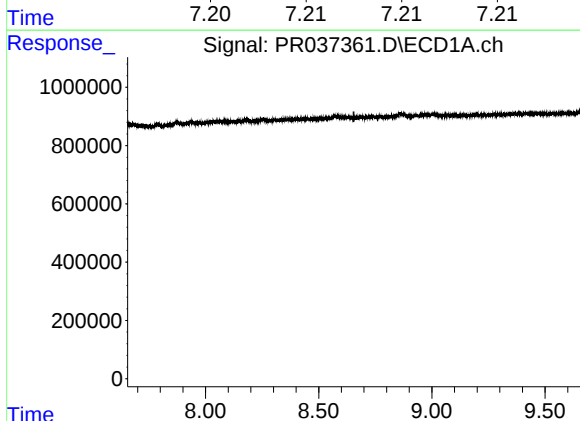


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

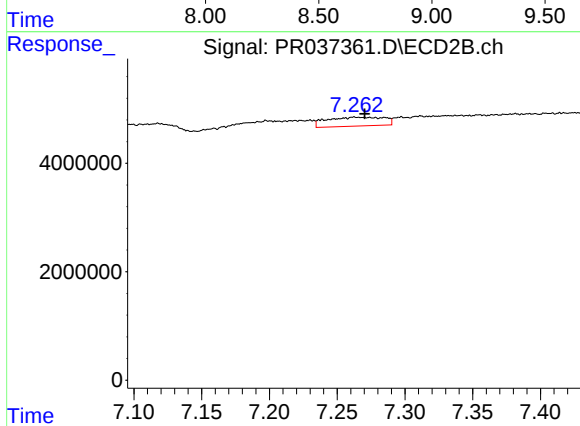

#42 AR-1268-2


R.T.: 7.263 min
Delta R.T.: -0.008 min
Response: 4775494
Conc: 4.51 ng/ml

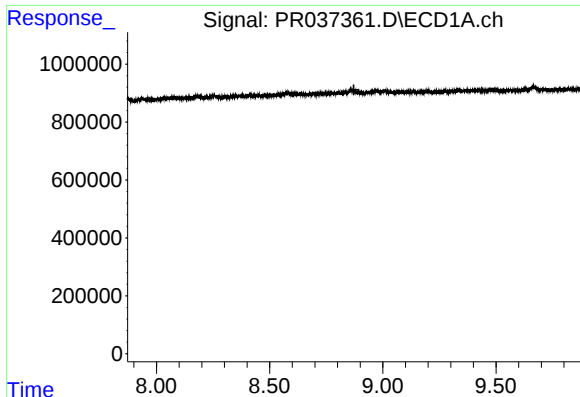

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

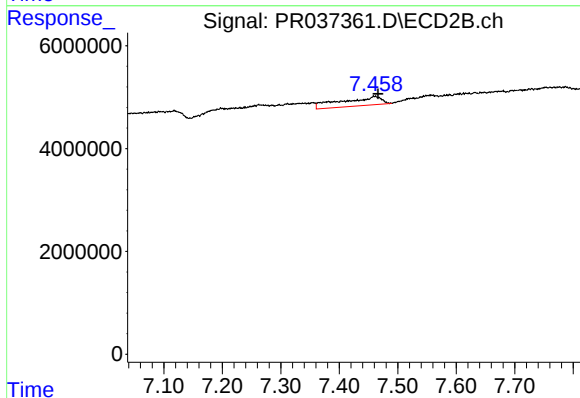


#43 AR-1268-3

R.T.: 7.460 min
Delta R.T.: -0.007 min
Response: 8213347
Conc: 9.27 ng/ml

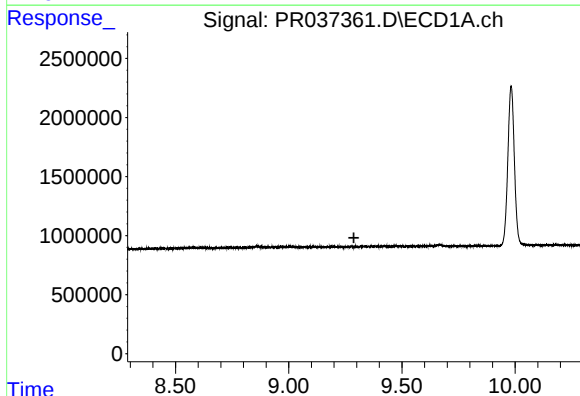


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

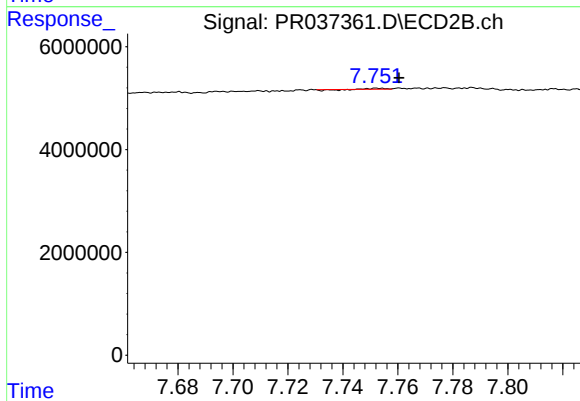

#44 AR-1268-4


R.T.: 7.753 min
Delta R.T.: -0.008 min
Response: 32045
Conc: 0.09 ng/ml

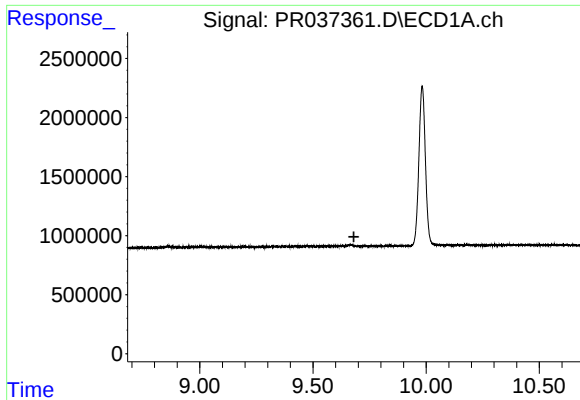

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

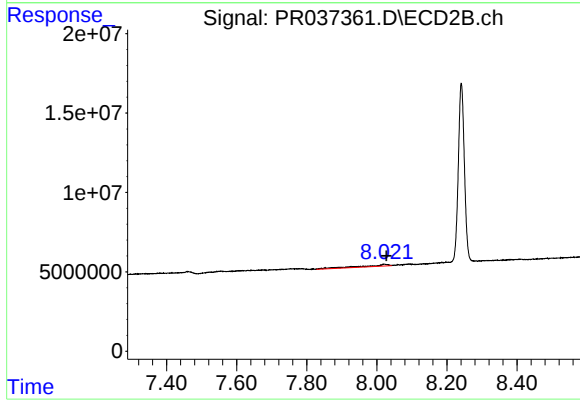

#45 AR-1268-5

R.T.: 8.022 min
Delta R.T.: -0.006 min
Response: 5872201
Conc: 2.31 ng/ml