

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 18:03
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1254 LOD 25PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:05:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	27127275	111.2E6	21.684	23.187
2)	SA Decachlor...	9.979	8.239	27833410	146.1E6	21.045	25.093
Target Compounds							
3)	L1 AR-1016-1	0.000	4.452	0	418437	N.D.	2.298 #
4)	L1 AR-1016-2	0.000	4.452	0	418437	N.D.	1.483 #
5)	L1 AR-1016-3	0.000	4.647	0	177022	N.D.	1.231 #
6)	L1 AR-1016-4	0.000	4.679	0	3553215	N.D.	32.117 #
7)	L1 AR-1016-5	5.989	4.883	549031	2132775	16.011	14.031
8)	L2 AR-1221-1	0.000	3.623	0	283629	N.D.	5.570 #
9)	L2 AR-1221-2	4.664	3.698	406071	2192259	44.900	59.034 #
10)	L2 AR-1221-3	4.664	3.737	406071	215878	13.249	1.763 #
11)	L3 AR-1232-1	4.664	3.737	406071	215878	13.882	1.845 #
12)	L3 AR-1232-2	0.000	4.452	0	418437	N.D.	3.027 #
13)	L3 AR-1232-3	0.000	4.647	0	177022	N.D.	2.522 #
14)	L3 AR-1232-4	0.000	4.718	0	1196954	N.D.	20.059 #
15)	L3 AR-1232-5	5.786	4.883	686676	2132775	58.712	31.252 #
16)	L4 AR-1242-1	0.000	4.452	0	418437	N.D.	2.855 #
17)	L4 AR-1242-2	0.000	4.452	0	418437	N.D.	1.834 #
18)	L4 AR-1242-3	0.000	4.647	0	177022	N.D.	1.531 #
19)	L4 AR-1242-4	0.000	4.718	0	1196954	N.D.	10.890 #
20)	L4 AR-1242-5	6.429	5.224	538625	9917316	16.738	59.851 #
21)	L5 AR-1248-1	0.000	4.452	0	418437	N.D.	4.157 #
22)	L5 AR-1248-2	5.786	4.679	686676	3553215	19.611	26.036 #
23)	L5 AR-1248-3	5.989	4.718	549031	1196954	13.421	8.551 #
24)	L5 AR-1248-4	6.389	4.883	865003	2132775	17.670	11.984 #
25)	L5 AR-1248-5	6.429	5.266	538625	2228422	11.403	11.392
26)	L6 AR-1254-1	6.361	5.224	1656495	9917316	30.322	28.790
27)	L6 AR-1254-2	6.578	5.370	2622336	8411966	30.600	28.086
28)	L6 AR-1254-3	6.944	5.760	2744077	12974933	30.167	27.395
29)	L6 AR-1254-4	7.228	5.985	2088179	8917825	31.163	25.433
30)	L6 AR-1254-5	7.642	6.393	2171570	13587787	30.211	30.684
31)	L7 AR-1260-1	7.103	5.886	1063609	5686042	16.119	19.454
32)	L7 AR-1260-2	7.358	6.072	1297521	6916337	16.279	15.016
33)	L7 AR-1260-3	0.000	6.219	0	5021907	N.D.	14.087 #
34)	L7 AR-1260-4	7.932	6.684	994475	181263	13.366	0.595 #
35)	L7 AR-1260-5	0.000	6.924	0	1246970	N.D.	1.438 #
36)	L8 AR-1262-1	0.000	6.489	0	1650744	N.D.	6.587 #
37)	L8 AR-1262-2	0.000	6.924	0	1246970	N.D.	0.993 #
38)	L8 AR-1262-3	0.000	7.260	0	13256604	N.D.	24.179 #
39)	L8 AR-1262-4	0.000	7.260	0	13256604	N.D.	14.768 #
40)	L8 AR-1262-5	0.000	7.780	0	699444	N.D.	1.828 #
41)	L9 AR-1268-1	0.000	7.260	0	13256604	N.D.	10.769 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 18:03
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1254 LOD 25PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:05:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.260	0	13256604	N.D.	12.519 #
43) L9	AR-1268-3	0.000	7.461	0	2546651	N.D.	2.874 #
44) L9	AR-1268-4	0.000	7.780	0	699444	N.D.	1.928 #
45) L9	AR-1268-5	0.000	8.018	0	2157387	N.D.	0.848 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 18:03
Operator : SM\SJ
Sample : K2241-07
Misc : AR1254 LOD 25PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:05:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

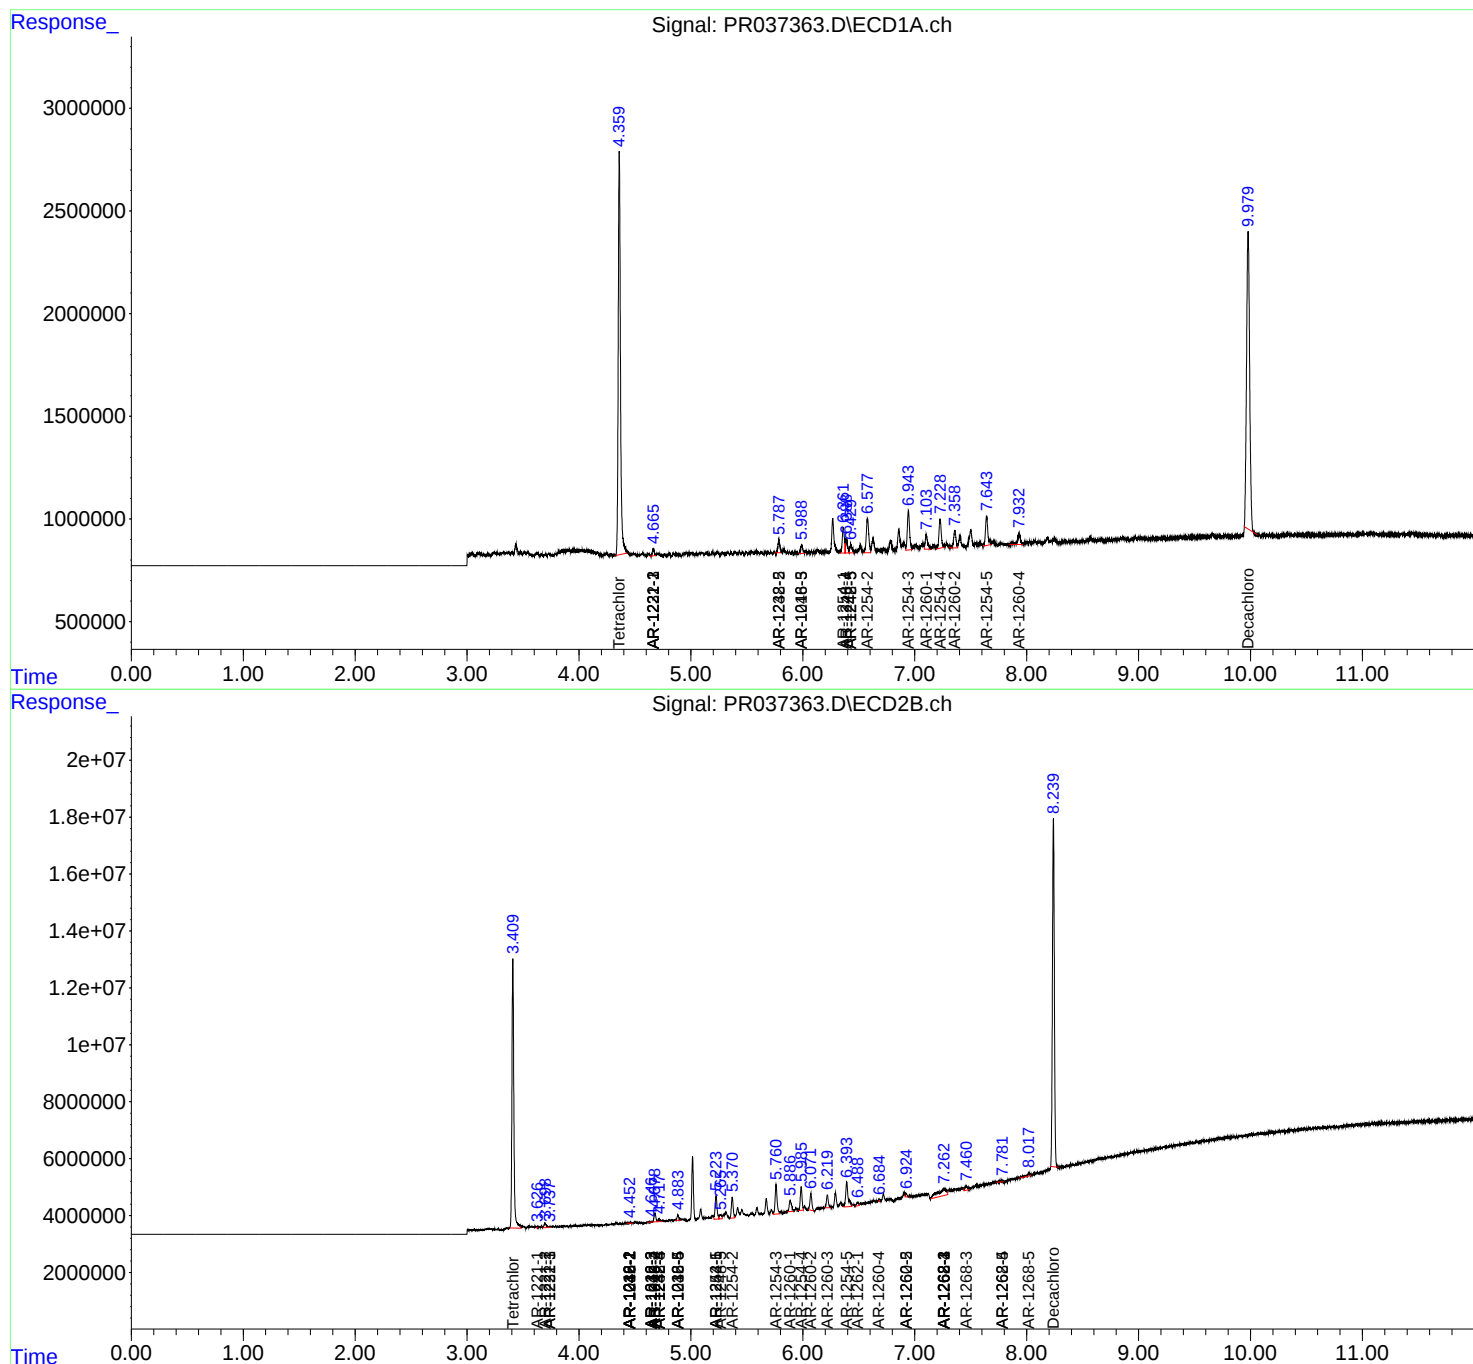


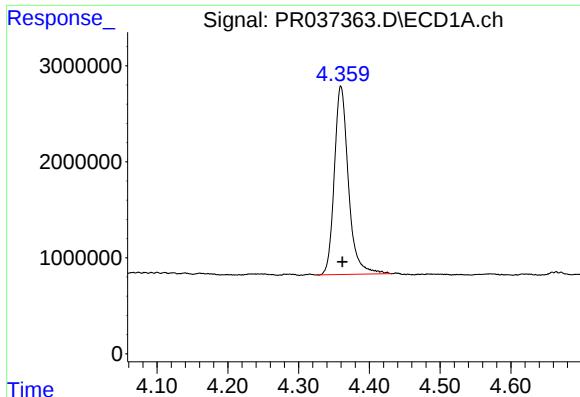

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 27127275
Conc: 21.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

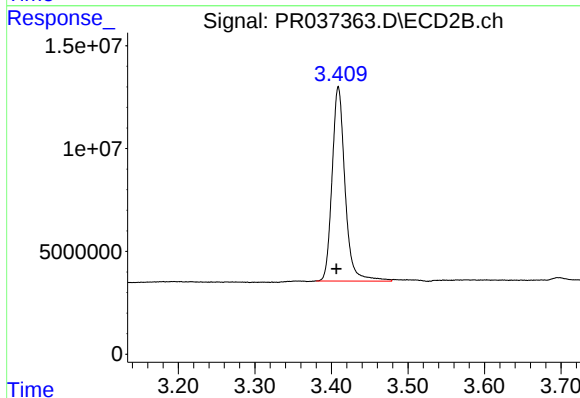


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.003 min
Response: 111195152
Conc: 23.19 ng/ml

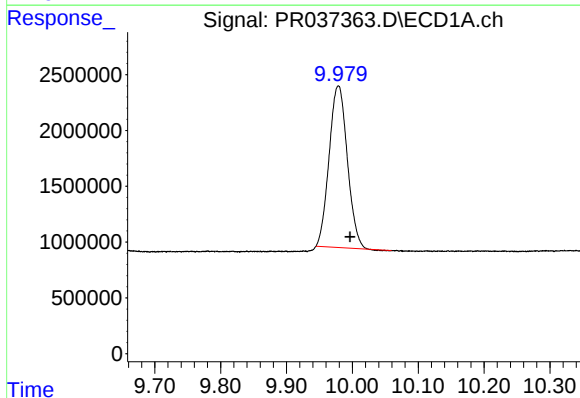


#2 Decachlorobiphenyl

R.T.: 9.979 min
Delta R.T.: -0.018 min
Response: 27833410
Conc: 21.04 ng/ml

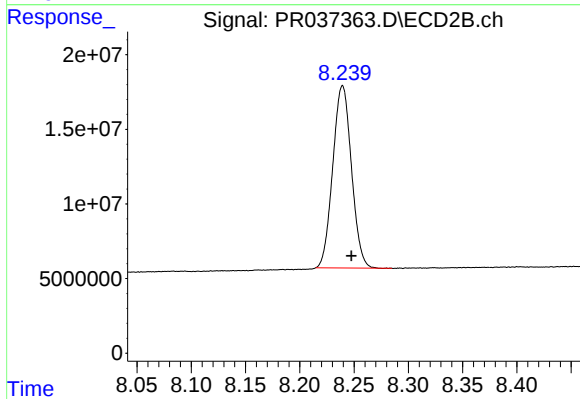

#2 Decachlorobiphenyl


R.T.: 8.239 min
Delta R.T.: -0.008 min
Response: 146146909
Conc: 25.09 ng/ml

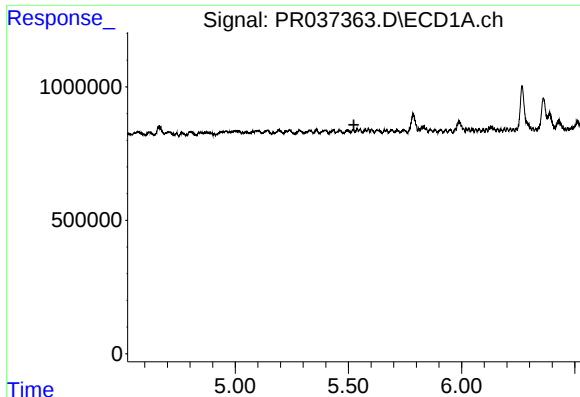

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

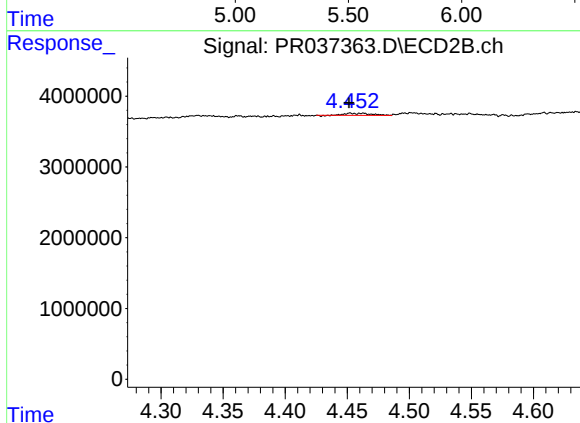


#3 AR-1016-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 418437
Conc: 2.30 ng/ml

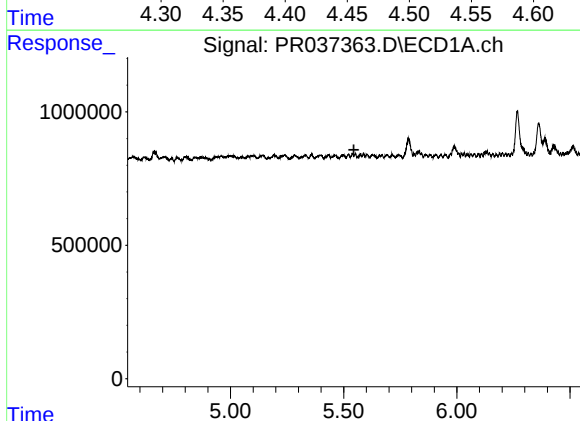


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

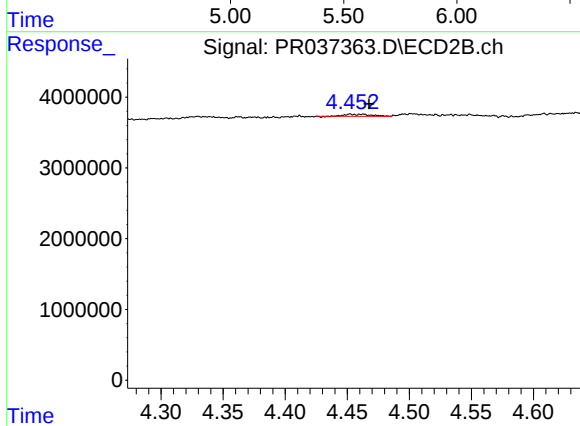

#4 AR-1016-2


R.T.: 4.452 min
Delta R.T.: -0.015 min
Response: 418437
Conc: 1.48 ng/ml

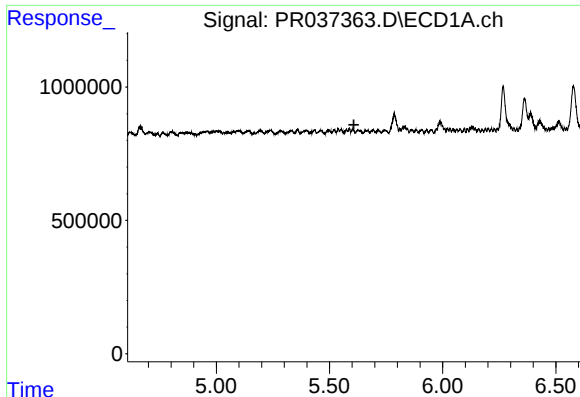

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

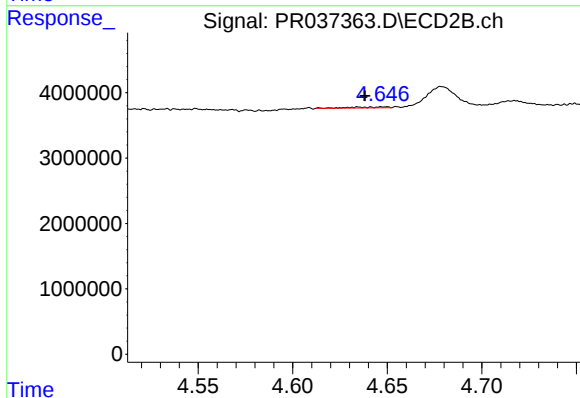


#5 AR-1016-3

R.T.: 4.647 min
Delta R.T.: 0.009 min
Response: 177022
Conc: 1.23 ng/ml

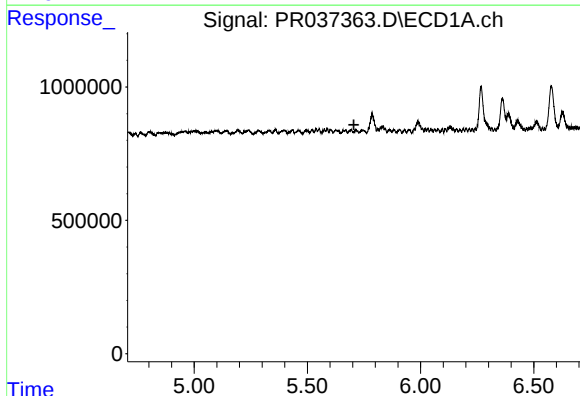


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

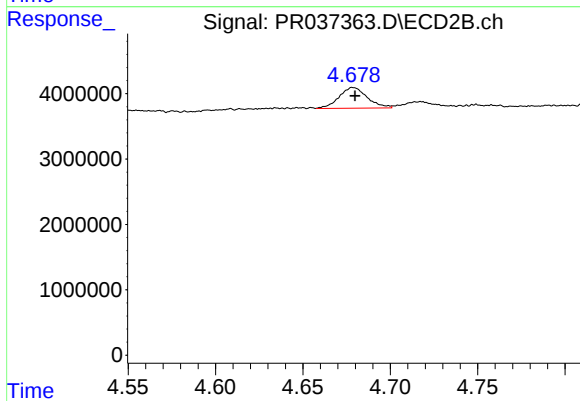

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: -0.001 min
Response: 3553215
Conc: 32.12 ng/ml

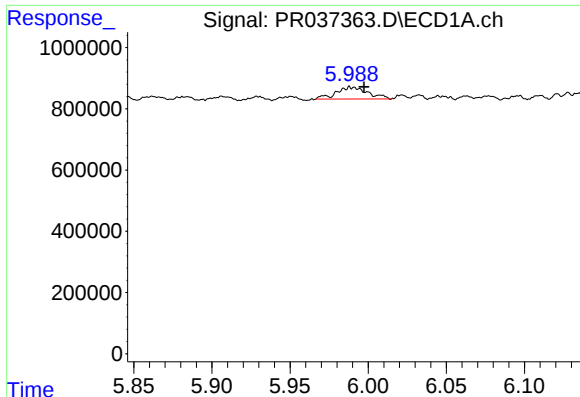

#7 AR-1016-5


R.T.: 5.989 min
Delta R.T.: -0.008 min
Response: 549031
Conc: 16.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

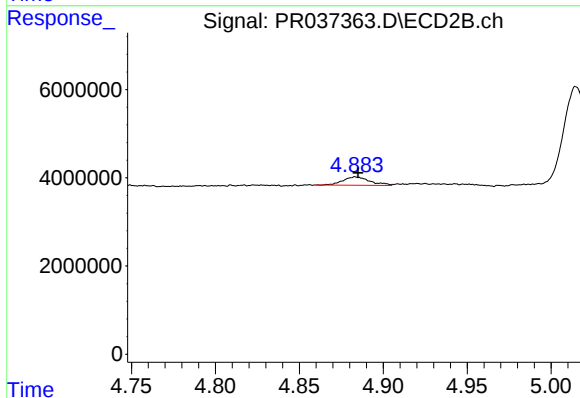


#7 AR-1016-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2132775
Conc: 14.03 ng/ml

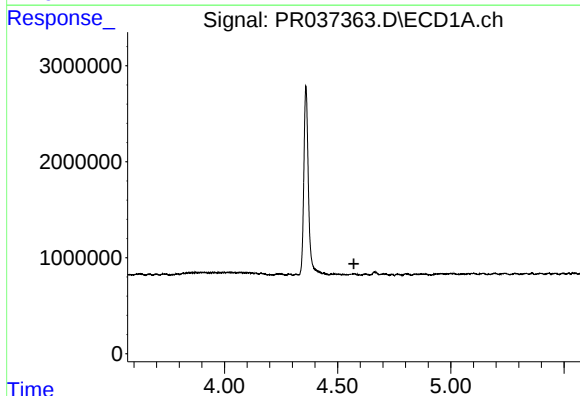


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

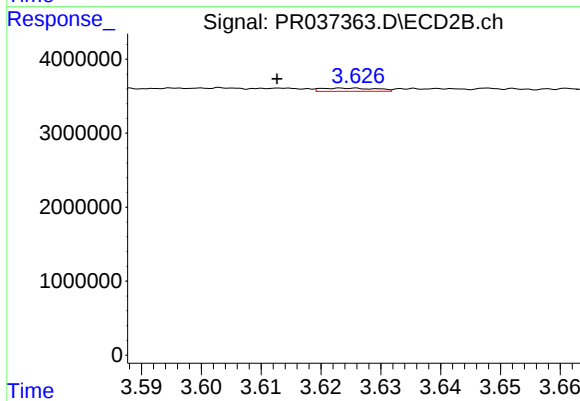

#8 AR-1221-1


R.T.: 3.623 min
Delta R.T.: 0.011 min
Response: 283629
Conc: 5.57 ng/ml

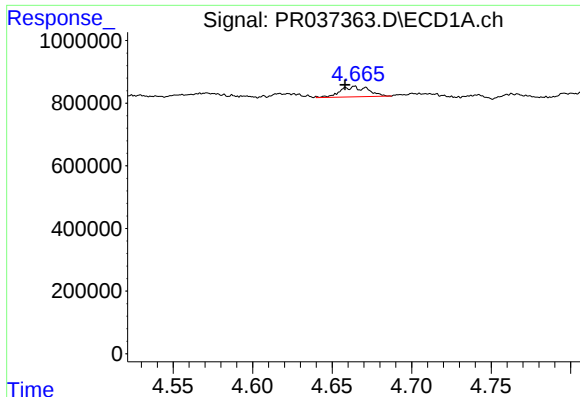

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 406071
Conc: 44.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

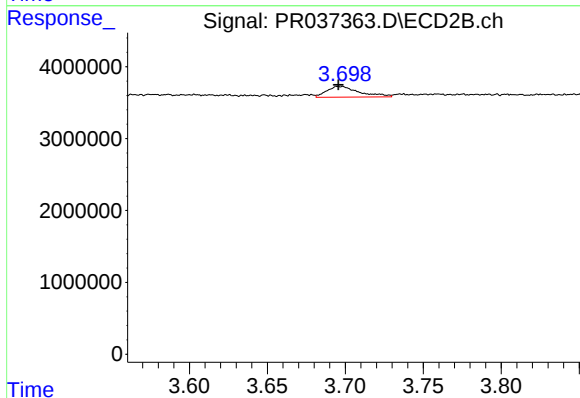


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.003 min
Response: 2192259
Conc: 59.03 ng/ml

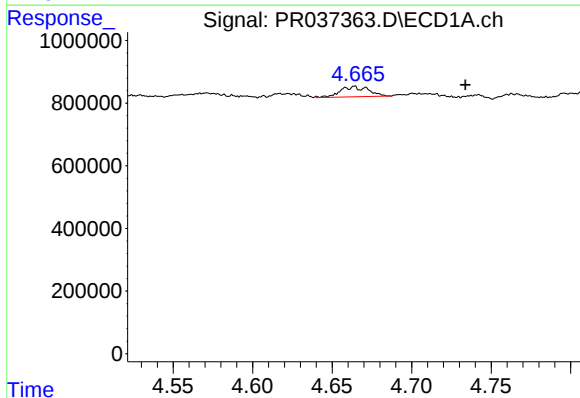


#10 AR-1221-3

R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 406071
Conc: 13.25 ng/ml

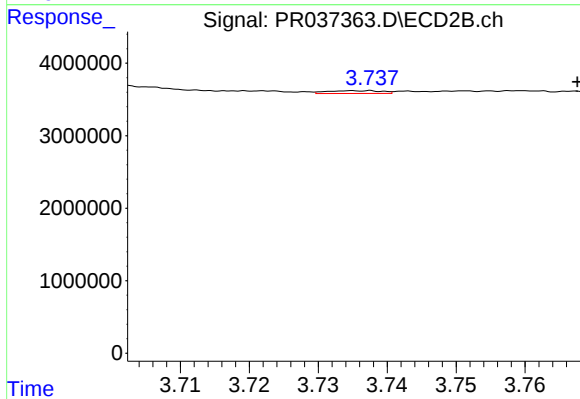

#10 AR-1221-3


R.T.: 3.737 min
Delta R.T.: -0.030 min
Response: 215878
Conc: 1.76 ng/ml

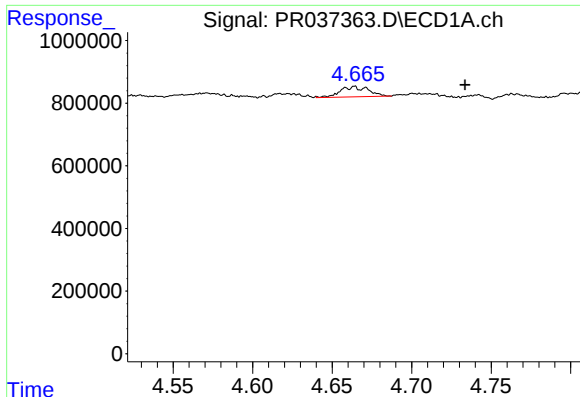

#11 AR-1232-1


R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 406071
Conc: 13.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

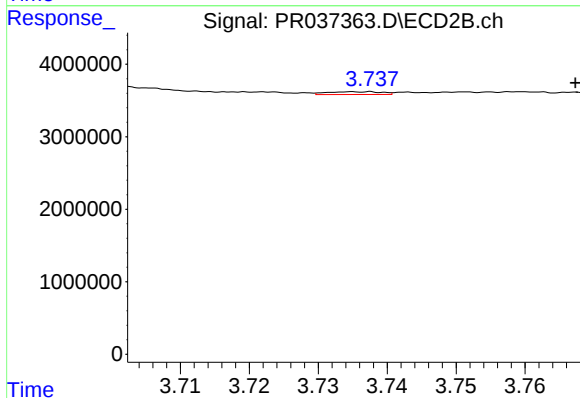


#11 AR-1232-1

R.T.: 3.737 min
Delta R.T.: -0.030 min
Response: 215878
Conc: 1.85 ng/ml

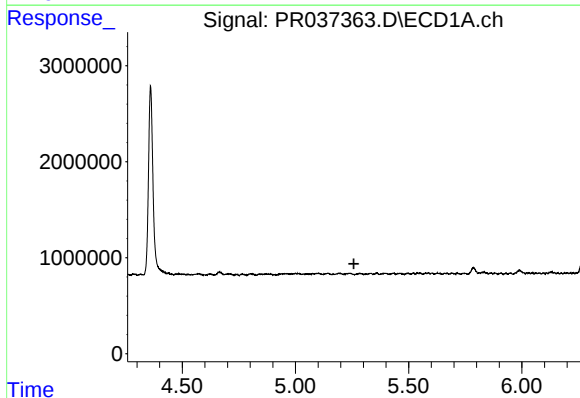


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

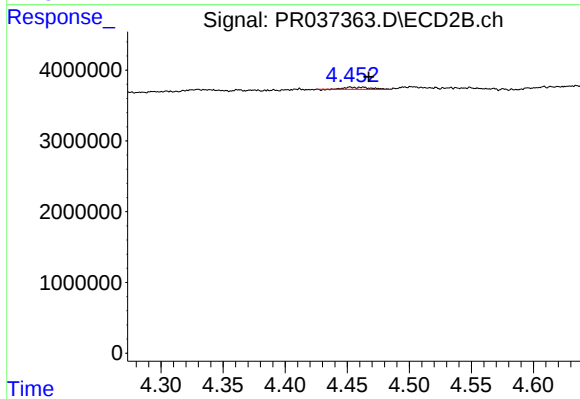

#12 AR-1232-2


R.T.: 4.452 min
Delta R.T.: -0.015 min
Response: 418437
Conc: 3.03 ng/ml

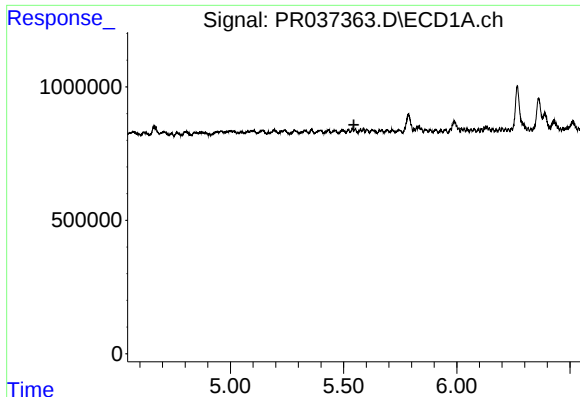

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

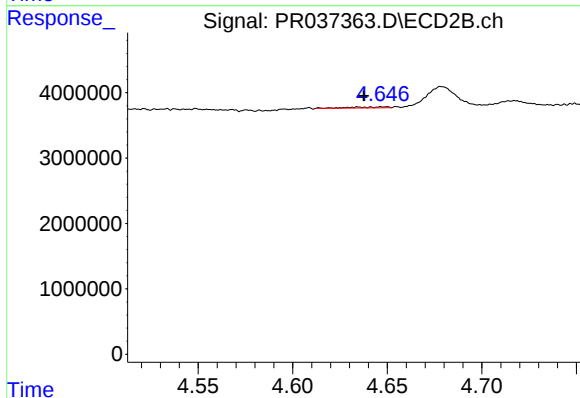


#13 AR-1232-3

R.T.: 4.647 min
Delta R.T.: 0.009 min
Response: 177022
Conc: 2.52 ng/ml

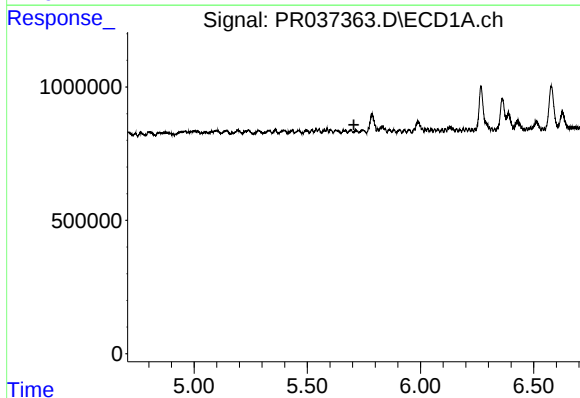


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

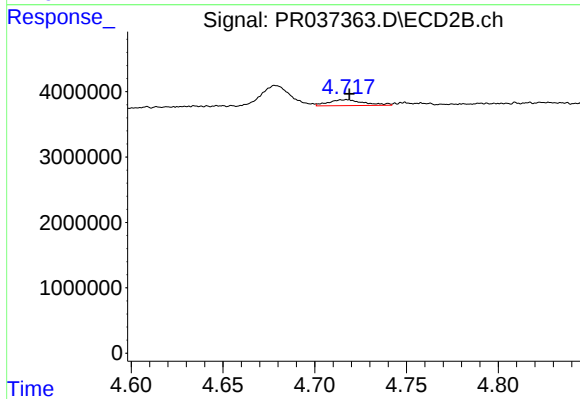

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 1196954
Conc: 20.06 ng/ml

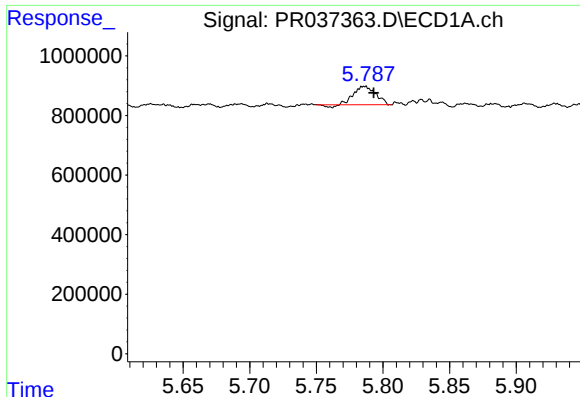

#15 AR-1232-5


R.T.: 5.786 min
Delta R.T.: -0.007 min
Response: 686676
Conc: 58.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

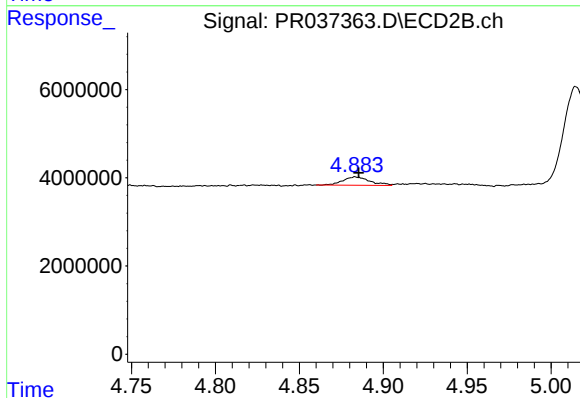


#15 AR-1232-5

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2132775
Conc: 31.25 ng/ml

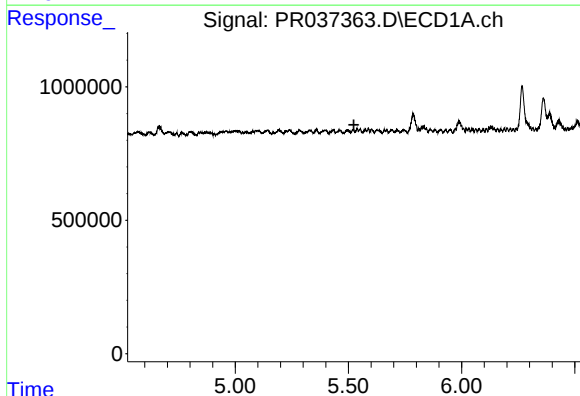


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

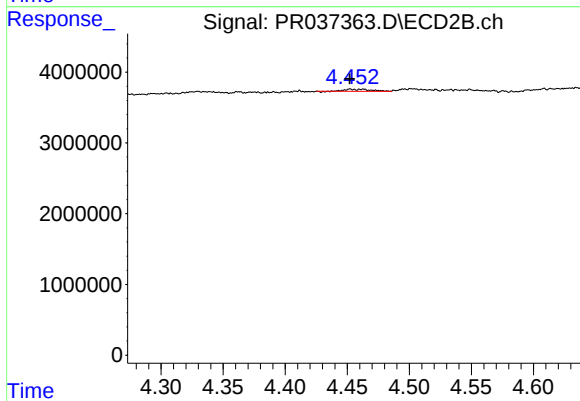

#16 AR-1242-1


R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 418437
Conc: 2.86 ng/ml

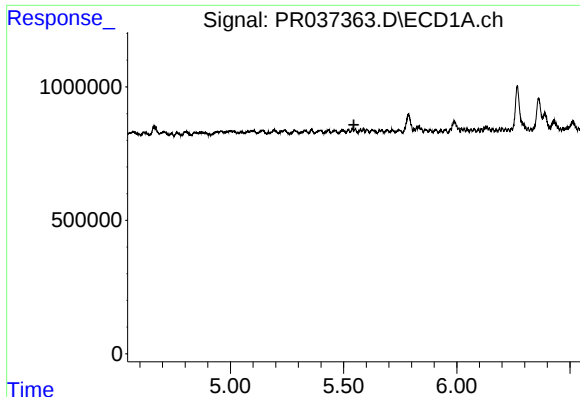

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

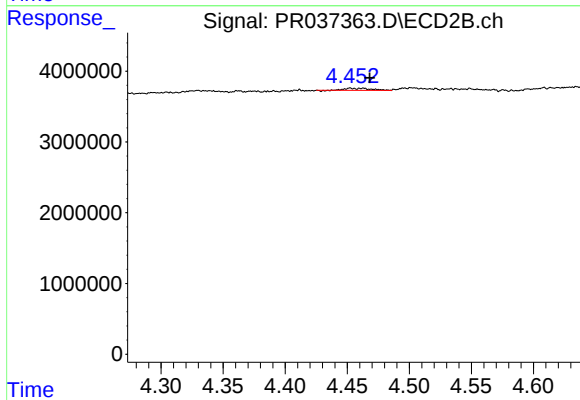


#17 AR-1242-2

R.T.: 4.452 min
Delta R.T.: -0.016 min
Response: 418437
Conc: 1.83 ng/ml

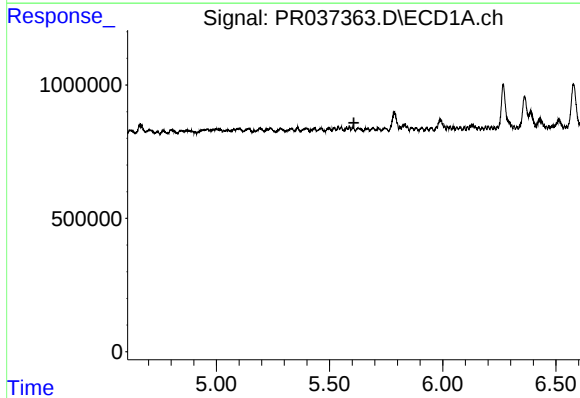


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

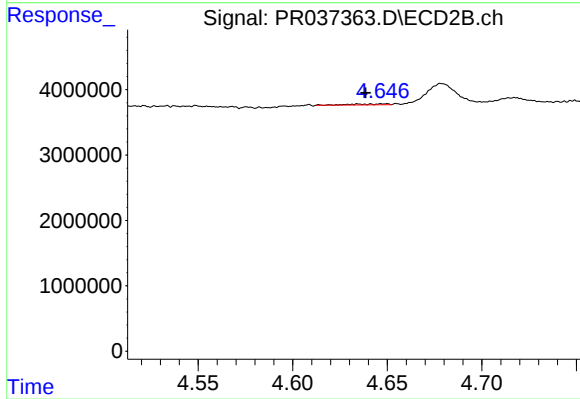

#18 AR-1242-3


R.T.: 4.647 min
Delta R.T.: 0.008 min
Response: 177022
Conc: 1.53 ng/ml

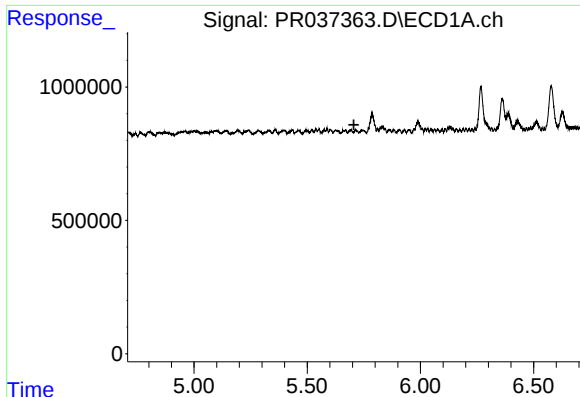

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

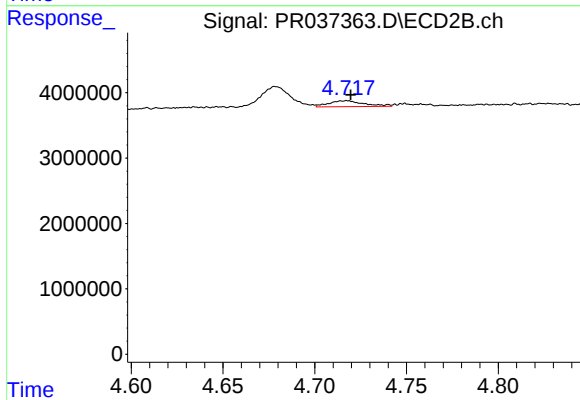


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 1196954
Conc: 10.89 ng/ml

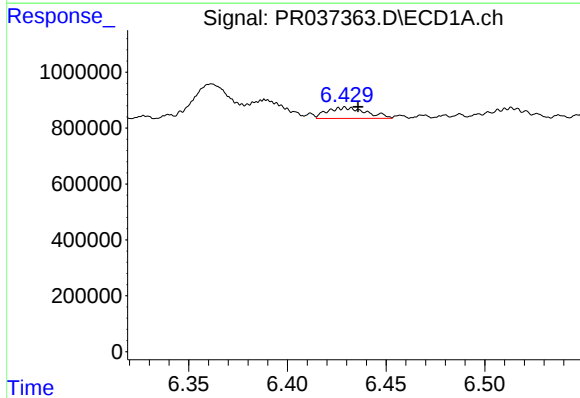


#20 AR-1242-5

R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 538625
Conc: 16.74 ng/ml

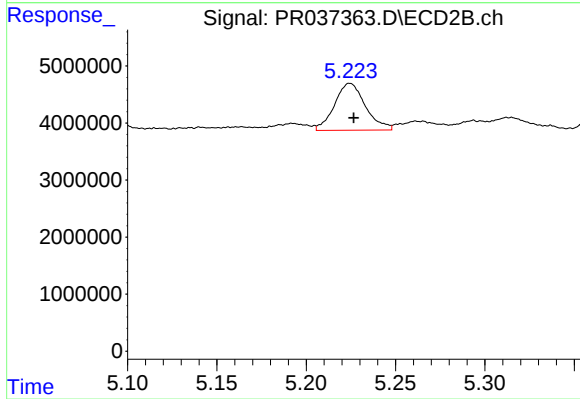

#20 AR-1242-5


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 9917316
Conc: 59.85 ng/ml

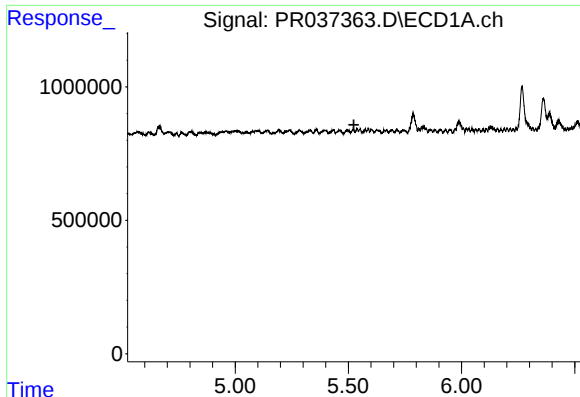

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

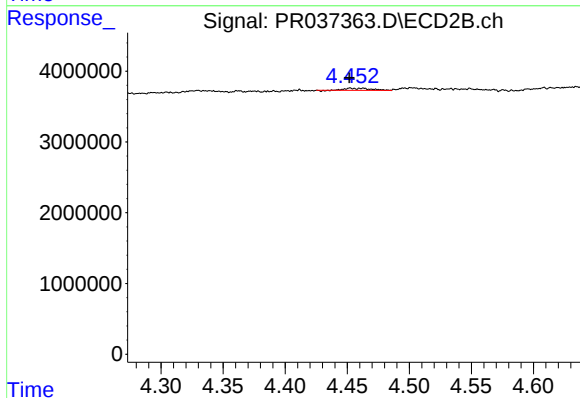


#21 AR-1248-1

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 418437
Conc: 4.16 ng/ml

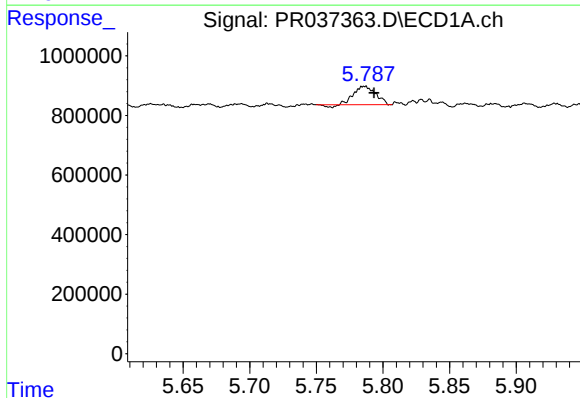


#22 AR-1248-2

R.T.: 5.786 min
Delta R.T.: -0.008 min
Response: 686676
Conc: 19.61 ng/ml

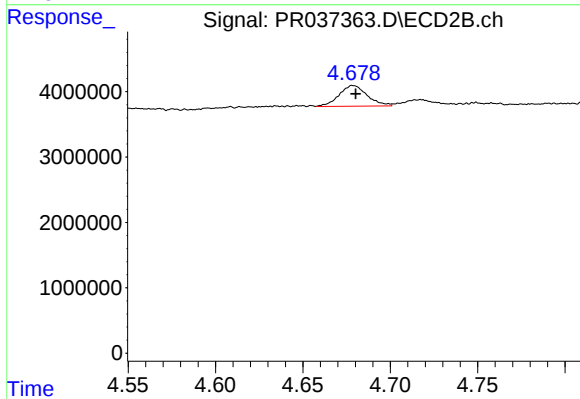

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: -0.002 min
Response: 3553215
Conc: 26.04 ng/ml

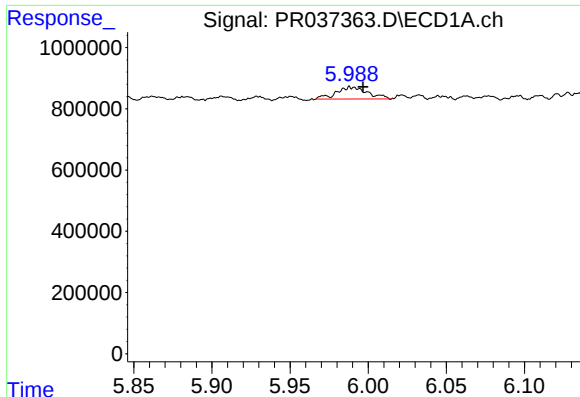

#23 AR-1248-3


R.T.: 5.989 min
Delta R.T.: -0.007 min
Response: 549031
Conc: 13.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

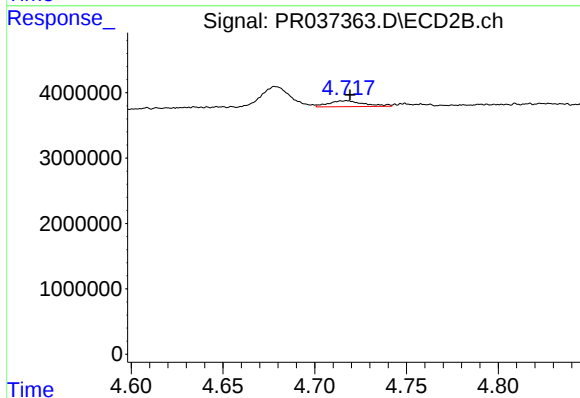


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 1196954
Conc: 8.55 ng/ml

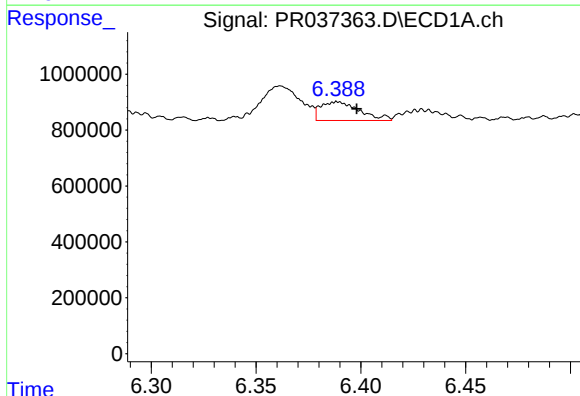


#24 AR-1248-4

R.T.: 6.389 min
Delta R.T.: -0.009 min
Response: 865003
Conc: 17.67 ng/ml

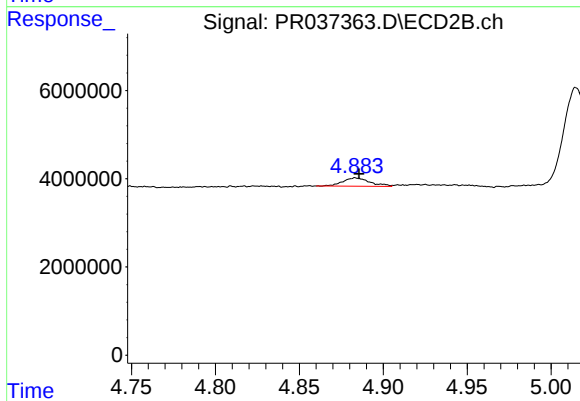

#24 AR-1248-4


R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 2132775
Conc: 11.98 ng/ml

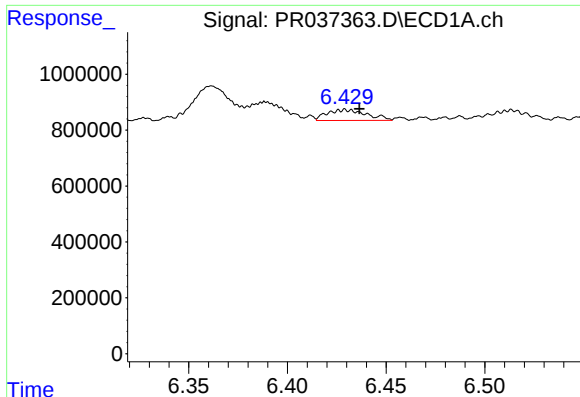

#25 AR-1248-5


R.T.: 6.429 min
Delta R.T.: -0.007 min
Response: 538625
Conc: 11.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

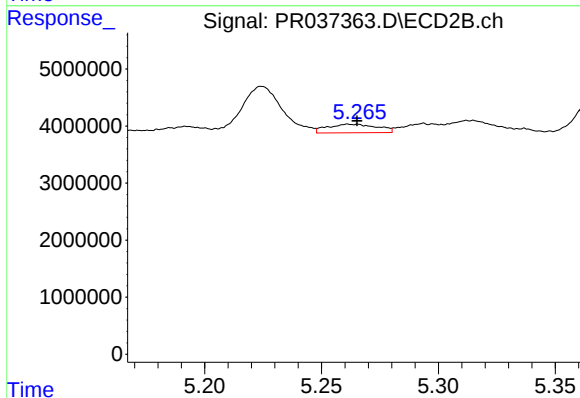


#25 AR-1248-5

R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 2228422
Conc: 11.39 ng/ml

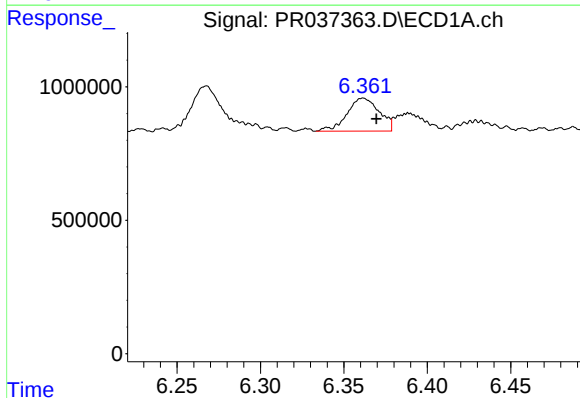


#26 AR-1254-1

R.T.: 6.361 min
Delta R.T.: -0.008 min
Response: 1656495
Conc: 30.32 ng/ml

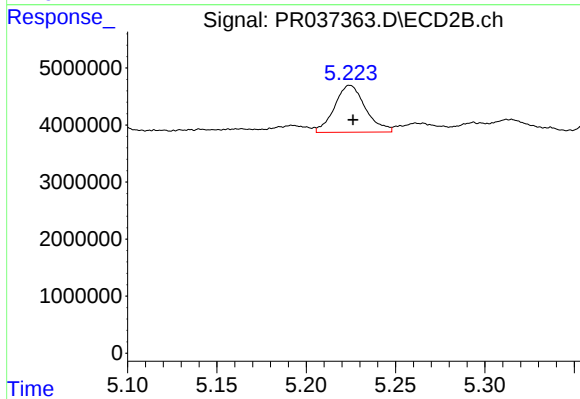

#26 AR-1254-1


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 9917316
Conc: 28.79 ng/ml

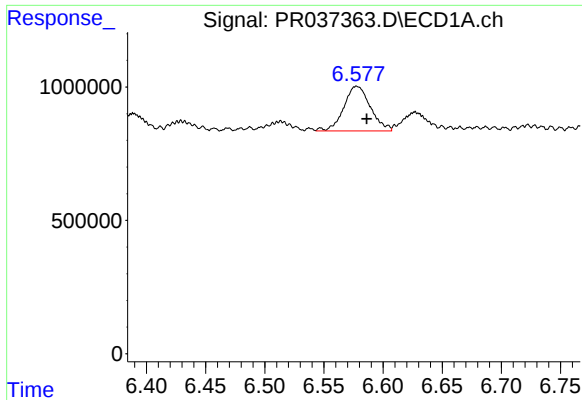

#27 AR-1254-2


R.T.: 6.578 min
Delta R.T.: -0.008 min
Response: 2622336
Conc: 30.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

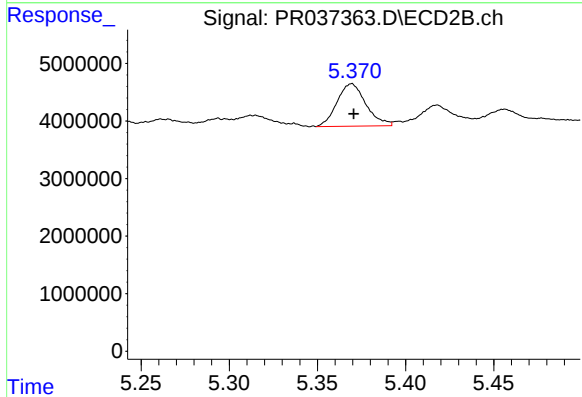


#27 AR-1254-2

R.T.: 5.370 min
Delta R.T.: -0.001 min
Response: 8411966
Conc: 28.09 ng/ml

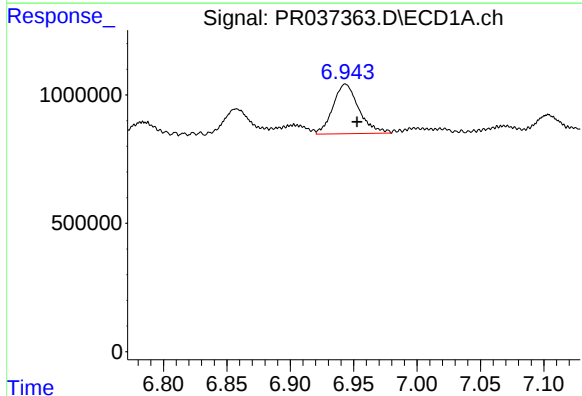


#28 AR-1254-3

R.T.: 6.944 min
Delta R.T.: -0.009 min
Response: 2744077
Conc: 30.17 ng/ml

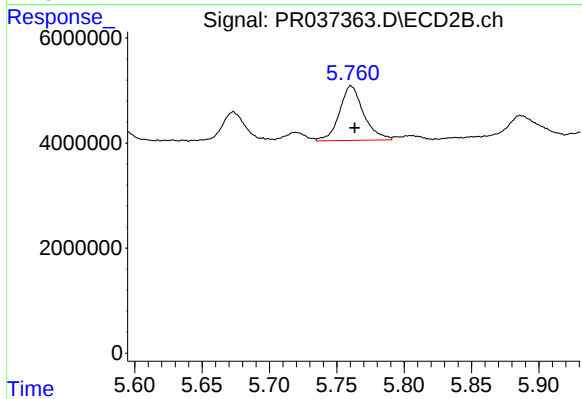

#28 AR-1254-3


R.T.: 5.760 min
Delta R.T.: -0.003 min
Response: 12974933
Conc: 27.40 ng/ml

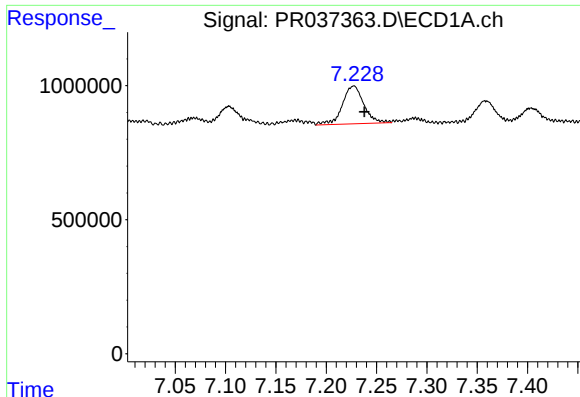

#29 AR-1254-4


R.T.: 7.228 min
Delta R.T.: -0.010 min
Response: 2088179
Conc: 31.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

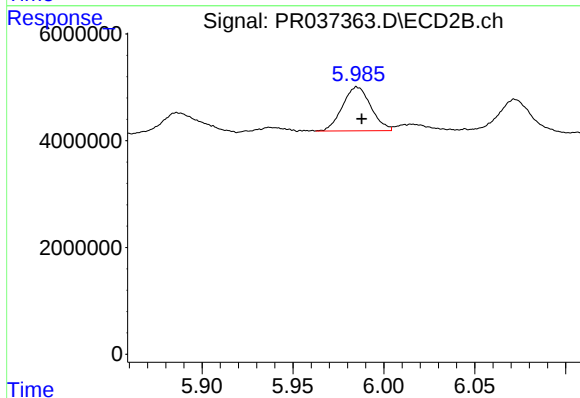


#29 AR-1254-4

R.T.: 5.985 min
Delta R.T.: -0.003 min
Response: 8917825
Conc: 25.43 ng/ml

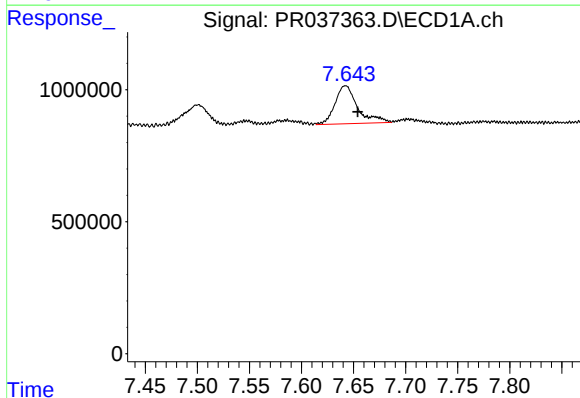


#30 AR-1254-5

R.T.: 7.642 min
Delta R.T.: -0.012 min
Response: 2171570
Conc: 30.21 ng/ml

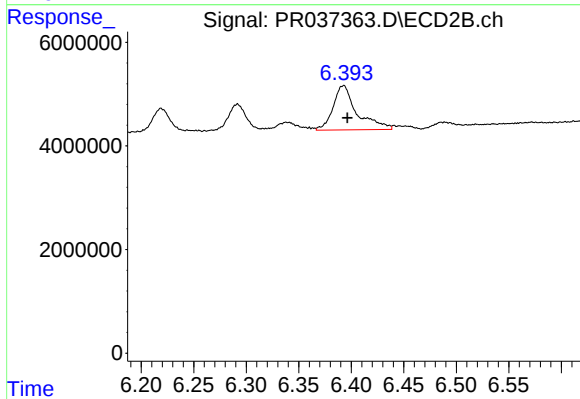

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 13587787
Conc: 30.68 ng/ml

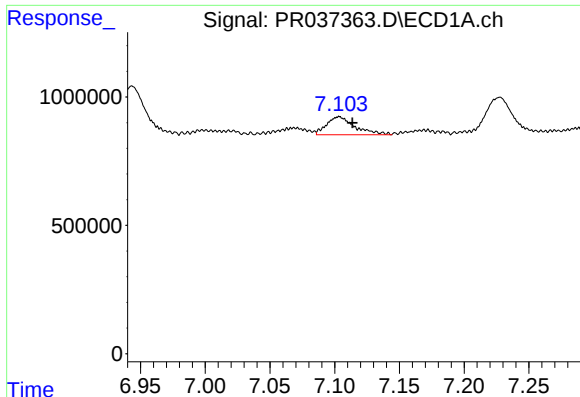

#31 AR-1260-1


R.T.: 7.103 min
Delta R.T.: -0.010 min
Response: 1063609
Conc: 16.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

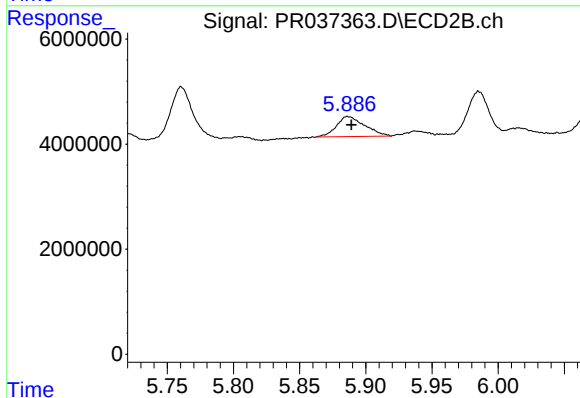


#31 AR-1260-1

R.T.: 5.886 min
Delta R.T.: -0.003 min
Response: 5686042
Conc: 19.45 ng/ml

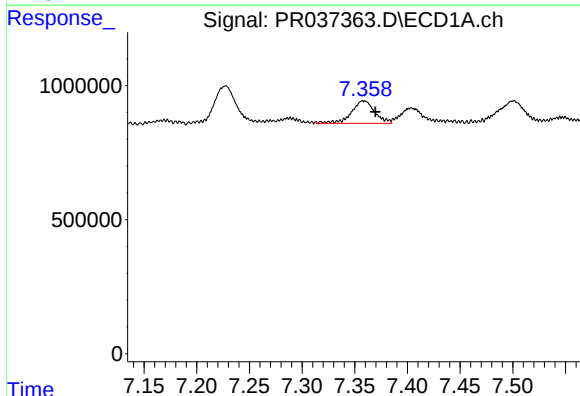


#32 AR-1260-2

R.T.: 7.358 min
Delta R.T.: -0.011 min
Response: 1297521
Conc: 16.28 ng/ml

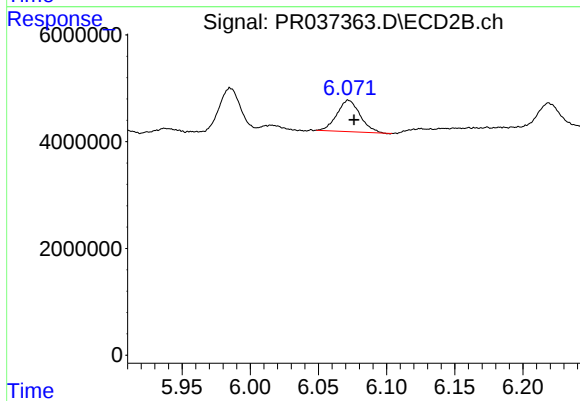

#32 AR-1260-2


R.T.: 6.072 min
Delta R.T.: -0.004 min
Response: 6916337
Conc: 15.02 ng/ml

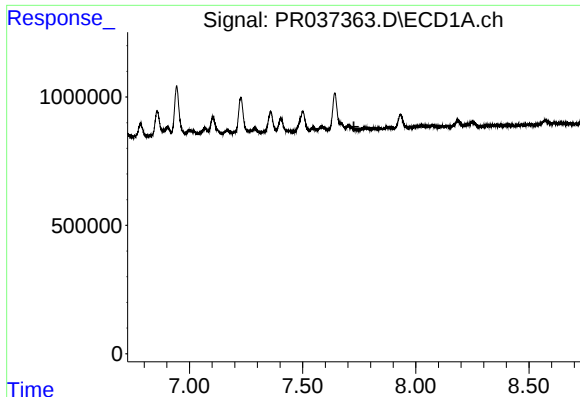

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

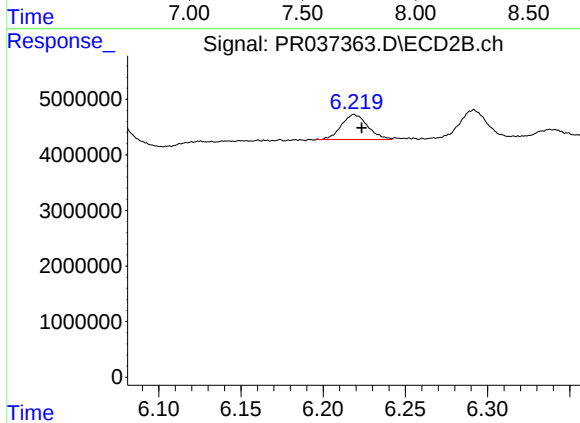


#33 AR-1260-3

R.T.: 6.219 min
Delta R.T.: -0.005 min
Response: 5021907
Conc: 14.09 ng/ml

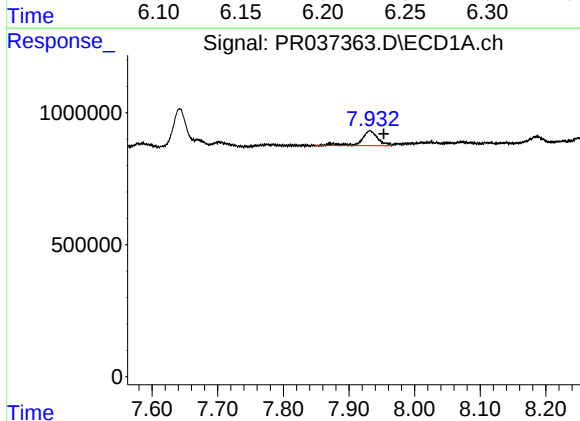


#34 AR-1260-4

R.T.: 7.932 min
Delta R.T.: -0.021 min
Response: 994475
Conc: 13.37 ng/ml

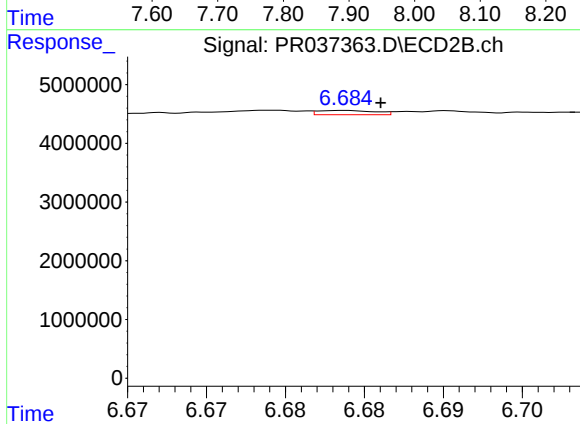

#34 AR-1260-4


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 181263
Conc: 0.59 ng/ml

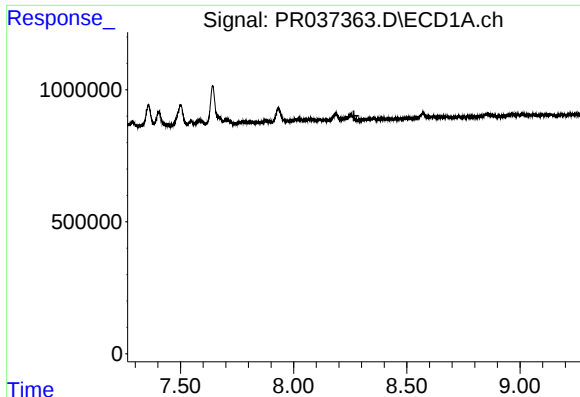

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

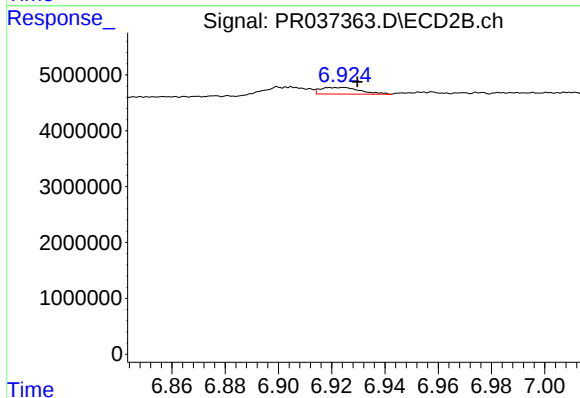


#35 AR-1260-5

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 1246970
Conc: 1.44 ng/ml

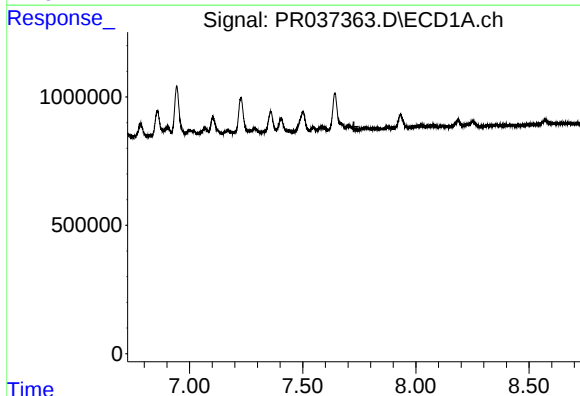


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

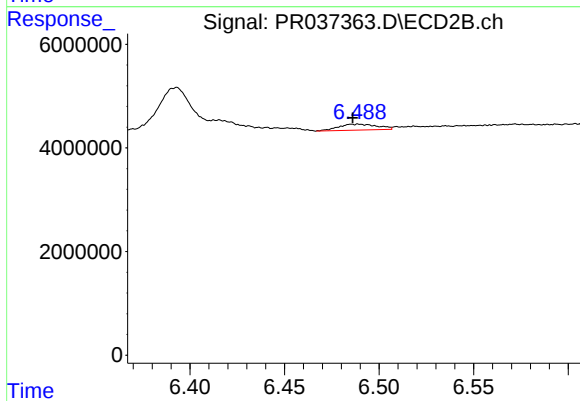

#36 AR-1262-1


R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 1650744
Conc: 6.59 ng/ml

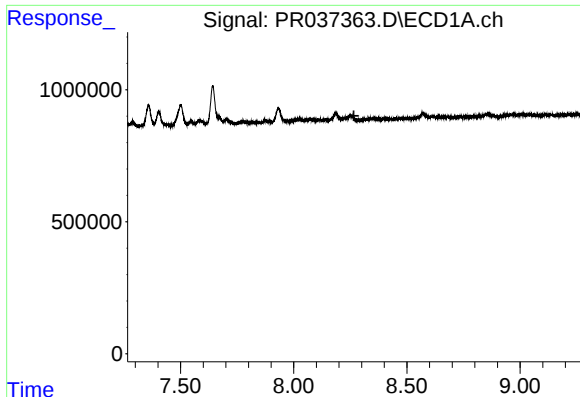

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

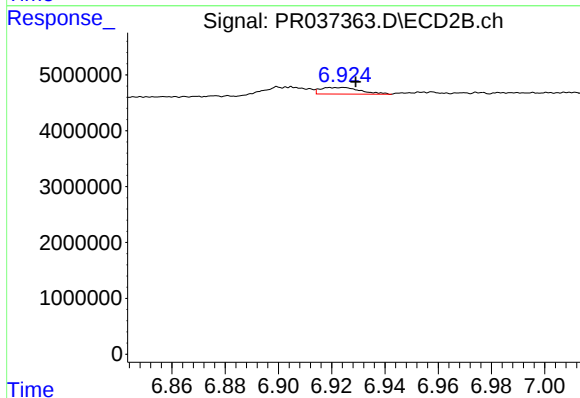


#37 AR-1262-2

R.T.: 6.924 min
Delta R.T.: -0.005 min
Response: 1246970
Conc: 0.99 ng/ml

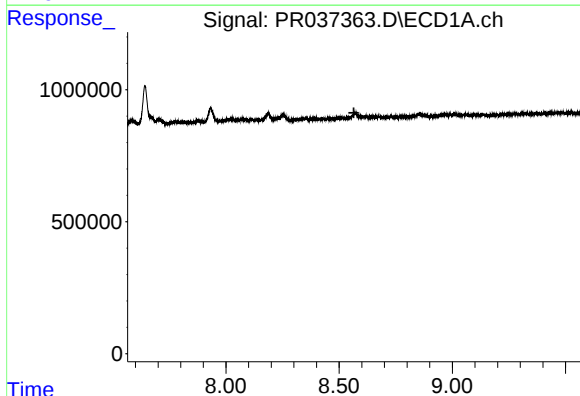


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.565 min
Response: 0
Conc: N.D.

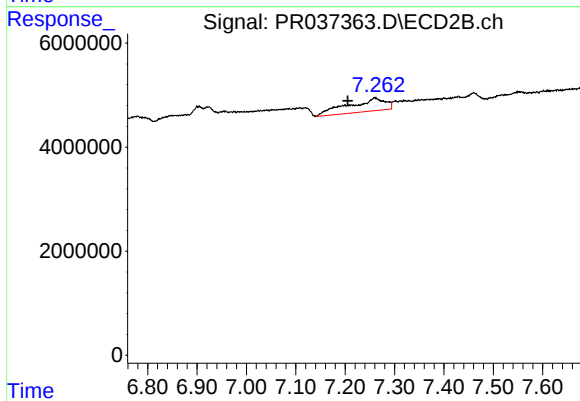

#38 AR-1262-3


R.T.: 7.260 min
Delta R.T.: 0.054 min
Response: 13256604
Conc: 24.18 ng/ml

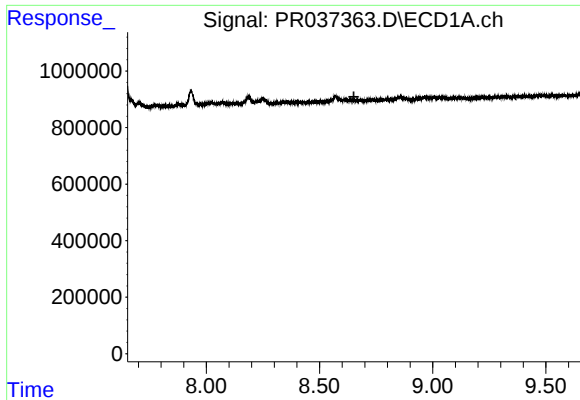

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

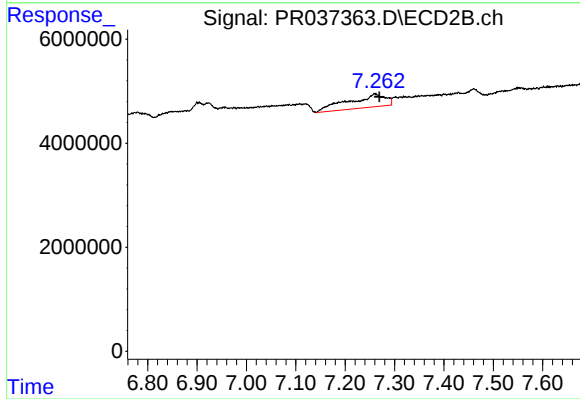


#39 AR-1262-4

R.T.: 7.260 min
Delta R.T.: -0.010 min
Response: 13256604
Conc: 14.77 ng/ml

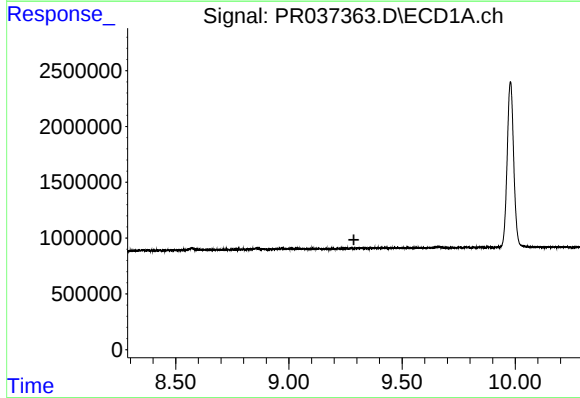


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

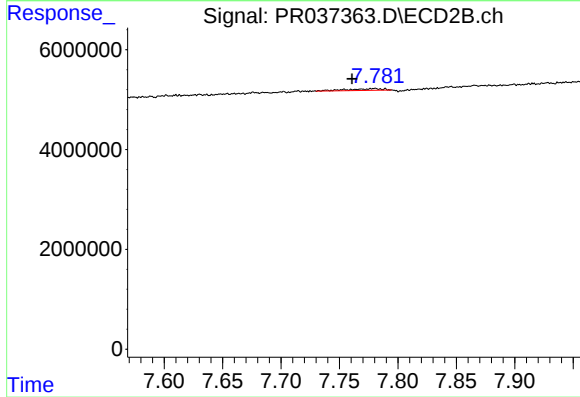

#40 AR-1262-5


R.T.: 7.780 min
Delta R.T.: 0.019 min
Response: 699444
Conc: 1.83 ng/ml

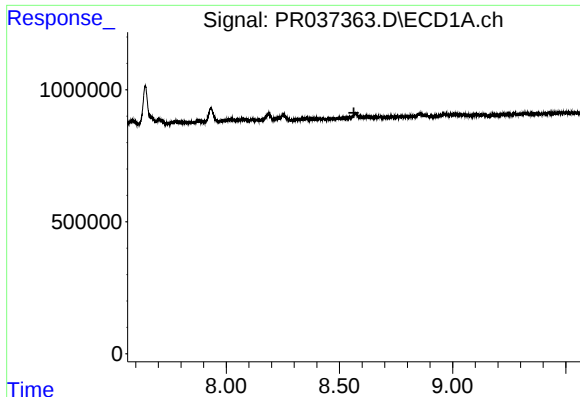

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

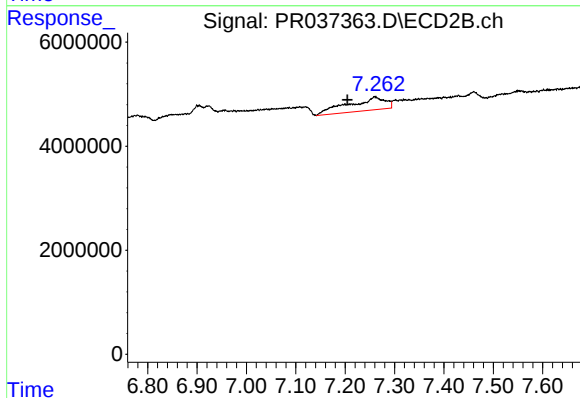


#41 AR-1268-1

R.T.: 7.260 min
Delta R.T.: 0.055 min
Response: 13256604
Conc: 10.77 ng/ml

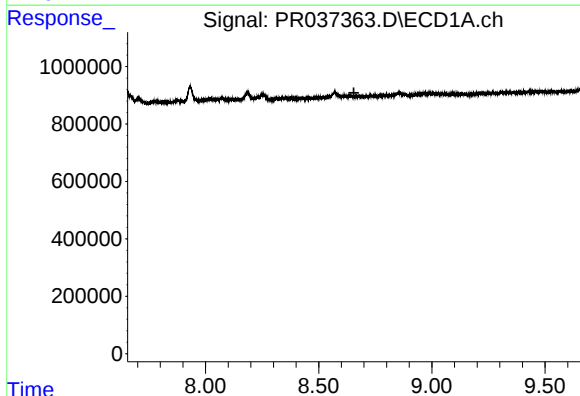


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.655 min
Response: 0
Conc: N.D.

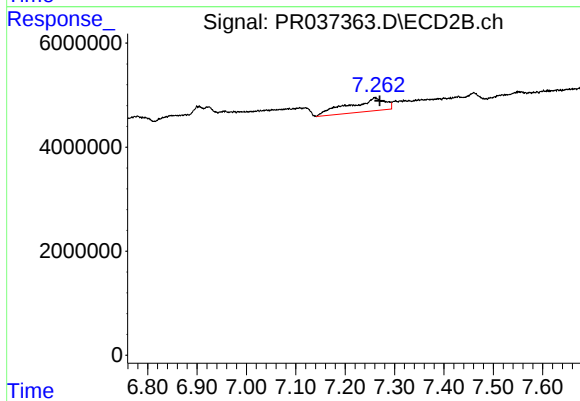

#42 AR-1268-2


R.T.: 7.260 min
Delta R.T.: -0.011 min
Response: 13256604
Conc: 12.52 ng/ml

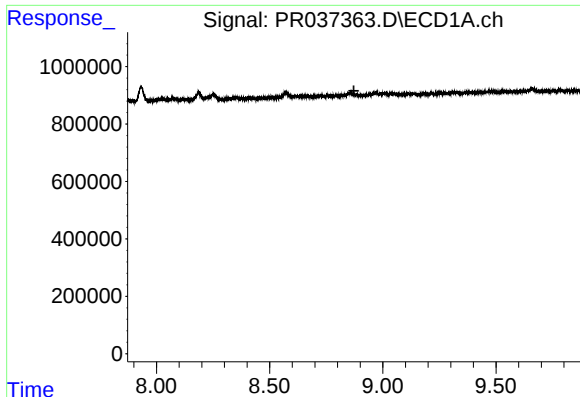

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

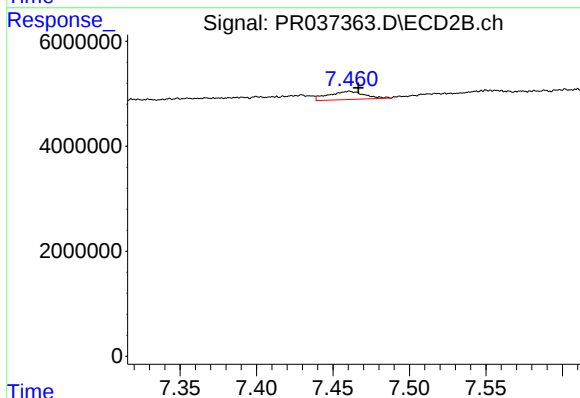


#43 AR-1268-3

R.T.: 7.461 min
Delta R.T.: -0.006 min
Response: 2546651
Conc: 2.87 ng/ml

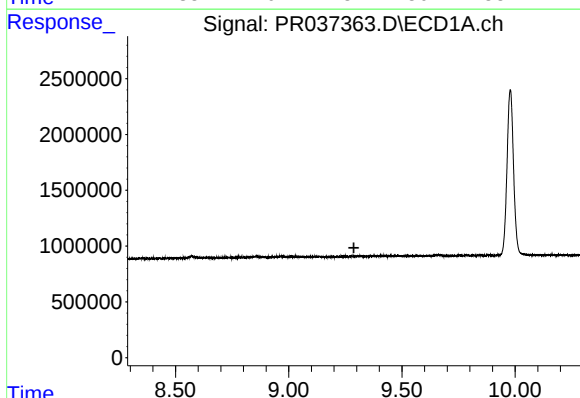


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

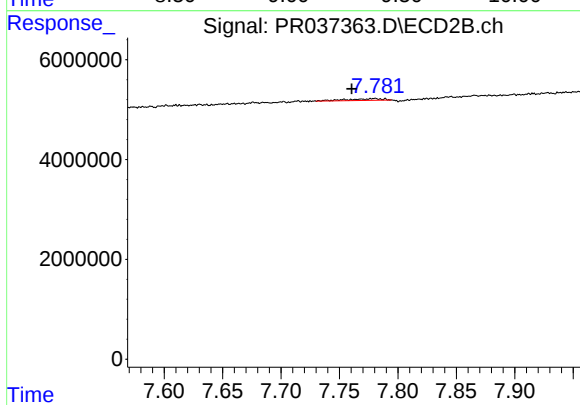

#44 AR-1268-4


R.T.: 7.780 min
Delta R.T.: 0.020 min
Response: 699444
Conc: 1.93 ng/ml

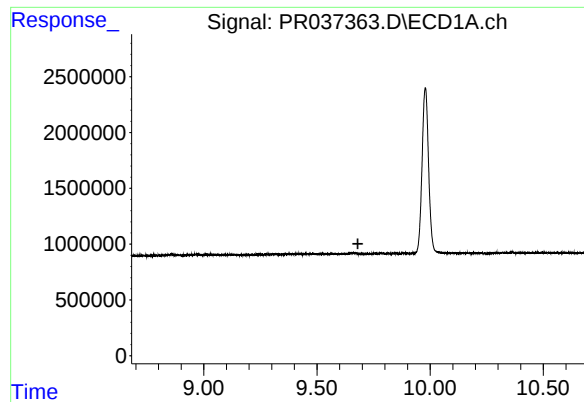

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

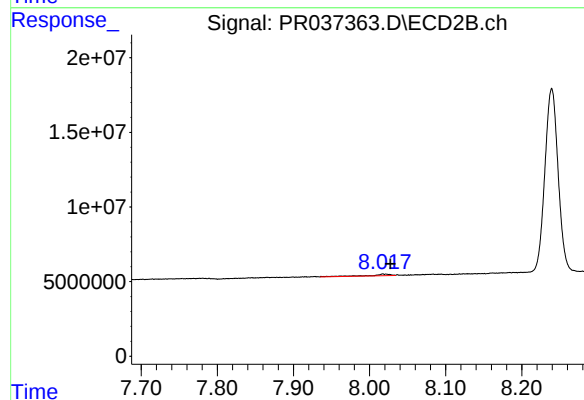

#45 AR-1268-5

R.T.: 8.018 min
Delta R.T.: -0.010 min
Response: 2157387
Conc: 0.85 ng/ml