

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 18:18
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1254 LOD 40PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:06:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	25729239	104.0E6	20.567	21.693
2)	SA Decachlor...	9.984	8.244	26998746	137.8E6	20.414	23.663
Target Compounds							
3)	L1 AR-1016-1	0.000	4.451	0	331692	N.D.	1.822 #
4)	L1 AR-1016-2	0.000	4.464	0	376397	N.D.	1.334 #
5)	L1 AR-1016-3	0.000	4.640	0	127169	N.D.	0.884 #
6)	L1 AR-1016-4	0.000	4.679	0	5349514	N.D.	48.353 #
7)	L1 AR-1016-5	5.990	4.884	1029045	3248604	30.010	21.371 #
8)	L2 AR-1221-1	0.000	3.573	0	397983	N.D.	7.816 #
9)	L2 AR-1221-2	4.664	3.698	566171	1744362	62.602	46.973
10)	L2 AR-1221-3	4.664	3.742	566171	232669	18.473	1.900 #
11)	L3 AR-1232-1	4.664	3.742	566171	232669	19.356	1.989 #
12)	L3 AR-1232-2	0.000	4.464	0	376397	N.D.	2.723 #
13)	L3 AR-1232-3	0.000	4.640	0	127169	N.D.	1.811 #
14)	L3 AR-1232-4	0.000	4.718	0	1588283	N.D.	26.617 #
15)	L3 AR-1232-5	5.788	4.884	1444551	3248604	123.512	47.603 #
16)	L4 AR-1242-1	0.000	4.451	0	331692	N.D.	2.264 #
17)	L4 AR-1242-2	0.000	4.464	0	376397	N.D.	1.650 #
18)	L4 AR-1242-3	0.000	4.640	0	127169	N.D.	1.100 #
19)	L4 AR-1242-4	0.000	4.718	0	1588283	N.D.	14.451 #
20)	L4 AR-1242-5	6.431	5.224	938662	15769012	29.170	95.166 #
21)	L5 AR-1248-1	0.000	4.451	0	331692	N.D.	3.295 #
22)	L5 AR-1248-2	5.788	4.679	1444551	5349514	41.256	39.198
23)	L5 AR-1248-3	5.990	4.718	1029045	1588283	25.154	11.347 #
24)	L5 AR-1248-4	6.390	4.884	1236645	3248604	25.261	18.254 #
25)	L5 AR-1248-5	6.431	5.263	938662	2744583	19.871	14.031 #
26)	L6 AR-1254-1	6.363	5.224	2568316	15769012	47.012	45.777
27)	L6 AR-1254-2	6.580	5.369	4182461	13216728	48.805	44.129
28)	L6 AR-1254-3	6.945	5.761	4430414	20246025	48.705	42.747
29)	L6 AR-1254-4	7.230	5.986	3272401	14718512	48.836	41.975
30)	L6 AR-1254-5	7.645	6.393	3783419	18005402	52.635	40.660
31)	L7 AR-1260-1	7.105	5.888	1900792	8586745	28.806	29.379
32)	L7 AR-1260-2	7.360	6.074	2153000	10705941	27.013	23.244
33)	L7 AR-1260-3	7.705	6.222	524503	8492668	8.382	23.822 #
34)	L7 AR-1260-4	7.935	6.686	1254432	1101958	16.860	3.616 #
35)	L7 AR-1260-5	8.255	6.925	527373	2018821	3.647	2.328 #
36)	L8 AR-1262-1	7.705	6.491	524503	893846	5.021	3.567 #
37)	L8 AR-1262-2	8.255	6.925	527373	2018821	2.713	1.607 #
38)	L8 AR-1262-3	8.576	7.208	631782	1968358	4.804	3.590 #
39)	L8 AR-1262-4	0.000	7.265	0	5463814	N.D.	6.087 #
40)	L8 AR-1262-5	0.000	7.762	0	332462	N.D.	0.869 #
41)	L9 AR-1268-1	8.576	7.208	631782	1968358	3.528	1.599 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 18:18
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1254 LOD 40PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:06:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.265	0	5463814	N.D.	5.160 #
43) L9	AR-1268-3	0.000	7.463	0	2767051	N.D.	3.122 #
44) L9	AR-1268-4	0.000	7.762	0	332462	N.D.	0.916 #
45) L9	AR-1268-5	0.000	8.025	0	473474	N.D.	0.186 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 18:18
Operator : SM\SJ
Sample : K2241-07
Misc : AR1254 LOD 40PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:06:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

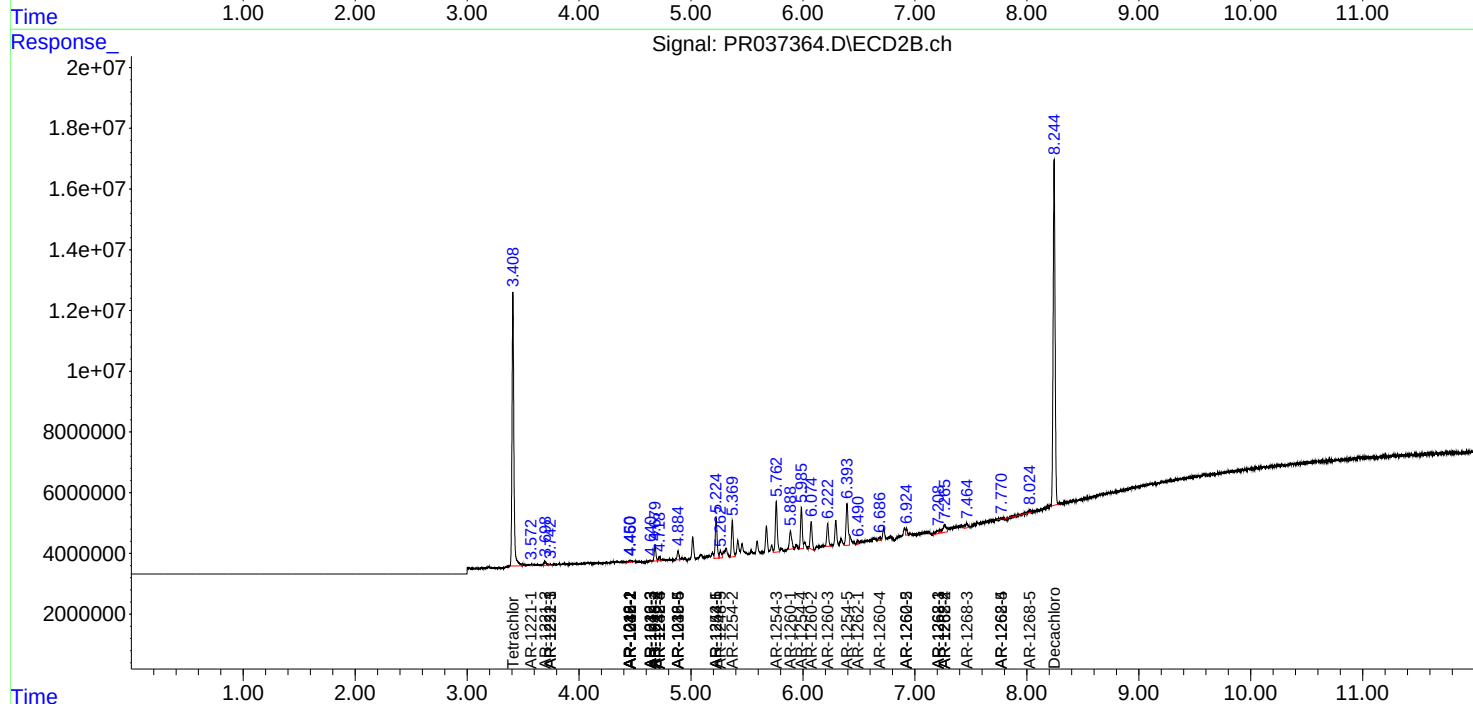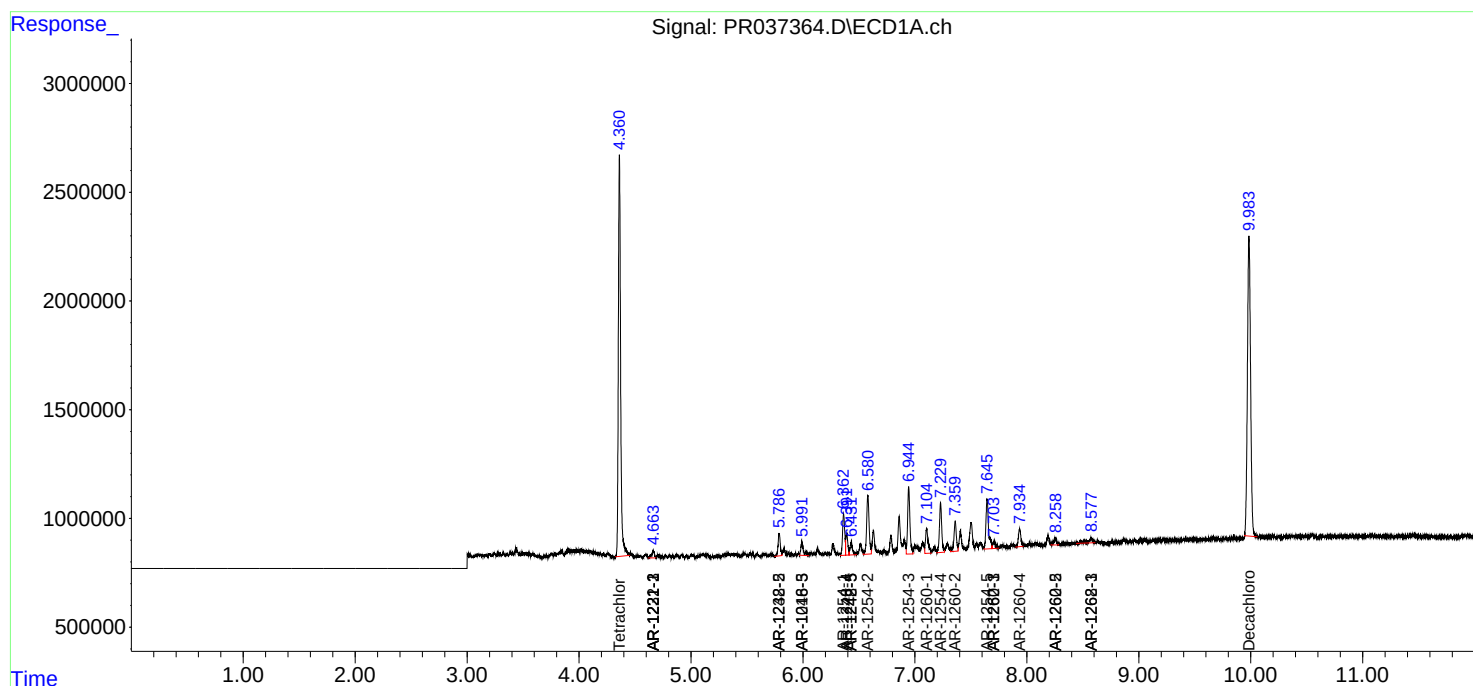


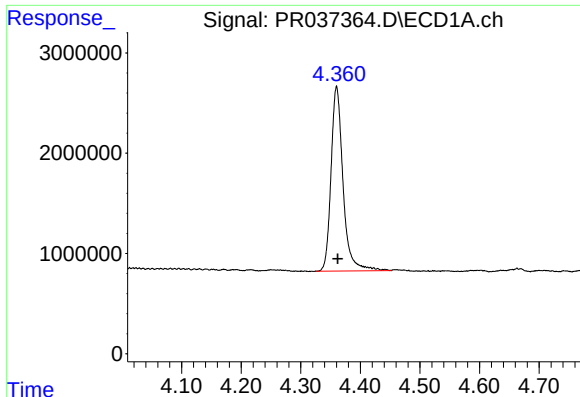

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 25729239
Conc: 20.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

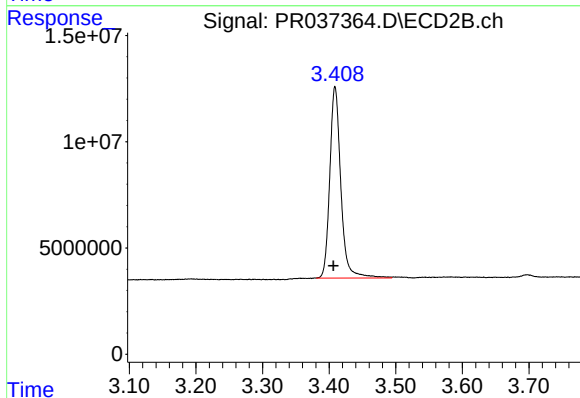


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.002 min
Response: 104028106
Conc: 21.69 ng/ml

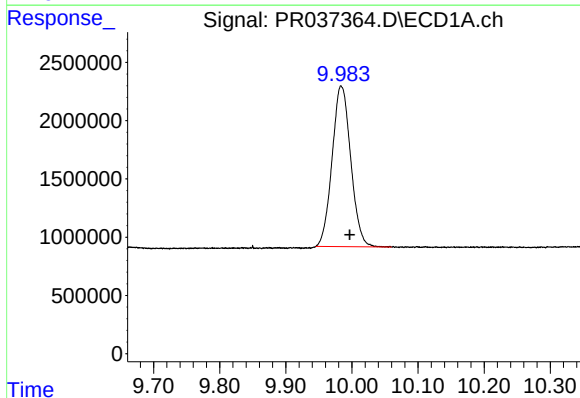


#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: -0.013 min
Response: 26998746
Conc: 20.41 ng/ml

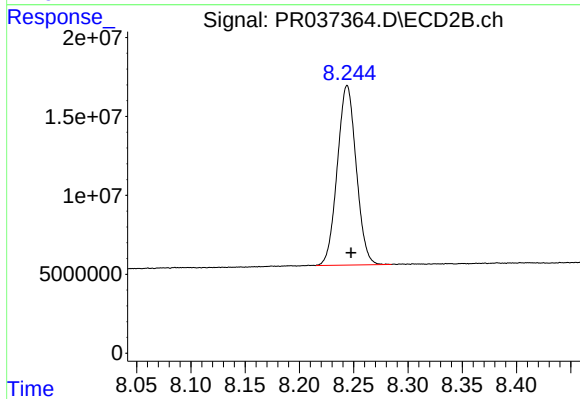

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 137821245
Conc: 23.66 ng/ml

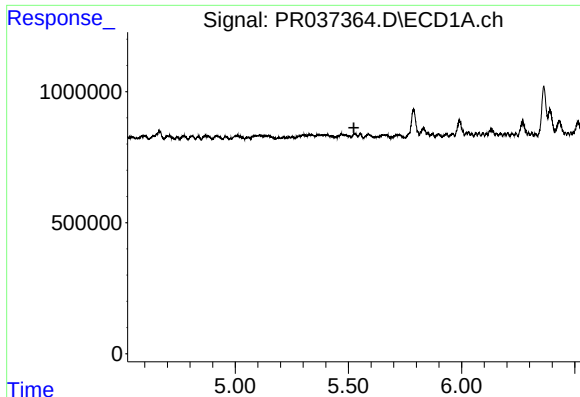

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

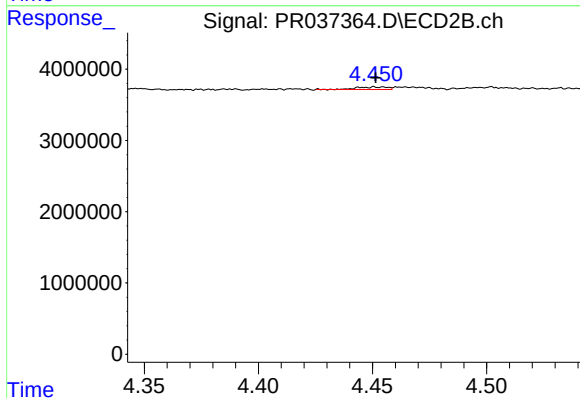


#3 AR-1016-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 331692
Conc: 1.82 ng/ml

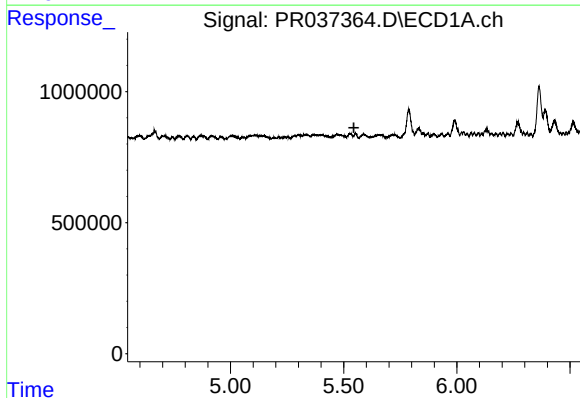


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

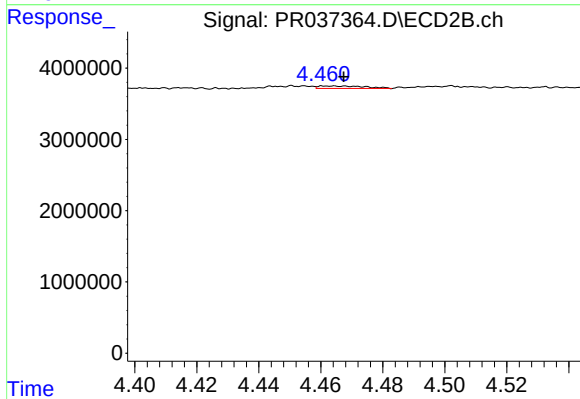

#4 AR-1016-2


R.T.: 4.464 min
Delta R.T.: -0.003 min
Response: 376397
Conc: 1.33 ng/ml

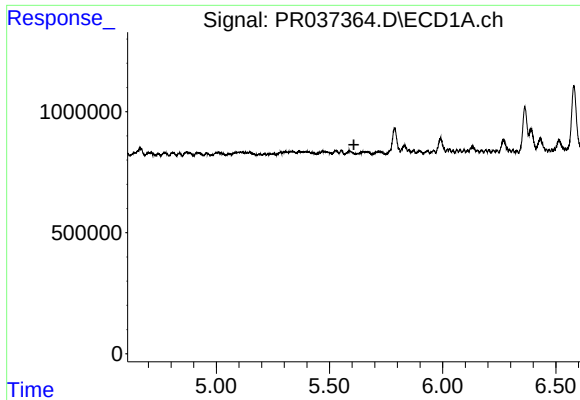

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

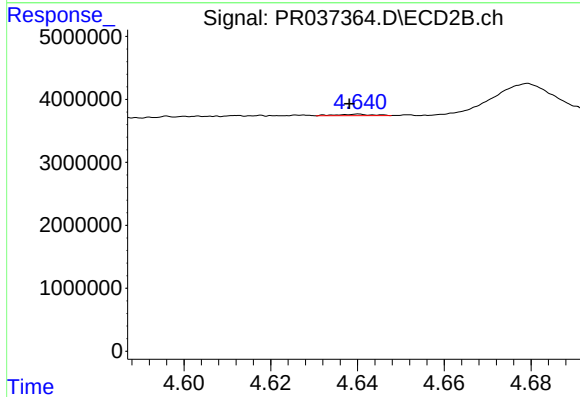


#5 AR-1016-3

R.T.: 4.640 min
Delta R.T.: 0.002 min
Response: 127169
Conc: 0.88 ng/ml

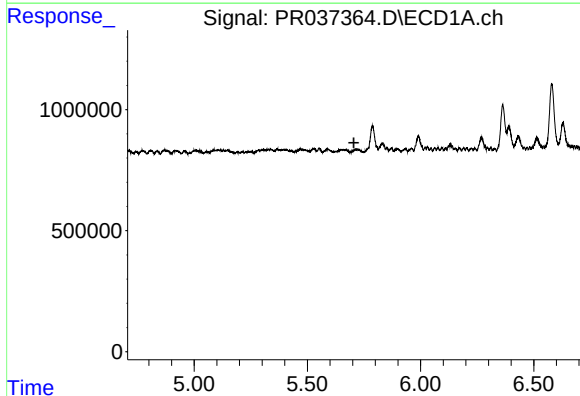


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

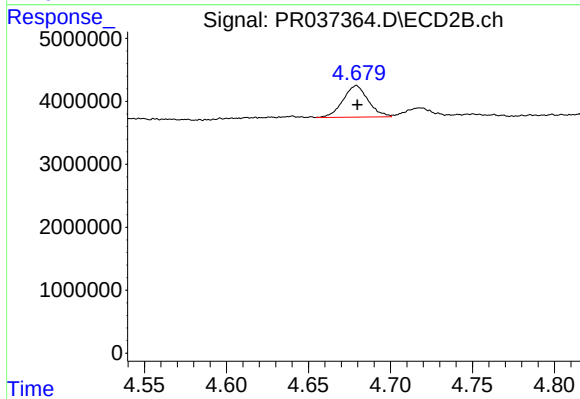

#6 AR-1016-4


R.T.: 4.679 min
Delta R.T.: 0.000 min
Response: 5349514
Conc: 48.35 ng/ml

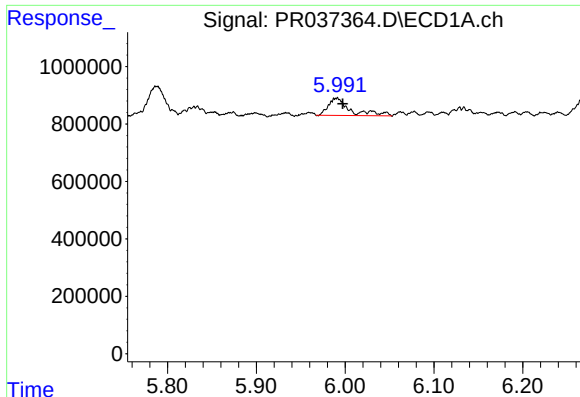

#7 AR-1016-5


R.T.: 5.990 min
Delta R.T.: -0.007 min
Response: 1029045
Conc: 30.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

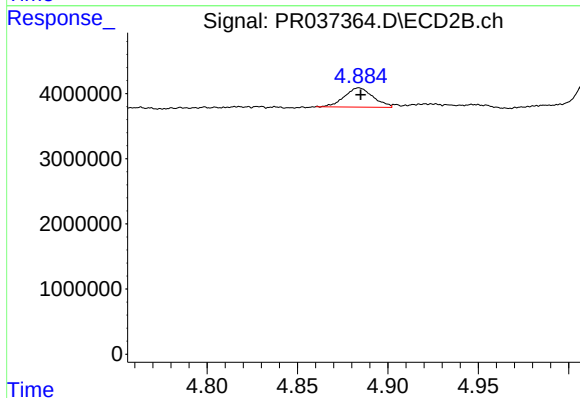


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 3248604
Conc: 21.37 ng/ml

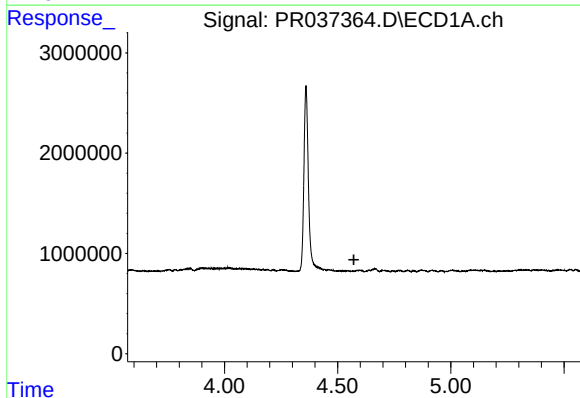


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

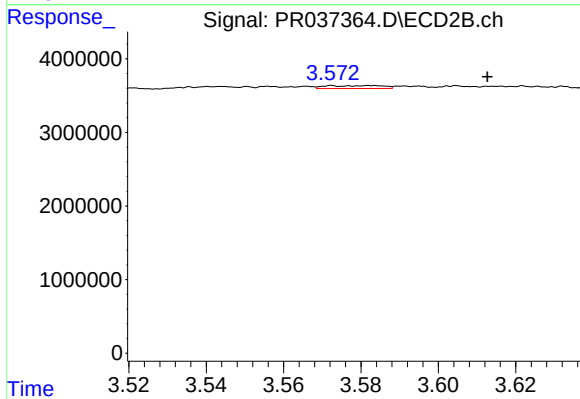

#8 AR-1221-1


R.T.: 3.573 min
Delta R.T.: -0.040 min
Response: 397983
Conc: 7.82 ng/ml

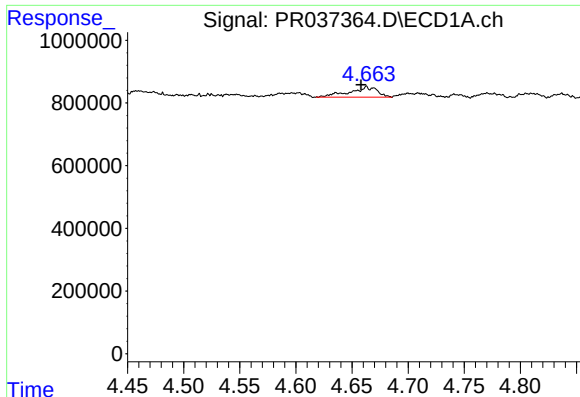

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 566171
Conc: 62.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

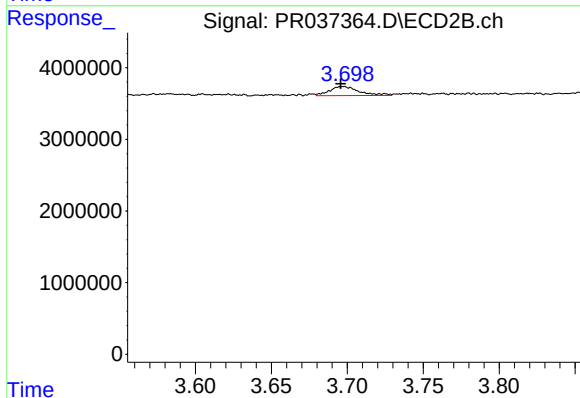


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 1744362
Conc: 46.97 ng/ml

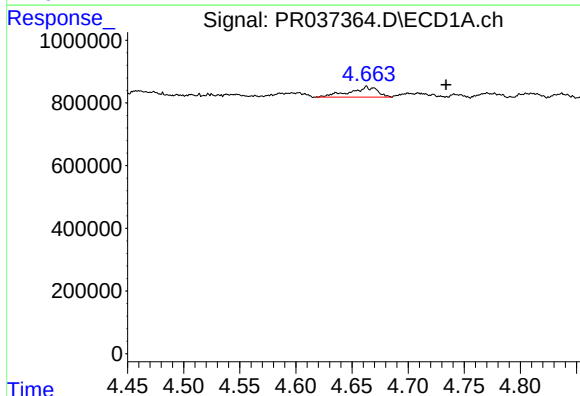


#10 AR-1221-3

R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 566171
Conc: 18.47 ng/ml

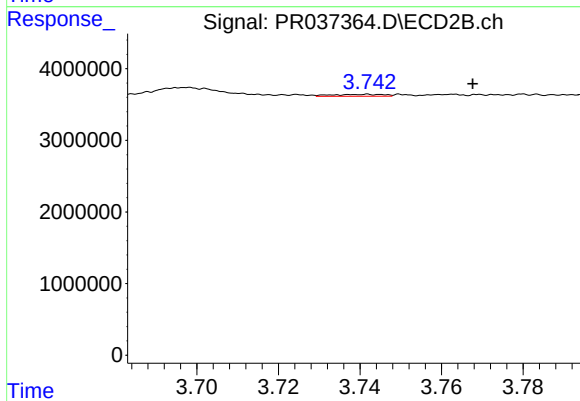

#10 AR-1221-3


R.T.: 3.742 min
Delta R.T.: -0.026 min
Response: 232669
Conc: 1.90 ng/ml

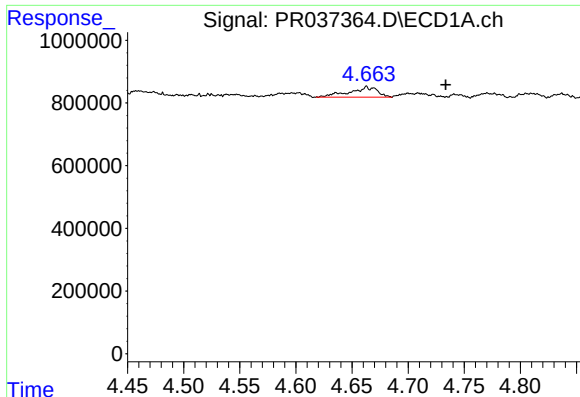

#11 AR-1232-1


R.T.: 4.664 min
Delta R.T.: -0.070 min
Response: 566171
Conc: 19.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

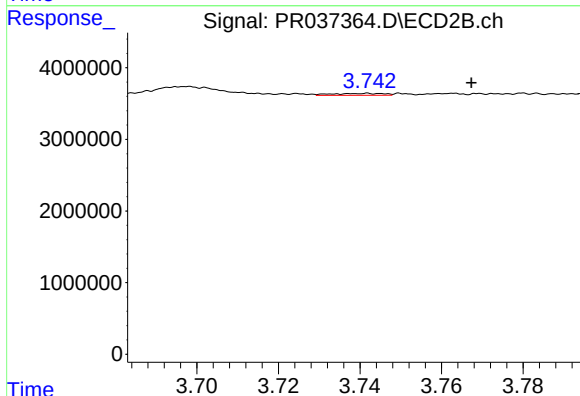


#11 AR-1232-1

R.T.: 3.742 min
Delta R.T.: -0.025 min
Response: 232669
Conc: 1.99 ng/ml

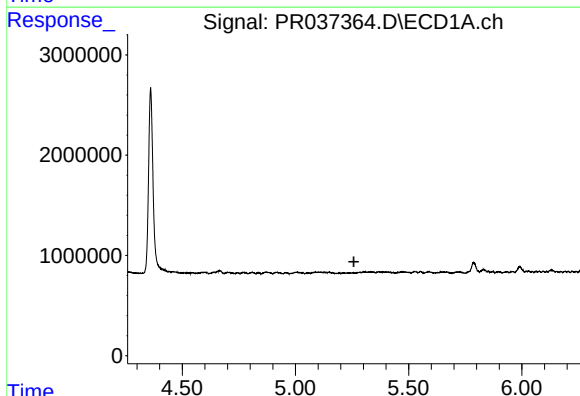


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

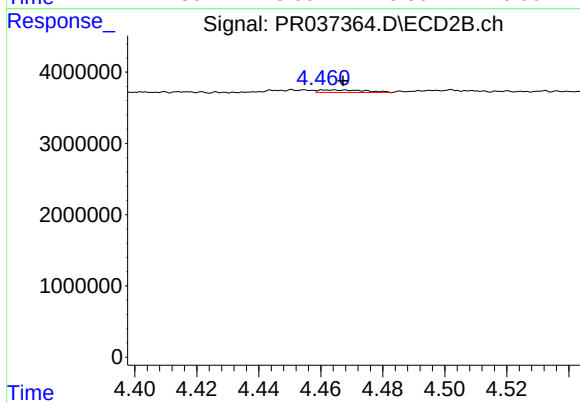

#12 AR-1232-2


R.T.: 4.464 min
Delta R.T.: -0.003 min
Response: 376397
Conc: 2.72 ng/ml

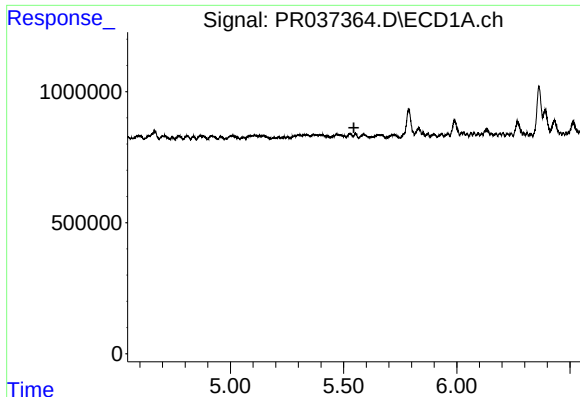

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

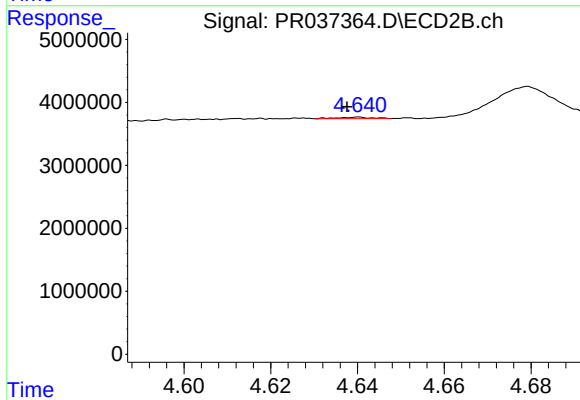


#13 AR-1232-3

R.T.: 4.640 min
Delta R.T.: 0.003 min
Response: 127169
Conc: 1.81 ng/ml

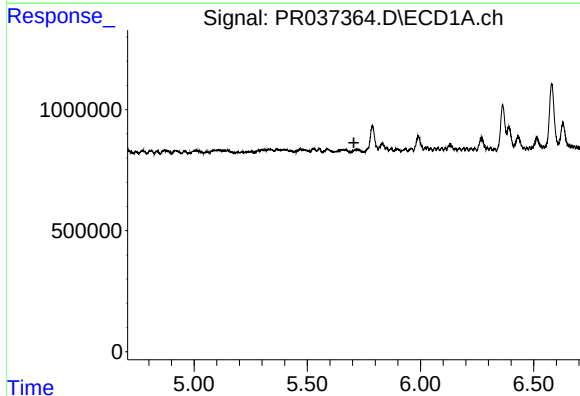


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

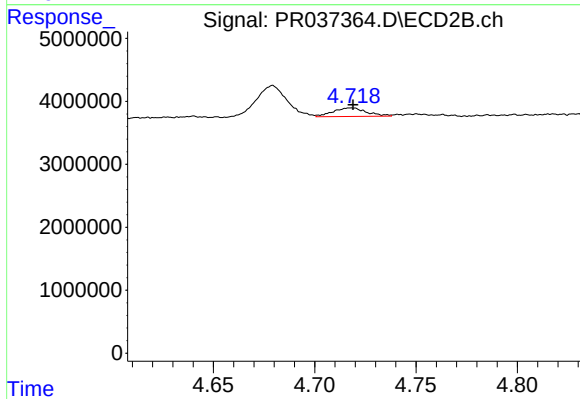

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 1588283
Conc: 26.62 ng/ml

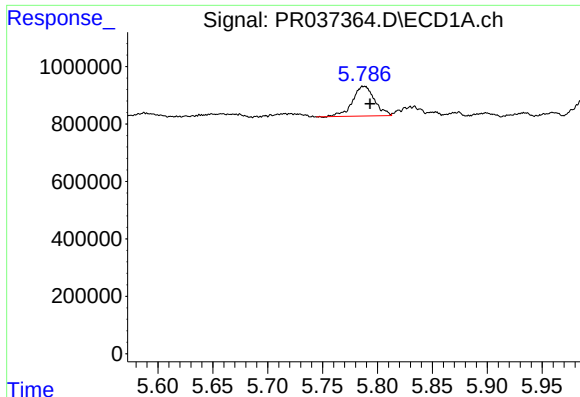

#15 AR-1232-5


R.T.: 5.788 min
Delta R.T.: -0.006 min
Response: 1444551
Conc: 123.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

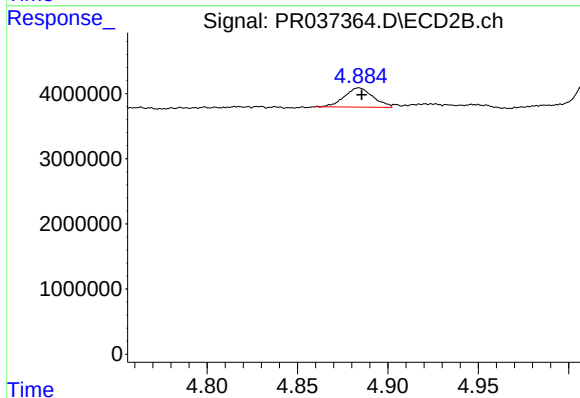


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 3248604
Conc: 47.60 ng/ml

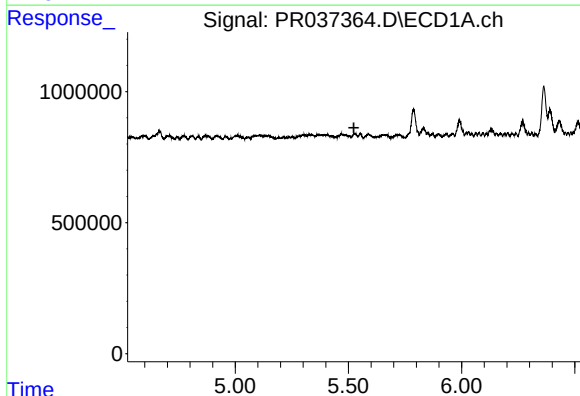


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

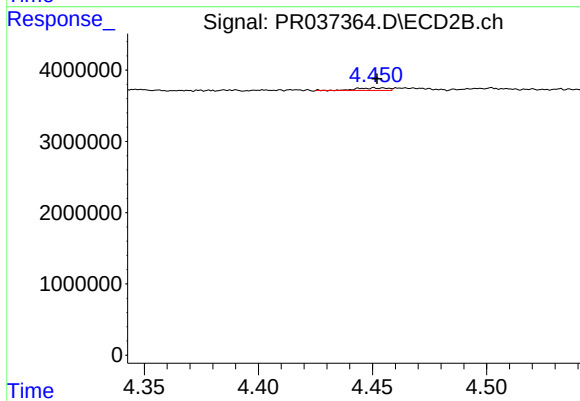

#16 AR-1242-1


R.T.: 4.451 min
Delta R.T.: -0.001 min
Response: 331692
Conc: 2.26 ng/ml

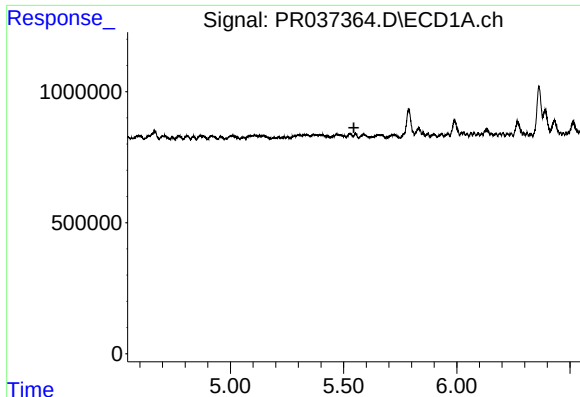

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

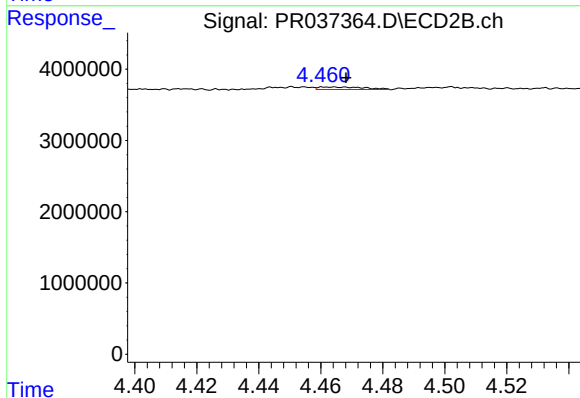


#17 AR-1242-2

R.T.: 4.464 min
Delta R.T.: -0.004 min
Response: 376397
Conc: 1.65 ng/ml

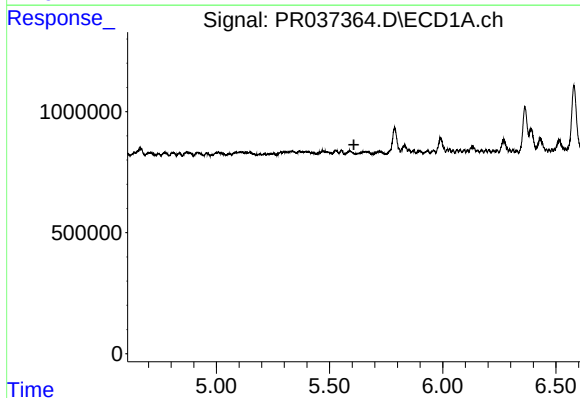


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

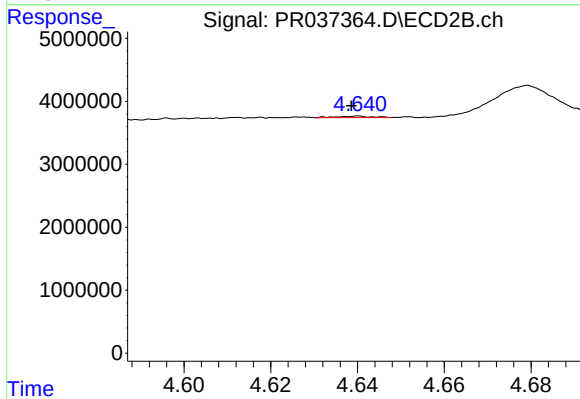

#18 AR-1242-3


R.T.: 4.640 min
Delta R.T.: 0.002 min
Response: 127169
Conc: 1.10 ng/ml

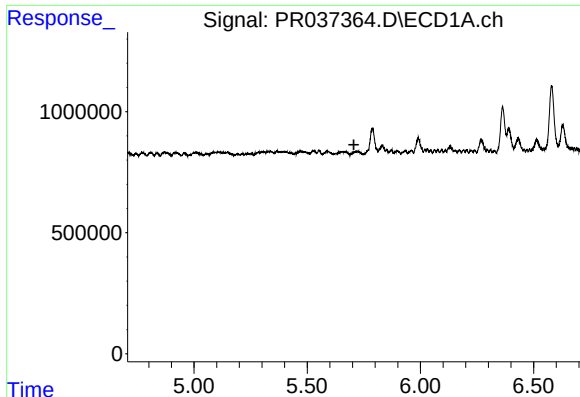

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

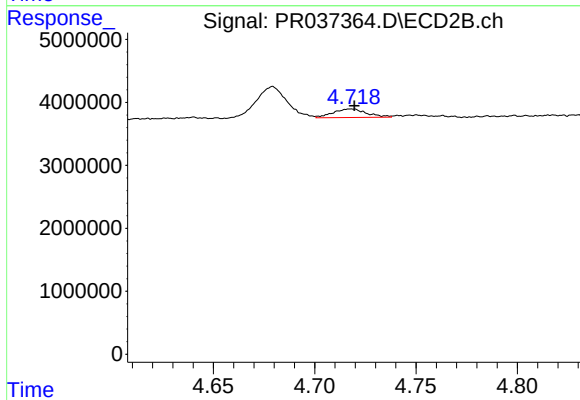


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 1588283
Conc: 14.45 ng/ml

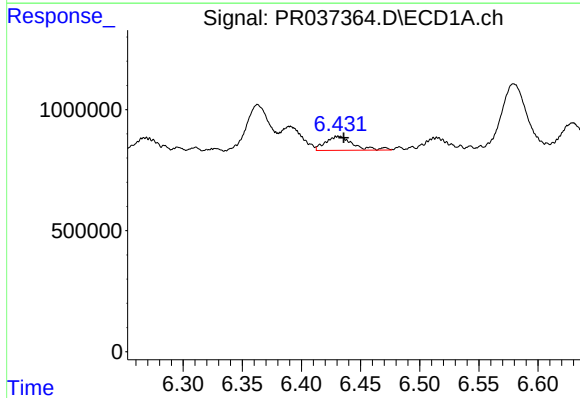


#20 AR-1242-5

R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 938662
Conc: 29.17 ng/ml

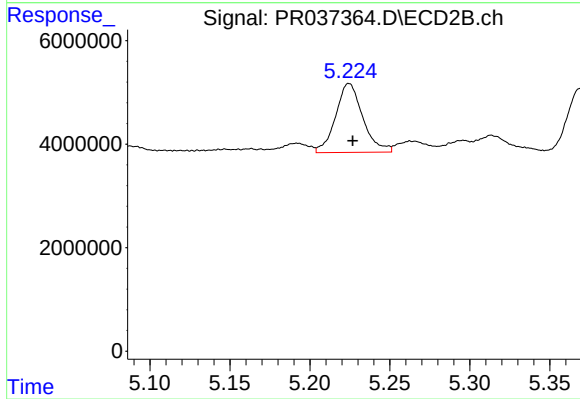

#20 AR-1242-5


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 15769012
Conc: 95.17 ng/ml

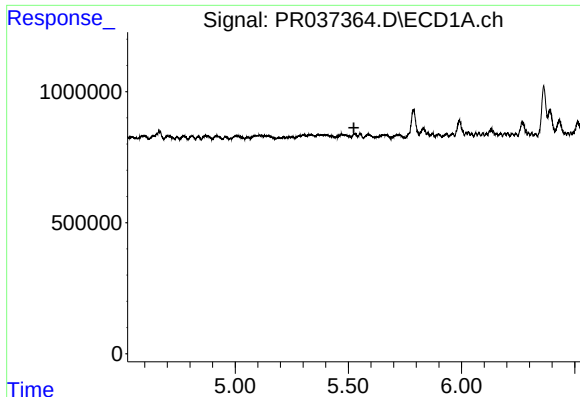

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

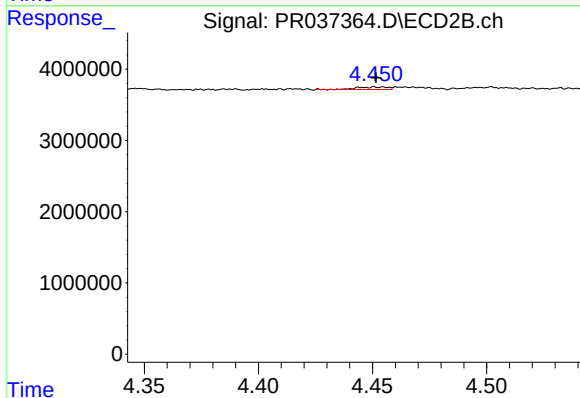


#21 AR-1248-1

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 331692
Conc: 3.30 ng/ml

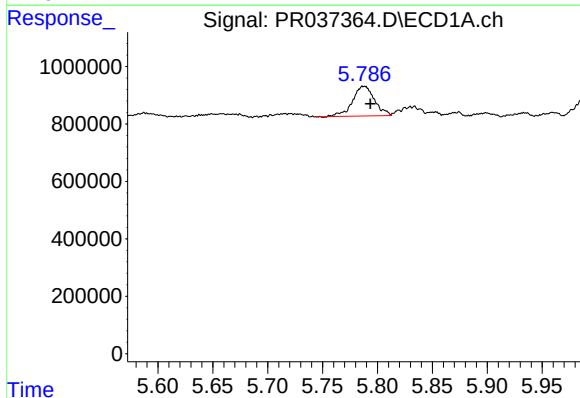


#22 AR-1248-2

R.T.: 5.788 min
Delta R.T.: -0.006 min
Response: 1444551
Conc: 41.26 ng/ml

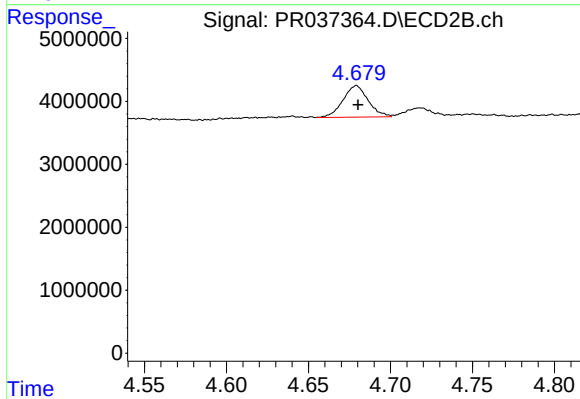

#22 AR-1248-2


R.T.: 4.679 min
Delta R.T.: 0.000 min
Response: 5349514
Conc: 39.20 ng/ml

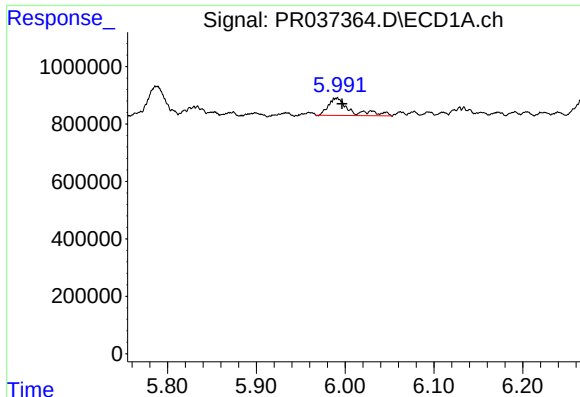

#23 AR-1248-3


R.T.: 5.990 min
Delta R.T.: -0.006 min
Response: 1029045
Conc: 25.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

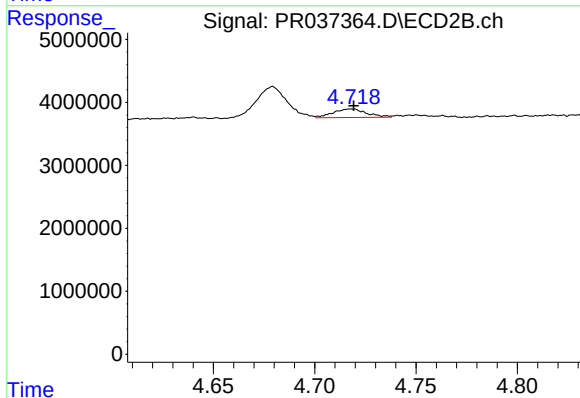


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 1588283
Conc: 11.35 ng/ml

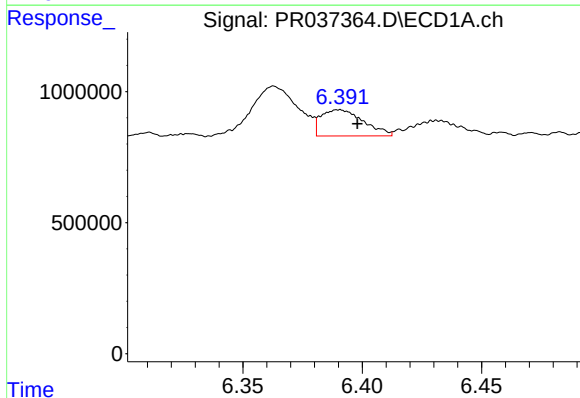


#24 AR-1248-4

R.T.: 6.390 min
Delta R.T.: -0.008 min
Response: 1236645
Conc: 25.26 ng/ml

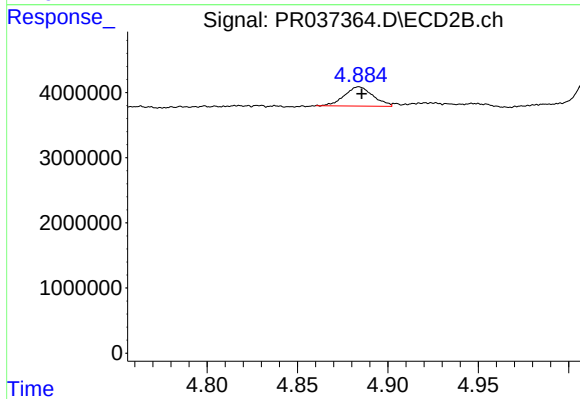

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 3248604
Conc: 18.25 ng/ml

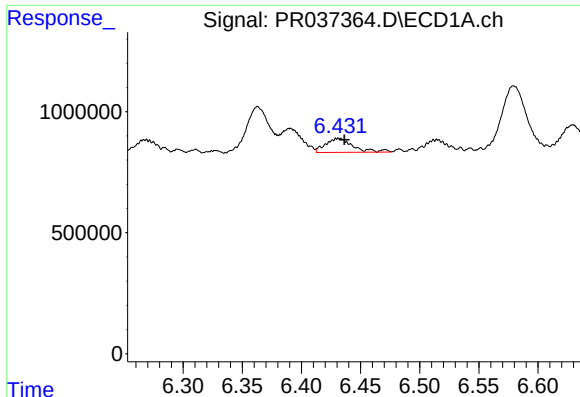

#25 AR-1248-5


R.T.: 6.431 min
Delta R.T.: -0.005 min
Response: 938662
Conc: 19.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

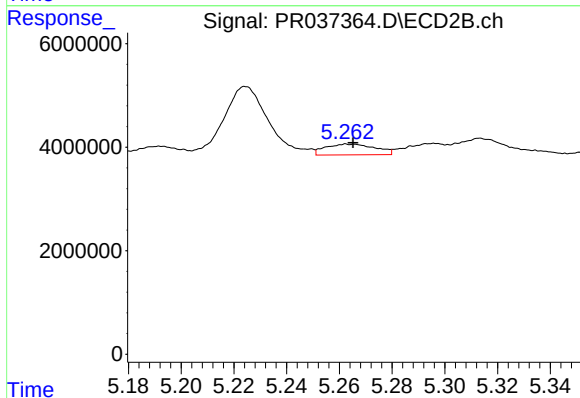


#25 AR-1248-5

R.T.: 5.263 min
Delta R.T.: -0.003 min
Response: 2744583
Conc: 14.03 ng/ml

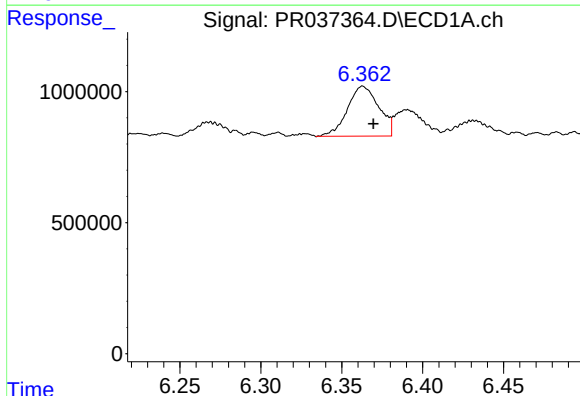


#26 AR-1254-1

R.T.: 6.363 min
Delta R.T.: -0.006 min
Response: 2568316
Conc: 47.01 ng/ml

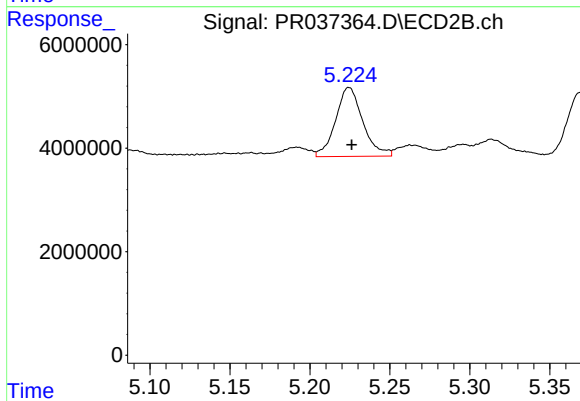

#26 AR-1254-1


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 15769012
Conc: 45.78 ng/ml

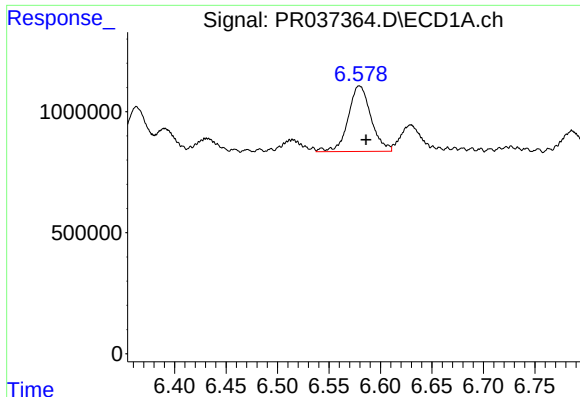

#27 AR-1254-2


R.T.: 6.580 min
Delta R.T.: -0.006 min
Response: 4182461
Conc: 48.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

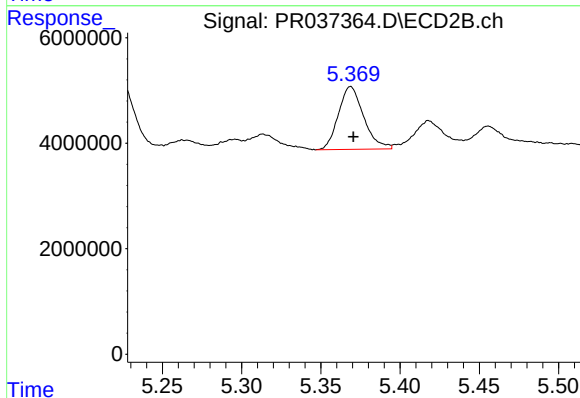


#27 AR-1254-2

R.T.: 5.369 min
Delta R.T.: -0.002 min
Response: 13216728
Conc: 44.13 ng/ml

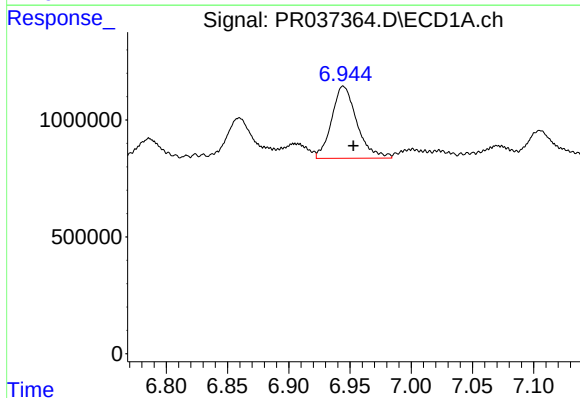


#28 AR-1254-3

R.T.: 6.945 min
Delta R.T.: -0.008 min
Response: 4430414
Conc: 48.71 ng/ml

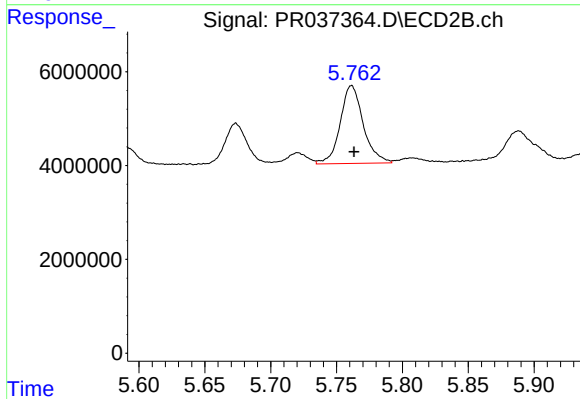

#28 AR-1254-3


R.T.: 5.761 min
Delta R.T.: -0.002 min
Response: 20246025
Conc: 42.75 ng/ml

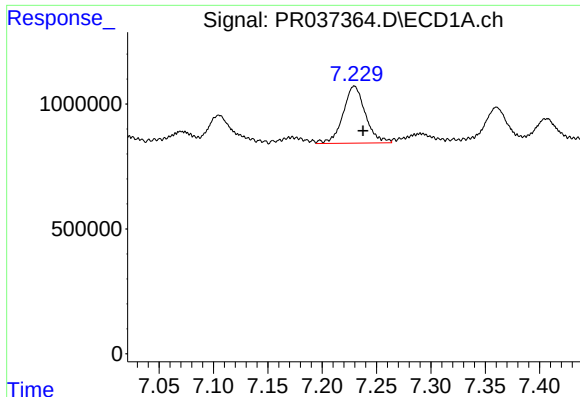

#29 AR-1254-4


R.T.: 7.230 min
Delta R.T.: -0.008 min
Response: 3272401
Conc: 48.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

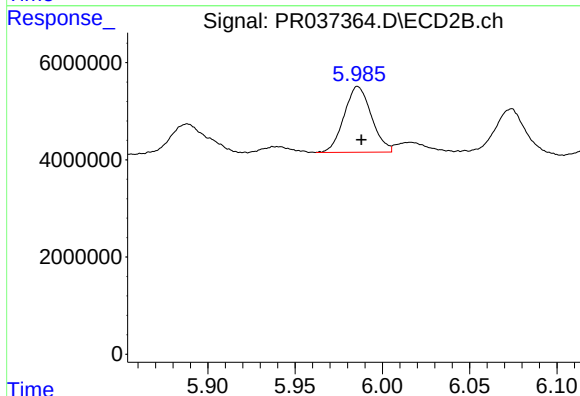


#29 AR-1254-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 14718512
Conc: 41.98 ng/ml

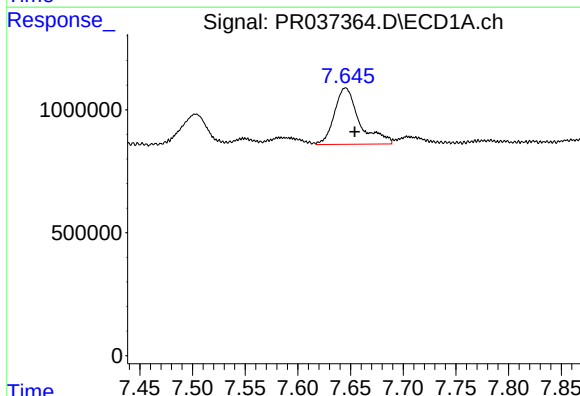


#30 AR-1254-5

R.T.: 7.645 min
Delta R.T.: -0.009 min
Response: 3783419
Conc: 52.63 ng/ml

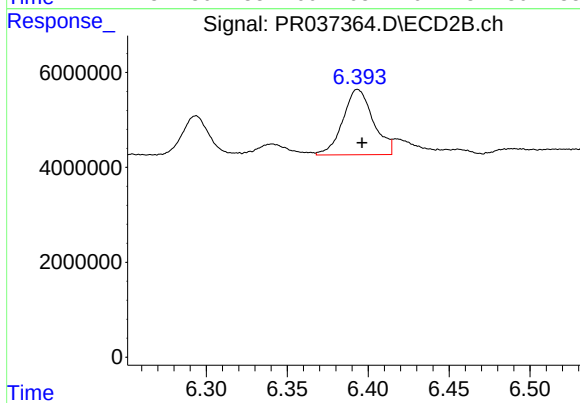

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 18005402
Conc: 40.66 ng/ml

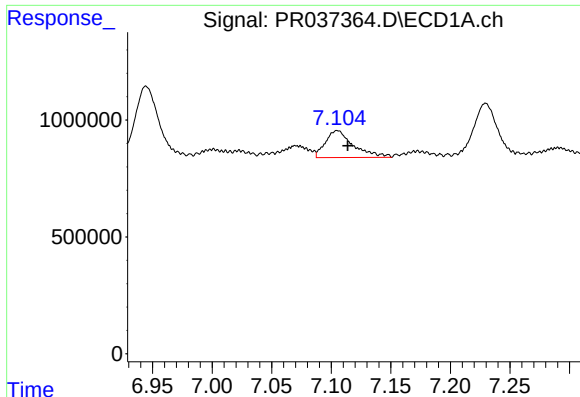

#31 AR-1260-1


R.T.: 7.105 min
Delta R.T.: -0.009 min
Response: 1900792
Conc: 28.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

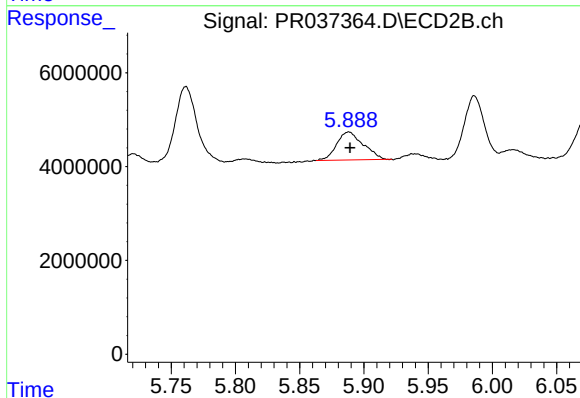


#31 AR-1260-1

R.T.: 5.888 min
Delta R.T.: 0.000 min
Response: 8586745
Conc: 29.38 ng/ml

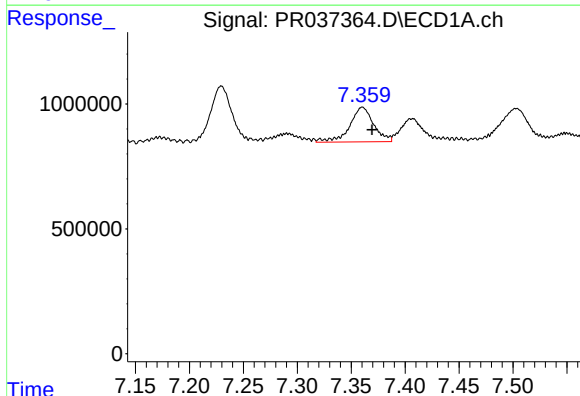


#32 AR-1260-2

R.T.: 7.360 min
Delta R.T.: -0.009 min
Response: 2153000
Conc: 27.01 ng/ml

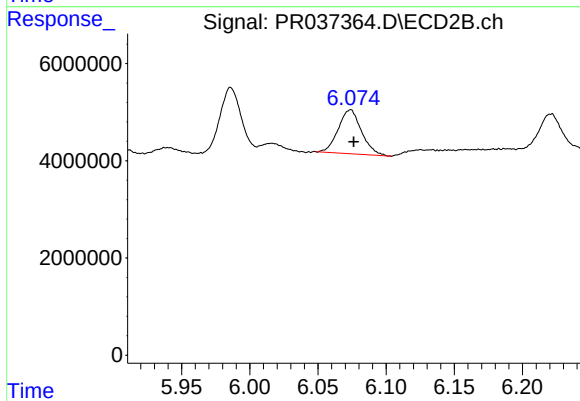

#32 AR-1260-2


R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 10705941
Conc: 23.24 ng/ml

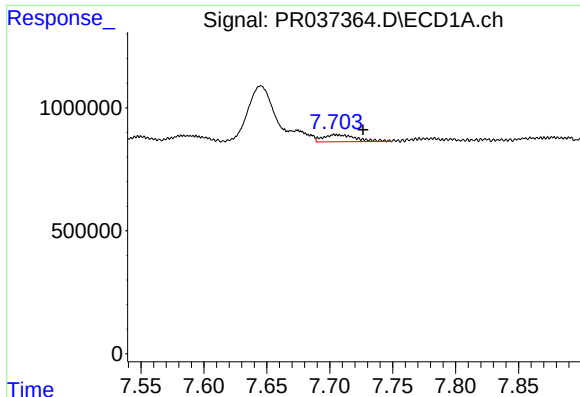

#33 AR-1260-3


R.T.: 7.705 min
Delta R.T.: -0.021 min
Response: 524503
Conc: 8.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

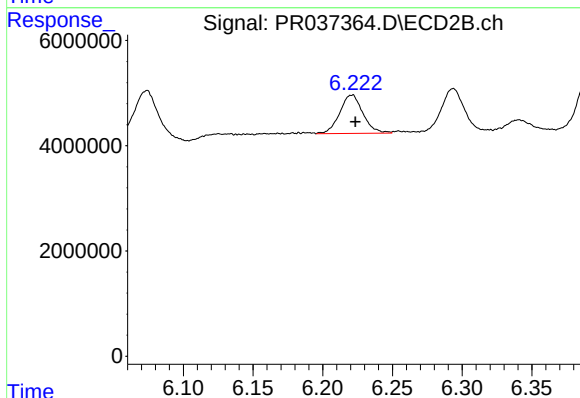


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 8492668
Conc: 23.82 ng/ml

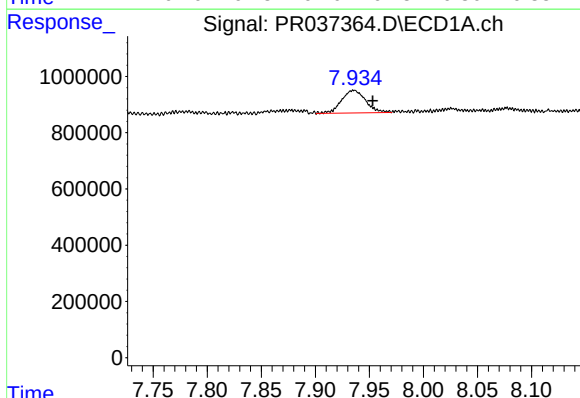


#34 AR-1260-4

R.T.: 7.935 min
Delta R.T.: -0.017 min
Response: 1254432
Conc: 16.86 ng/ml

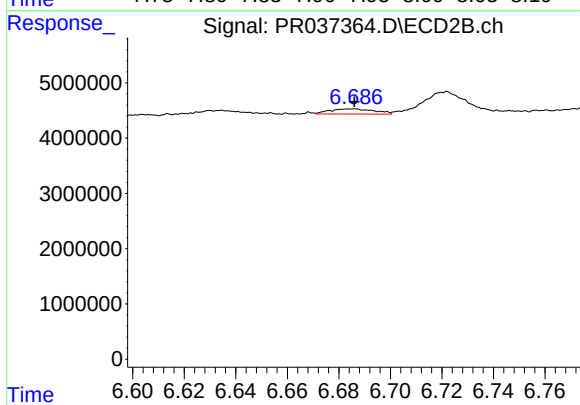

#34 AR-1260-4


R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 1101958
Conc: 3.62 ng/ml

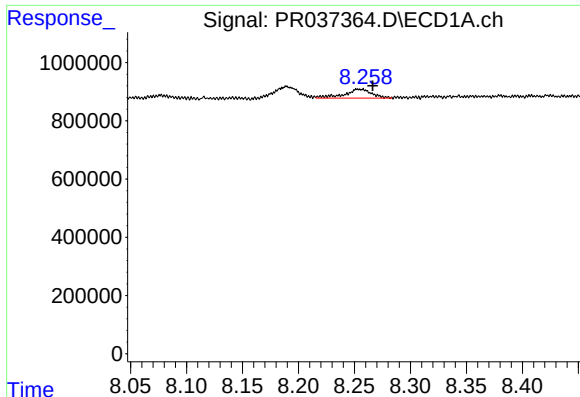

#35 AR-1260-5


R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 527373
Conc: 3.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

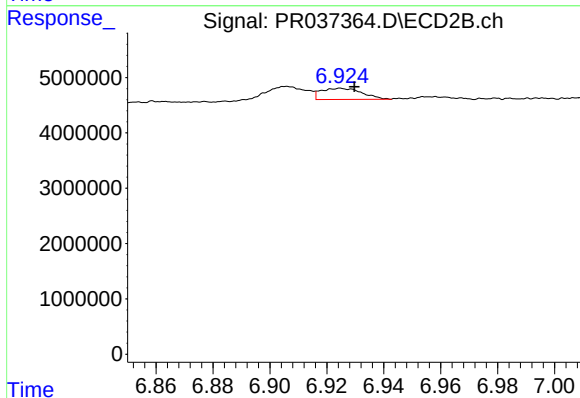


#35 AR-1260-5

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 2018821
Conc: 2.33 ng/ml

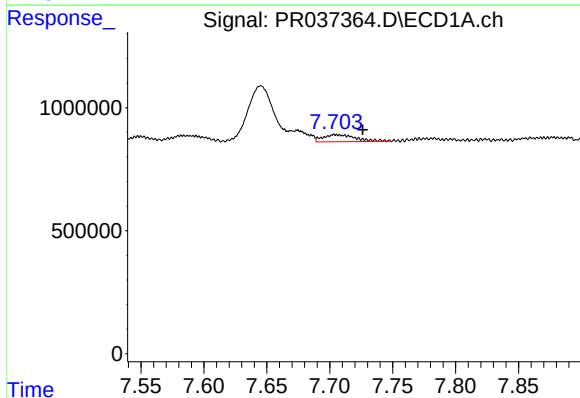


#36 AR-1262-1

R.T.: 7.705 min
Delta R.T.: -0.021 min
Response: 524503
Conc: 5.02 ng/ml

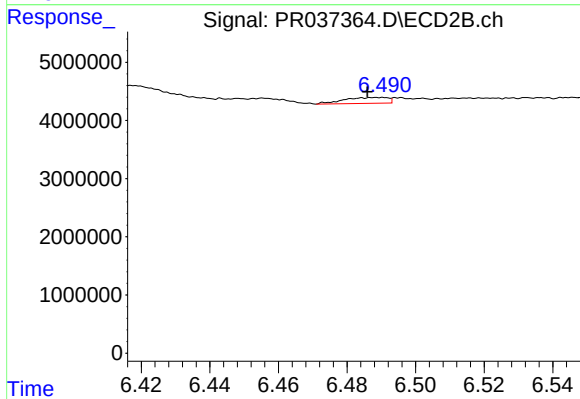

#36 AR-1262-1


R.T.: 6.491 min
Delta R.T.: 0.005 min
Response: 893846
Conc: 3.57 ng/ml

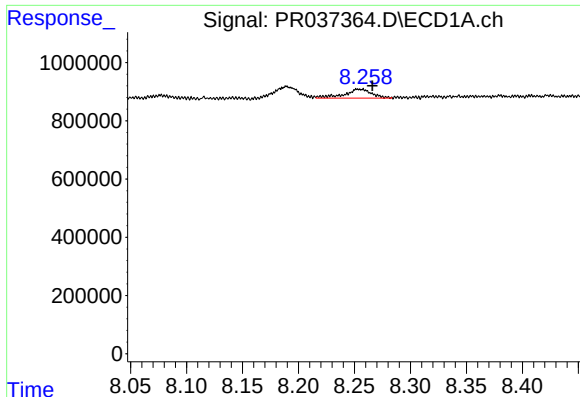

#37 AR-1262-2


R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 527373
Conc: 2.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

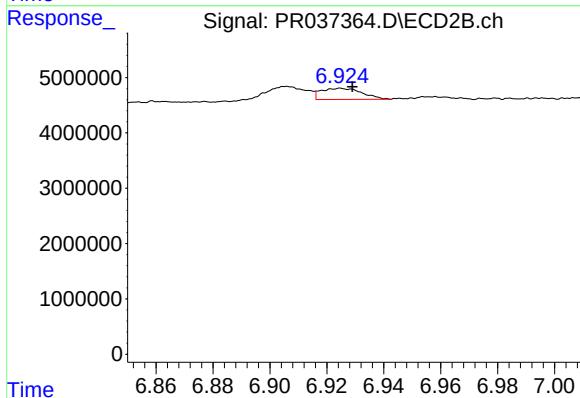


#37 AR-1262-2

R.T.: 6.925 min
Delta R.T.: -0.004 min
Response: 2018821
Conc: 1.61 ng/ml

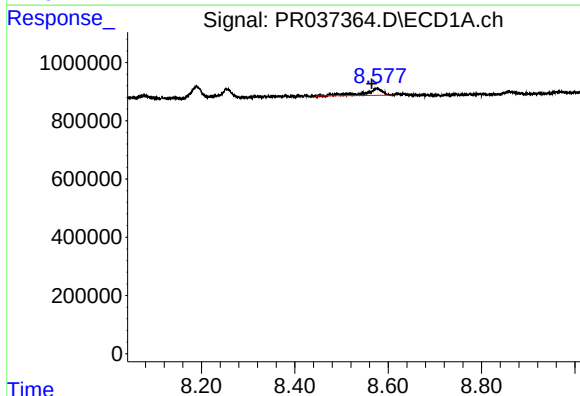


#38 AR-1262-3

R.T.: 8.576 min
Delta R.T.: 0.011 min
Response: 631782
Conc: 4.80 ng/ml

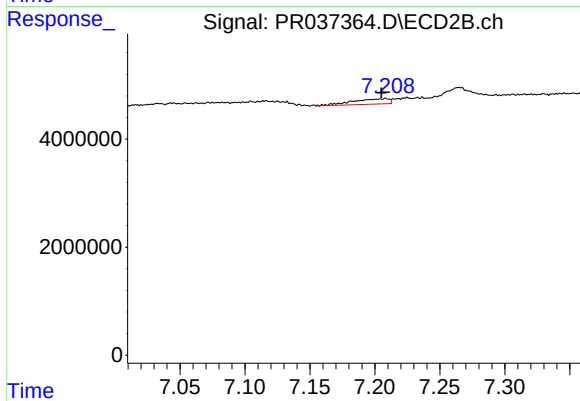

#38 AR-1262-3


R.T.: 7.208 min
Delta R.T.: 0.003 min
Response: 1968358
Conc: 3.59 ng/ml

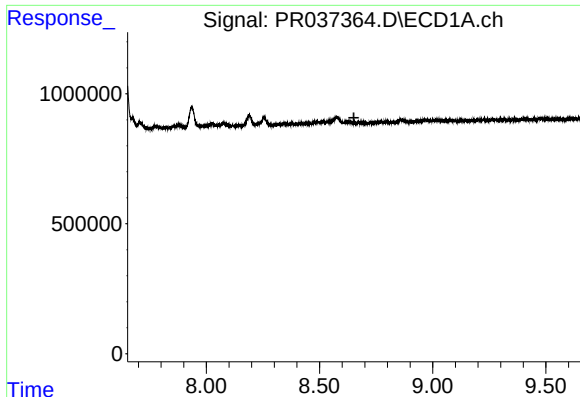

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

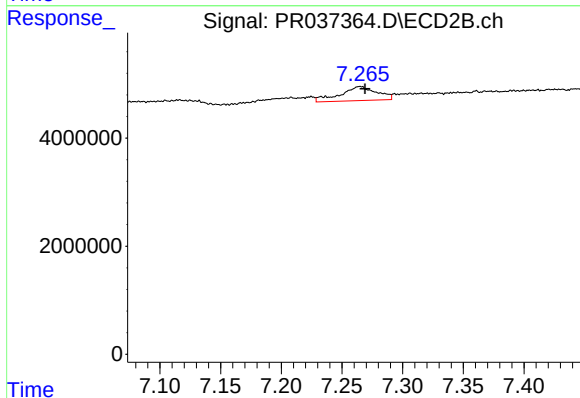


#39 AR-1262-4

R.T.: 7.265 min
Delta R.T.: -0.004 min
Response: 5463814
Conc: 6.09 ng/ml

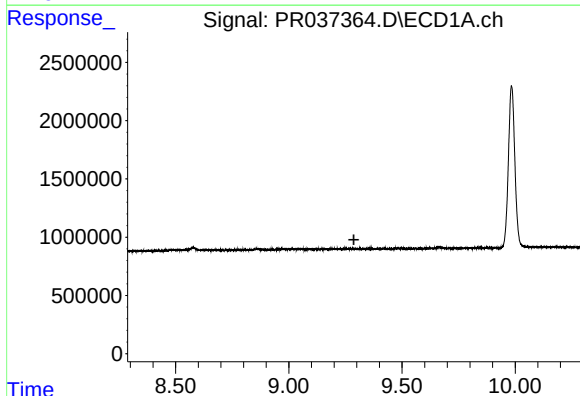


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

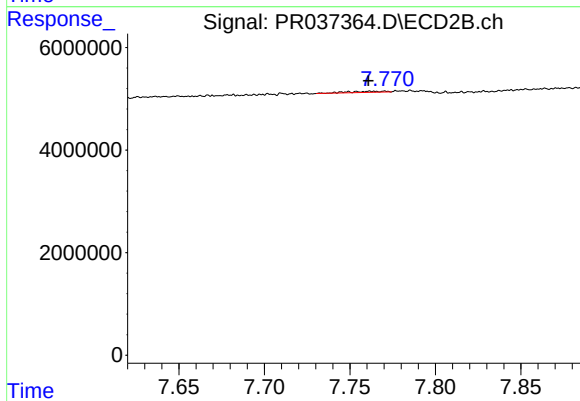

#40 AR-1262-5


R.T.: 7.762 min
Delta R.T.: 0.001 min
Response: 332462
Conc: 0.87 ng/ml

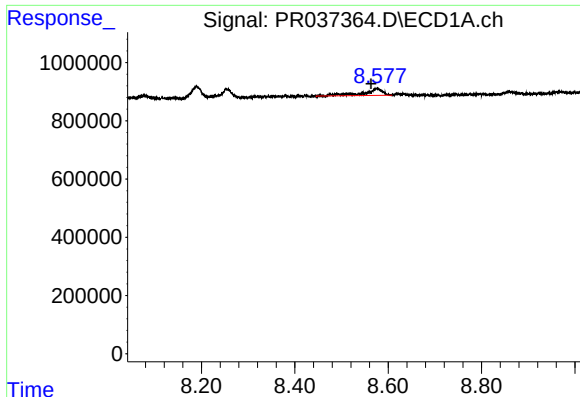

#41 AR-1268-1


R.T.: 8.576 min
Delta R.T.: 0.012 min
Response: 631782
Conc: 3.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

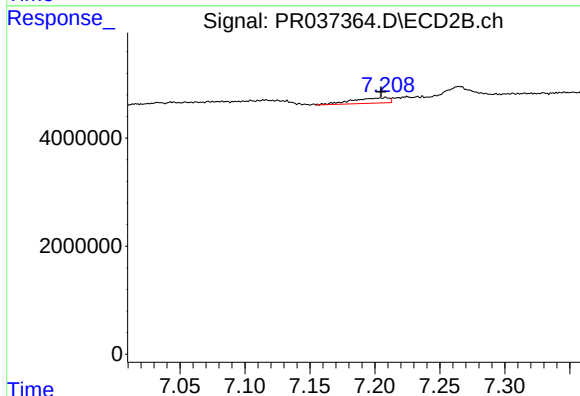


#41 AR-1268-1

R.T.: 7.208 min
Delta R.T.: 0.004 min
Response: 1968358
Conc: 1.60 ng/ml

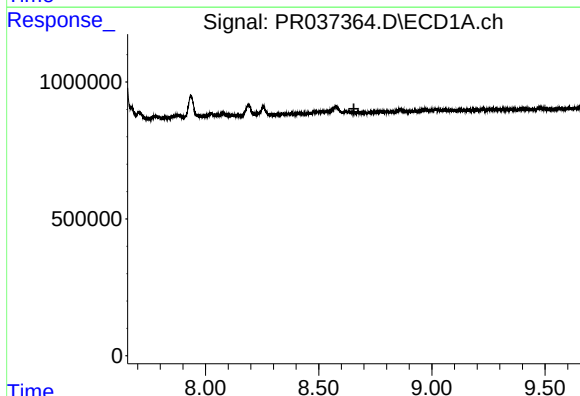


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.655 min
Response: 0
Conc: N.D.

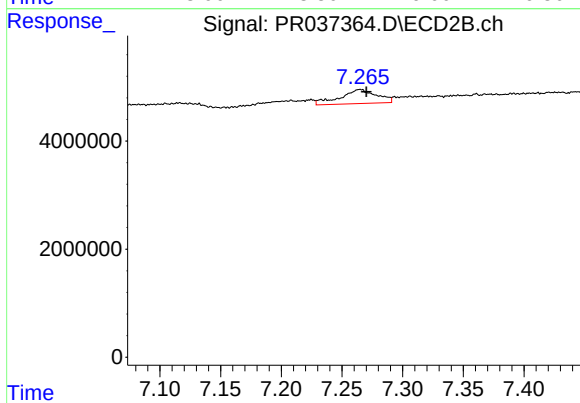

#42 AR-1268-2


R.T.: 7.265 min
Delta R.T.: -0.005 min
Response: 5463814
Conc: 5.16 ng/ml

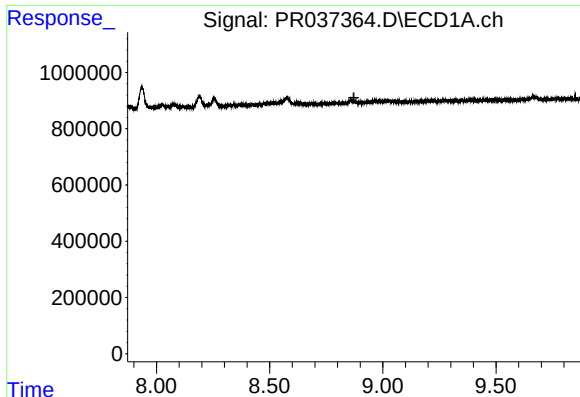

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

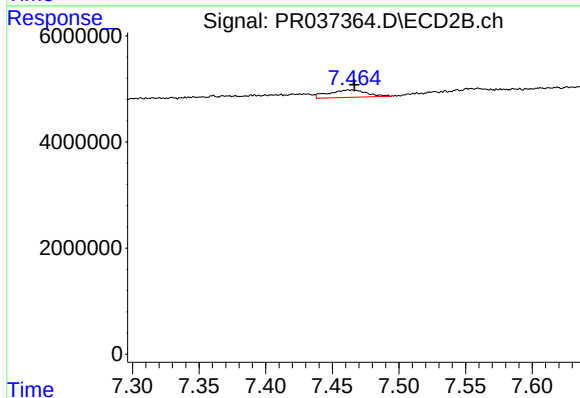


#43 AR-1268-3

R.T.: 7.463 min
Delta R.T.: -0.004 min
Response: 2767051
Conc: 3.12 ng/ml

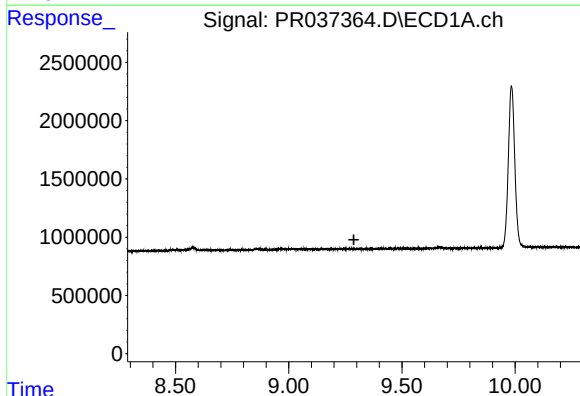


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

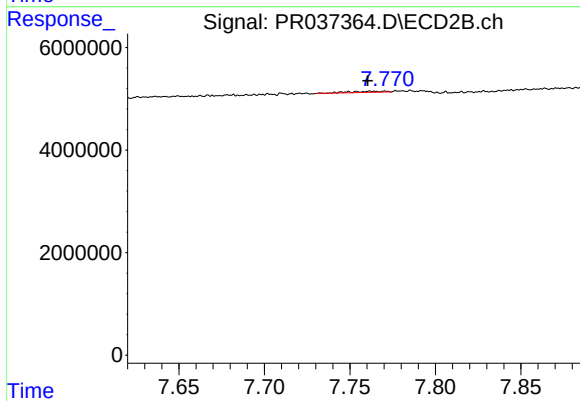

#44 AR-1268-4


R.T.: 7.762 min
Delta R.T.: 0.002 min
Response: 332462
Conc: 0.92 ng/ml

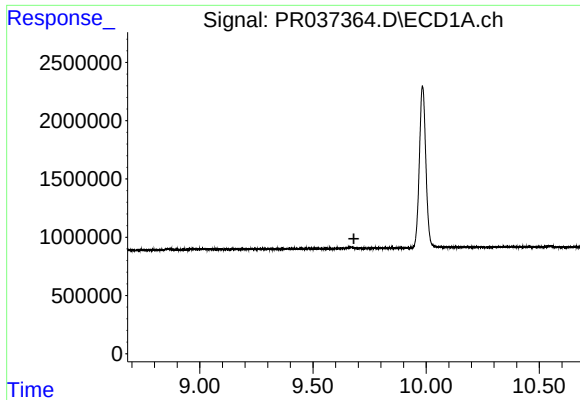

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

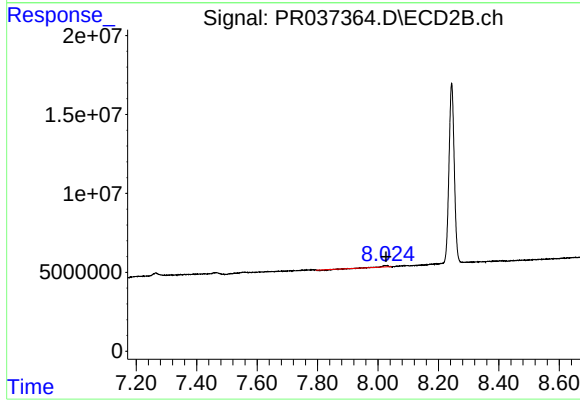

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: -0.003 min
Response: 473474
Conc: 0.19 ng/ml