

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:01
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1262 LOD 40PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:08:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.361	3.411	23715786	97241102	18.957	20.277
2)	SA Decachlor...	9.983	8.244	25769357	129.1E6	19.484	22.163
Target Compounds							
3)	L1 AR-1016-1	0.000	4.468	0	713148	N.D.	3.917 #
4)	L1 AR-1016-2	0.000	4.468	0	713148	N.D.	2.528 #
5)	L1 AR-1016-3	0.000	4.681	0	377743	N.D.	2.627 #
6)	L1 AR-1016-4	0.000	4.681	0	377743	N.D.	3.414 #
7)	L1 AR-1016-5	0.000	4.886	0	1290310	N.D.	8.488 #
8)	L2 AR-1221-1	0.000	3.616	0	400367	N.D.	7.863 #
9)	L2 AR-1221-2	4.660	3.698	99320	1514709	10.982	40.788 #
10)	L2 AR-1221-3	0.000	3.783	0	131495	N.D.	1.074 #
11)	L3 AR-1232-1	0.000	3.783	0	131495	N.D.	1.124 #
12)	L3 AR-1232-2	0.000	4.468	0	713148	N.D.	5.159 #
13)	L3 AR-1232-3	0.000	4.681	0	377743	N.D.	5.381 #
14)	L3 AR-1232-4	0.000	4.723	0	201503	N.D.	3.377 #
15)	L3 AR-1232-5	0.000	4.886	0	1290310	N.D.	18.907 #
16)	L4 AR-1242-1	0.000	4.468	0	713148	N.D.	4.867 #
17)	L4 AR-1242-2	0.000	4.468	0	713148	N.D.	3.126 #
18)	L4 AR-1242-3	0.000	4.681	0	377743	N.D.	3.267 #
19)	L4 AR-1242-4	0.000	4.723	0	201503	N.D.	1.833 #
20)	L4 AR-1242-5	0.000	5.224	0	5120026	N.D.	30.899 #
21)	L5 AR-1248-1	0.000	4.468	0	713148	N.D.	7.084 #
22)	L5 AR-1248-2	0.000	4.681	0	377743	N.D.	2.768 #
23)	L5 AR-1248-3	0.000	4.723	0	201503	N.D.	1.440 #
24)	L5 AR-1248-4	6.363	4.886	534583	1290310	10.920	7.250 #
25)	L5 AR-1248-5	0.000	5.263	0	4203946	N.D.	21.491 #
26)	L6 AR-1254-1	6.363	5.224	534583	5120026	9.785	14.863 #
27)	L6 AR-1254-2	6.578	5.371	845070	4251772	9.861	14.196 #
28)	L6 AR-1254-3	6.949	5.775	643462	12570706	7.074	26.542 #
29)	L6 AR-1254-4	7.291	5.985	446893	459277	6.669	1.310 #
30)	L6 AR-1254-5	7.642	6.393	3663431	15764419	50.965	35.600 #
31)	L7 AR-1260-1	7.105	5.887	3012479	12559894	45.653	42.973
32)	L7 AR-1260-2	7.361	6.073	3602865	20995459	45.203	45.584
33)	L7 AR-1260-3	7.717	6.222	4826118	17234633	77.125	48.344 #
34)	L7 AR-1260-4	7.943	6.683	4355530	21794051	58.539	71.511
35)	L7 AR-1260-5	8.255	6.926	7647028	48459048	52.876	55.877
36)	L8 AR-1262-1	7.717	6.484	4826118	9993613	46.204	39.876
37)	L8 AR-1262-2	8.255	6.926	7647028	48459048	39.340	38.584
38)	L8 AR-1262-3	8.553	7.201	5760009	20039287	43.799	36.550
39)	L8 AR-1262-4	8.642	7.266	4449815	38598221	45.300	42.999
40)	L8 AR-1262-5	9.276	7.758	2893430	15272450	41.909	39.916
41)	L9 AR-1268-1	8.553	7.201	5760009	20039287	32.162	16.279 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:01
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1262 LOD 40PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:08:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.642	7.266	4449815	38598221	27.051	36.451 #
43) L9	AR-1268-3	8.859	7.464	627472	15048080	4.533	16.980 #
44) L9	AR-1268-4	9.276	7.758	2893430	15272450	46.380	42.098
45) L9	AR-1268-5	9.667	8.024	1217592	1928538	2.671	0.758 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 19:01
Operator : SM\SJ
Sample : K2241-07
Misc : AR1262 LOD 40PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:08:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

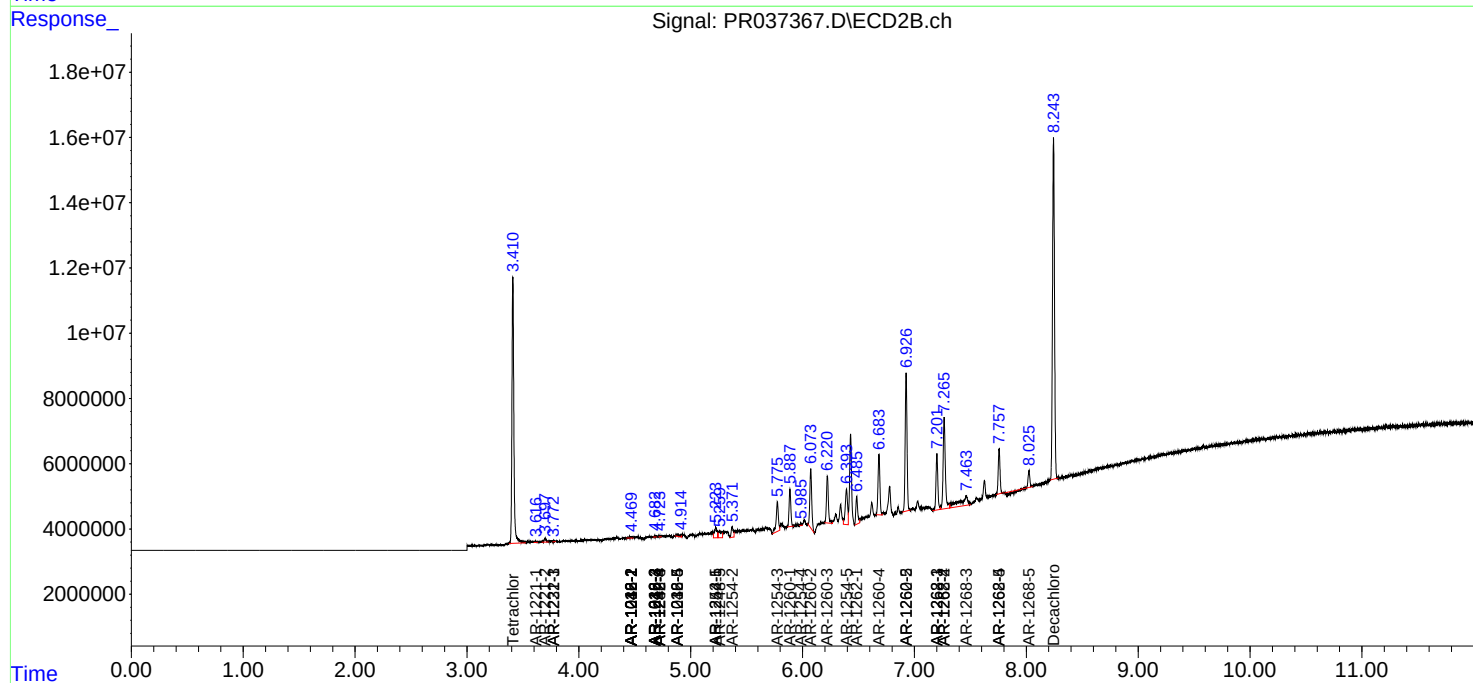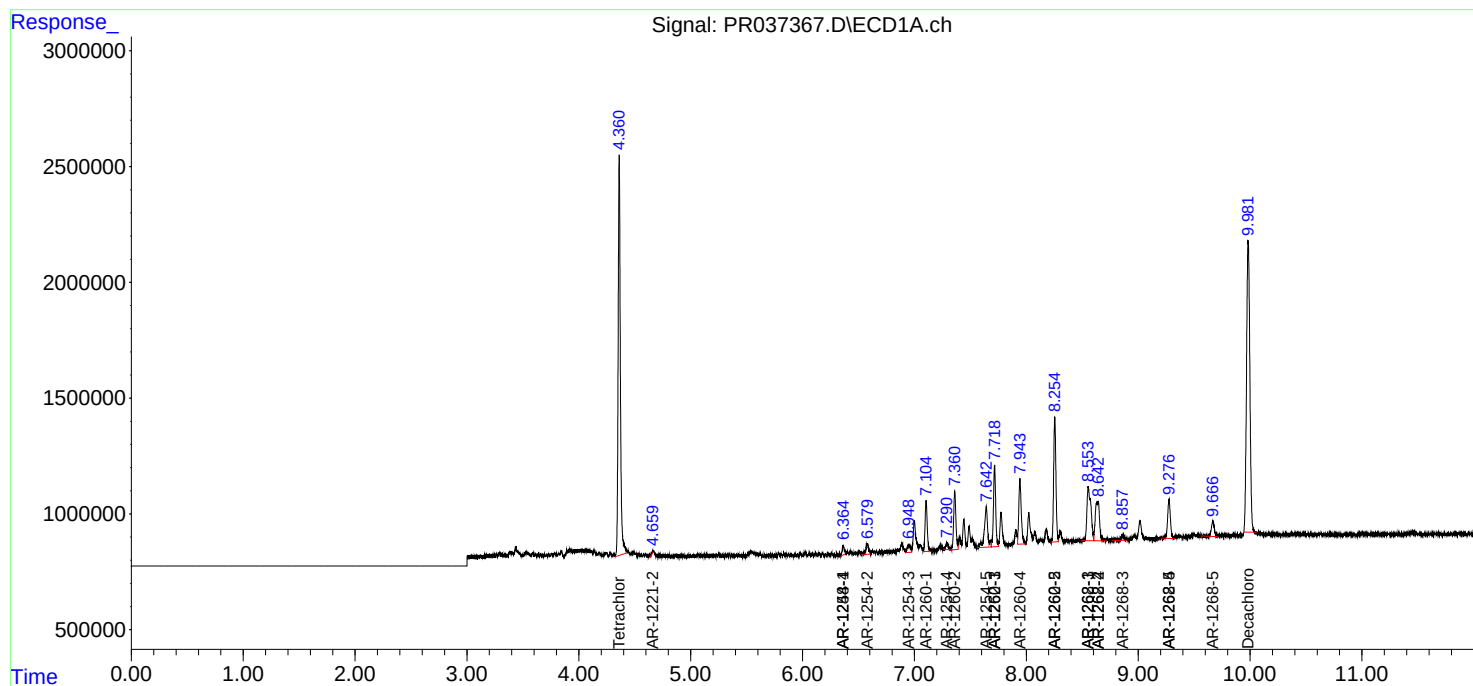


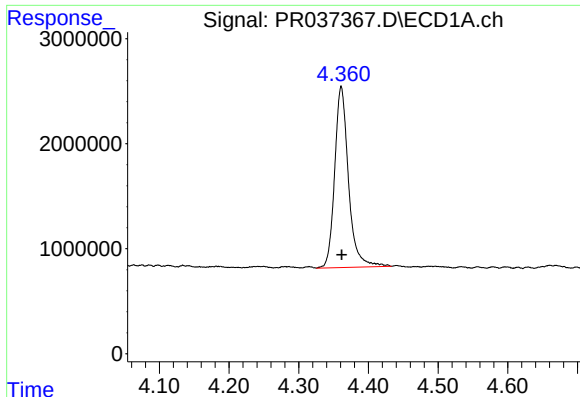

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 23715786
Conc: 18.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

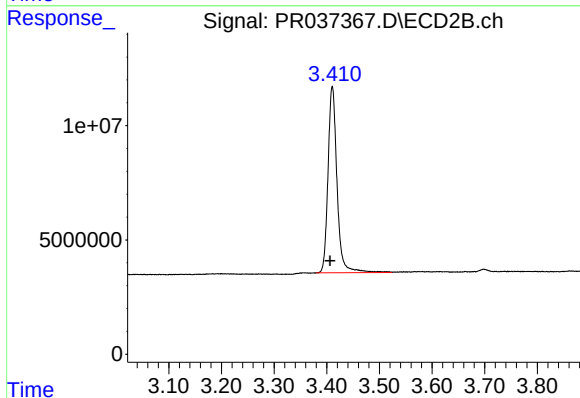


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.004 min
Response: 97241102
Conc: 20.28 ng/ml

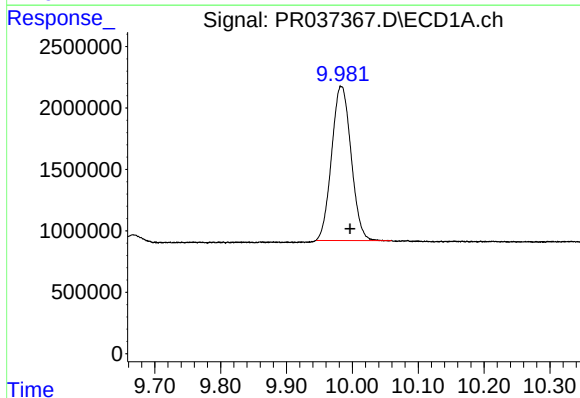


#2 Decachlorobiphenyl

R.T.: 9.983 min
Delta R.T.: -0.014 min
Response: 25769357
Conc: 19.48 ng/ml

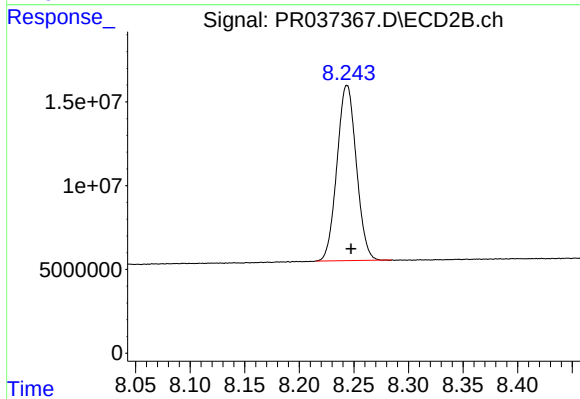

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 129081667
Conc: 22.16 ng/ml

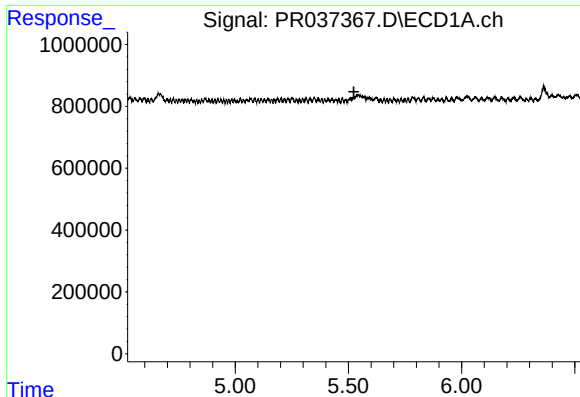

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

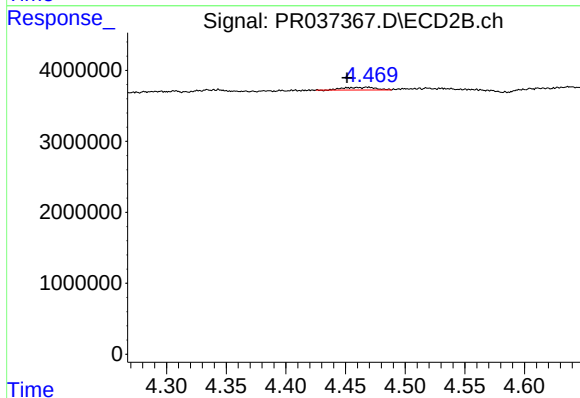


#3 AR-1016-1

R.T.: 4.468 min
Delta R.T.: 0.017 min
Response: 713148
Conc: 3.92 ng/ml

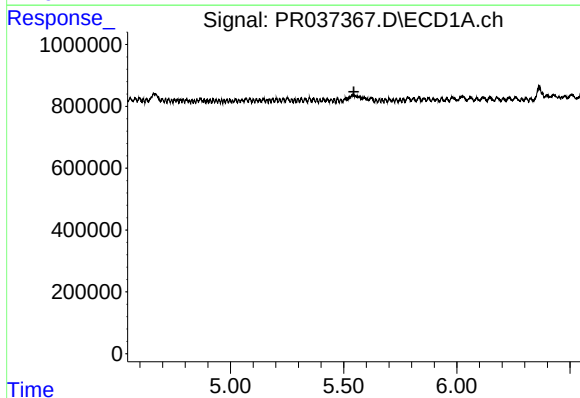


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

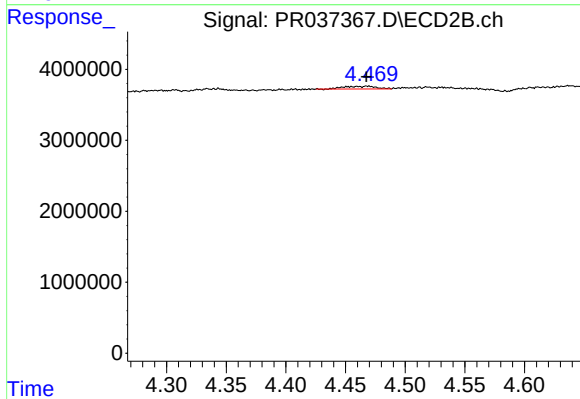

#4 AR-1016-2


R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 713148
Conc: 2.53 ng/ml

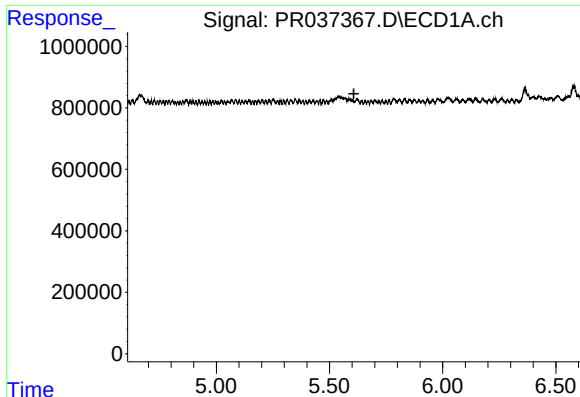

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

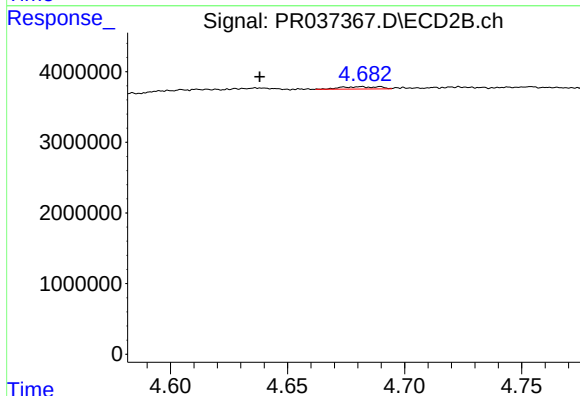


#5 AR-1016-3

R.T.: 4.681 min
Delta R.T.: 0.043 min
Response: 377743
Conc: 2.63 ng/ml

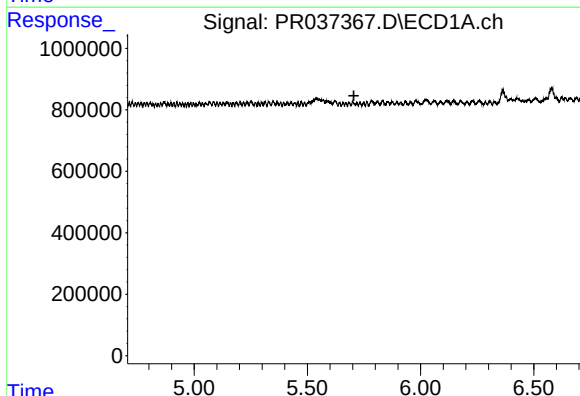


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

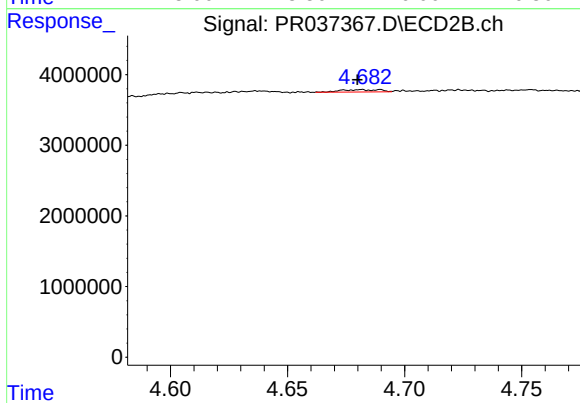

#6 AR-1016-4


R.T.: 4.681 min
Delta R.T.: 0.002 min
Response: 377743
Conc: 3.41 ng/ml

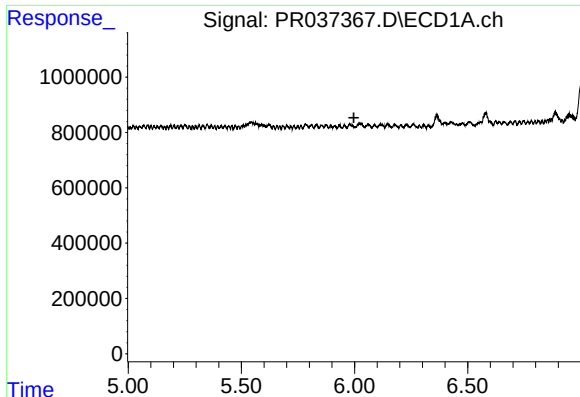

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

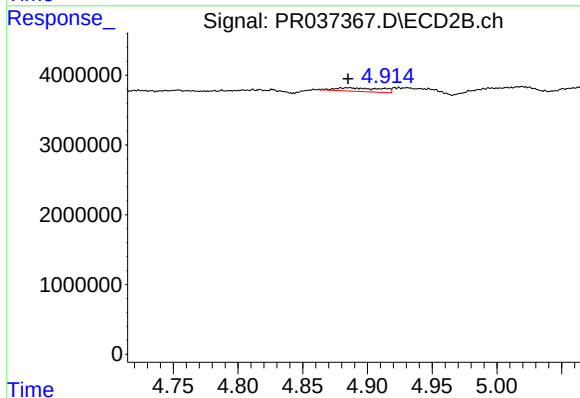


#7 AR-1016-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 1290310
Conc: 8.49 ng/ml

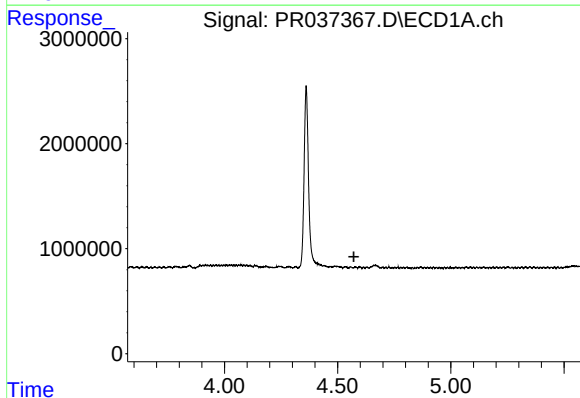


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

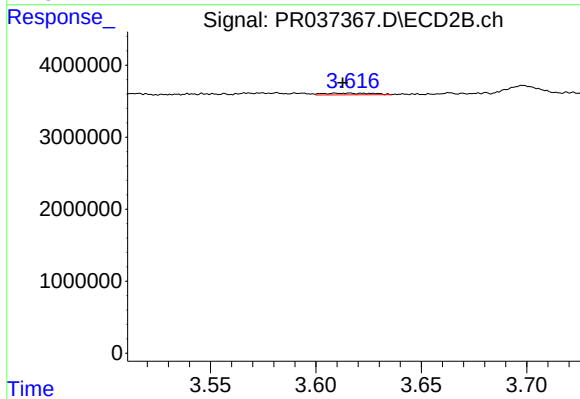

#8 AR-1221-1


R.T.: 3.616 min
Delta R.T.: 0.003 min
Response: 400367
Conc: 7.86 ng/ml

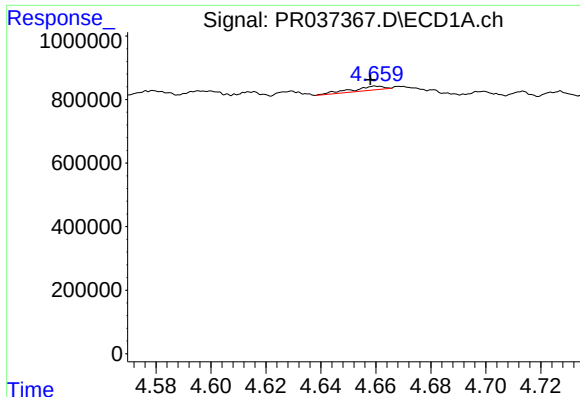

#9 AR-1221-2


R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 99320
Conc: 10.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

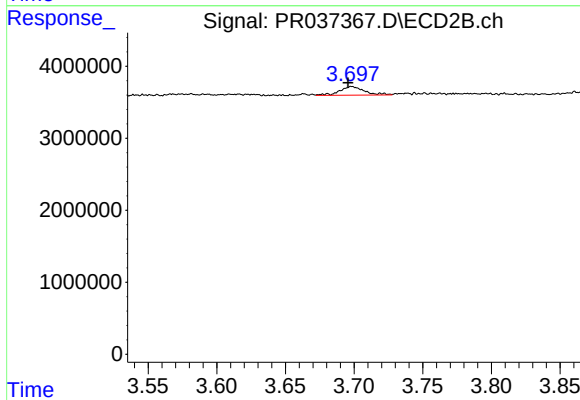


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.003 min
Response: 1514709
Conc: 40.79 ng/ml

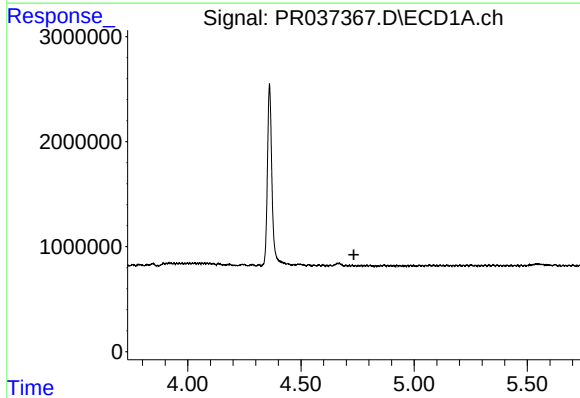


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

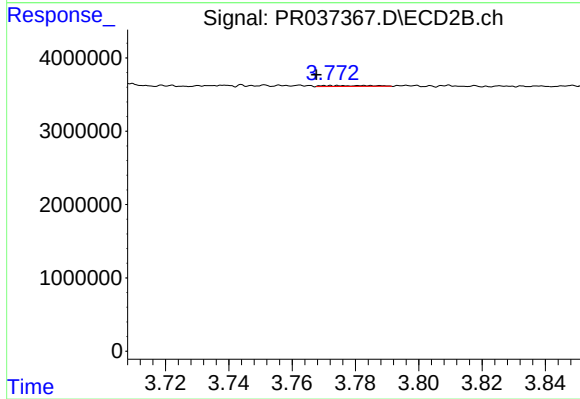

#10 AR-1221-3


R.T.: 3.783 min
Delta R.T.: 0.015 min
Response: 131495
Conc: 1.07 ng/ml

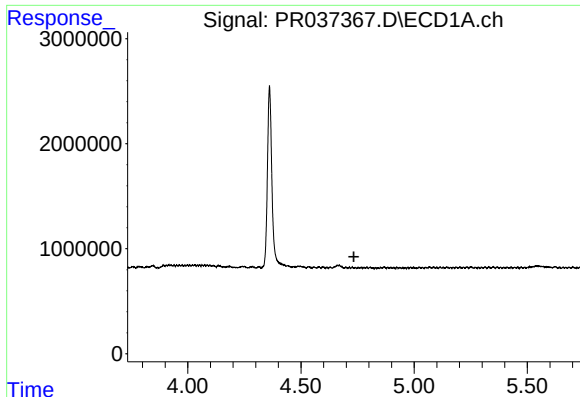

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

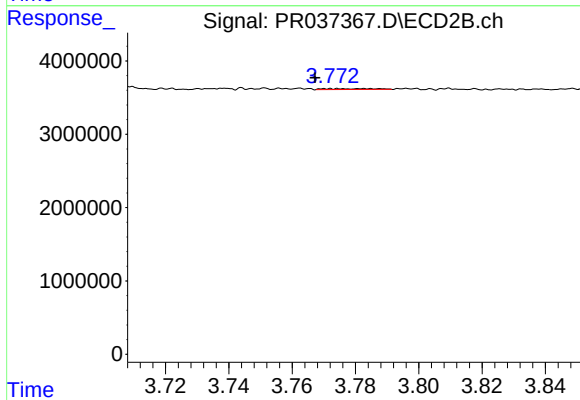


#11 AR-1232-1

R.T.: 3.783 min
Delta R.T.: 0.016 min
Response: 131495
Conc: 1.12 ng/ml

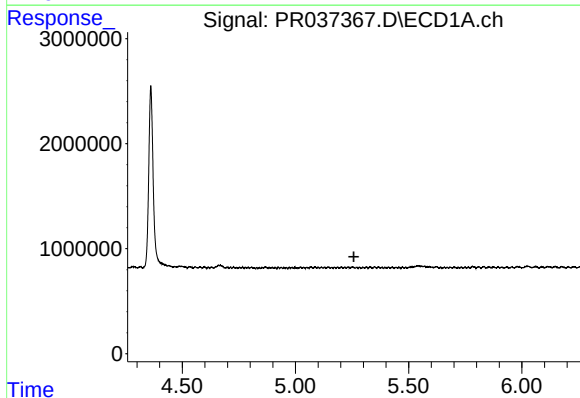


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

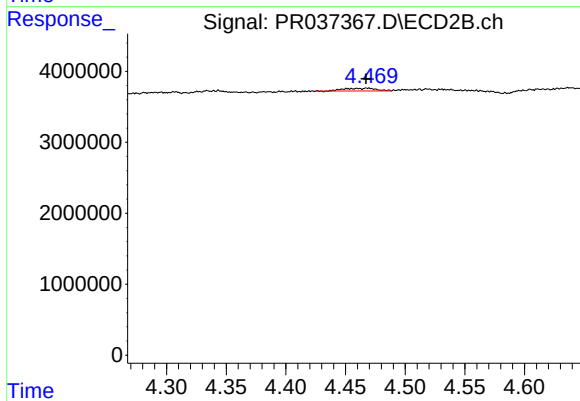

#12 AR-1232-2


R.T.: 4.468 min
Delta R.T.: 0.001 min
Response: 713148
Conc: 5.16 ng/ml

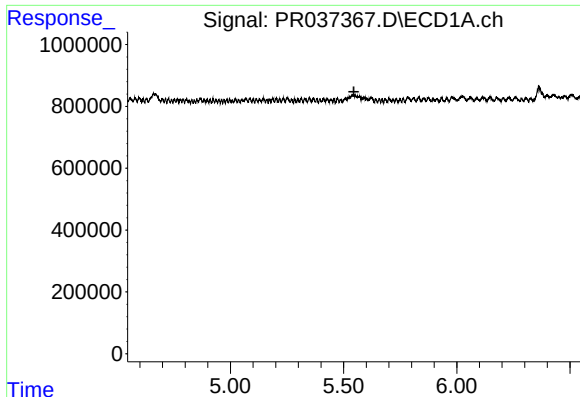

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

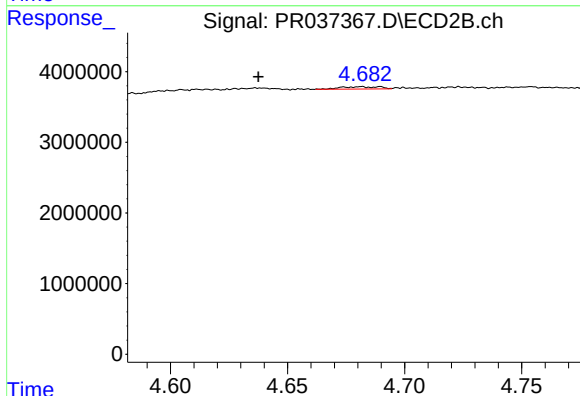


#13 AR-1232-3

R.T.: 4.681 min
Delta R.T.: 0.044 min
Response: 377743
Conc: 5.38 ng/ml

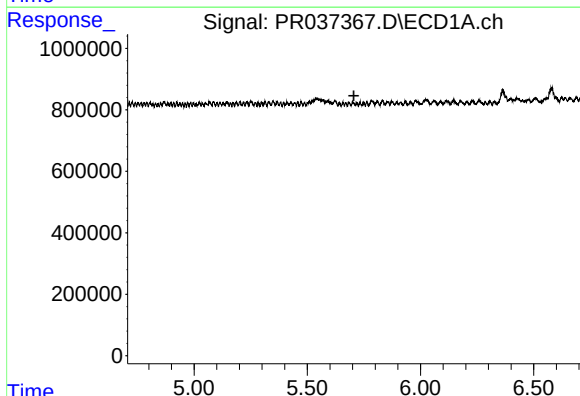


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

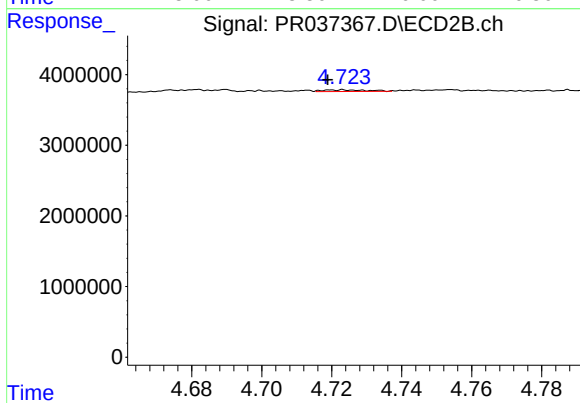

#14 AR-1232-4


R.T.: 4.723 min
Delta R.T.: 0.005 min
Response: 201503
Conc: 3.38 ng/ml

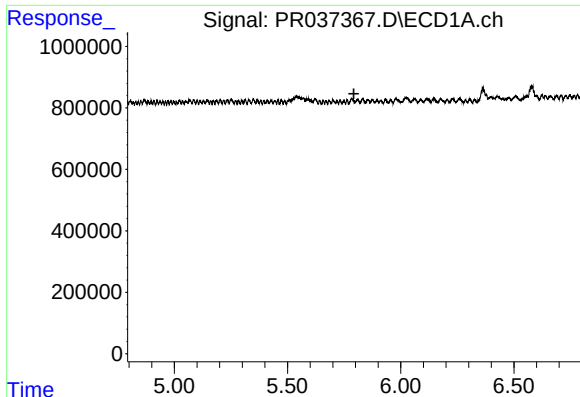

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

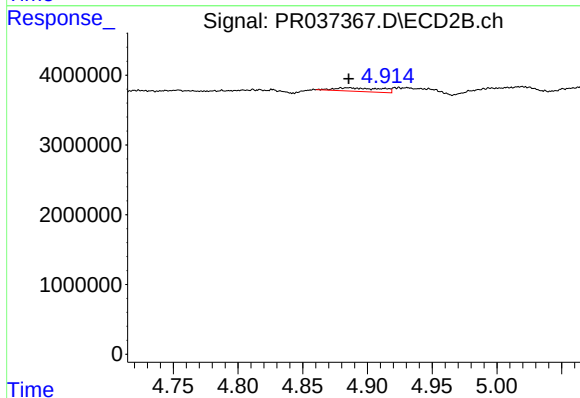


#15 AR-1232-5

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 1290310
Conc: 18.91 ng/ml

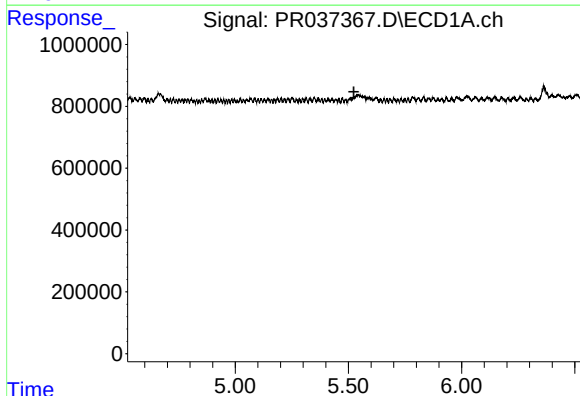


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

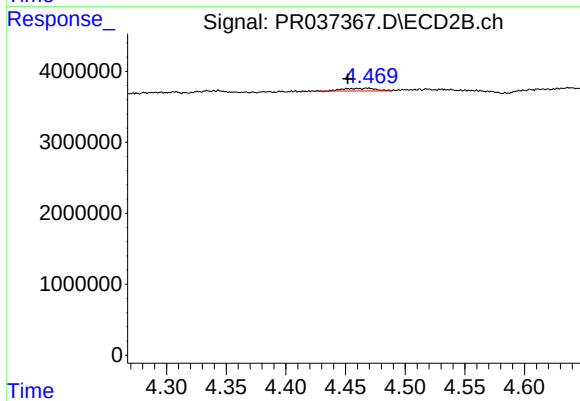

#16 AR-1242-1


R.T.: 4.468 min
Delta R.T.: 0.016 min
Response: 713148
Conc: 4.87 ng/ml

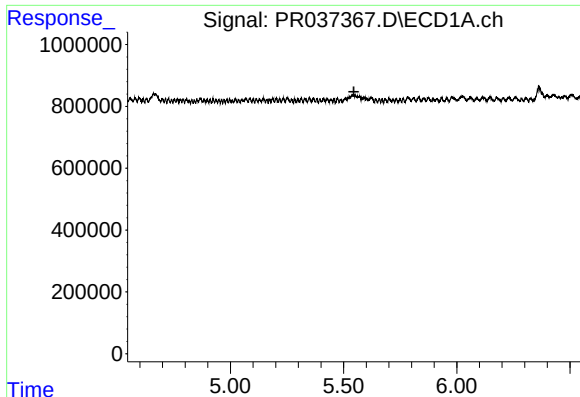

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

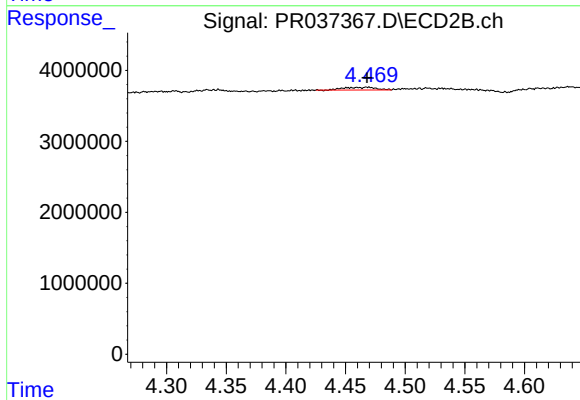


#17 AR-1242-2

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 713148
Conc: 3.13 ng/ml

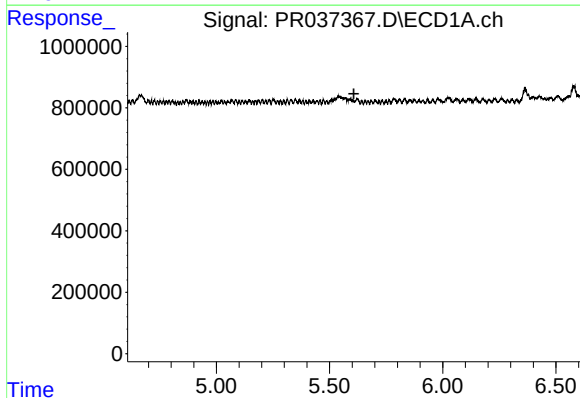


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

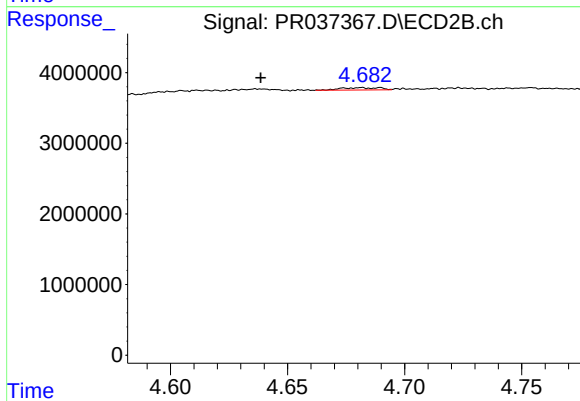

#18 AR-1242-3


R.T.: 4.681 min
Delta R.T.: 0.043 min
Response: 377743
Conc: 3.27 ng/ml

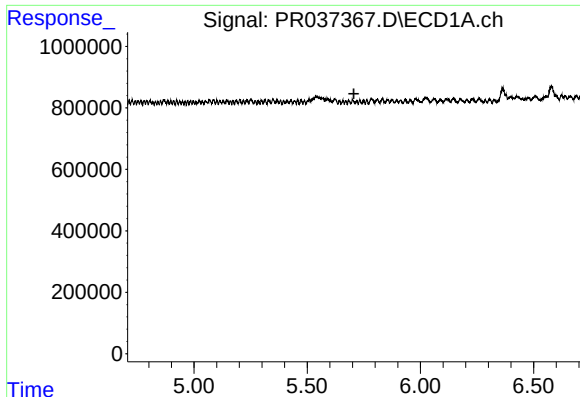

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

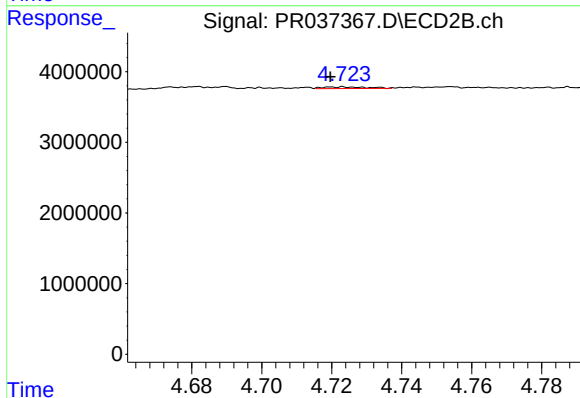


#19 AR-1242-4

R.T.: 4.723 min
Delta R.T.: 0.004 min
Response: 201503
Conc: 1.83 ng/ml

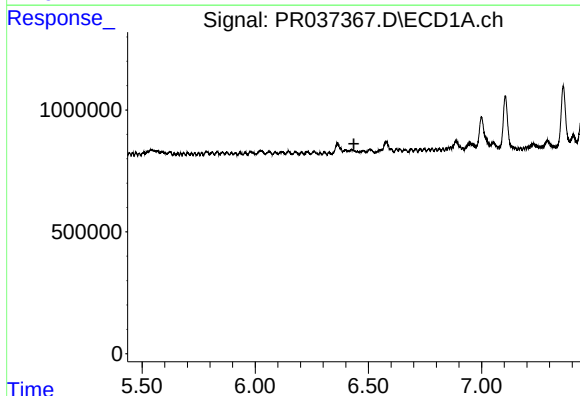


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

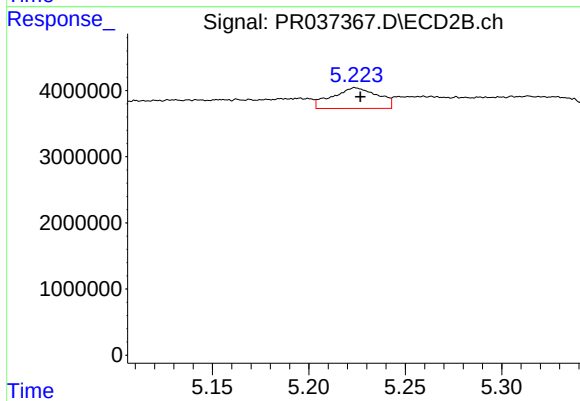

#20 AR-1242-5


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 5120026
Conc: 30.90 ng/ml

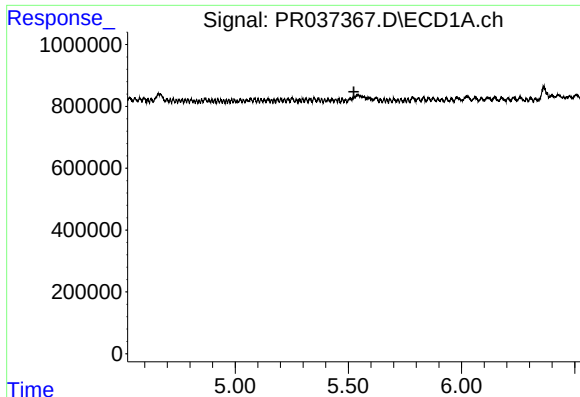

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

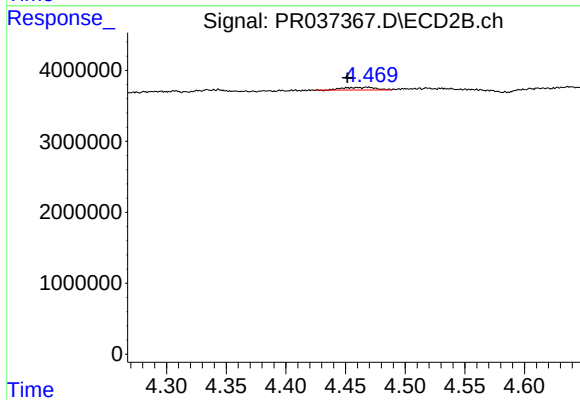


#21 AR-1248-1

R.T.: 4.468 min
Delta R.T.: 0.017 min
Response: 713148
Conc: 7.08 ng/ml

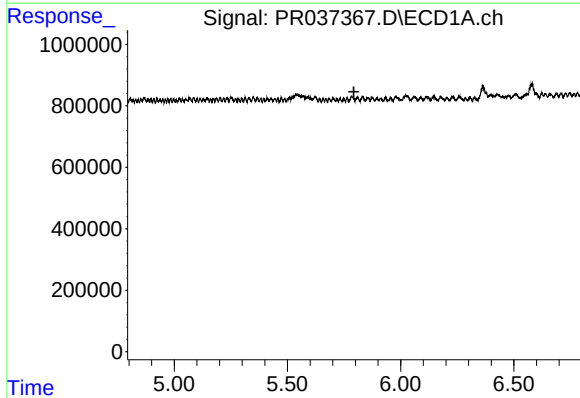


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

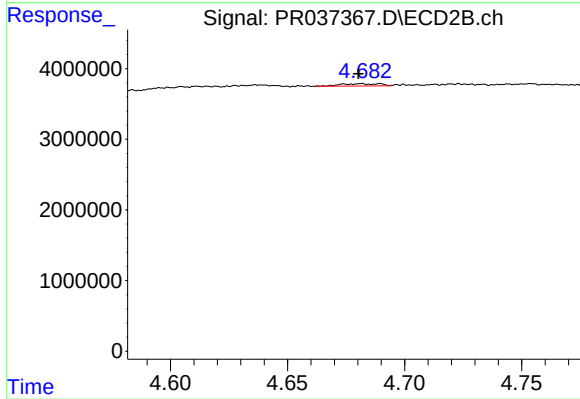

#22 AR-1248-2


R.T.: 4.681 min
Delta R.T.: 0.001 min
Response: 377743
Conc: 2.77 ng/ml

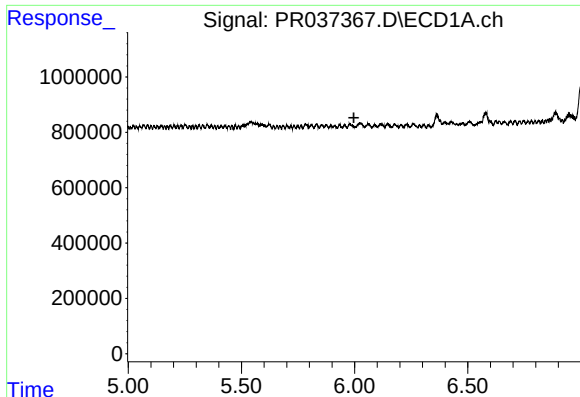

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

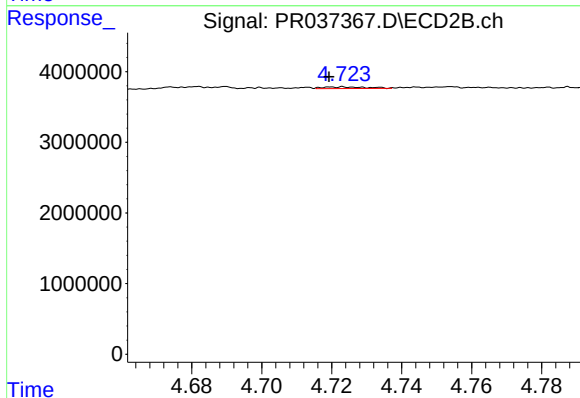


#23 AR-1248-3

R.T.: 4.723 min
Delta R.T.: 0.004 min
Response: 201503
Conc: 1.44 ng/ml

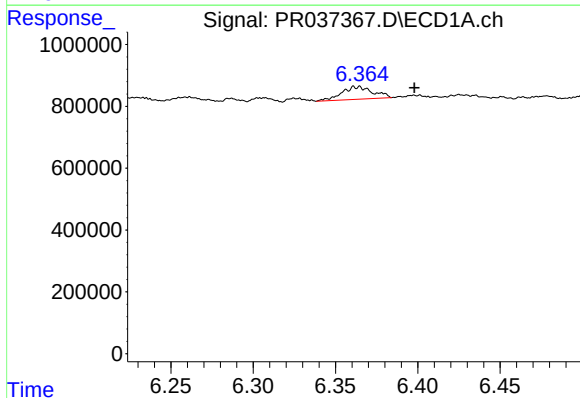


#24 AR-1248-4

R.T.: 6.363 min
Delta R.T.: -0.035 min
Response: 534583
Conc: 10.92 ng/ml

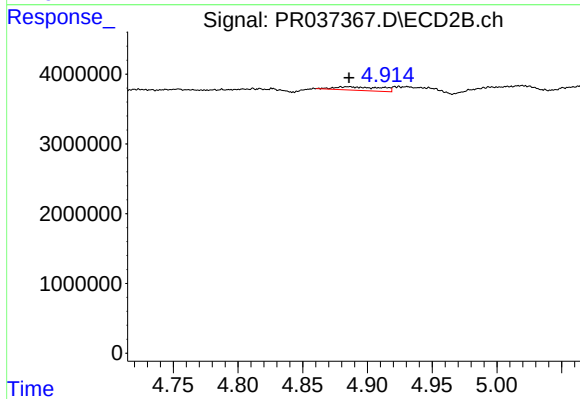

#24 AR-1248-4


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 1290310
Conc: 7.25 ng/ml

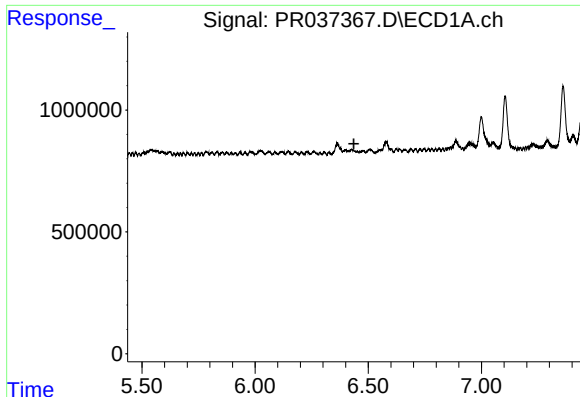

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

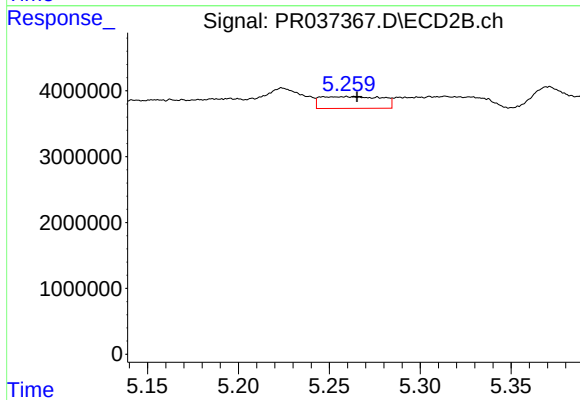


#25 AR-1248-5

R.T.: 5.263 min
Delta R.T.: -0.002 min
Response: 4203946
Conc: 21.49 ng/ml

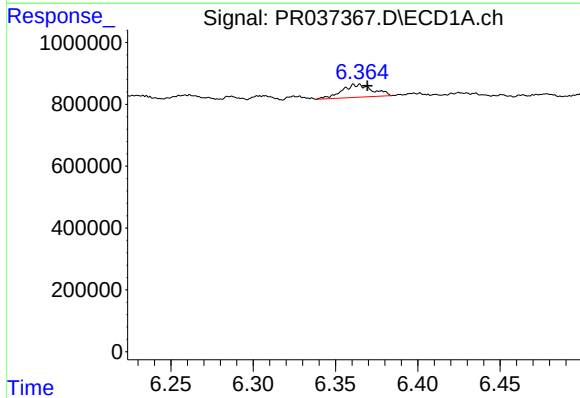


#26 AR-1254-1

R.T.: 6.363 min
Delta R.T.: -0.006 min
Response: 534583
Conc: 9.79 ng/ml

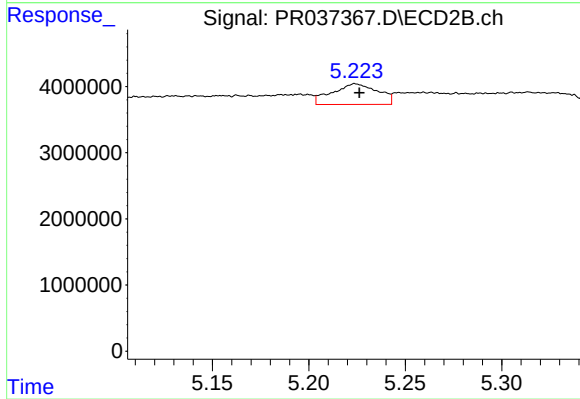

#26 AR-1254-1


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 5120026
Conc: 14.86 ng/ml

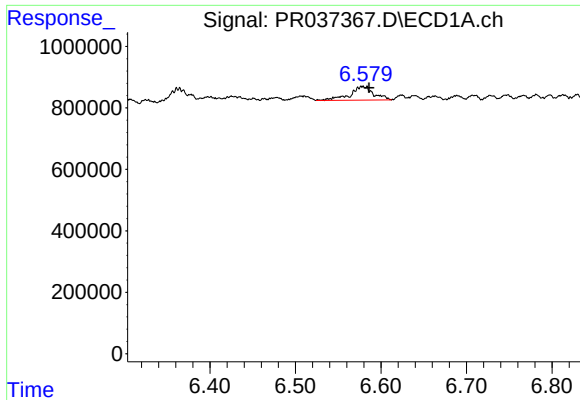

#27 AR-1254-2


R.T.: 6.578 min
Delta R.T.: -0.008 min
Response: 845070
Conc: 9.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

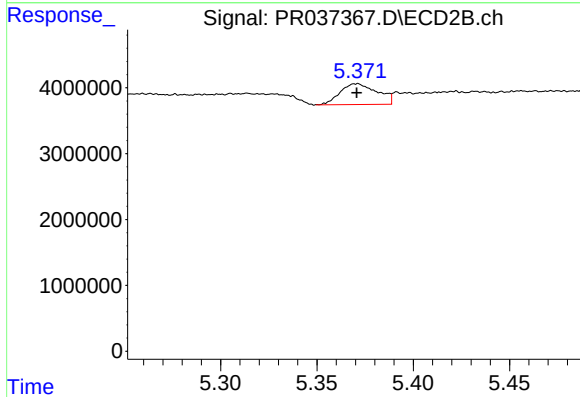


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 4251772
Conc: 14.20 ng/ml

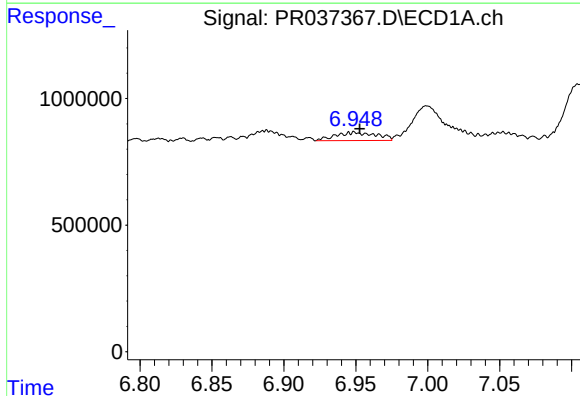


#28 AR-1254-3

R.T.: 6.949 min
Delta R.T.: -0.004 min
Response: 643462
Conc: 7.07 ng/ml

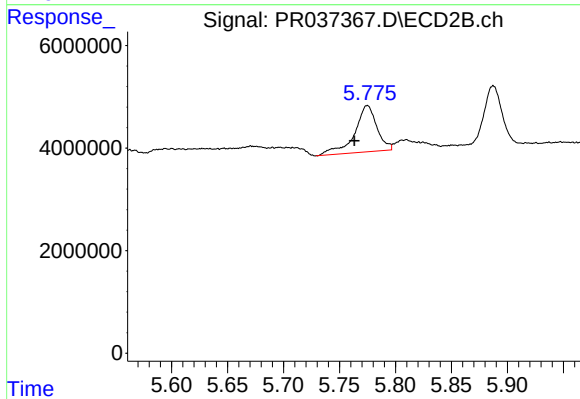

#28 AR-1254-3


R.T.: 5.775 min
Delta R.T.: 0.012 min
Response: 12570706
Conc: 26.54 ng/ml

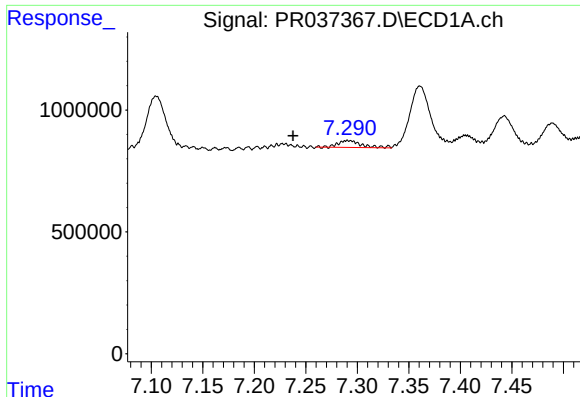

#29 AR-1254-4


R.T.: 7.291 min
Delta R.T.: 0.053 min
Response: 446893
Conc: 6.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

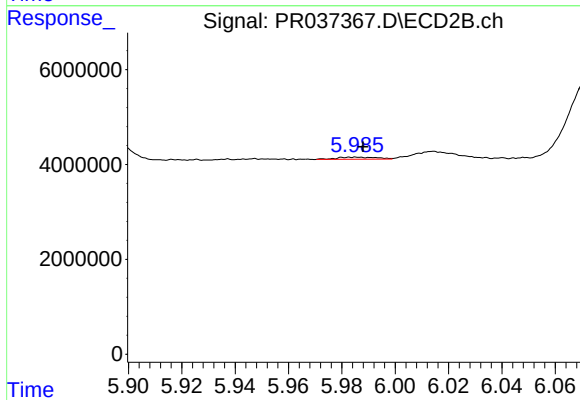


#29 AR-1254-4

R.T.: 5.985 min
Delta R.T.: -0.002 min
Response: 459277
Conc: 1.31 ng/ml

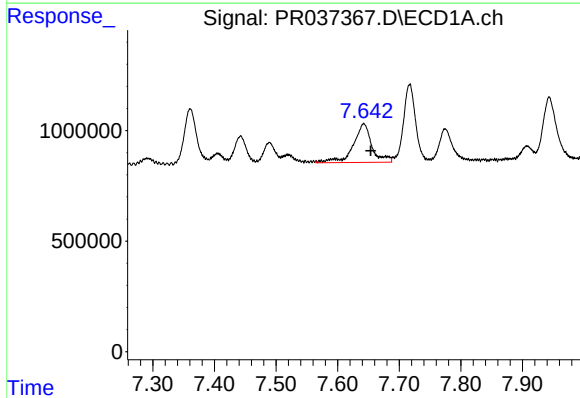


#30 AR-1254-5

R.T.: 7.642 min
Delta R.T.: -0.011 min
Response: 3663431
Conc: 50.97 ng/ml

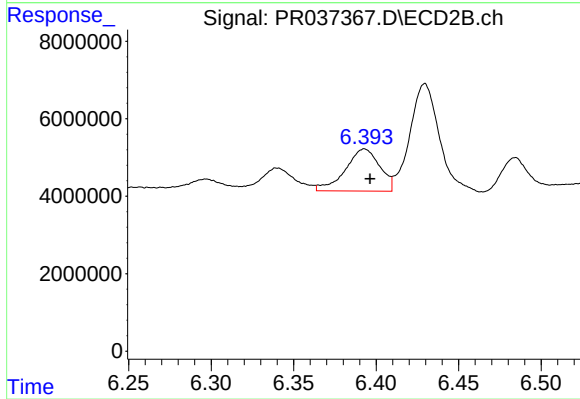

#30 AR-1254-5


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 15764419
Conc: 35.60 ng/ml

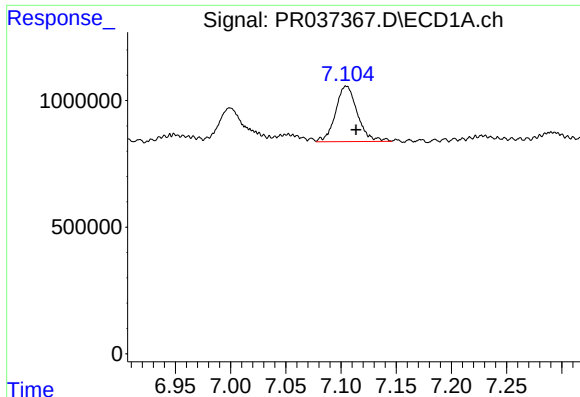

#31 AR-1260-1


R.T.: 7.105 min
Delta R.T.: -0.009 min
Response: 3012479
Conc: 45.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

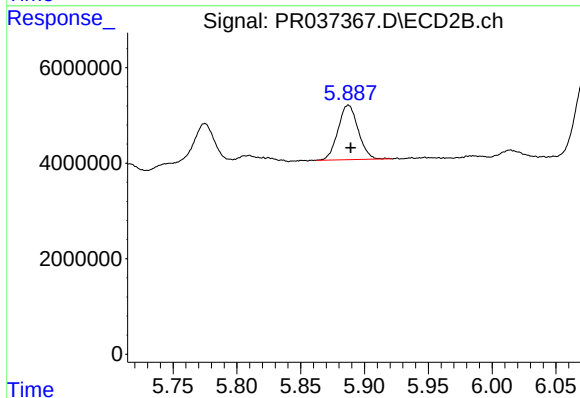


#31 AR-1260-1

R.T.: 5.887 min
Delta R.T.: -0.002 min
Response: 12559894
Conc: 42.97 ng/ml

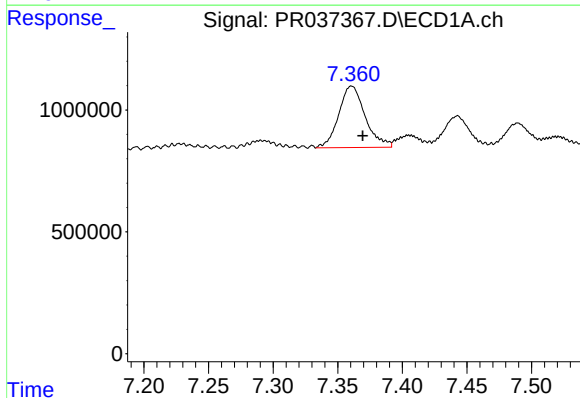


#32 AR-1260-2

R.T.: 7.361 min
Delta R.T.: -0.009 min
Response: 3602865
Conc: 45.20 ng/ml

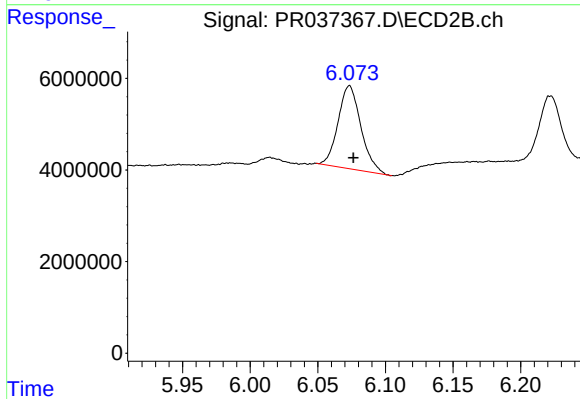

#32 AR-1260-2


R.T.: 6.073 min
Delta R.T.: -0.003 min
Response: 20995459
Conc: 45.58 ng/ml

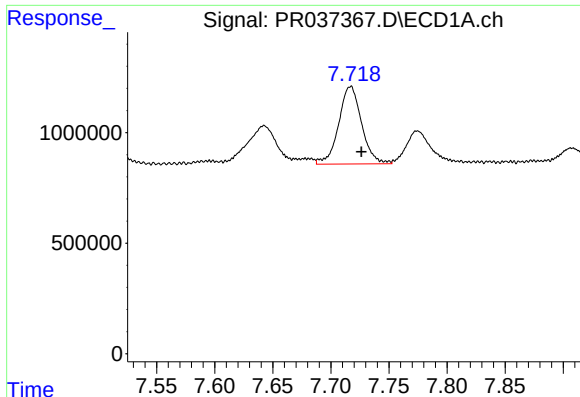

#33 AR-1260-3


R.T.: 7.717 min
Delta R.T.: -0.009 min
Response: 4826118
Conc: 77.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

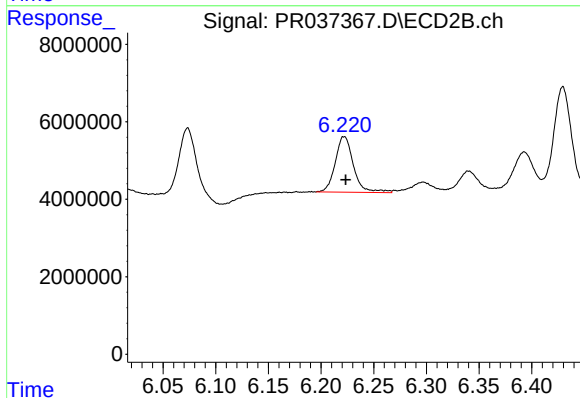


#33 AR-1260-3

R.T.: 6.222 min
Delta R.T.: -0.001 min
Response: 17234633
Conc: 48.34 ng/ml

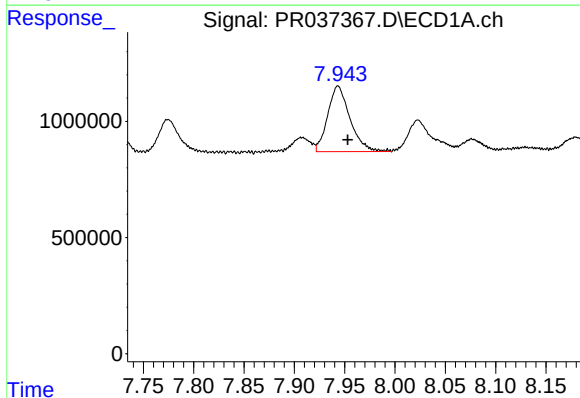


#34 AR-1260-4

R.T.: 7.943 min
Delta R.T.: -0.010 min
Response: 4355530
Conc: 58.54 ng/ml

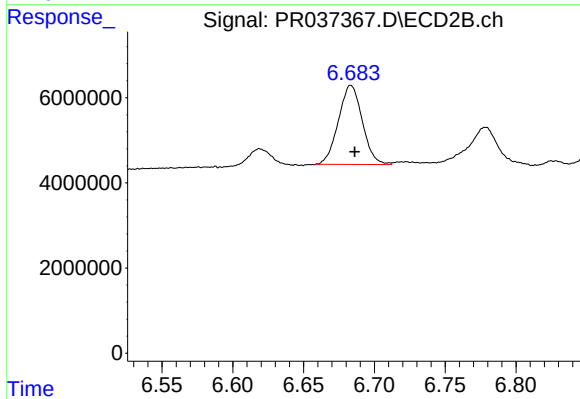

#34 AR-1260-4


R.T.: 6.683 min
Delta R.T.: -0.003 min
Response: 21794051
Conc: 71.51 ng/ml

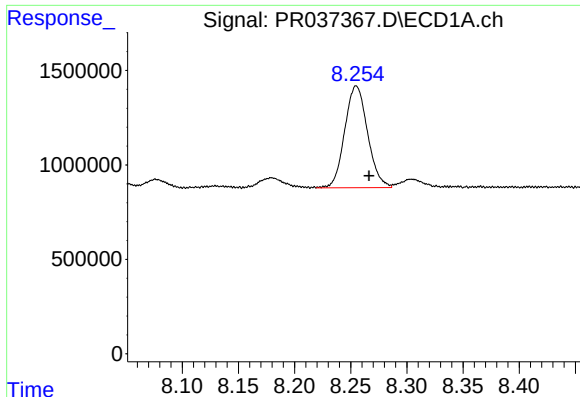

#35 AR-1260-5


R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 7647028
Conc: 52.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

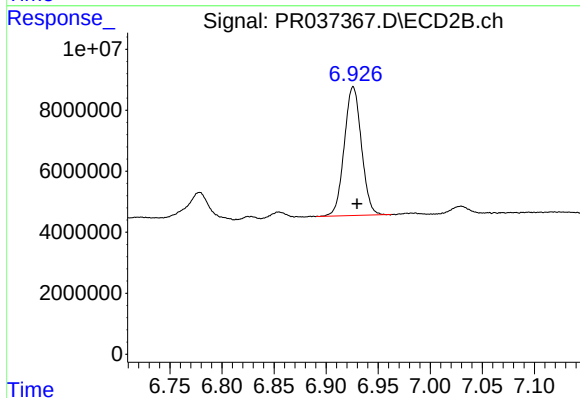


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 48459048
Conc: 55.88 ng/ml

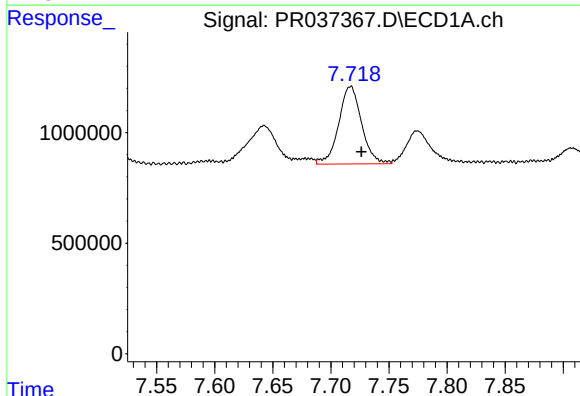


#36 AR-1262-1

R.T.: 7.717 min
Delta R.T.: -0.009 min
Response: 4826118
Conc: 46.20 ng/ml

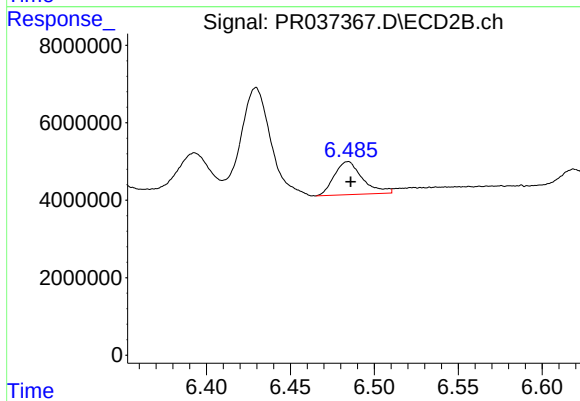

#36 AR-1262-1


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 9993613
Conc: 39.88 ng/ml

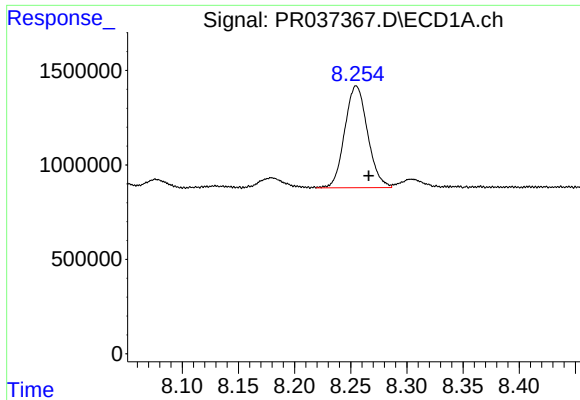

#37 AR-1262-2


R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 7647028
Conc: 39.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

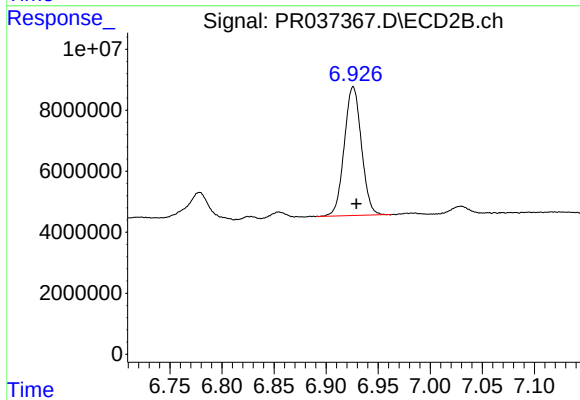


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 48459048
Conc: 38.58 ng/ml

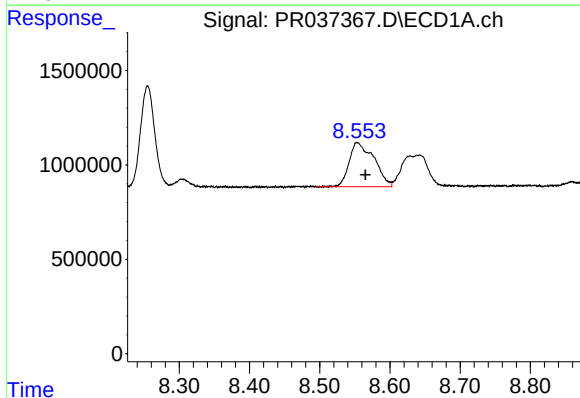


#38 AR-1262-3

R.T.: 8.553 min
Delta R.T.: -0.012 min
Response: 5760009
Conc: 43.80 ng/ml

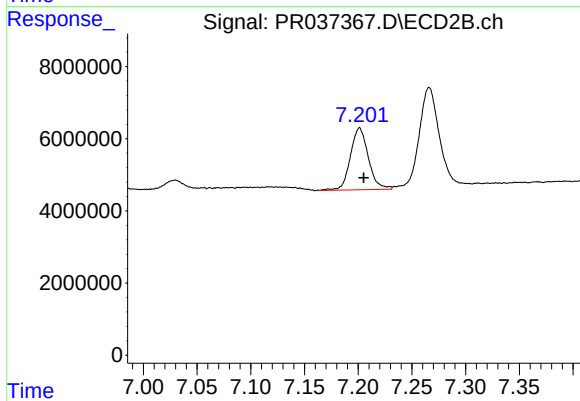

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 20039287
Conc: 36.55 ng/ml

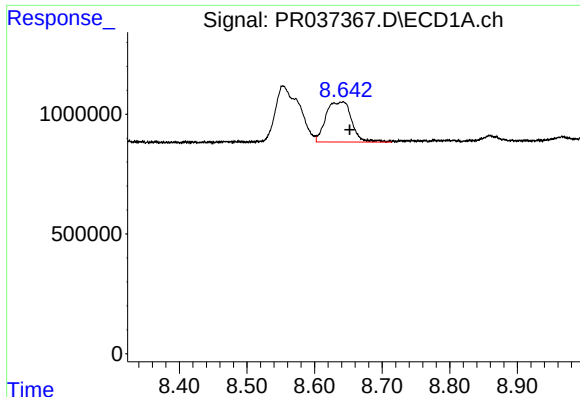

#39 AR-1262-4


R.T.: 8.642 min
Delta R.T.: -0.009 min
Response: 4449815
Conc: 45.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

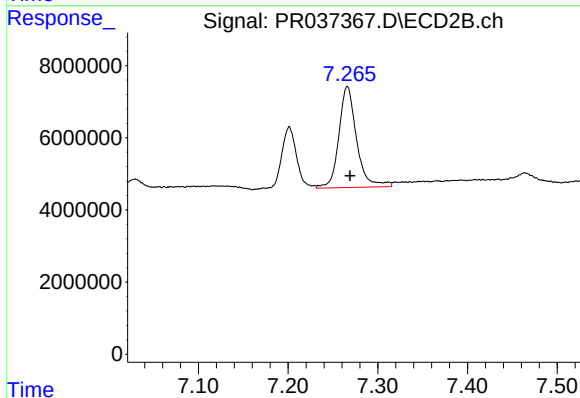


#39 AR-1262-4

R.T.: 7.266 min
Delta R.T.: -0.003 min
Response: 38598221
Conc: 43.00 ng/ml

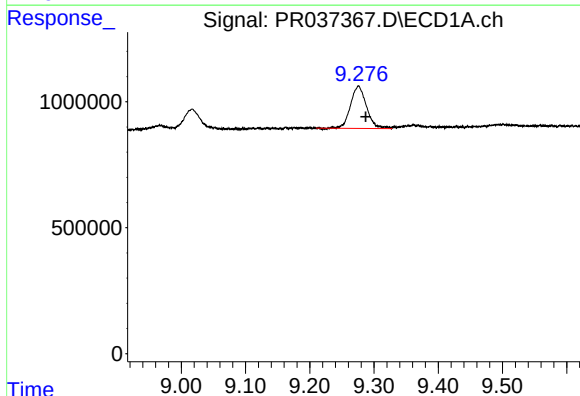


#40 AR-1262-5

R.T.: 9.276 min
Delta R.T.: -0.011 min
Response: 2893430
Conc: 41.91 ng/ml

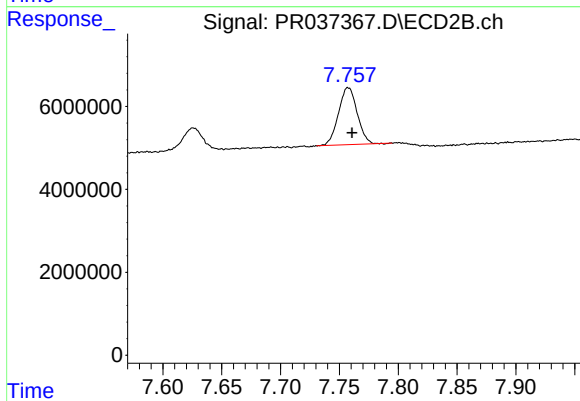

#40 AR-1262-5


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 15272450
Conc: 39.92 ng/ml

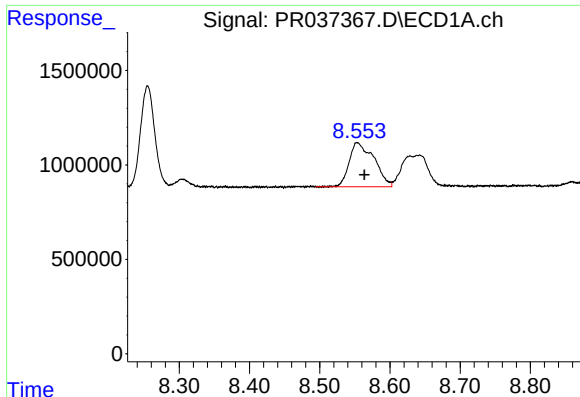

#41 AR-1268-1


R.T.: 8.553 min
Delta R.T.: -0.010 min
Response: 5760009
Conc: 32.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

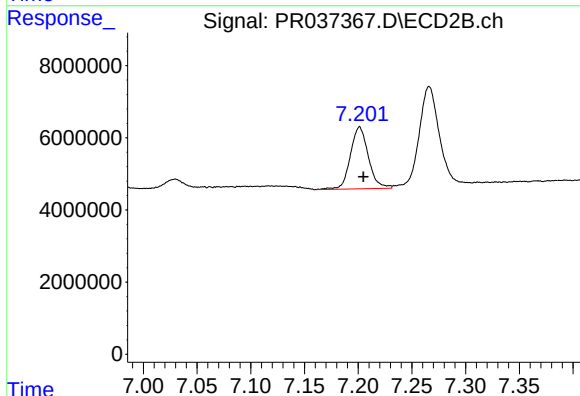


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.003 min
Response: 20039287
Conc: 16.28 ng/ml

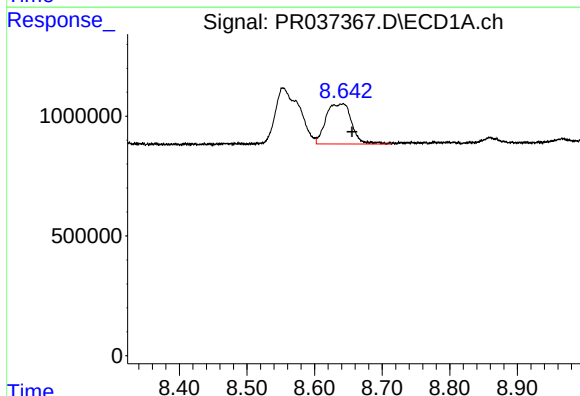


#42 AR-1268-2

R.T.: 8.642 min
Delta R.T.: -0.013 min
Response: 4449815
Conc: 27.05 ng/ml

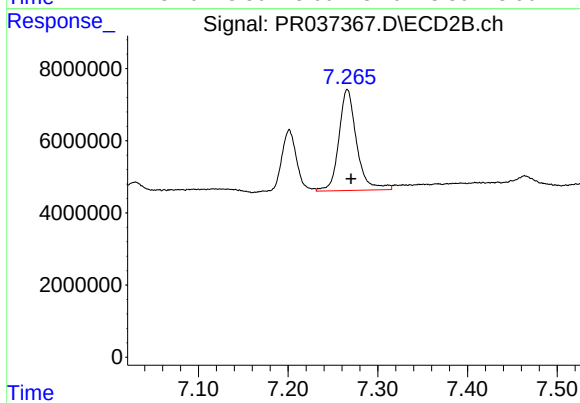

#42 AR-1268-2


R.T.: 7.266 min
Delta R.T.: -0.004 min
Response: 38598221
Conc: 36.45 ng/ml

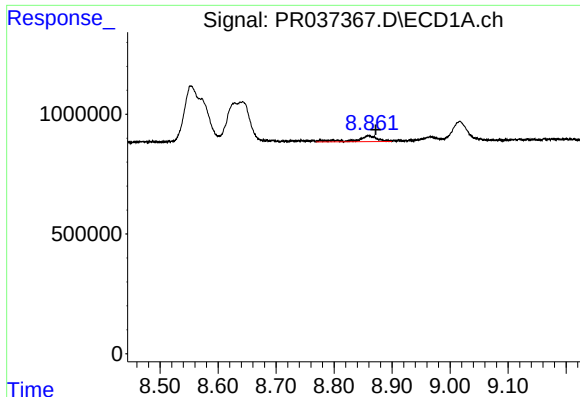

#43 AR-1268-3


R.T.: 8.859 min
Delta R.T.: -0.013 min
Response: 627472
Conc: 4.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

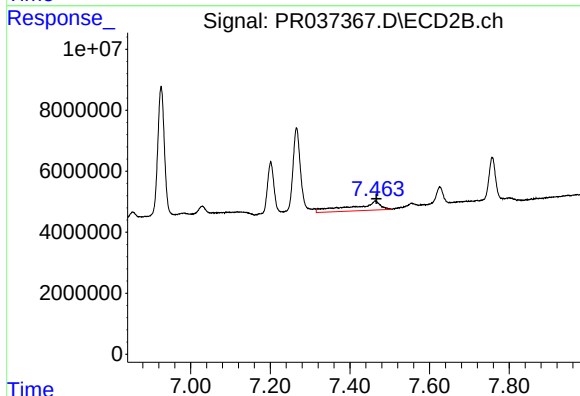


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 15048080
Conc: 16.98 ng/ml

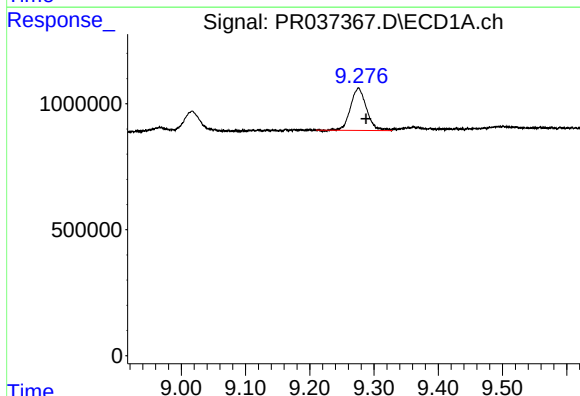


#44 AR-1268-4

R.T.: 9.276 min
Delta R.T.: -0.012 min
Response: 2893430
Conc: 46.38 ng/ml

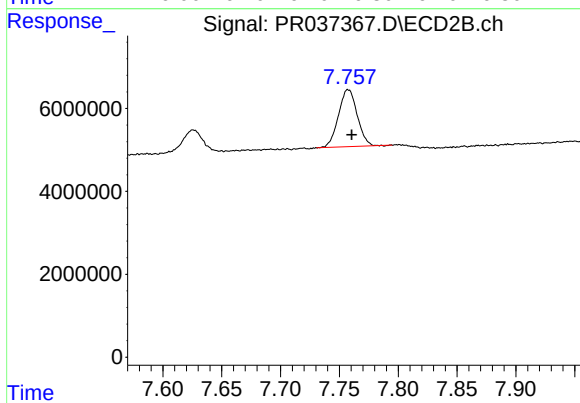

#44 AR-1268-4


R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 15272450
Conc: 42.10 ng/ml

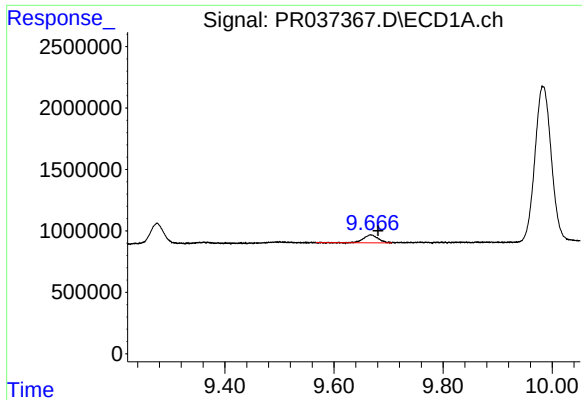

#45 AR-1268-5

R.T.: 9.667 min
Delta R.T.: -0.014 min
Response: 1217592
Conc: 2.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

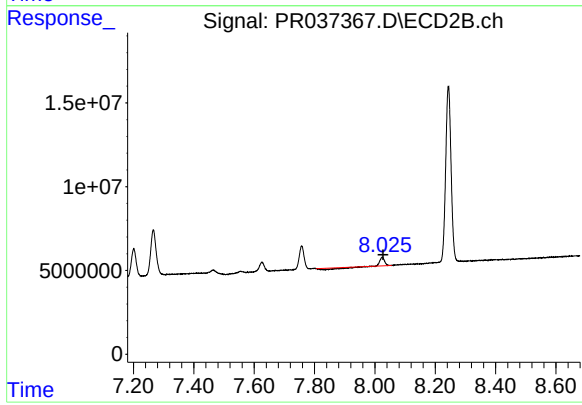

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.003 min
Response: 1928538
Conc: 0.76 ng/ml