

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:30
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1268 LOD 25PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:09:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	29081729	118.4E6	23.247	24.695
2)	SA Decachlor...	9.985	8.243	32028979	166.2E6	24.217	28.534
Target Compounds							
3)	L1 AR-1016-1	0.000	4.460	0	456664	N.D.	2.508 #
4)	L1 AR-1016-2	0.000	4.460	0	456664	N.D.	1.619 #
5)	L1 AR-1016-3	0.000	4.600	0	63060	N.D.	0.439 #
6)	L1 AR-1016-4	0.000	4.682	0	404584	N.D.	3.657 #
7)	L1 AR-1016-5	0.000	4.928	0	1293068	N.D.	8.507 #
8)	L2 AR-1221-1	0.000	3.664	0	81702	N.D.	1.605 #
9)	L2 AR-1221-2	4.663	3.698	420173	1658098	46.459	44.650
10)	L2 AR-1221-3	0.000	3.741	0	89564	N.D.	0.731 #
11)	L3 AR-1232-1	0.000	3.741	0	89564	N.D.	0.766 #
12)	L3 AR-1232-2	0.000	4.460	0	456664	N.D.	3.304 #
13)	L3 AR-1232-3	0.000	4.600	0	63060	N.D.	0.898 #
14)	L3 AR-1232-4	0.000	4.703	0	128051	N.D.	2.146 #
15)	L3 AR-1232-5	0.000	4.928	0	1293068	N.D.	18.948 #
16)	L4 AR-1242-1	0.000	4.460	0	456664	N.D.	3.116 #
17)	L4 AR-1242-2	0.000	4.460	0	456664	N.D.	2.002 #
18)	L4 AR-1242-3	0.000	4.600	0	63060	N.D.	0.545 #
19)	L4 AR-1242-4	0.000	4.735	0	39269	N.D.	0.357 #
20)	L4 AR-1242-5	0.000	5.256	0	1353678	N.D.	8.169 #
21)	L5 AR-1248-1	0.000	4.460	0	456664	N.D.	4.537 #
22)	L5 AR-1248-2	0.000	4.682	0	404584	N.D.	2.965 #
23)	L5 AR-1248-3	0.000	4.735	0	39269	N.D.	0.281 #
24)	L5 AR-1248-4	0.000	4.928	0	1293068	N.D.	7.266 #
25)	L5 AR-1248-5	0.000	5.256	0	1353678	N.D.	6.920 #
26)	L6 AR-1254-1	0.000	5.256	0	1353678	N.D.	3.930 #
27)	L6 AR-1254-2	0.000	5.330	0	724378	N.D.	2.419 #
28)	L6 AR-1254-3	0.000	5.768	0	1762587	N.D.	3.722 #
30)	L6 AR-1254-5	7.716	6.430	1155694	11104987	16.078	25.078 #
31)	L7 AR-1260-1	0.000	5.913	0	35443	N.D.	0.121 #
32)	L7 AR-1260-2	0.000	6.065	0	1607347	N.D.	3.490 #
33)	L7 AR-1260-3	7.716	6.221	1155694	503067	18.469	1.411 #
34)	L7 AR-1260-4	7.959	6.677	1807210	7810682	24.289	25.629
35)	L7 AR-1260-5	8.255	6.926	600457	3240953	4.152	3.737
36)	L8 AR-1262-1	7.716	6.490	1155694	2322284	11.064	9.266
37)	L8 AR-1262-2	8.255	6.926	600457	3240953	3.089	2.580
38)	L8 AR-1262-3	8.554	7.202	5686418	38871765	43.239	70.900 #
39)	L8 AR-1262-4	8.645	7.267	5209074	33705283	53.030	37.549 #
40)	L8 AR-1262-5	9.276	7.757	2047772	10921696	29.660	28.545
41)	L9 AR-1268-1	8.554	7.202	5686418	38871765	31.751	31.577
42)	L9 AR-1268-2	8.645	7.267	5209074	33705283	31.667	31.830

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:30
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1268 LOD 25PPB
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:09:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.861	7.464	4857251	28080809	35.086	31.685
44) L9	AR-1268-4	9.276	7.757	2047772	10921696	32.824	30.105
45) L9	AR-1268-5	9.668	8.024	13055700	74071281	28.639	29.114



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 19:30
Operator : SM\SJ
Sample : K2241-07
Misc : AR1268 LOD 25PPB
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:09:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

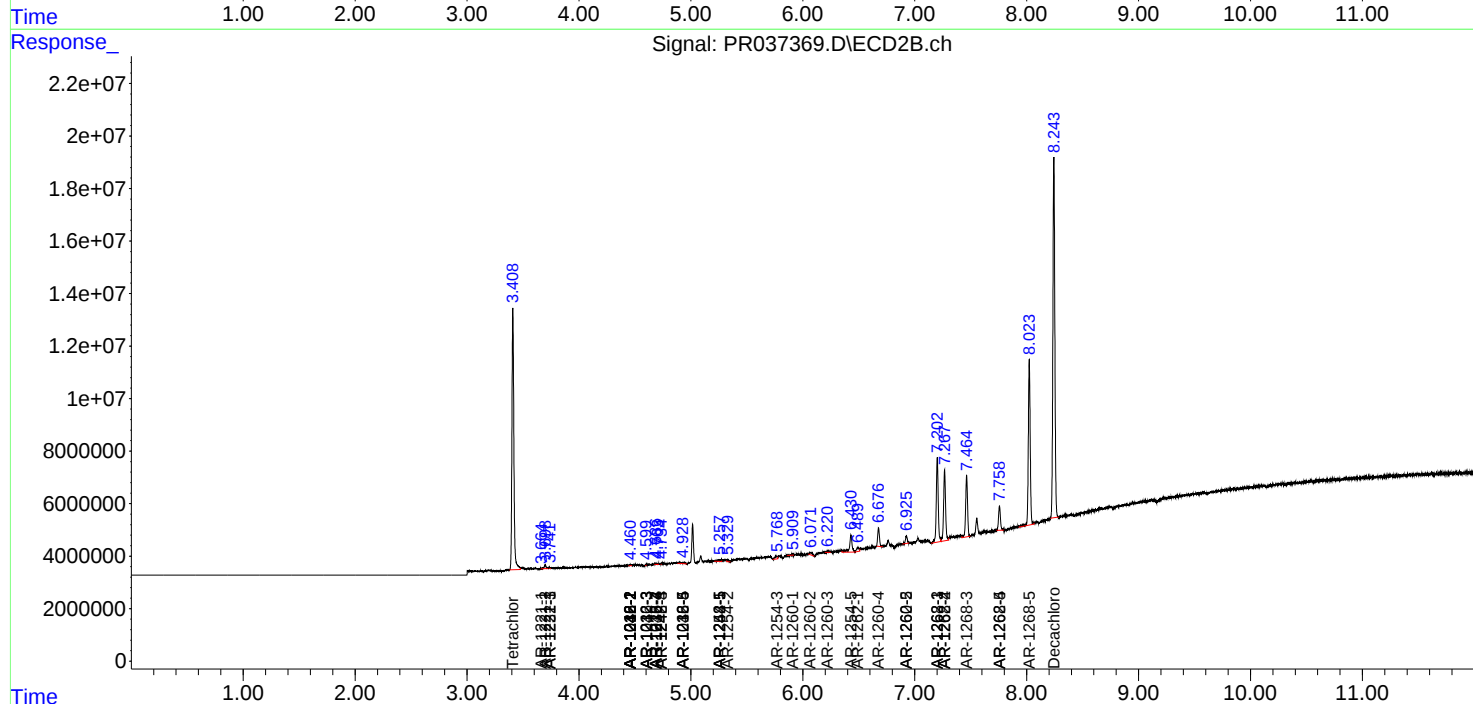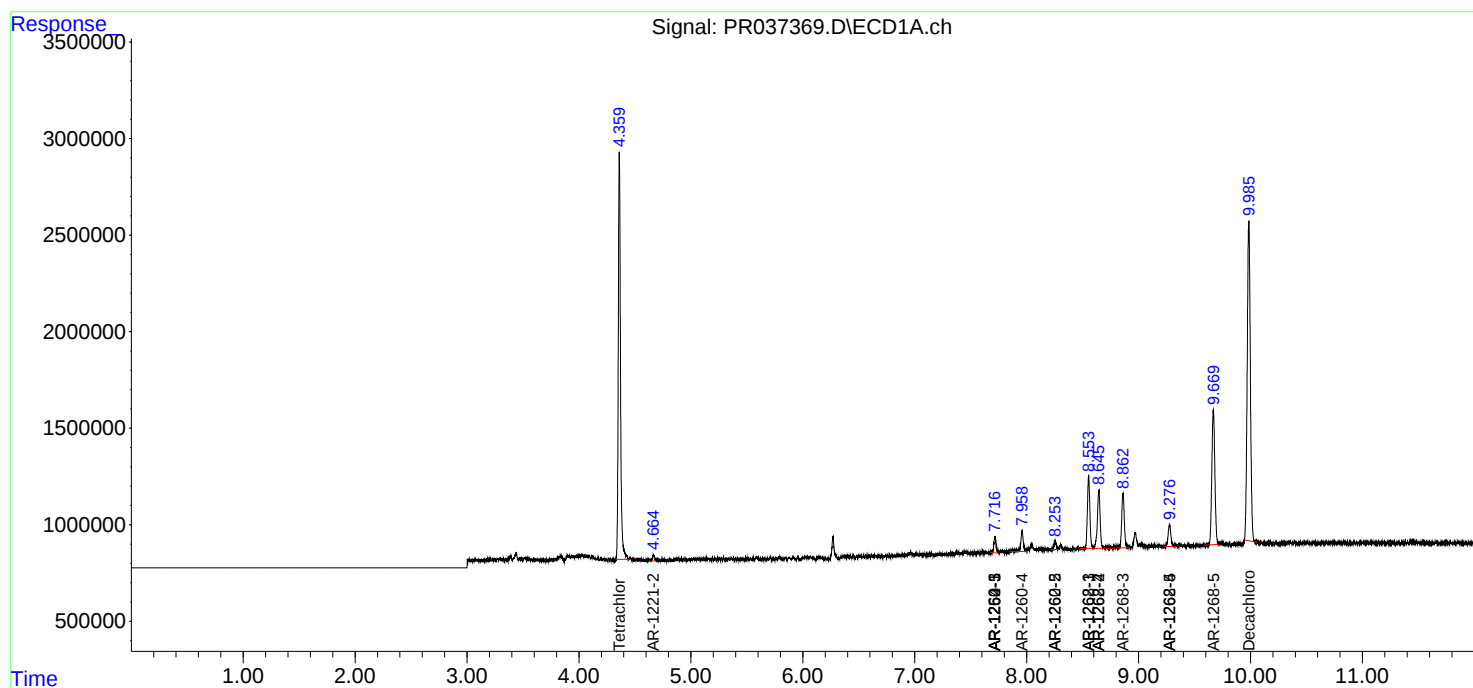


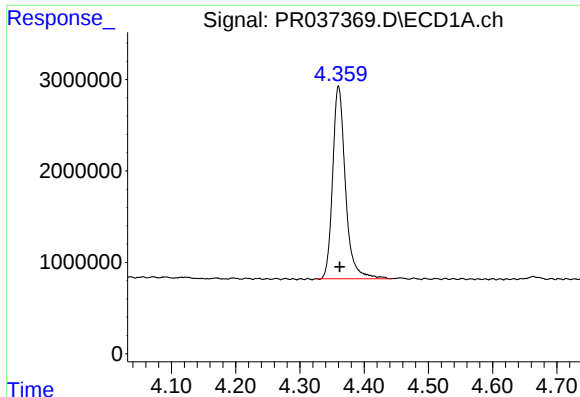

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 29081729
Conc: 23.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

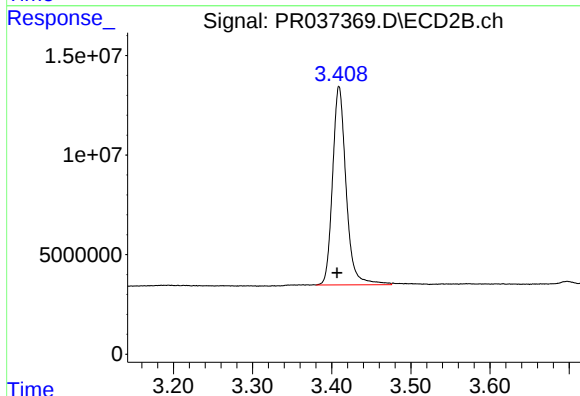


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.003 min
Response: 118427530
Conc: 24.70 ng/ml

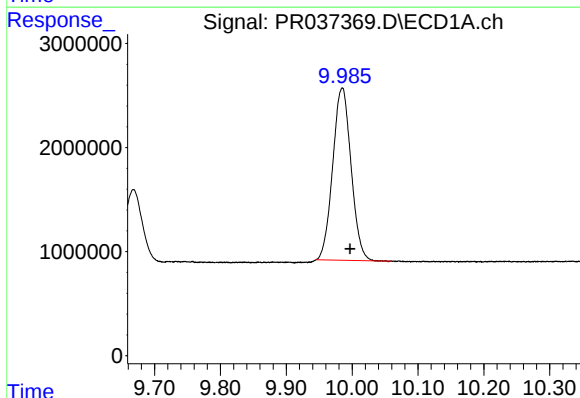


#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.012 min
Response: 32028979
Conc: 24.22 ng/ml

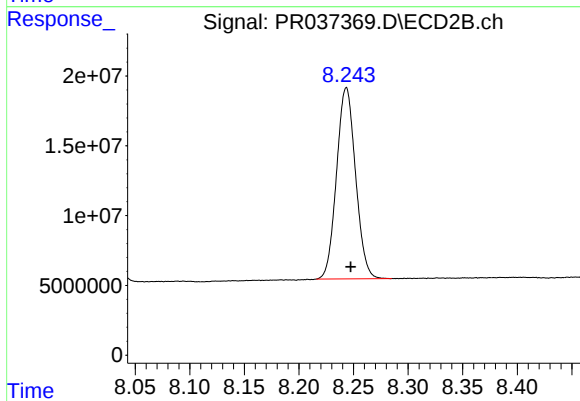

#2 Decachlorobiphenyl


R.T.: 8.243 min
Delta R.T.: -0.004 min
Response: 166189333
Conc: 28.53 ng/ml

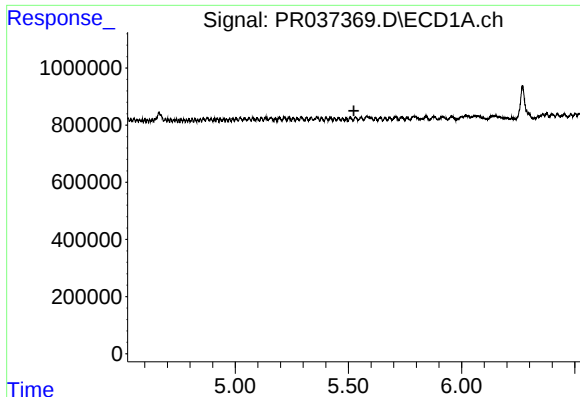

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

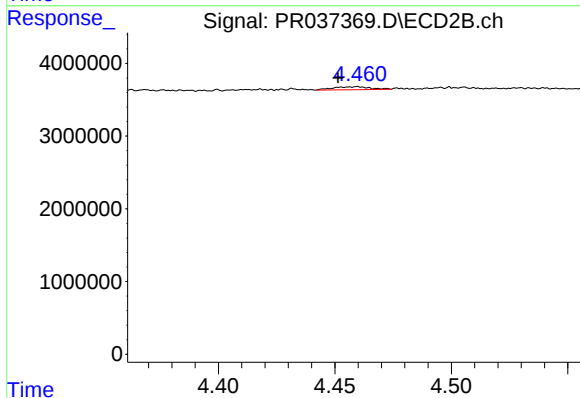


#3 AR-1016-1

R.T.: 4.460 min
Delta R.T.: 0.008 min
Response: 456664
Conc: 2.51 ng/ml

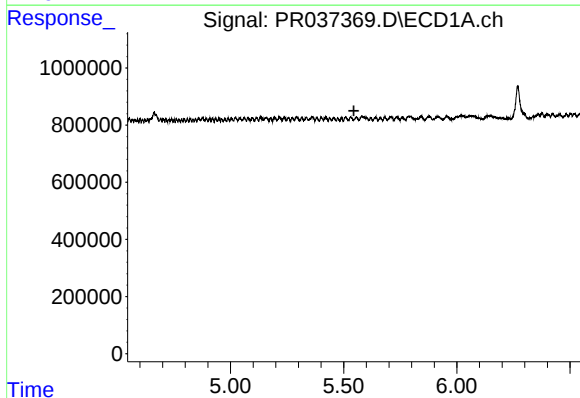


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

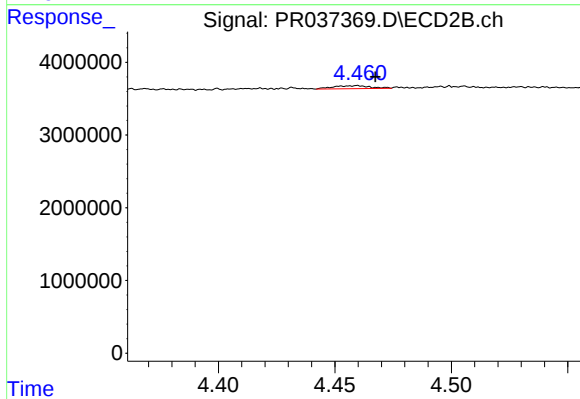

#4 AR-1016-2


R.T.: 4.460 min
Delta R.T.: -0.008 min
Response: 456664
Conc: 1.62 ng/ml

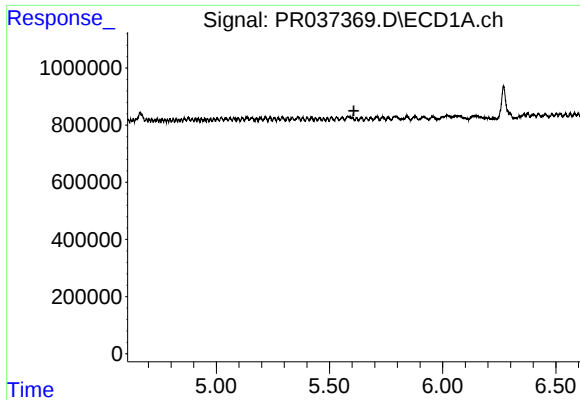

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

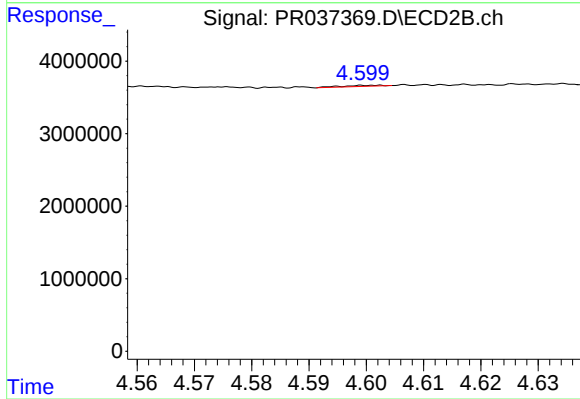


#5 AR-1016-3

R.T.: 4.600 min
Delta R.T.: -0.038 min
Response: 63060
Conc: 0.44 ng/ml

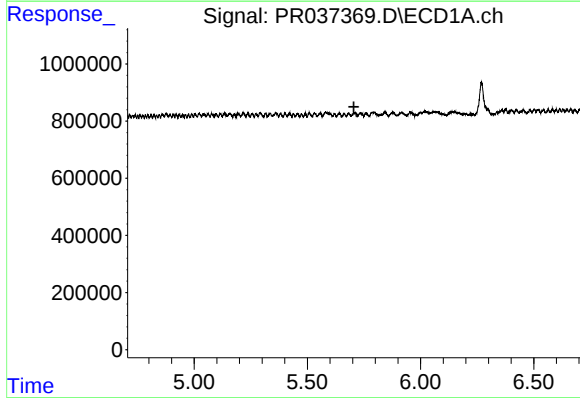


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

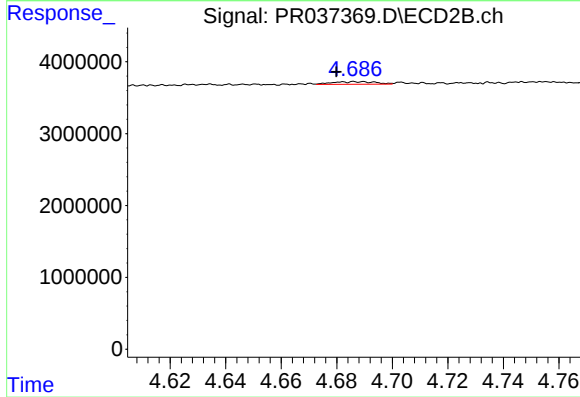

#6 AR-1016-4


R.T.: 4.682 min
Delta R.T.: 0.002 min
Response: 404584
Conc: 3.66 ng/ml

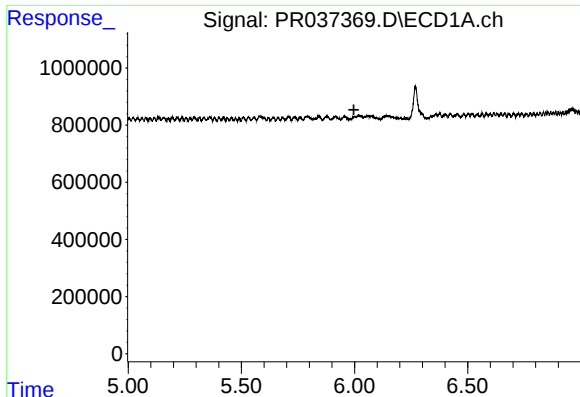

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

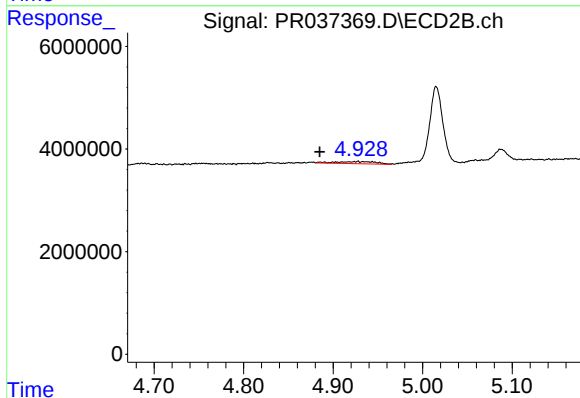


#7 AR-1016-5

R.T.: 4.928 min
Delta R.T.: 0.043 min
Response: 1293068
Conc: 8.51 ng/ml

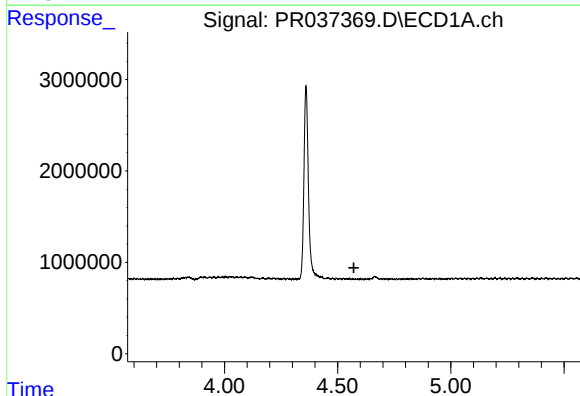


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

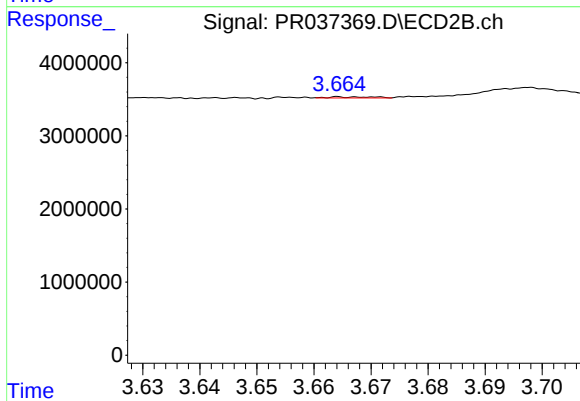

#8 AR-1221-1


R.T.: 3.664 min
Delta R.T.: 0.052 min
Response: 81702
Conc: 1.60 ng/ml

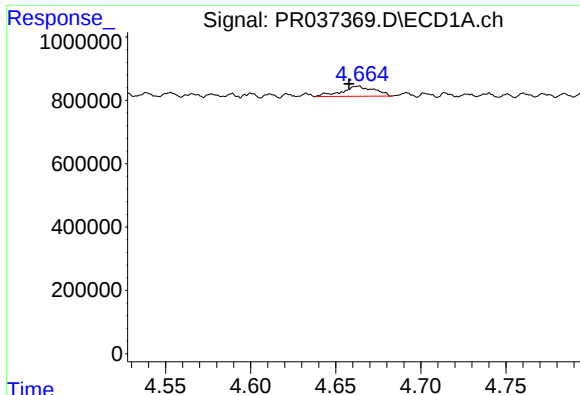

#9 AR-1221-2


R.T.: 4.663 min
Delta R.T.: 0.005 min
Response: 420173
Conc: 46.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

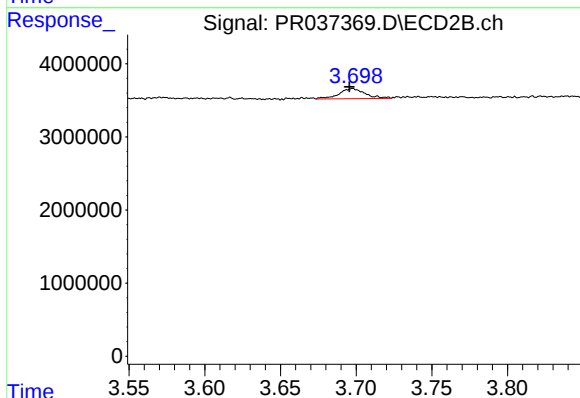


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 1658098
Conc: 44.65 ng/ml

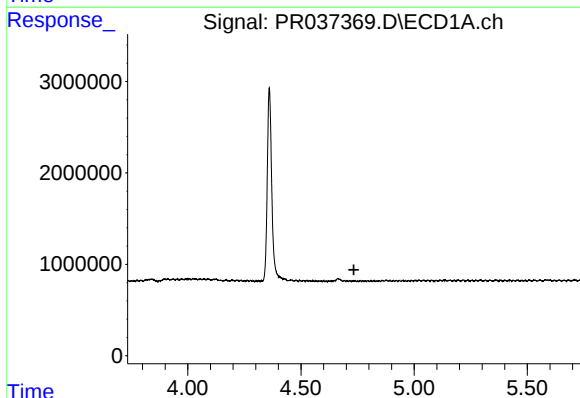


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

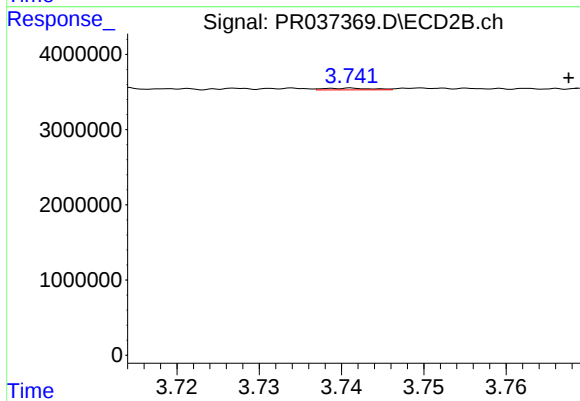

#10 AR-1221-3


R.T.: 3.741 min
Delta R.T.: -0.026 min
Response: 89564
Conc: 0.73 ng/ml

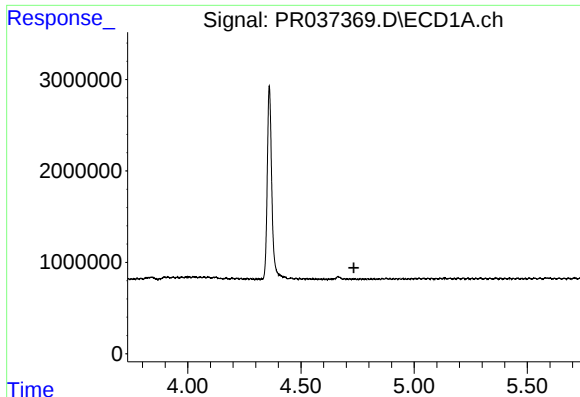

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

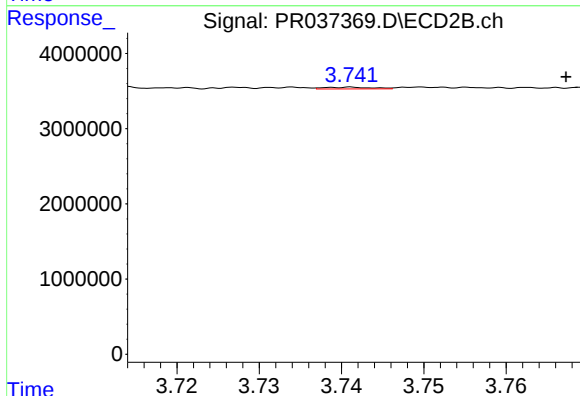


#11 AR-1232-1

R.T.: 3.741 min
Delta R.T.: -0.026 min
Response: 89564
Conc: 0.77 ng/ml

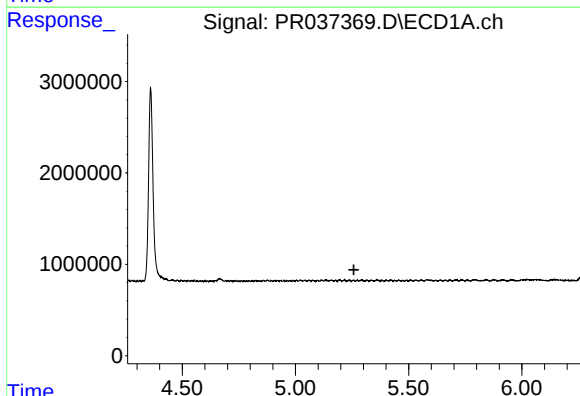


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

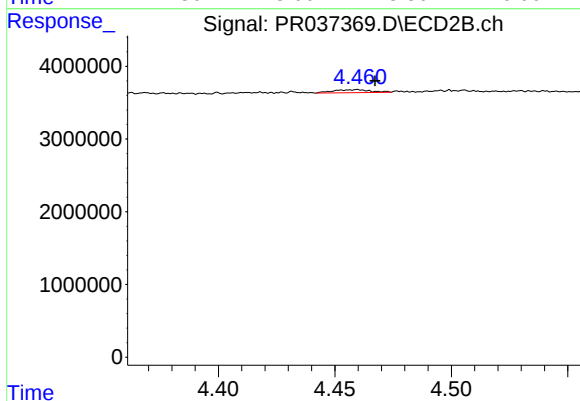

#12 AR-1232-2


R.T.: 4.460 min
Delta R.T.: -0.007 min
Response: 456664
Conc: 3.30 ng/ml

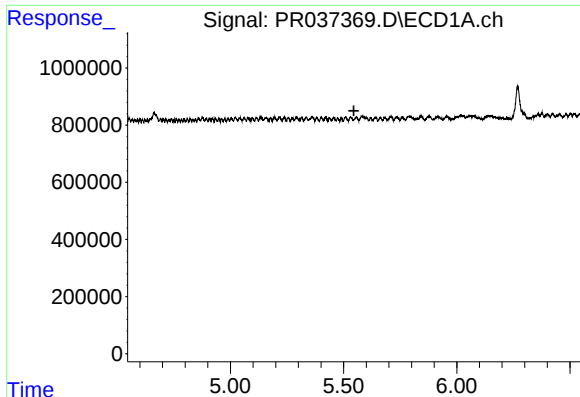

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

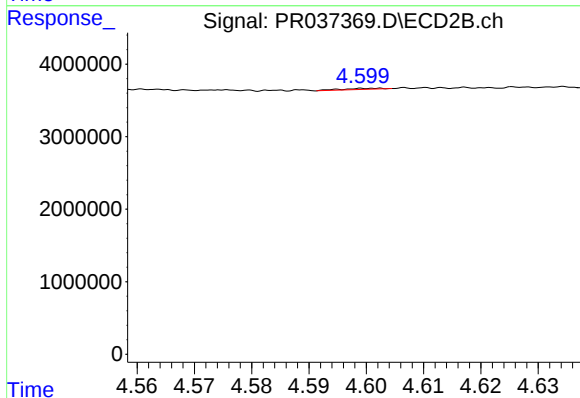


#13 AR-1232-3

R.T.: 4.600 min
Delta R.T.: -0.038 min
Response: 63060
Conc: 0.90 ng/ml

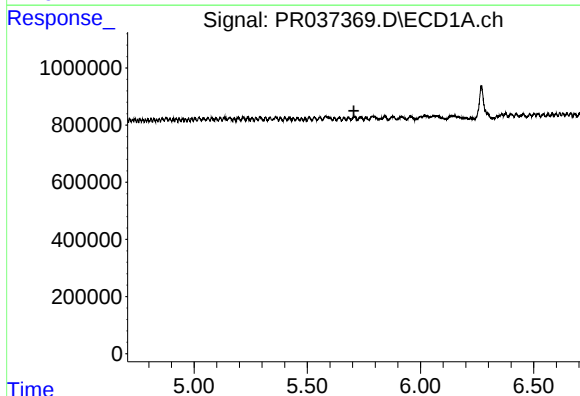


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

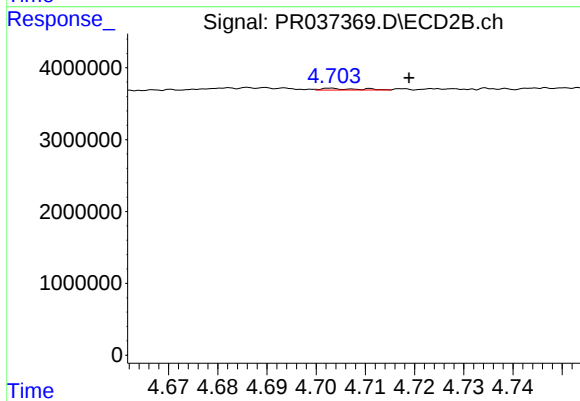

#14 AR-1232-4


R.T.: 4.703 min
Delta R.T.: -0.016 min
Response: 128051
Conc: 2.15 ng/ml

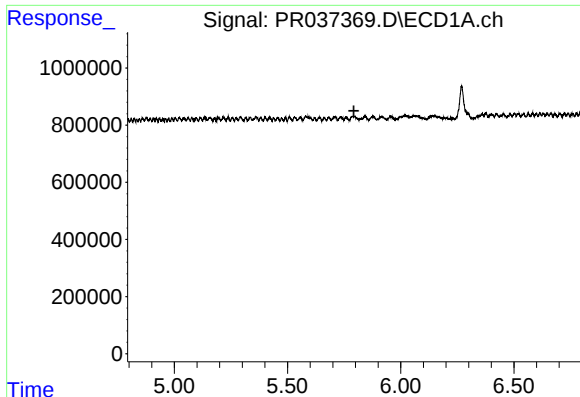

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

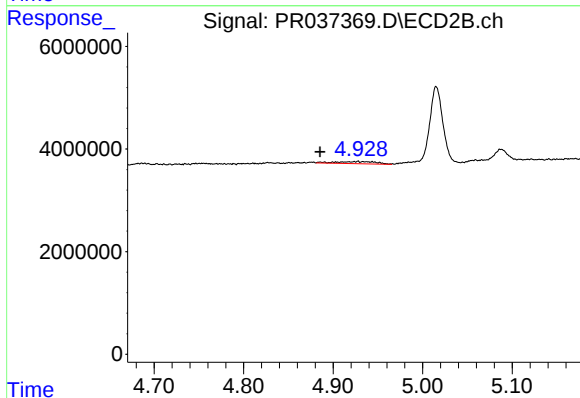


#15 AR-1232-5

R.T.: 4.928 min
Delta R.T.: 0.042 min
Response: 1293068
Conc: 18.95 ng/ml

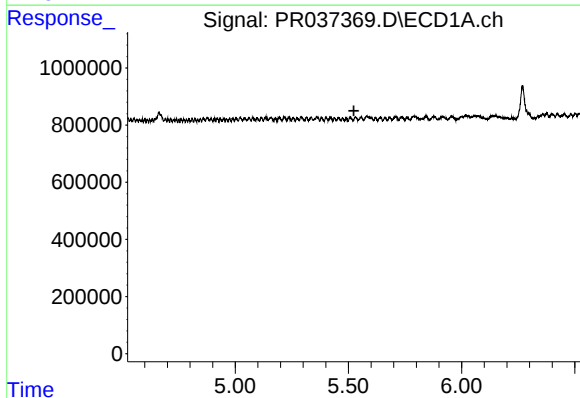


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

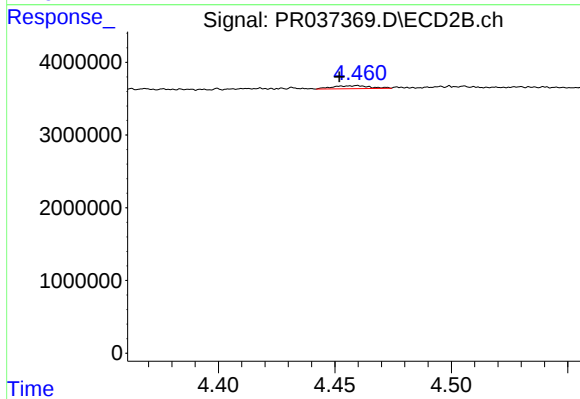

#16 AR-1242-1


R.T.: 4.460 min
Delta R.T.: 0.008 min
Response: 456664
Conc: 3.12 ng/ml

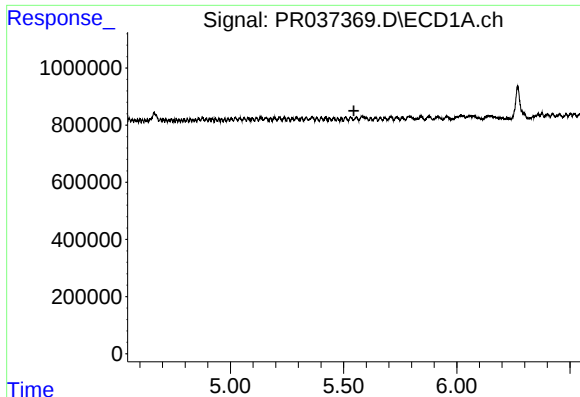

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

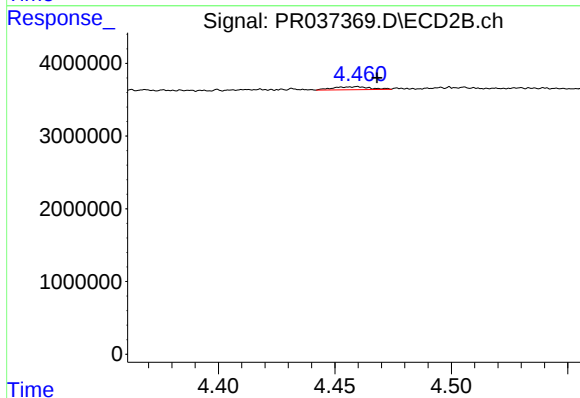


#17 AR-1242-2

R.T.: 4.460 min
Delta R.T.: -0.008 min
Response: 456664
Conc: 2.00 ng/ml

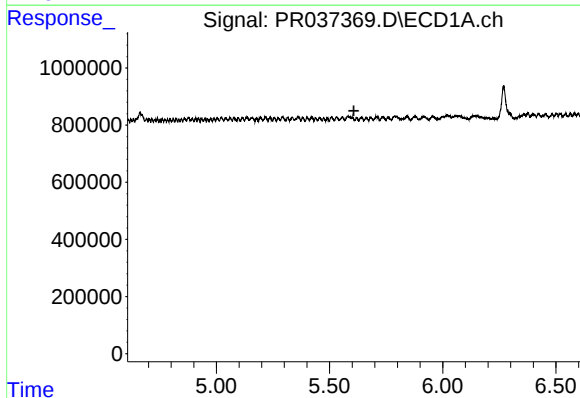


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

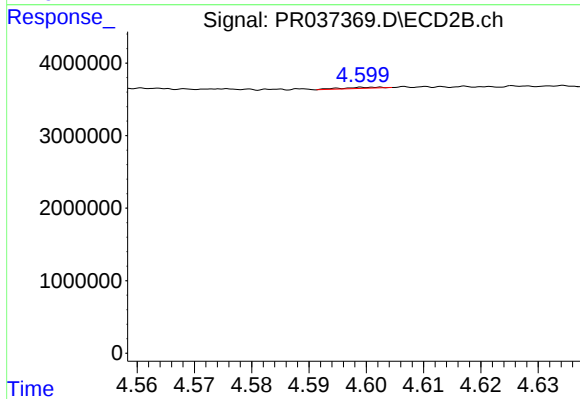

#18 AR-1242-3


R.T.: 4.600 min
Delta R.T.: -0.039 min
Response: 63060
Conc: 0.55 ng/ml

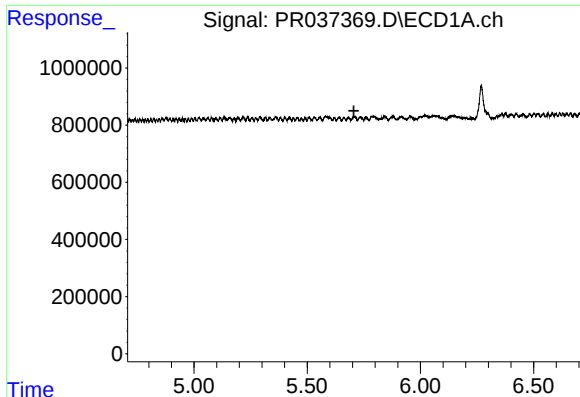

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

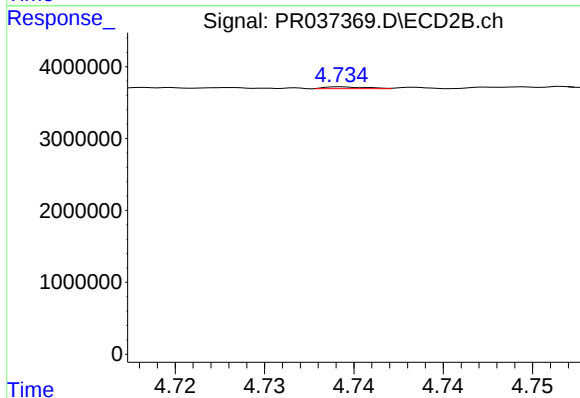


#19 AR-1242-4

R.T.: 4.735 min
Delta R.T.: 0.015 min
Response: 39269
Conc: 0.36 ng/ml

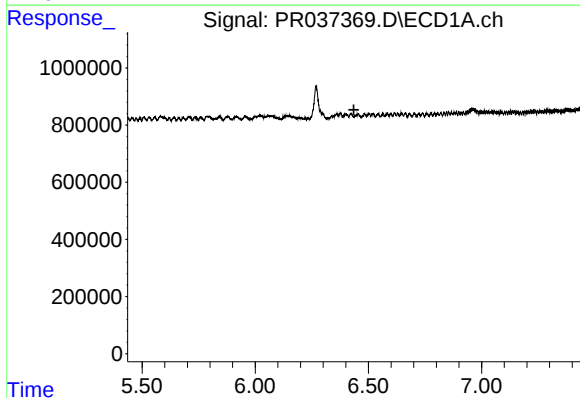


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

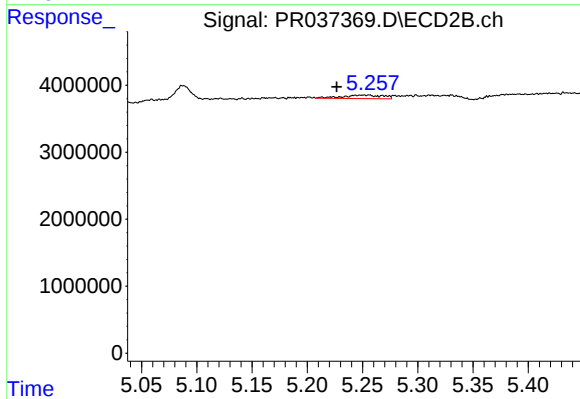

#20 AR-1242-5


R.T.: 5.256 min
Delta R.T.: 0.029 min
Response: 1353678
Conc: 8.17 ng/ml

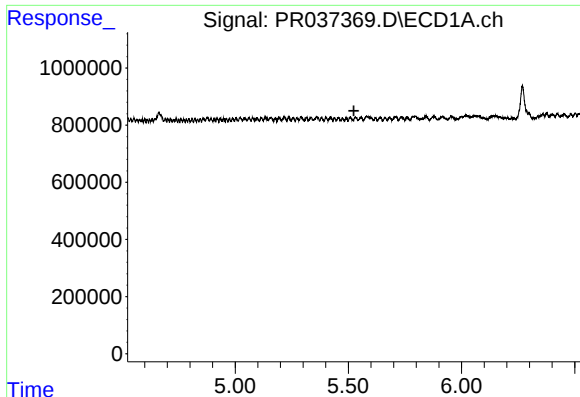

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

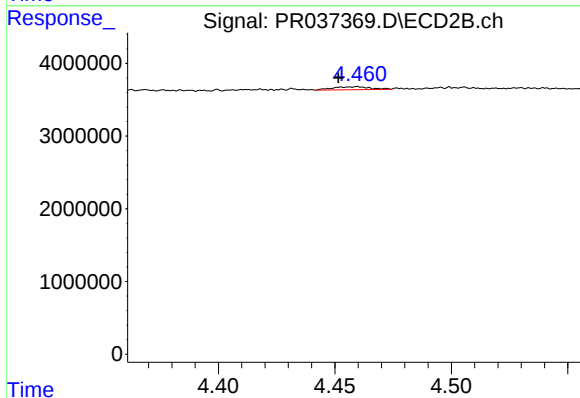


#21 AR-1248-1

R.T.: 4.460 min
Delta R.T.: 0.008 min
Response: 456664
Conc: 4.54 ng/ml

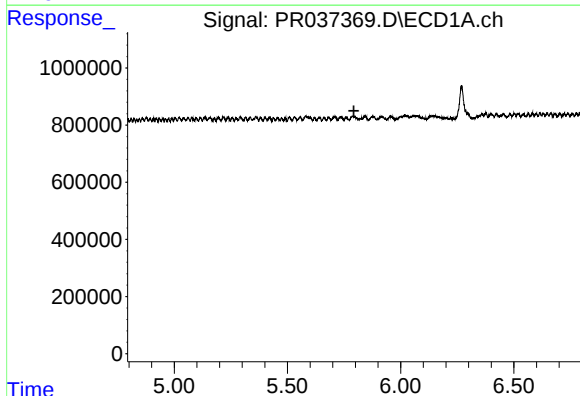


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

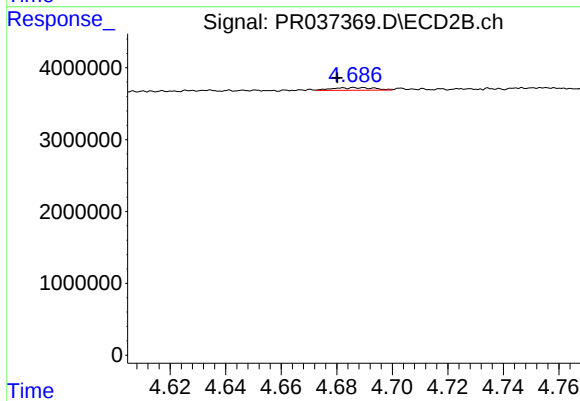

#22 AR-1248-2


R.T.: 4.682 min
Delta R.T.: 0.002 min
Response: 404584
Conc: 2.96 ng/ml

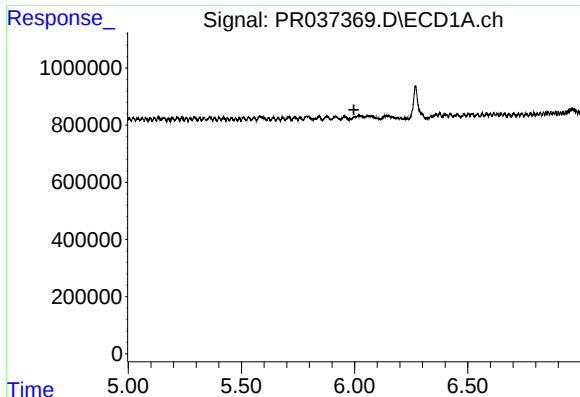

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

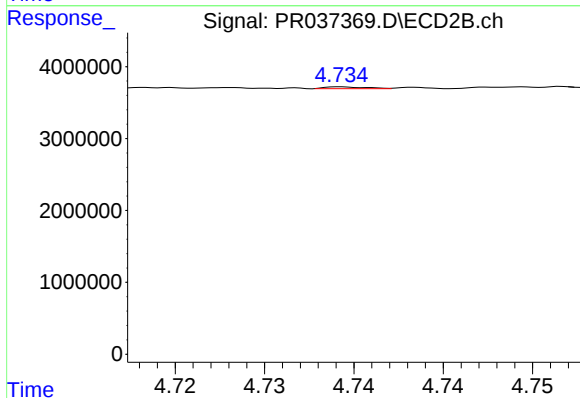


#23 AR-1248-3

R.T.: 4.735 min
Delta R.T.: 0.015 min
Response: 39269
Conc: 0.28 ng/ml

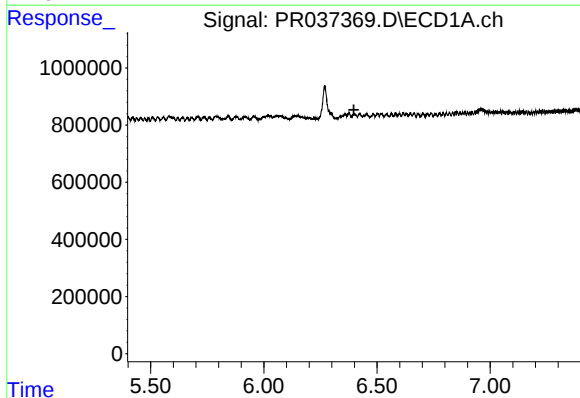


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

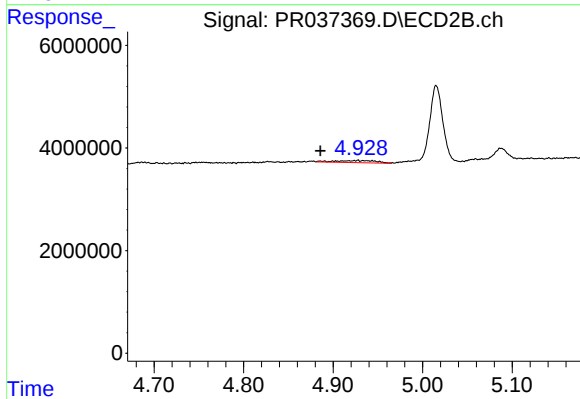

#24 AR-1248-4


R.T.: 4.928 min
Delta R.T.: 0.042 min
Response: 1293068
Conc: 7.27 ng/ml

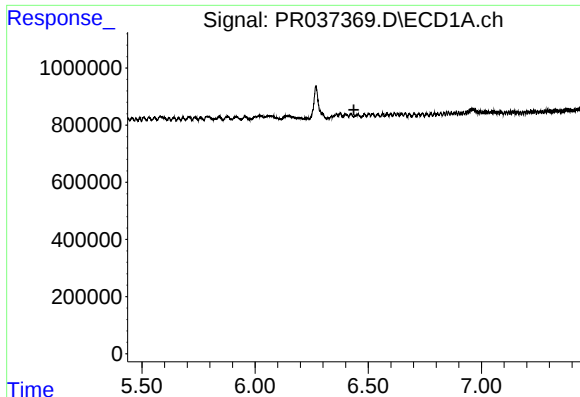

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

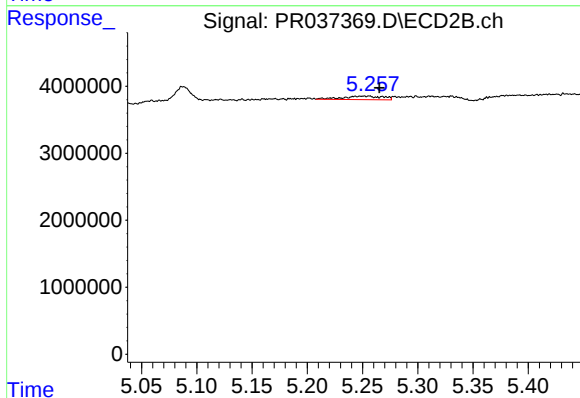


#25 AR-1248-5

R.T.: 5.256 min
Delta R.T.: -0.009 min
Response: 1353678
Conc: 6.92 ng/ml

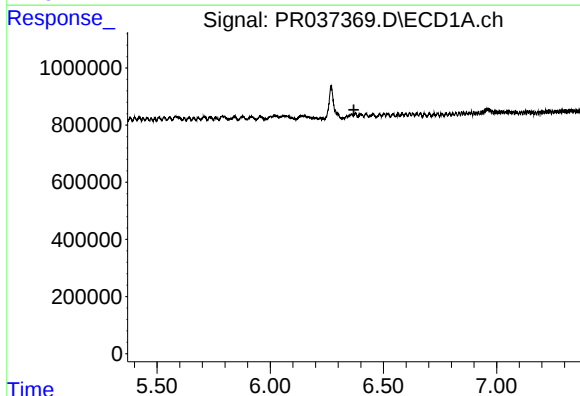


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

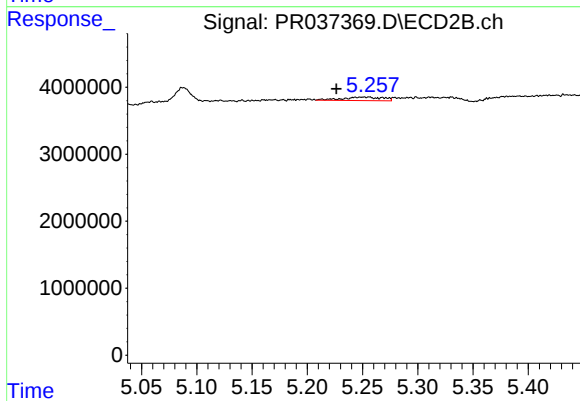

#26 AR-1254-1


R.T.: 5.256 min
Delta R.T.: 0.030 min
Response: 1353678
Conc: 3.93 ng/ml

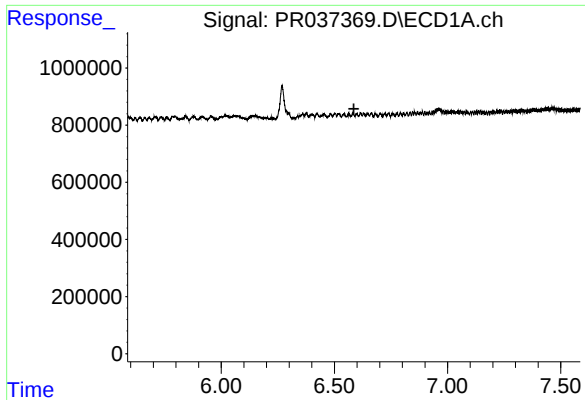

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

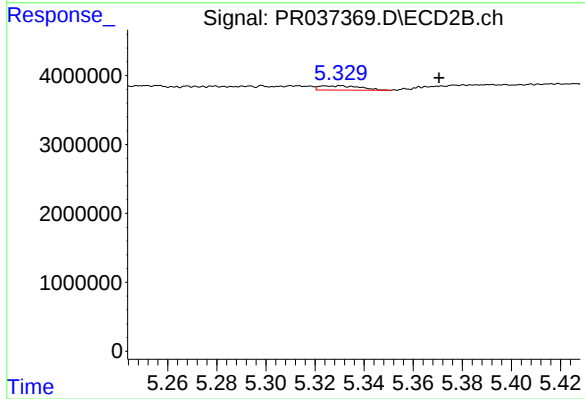


#27 AR-1254-2

R.T.: 5.330 min
Delta R.T.: -0.040 min
Response: 724378
Conc: 2.42 ng/ml

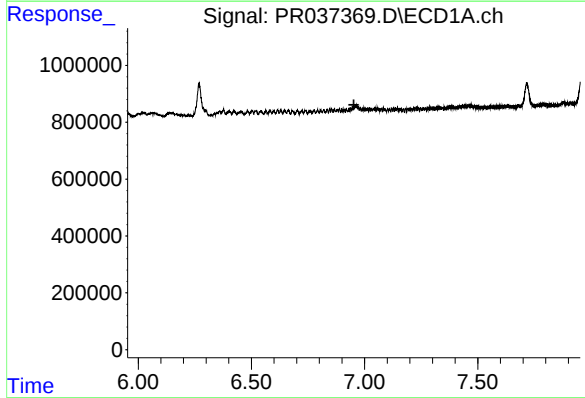


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.953 min
Response: 0
Conc: N.D.

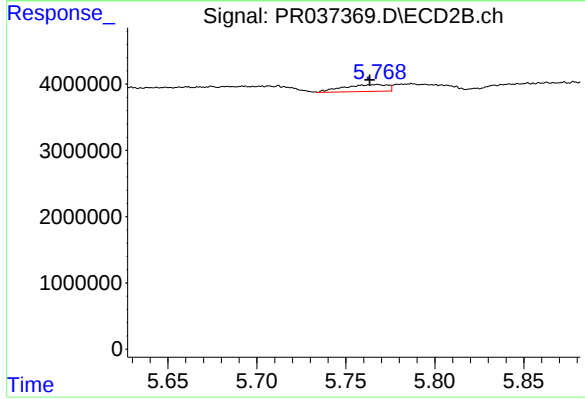

#28 AR-1254-3


R.T.: 5.768 min
Delta R.T.: 0.004 min
Response: 1762587
Conc: 3.72 ng/ml

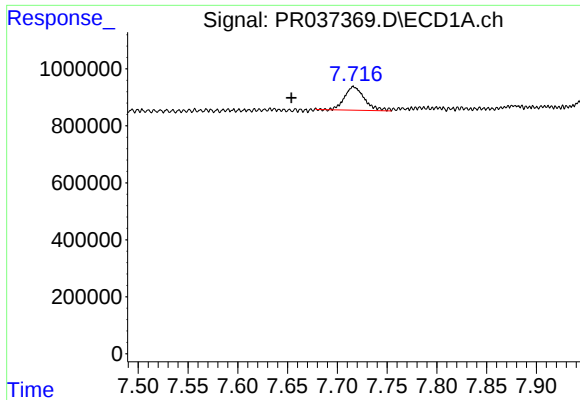

#30 AR-1254-5


R.T.: 7.716 min
Delta R.T.: 0.062 min
Response: 1155694
Conc: 16.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

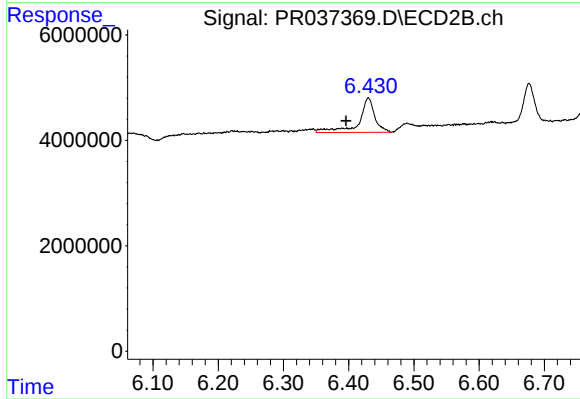


#30 AR-1254-5

R.T.: 6.430 min
Delta R.T.: 0.034 min
Response: 11104987
Conc: 25.08 ng/ml

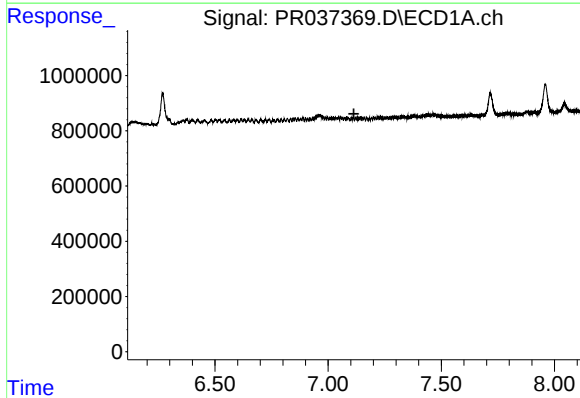


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.114 min
Response: 0
Conc: N.D.

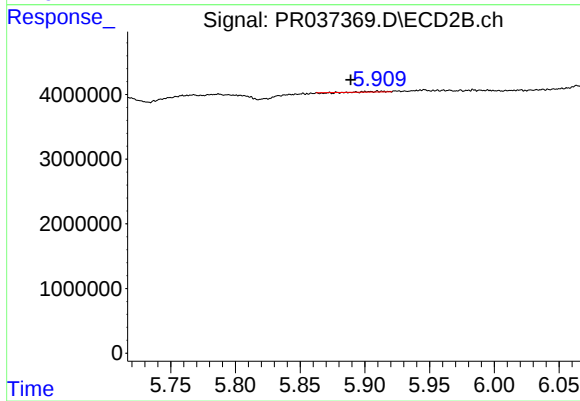

#31 AR-1260-1


R.T.: 5.913 min
Delta R.T.: 0.024 min
Response: 35443
Conc: 0.12 ng/ml

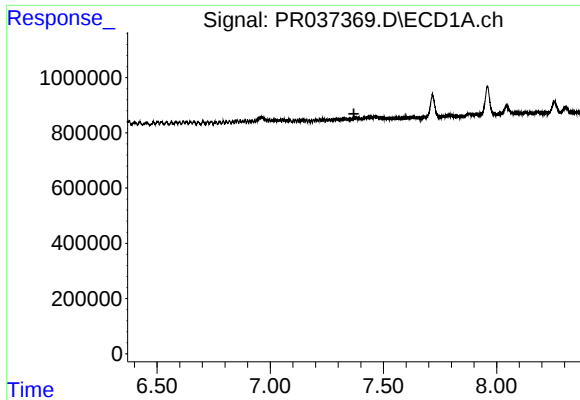

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

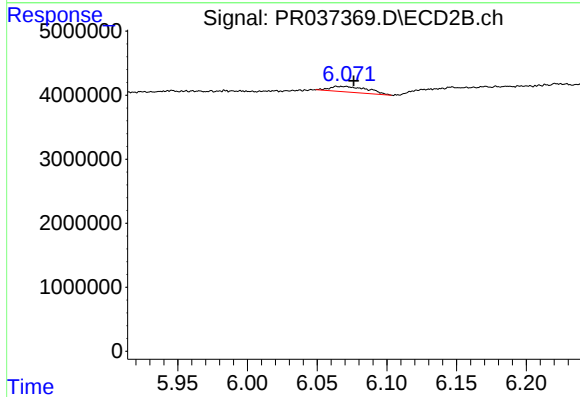


#32 AR-1260-2

R.T.: 6.065 min
Delta R.T.: -0.012 min
Response: 1607347
Conc: 3.49 ng/ml

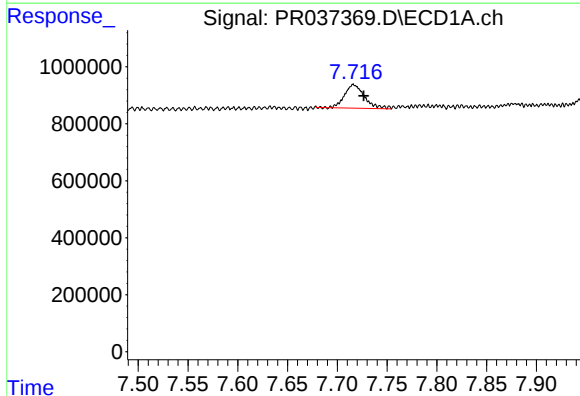


#33 AR-1260-3

R.T.: 7.716 min
Delta R.T.: -0.010 min
Response: 1155694
Conc: 18.47 ng/ml

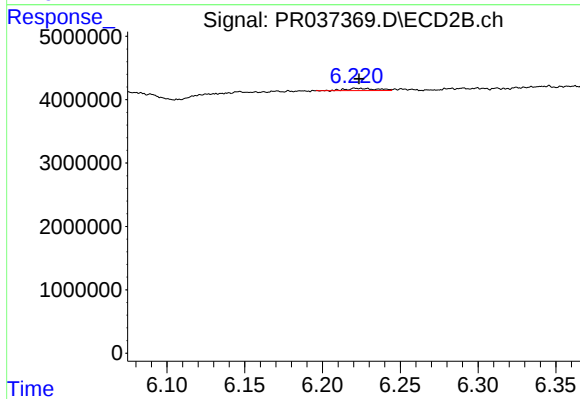

#33 AR-1260-3


R.T.: 6.221 min
Delta R.T.: -0.002 min
Response: 503067
Conc: 1.41 ng/ml

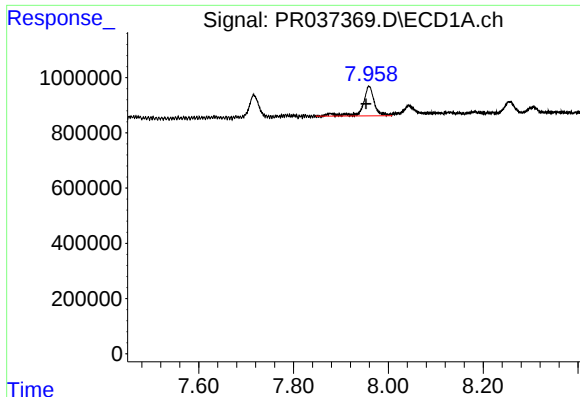

#34 AR-1260-4


R.T.: 7.959 min
Delta R.T.: 0.006 min
Response: 1807210
Conc: 24.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

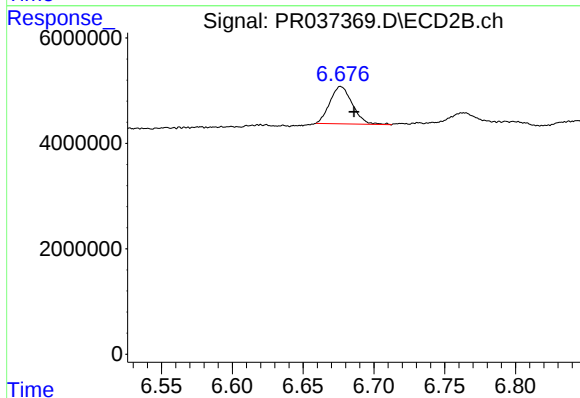


#34 AR-1260-4

R.T.: 6.677 min
Delta R.T.: -0.009 min
Response: 7810682
Conc: 25.63 ng/ml

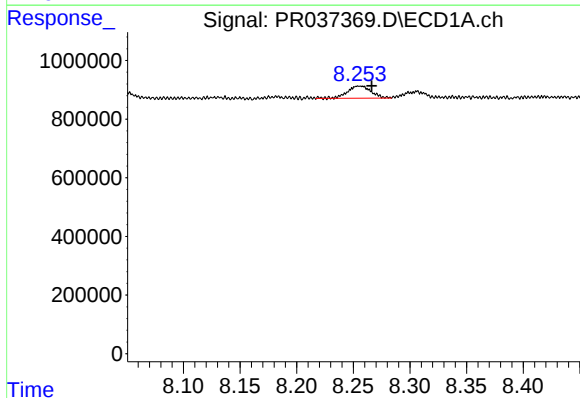


#35 AR-1260-5

R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 600457
Conc: 4.15 ng/ml

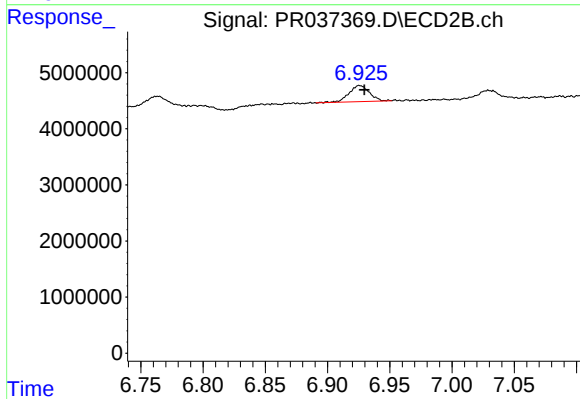

#35 AR-1260-5


R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 3240953
Conc: 3.74 ng/ml

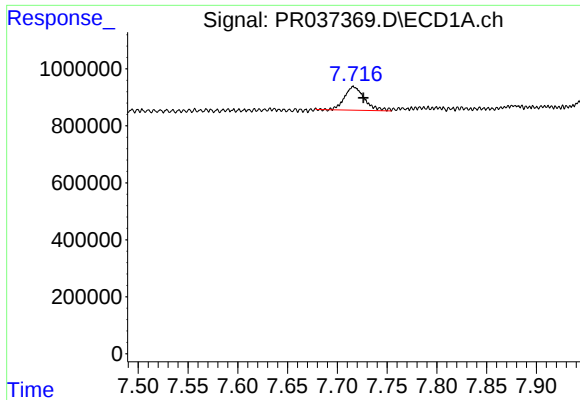

#36 AR-1262-1


R.T.: 7.716 min
Delta R.T.: -0.010 min
Response: 1155694
Conc: 11.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

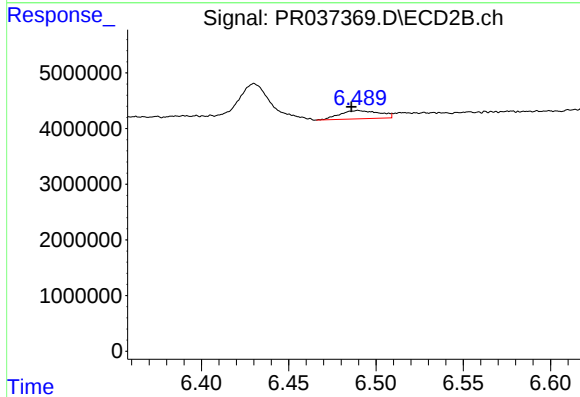


#36 AR-1262-1

R.T.: 6.490 min
Delta R.T.: 0.004 min
Response: 2322284
Conc: 9.27 ng/ml

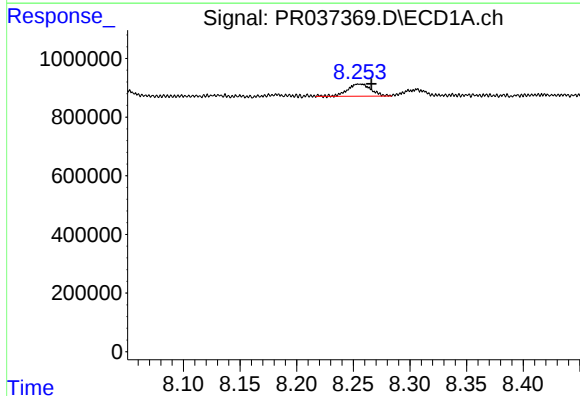


#37 AR-1262-2

R.T.: 8.255 min
Delta R.T.: -0.011 min
Response: 600457
Conc: 3.09 ng/ml

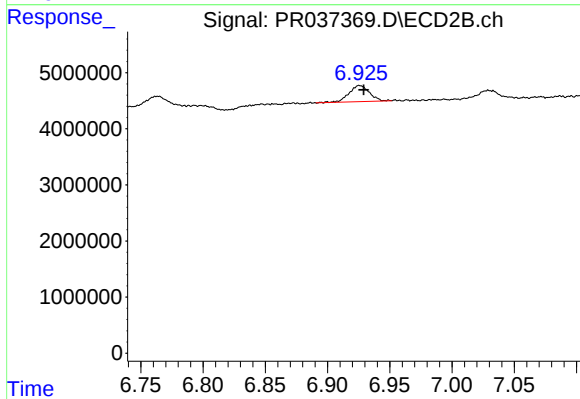

#37 AR-1262-2


R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 3240953
Conc: 2.58 ng/ml

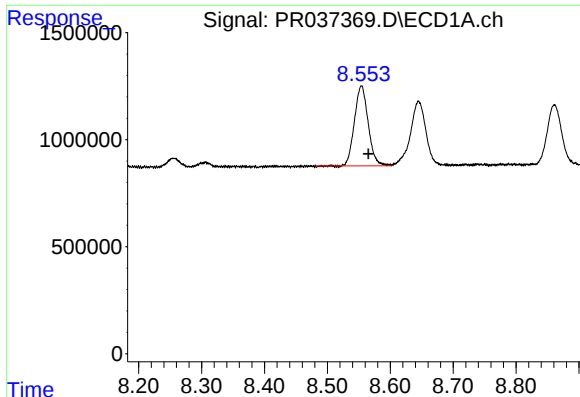

#38 AR-1262-3


R.T.: 8.554 min
Delta R.T.: -0.011 min
Response: 5686418
Conc: 43.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

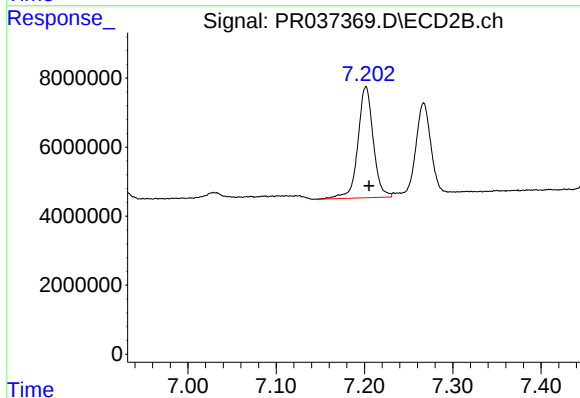


#38 AR-1262-3

R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 38871765
Conc: 70.90 ng/ml

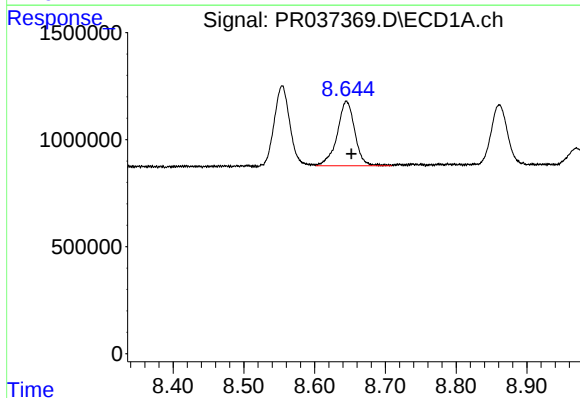


#39 AR-1262-4

R.T.: 8.645 min
Delta R.T.: -0.007 min
Response: 5209074
Conc: 53.03 ng/ml

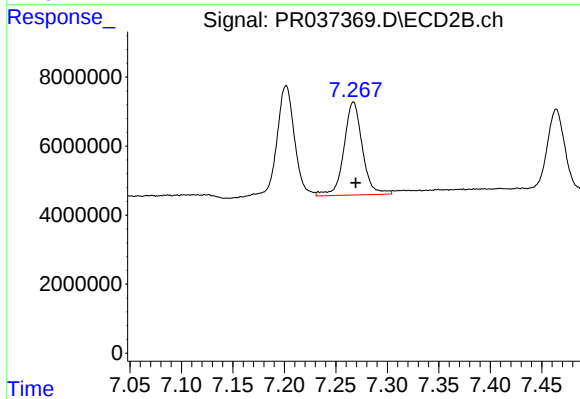

#39 AR-1262-4


R.T.: 7.267 min
Delta R.T.: -0.002 min
Response: 33705283
Conc: 37.55 ng/ml

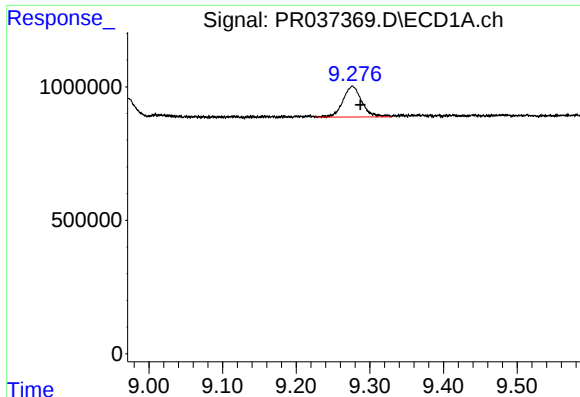

#40 AR-1262-5


R.T.: 9.276 min
Delta R.T.: -0.011 min
Response: 2047772
Conc: 29.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

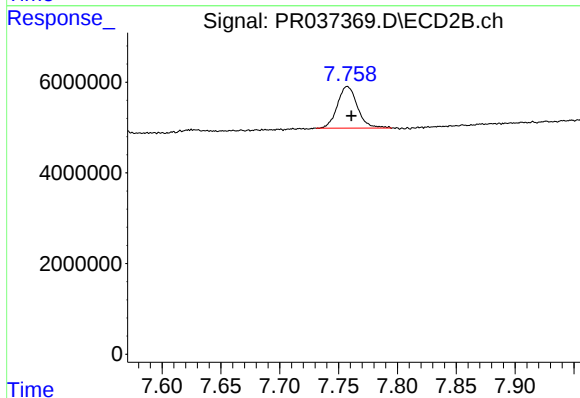


#40 AR-1262-5

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 10921696
Conc: 28.54 ng/ml

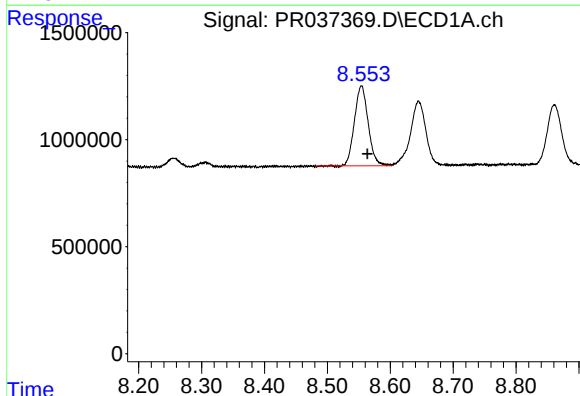


#41 AR-1268-1

R.T.: 8.554 min
Delta R.T.: -0.009 min
Response: 5686418
Conc: 31.75 ng/ml

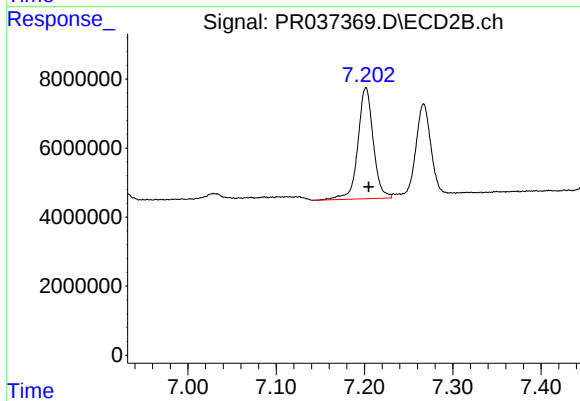

#41 AR-1268-1


R.T.: 7.202 min
Delta R.T.: -0.003 min
Response: 38871765
Conc: 31.58 ng/ml

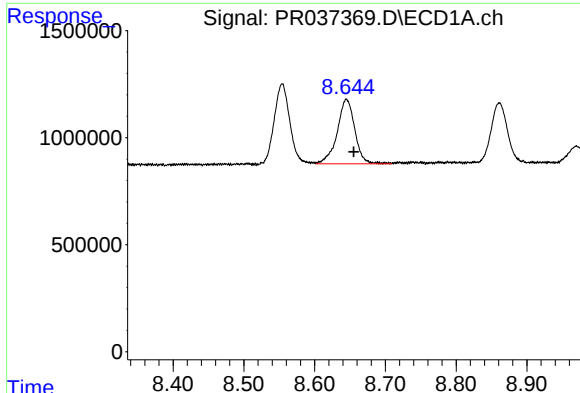

#42 AR-1268-2


R.T.: 8.645 min
Delta R.T.: -0.010 min
Response: 5209074
Conc: 31.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

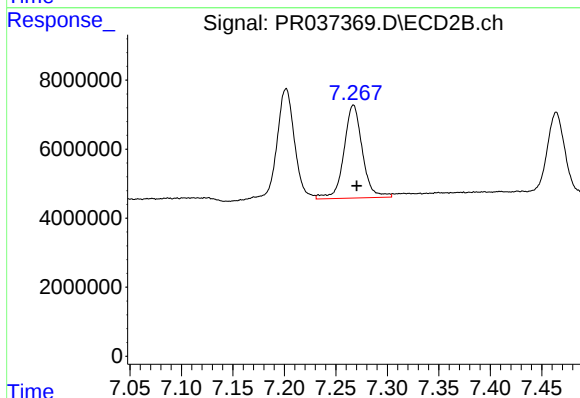


#42 AR-1268-2

R.T.: 7.267 min
Delta R.T.: -0.003 min
Response: 33705283
Conc: 31.83 ng/ml

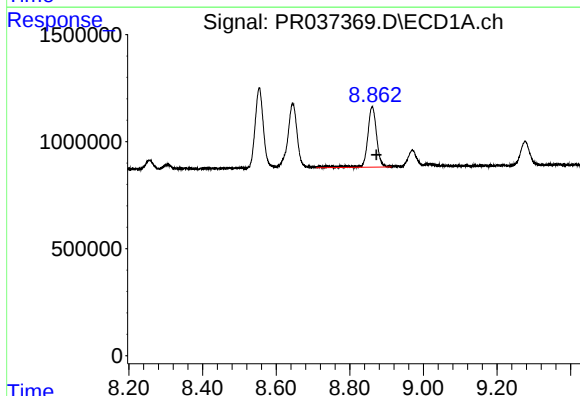


#43 AR-1268-3

R.T.: 8.861 min
Delta R.T.: -0.011 min
Response: 4857251
Conc: 35.09 ng/ml

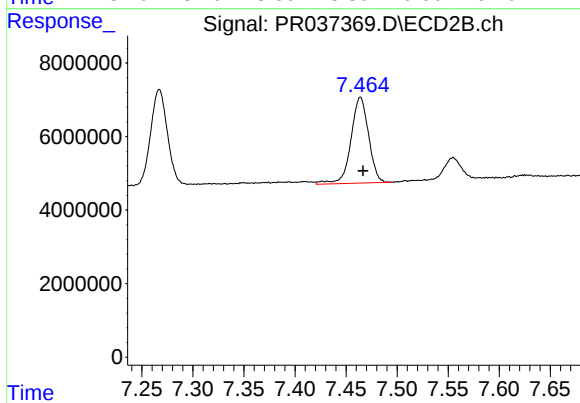

#43 AR-1268-3


R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 28080809
Conc: 31.69 ng/ml

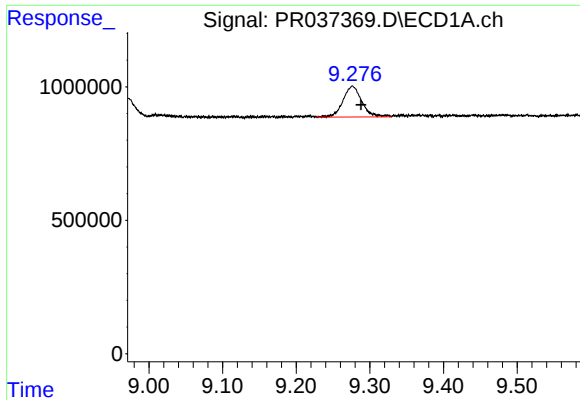

#44 AR-1268-4


R.T.: 9.276 min
Delta R.T.: -0.011 min
Response: 2047772
Conc: 32.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

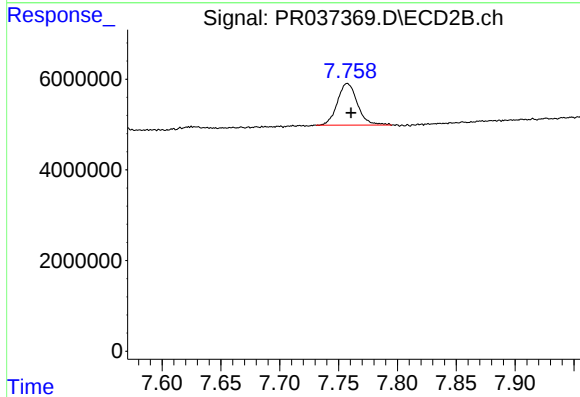


#44 AR-1268-4

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 10921696
Conc: 30.11 ng/ml

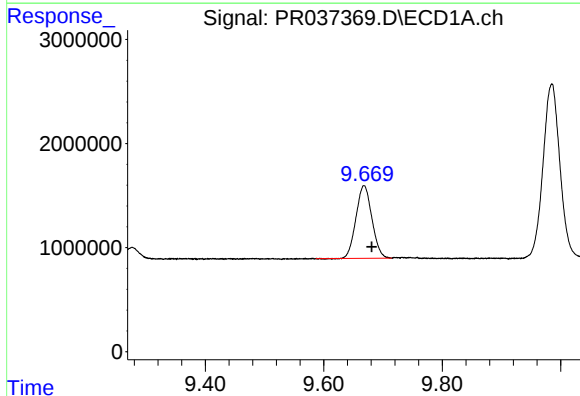

#45 AR-1268-5

R.T.: 9.668 min
Delta R.T.: -0.013 min
Response: 13055700
Conc: 28.64 ng/ml

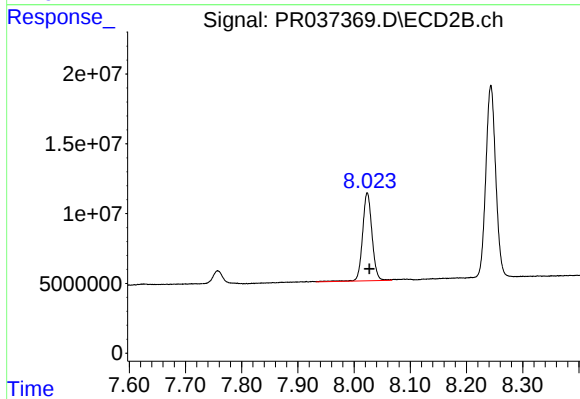

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.004 min
Response: 74071281
Conc: 29.11 ng/ml