

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:45
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1268 LOD 40PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:10:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.409	28272701	115.8E6	22.600	24.140
2)	SA Decachlor...	9.985	8.244	32805287	171.1E6	24.804	29.385
Target Compounds							
3)	L1 AR-1016-1	0.000	4.461	0	93521	N.D.	0.514 #
4)	L1 AR-1016-2	0.000	4.461	0	93521	N.D.	0.331 #
5)	L1 AR-1016-3	0.000	4.686	0	417081	N.D.	2.901 #
6)	L1 AR-1016-4	0.000	4.686	0	417081	N.D.	3.770 #
7)	L1 AR-1016-5	0.000	4.924	0	2049861	N.D.	13.485 #
8)	L2 AR-1221-1	0.000	3.593	0	640133	N.D.	12.572 #
9)	L2 AR-1221-2	0.000	3.698	0	1907445	N.D.	51.364 #
10)	L2 AR-1221-3	0.000	3.741	0	220158	N.D.	1.798 #
11)	L3 AR-1232-1	0.000	3.741	0	220158	N.D.	1.882 #
12)	L3 AR-1232-2	0.000	4.461	0	93521	N.D.	0.677 #
13)	L3 AR-1232-3	0.000	4.686	0	417081	N.D.	5.941 #
14)	L3 AR-1232-4	0.000	4.718	0	203968	N.D.	3.418 #
15)	L3 AR-1232-5	0.000	4.924	0	2049861	N.D.	30.037 #
16)	L4 AR-1242-1	0.000	4.461	0	93521	N.D.	0.638 #
17)	L4 AR-1242-2	0.000	4.461	0	93521	N.D.	0.410 #
18)	L4 AR-1242-3	0.000	4.686	0	417081	N.D.	3.607 #
19)	L4 AR-1242-4	0.000	4.718	0	203968	N.D.	1.856 #
20)	L4 AR-1242-5	0.000	5.253	0	2811746	N.D.	16.969 #
21)	L5 AR-1248-1	0.000	4.461	0	93521	N.D.	0.929 #
22)	L5 AR-1248-2	0.000	4.686	0	417081	N.D.	3.056 #
23)	L5 AR-1248-3	0.000	4.718	0	203968	N.D.	1.457 #
24)	L5 AR-1248-4	0.000	4.924	0	2049861	N.D.	11.518 #
25)	L5 AR-1248-5	0.000	5.273	0	812634	N.D.	4.154 #
26)	L6 AR-1254-1	0.000	5.253	0	2811746	N.D.	8.162 #
27)	L6 AR-1254-2	0.000	5.318	0	2589248	N.D.	8.645 #
28)	L6 AR-1254-3	0.000	5.768	0	3451968	N.D.	7.288 #
30)	L6 AR-1254-5	7.717	6.430	2527654	15757273	35.164	35.584
32)	L7 AR-1260-2	0.000	6.069	0	1326105	N.D.	2.879 #
33)	L7 AR-1260-3	7.717	6.224	2527654	1880417	40.394	5.275 #
34)	L7 AR-1260-4	7.959	6.677	3583016	14135367	48.156	46.381
35)	L7 AR-1260-5	8.256	6.926	1338014	5756473	9.252	6.638 #
36)	L8 AR-1262-1	7.717	6.486	2527654	2668594	24.199	10.648 #
37)	L8 AR-1262-2	8.256	6.926	1338014	5756473	6.883	4.583 #
38)	L8 AR-1262-3	8.553	7.201	10167424	69858715	77.313	127.418 #
39)	L8 AR-1262-4	8.645	7.267	9358838	58189761	95.276	64.825 #
40)	L8 AR-1262-5	9.277	7.757	3533129	19287585	51.175	50.409
41)	L9 AR-1268-1	8.553	7.201	10167424	69858715	56.772	56.748
42)	L9 AR-1268-2	8.645	7.267	9358838	58189761	56.894	54.952
43)	L9 AR-1268-3	8.861	7.464	8050392	55065164	58.152	62.133

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
 Data File : PR037370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:45
 Operator : SM\SJ
 Sample : K2241-07
 Misc : AR1268 LOD 40PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:10:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.277	7.757	3533129	19287585	56.634	53.166
45) L9	AR-1268-5	9.668	8.024	23672057	132.4E6	51.927	52.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042419\
Data File : PR037370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 19:45
Operator : SM\SJ
Sample : K2241-07
Misc : AR1268 LOD 40PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:10:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

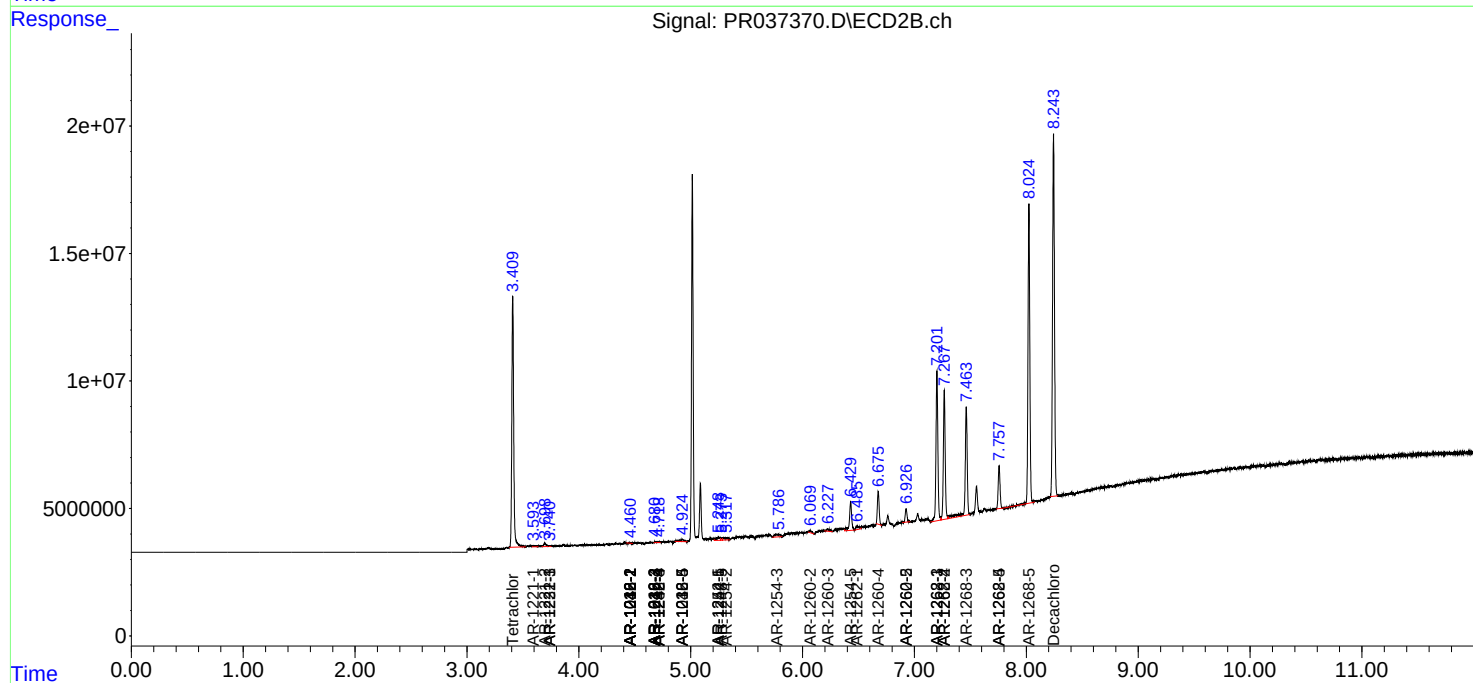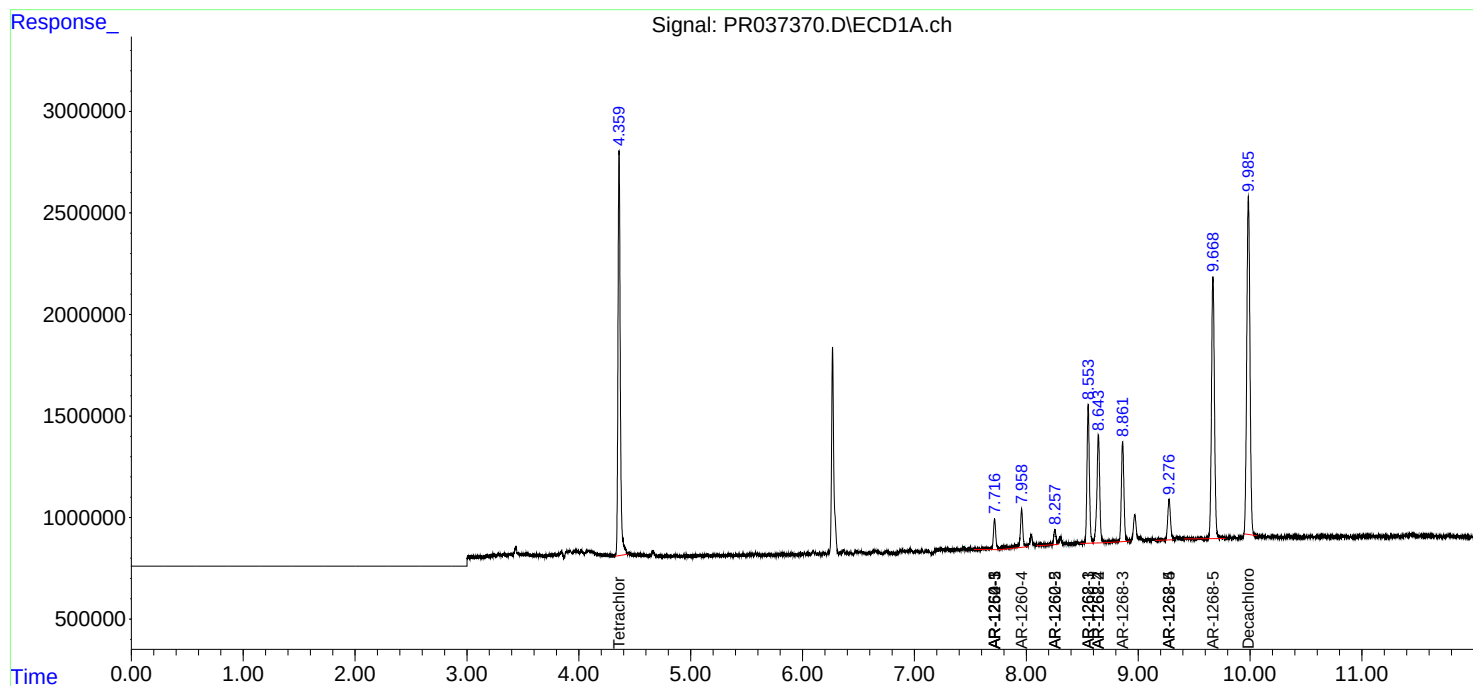


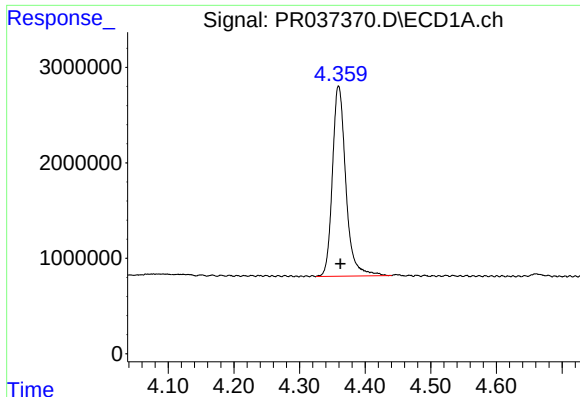

#1 Tetrachloro-m-xylene


R.T.: 4.360 min
Delta R.T.: -0.002 min
Response: 28272701
Conc: 22.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

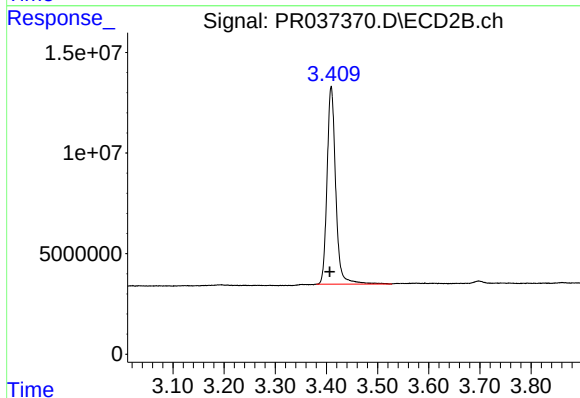


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.003 min
Response: 115762020
Conc: 24.14 ng/ml

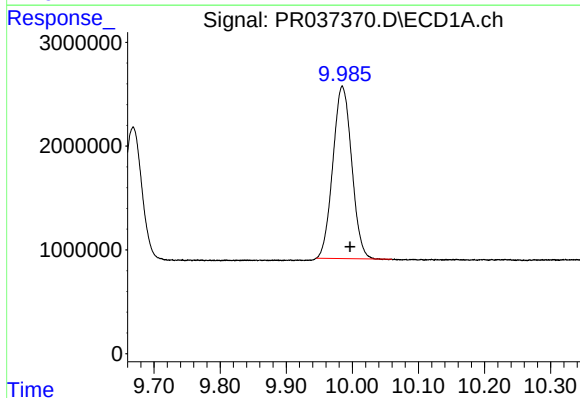


#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.012 min
Response: 32805287
Conc: 24.80 ng/ml

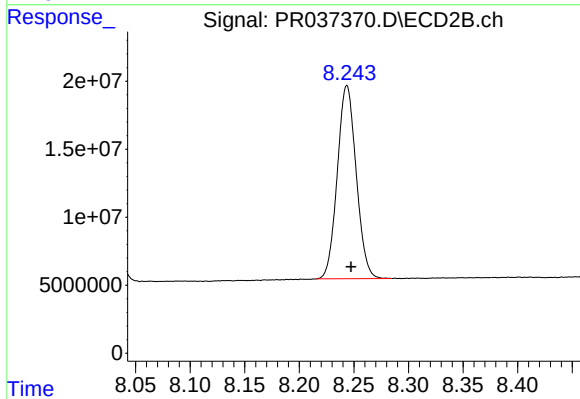

#2 Decachlorobiphenyl


R.T.: 8.244 min
Delta R.T.: -0.004 min
Response: 171145837
Conc: 29.39 ng/ml

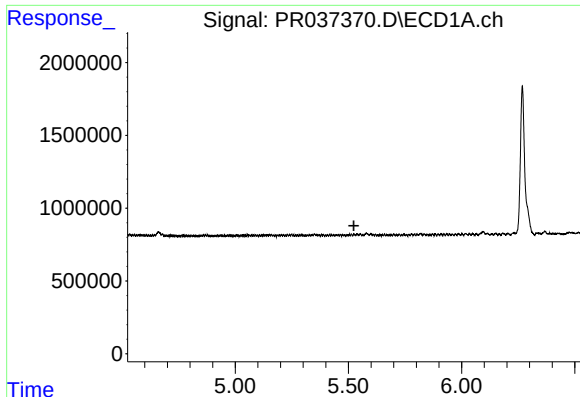

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

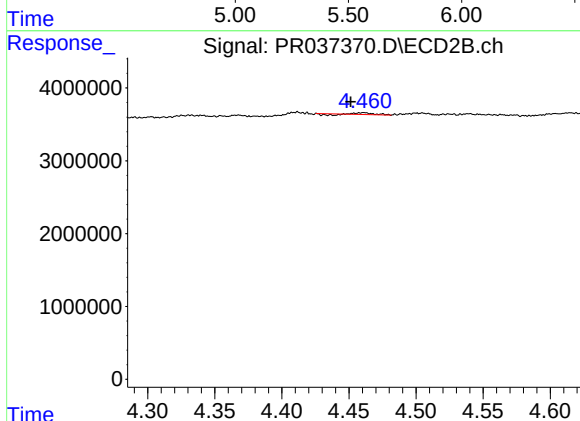


#3 AR-1016-1

R.T.: 4.461 min
Delta R.T.: 0.010 min
Response: 93521
Conc: 0.51 ng/ml

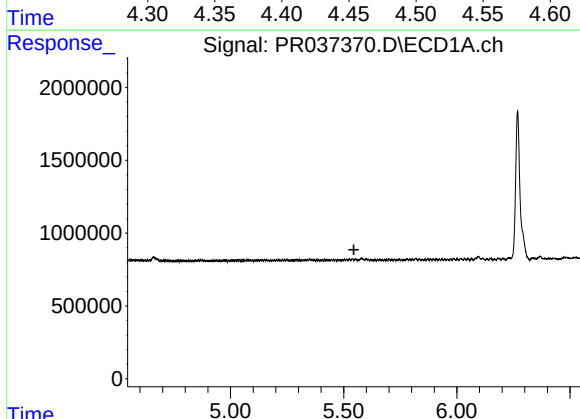


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

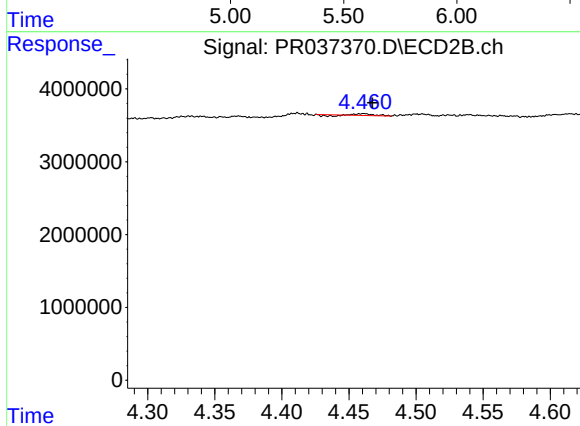

#4 AR-1016-2


R.T.: 4.461 min
Delta R.T.: -0.006 min
Response: 93521
Conc: 0.33 ng/ml

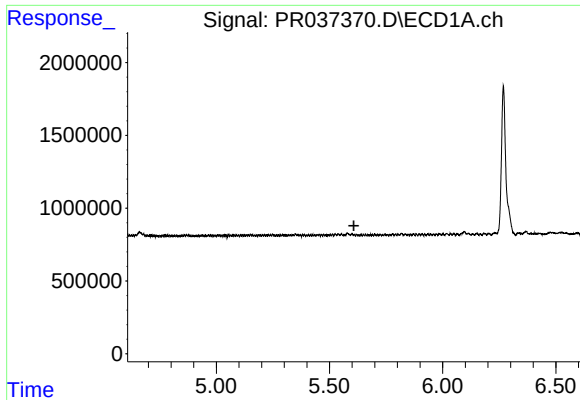

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

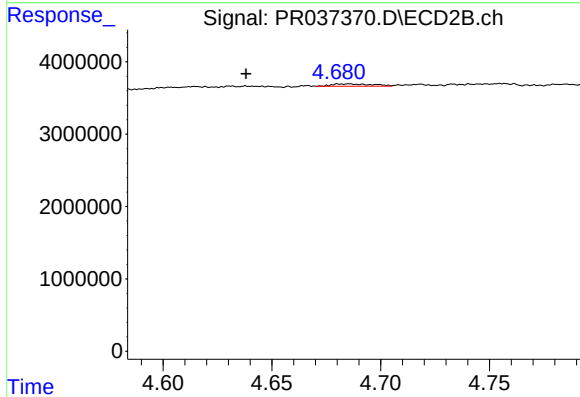


#5 AR-1016-3

R.T.: 4.686 min
Delta R.T.: 0.047 min
Response: 417081
Conc: 2.90 ng/ml

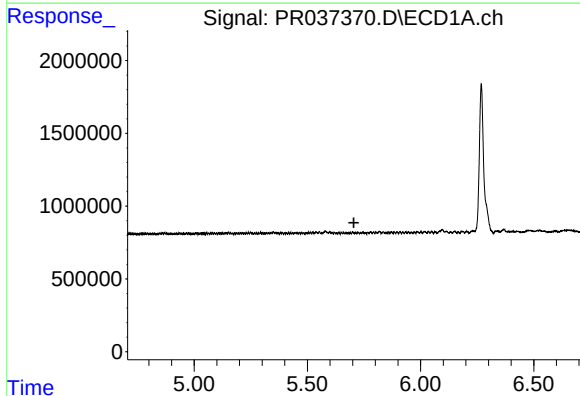


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

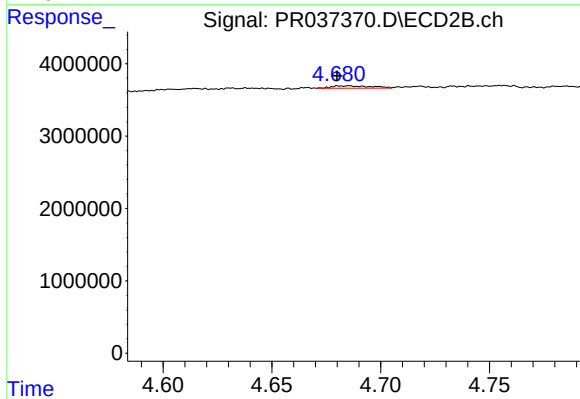

#6 AR-1016-4


R.T.: 4.686 min
Delta R.T.: 0.006 min
Response: 417081
Conc: 3.77 ng/ml

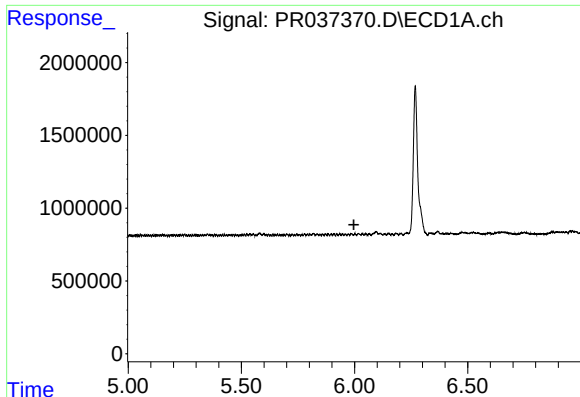

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

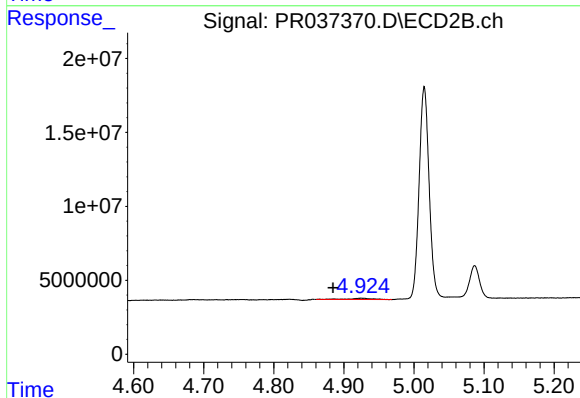


#7 AR-1016-5

R.T.: 4.924 min
Delta R.T.: 0.039 min
Response: 2049861
Conc: 13.49 ng/ml

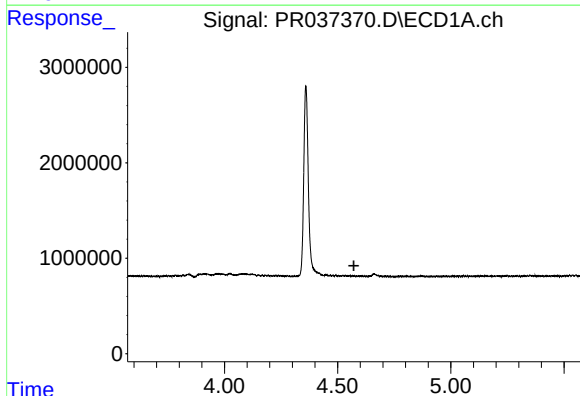


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

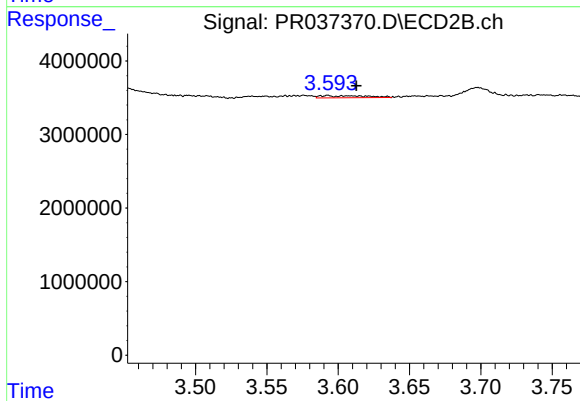

#8 AR-1221-1


R.T.: 3.593 min
Delta R.T.: -0.020 min
Response: 640133
Conc: 12.57 ng/ml

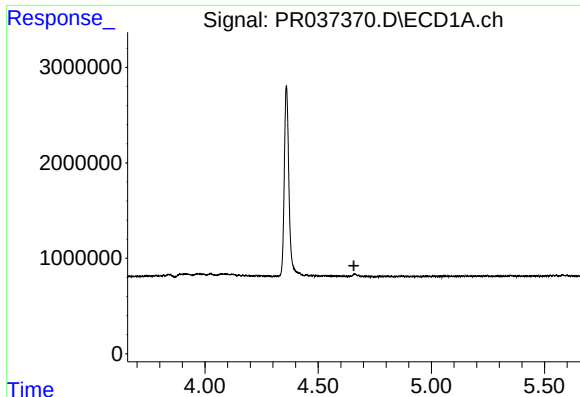

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

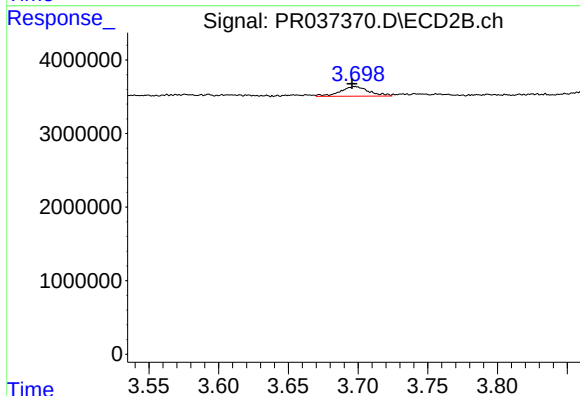


#9 AR-1221-2

R.T.: 3.698 min
Delta R.T.: 0.002 min
Response: 1907445
Conc: 51.36 ng/ml

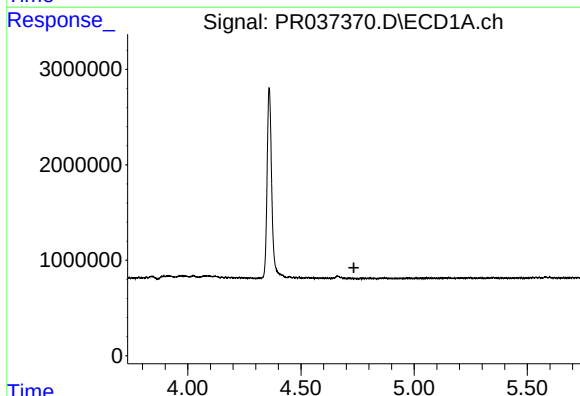


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

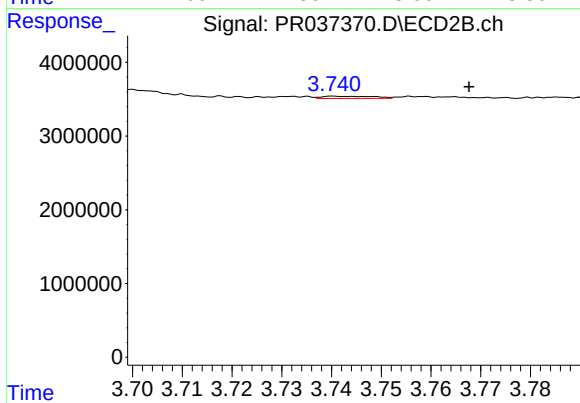

#10 AR-1221-3


R.T.: 3.741 min
Delta R.T.: -0.026 min
Response: 220158
Conc: 1.80 ng/ml

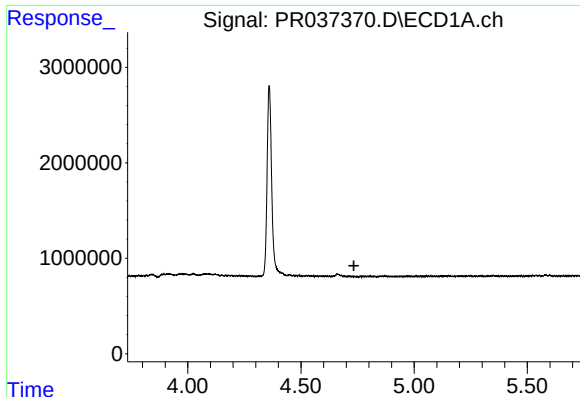

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

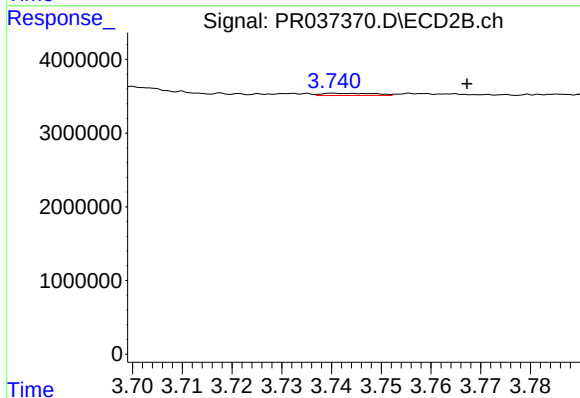


#11 AR-1232-1

R.T.: 3.741 min
Delta R.T.: -0.026 min
Response: 220158
Conc: 1.88 ng/ml

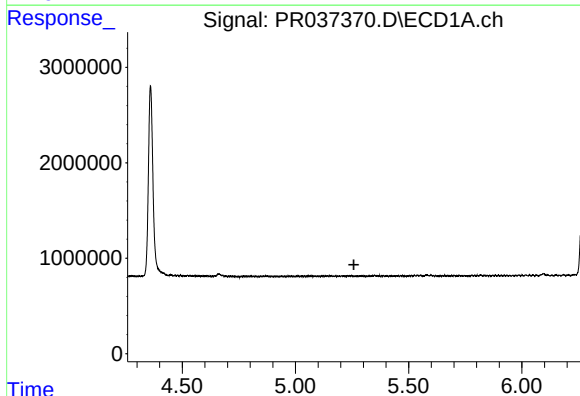


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

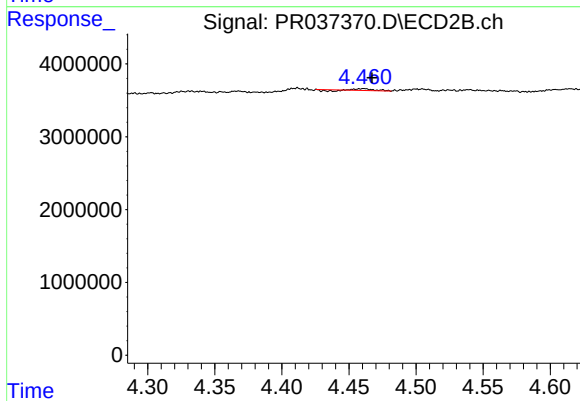

#12 AR-1232-2


R.T.: 4.461 min
Delta R.T.: -0.006 min
Response: 93521
Conc: 0.68 ng/ml

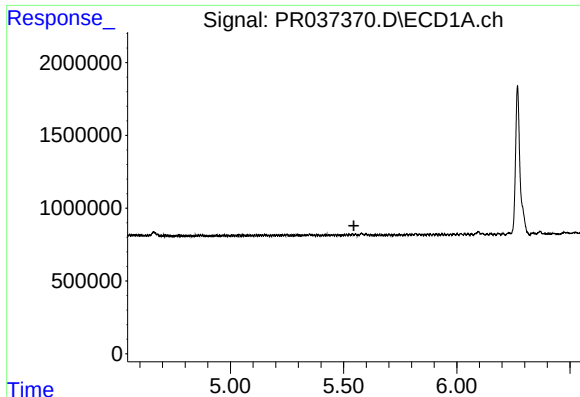

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

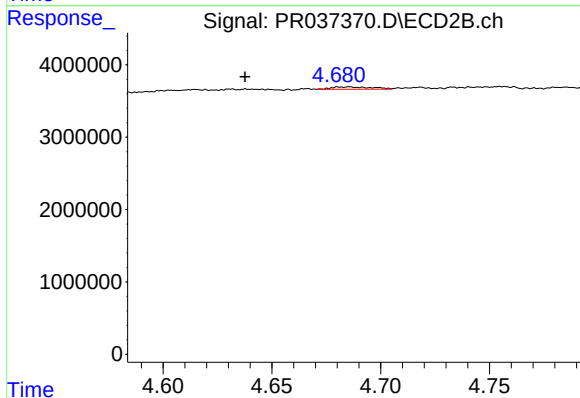


#13 AR-1232-3

R.T.: 4.686 min
Delta R.T.: 0.048 min
Response: 417081
Conc: 5.94 ng/ml

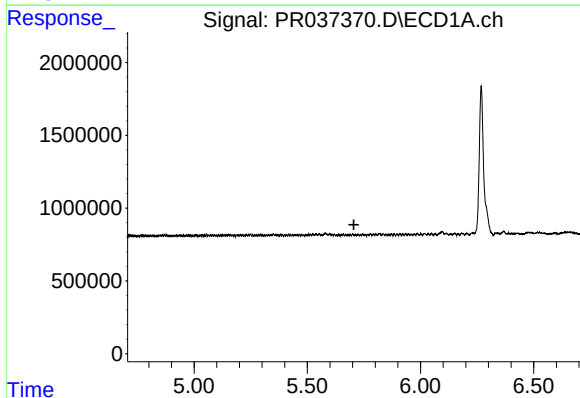


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

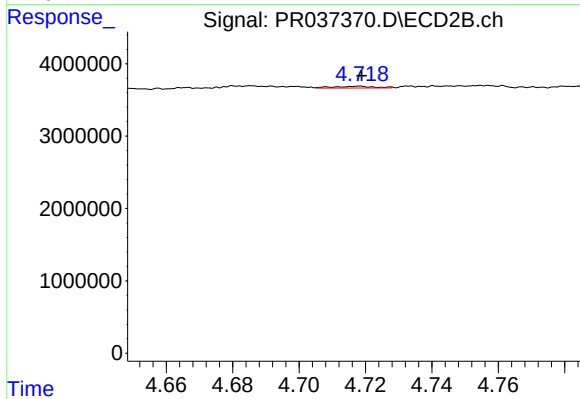

#14 AR-1232-4


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 203968
Conc: 3.42 ng/ml

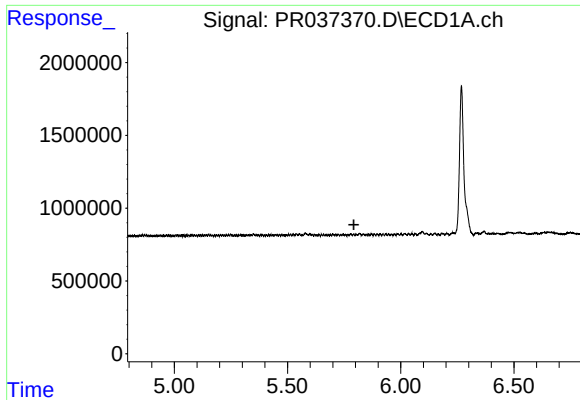

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

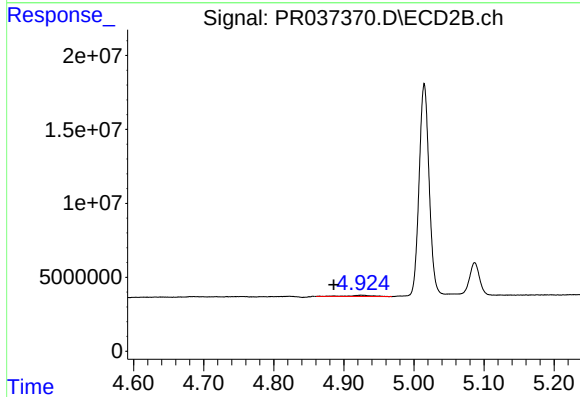


#15 AR-1232-5

R.T.: 4.924 min
Delta R.T.: 0.039 min
Response: 2049861
Conc: 30.04 ng/ml

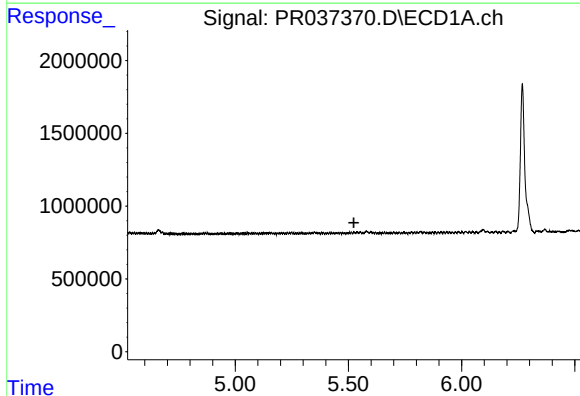


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

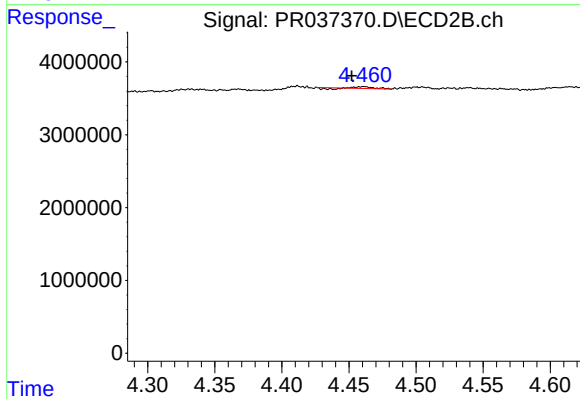

#16 AR-1242-1


R.T.: 4.461 min
Delta R.T.: 0.009 min
Response: 93521
Conc: 0.64 ng/ml

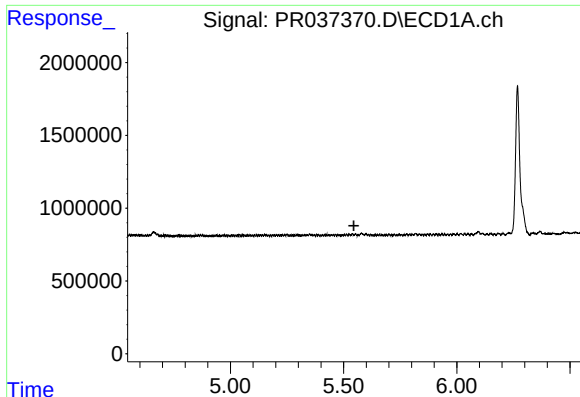

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

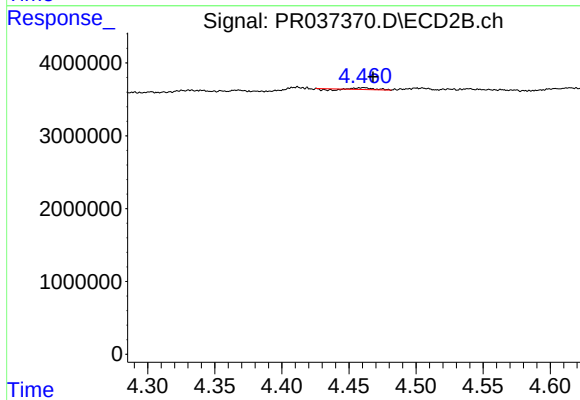


#17 AR-1242-2

R.T.: 4.461 min
Delta R.T.: -0.007 min
Response: 93521
Conc: 0.41 ng/ml

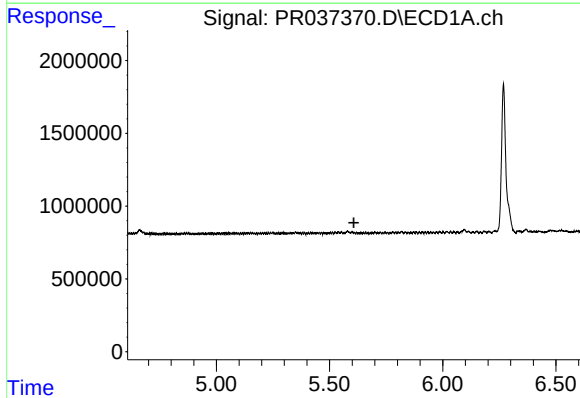


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

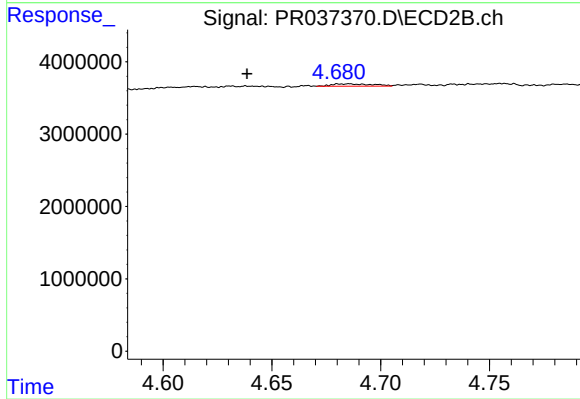

#18 AR-1242-3


R.T.: 4.686 min
Delta R.T.: 0.047 min
Response: 417081
Conc: 3.61 ng/ml

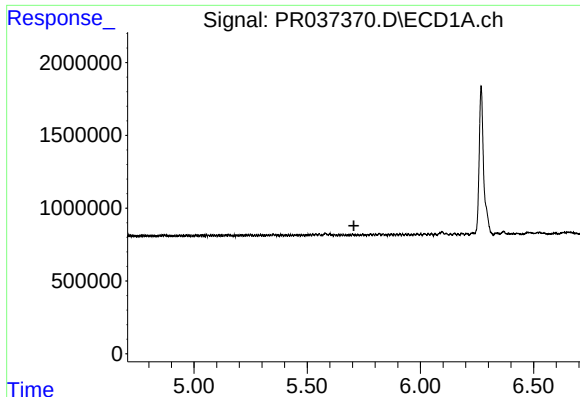

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

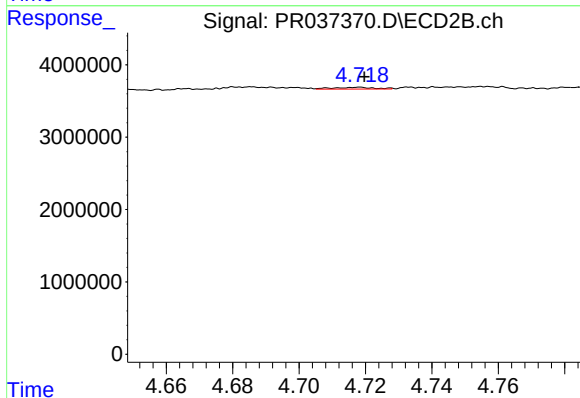


#19 AR-1242-4

R.T.: 4.718 min
Delta R.T.: -0.002 min
Response: 203968
Conc: 1.86 ng/ml

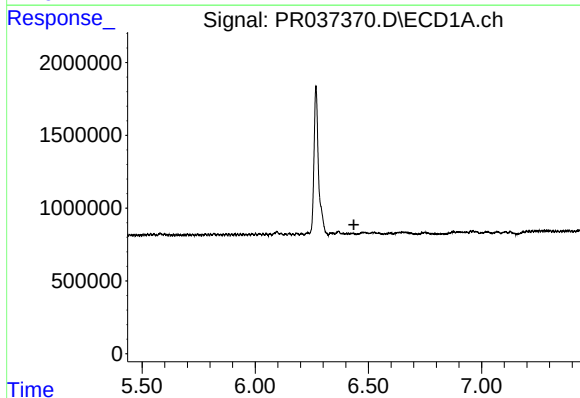


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

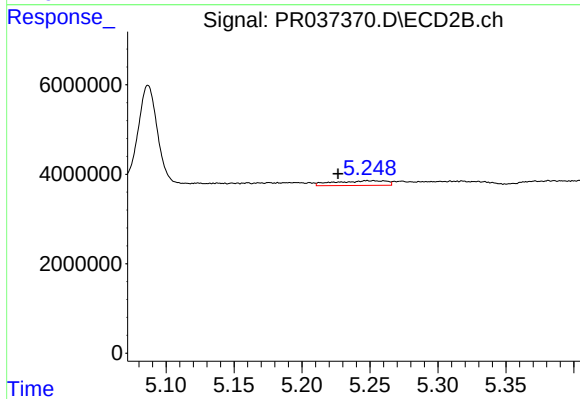

#20 AR-1242-5


R.T.: 5.253 min
Delta R.T.: 0.026 min
Response: 2811746
Conc: 16.97 ng/ml

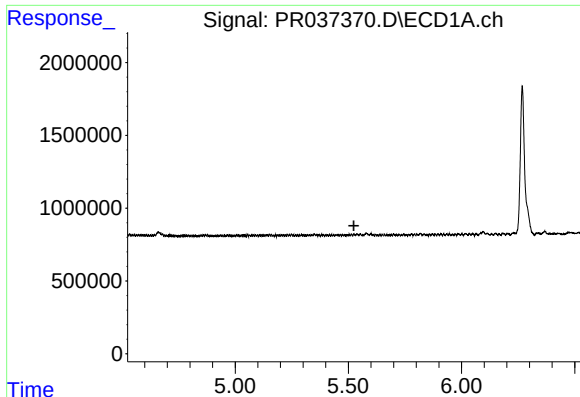

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

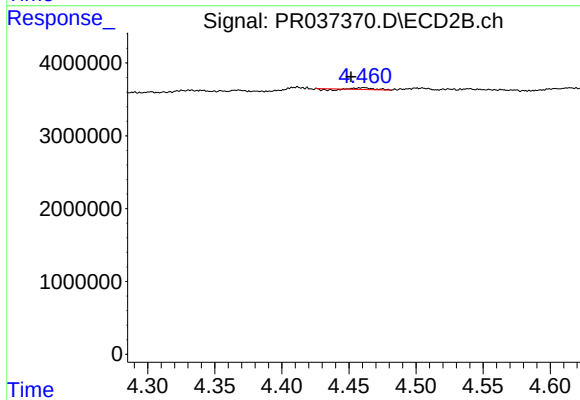


#21 AR-1248-1

R.T.: 4.461 min
Delta R.T.: 0.010 min
Response: 93521
Conc: 0.93 ng/ml

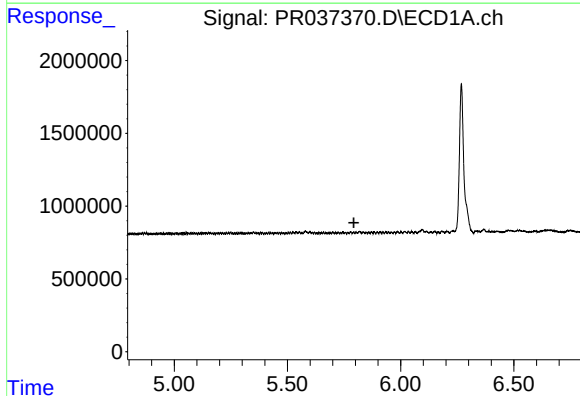


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

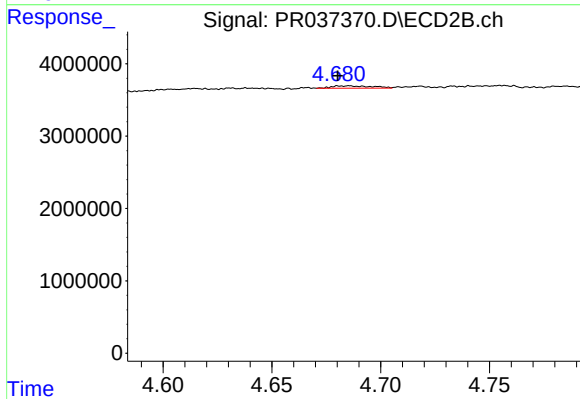

#22 AR-1248-2


R.T.: 4.686 min
Delta R.T.: 0.005 min
Response: 417081
Conc: 3.06 ng/ml

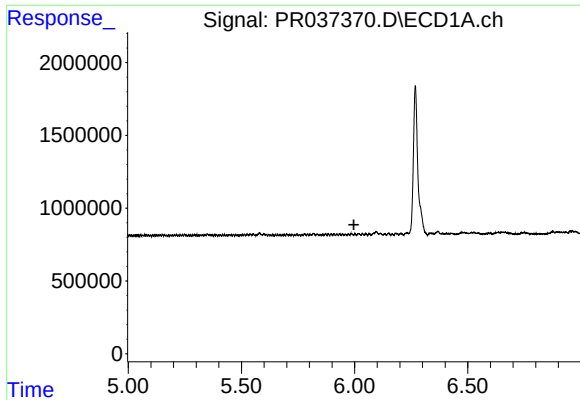

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

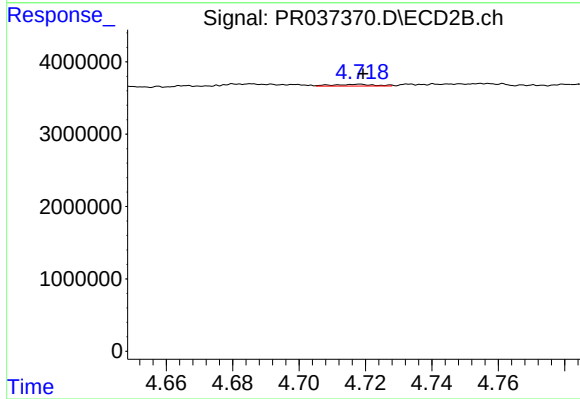


#23 AR-1248-3

R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 203968
Conc: 1.46 ng/ml

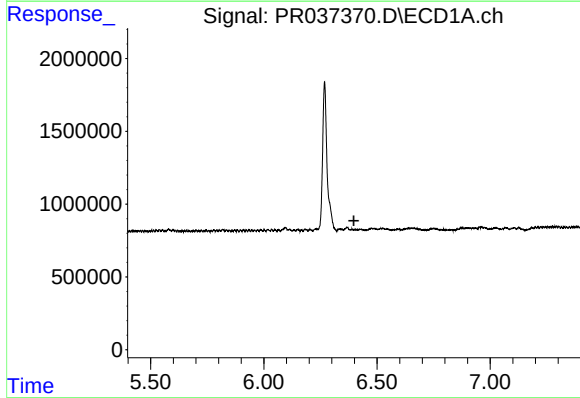


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

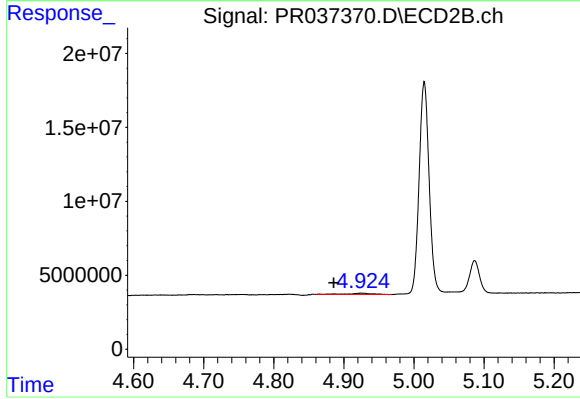

#24 AR-1248-4


R.T.: 4.924 min
Delta R.T.: 0.039 min
Response: 2049861
Conc: 11.52 ng/ml

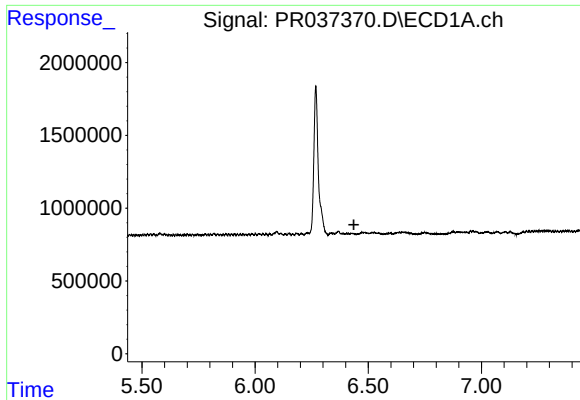

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

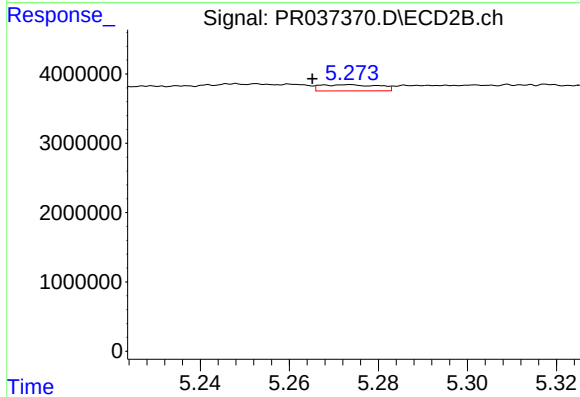


#25 AR-1248-5

R.T.: 5.273 min
Delta R.T.: 0.008 min
Response: 812634
Conc: 4.15 ng/ml

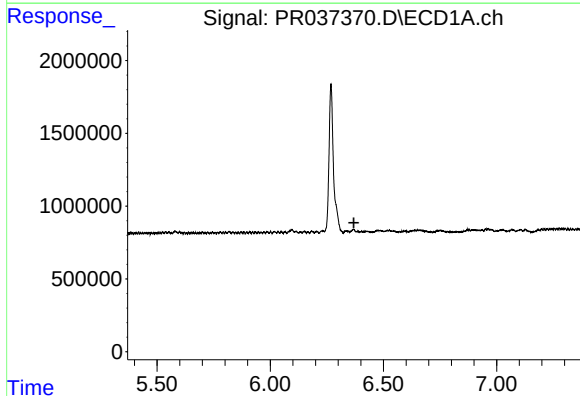


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

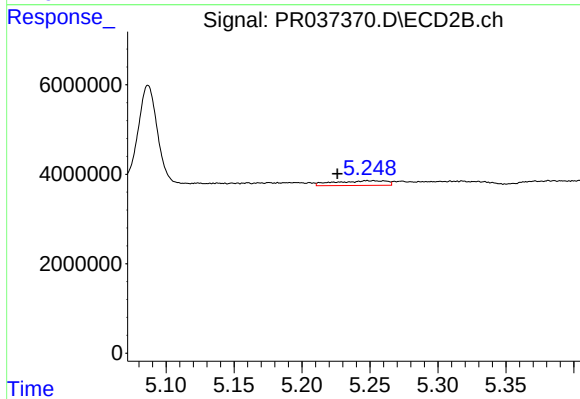

#26 AR-1254-1


R.T.: 5.253 min
Delta R.T.: 0.026 min
Response: 2811746
Conc: 8.16 ng/ml

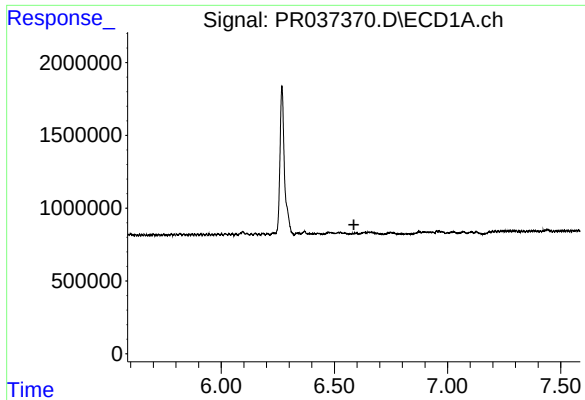

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

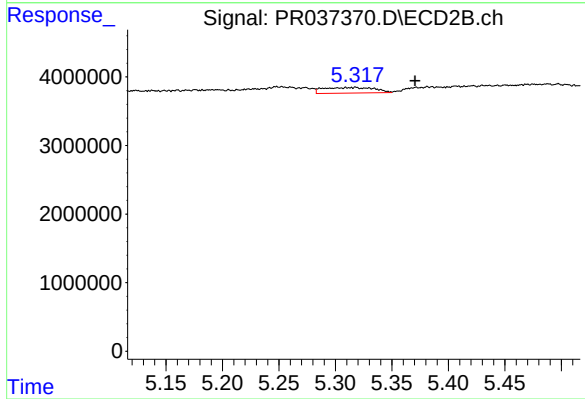


#27 AR-1254-2

R.T.: 5.318 min
Delta R.T.: -0.053 min
Response: 2589248
Conc: 8.65 ng/ml

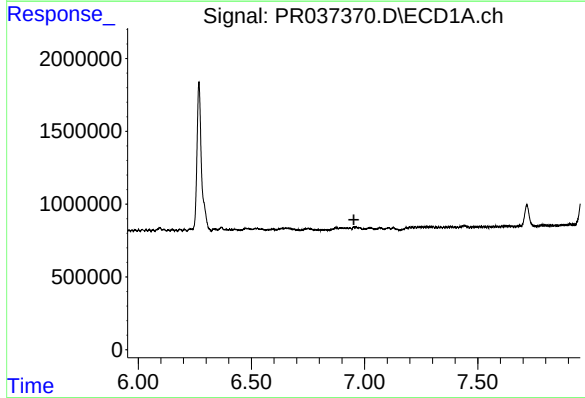


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

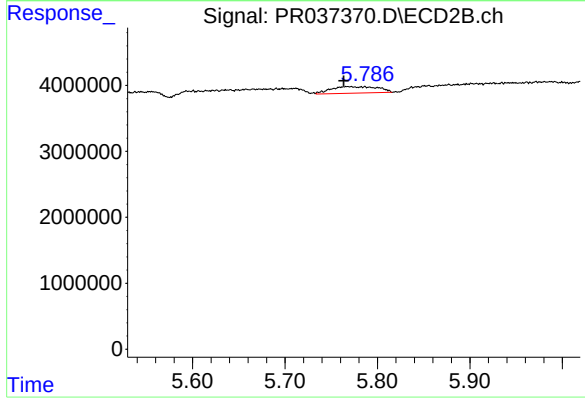

#28 AR-1254-3


R.T.: 5.768 min
Delta R.T.: 0.004 min
Response: 3451968
Conc: 7.29 ng/ml

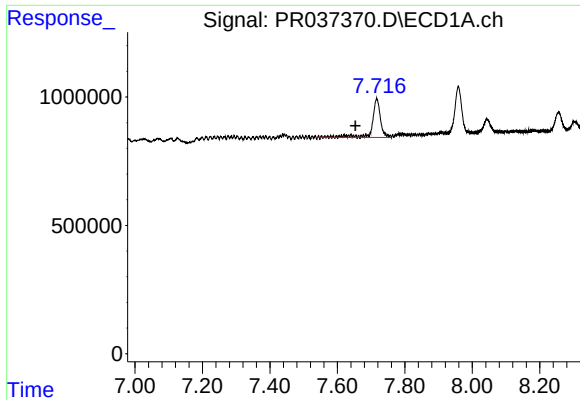

#30 AR-1254-5


R.T.: 7.717 min
Delta R.T.: 0.063 min
Response: 2527654
Conc: 35.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

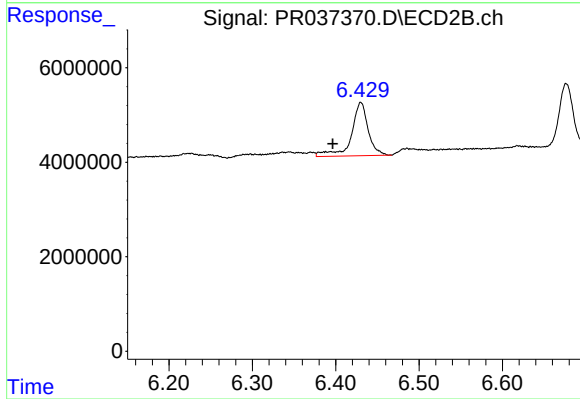


#30 AR-1254-5

R.T.: 6.430 min
Delta R.T.: 0.034 min
Response: 15757273
Conc: 35.58 ng/ml

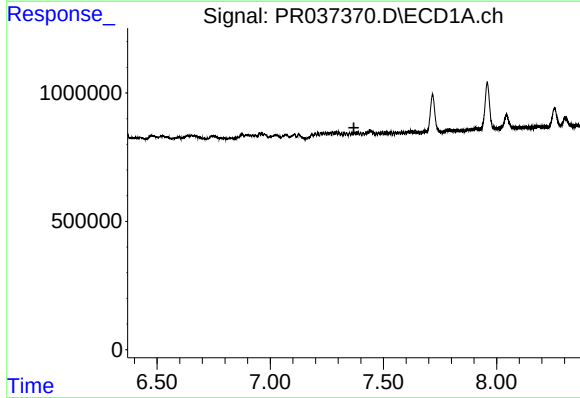


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

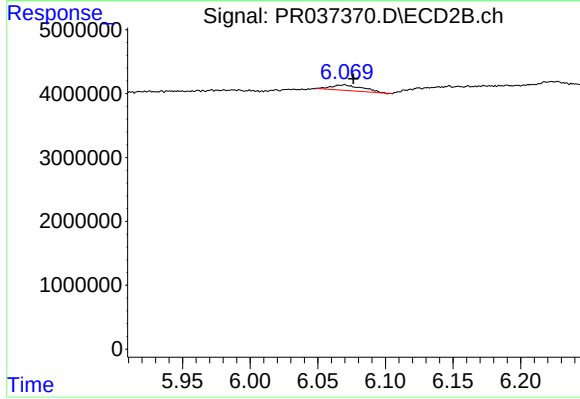

#32 AR-1260-2


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 1326105
Conc: 2.88 ng/ml

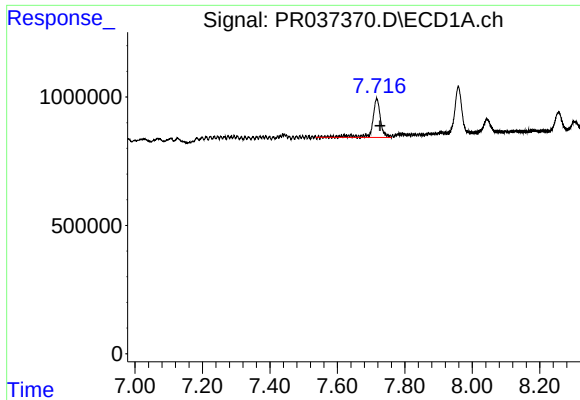

#33 AR-1260-3


R.T.: 7.717 min
Delta R.T.: -0.010 min
Response: 2527654
Conc: 40.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

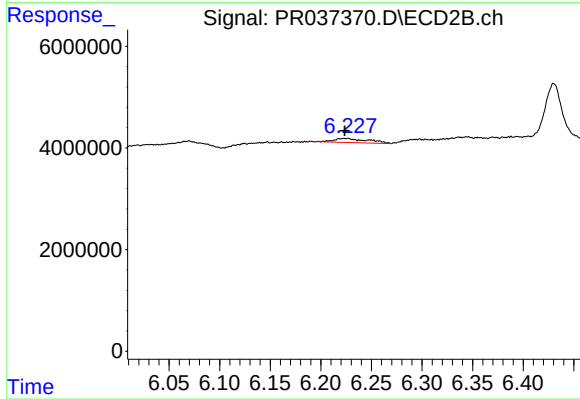


#33 AR-1260-3

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 1880417
Conc: 5.27 ng/ml

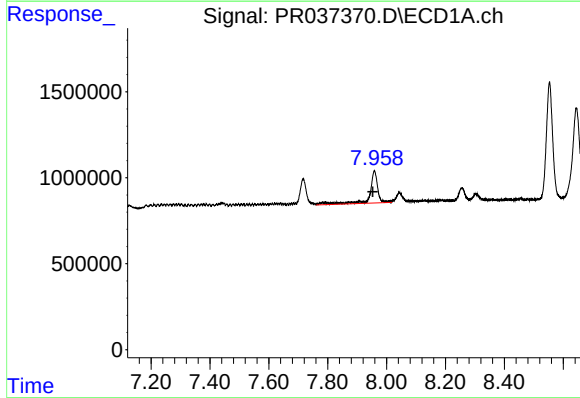


#34 AR-1260-4

R.T.: 7.959 min
Delta R.T.: 0.006 min
Response: 3583016
Conc: 48.16 ng/ml

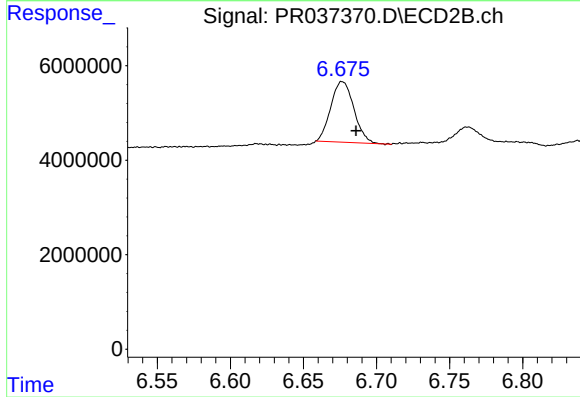

#34 AR-1260-4


R.T.: 6.677 min
Delta R.T.: -0.009 min
Response: 14135367
Conc: 46.38 ng/ml

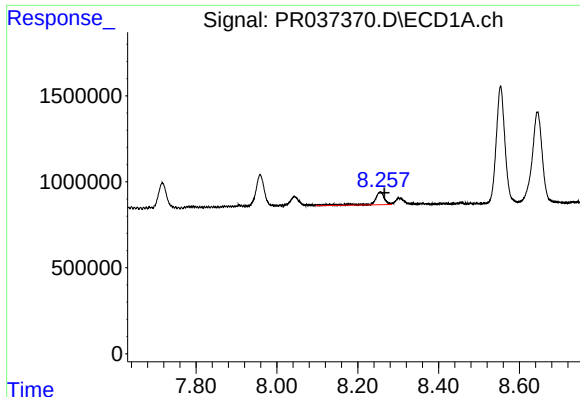

#35 AR-1260-5


R.T.: 8.256 min
Delta R.T.: -0.010 min
Response: 1338014
Conc: 9.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

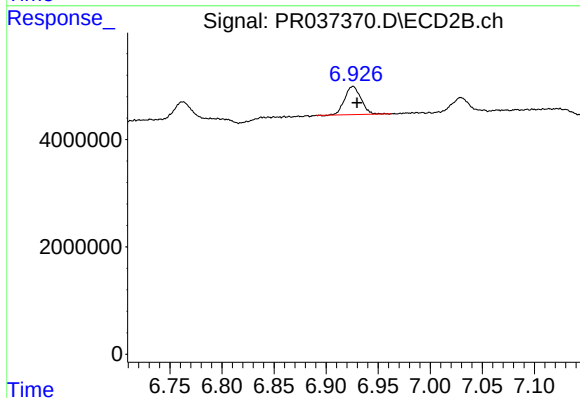


#35 AR-1260-5

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 5756473
Conc: 6.64 ng/ml

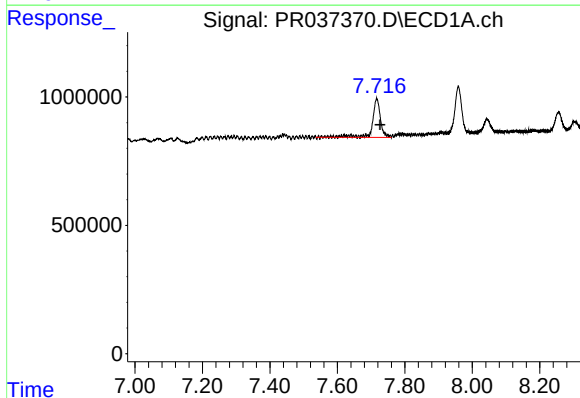


#36 AR-1262-1

R.T.: 7.717 min
Delta R.T.: -0.009 min
Response: 2527654
Conc: 24.20 ng/ml

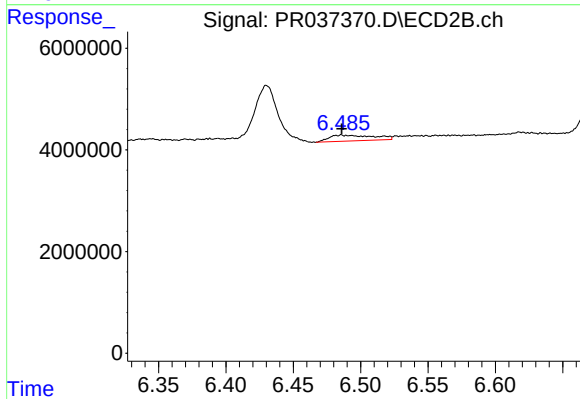

#36 AR-1262-1


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 2668594
Conc: 10.65 ng/ml

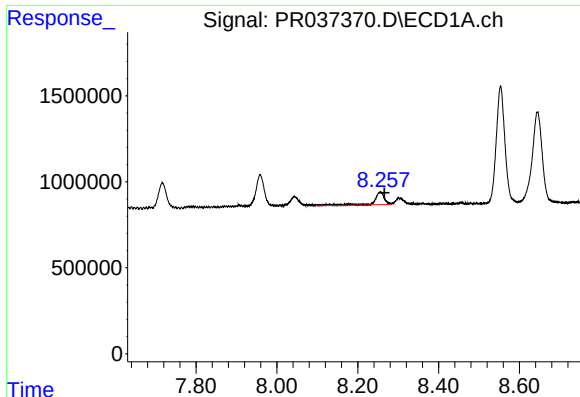

#37 AR-1262-2


R.T.: 8.256 min
Delta R.T.: -0.010 min
Response: 1338014
Conc: 6.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

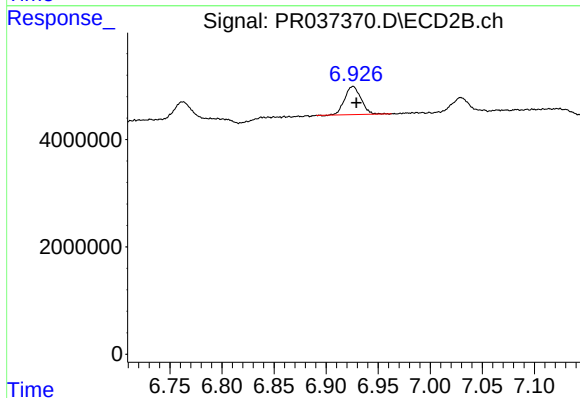


#37 AR-1262-2

R.T.: 6.926 min
Delta R.T.: -0.003 min
Response: 5756473
Conc: 4.58 ng/ml

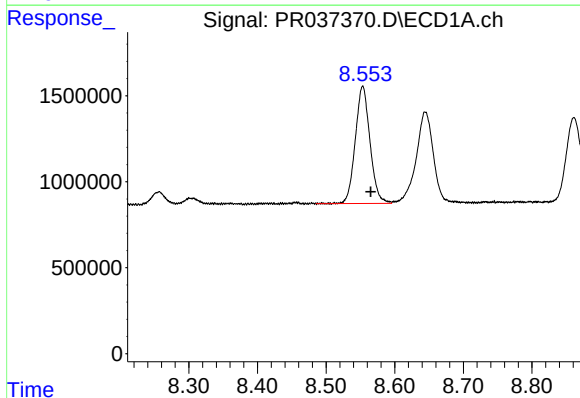


#38 AR-1262-3

R.T.: 8.553 min
Delta R.T.: -0.012 min
Response: 10167424
Conc: 77.31 ng/ml

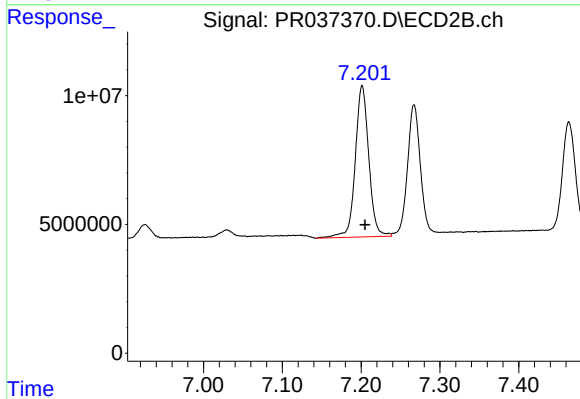

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.004 min
Response: 69858715
Conc: 127.42 ng/ml

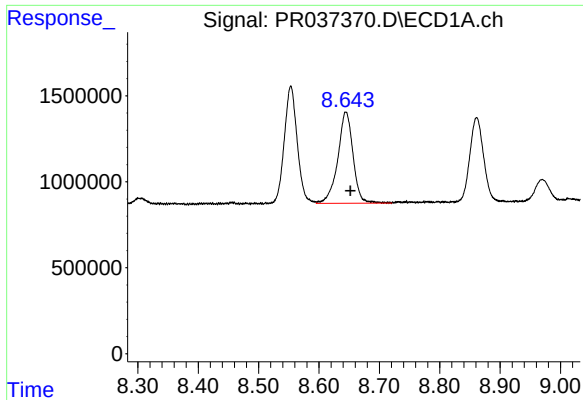

#39 AR-1262-4


R.T.: 8.645 min
Delta R.T.: -0.007 min
Response: 9358838
Conc: 95.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

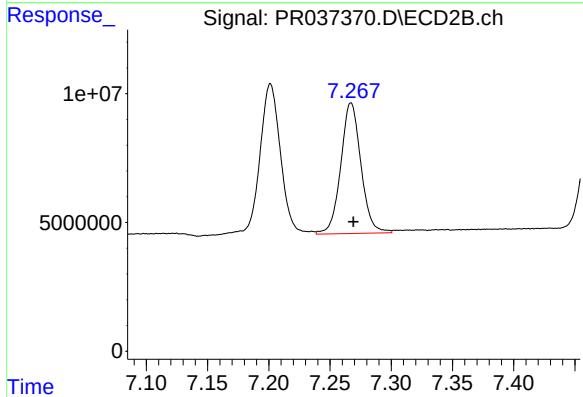


#39 AR-1262-4

R.T.: 7.267 min
Delta R.T.: -0.002 min
Response: 58189761
Conc: 64.82 ng/ml

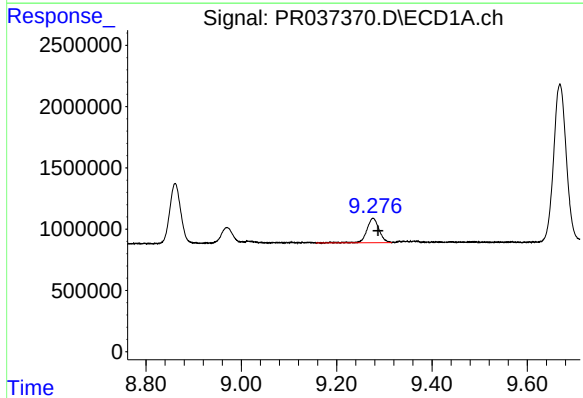


#40 AR-1262-5

R.T.: 9.277 min
Delta R.T.: -0.011 min
Response: 3533129
Conc: 51.17 ng/ml

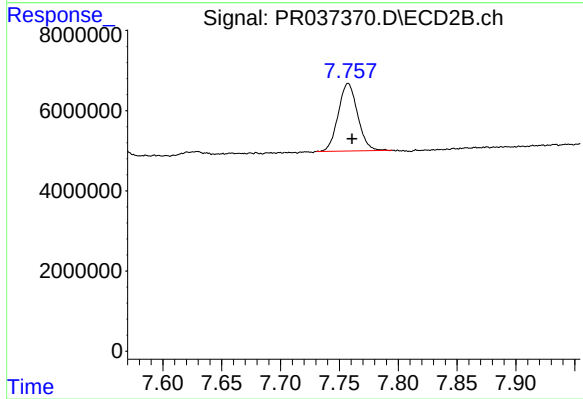

#40 AR-1262-5


R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 19287585
Conc: 50.41 ng/ml

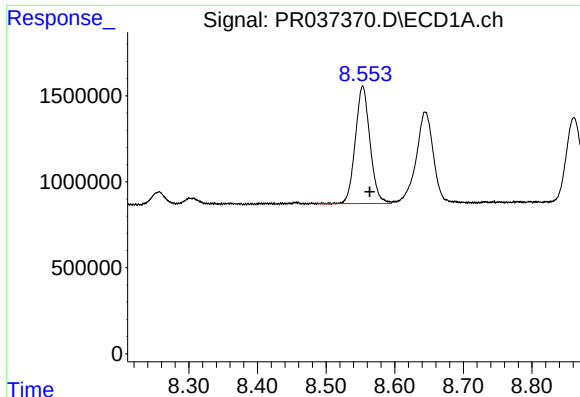

#41 AR-1268-1


R.T.: 8.553 min
Delta R.T.: -0.010 min
Response: 10167424
Conc: 56.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

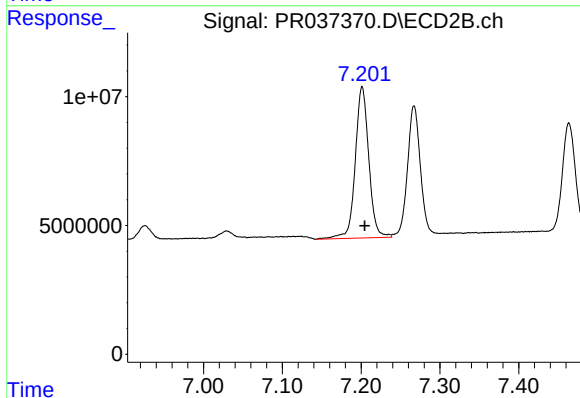


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.003 min
Response: 69858715
Conc: 56.75 ng/ml

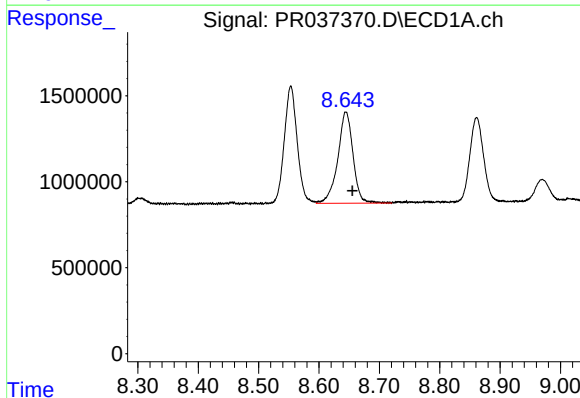


#42 AR-1268-2

R.T.: 8.645 min
Delta R.T.: -0.011 min
Response: 9358838
Conc: 56.89 ng/ml

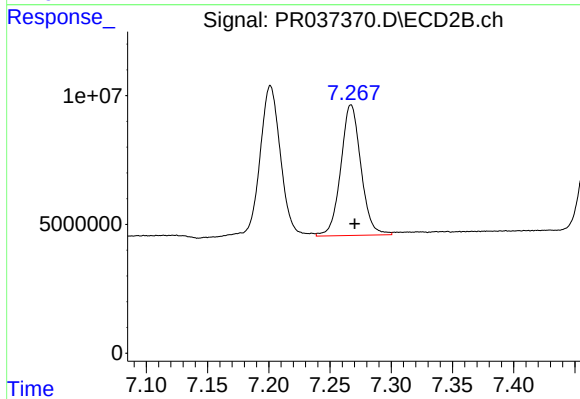

#42 AR-1268-2


R.T.: 7.267 min
Delta R.T.: -0.003 min
Response: 58189761
Conc: 54.95 ng/ml

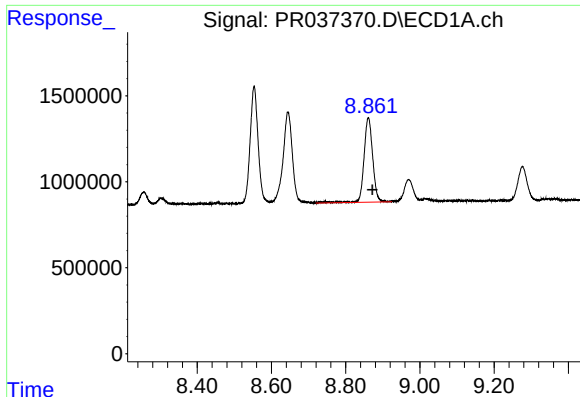

#43 AR-1268-3


R.T.: 8.861 min
Delta R.T.: -0.011 min
Response: 8050392
Conc: 58.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

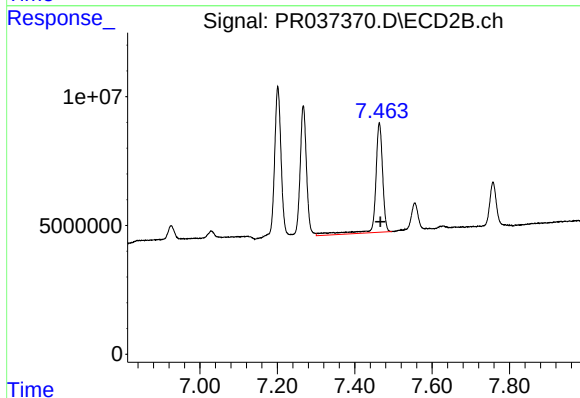


#43 AR-1268-3

R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 55065164
Conc: 62.13 ng/ml

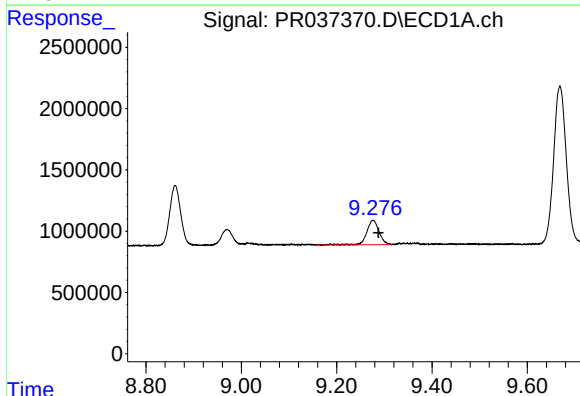


#44 AR-1268-4

R.T.: 9.277 min
Delta R.T.: -0.011 min
Response: 3533129
Conc: 56.63 ng/ml

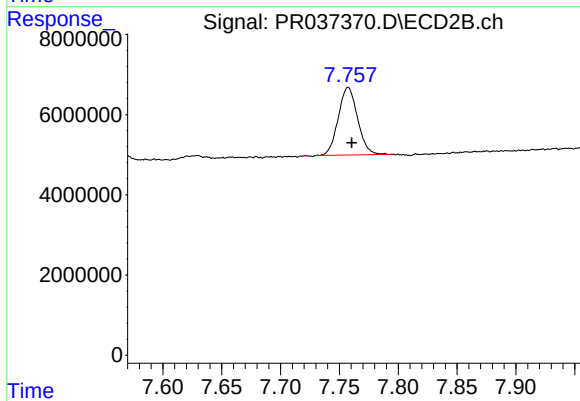

#44 AR-1268-4


R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 19287585
Conc: 53.17 ng/ml

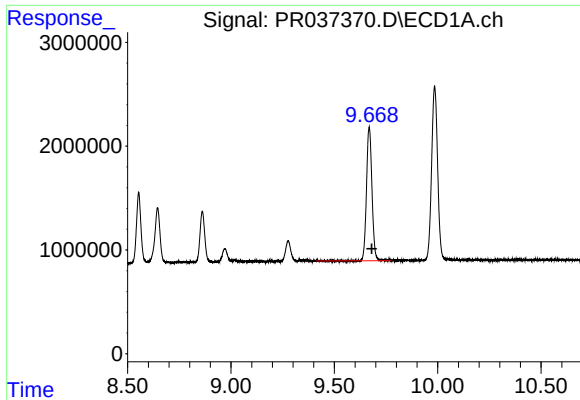

#45 AR-1268-5

R.T.: 9.668 min
Delta R.T.: -0.012 min
Response: 23672057
Conc: 51.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT2-2019

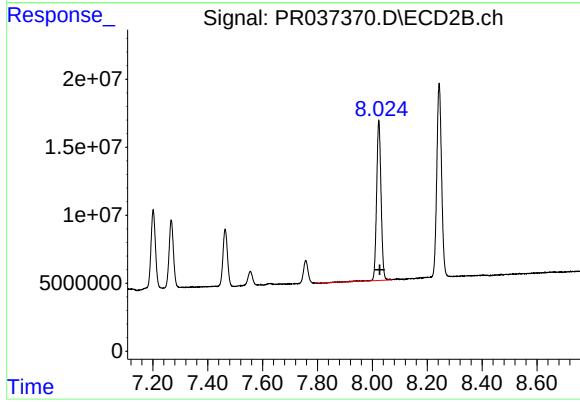

#45 AR-1268-5

R.T.: 8.024 min
Delta R.T.: -0.004 min
Response: 132411434
Conc: 52.04 ng/ml