

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021320\
 Data File : PR044739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Feb 2020 11:35
 Operator : AJ\MA
 Sample : L1490-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 00:28:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR012620CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 22:56:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.692	3.956	151.4E6	299.5E6	20.999	20.115
2)	SA Decachlor...	10.575	9.027	320.8E6	567.7E6	43.299	42.419
Target Compounds							
9)	L2 AR-1221-2	4.999	0.000	1518210	0	26.927	N.D. #
10)	L2 AR-1221-3	4.999f	0.000	1518210	0	7.868	N.D. #
11)	L3 AR-1232-1	4.999f	0.000	1518210	0	10.512	N.D. #
12)	L3 AR-1232-2	5.604	0.000	86800	0	1.186	N.D. #
27)	L6 AR-1254-2	6.963	0.000	927590	0	1.986	N.D. #
28)	L6 AR-1254-3	7.324	0.000	1163350	0	2.300	N.D. #
32)	L7 AR-1260-2	7.779f	0.000	1453875	0	3.206	N.D. #
43)	L9 AR-1268-3	9.324	0.000	1561295	0	1.726	N.D. #
45)	L9 AR-1268-5	10.218	0.000	2217993	0	0.699	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021320\
Data File : PR044739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Feb 2020 11:35
Operator : AJ\MA
Sample : L1490-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 00:28:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR012620CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 22:56:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

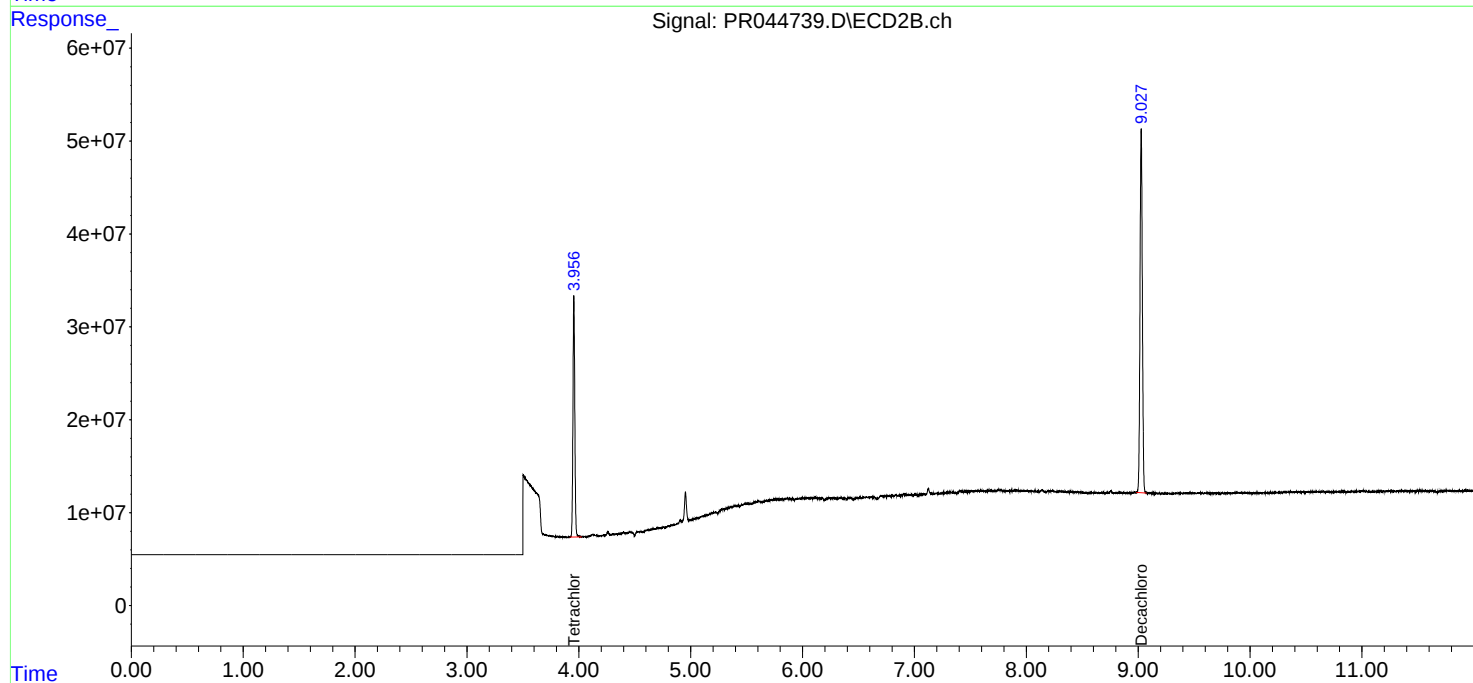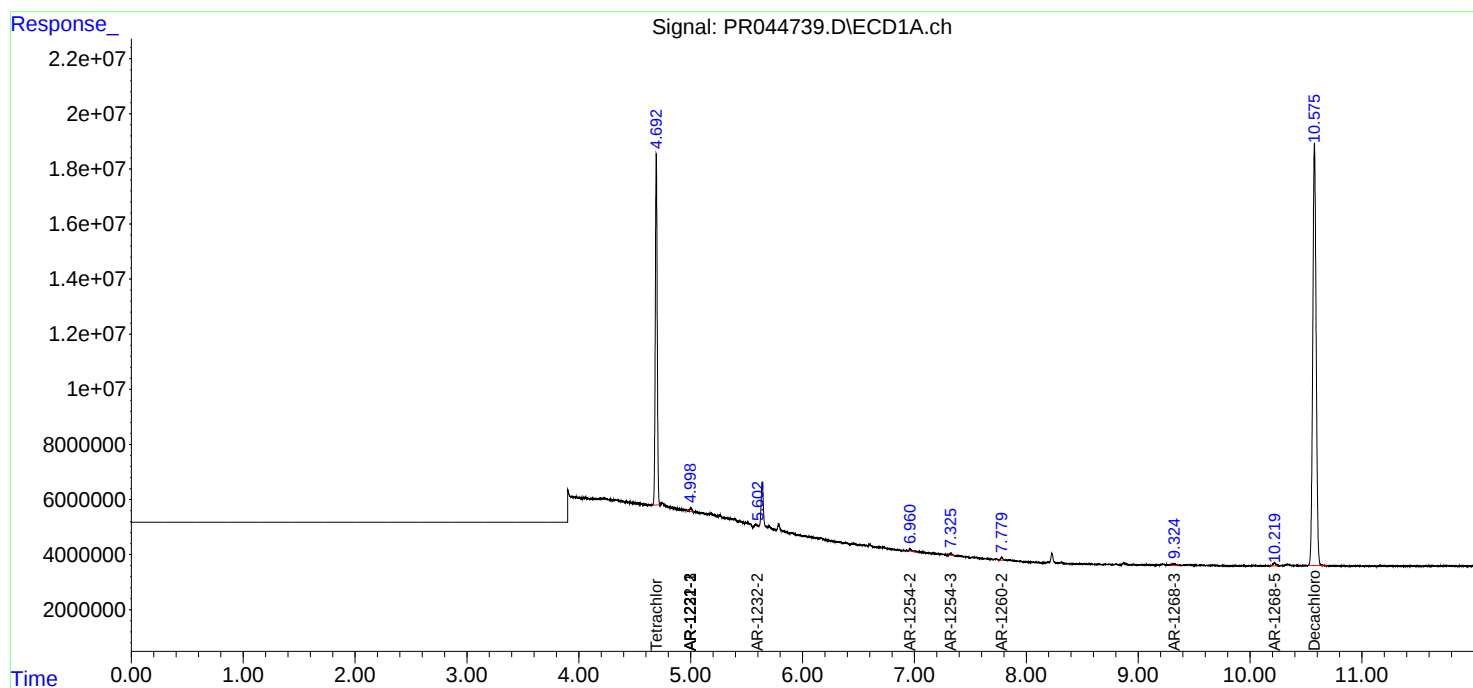


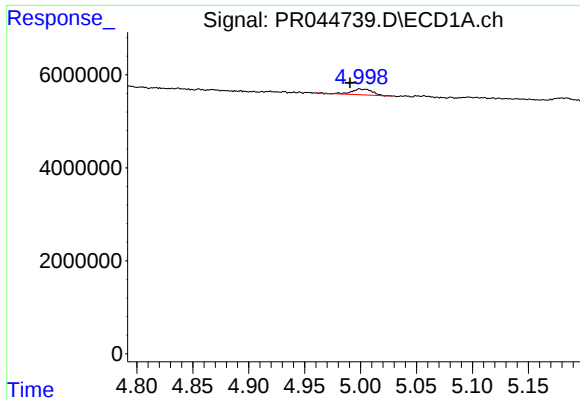

#9 AR-1221-2


R.T.: 4.999 min
Delta R.T.: 0.009 min
Response: 1518210
Conc: 26.93 ng/ml

Instrument :
ECD_R
ClientSampleId :

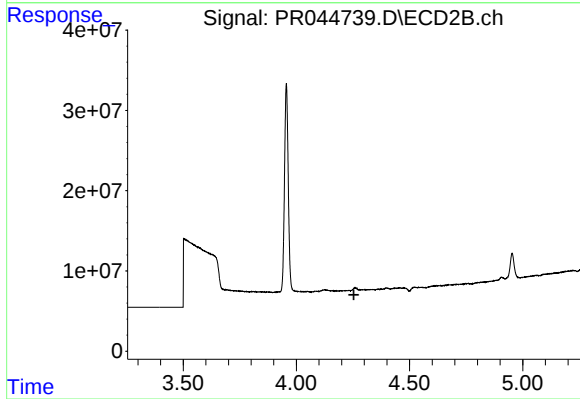


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.254 min
Response: 0
Conc: N.D.

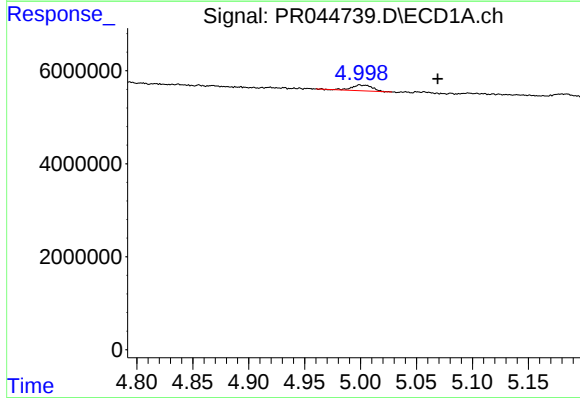


#10 AR-1221-3

R.T.: 4.999 min
Delta R.T.: -0.069 min
Response: 1518210
Conc: 7.87 ng/ml

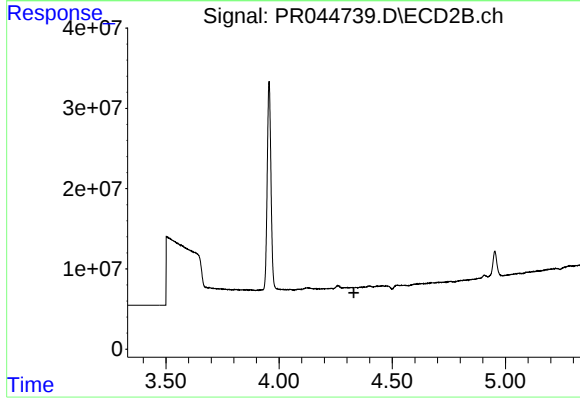

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

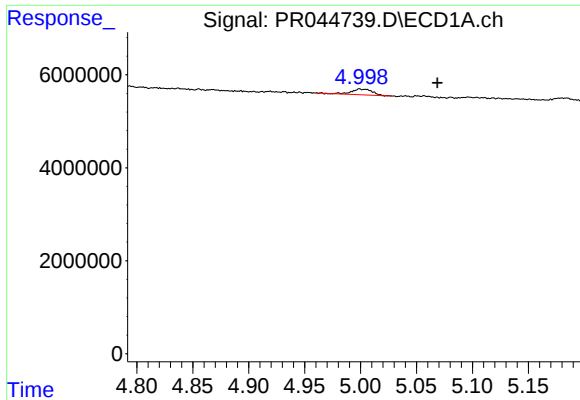

#11 AR-1232-1


R.T.: 4.999 min
Delta R.T.: -0.069 min
Response: 1518210
Conc: 10.51 ng/ml

Instrument :
ECD_R
ClientSampleId :

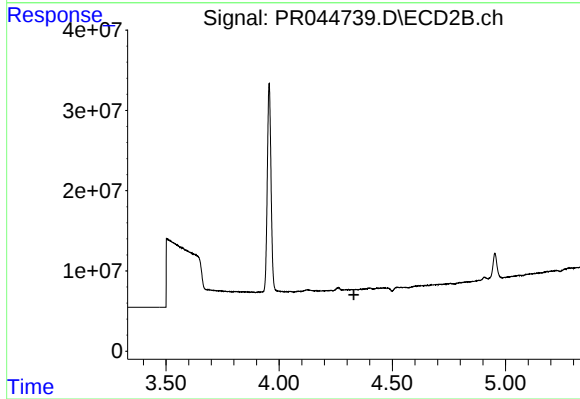


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

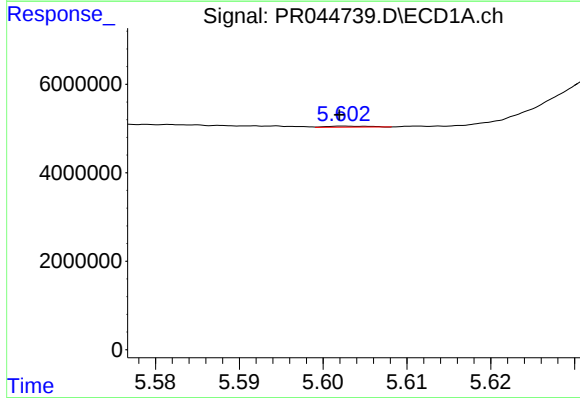


#12 AR-1232-2

R.T.: 5.604 min
Delta R.T.: 0.002 min
Response: 86800
Conc: 1.19 ng/ml

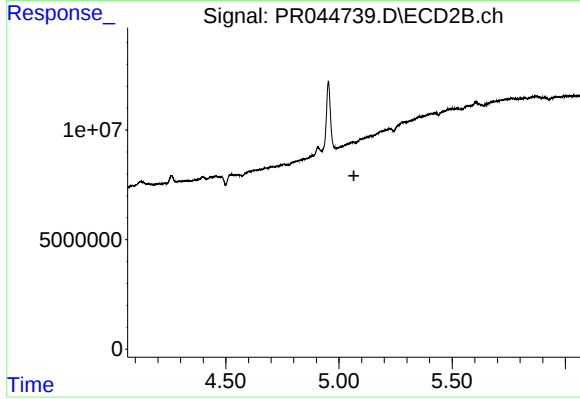

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 5.066 min
Response: 0
Conc: N.D.

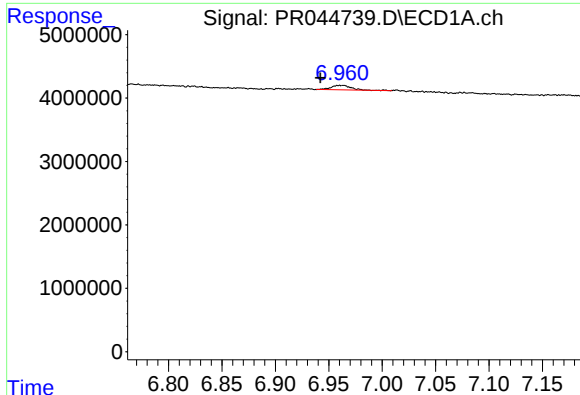

#27 AR-1254-2


R.T.: 6.963 min
Delta R.T.: 0.021 min
Response: 927590
Conc: 1.99 ng/ml

Instrument :
ECD_R
ClientSampleId :

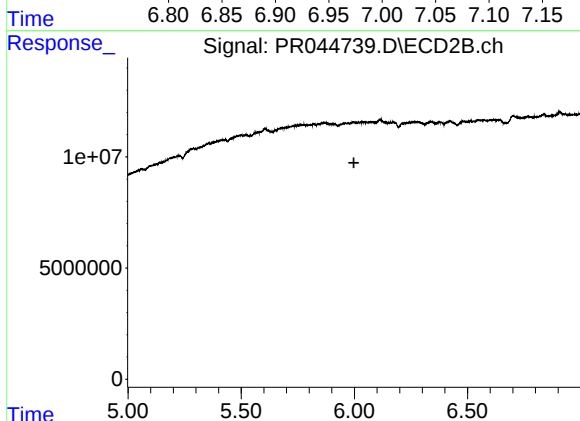


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.998 min
Response: 0
Conc: N.D.

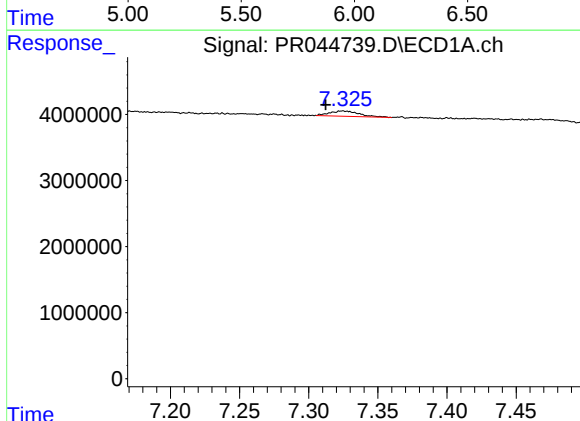


#28 AR-1254-3

R.T.: 7.324 min
Delta R.T.: 0.012 min
Response: 1163350
Conc: 2.30 ng/ml

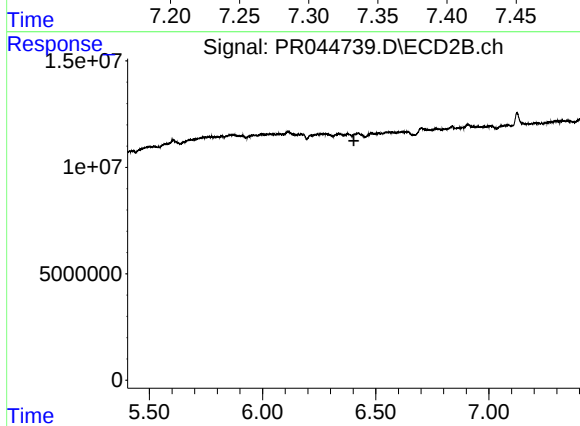

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.403 min
Response: 0
Conc: N.D.

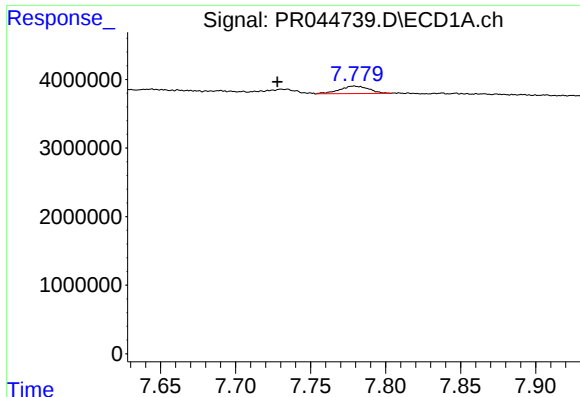

#32 AR-1260-2


R.T.: 7.779 min
Delta R.T.: 0.051 min
Response: 1453875
Conc: 3.21 ng/ml

Instrument :
ECD_R
ClientSampleId :

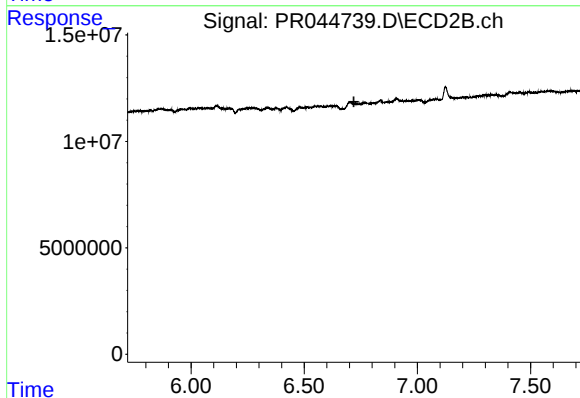


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.719 min
Response: 0
Conc: N.D.

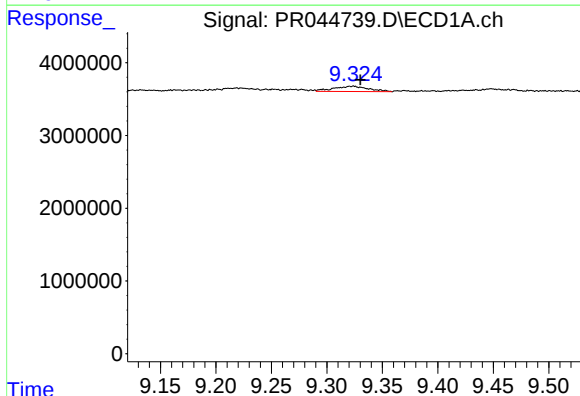


#43 AR-1268-3

R.T.: 9.324 min
Delta R.T.: -0.007 min
Response: 1561295
Conc: 1.73 ng/ml

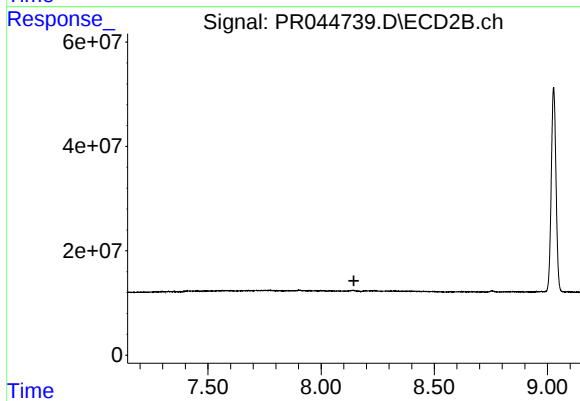

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.145 min
Response: 0
Conc: N.D.

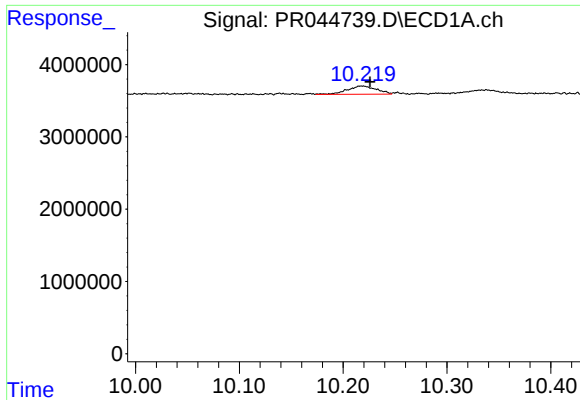

#45 AR-1268-5

R.T.: 10.218 min
Delta R.T.: -0.008 min
Response: 2217993
Conc: 0.70 ng/ml

Instrument :
ECD_R
ClientSampleId :

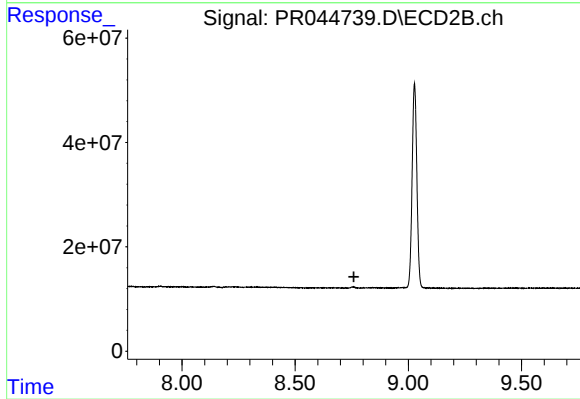

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.759 min
Response: 0
Conc: N.D.