

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030819\
 Data File : PR036010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 20:38
 Operator : SM\SJ
 Sample : K1808-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 21:53:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 07 10:54:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.481	31198649	101.9E6	19.631	19.397
2) SA Decachlor...	10.071	8.354	23021033	89056439	14.395	13.568

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030819\
Data File : PR036010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 20:38
Operator : SM\SJ
Sample : K1808-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 21:53:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 07 10:54:32 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

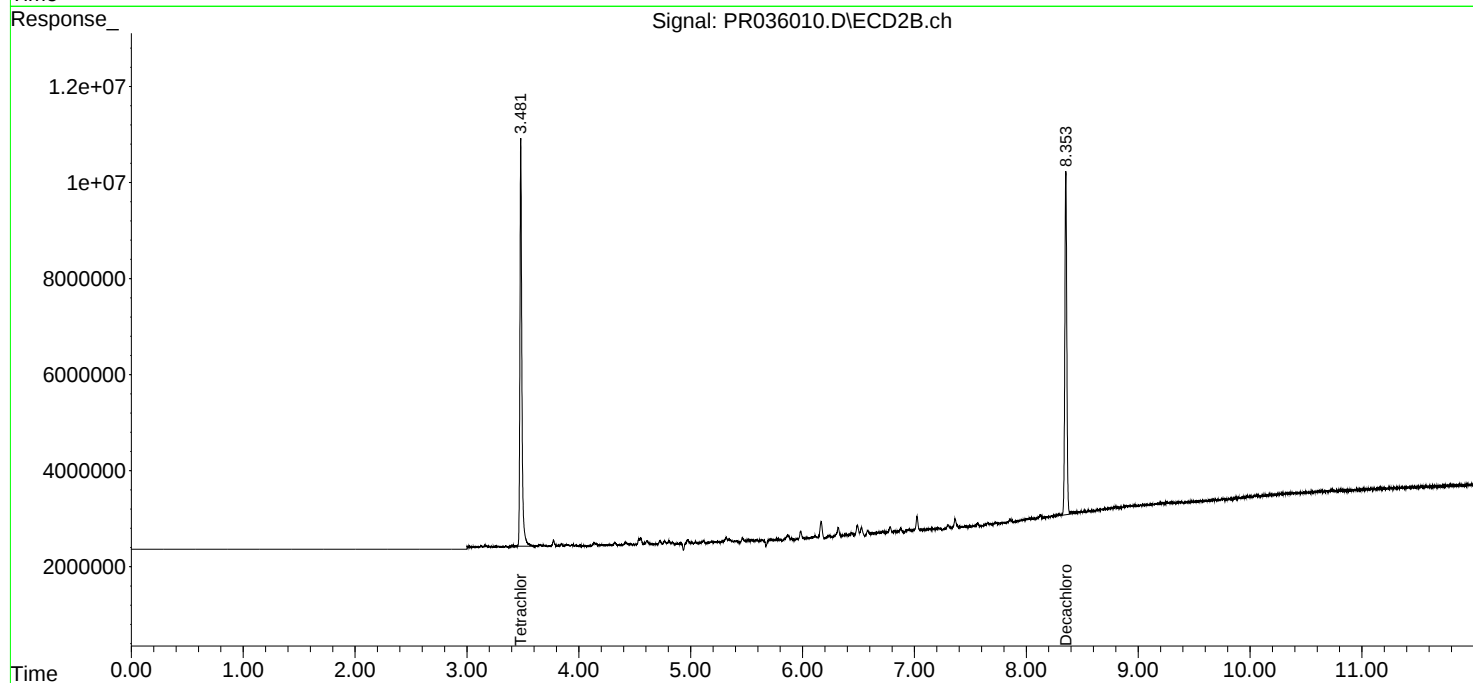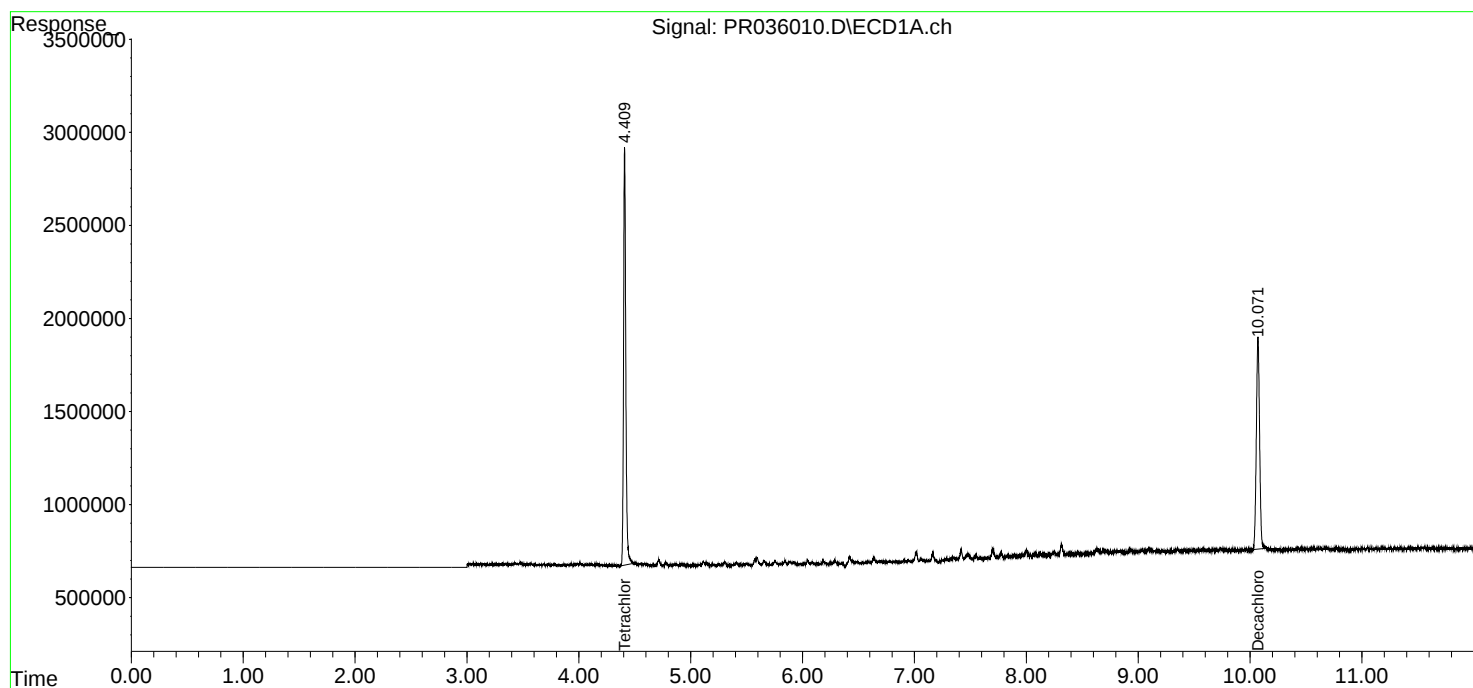


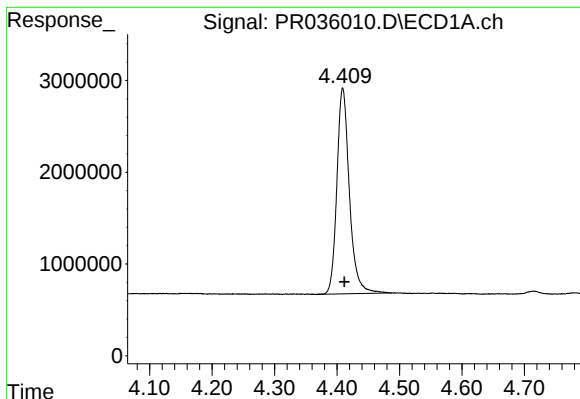

#1 Tetrachloro-m-xylene


R.T.: 4.409 min
Delta R.T.: -0.003 min
Response: 31198649
Conc: 19.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

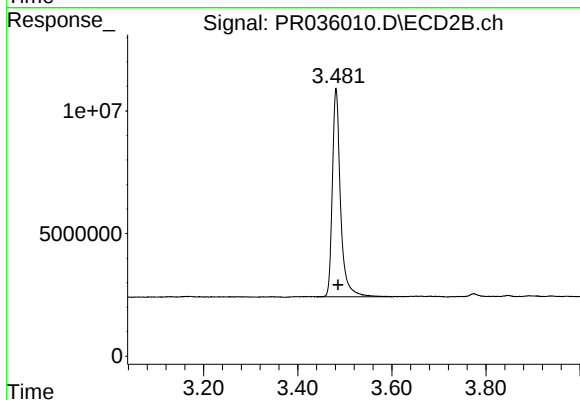


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: -0.004 min
Response: 101874171
Conc: 19.40 ng/ml

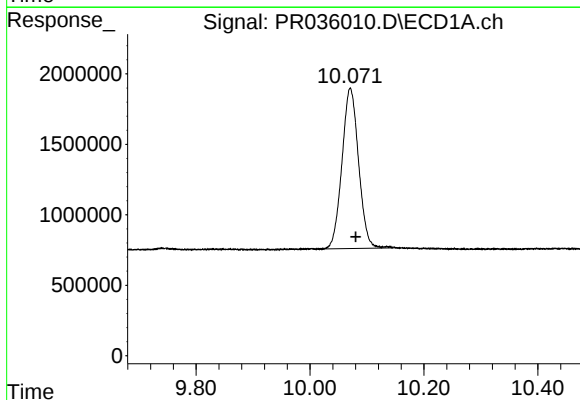

#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: -0.010 min
Response: 23021033
Conc: 14.40 ng/ml

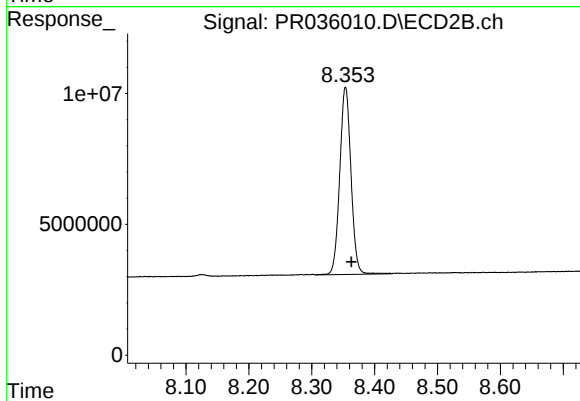

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: -0.009 min
Response: 89056439
Conc: 13.57 ng/ml