

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031119\
 Data File : PR036054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 16:43
 Operator : SM\SJ
 Sample : K1807-31
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 03:50:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 07 10:54:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.408	3.481	22662330	76046772	14.260	14.480
2) SA Decachlor...	10.071	8.354	20332136	78275019	12.714	11.925
Target Compounds						
28) L6 AR-1254-3	7.018	0.000	1501816	0	14.423	N.D. #
29) L6 AR-1254-4	7.232	0.000	6386278	0	81.547	N.D. #
31) L7 AR-1260-1	7.232	0.000	6386278	0	65.768	N.D. #
32) L7 AR-1260-2	0.000	6.162	0	17626873	N.D.	33.744 #
35) L7 AR-1260-5	0.000	7.030	0	3383524	N.D.	3.746 #
37) L8 AR-1262-2	0.000	7.030	0	3383524	N.D.	3.247 #
43) L9 AR-1268-3	0.000	7.565	0	14252026	N.D.	14.529 #
45) L9 AR-1268-5	0.000	8.126	0	2123218	N.D.	0.798 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031119\
Data File : PR036054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 16:43
Operator : SM\SJ
Sample : K1807-31
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
TP-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:50:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 07 10:54:32 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

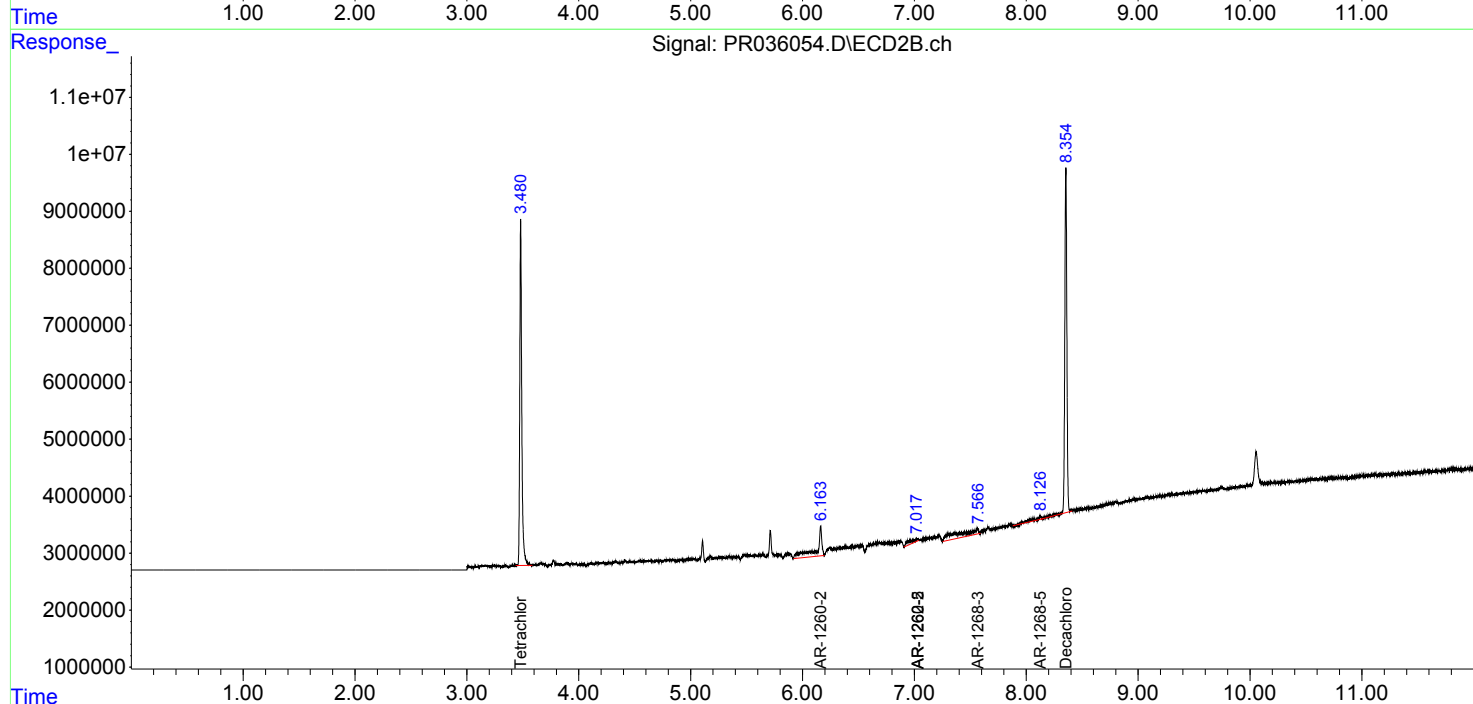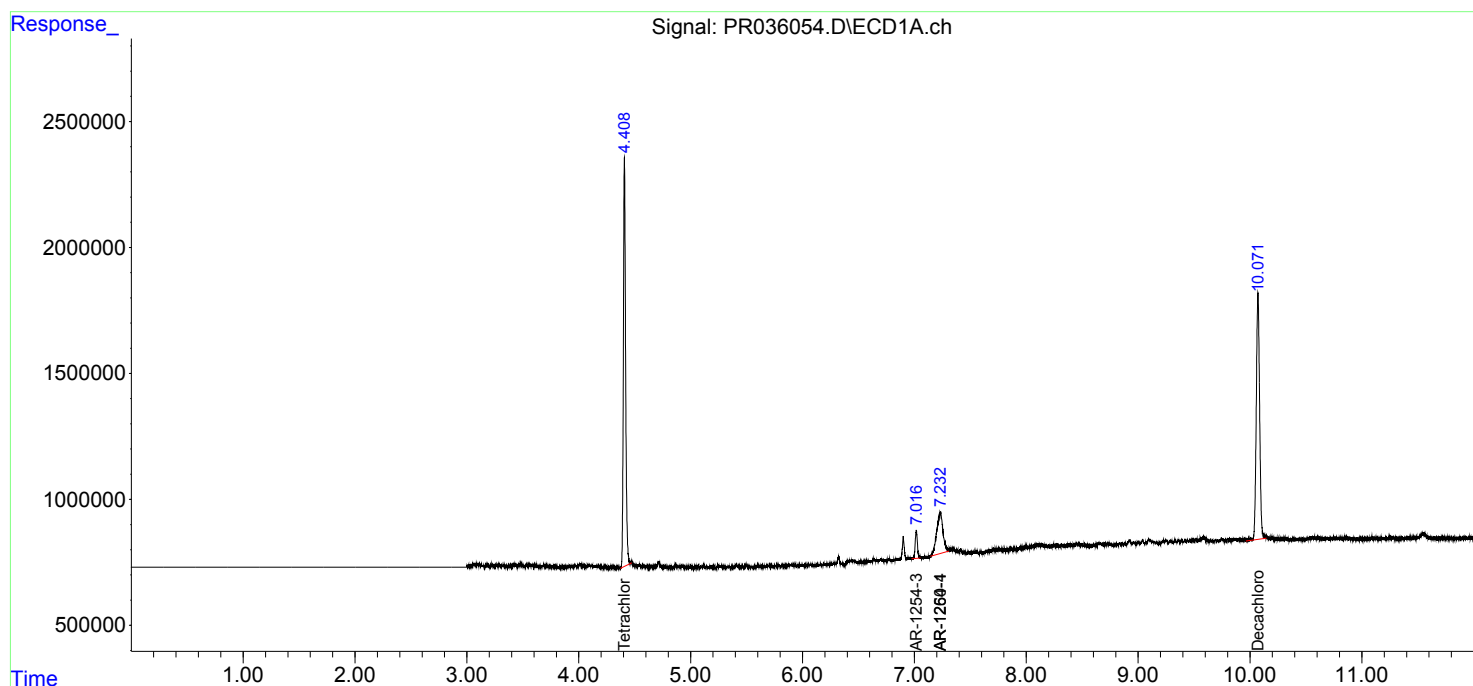


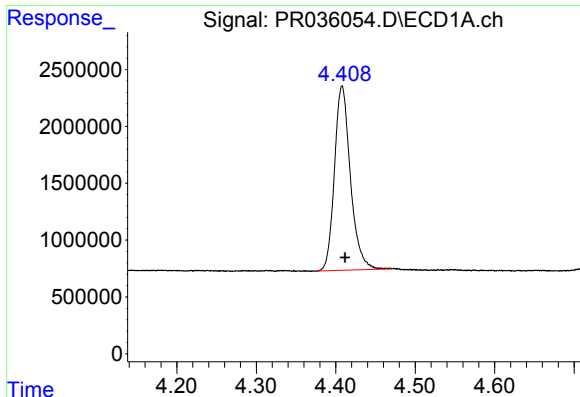

#1 Tetrachloro-m-xylene


R.T.: 4.408 min
Delta R.T.: -0.004 min
Response: 22662330
Conc: 14.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-13

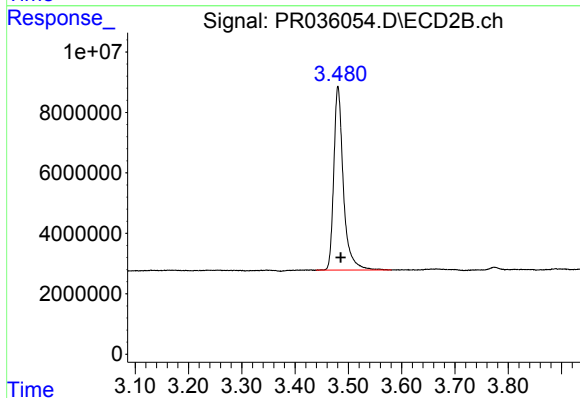


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: -0.005 min
Response: 76046772
Conc: 14.48 ng/ml

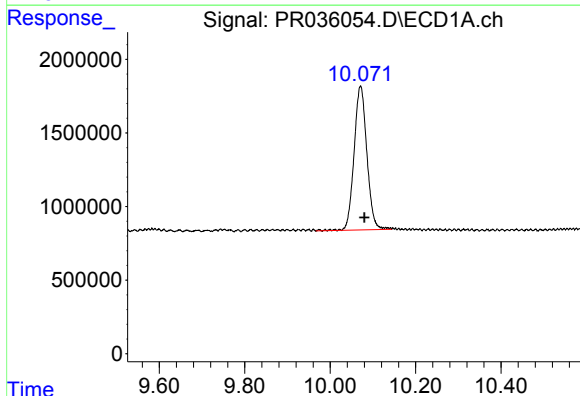


#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: -0.009 min
Response: 20332136
Conc: 12.71 ng/ml

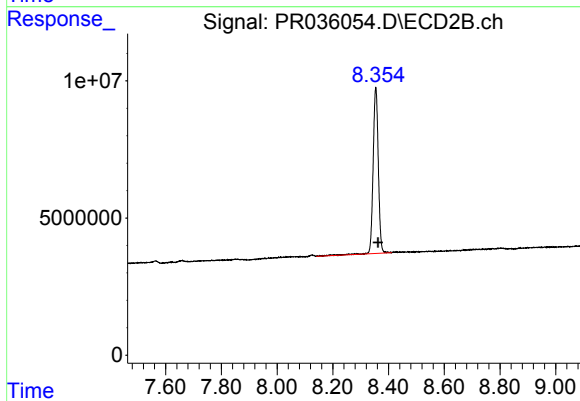

#2 Decachlorobiphenyl


R.T.: 8.354 min
Delta R.T.: -0.009 min
Response: 78275019
Conc: 11.93 ng/ml

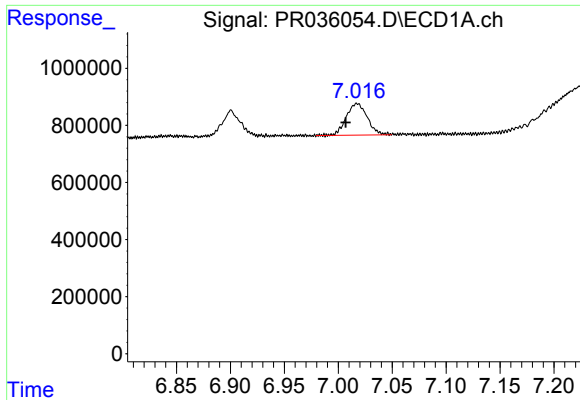

#28 AR-1254-3


R.T.: 7.018 min
Delta R.T.: 0.011 min
Response: 1501816
Conc: 14.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-13

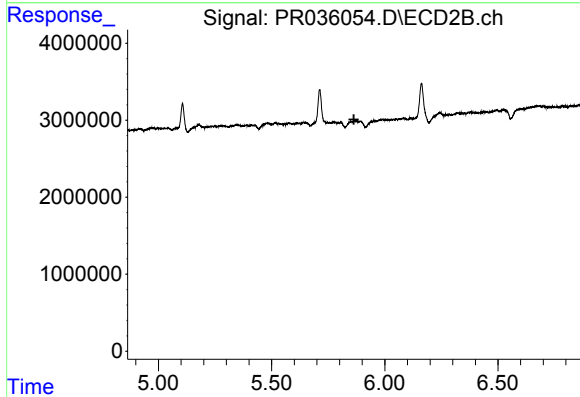


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.864 min
Response: 0
Conc: N.D.

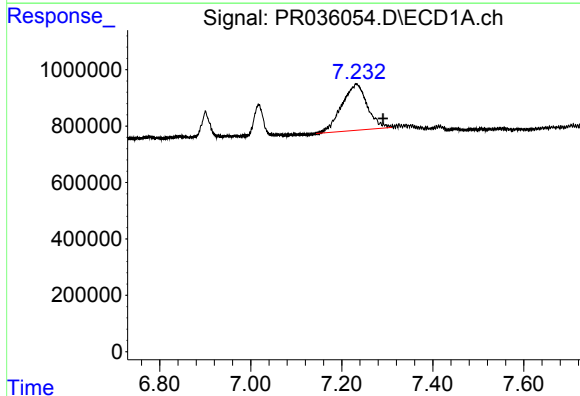


#29 AR-1254-4

R.T.: 7.232 min
Delta R.T.: -0.059 min
Response: 6386278
Conc: 81.55 ng/ml

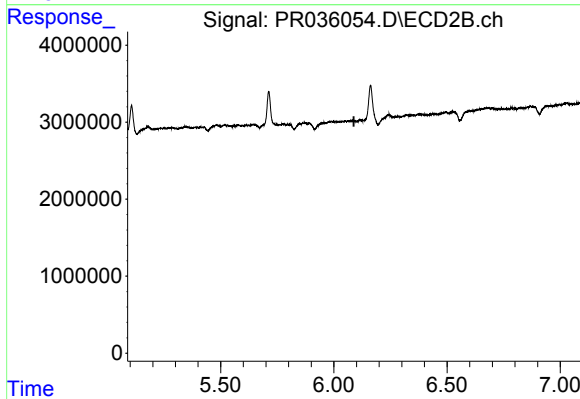

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

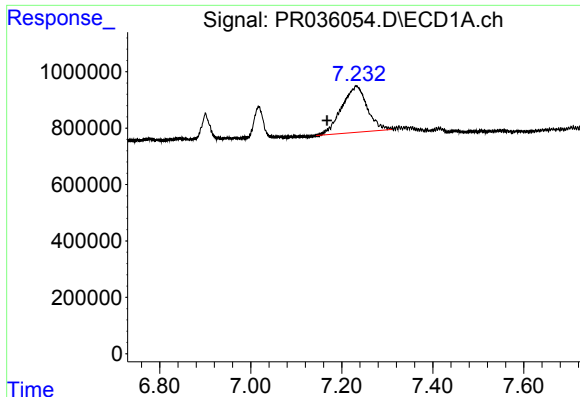

#31 AR-1260-1


R.T.: 7.232 min
Delta R.T.: 0.064 min
Response: 6386278
Conc: 65.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-13

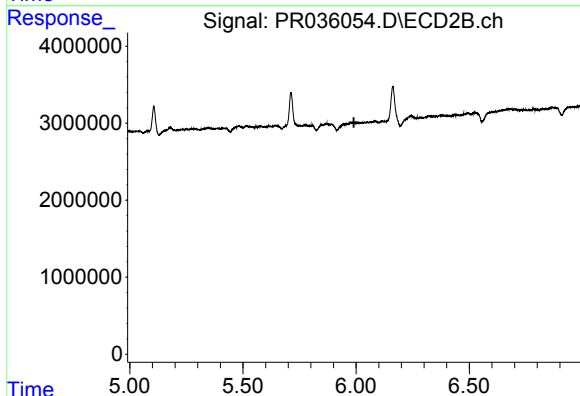


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.990 min
Response: 0
Conc: N.D.

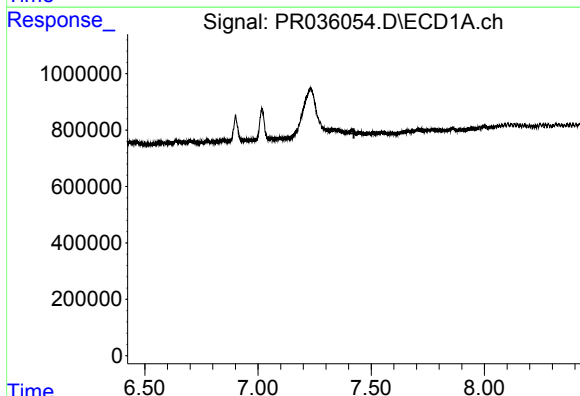


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.424 min
Response: 0
Conc: N.D.

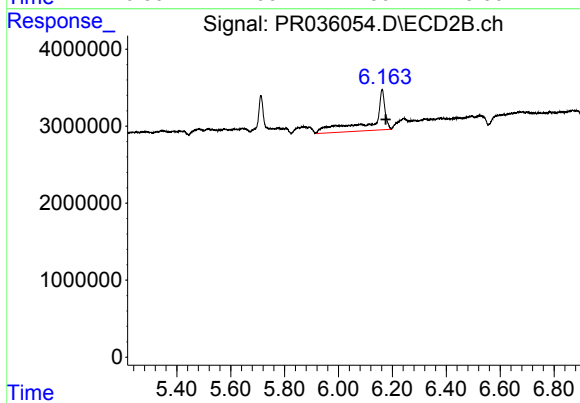

#32 AR-1260-2


R.T.: 6.162 min
Delta R.T.: -0.014 min
Response: 17626873
Conc: 33.74 ng/ml

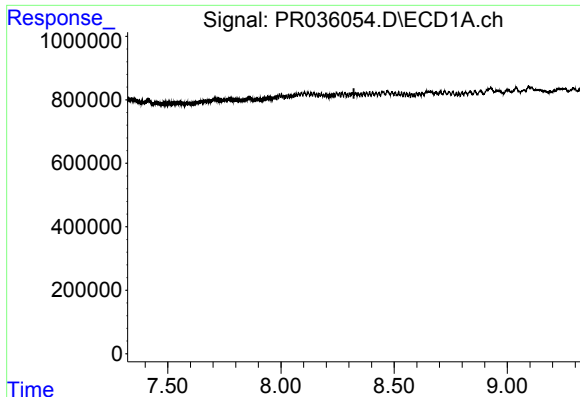

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
TP-13

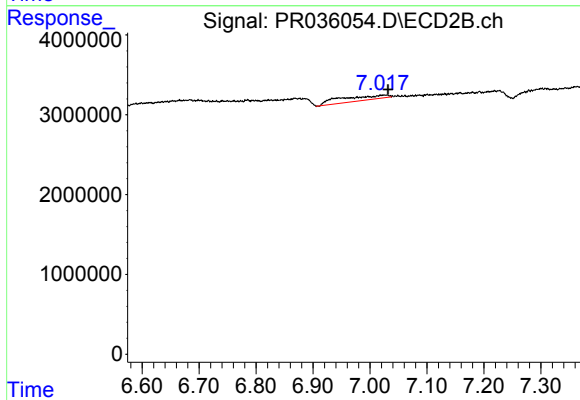


#35 AR-1260-5

R.T.: 7.030 min
Delta R.T.: -0.002 min
Response: 3383524
Conc: 3.75 ng/ml

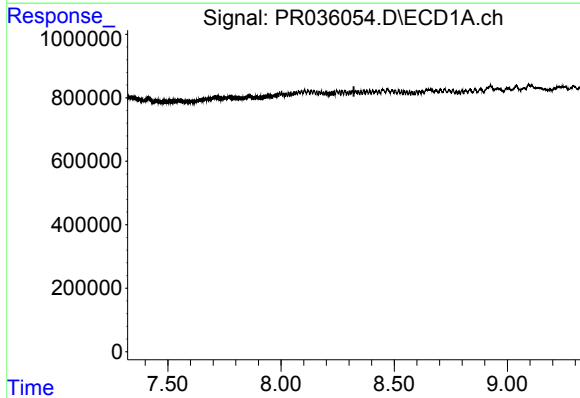


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.322 min
Response: 0
Conc: N.D.

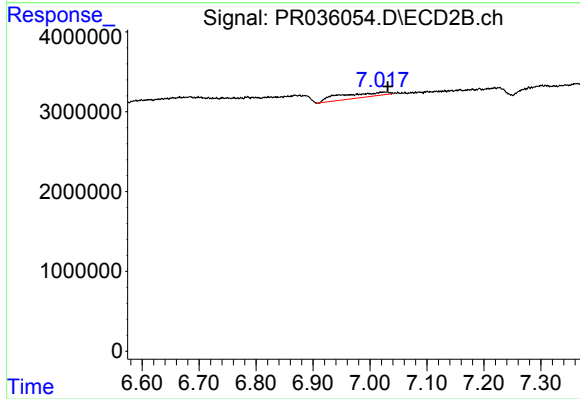

#37 AR-1262-2


R.T.: 7.030 min
Delta R.T.: -0.002 min
Response: 3383524
Conc: 3.25 ng/ml

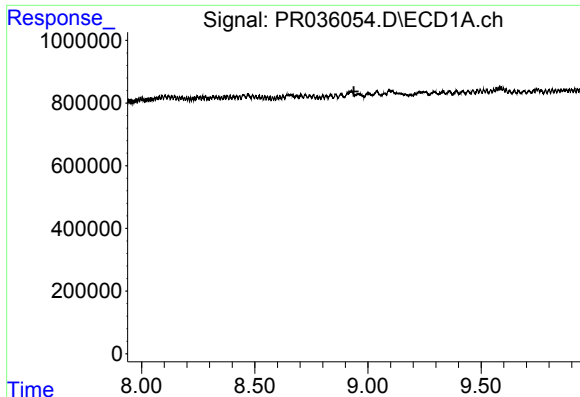

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.938 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
TP-13

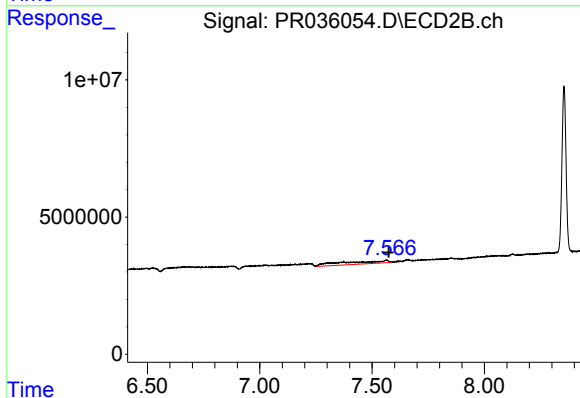


#43 AR-1268-3

R.T.: 7.565 min
Delta R.T.: -0.008 min
Response: 14252026
Conc: 14.53 ng/ml

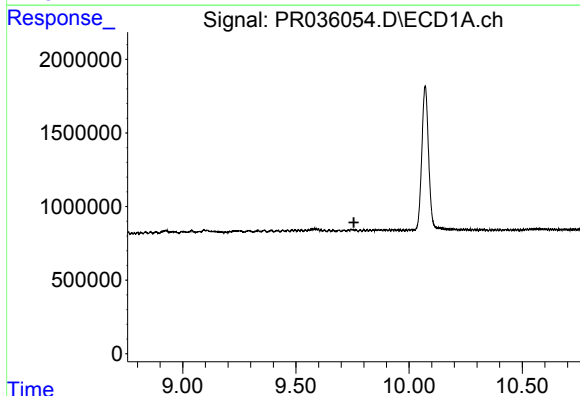

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

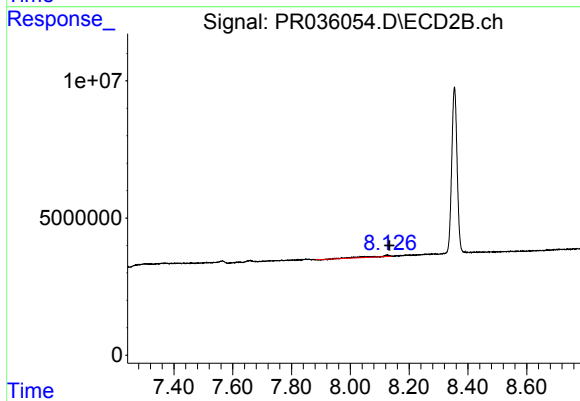

#45 AR-1268-5

R.T.: 8.126 min
Delta R.T.: -0.008 min
Response: 2123218
Conc: 0.80 ng/ml