

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031219\
 Data File : PR036089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 18:46
 Operator : SM\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 00:45:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 07 10:54:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.408	3.482	35559573	115.2E6	22.375	21.939
2)	SA Decachlor...	10.068	8.351	32549841	112.1E6	20.353	17.077
Target Compounds							
7)	L1 AR-1016-5	0.000	4.975	0	5882224	N.D.	36.278 #
9)	L2 AR-1221-2	0.000	3.774	0	1574405	N.D.	30.751 #
15)	L3 AR-1232-5	0.000	4.975	0	5882224	N.D.	100.692 #
24)	L5 AR-1248-4	0.000	4.975	0	5882224	N.D.	25.159 #
29)	L6 AR-1254-4	7.226	0.000	5631380	0	71.907	N.D. #
31)	L7 AR-1260-1	7.226	0.000	5631380	0	57.994	N.D. #
32)	L7 AR-1260-2	0.000	6.161	0	9526911	N.D.	18.238 #
45)	L9 AR-1268-5	0.000	8.122	0	1936763	N.D.	0.728 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031219\
Data File : PR036089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 18:46
Operator : SM\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 00:45:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 07 10:54:32 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

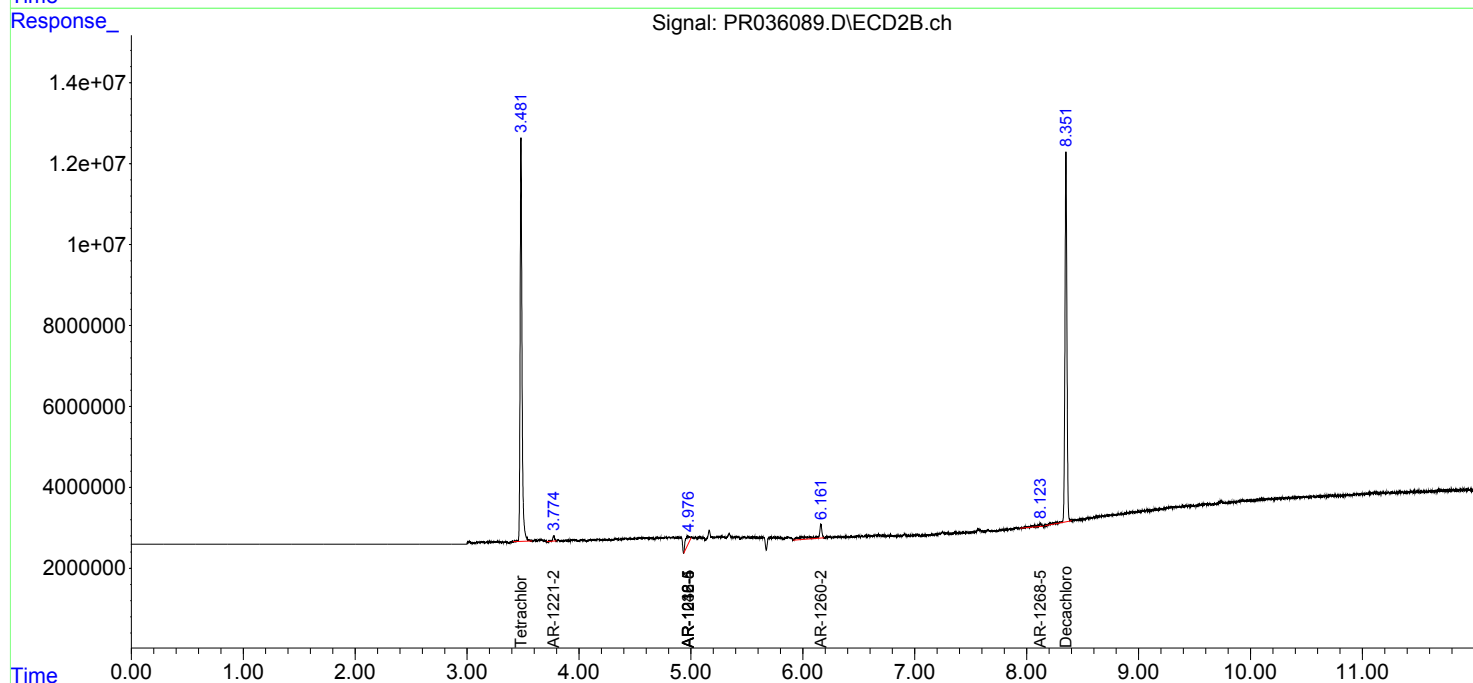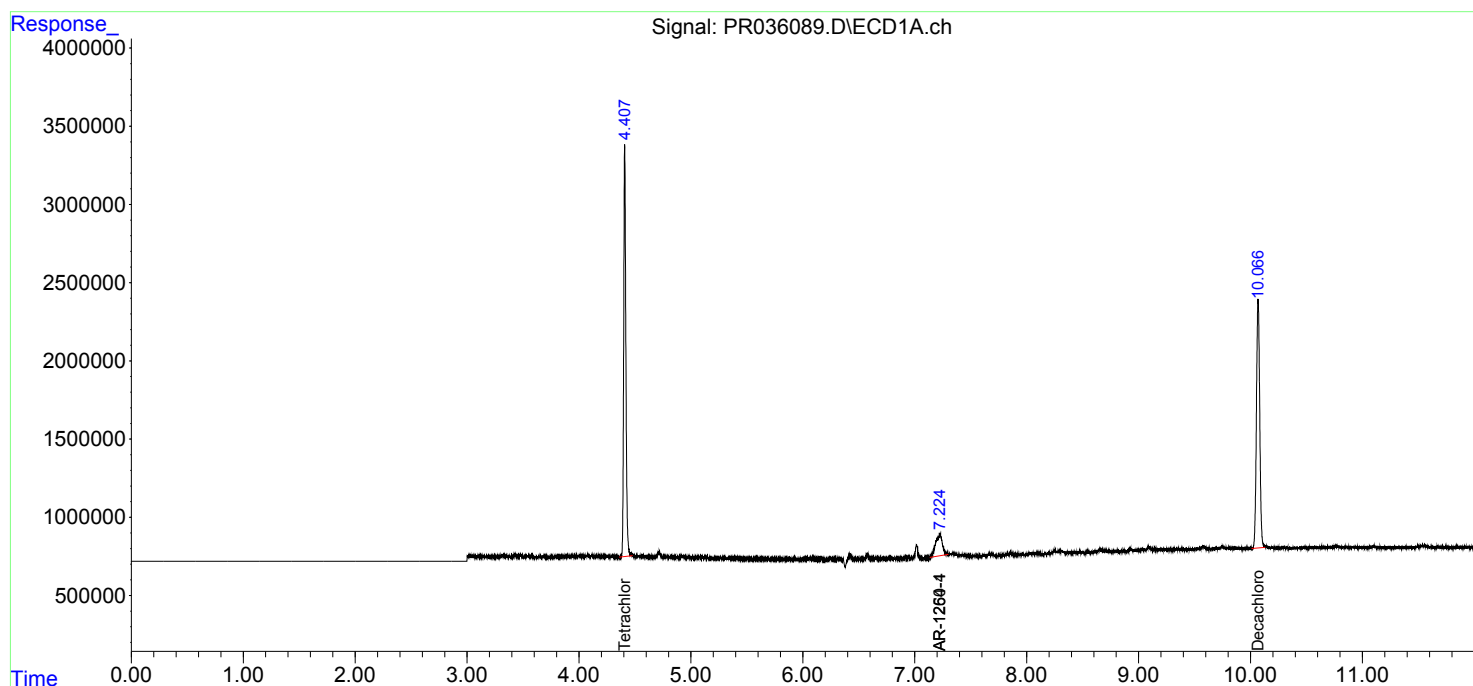


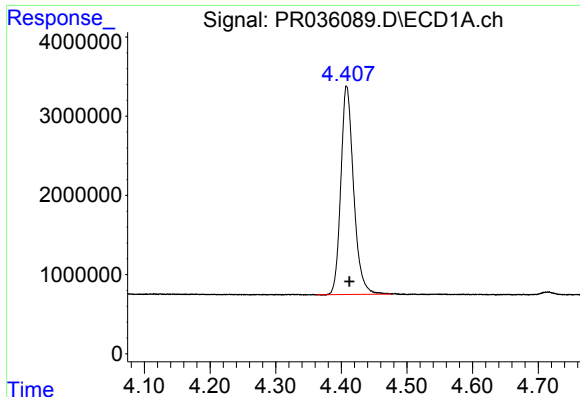

#1 Tetrachloro-m-xylene


R.T.: 4.408 min
Delta R.T.: -0.004 min
Response: 35559573
Conc: 22.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

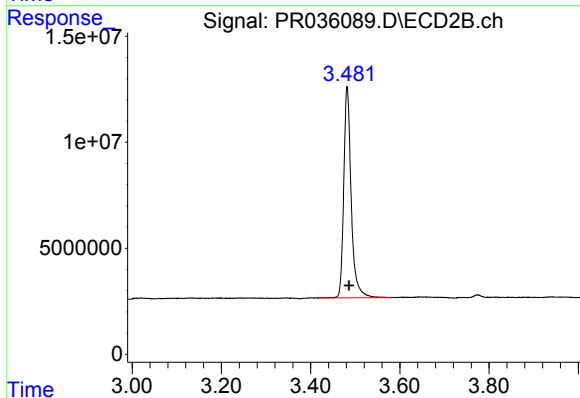


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: -0.004 min
Response: 115222498
Conc: 21.94 ng/ml

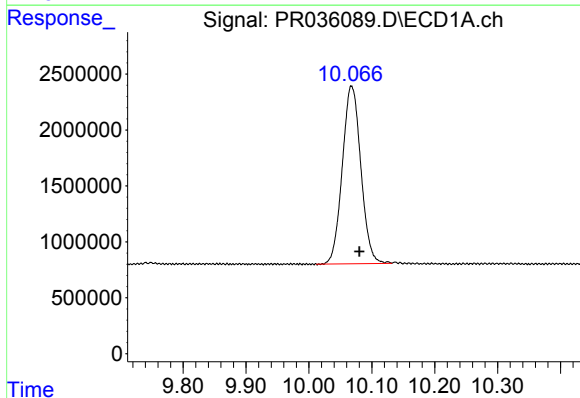


#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: -0.013 min
Response: 32549841
Conc: 20.35 ng/ml

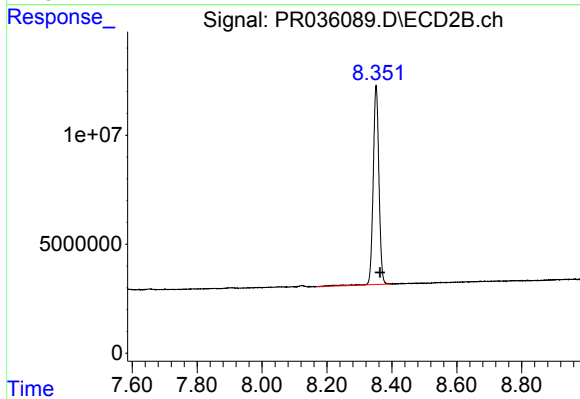

#2 Decachlorobiphenyl


R.T.: 8.351 min
Delta R.T.: -0.012 min
Response: 112092687
Conc: 17.08 ng/ml

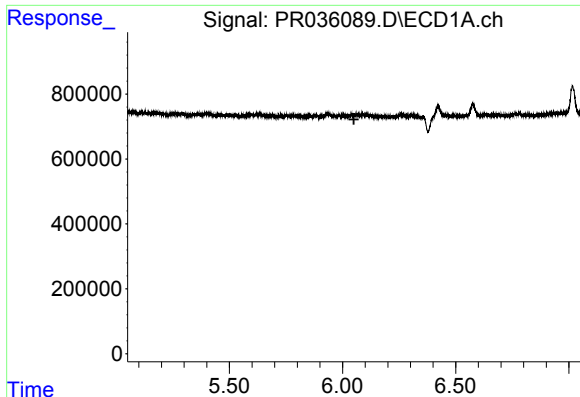

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

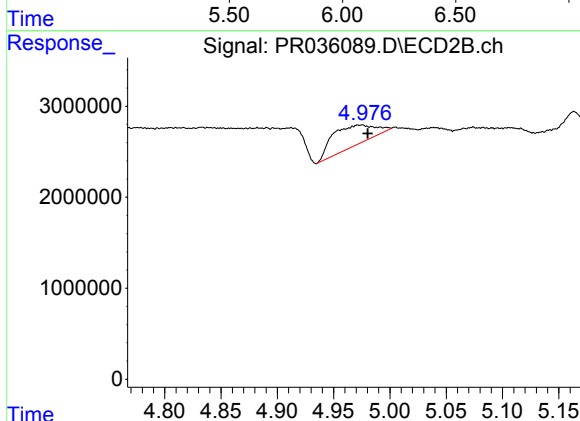


#7 AR-1016-5

R.T.: 4.975 min
Delta R.T.: -0.005 min
Response: 5882224
Conc: 36.28 ng/ml

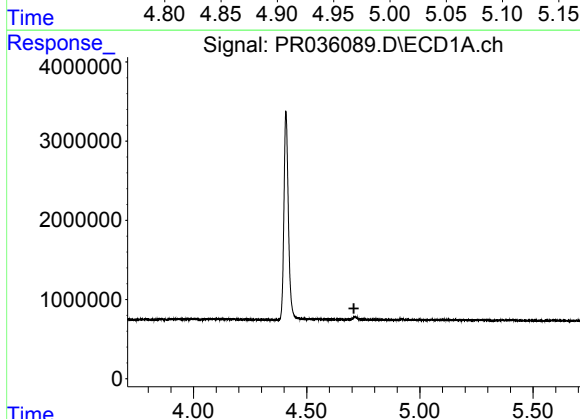


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.709 min
Response: 0
Conc: N.D.

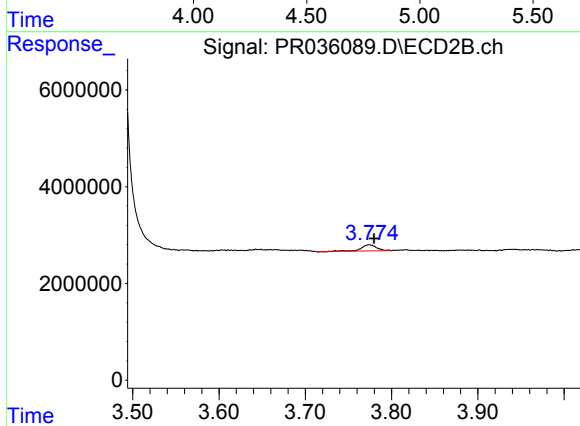

#9 AR-1221-2


R.T.: 3.774 min
Delta R.T.: -0.006 min
Response: 1574405
Conc: 30.75 ng/ml

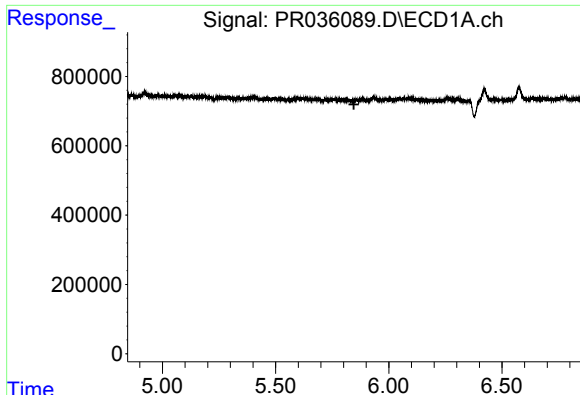

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

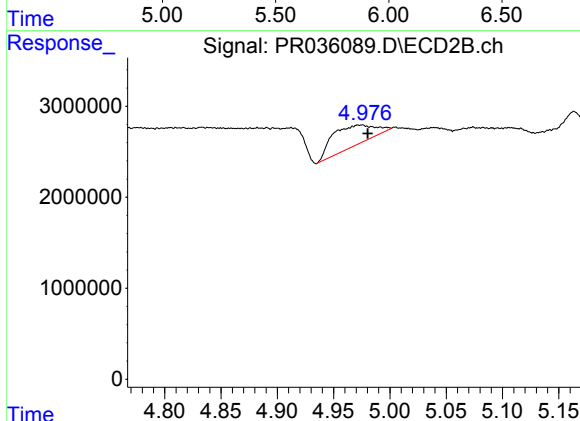


#15 AR-1232-5

R.T.: 4.975 min
Delta R.T.: -0.005 min
Response: 5882224
Conc: 100.69 ng/ml

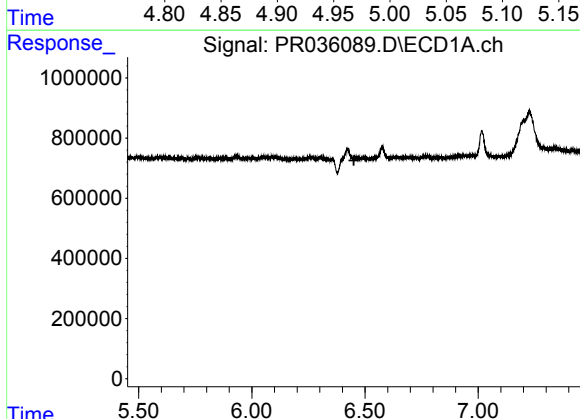


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

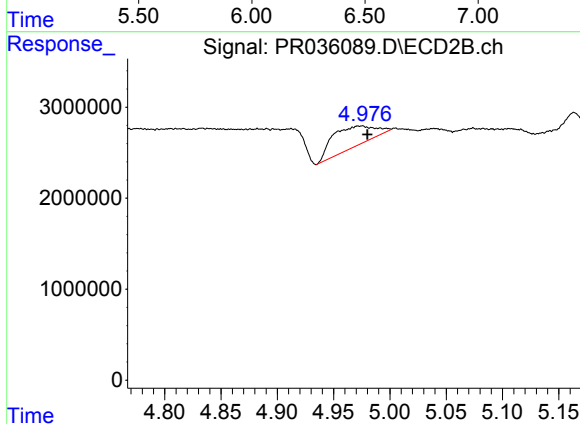

#24 AR-1248-4


R.T.: 4.975 min
Delta R.T.: -0.005 min
Response: 5882224
Conc: 25.16 ng/ml

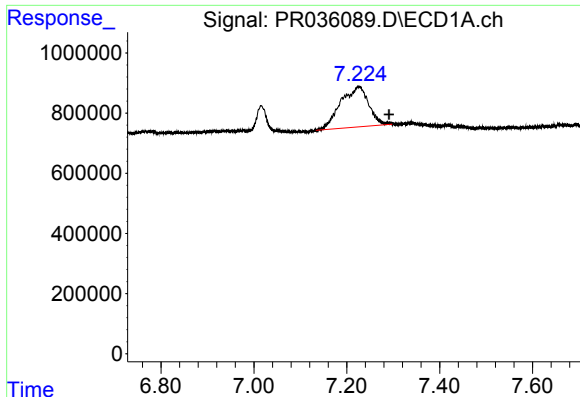

#29 AR-1254-4


R.T.: 7.226 min
Delta R.T.: -0.064 min
Response: 5631380
Conc: 71.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

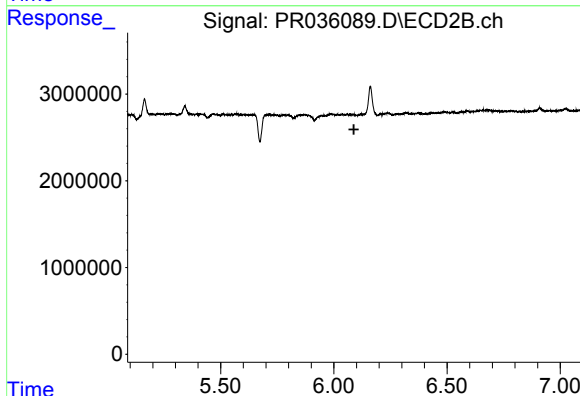


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

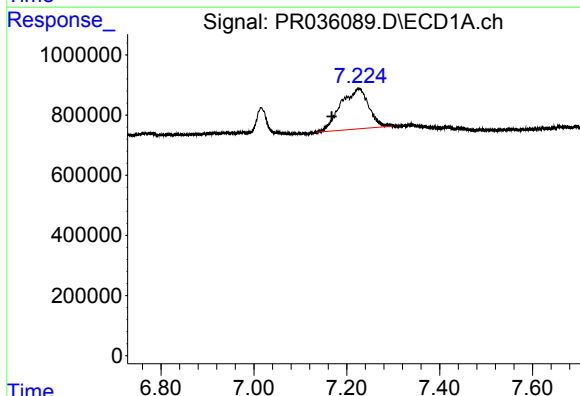


#31 AR-1260-1

R.T.: 7.226 min
Delta R.T.: 0.059 min
Response: 5631380
Conc: 57.99 ng/ml

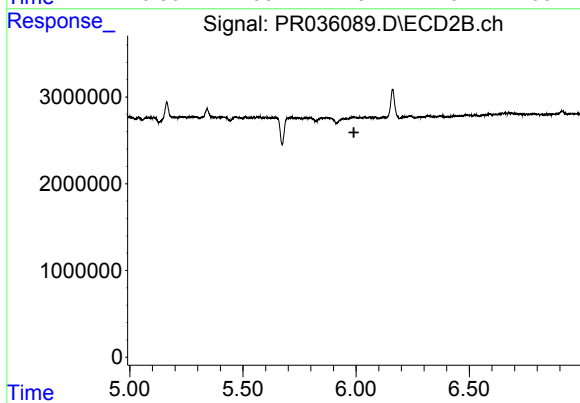

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 5.990 min
Response: 0
Conc: N.D.

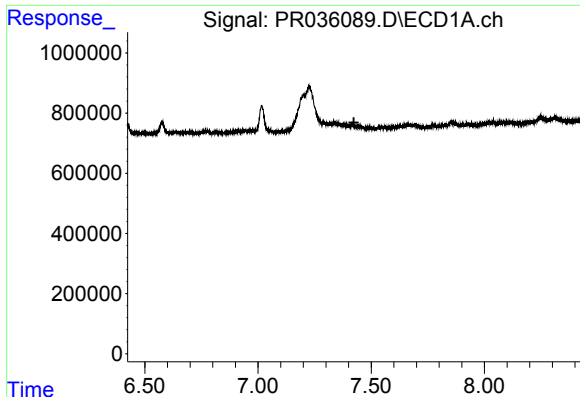

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

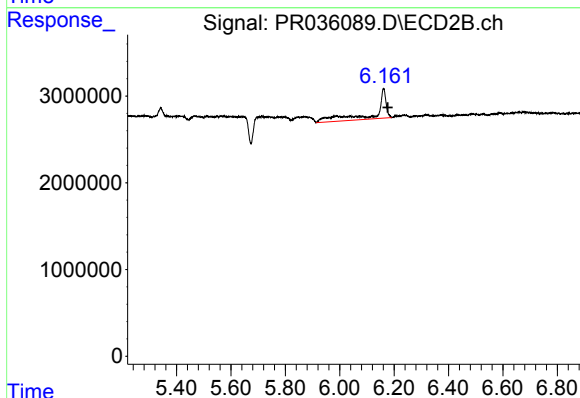


#32 AR-1260-2

R.T.: 6.161 min
Delta R.T.: -0.015 min
Response: 9526911
Conc: 18.24 ng/ml

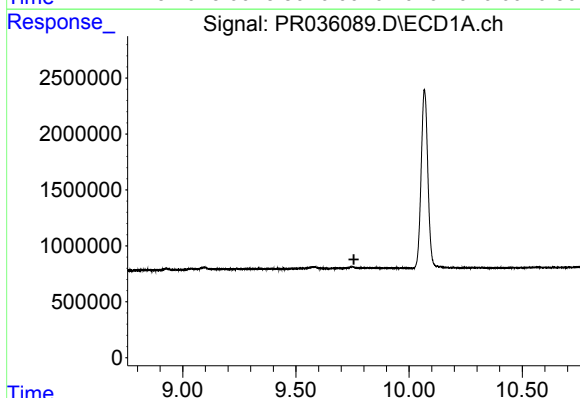

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

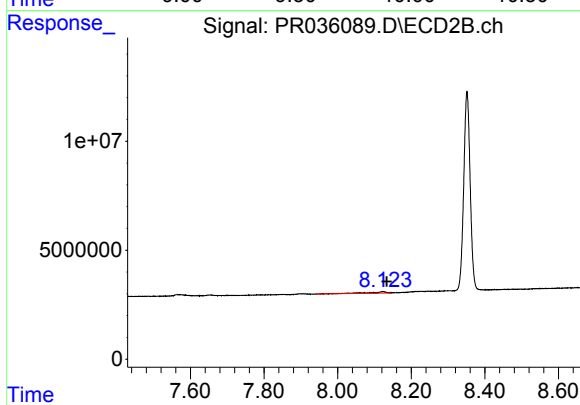

#45 AR-1268-5

R.T.: 8.122 min
Delta R.T.: -0.011 min
Response: 1936763
Conc: 0.73 ng/ml