

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040319\
 Data File : PR036802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 08:24
 Operator : SM\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 09:19:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.465	39460962	145.7E6	24.769	24.879
2)	SA Decachlor...	10.044	8.328	40488322	170.0E6	21.611	21.301
Target Compounds							
28)	L6 AR-1254-3	0.000	5.846	0 8815520	N.D.	17.329	#
30)	L6 AR-1254-5	0.000	6.490	0 26046298	N.D.	51.229	#
36)	L8 AR-1262-1	0.000	6.560	0 28328773	N.D.	103.345	#
39)	L8 AR-1262-4	0.000	7.406	0 52037673	N.D.	56.649	#
40)	L8 AR-1262-5	0.000	7.827	0 40310513	N.D.	100.356	#
42)	L9 AR-1268-2	0.000	7.406	0 52037673	N.D.	41.450	#
43)	L9 AR-1268-3	0.000	7.525	0 32975380	N.D.	33.904	#
44)	L9 AR-1268-4	0.000	7.827	0 40310513	N.D.	92.799	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040319\
Data File : PR036802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 08:24
Operator : SM\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 09:19:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

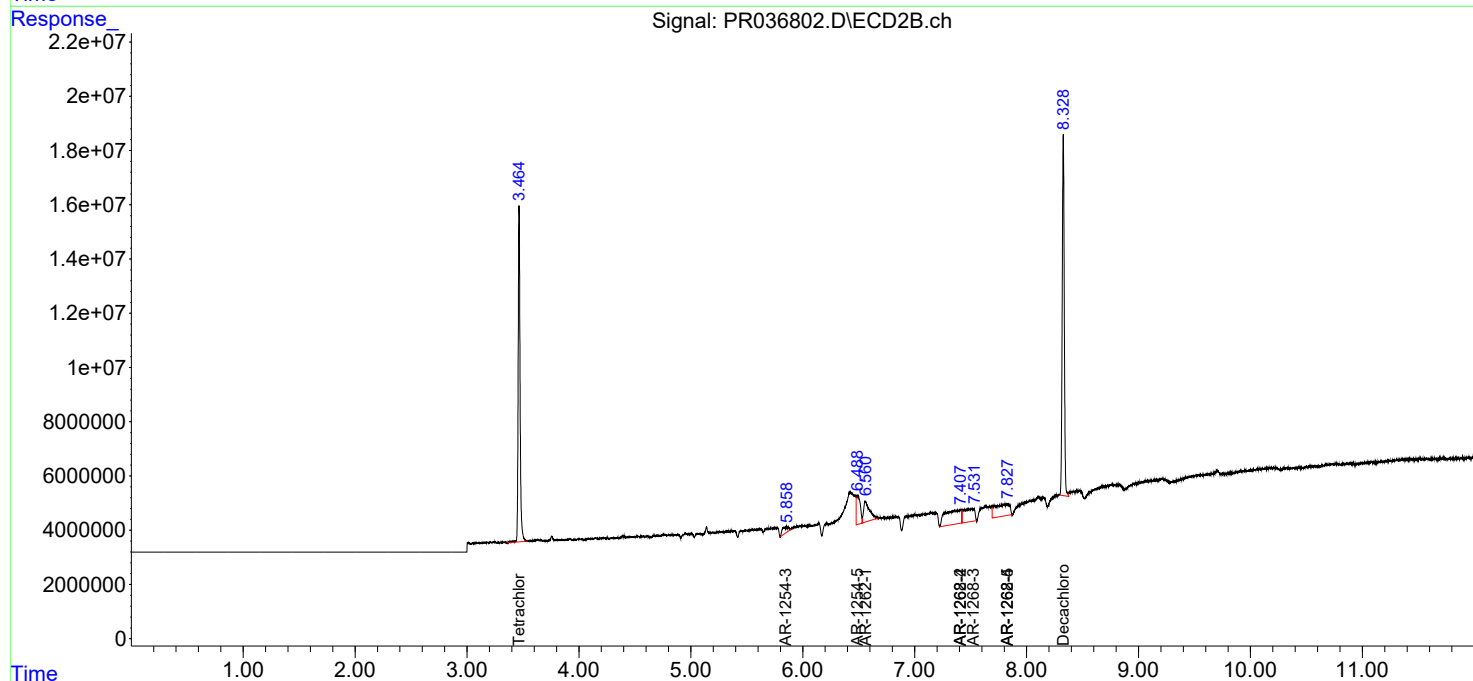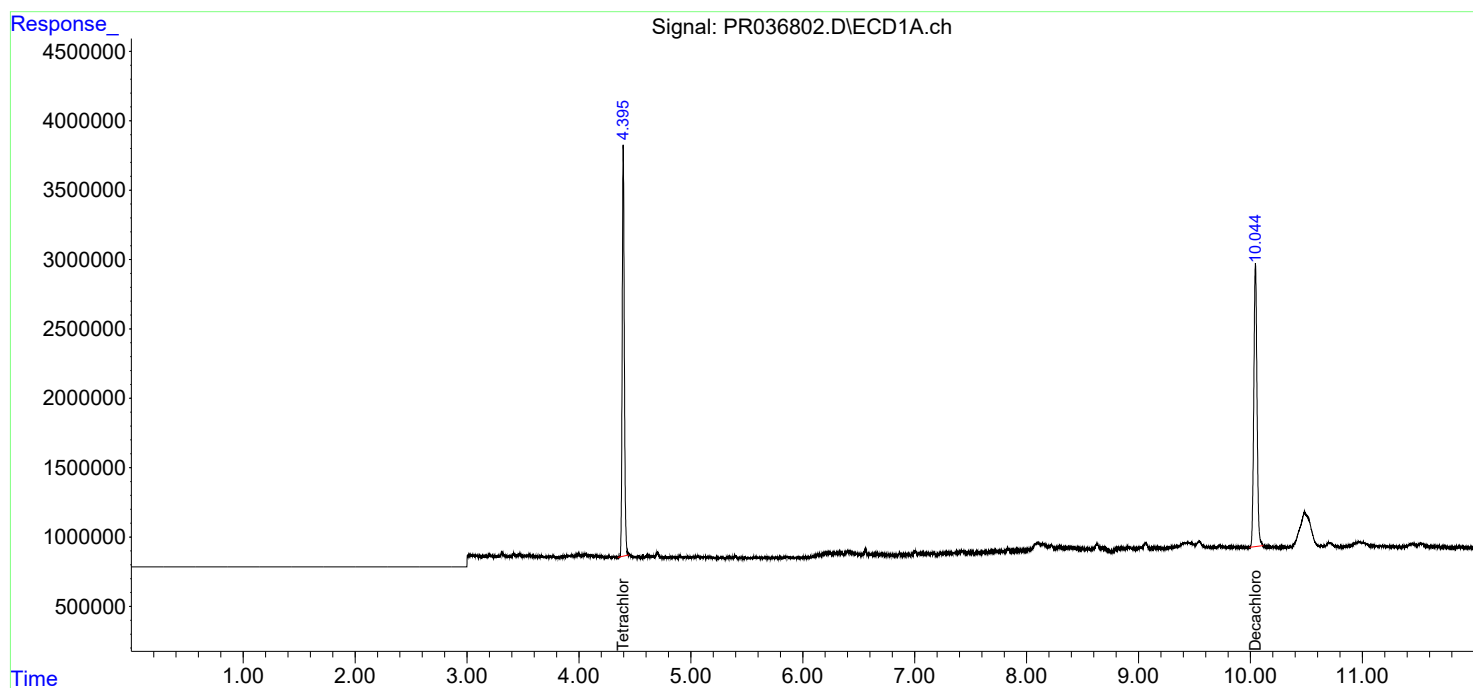


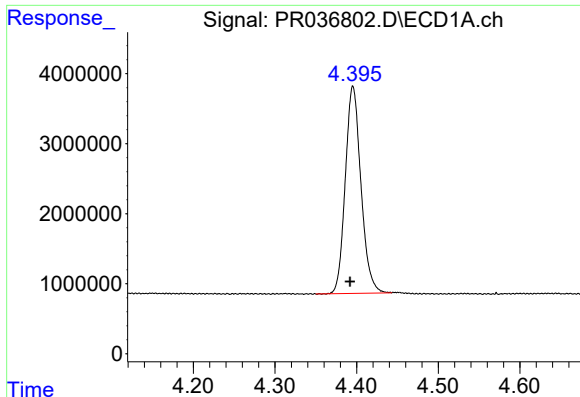

#1 Tetrachloro-m-xylene


R.T.: 4.396 min
Delta R.T.: 0.004 min
Response: 39460962
Conc: 24.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

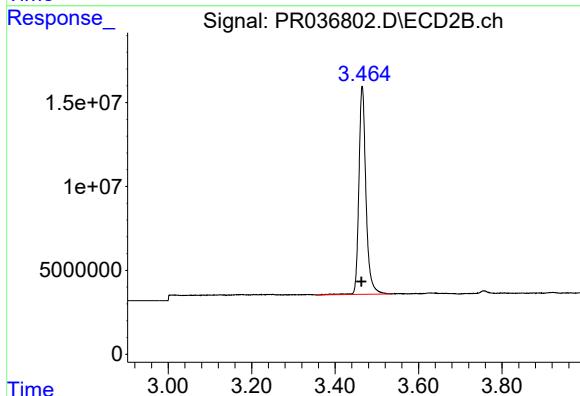


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.002 min
Response: 145738356
Conc: 24.88 ng/ml

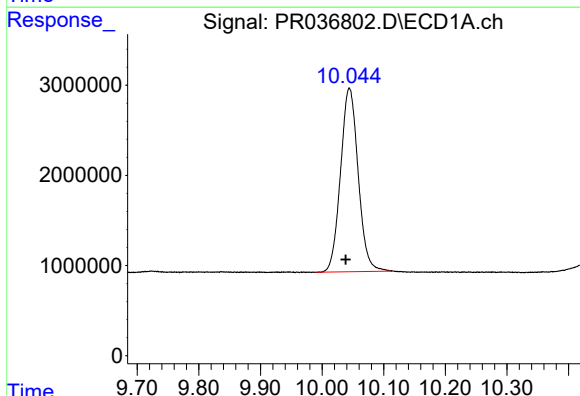


#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: 0.006 min
Response: 40488322
Conc: 21.61 ng/ml

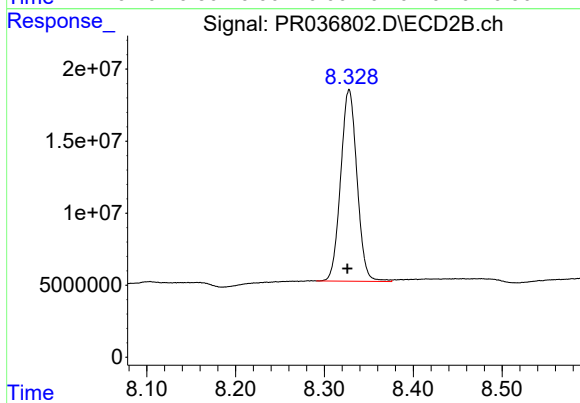

#2 Decachlorobiphenyl


R.T.: 8.328 min
Delta R.T.: 0.002 min
Response: 170030780
Conc: 21.30 ng/ml

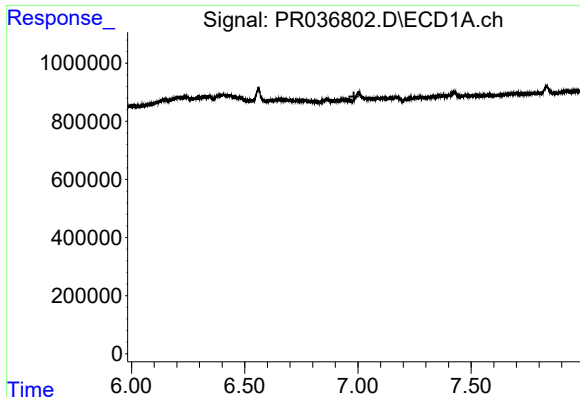

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.982 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

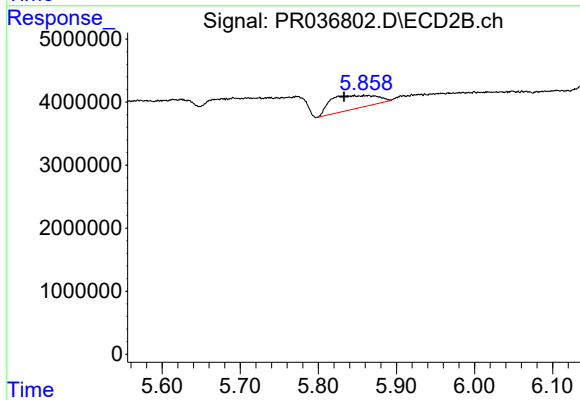


#28 AR-1254-3

R.T.: 5.846 min
Delta R.T.: 0.013 min
Response: 8815520
Conc: 17.33 ng/ml

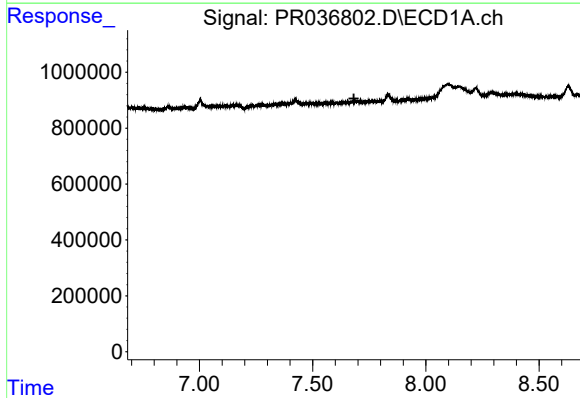


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.682 min
Response: 0
Conc: N.D.

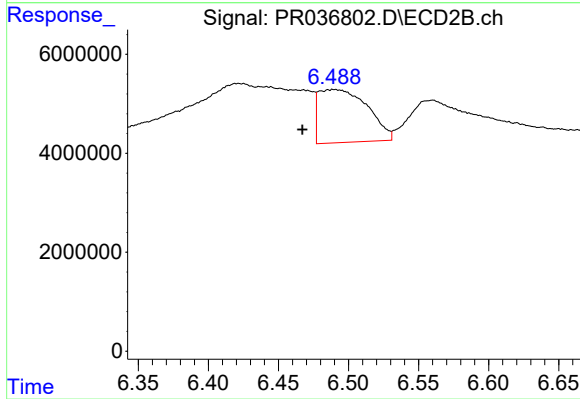

#30 AR-1254-5


R.T.: 6.490 min
Delta R.T.: 0.023 min
Response: 26046298
Conc: 51.23 ng/ml

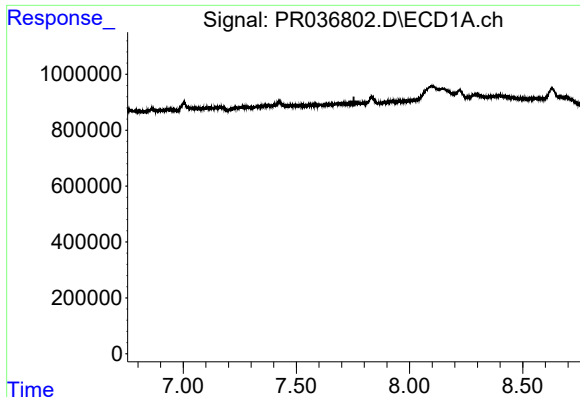

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.754 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

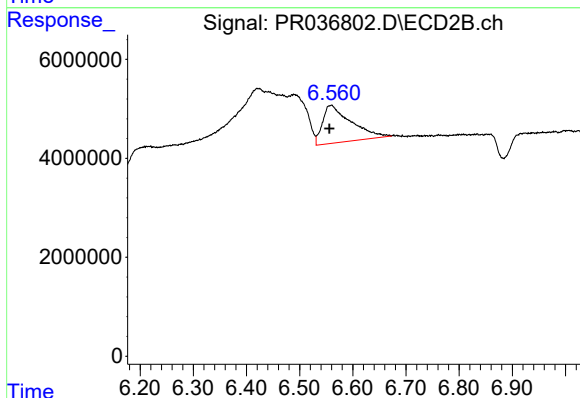


#36 AR-1262-1

R.T.: 6.560 min
Delta R.T.: 0.004 min
Response: 28328773
Conc: 103.35 ng/ml

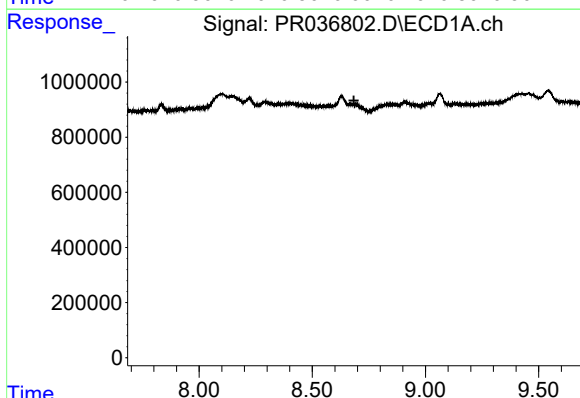


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.684 min
Response: 0
Conc: N.D.

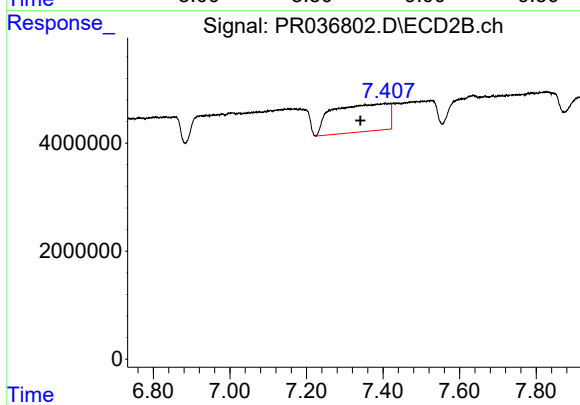

#39 AR-1262-4


R.T.: 7.406 min
Delta R.T.: 0.065 min
Response: 52037673
Conc: 56.65 ng/ml

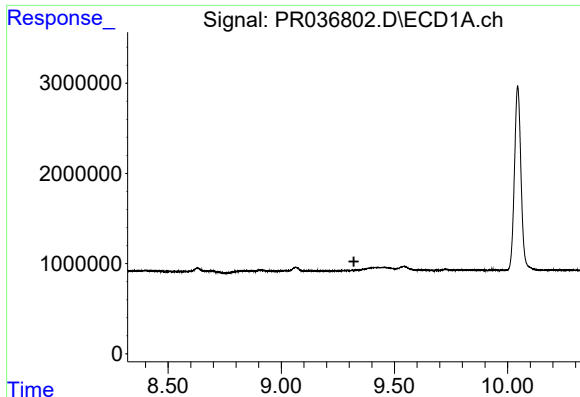

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

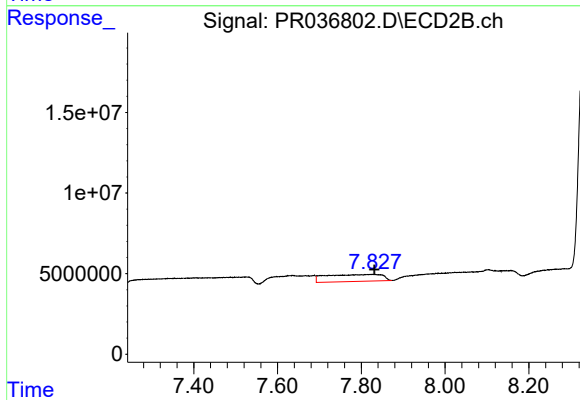


#40 AR-1262-5

R.T.: 7.827 min
Delta R.T.: -0.004 min
Response: 40310513
Conc: 100.36 ng/ml

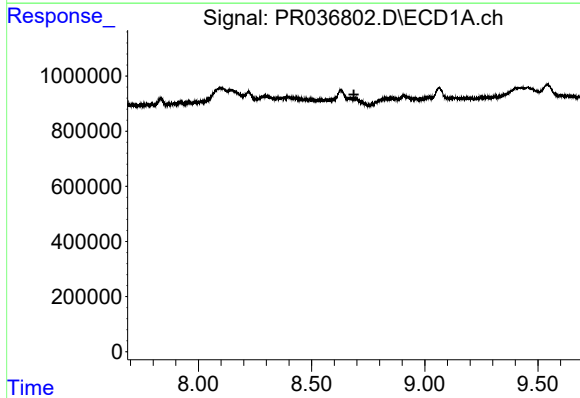


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.687 min
Response: 0
Conc: N.D.

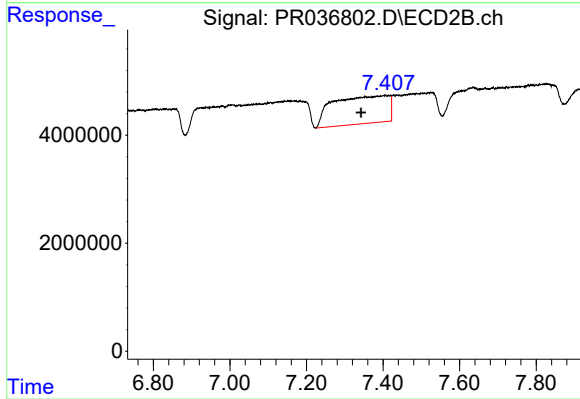

#42 AR-1268-2


R.T.: 7.406 min
Delta R.T.: 0.064 min
Response: 52037673
Conc: 41.45 ng/ml

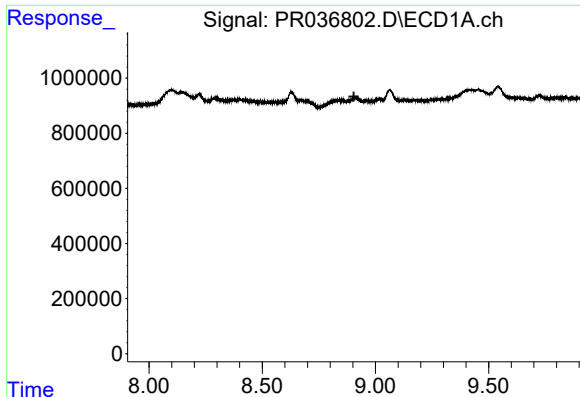

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

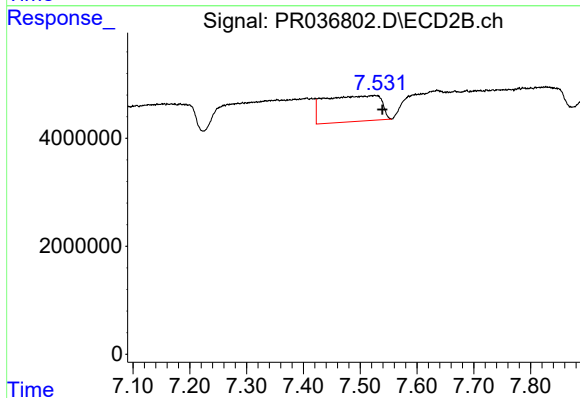


#43 AR-1268-3

R.T.: 7.525 min
Delta R.T.: -0.013 min
Response: 32975380
Conc: 33.90 ng/ml

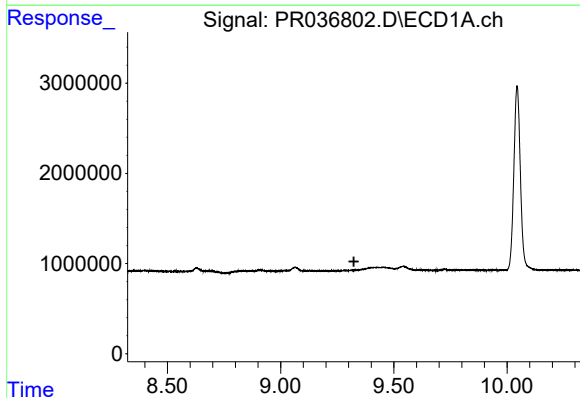

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.323 min
Response: 0
Conc: N.D.

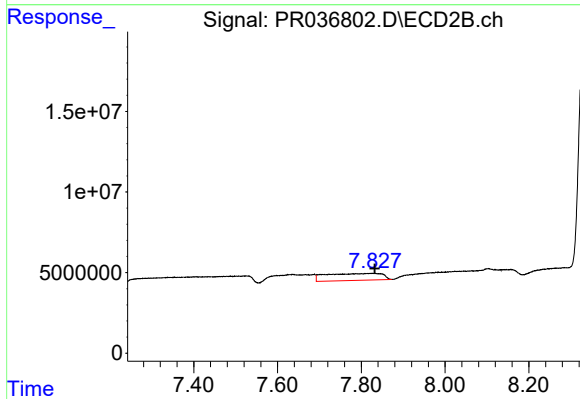

#44 AR-1268-4

R.T.: 7.827 min
Delta R.T.: -0.005 min
Response: 40310513
Conc: 92.80 ng/ml