

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040319\
 Data File : PR036806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 09:46
 Operator : SM\SJ
 Sample : K2138-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 S6A(12-20)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 10:56:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.393	3.465	30792207	118.2E6	19.328	20.176
2) SA Decachlor...	10.035	8.324	33560510	142.9E6	17.913	17.908
Target Compounds						
28) L6 AR-1254-3	0.000	5.833	0	2758326	N.D.	5.422 #
30) L6 AR-1254-5	0.000	6.501	0	36296015	N.D.	71.389 #
32) L7 AR-1260-2	0.000	6.139	0	29509116	N.D.	45.116 #
33) L7 AR-1260-3	0.000	6.325	0	28391474	N.D.	53.681 #
36) L8 AR-1262-1	0.000	6.501	0	36296015	N.D.	132.410 #
40) L8 AR-1262-5	0.000	7.841	0	41096611	N.D.	102.313 #
43) L9 AR-1268-3	0.000	7.527	0	71233075	N.D.	73.239 #
44) L9 AR-1268-4	0.000	7.841	0	41096611	N.D.	94.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040319\
Data File : PR036806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 09:46
Operator : SM\SJ
Sample : K2138-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 10:56:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

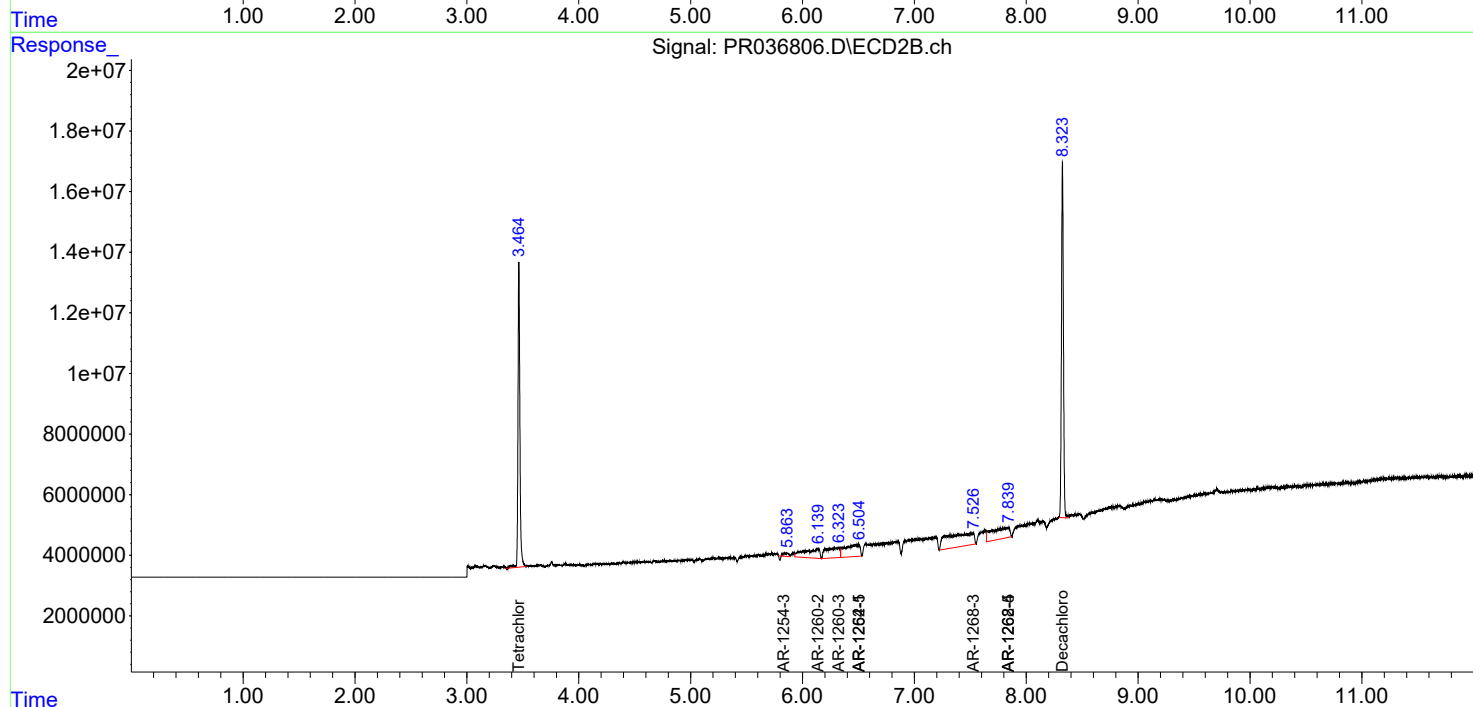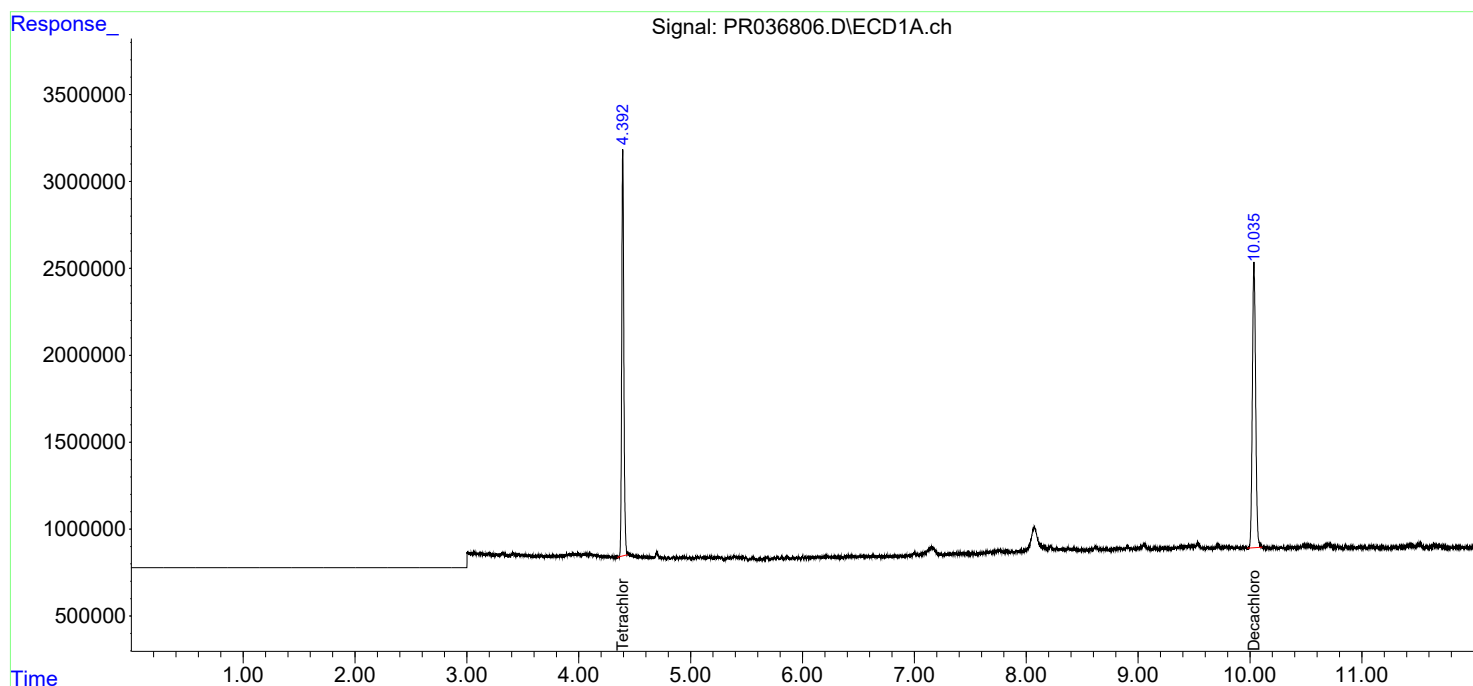


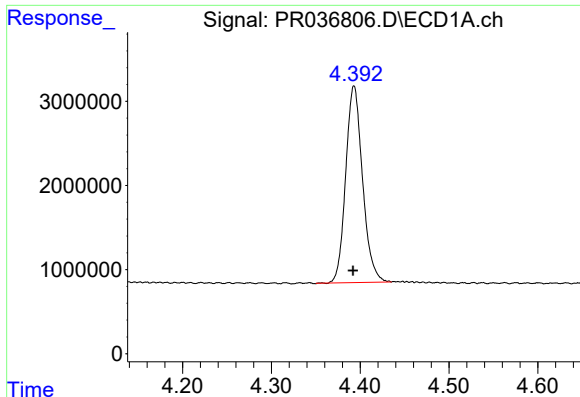

#1 Tetrachloro-m-xylene


R.T.: 4.393 min
Delta R.T.: 0.001 min
Response: 30792207
Conc: 19.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

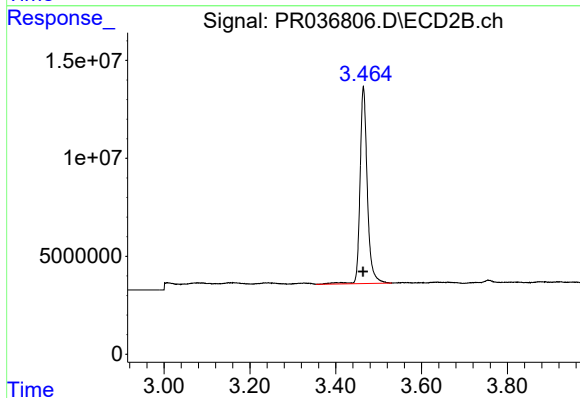


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 118189639
Conc: 20.18 ng/ml

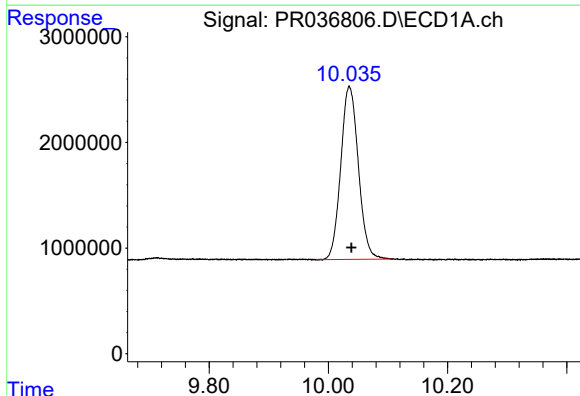


#2 Decachlorobiphenyl

R.T.: 10.035 min
Delta R.T.: -0.003 min
Response: 33560510
Conc: 17.91 ng/ml

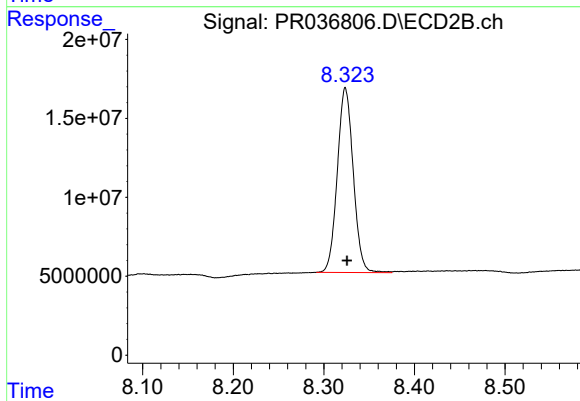

#2 Decachlorobiphenyl


R.T.: 8.324 min
Delta R.T.: -0.002 min
Response: 142944775
Conc: 17.91 ng/ml

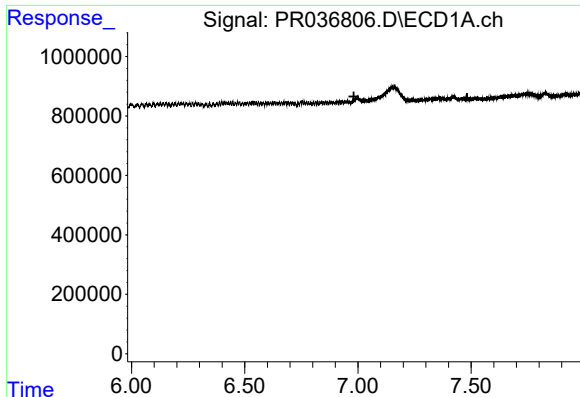

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.982 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

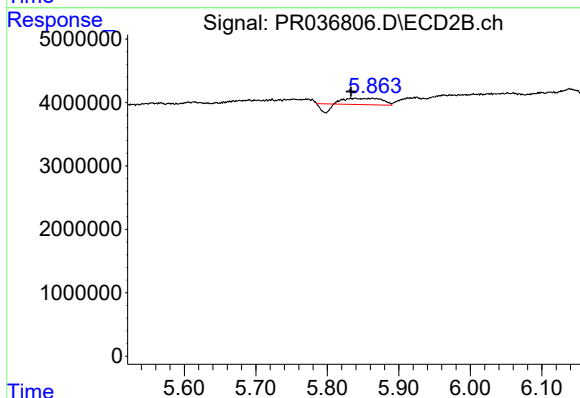


#28 AR-1254-3

R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 2758326
Conc: 5.42 ng/ml

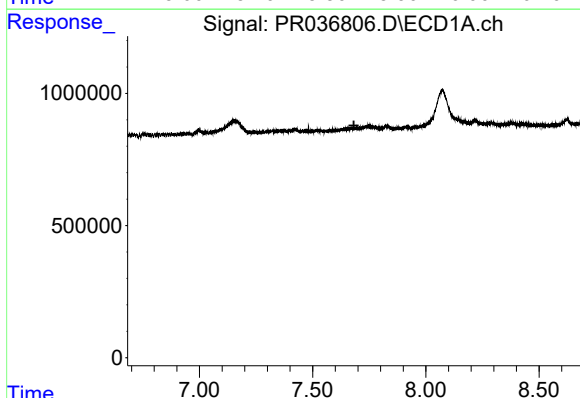


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.682 min
Response: 0
Conc: N.D.

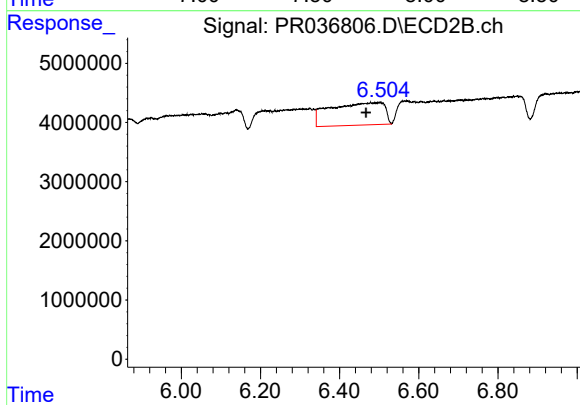

#30 AR-1254-5


R.T.: 6.501 min
Delta R.T.: 0.034 min
Response: 36296015
Conc: 71.39 ng/ml

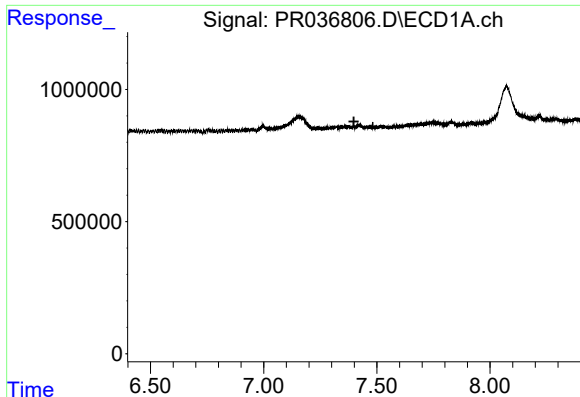

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

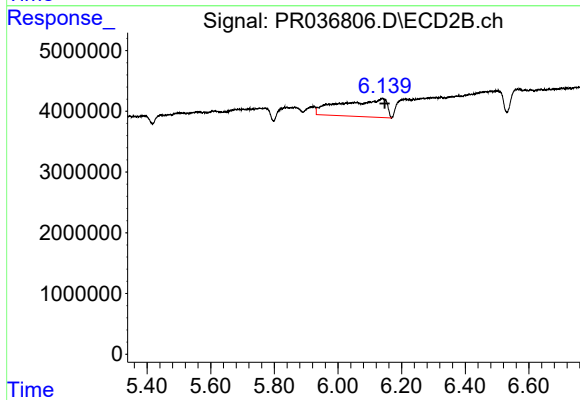


#32 AR-1260-2

R.T.: 6.139 min
Delta R.T.: -0.008 min
Response: 29509116
Conc: 45.12 ng/ml

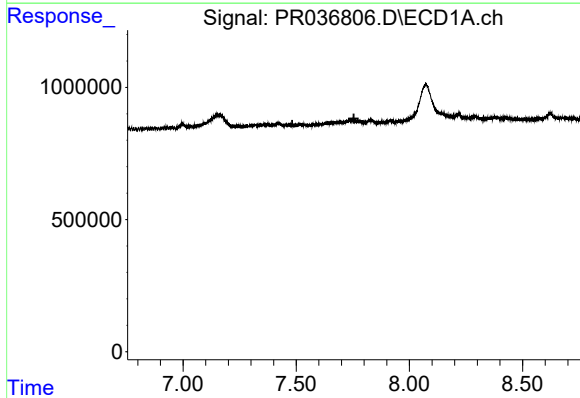


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.755 min
Response: 0
Conc: N.D.

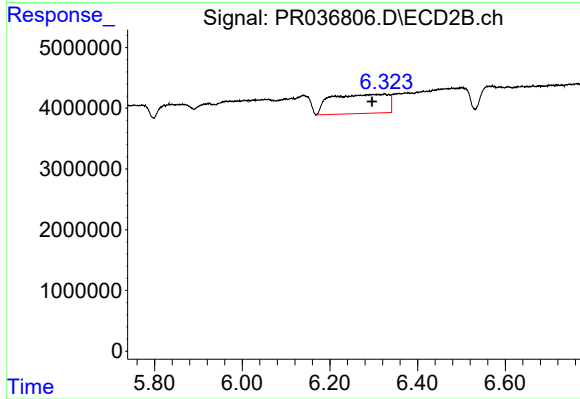

#33 AR-1260-3


R.T.: 6.325 min
Delta R.T.: 0.029 min
Response: 28391474
Conc: 53.68 ng/ml

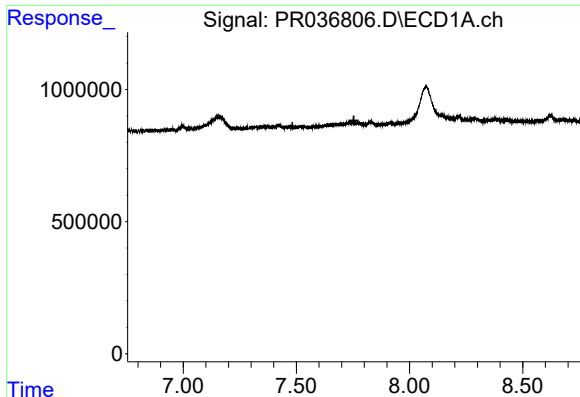

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.754 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

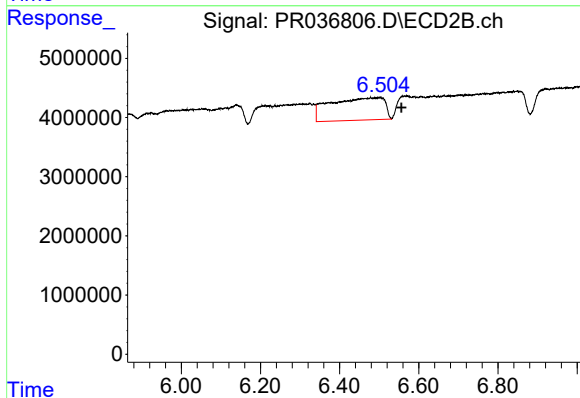


#36 AR-1262-1

R.T.: 6.501 min
Delta R.T.: -0.055 min
Response: 36296015
Conc: 132.41 ng/ml

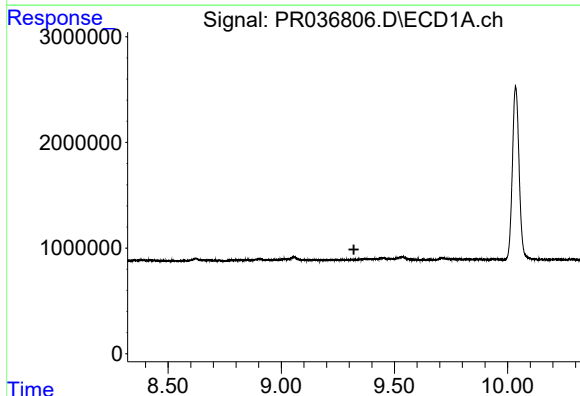


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.321 min
Response: 0
Conc: N.D.

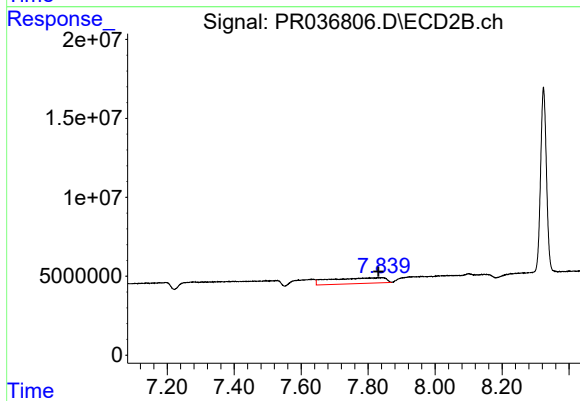

#40 AR-1262-5


R.T.: 7.841 min
Delta R.T.: 0.009 min
Response: 41096611
Conc: 102.31 ng/ml

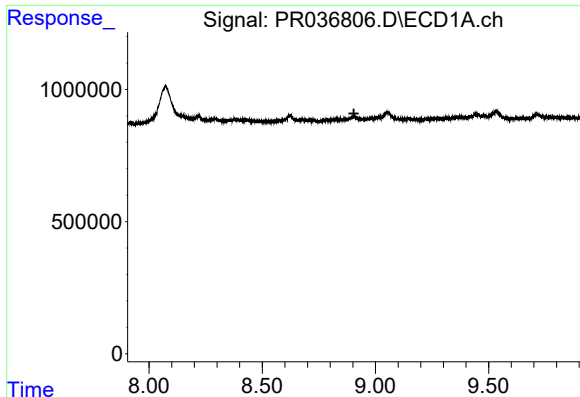

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
S6A(12-20)COMP

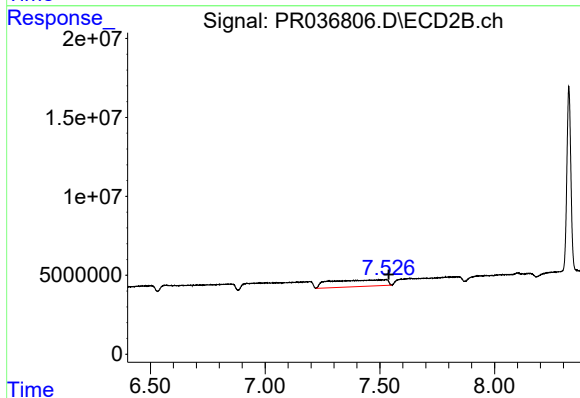


#43 AR-1268-3

R.T.: 7.527 min
Delta R.T.: -0.012 min
Response: 71233075
Conc: 73.24 ng/ml

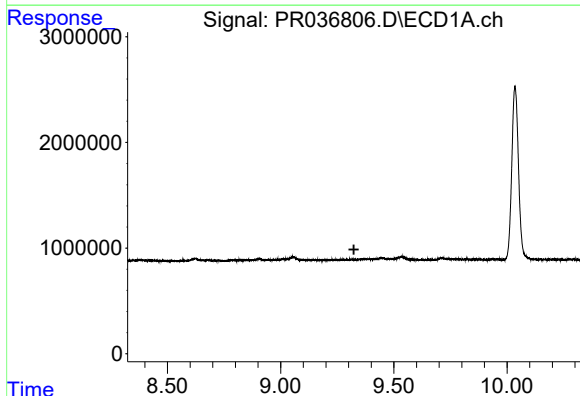

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.323 min
Response: 0
Conc: N.D.

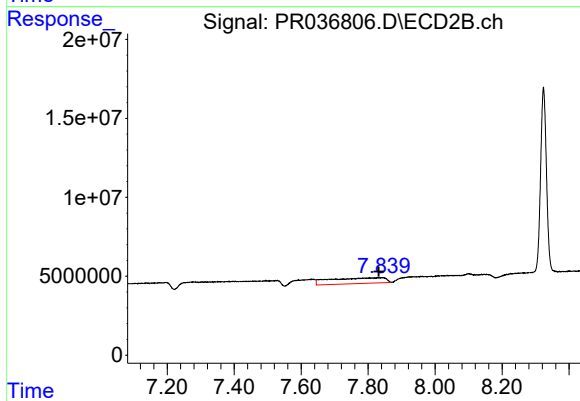

#44 AR-1268-4

R.T.: 7.841 min
Delta R.T.: 0.008 min
Response: 41096611
Conc: 94.61 ng/ml