

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040519\
 Data File : PR036960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 19:47
 Operator : SM\SJ
 Sample : K2257-33
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 RO-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 01:25:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.397	3.469	20922365	77910401	13.133	13.300
2)	SA Decachlor...	10.036	8.323	30164975	125.7E6	16.101	15.746
Target Compounds							
10)	L2 AR-1221-3	0.000	3.890	0	6875742	N.D.	45.672 #
11)	L3 AR-1232-1	0.000	3.890	0	6875742	N.D.	72.723 #
35)	L7 AR-1260-5	0.000	7.000	0	4918039	N.D.	3.694 #
37)	L8 AR-1262-2	0.000	7.000	0	4918039	N.D.	3.588 #
38)	L8 AR-1262-3	0.000	7.338	0	4987166	N.D.	9.136 #
39)	L8 AR-1262-4	0.000	7.338	0	4987166	N.D.	5.429 #
41)	L9 AR-1268-1	0.000	7.338	0	4987166	N.D.	3.370 #
42)	L9 AR-1268-2	0.000	7.338	0	4987166	N.D.	3.972 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040519\
Data File : PR036960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 19:47
Operator : SM\SJ
Sample : K2257-33
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
RO-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 01:25:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

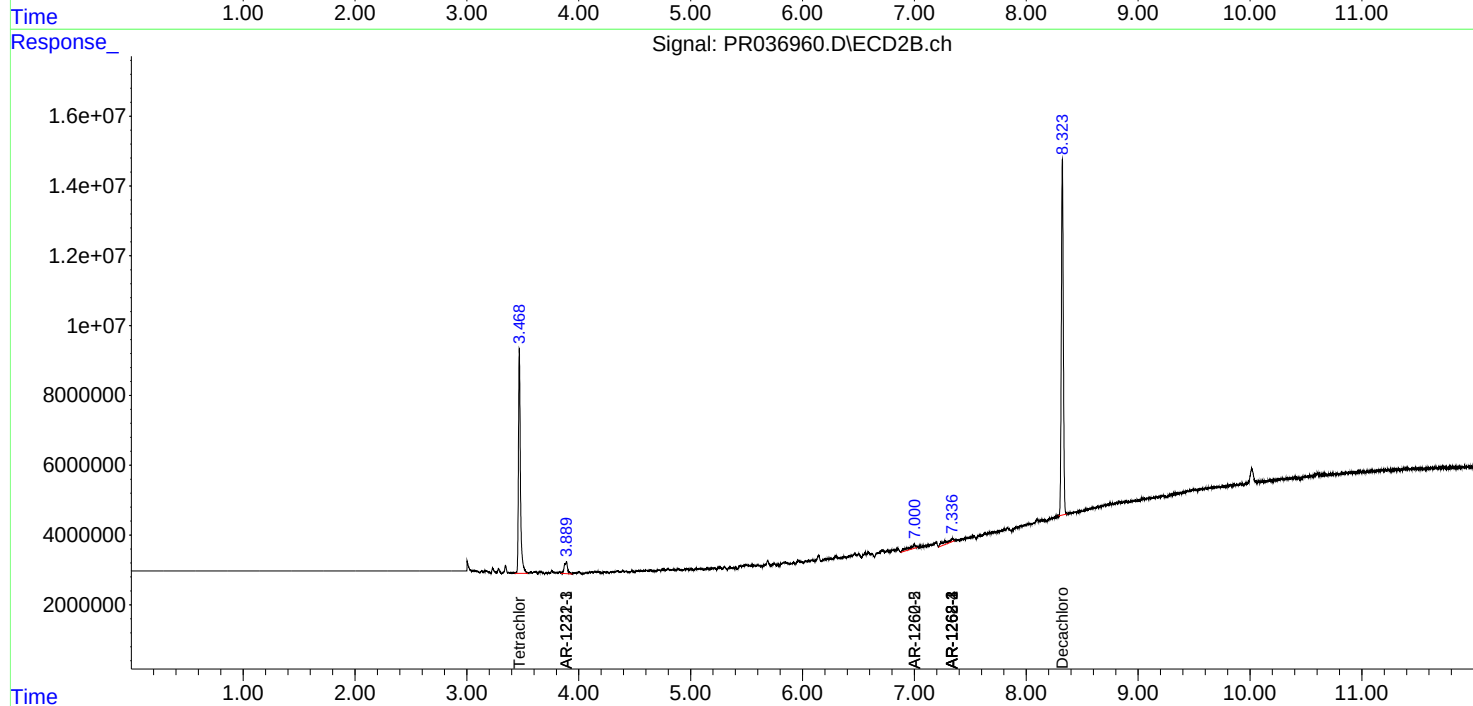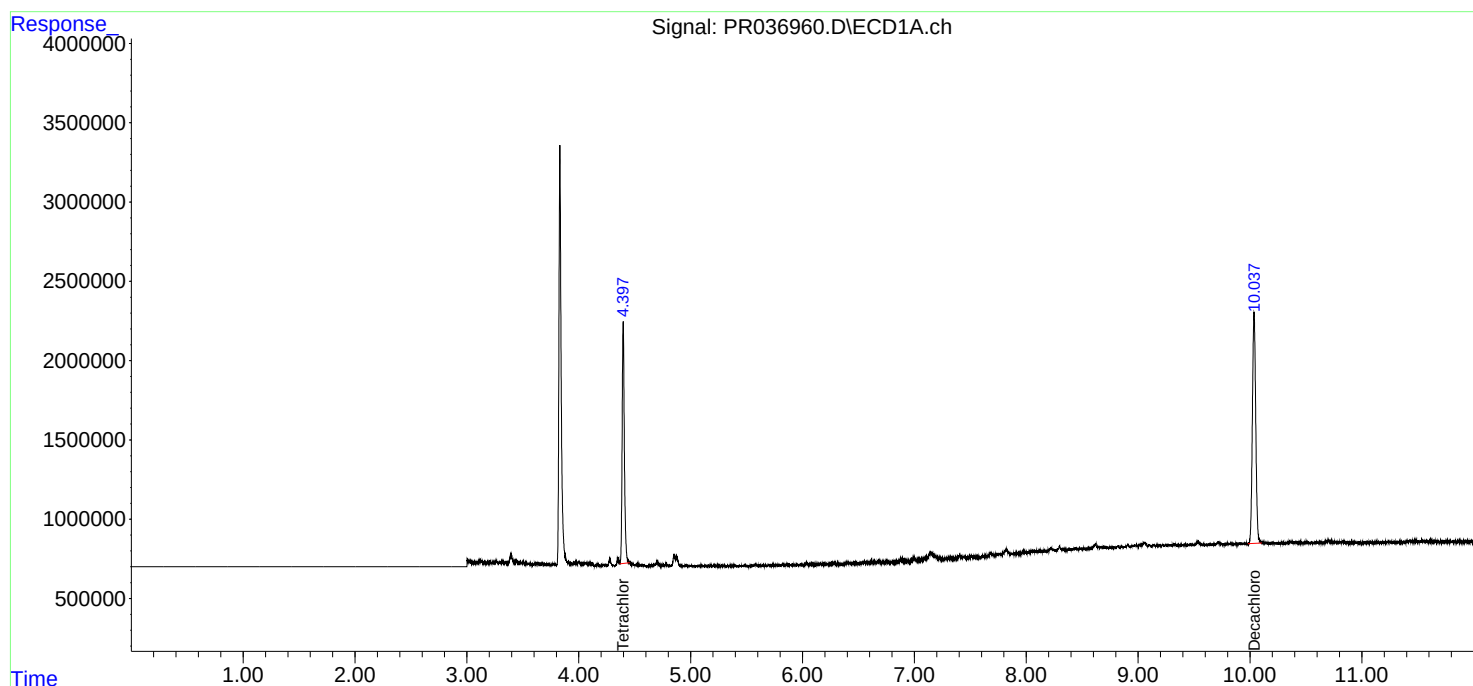


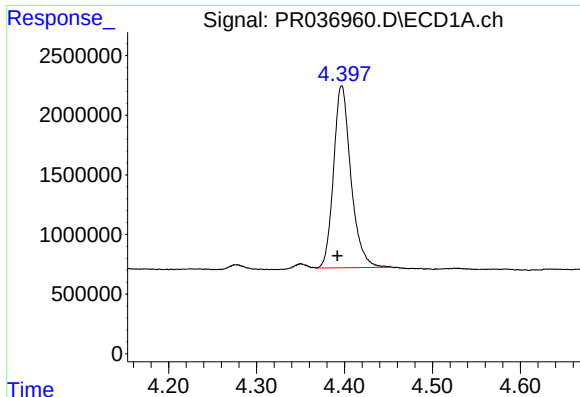

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.005 min
Response: 20922365
Conc: 13.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
RO-20

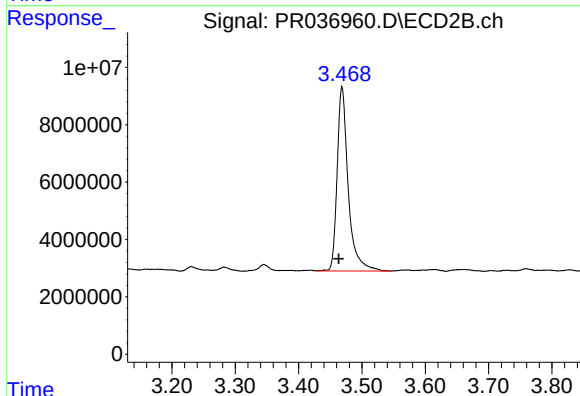


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.005 min
Response: 77910401
Conc: 13.30 ng/ml

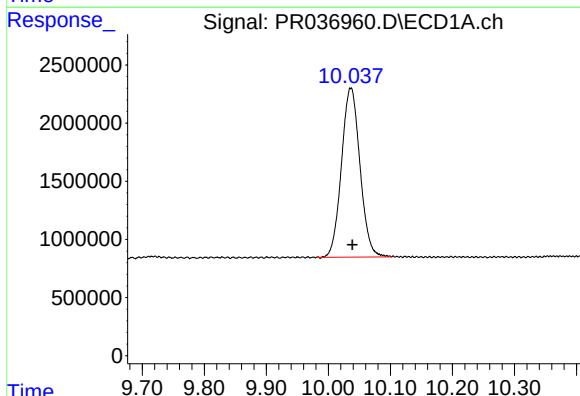


#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: -0.002 min
Response: 30164975
Conc: 16.10 ng/ml

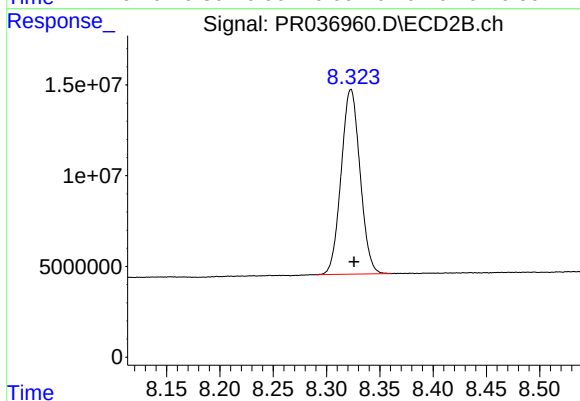

#2 Decachlorobiphenyl


R.T.: 8.323 min
Delta R.T.: -0.003 min
Response: 125689554
Conc: 15.75 ng/ml

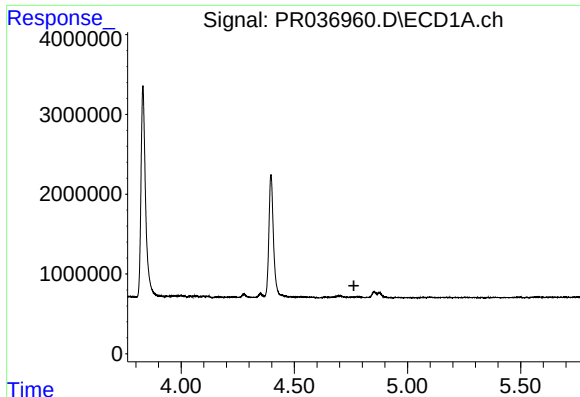

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
RO-20

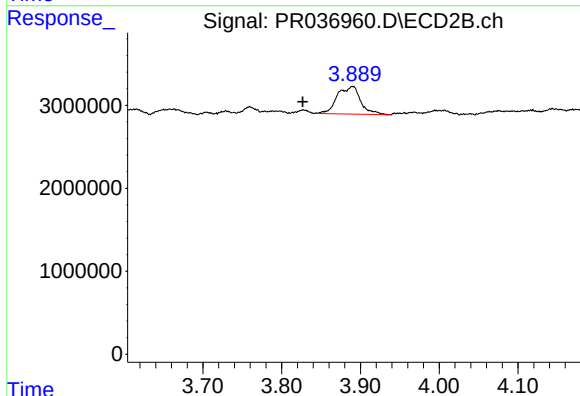


#10 AR-1221-3

R.T.: 3.890 min
Delta R.T.: 0.063 min
Response: 6875742
Conc: 45.67 ng/ml

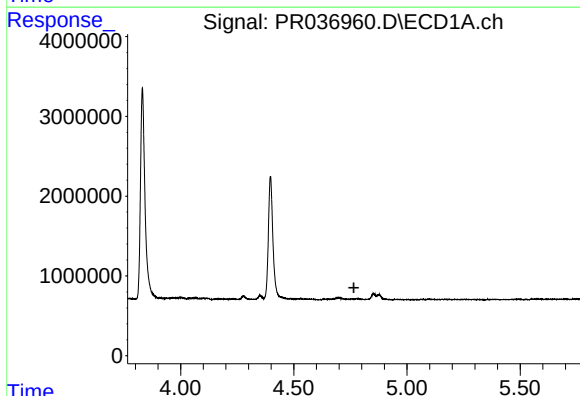


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.766 min
Response: 0
Conc: N.D.

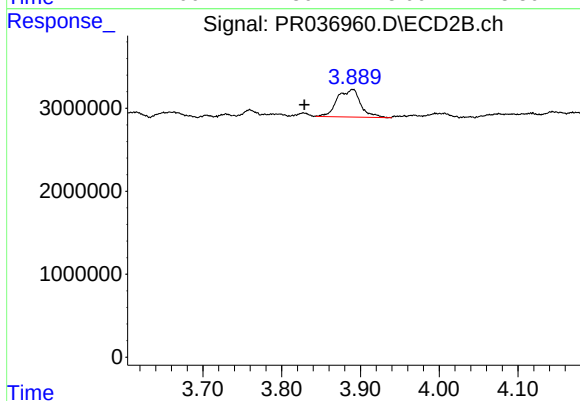

#11 AR-1232-1


R.T.: 3.890 min
Delta R.T.: 0.061 min
Response: 6875742
Conc: 72.72 ng/ml

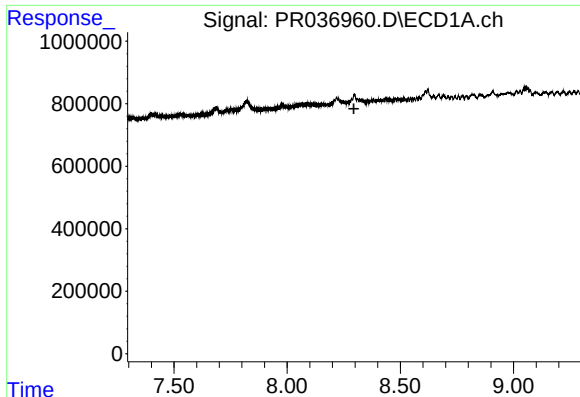

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
RO-20

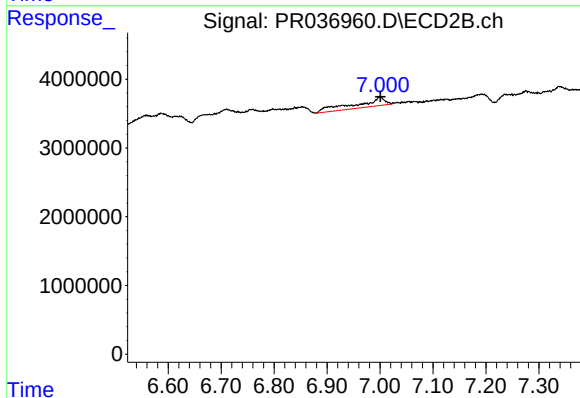


#35 AR-1260-5

R.T.: 7.000 min
Delta R.T.: 0.000 min
Response: 4918039
Conc: 3.69 ng/ml

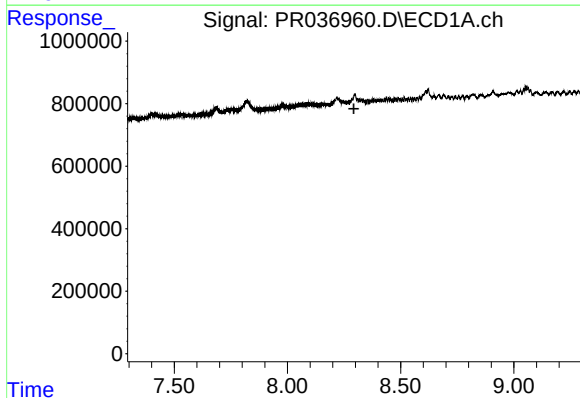


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.294 min
Response: 0
Conc: N.D.

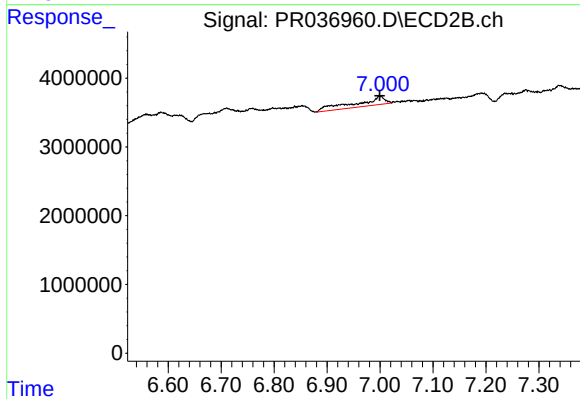

#37 AR-1262-2


R.T.: 7.000 min
Delta R.T.: 0.000 min
Response: 4918039
Conc: 3.59 ng/ml

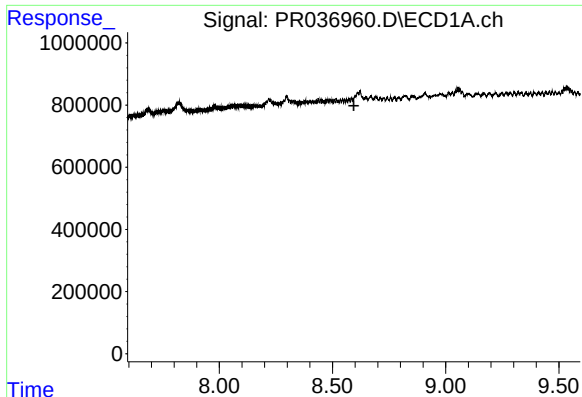

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
RO-20

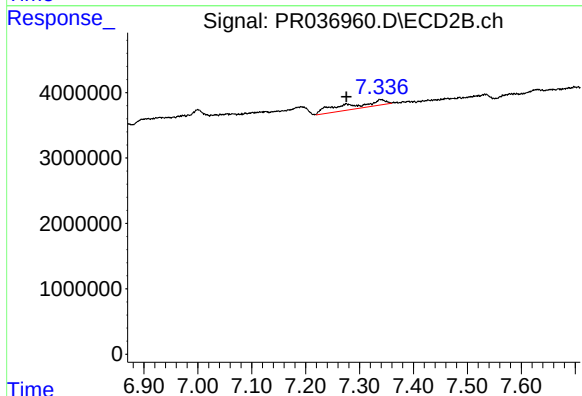


#38 AR-1262-3

R.T.: 7.338 min
Delta R.T.: 0.062 min
Response: 4987166
Conc: 9.14 ng/ml

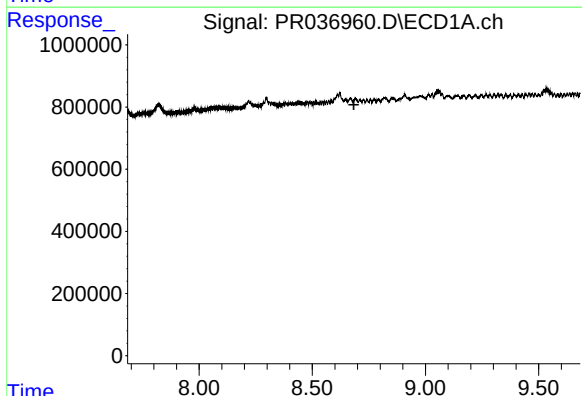


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.684 min
Response: 0
Conc: N.D.

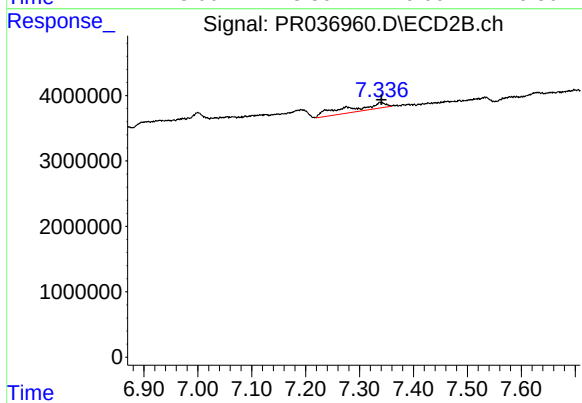

#39 AR-1262-4


R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 4987166
Conc: 5.43 ng/ml

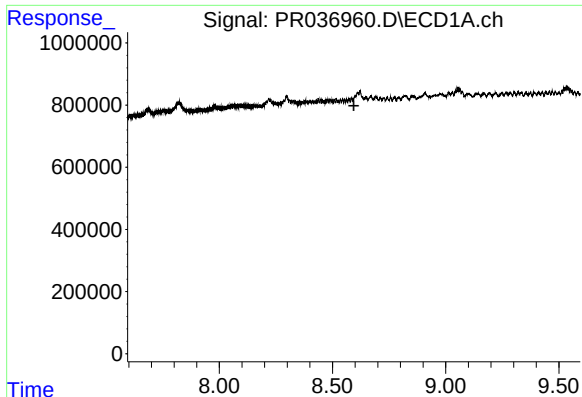

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
RO-20

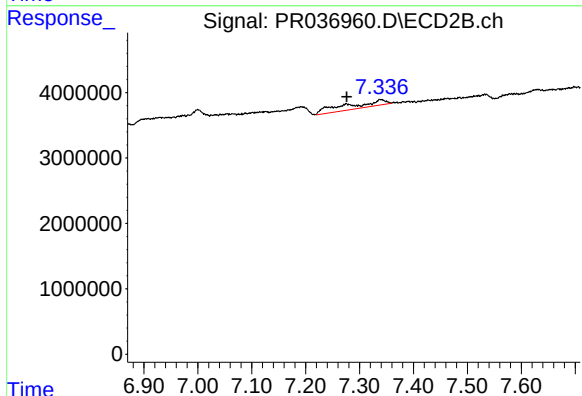


#41 AR-1268-1

R.T.: 7.338 min
Delta R.T.: 0.062 min
Response: 4987166
Conc: 3.37 ng/ml

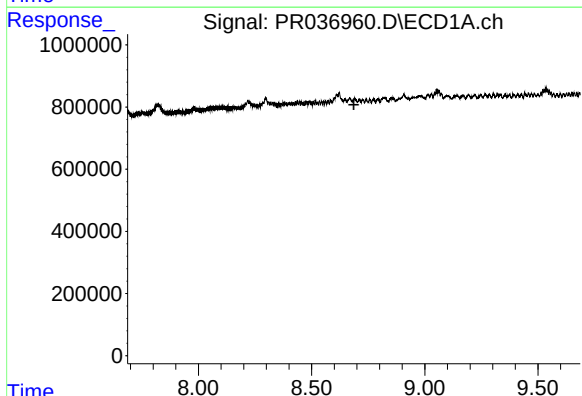

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.687 min
Response: 0
Conc: N.D.

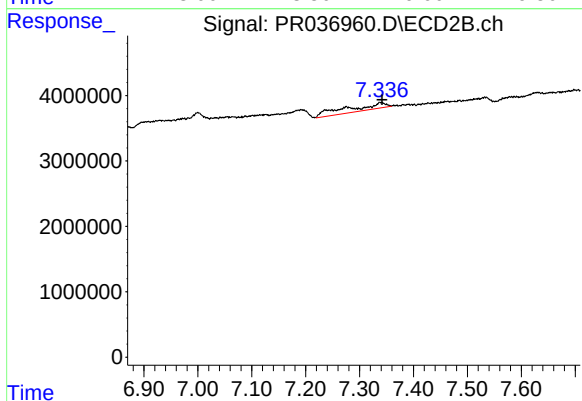

#42 AR-1268-2

R.T.: 7.338 min
Delta R.T.: -0.004 min
Response: 4987166
Conc: 3.97 ng/ml