

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
 Data File : PR037025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 18:54
 Operator : SM\SJ
 Sample : K1560-07
 Misc : AR1660 LOD 25PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 03:48:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.471	34409610	138.5E6	21.598	23.639
2)	SA Decachlor...	10.035	8.322	46297847	211.3E6	24.711	26.468
Target Compounds							
3)	L1 AR-1016-1	0.000	4.518	0	7350983	N.D.	30.440 #
4)	L1 AR-1016-2	0.000	4.534	0	11707404	N.D.	29.988 #
5)	L1 AR-1016-3	0.000	4.704	0	6190461	N.D.	31.737 #
6)	L1 AR-1016-4	0.000	4.745	0	3949253	N.D.	26.007 #
7)	L1 AR-1016-5	0.000	4.952	0	6672007	N.D.	32.104 #
10)	L2 AR-1221-3	0.000	3.832	0	3237329	N.D.	21.504 #
11)	L3 AR-1232-1	0.000	3.832	0	3237329	N.D.	34.240 #
12)	L3 AR-1232-2	0.000	4.534	0	11707404	N.D.	98.015 #
13)	L3 AR-1232-3	0.000	4.704	0	6190461	N.D.	107.741 #
14)	L3 AR-1232-4	0.000	4.785	0	4277222	N.D.	86.466 #
15)	L3 AR-1232-5	0.000	4.952	0	6672007	N.D.	116.415 #
16)	L4 AR-1242-1	0.000	4.518	0	7350983	N.D.	64.332 #
17)	L4 AR-1242-2	0.000	4.534	0	11707404	N.D.	61.557 #
18)	L4 AR-1242-3	0.000	4.704	0	6190461	N.D.	64.745 #
19)	L4 AR-1242-4	0.000	4.785	0	4277222	N.D.	47.373 #
20)	L4 AR-1242-5	0.000	5.294	0	5978144	N.D.	43.303 #
21)	L5 AR-1248-1	0.000	4.518	0	7350983	N.D.	75.695 #
22)	L5 AR-1248-2	0.000	4.745	0	3949253	N.D.	29.246 #
23)	L5 AR-1248-3	0.000	4.785	0	4277222	N.D.	30.733 #
24)	L5 AR-1248-4	0.000	4.952	0	6672007	N.D.	37.831 #
25)	L5 AR-1248-5	0.000	5.294	0	5978144	N.D.	30.750 #
26)	L6 AR-1254-1	0.000	5.294	0	5978144	N.D.	18.177 #
27)	L6 AR-1254-2	0.000	5.439	0	5498557	N.D.	18.573 #
28)	L6 AR-1254-3	0.000	5.846	0	10734011	N.D.	21.100 #
29)	L6 AR-1254-4	0.000	6.086	0	5350508	N.D.	13.962 #
30)	L6 AR-1254-5	7.681	6.465	4286747	25502141	41.960	50.159
31)	L7 AR-1260-1	7.142	5.958	3490672	14944540	34.250	34.169
32)	L7 AR-1260-2	7.398	6.144	4311968	26272690	35.140	40.168
33)	L7 AR-1260-3	7.754	6.294	2870691	26282929	29.905	49.694 #
34)	L7 AR-1260-4	7.980	6.756	4343156	18496945	39.194	39.664
35)	L7 AR-1260-5	8.294	6.998	6981807	41829343	32.047	31.415
36)	L8 AR-1262-1	7.754	6.555	2870691	12018396	24.480	43.844 #
37)	L8 AR-1262-2	8.294	6.998	6981807	41829343	32.377	30.518
38)	L8 AR-1262-3	8.615	7.274	4392997	17712910	30.074	32.449
39)	L8 AR-1262-4	8.615	7.339	4392997	31077568	40.095	33.832
40)	L8 AR-1262-5	0.000	7.830	0	14344556	N.D.	35.712 #
41)	L9 AR-1268-1	8.615	7.274	4392997	17712910	18.787	11.968 #
42)	L9 AR-1268-2	0.000	7.339	0	31077568	N.D.	24.755 #
44)	L9 AR-1268-4	0.000	7.830	0	14344556	N.D.	33.023 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
 Data File : PR037025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 18:54
 Operator : SM\SJ
 Sample : K1560-07
 Misc : AR1660 LOD 25PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 03:48:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.097	0	4039320	N.D.	1.338 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
Data File : PR037025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2019 18:54
Operator : SM\SJ
Sample : K1560-07
Misc : AR1660 LOD 25PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 03:48:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

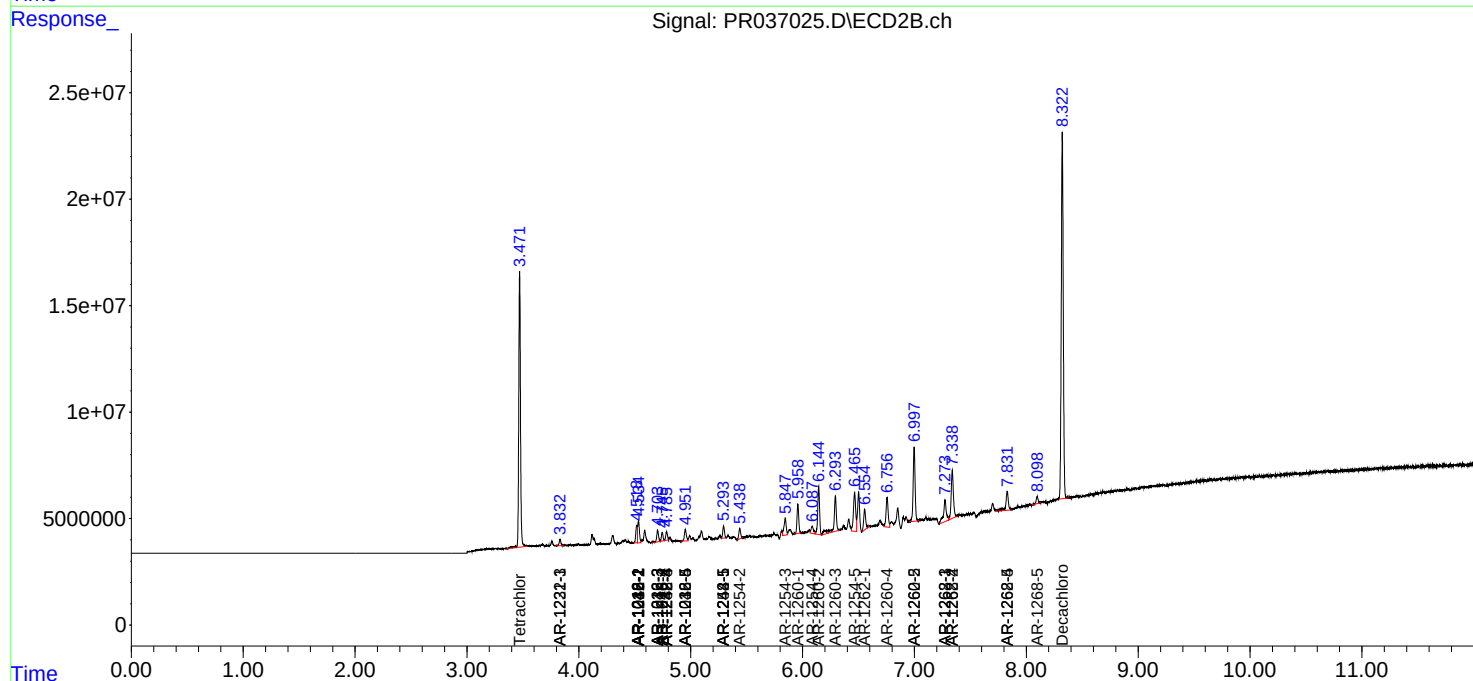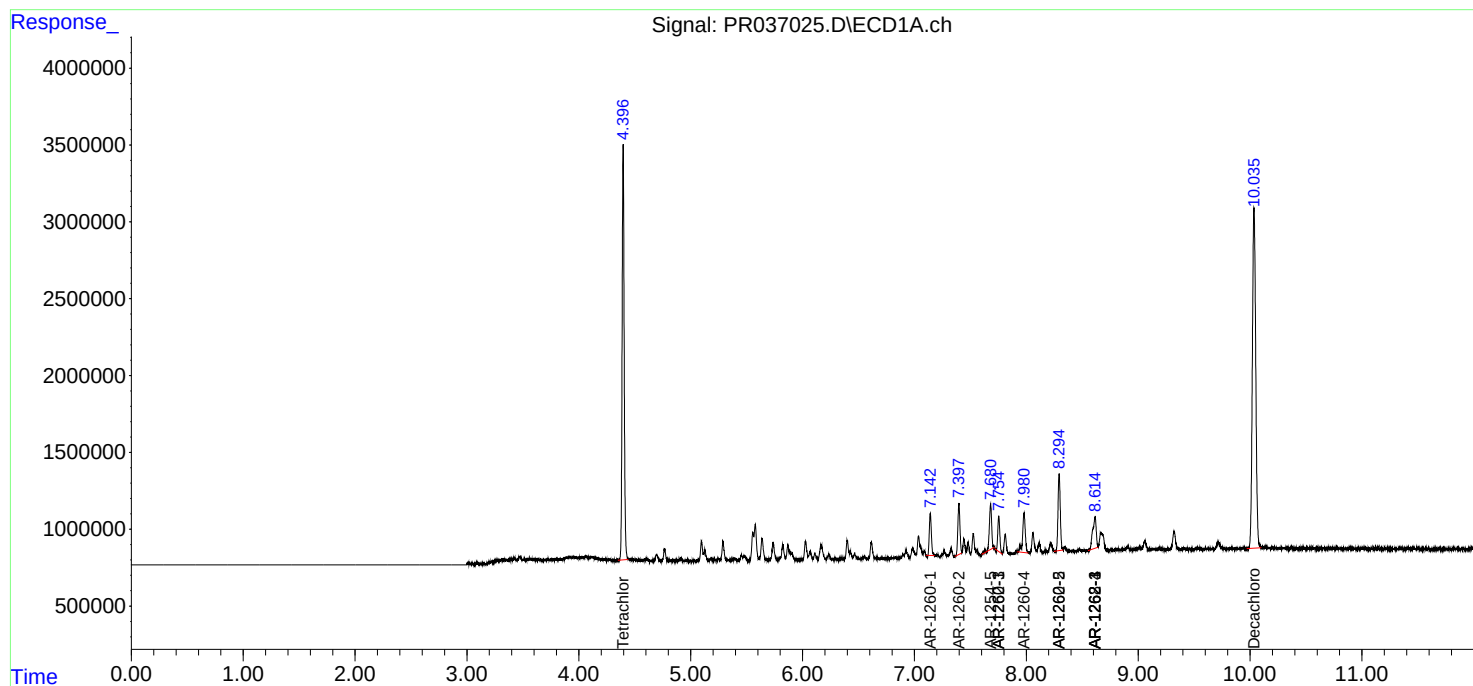


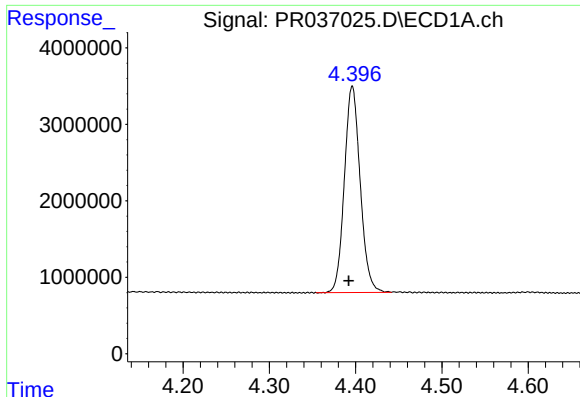

#1 Tetrachloro-m-xylene


R.T.: 4.396 min
Delta R.T.: 0.004 min
Response: 34409610
Conc: 21.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

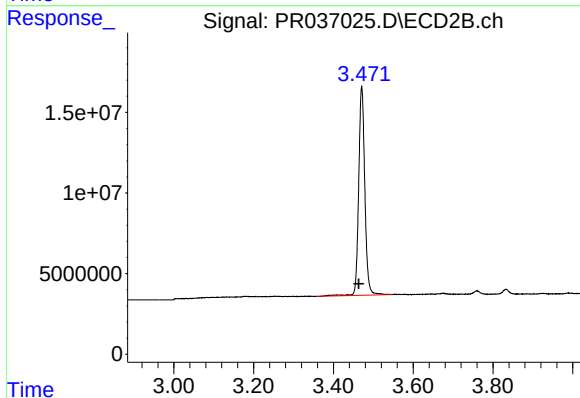


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.007 min
Response: 138475795
Conc: 23.64 ng/ml

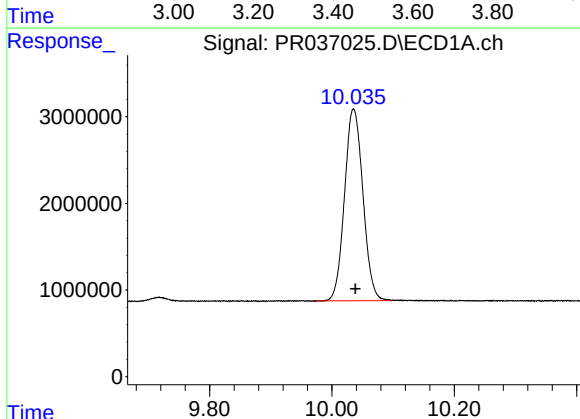


#2 Decachlorobiphenyl

R.T.: 10.035 min
Delta R.T.: -0.003 min
Response: 46297847
Conc: 24.71 ng/ml

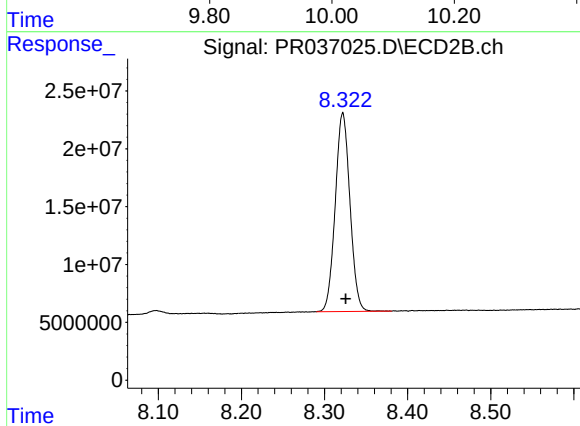

#2 Decachlorobiphenyl


R.T.: 8.322 min
Delta R.T.: -0.004 min
Response: 211277260
Conc: 26.47 ng/ml

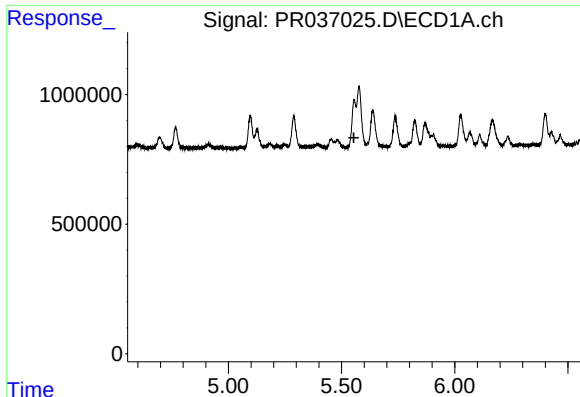

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

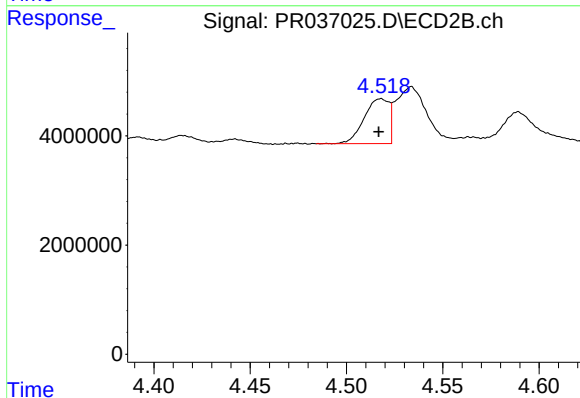


#3 AR-1016-1

R.T.: 4.518 min
Delta R.T.: 0.001 min
Response: 7350983
Conc: 30.44 ng/ml

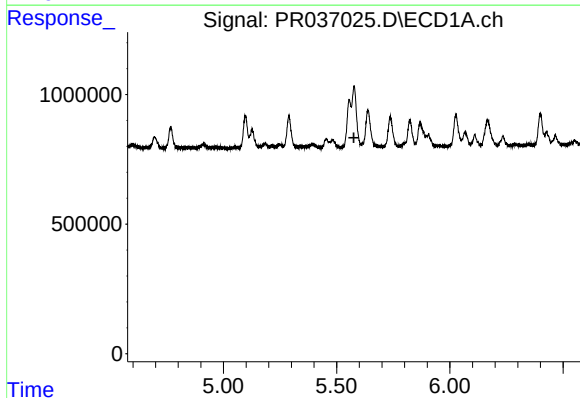


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.576 min
Response: 0
Conc: N.D.

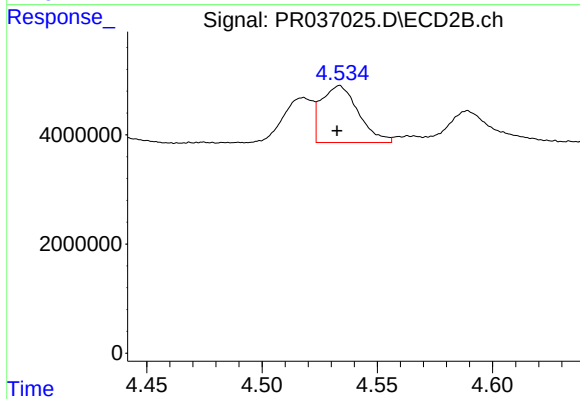

#4 AR-1016-2


R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 11707404
Conc: 29.99 ng/ml

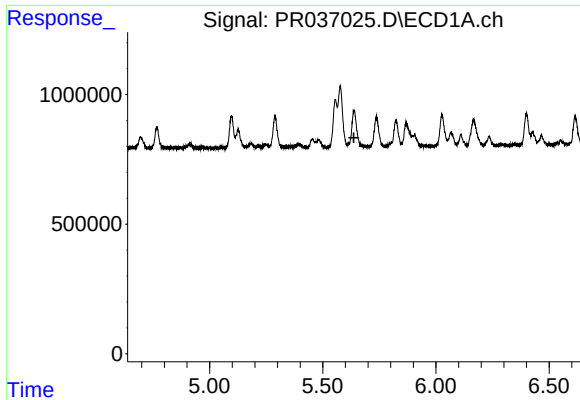

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.638 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

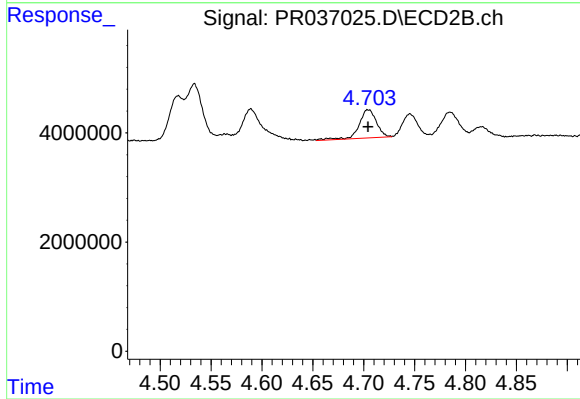


#5 AR-1016-3

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 6190461
Conc: 31.74 ng/ml

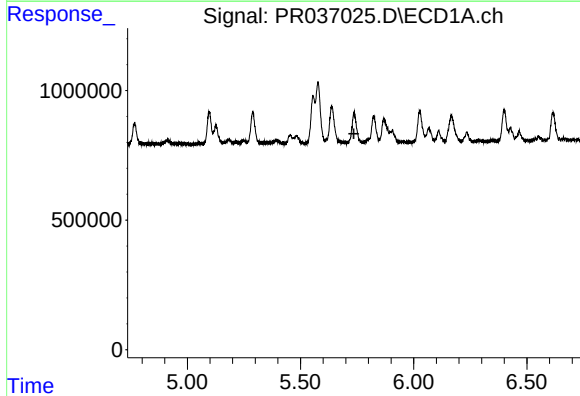


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

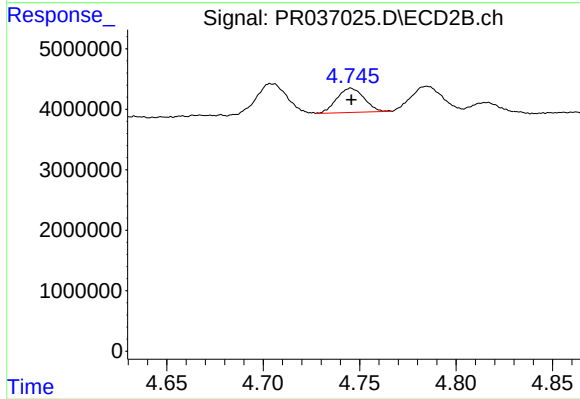

#6 AR-1016-4


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 3949253
Conc: 26.01 ng/ml

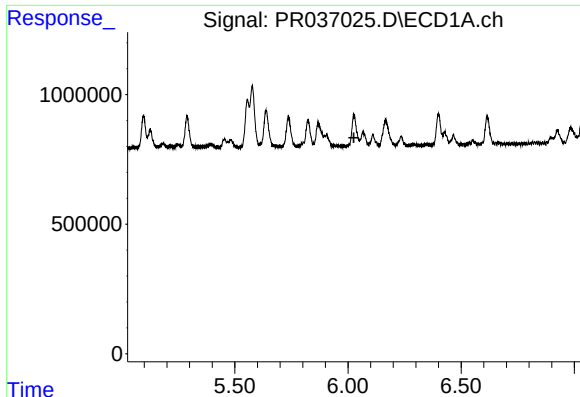

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

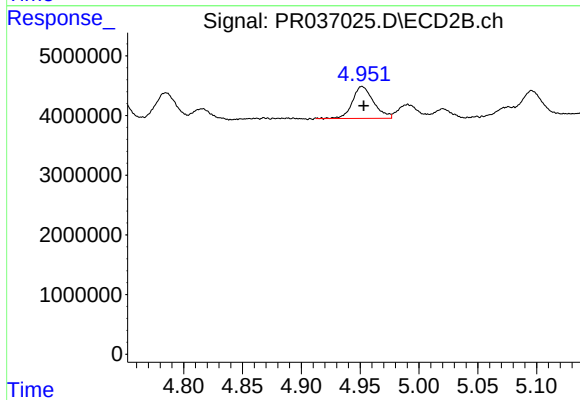


#7 AR-1016-5

R.T.: 4.952 min
Delta R.T.: -0.001 min
Response: 6672007
Conc: 32.10 ng/ml

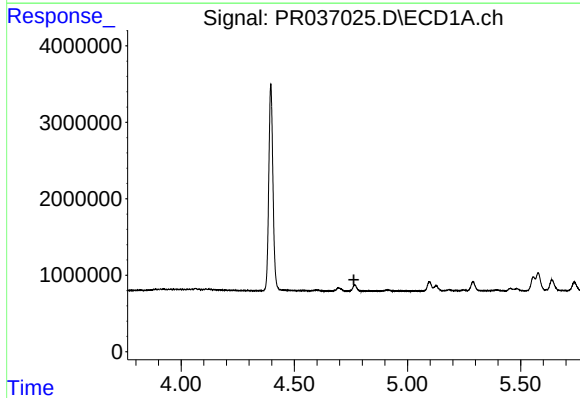


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.763 min
Response: 0
Conc: N.D.

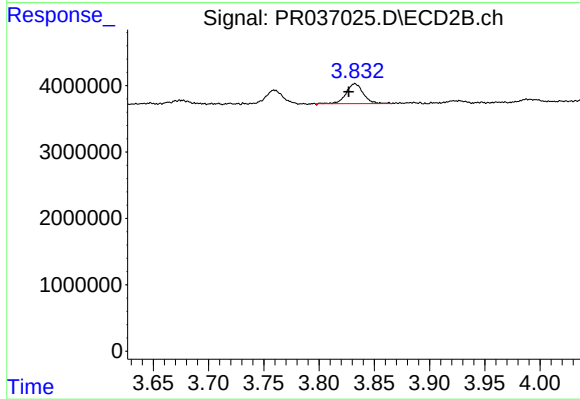

#10 AR-1221-3


R.T.: 3.832 min
Delta R.T.: 0.006 min
Response: 3237329
Conc: 21.50 ng/ml

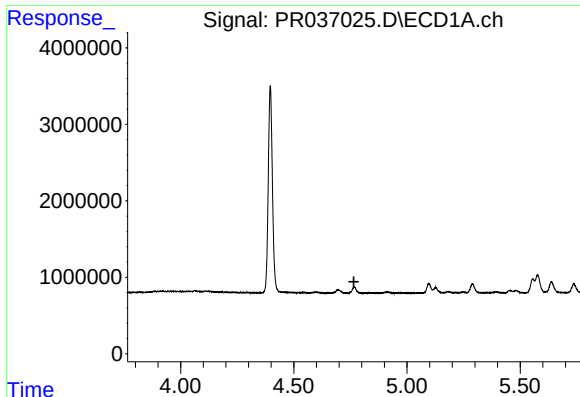

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

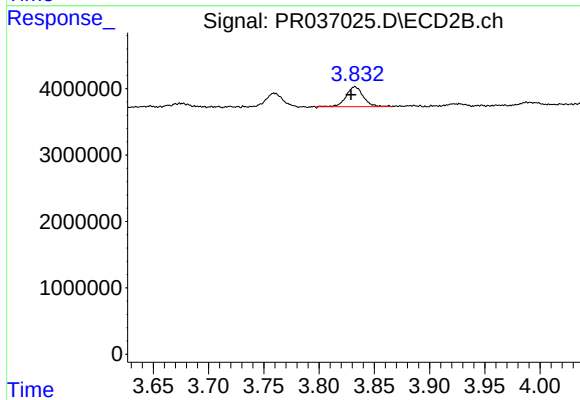


#11 AR-1232-1

R.T.: 3.832 min
Delta R.T.: 0.003 min
Response: 3237329
Conc: 34.24 ng/ml

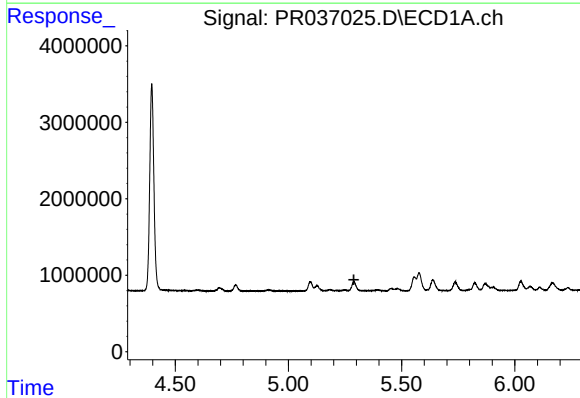


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

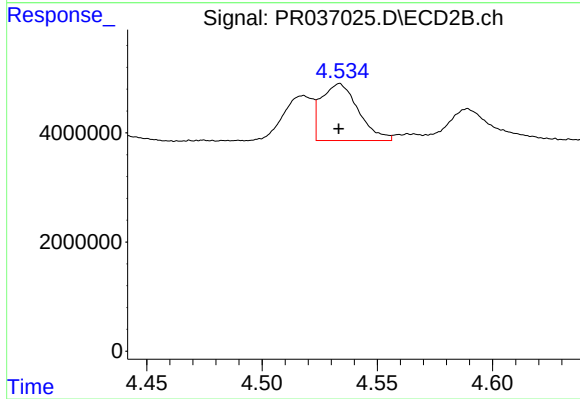

#12 AR-1232-2


R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 11707404
Conc: 98.02 ng/ml

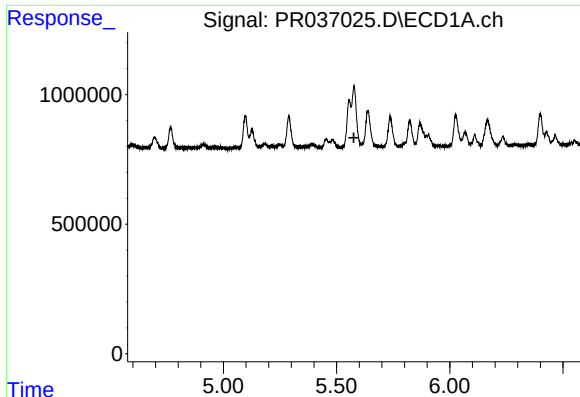

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

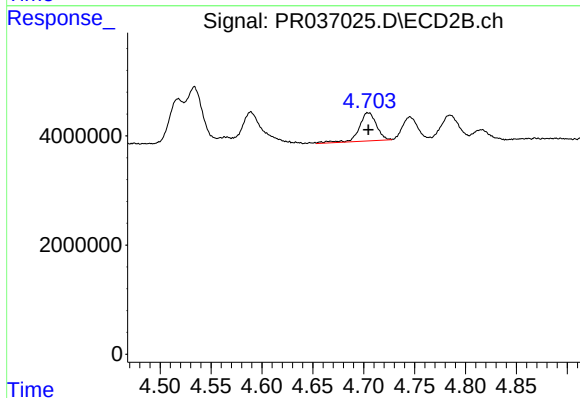


#13 AR-1232-3

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 6190461
Conc: 107.74 ng/ml

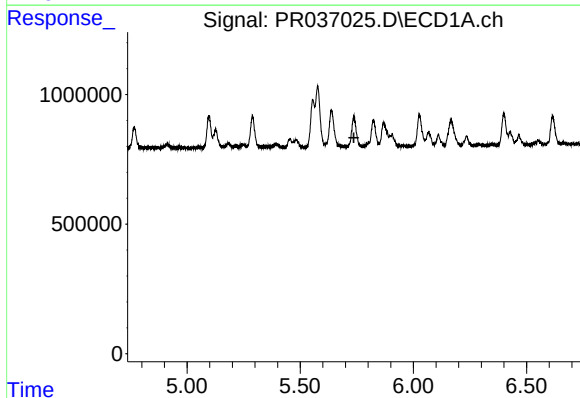


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

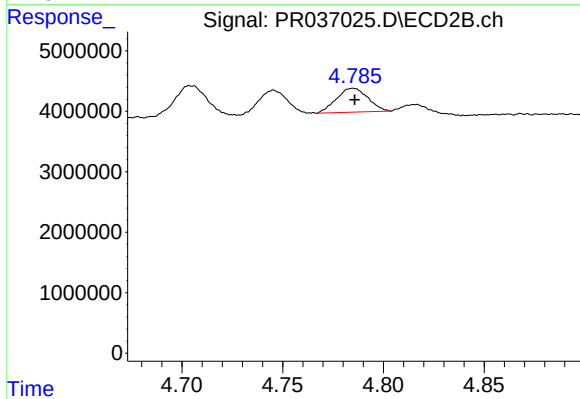

#14 AR-1232-4


R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 4277222
Conc: 86.47 ng/ml

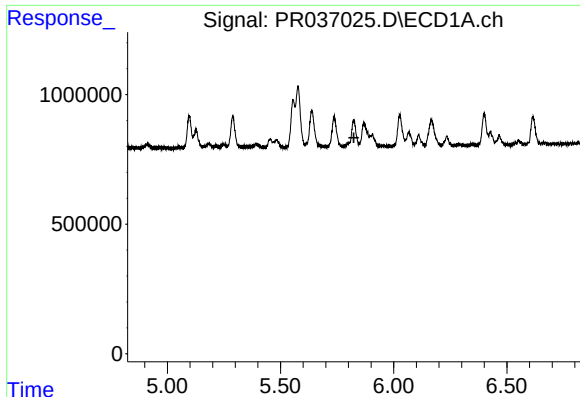

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

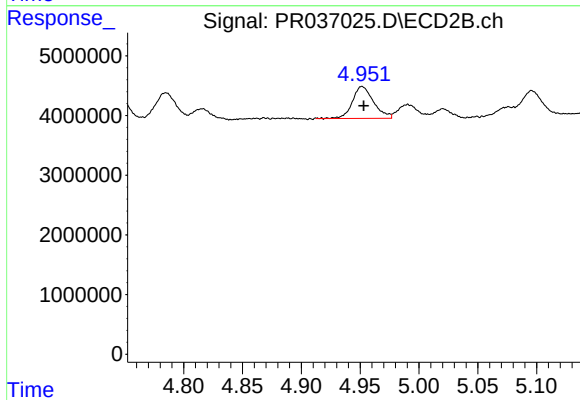


#15 AR-1232-5

R.T.: 4.952 min
Delta R.T.: -0.001 min
Response: 6672007
Conc: 116.42 ng/ml

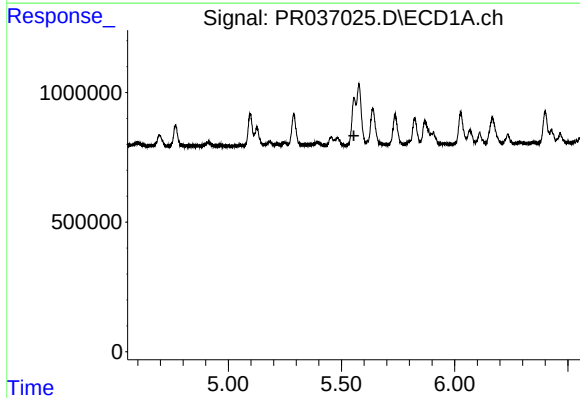


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

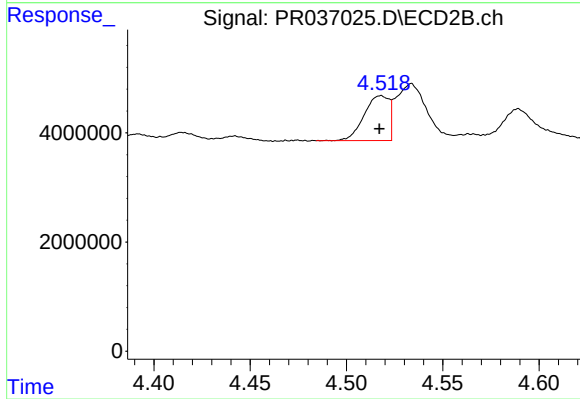

#16 AR-1242-1


R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 7350983
Conc: 64.33 ng/ml

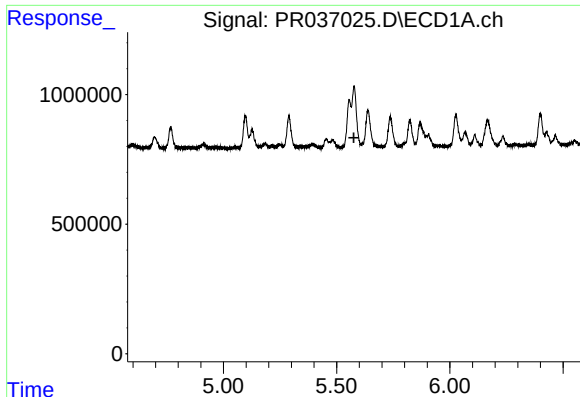

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

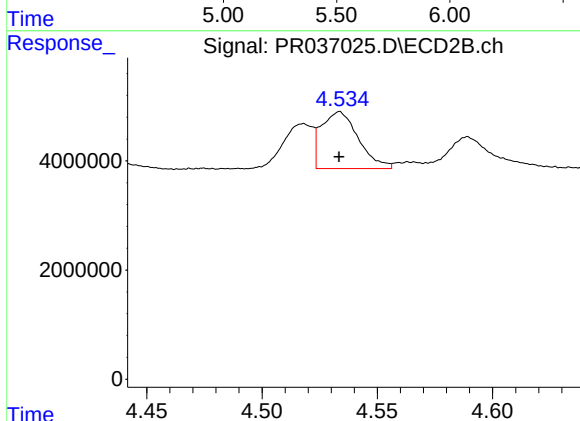


#17 AR-1242-2

R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 11707404
Conc: 61.56 ng/ml

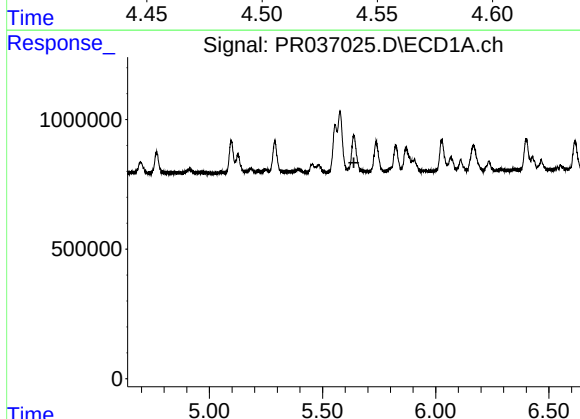


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.639 min
Response: 0
Conc: N.D.

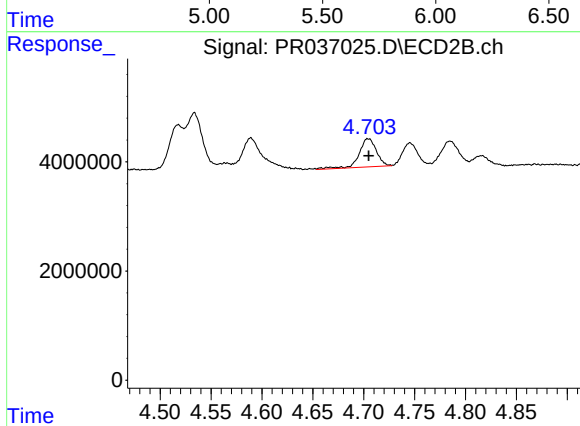

#18 AR-1242-3


R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 6190461
Conc: 64.75 ng/ml

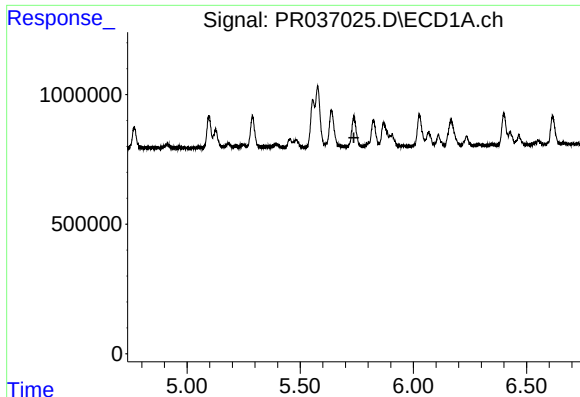

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

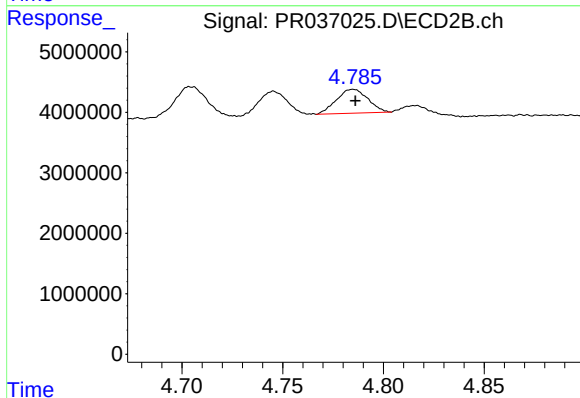


#19 AR-1242-4

R.T.: 4.785 min
Delta R.T.: -0.001 min
Response: 4277222
Conc: 47.37 ng/ml

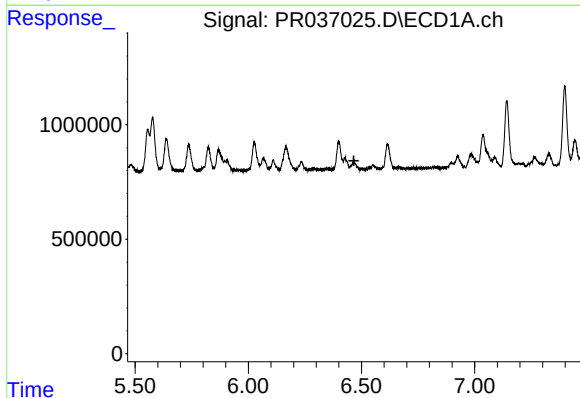


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

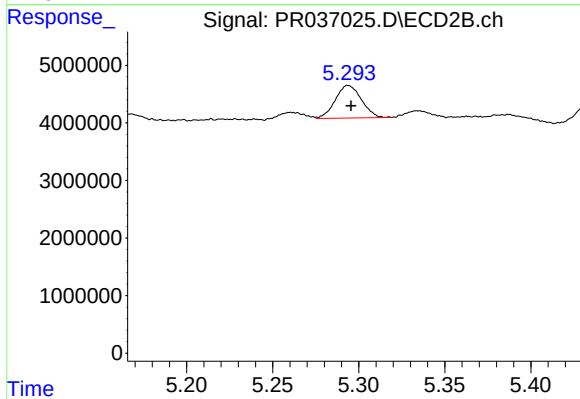

#20 AR-1242-5


R.T.: 5.294 min
Delta R.T.: -0.002 min
Response: 5978144
Conc: 43.30 ng/ml

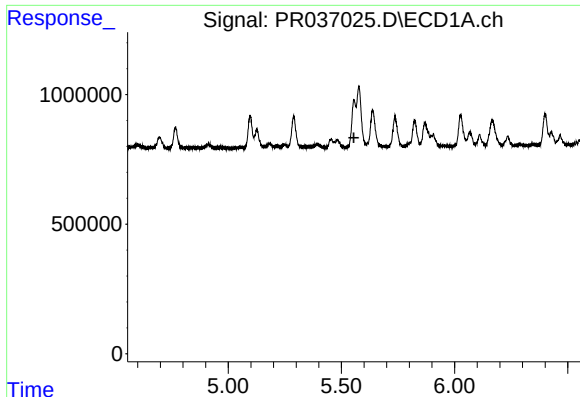

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

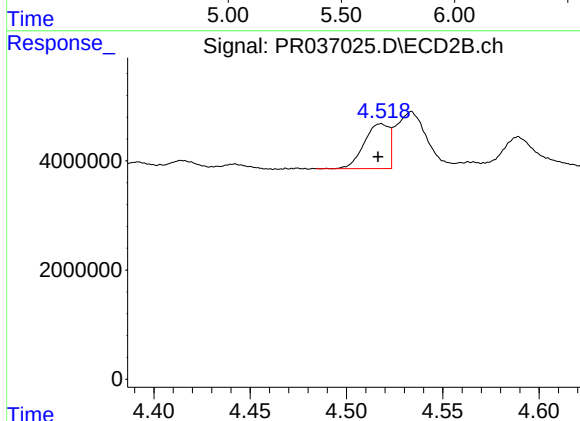


#21 AR-1248-1

R.T.: 4.518 min
Delta R.T.: 0.001 min
Response: 7350983
Conc: 75.69 ng/ml

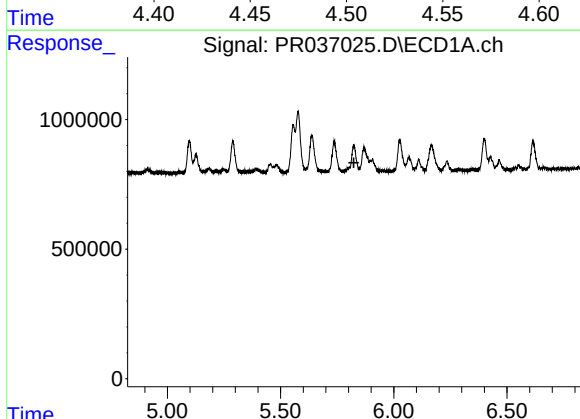


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

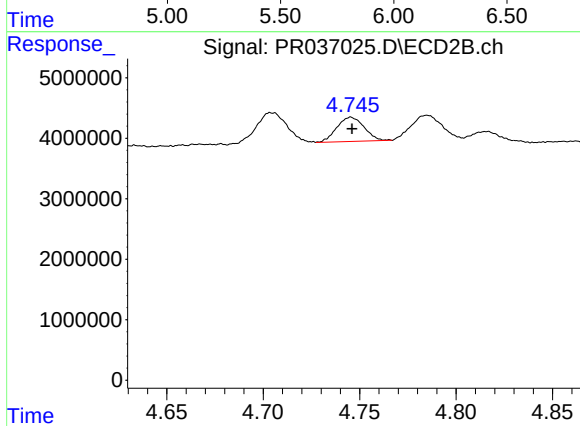

#22 AR-1248-2


R.T.: 4.745 min
Delta R.T.: 0.000 min
Response: 3949253
Conc: 29.25 ng/ml

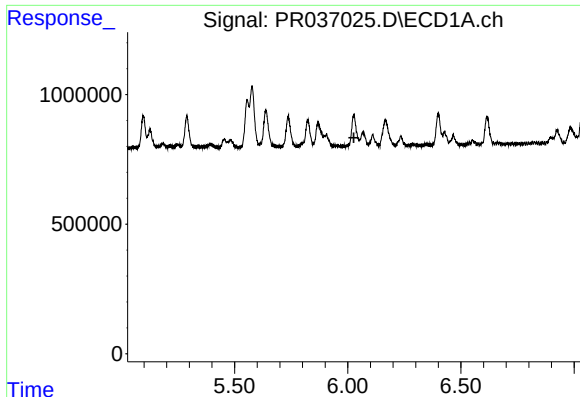

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

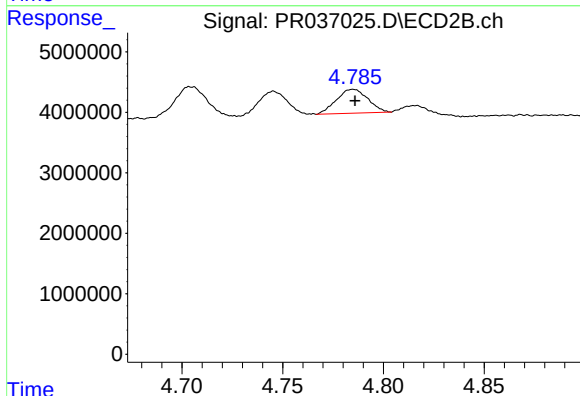


#23 AR-1248-3

R.T.: 4.785 min
Delta R.T.: -0.001 min
Response: 4277222
Conc: 30.73 ng/ml

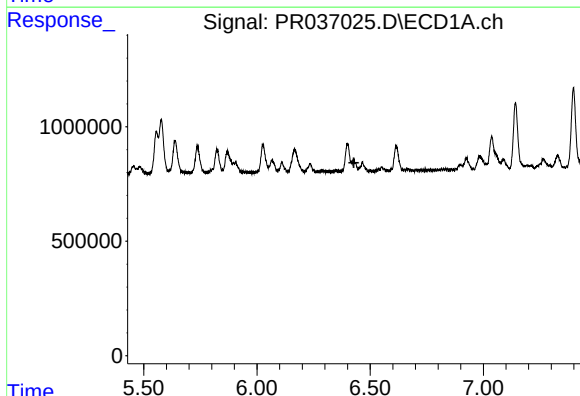


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

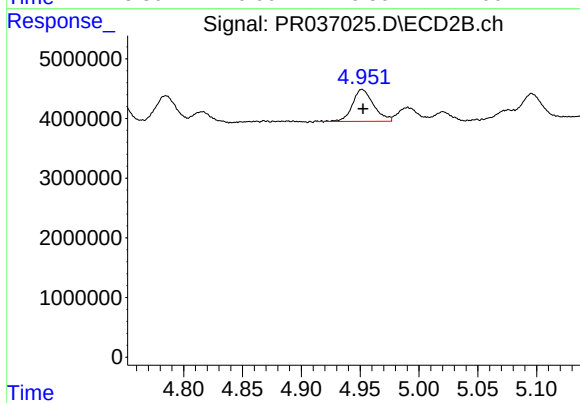

#24 AR-1248-4


R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 6672007
Conc: 37.83 ng/ml

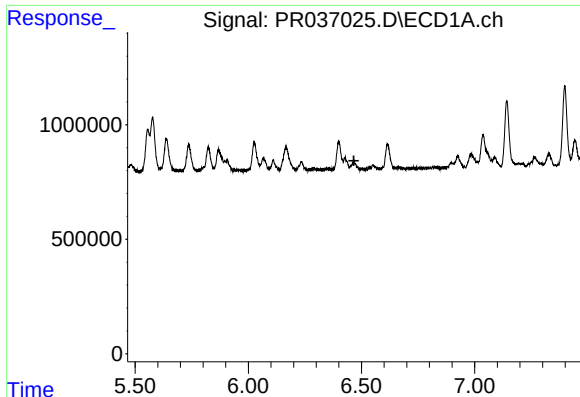

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

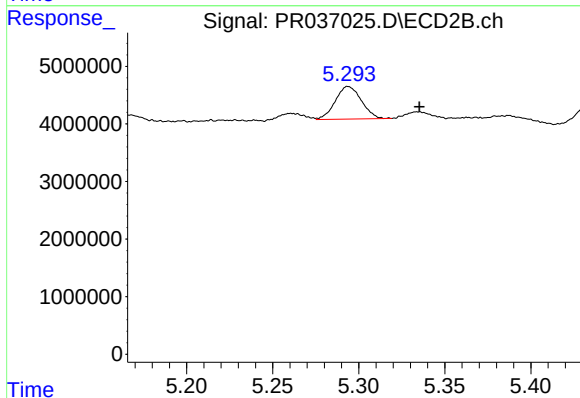


#25 AR-1248-5

R.T.: 5.294 min
Delta R.T.: -0.041 min
Response: 5978144
Conc: 30.75 ng/ml

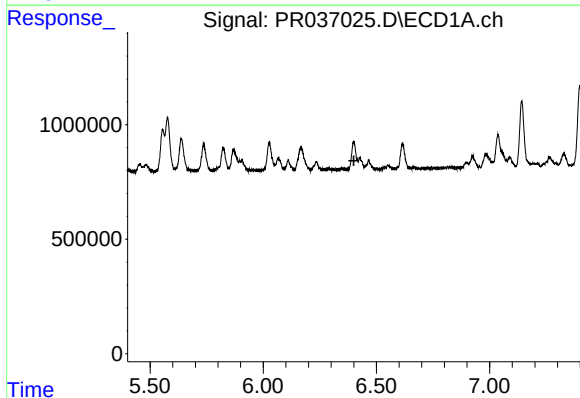


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.400 min
Response: 0
Conc: N.D.

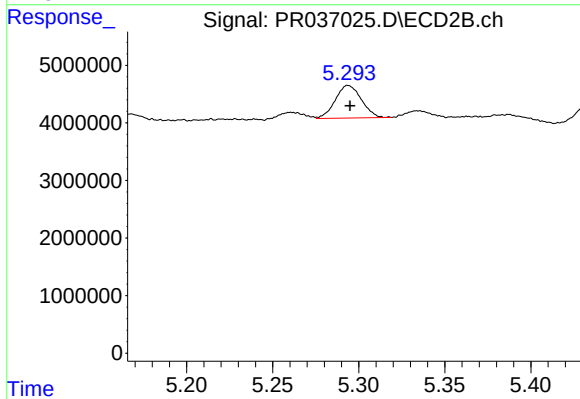

#26 AR-1254-1


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 5978144
Conc: 18.18 ng/ml

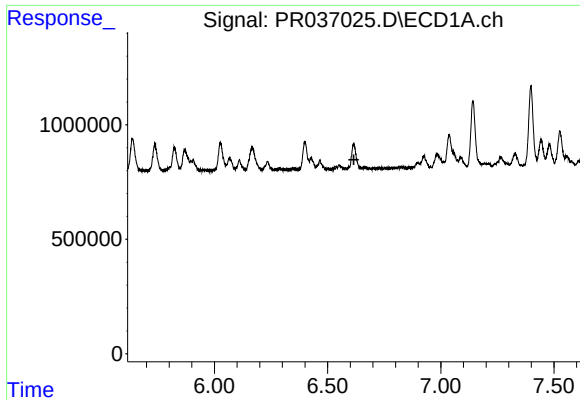

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

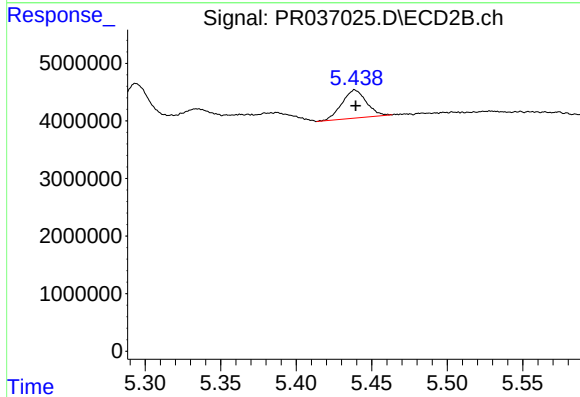


#27 AR-1254-2

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 5498557
Conc: 18.57 ng/ml

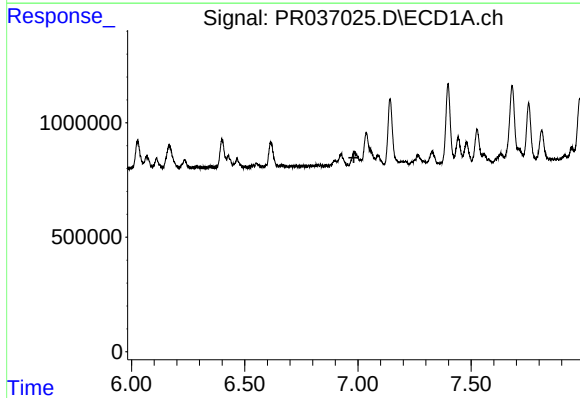


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.982 min
Response: 0
Conc: N.D.

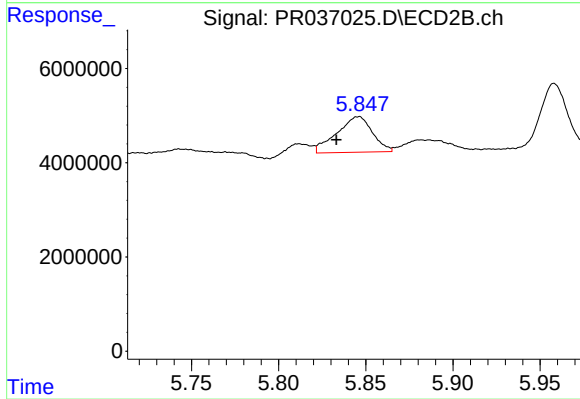

#28 AR-1254-3


R.T.: 5.846 min
Delta R.T.: 0.013 min
Response: 10734011
Conc: 21.10 ng/ml

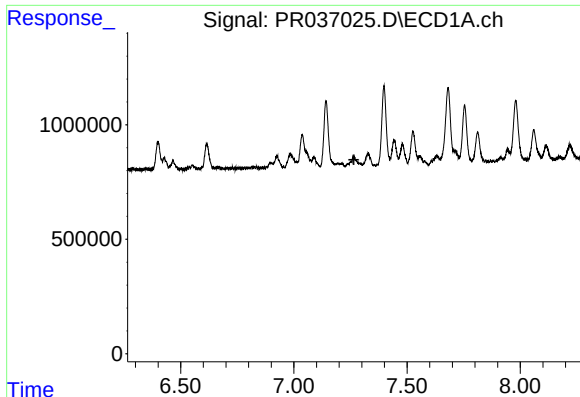

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.265 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

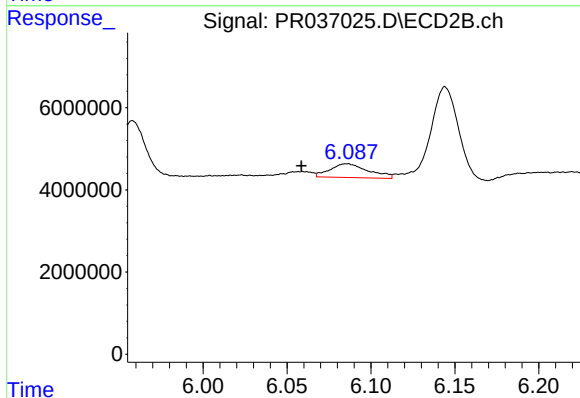


#29 AR-1254-4

R.T.: 6.086 min
Delta R.T.: 0.027 min
Response: 5350508
Conc: 13.96 ng/ml

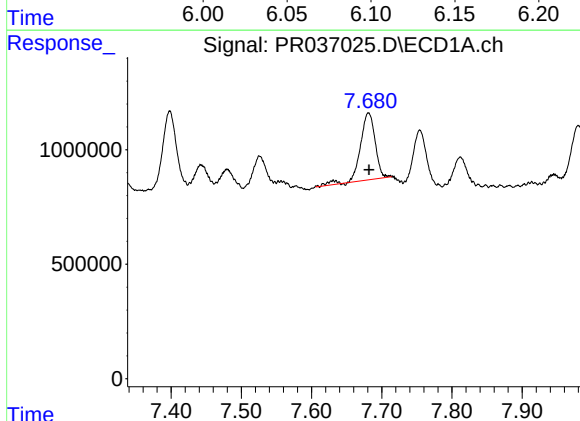


#30 AR-1254-5

R.T.: 7.681 min
Delta R.T.: -0.001 min
Response: 4286747
Conc: 41.96 ng/ml

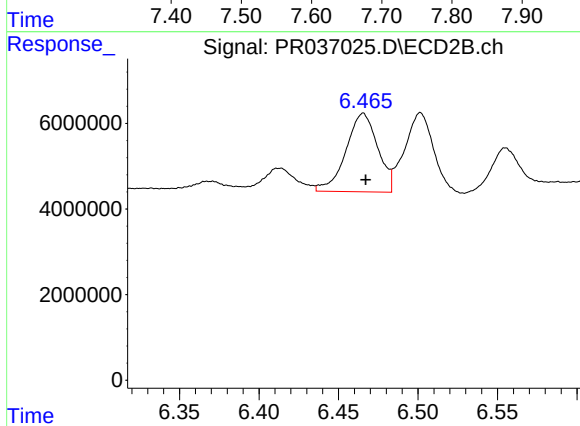

#30 AR-1254-5


R.T.: 6.465 min
Delta R.T.: -0.002 min
Response: 25502141
Conc: 50.16 ng/ml

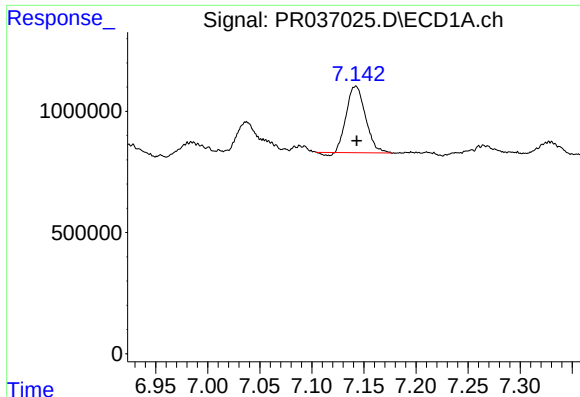

#31 AR-1260-1


R.T.: 7.142 min
Delta R.T.: 0.000 min
Response: 3490672
Conc: 34.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

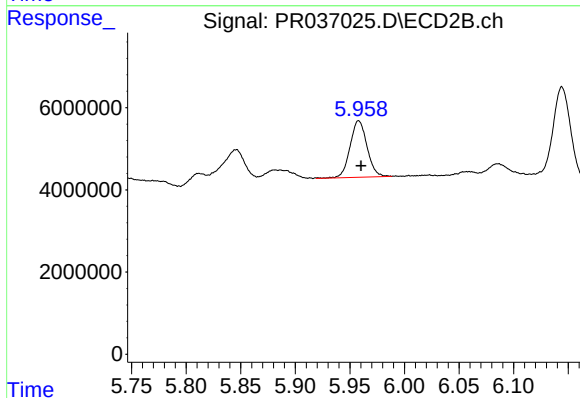


#31 AR-1260-1

R.T.: 5.958 min
Delta R.T.: -0.002 min
Response: 14944540
Conc: 34.17 ng/ml

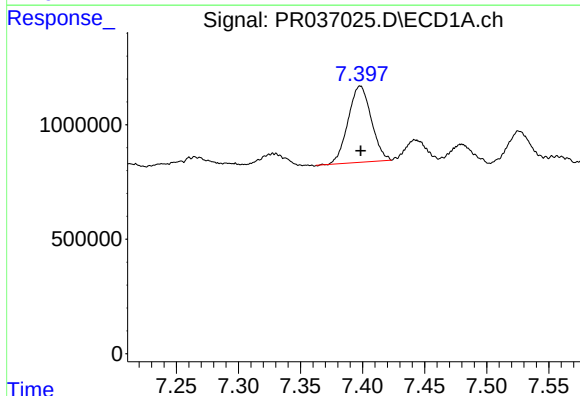


#32 AR-1260-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 4311968
Conc: 35.14 ng/ml

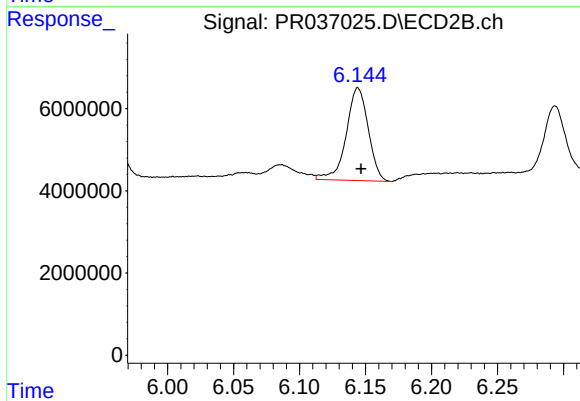

#32 AR-1260-2


R.T.: 6.144 min
Delta R.T.: -0.002 min
Response: 26272690
Conc: 40.17 ng/ml

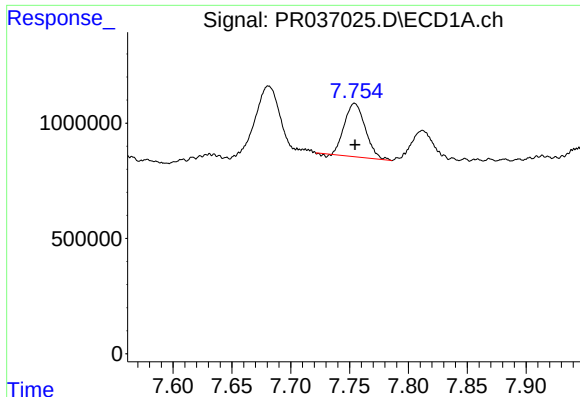

#33 AR-1260-3


R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 2870691
Conc: 29.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

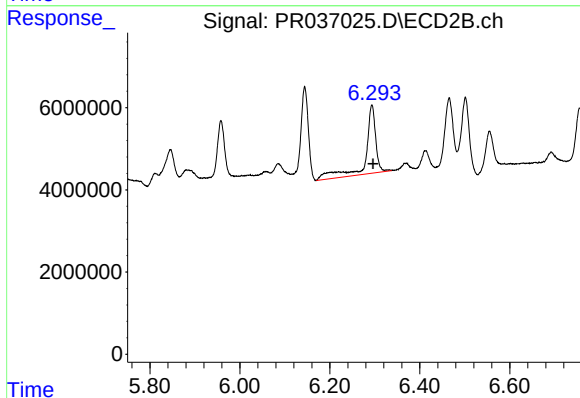


#33 AR-1260-3

R.T.: 6.294 min
Delta R.T.: -0.002 min
Response: 26282929
Conc: 49.69 ng/ml

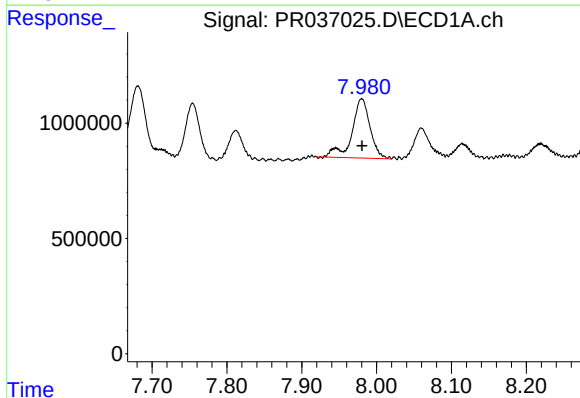


#34 AR-1260-4

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 4343156
Conc: 39.19 ng/ml

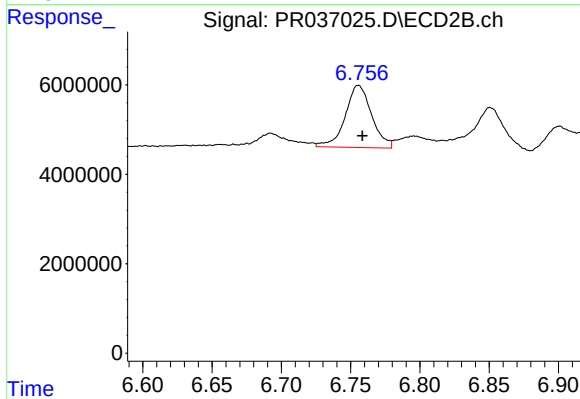

#34 AR-1260-4


R.T.: 6.756 min
Delta R.T.: -0.003 min
Response: 18496945
Conc: 39.66 ng/ml

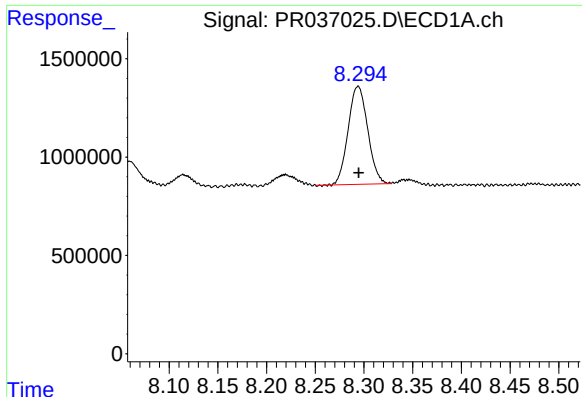

#35 AR-1260-5


R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 6981807
Conc: 32.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

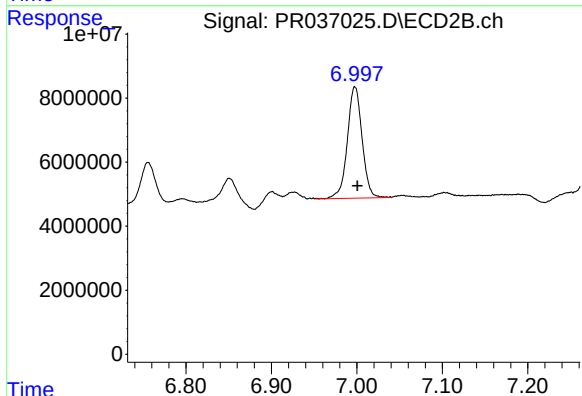


#35 AR-1260-5

R.T.: 6.998 min
Delta R.T.: -0.003 min
Response: 41829343
Conc: 31.42 ng/ml

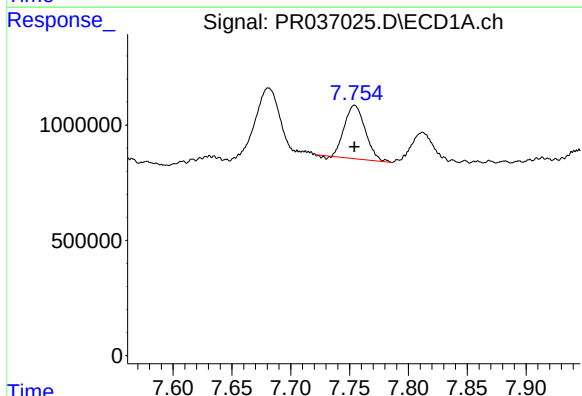


#36 AR-1262-1

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 2870691
Conc: 24.48 ng/ml

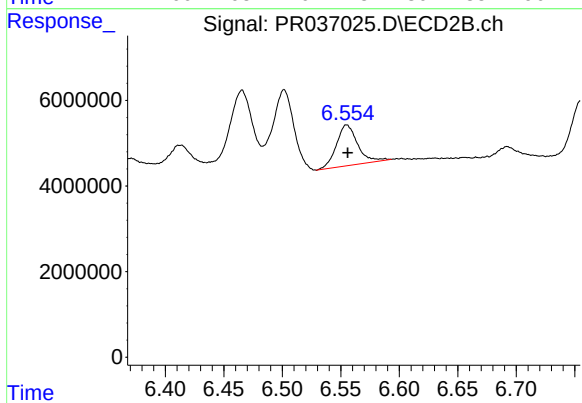

#36 AR-1262-1


R.T.: 6.555 min
Delta R.T.: 0.000 min
Response: 12018396
Conc: 43.84 ng/ml

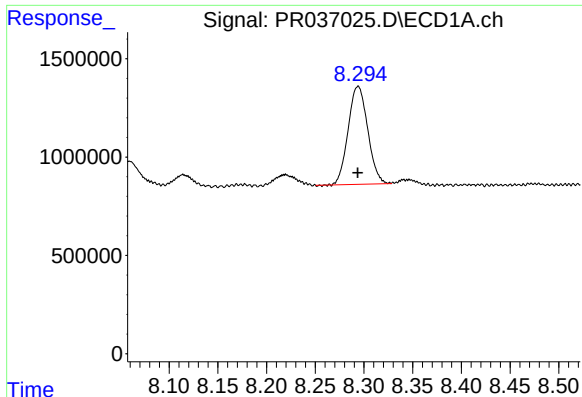

#37 AR-1262-2


R.T.: 8.294 min
Delta R.T.: 0.000 min
Response: 6981807
Conc: 32.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

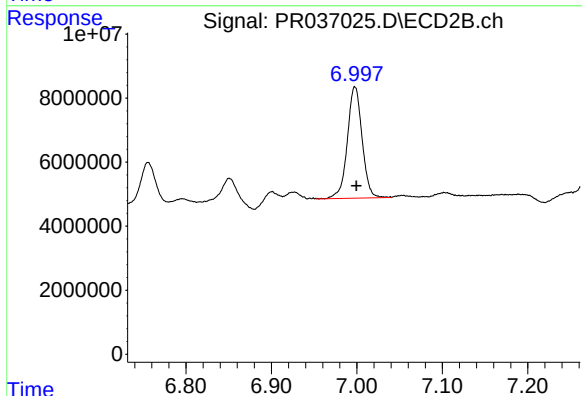


#37 AR-1262-2

R.T.: 6.998 min
Delta R.T.: -0.002 min
Response: 41829343
Conc: 30.52 ng/ml

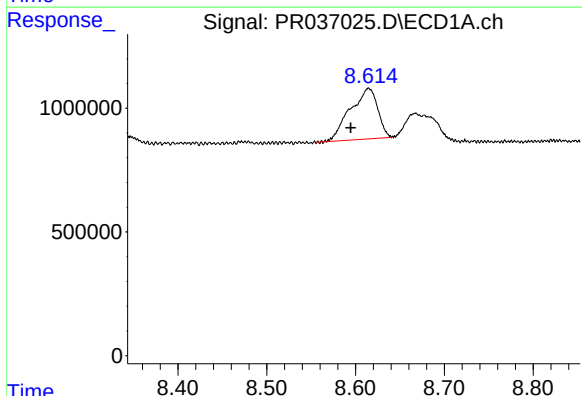


#38 AR-1262-3

R.T.: 8.615 min
Delta R.T.: 0.020 min
Response: 4392997
Conc: 30.07 ng/ml

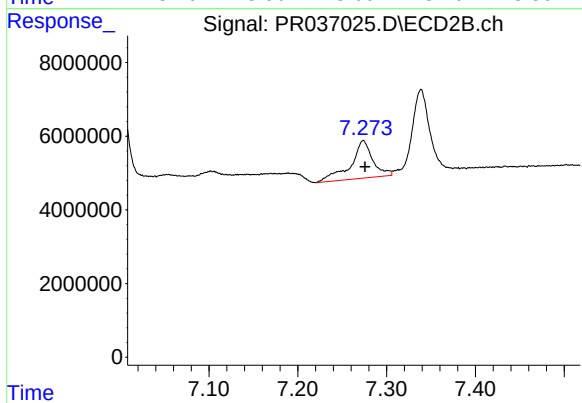

#38 AR-1262-3


R.T.: 7.274 min
Delta R.T.: -0.002 min
Response: 17712910
Conc: 32.45 ng/ml

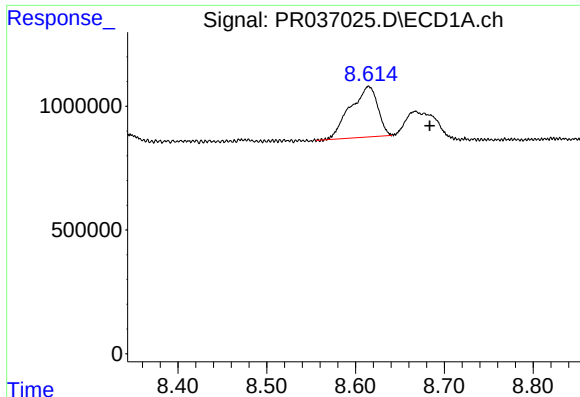

#39 AR-1262-4


R.T.: 8.615 min
Delta R.T.: -0.069 min
Response: 4392997
Conc: 40.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

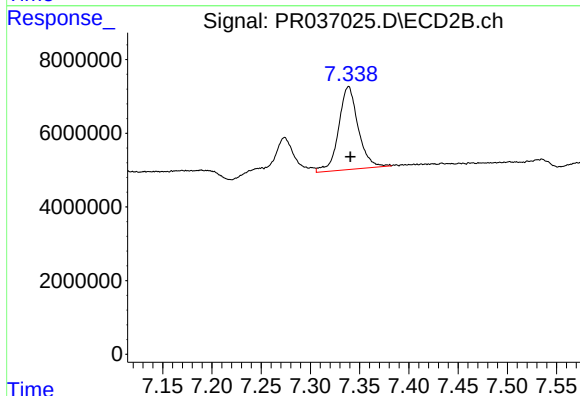


#39 AR-1262-4

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 31077568
Conc: 33.83 ng/ml

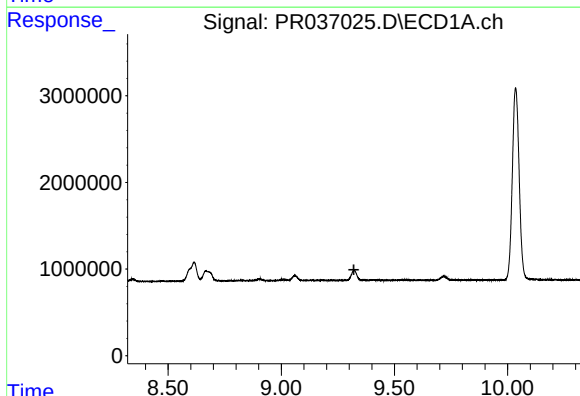


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.321 min
Response: 0
Conc: N.D.

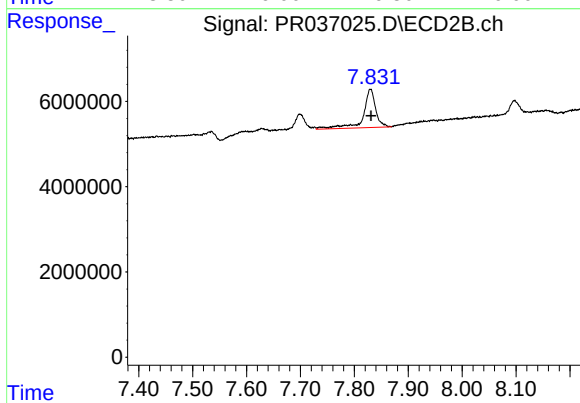

#40 AR-1262-5


R.T.: 7.830 min
Delta R.T.: -0.001 min
Response: 14344556
Conc: 35.71 ng/ml

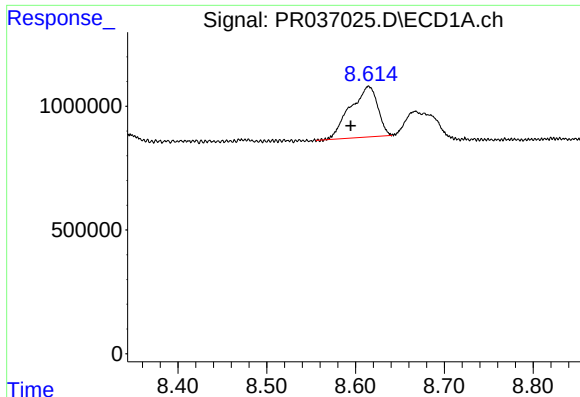

#41 AR-1268-1


R.T.: 8.615 min
Delta R.T.: 0.020 min
Response: 4392997
Conc: 18.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

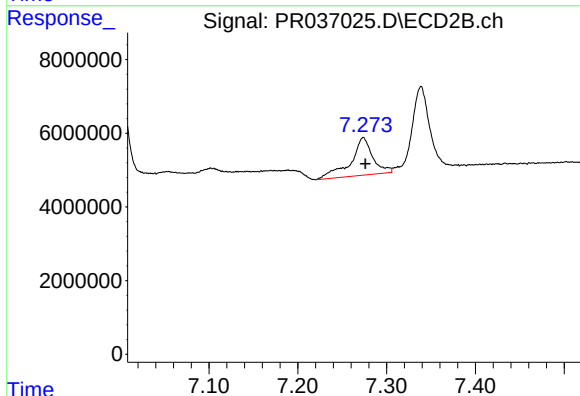


#41 AR-1268-1

R.T.: 7.274 min
Delta R.T.: -0.003 min
Response: 17712910
Conc: 11.97 ng/ml

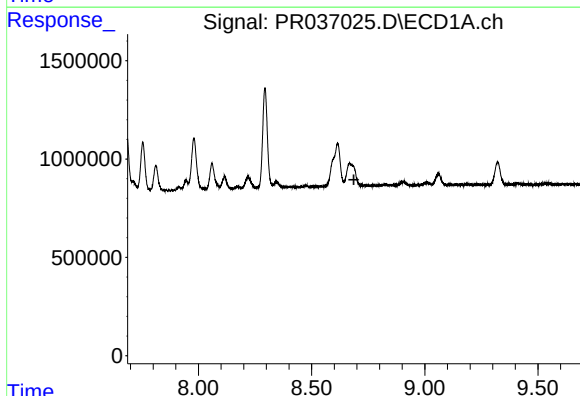


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.687 min
Response: 0
Conc: N.D.

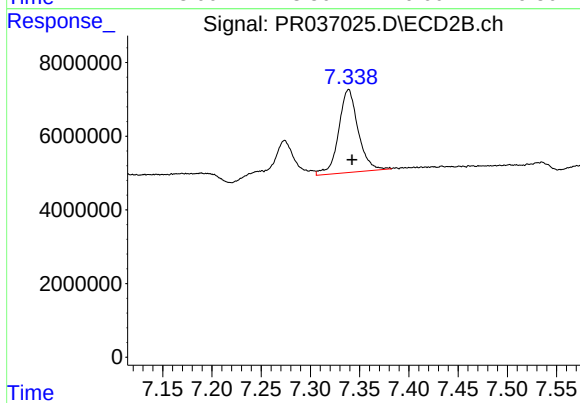

#42 AR-1268-2


R.T.: 7.339 min
Delta R.T.: -0.003 min
Response: 31077568
Conc: 24.75 ng/ml

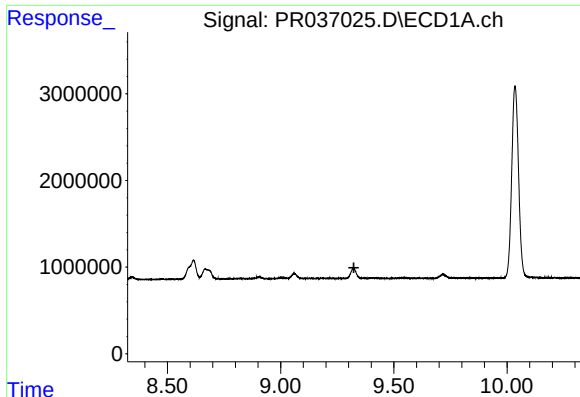

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

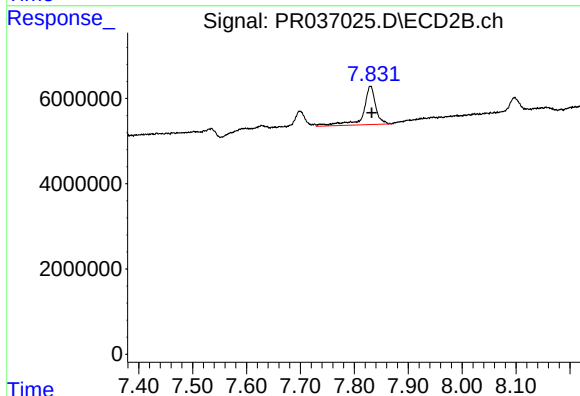


#44 AR-1268-4

R.T.: 7.830 min
Delta R.T.: -0.002 min
Response: 14344556
Conc: 33.02 ng/ml

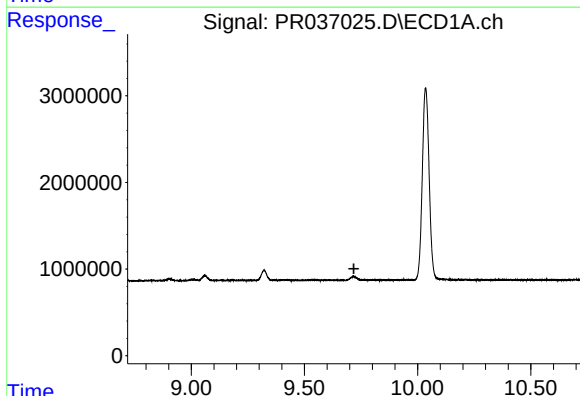

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.719 min
Response: 0
Conc: N.D.

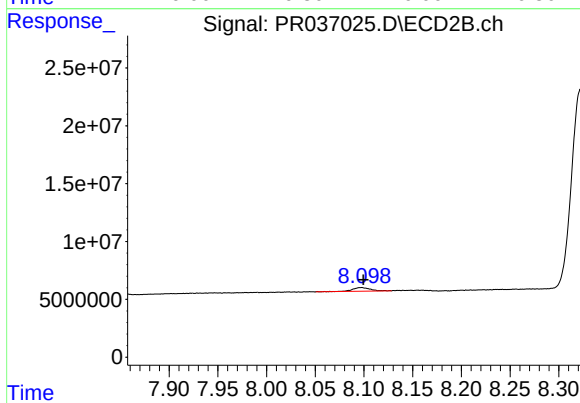

#45 AR-1268-5

R.T.: 8.097 min
Delta R.T.: -0.002 min
Response: 4039320
Conc: 1.34 ng/ml