

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
 Data File : PR037028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 19:37
 Operator : SM\SJ
 Sample : K1560-07
 Misc : AR1221 LOD 25PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 03:50:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.403	3.482	28849441	119.5E6	18.108	20.398
2)	SA Decachlor...	10.036	8.322	42946874	195.0E6	22.923	24.428
Target Compounds							
8)	L2 AR-1221-1	0.000	3.685	0	2689570	N.D.	43.797 #
9)	L2 AR-1221-2	0.000	3.768	0	3088904	N.D.	68.306 #
10)	L2 AR-1221-3	0.000	3.840	0	6454088	N.D.	42.871 #
11)	L3 AR-1232-1	0.000	3.840	0	6454088	N.D.	68.263 #
36)	L8 AR-1262-1	0.000	6.560	0	1363968	N.D.	4.976 #
40)	L8 AR-1262-5	0.000	7.841	0	15774758	N.D.	39.272 #
43)	L9 AR-1268-3	0.000	7.534	0	23143643	N.D.	23.795 #
44)	L9 AR-1268-4	0.000	7.841	0	15774758	N.D.	36.315 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
Data File : PR037028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2019 19:37
Operator : SM\SJ
Sample : K1560-07
Misc : AR1221 LOD 25PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 03:50:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

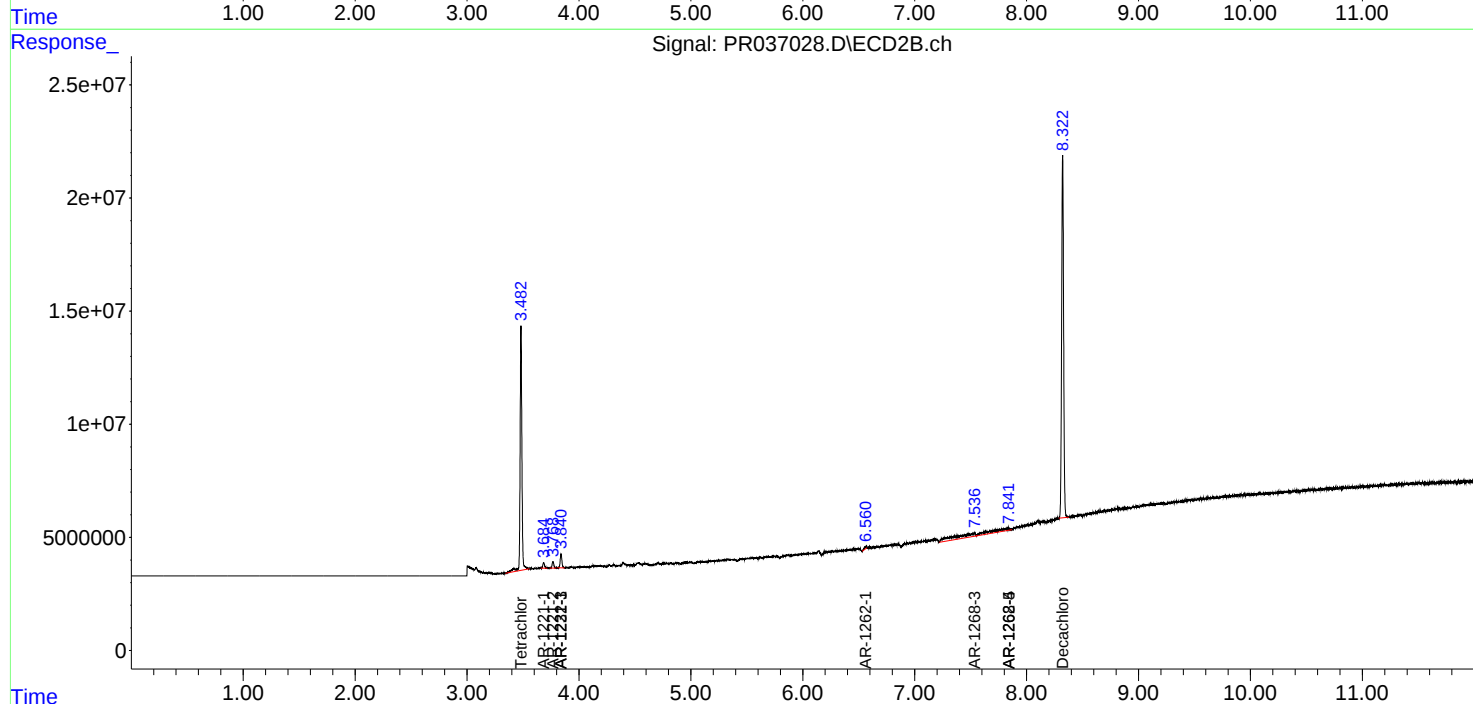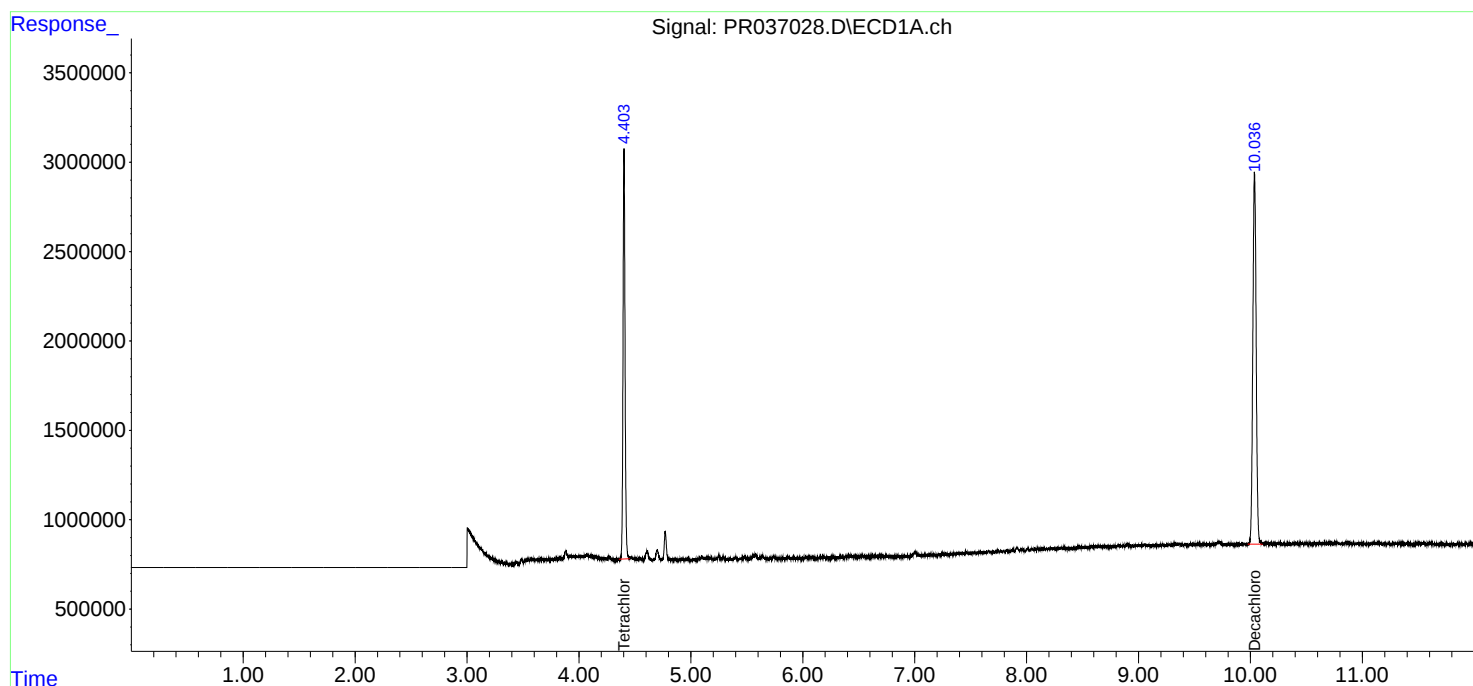


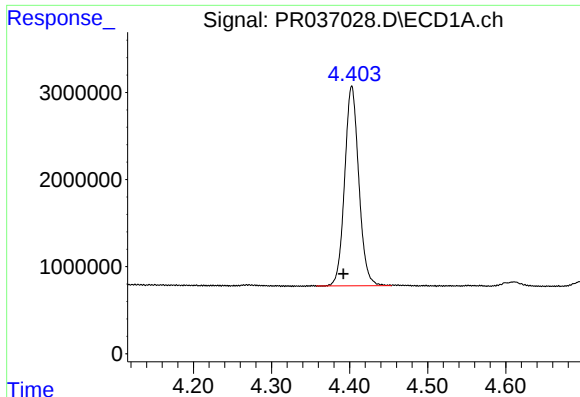

#1 Tetrachloro-m-xylene


R.T.: 4.403 min
Delta R.T.: 0.011 min
Response: 28849441
Conc: 18.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

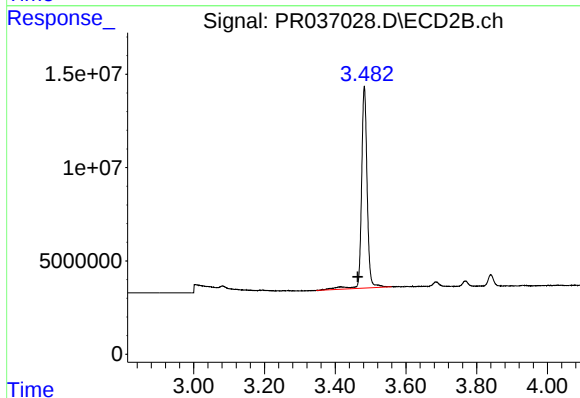


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.019 min
Response: 119490980
Conc: 20.40 ng/ml

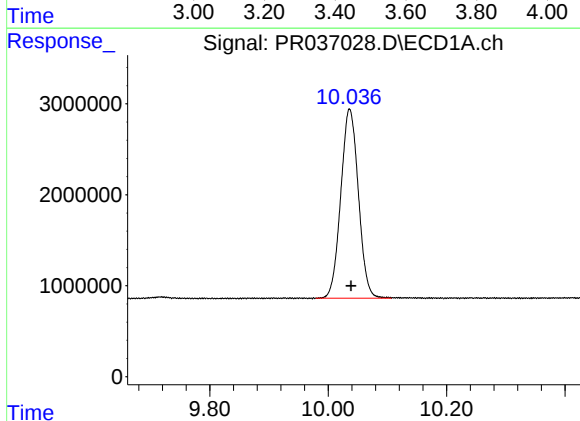


#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: -0.003 min
Response: 42946874
Conc: 22.92 ng/ml

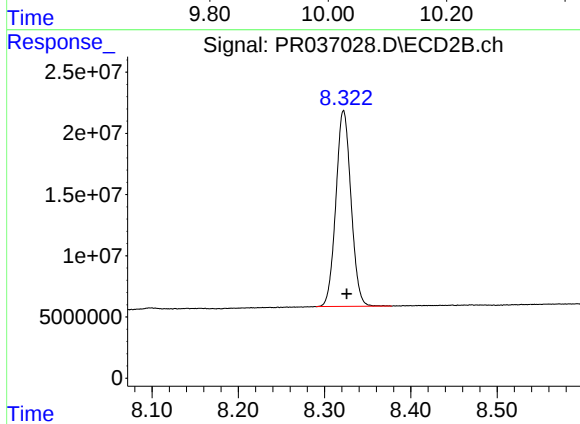

#2 Decachlorobiphenyl


R.T.: 8.322 min
Delta R.T.: -0.004 min
Response: 194993738
Conc: 24.43 ng/ml

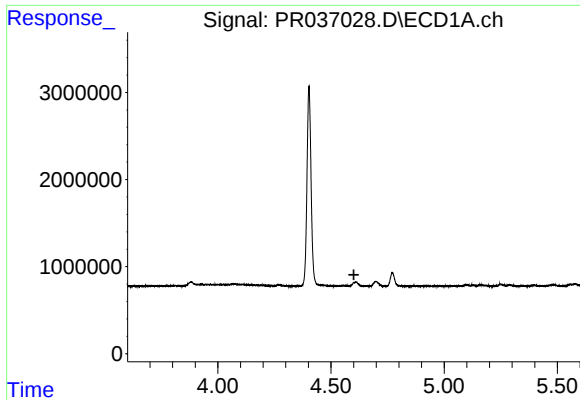

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

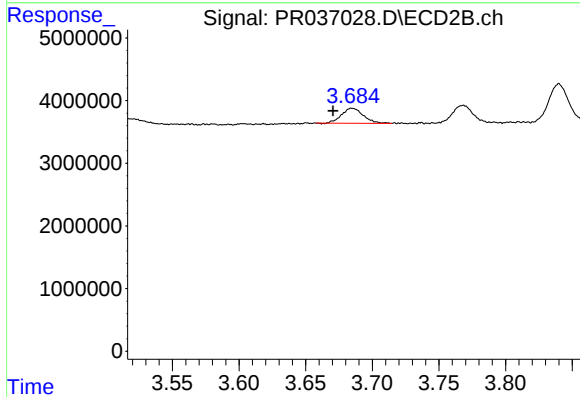


#8 AR-1221-1

R.T.: 3.685 min
Delta R.T.: 0.014 min
Response: 2689570
Conc: 43.80 ng/ml

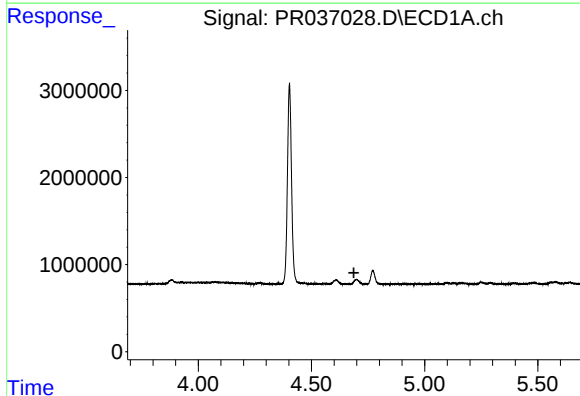


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.688 min
Response: 0
Conc: N.D.

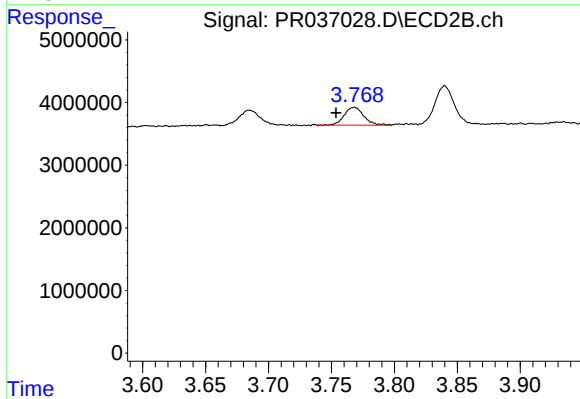

#9 AR-1221-2


R.T.: 3.768 min
Delta R.T.: 0.014 min
Response: 3088904
Conc: 68.31 ng/ml

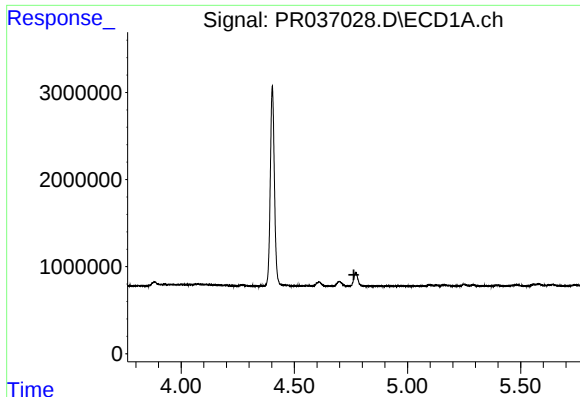

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

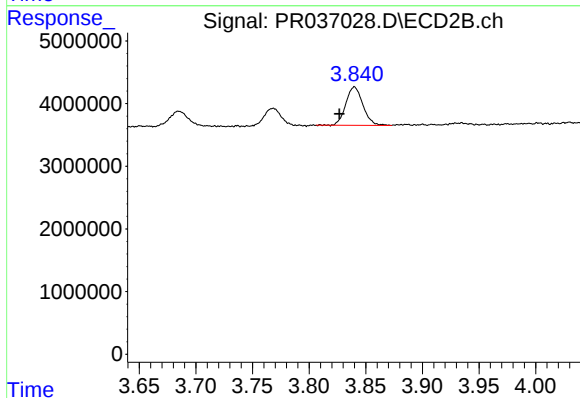


#10 AR-1221-3

R.T.: 3.840 min
Delta R.T.: 0.013 min
Response: 6454088
Conc: 42.87 ng/ml

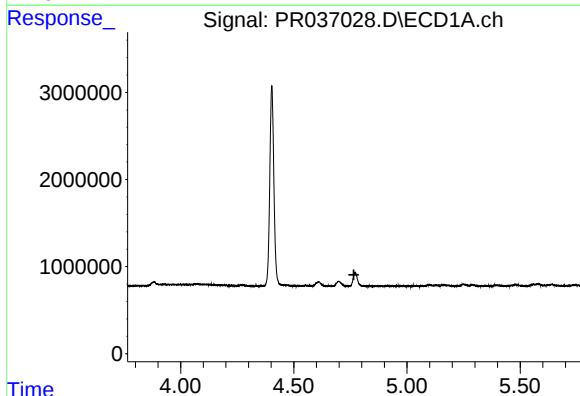


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.766 min
Response: 0
Conc: N.D.

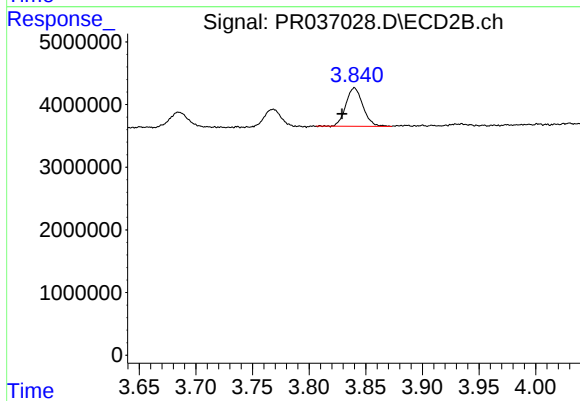

#11 AR-1232-1


R.T.: 3.840 min
Delta R.T.: 0.011 min
Response: 6454088
Conc: 68.26 ng/ml

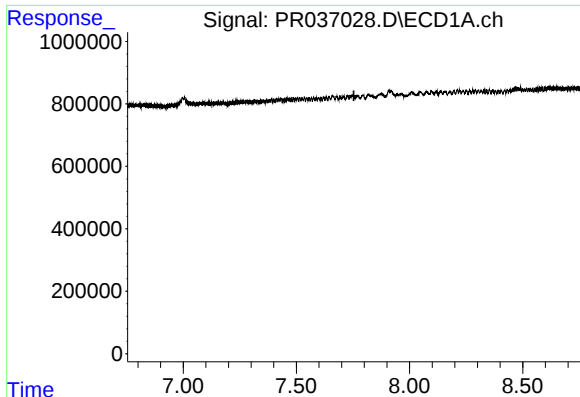

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.754 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

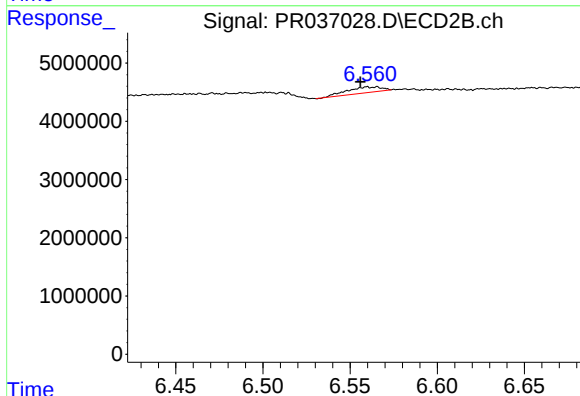


#36 AR-1262-1

R.T.: 6.560 min
Delta R.T.: 0.004 min
Response: 1363968
Conc: 4.98 ng/ml

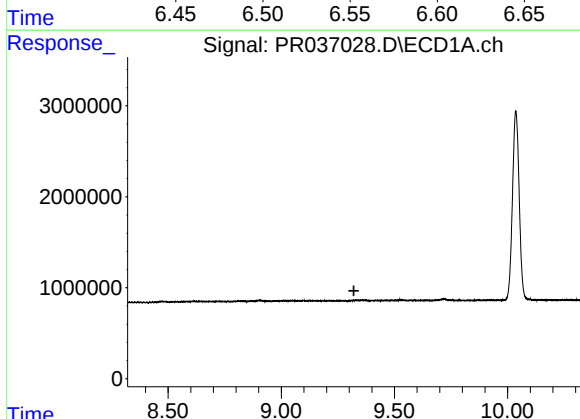


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.321 min
Response: 0
Conc: N.D.

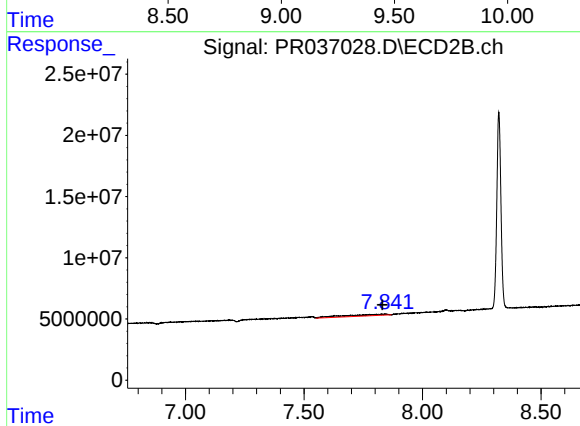

#40 AR-1262-5


R.T.: 7.841 min
Delta R.T.: 0.010 min
Response: 15774758
Conc: 39.27 ng/ml

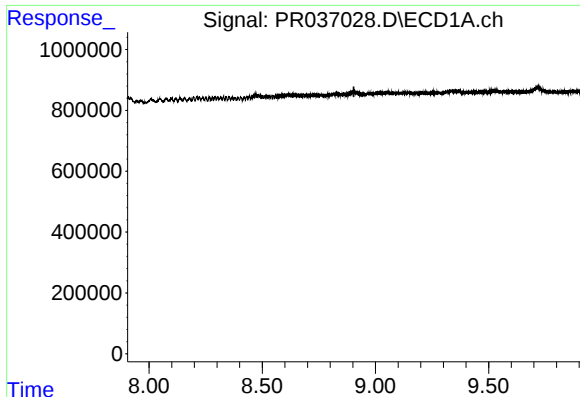

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

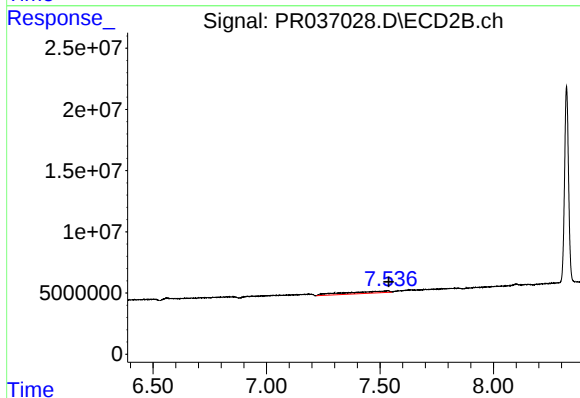


#43 AR-1268-3

R.T.: 7.534 min
Delta R.T.: -0.005 min
Response: 23143643
Conc: 23.80 ng/ml

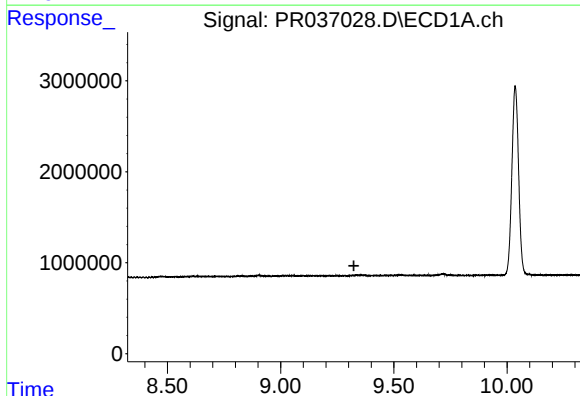

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.323 min
Response: 0
Conc: N.D.

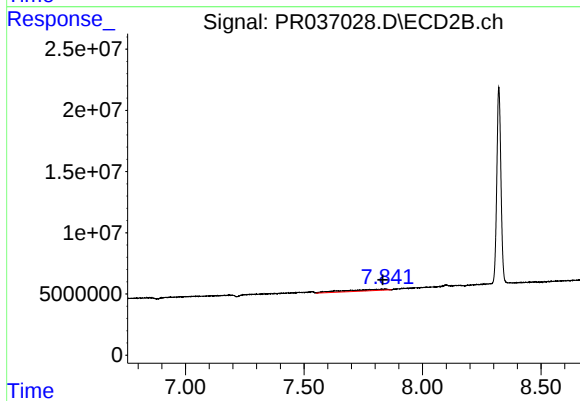

#44 AR-1268-4

R.T.: 7.841 min
Delta R.T.: 0.009 min
Response: 15774758
Conc: 36.32 ng/ml