

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
 Data File : PR036994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 08:14
 Operator : SM\SJ
 Sample : K2305-01 (Sig #1); K2305-01RE (Sig #2)
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-EF-02-001-ABCD

Manual Integrations
 APPROVED

mohammad
 4/11/2019 3:38:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 09:15:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.470	20970710	81145272	13.163	13.852m
2)	SA Decachlor...	10.036	8.321	22396875	86158277	11.954	10.794

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040919\
Data File : PR036994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2019 08:14
Operator : SM\SJ
Sample : K2305-01 (Sig #1); K2305-01RE (Sig #2)
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
FK-EF-02-001-ABCD


Manual Integrations
APPROVED

mohammad
4/11/2019 3:38:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 09:15:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

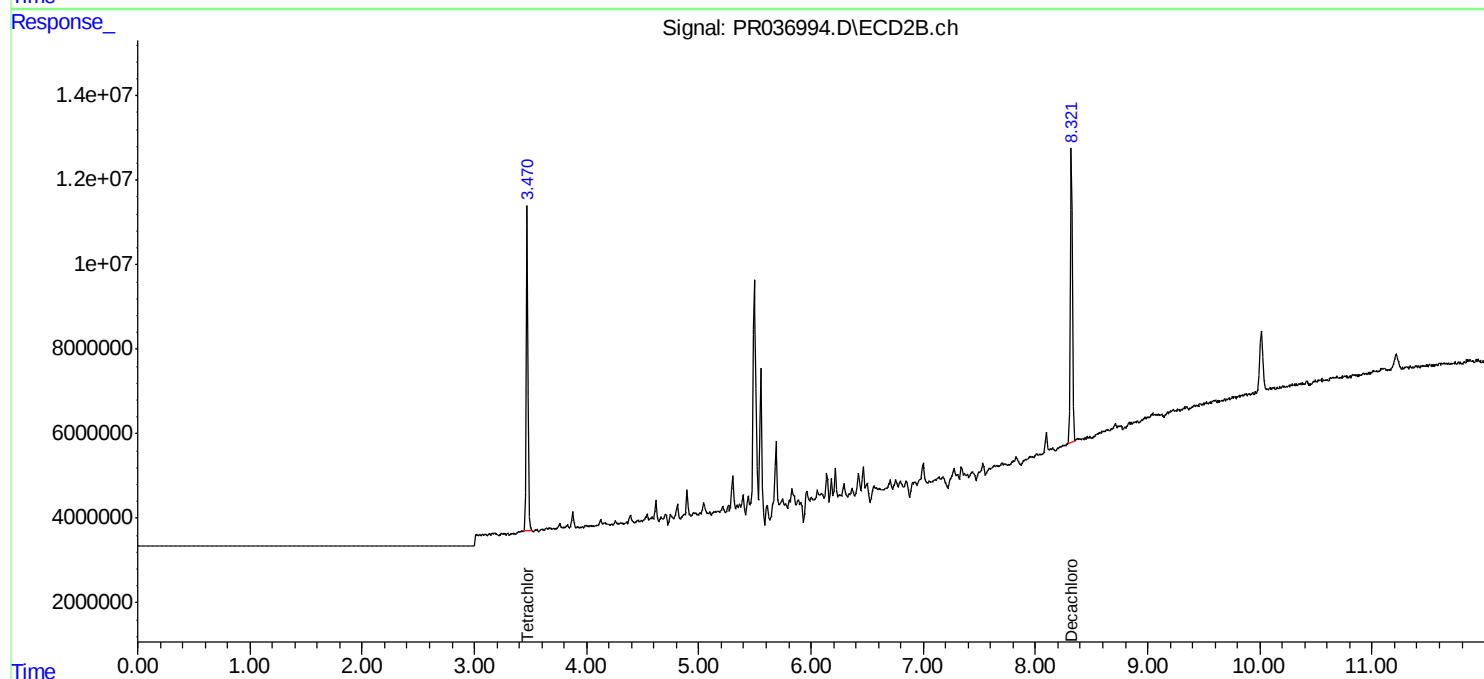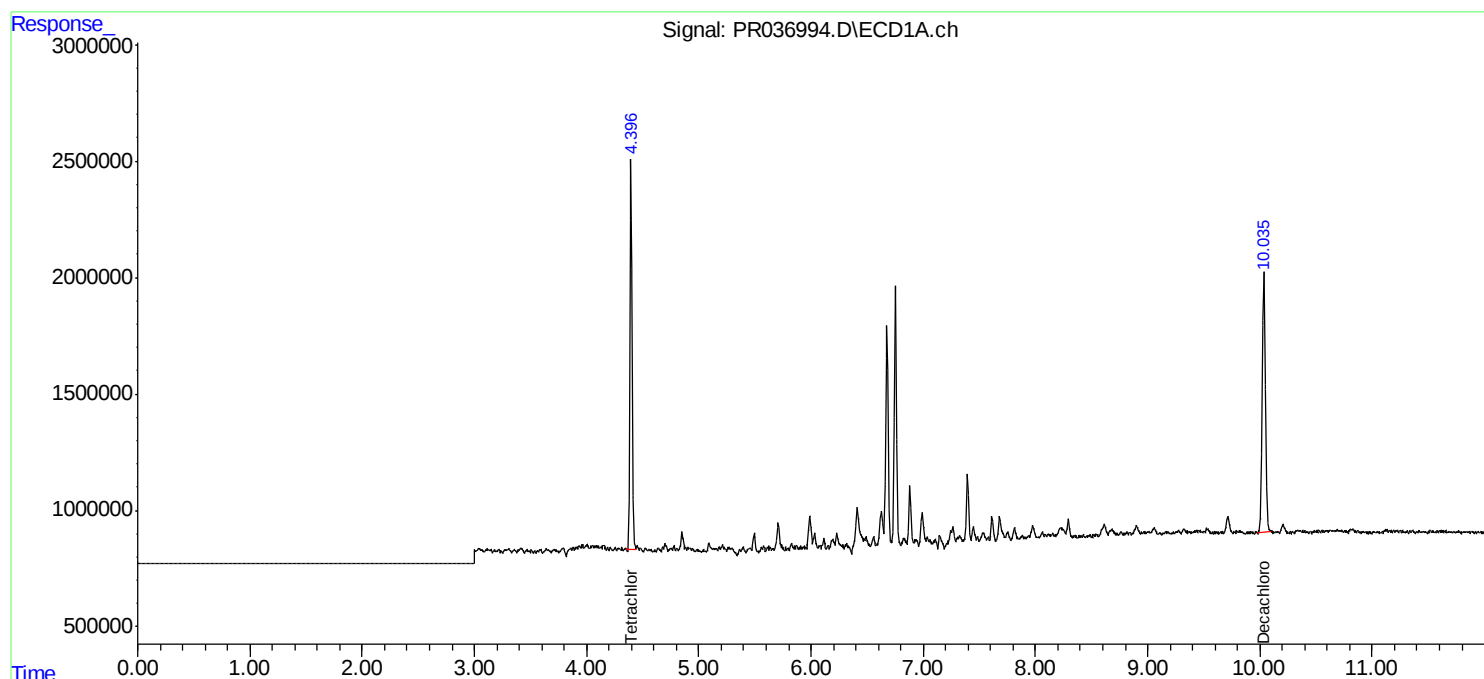

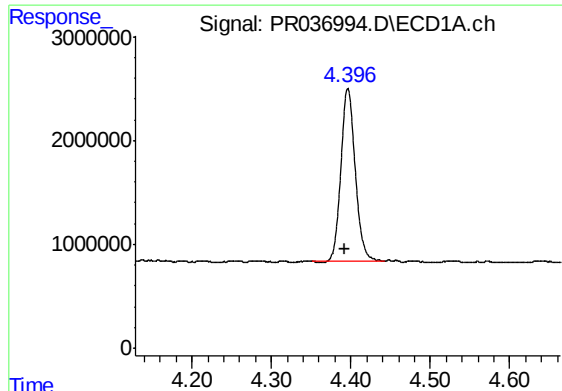


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: 0.004 min
Response: 20970710
Conc: 13.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-EF-02-001-ABCD


Manual Integrations
APPROVED

mohammad
4/11/2019 3:38:06 PM

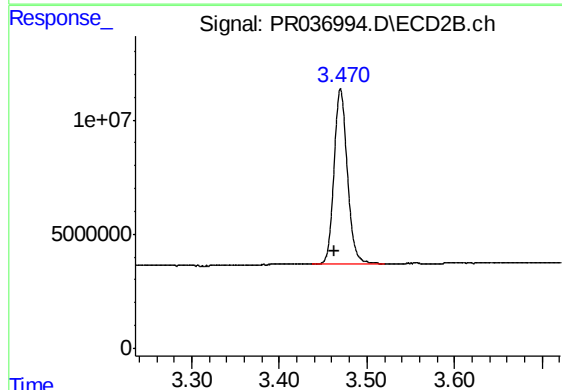


#1 Tetrachloro-m-xylene

R.T.: 3.470 min
Delta R.T.: 0.006 min
Response: 81145272
Conc: 13.85 ng/ml m

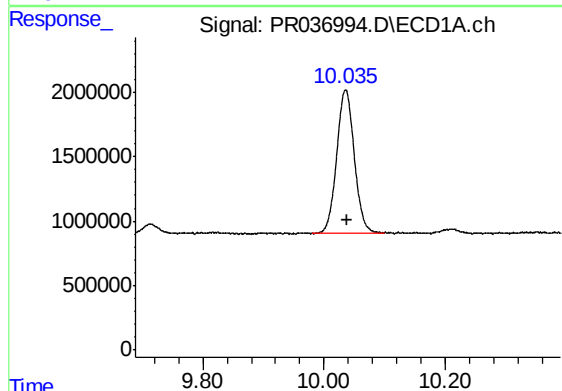

#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: -0.003 min
Response: 22396875
Conc: 11.95 ng/ml

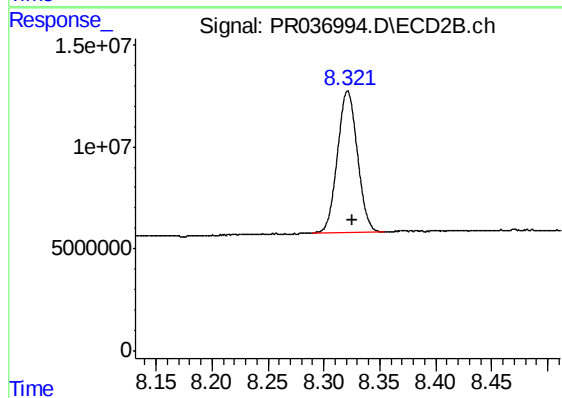

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.004 min
Response: 86158277
Conc: 10.79 ng/ml