

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041019\
 Data File : PR037060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2019 14:04
 Operator : SM\SJ
 Sample : K2316-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SPLP-LEACHATE-AMND-CS-2

Manual Integrations
 APPROVED

mohammad
 4/11/2019 3:49:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 00:59:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.393	3.466	34894637	140.4E6	21.903m	23.974
2) SA Decachlor...	10.034	8.320	19724625	81323234	10.528	10.188

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041019\
Data File : PR037060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2019 14:04
Operator : SM\SJ
Sample : K2316-12
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SPLP-LEACHATE-AMND-CS-2


Manual Integrations
APPROVED

mohammad
4/11/2019 3:49:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 00:59:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

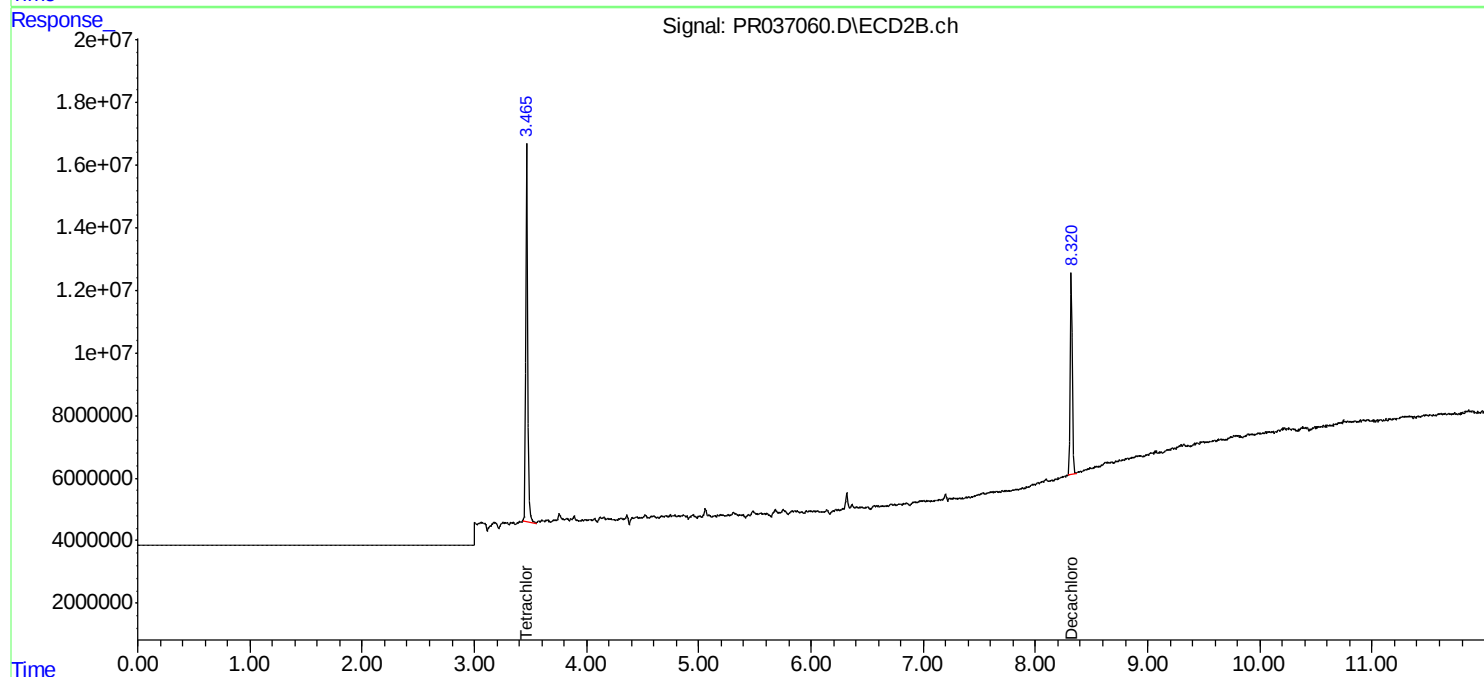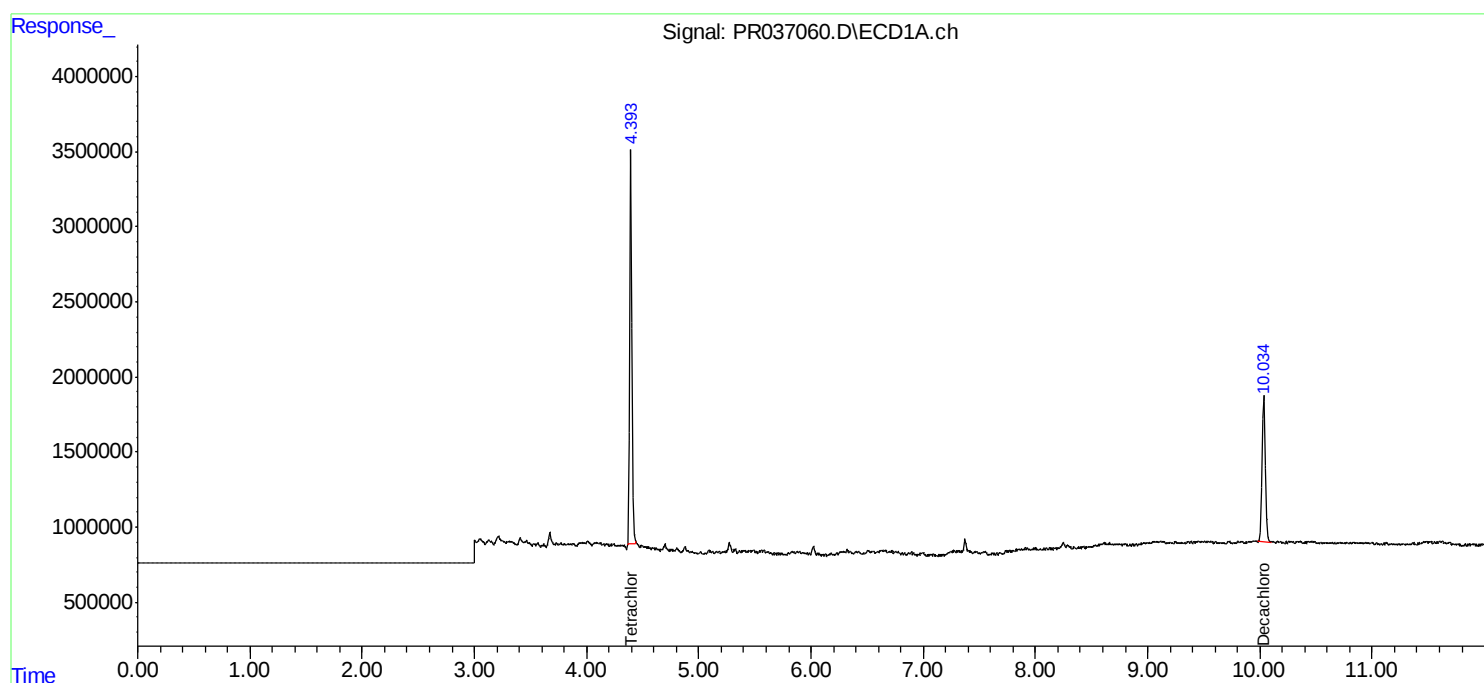

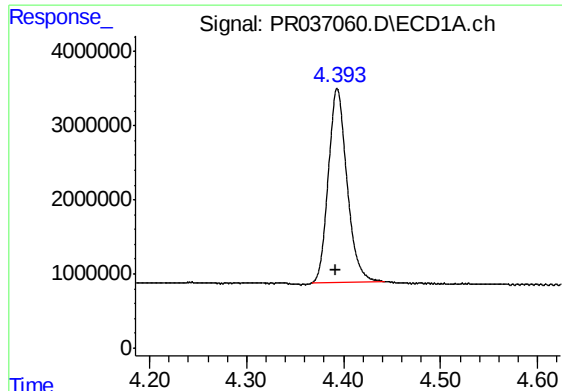


#1 Tetrachloro-m-xylene

R.T.: 4.393 min
Delta R.T.: 0.000 min
Response: 34894637
Conc: 21.90 ng/ml m

Instrument :
ECD_R
ClientSampleId :
SPLP-LEACHATE-AMND-CS-2


Manual Integrations
APPROVED

mohammad
4/11/2019 3:49:37 PM

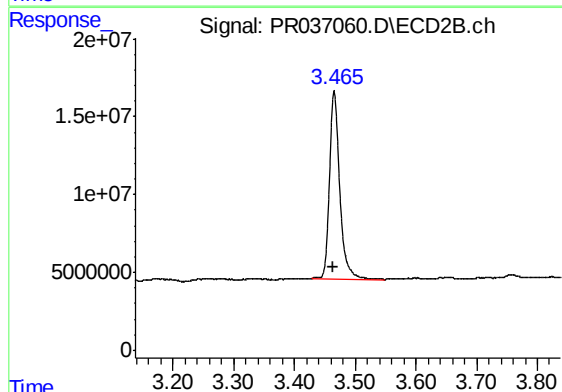


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.002 min
Response: 140440701
Conc: 23.97 ng/ml

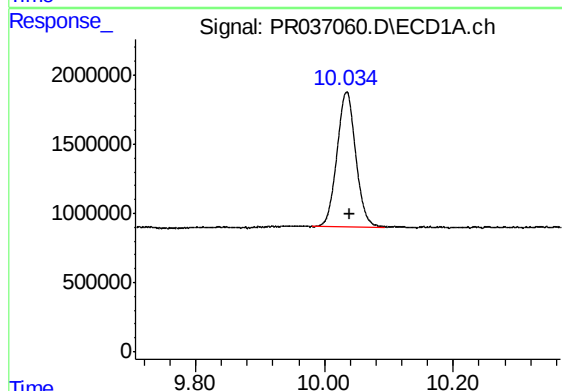

#2 Decachlorobiphenyl

R.T.: 10.034 min
Delta R.T.: -0.004 min
Response: 19724625
Conc: 10.53 ng/ml

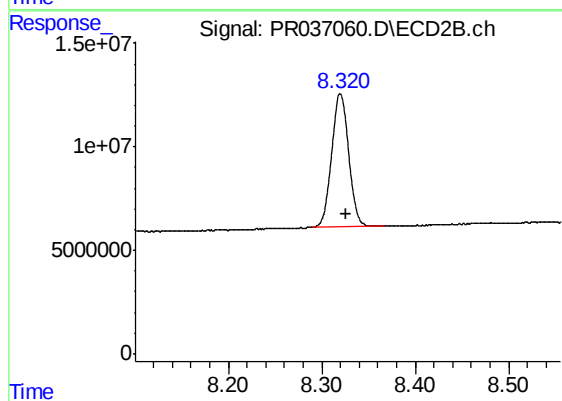

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.006 min
Response: 81323234
Conc: 10.19 ng/ml