

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041119\
 Data File : PR037117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 23:16
 Operator : SM\SJ
 Sample : K2316-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20190174-AMND-COMP-CS-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:04:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.448	0.000	15818643	0	9.929	N.D. #
2)	SA Decachlor...	10.028	8.316	12850222	42988655	6.859	5.386
Target Compounds							
7)	L1 AR-1016-5	0.000	4.968	0	3020686	N.D.	14.535 #
15)	L3 AR-1232-5	0.000	4.968	0	3020686	N.D.	52.706 #
20)	L4 AR-1242-5	0.000	5.306	0	2842223	N.D.	20.588 #
24)	L5 AR-1248-4	0.000	4.968	0	3020686	N.D.	17.128 #
25)	L5 AR-1248-5	0.000	5.306	0	2842223	N.D.	14.620 #
26)	L6 AR-1254-1	0.000	5.306	0	2842223	N.D.	8.642 #
29)	L6 AR-1254-4	0.000	6.058	0	6893076	N.D.	17.987 #
33)	L7 AR-1260-3	0.000	6.317	0	4161406	N.D.	7.868 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041119\
Data File : PR037117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 23:16
Operator : SM\SJ
Sample : K2316-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:04:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

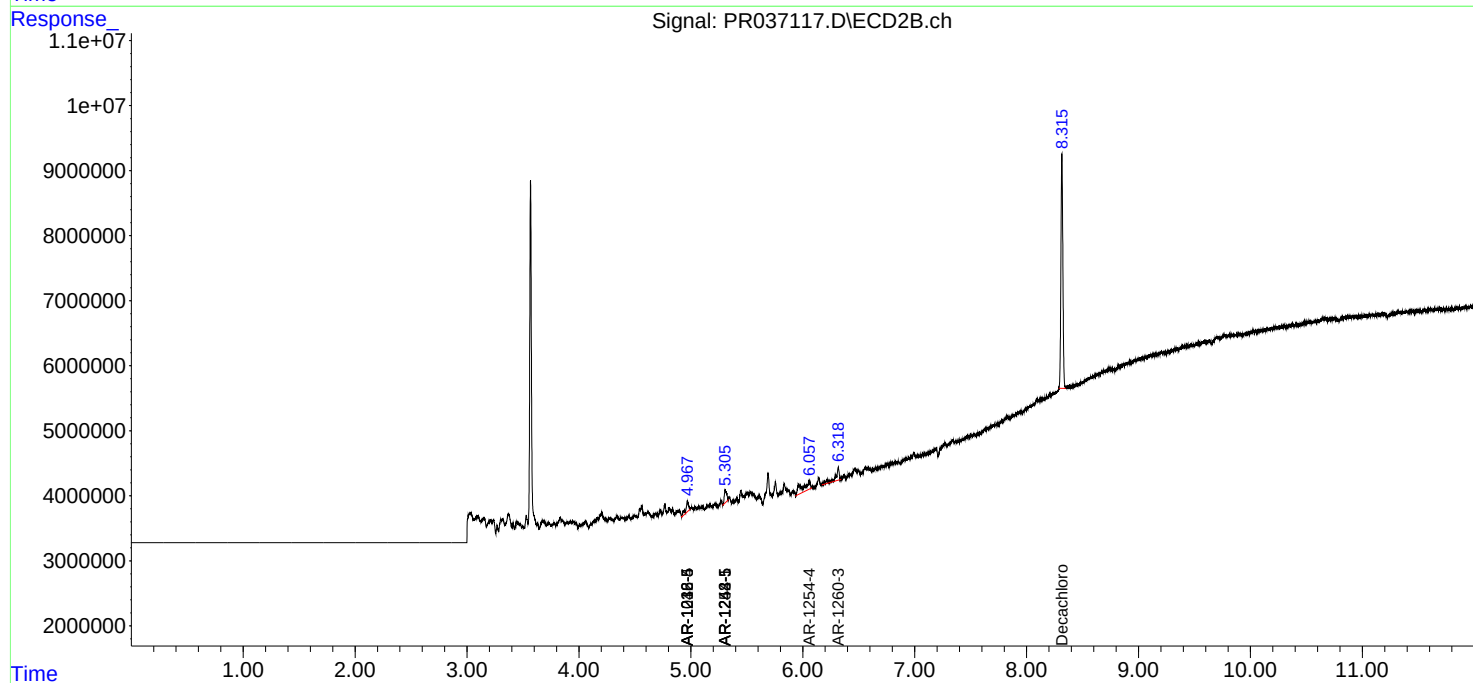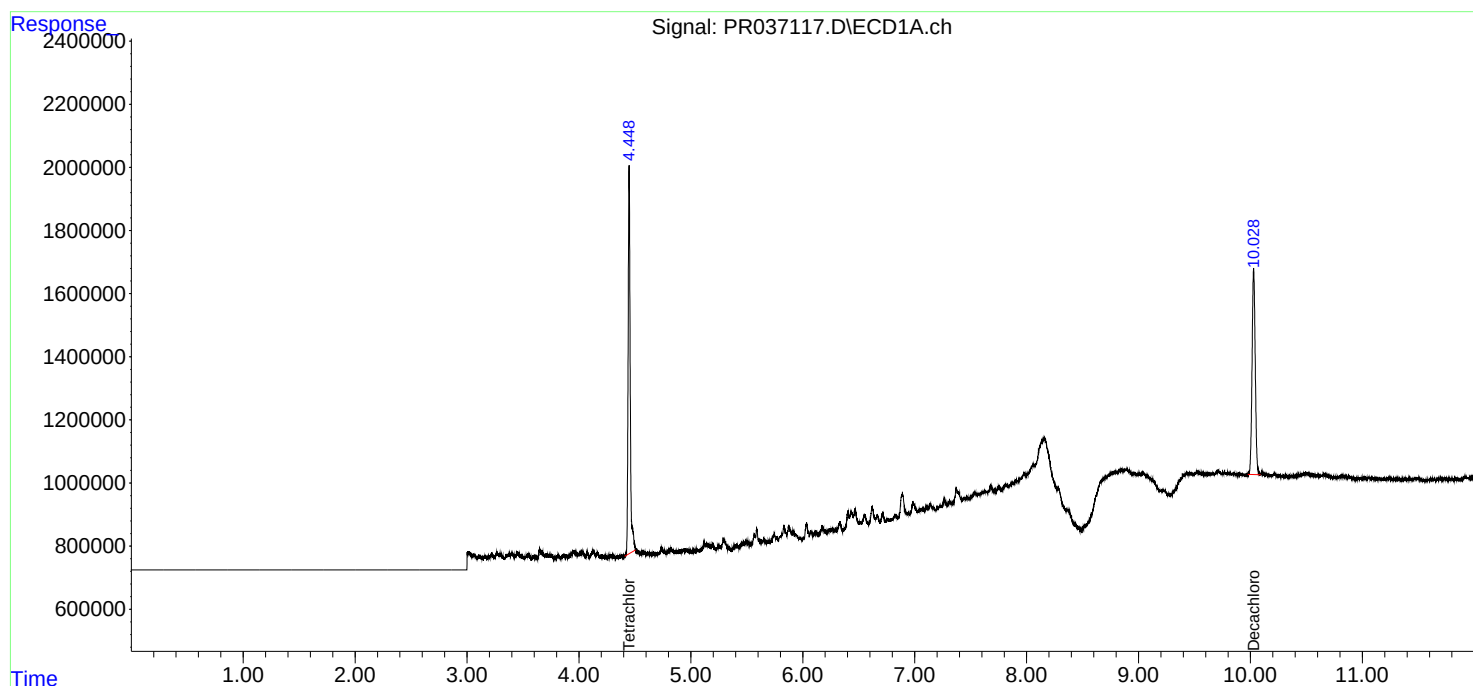


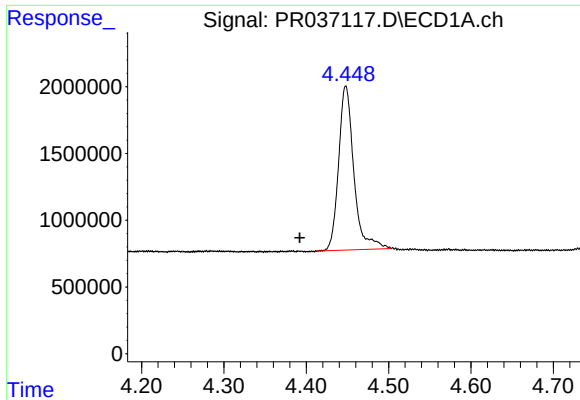

#1 Tetrachloro-m-xylene


R.T.: 4.448 min
Delta R.T.: 0.056 min
Response: 15818643
Conc: 9.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

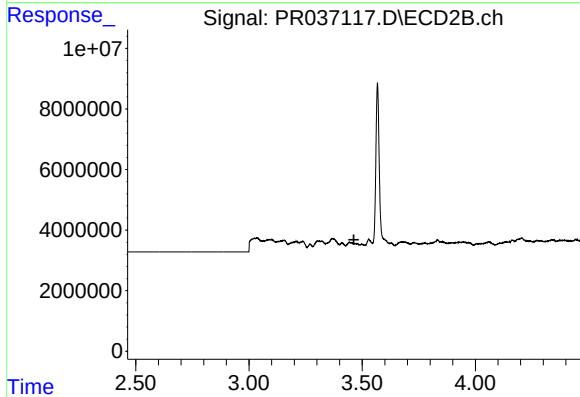


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.464 min
Response: 0
Conc: N.D.

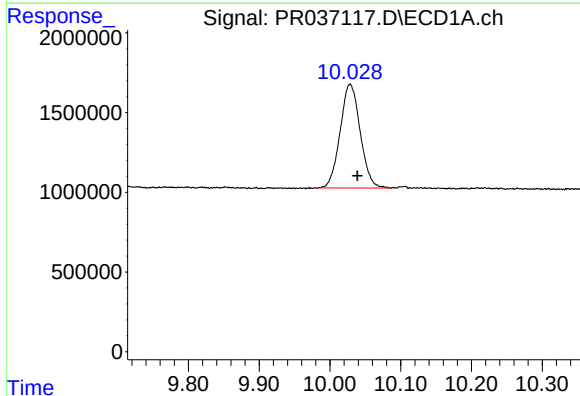


#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: -0.010 min
Response: 12850222
Conc: 6.86 ng/ml

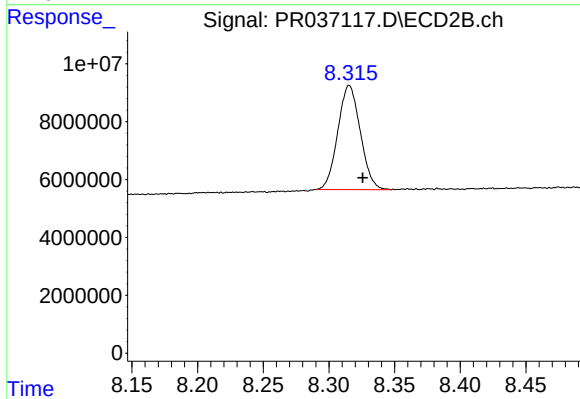

#2 Decachlorobiphenyl


R.T.: 8.316 min
Delta R.T.: -0.010 min
Response: 42988655
Conc: 5.39 ng/ml

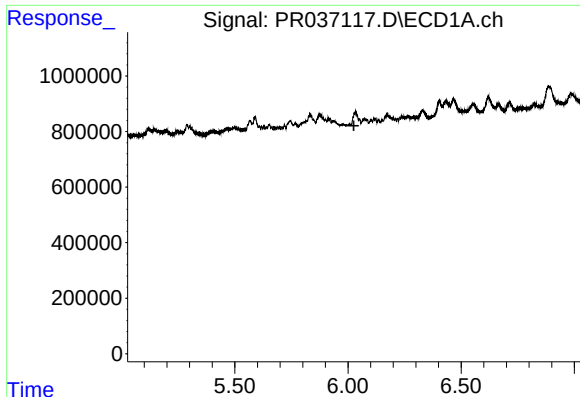

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

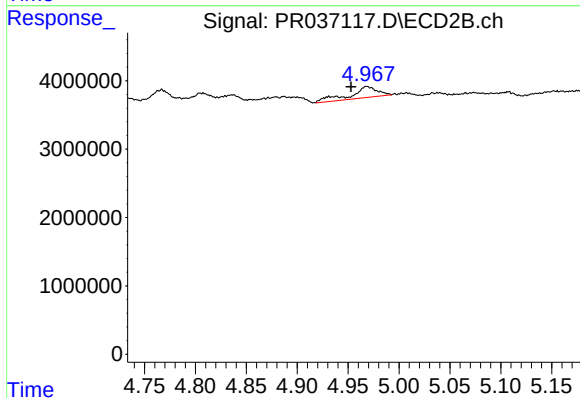


#7 AR-1016-5

R.T.: 4.968 min
Delta R.T.: 0.015 min
Response: 3020686
Conc: 14.53 ng/ml

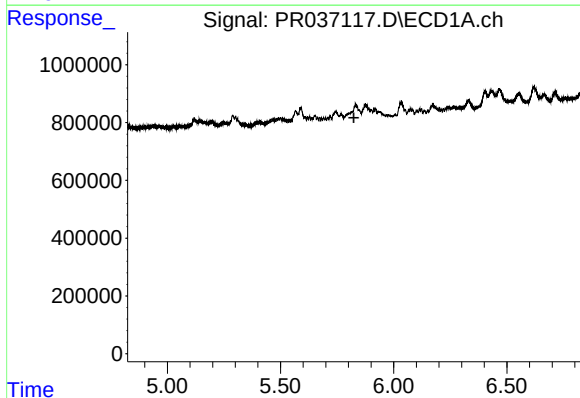


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

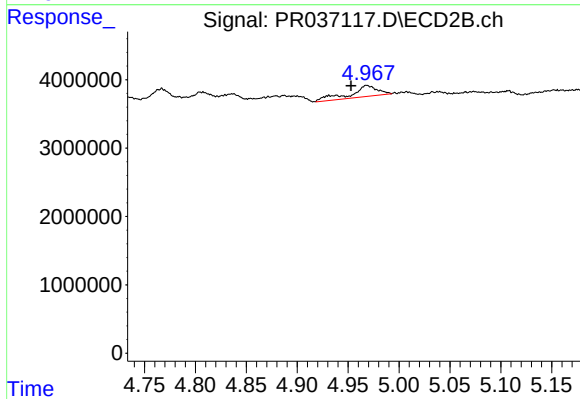

#15 AR-1232-5


R.T.: 4.968 min
Delta R.T.: 0.015 min
Response: 3020686
Conc: 52.71 ng/ml

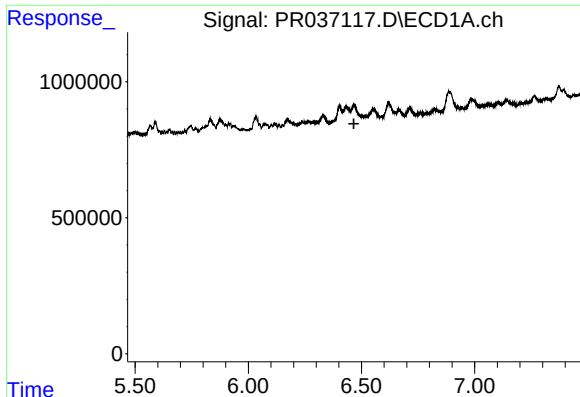

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

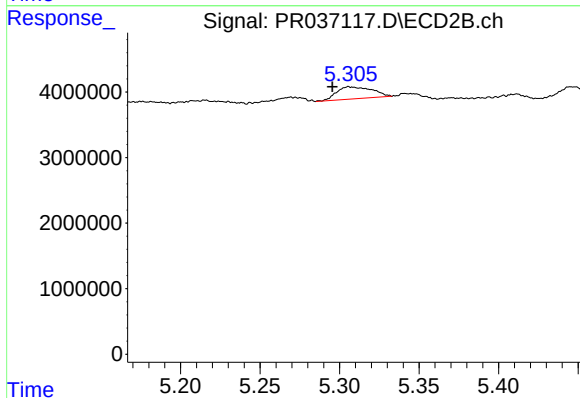


#20 AR-1242-5

R.T.: 5.306 min
Delta R.T.: 0.011 min
Response: 2842223
Conc: 20.59 ng/ml

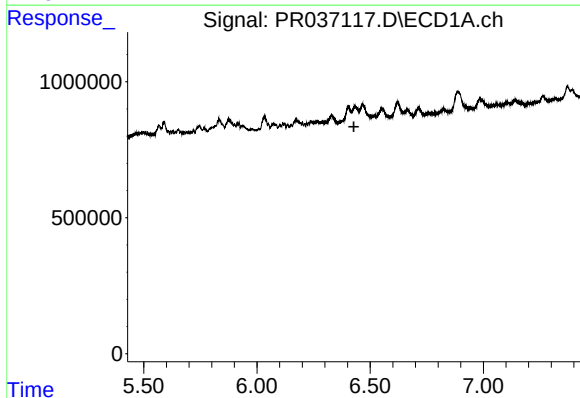


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

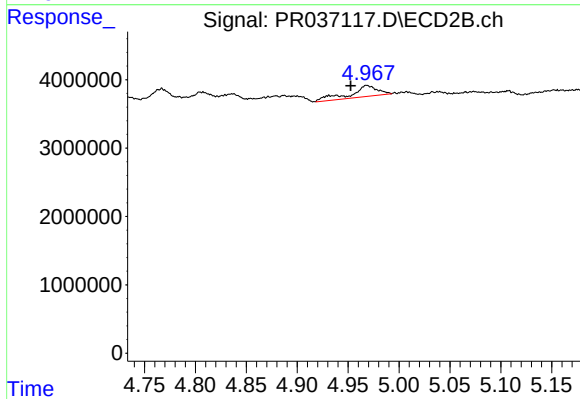

#24 AR-1248-4


R.T.: 4.968 min
Delta R.T.: 0.016 min
Response: 3020686
Conc: 17.13 ng/ml

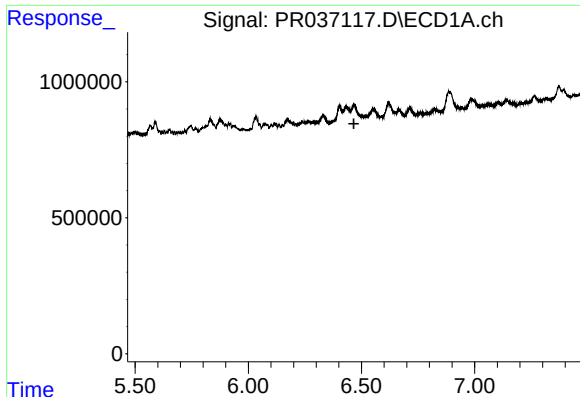

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

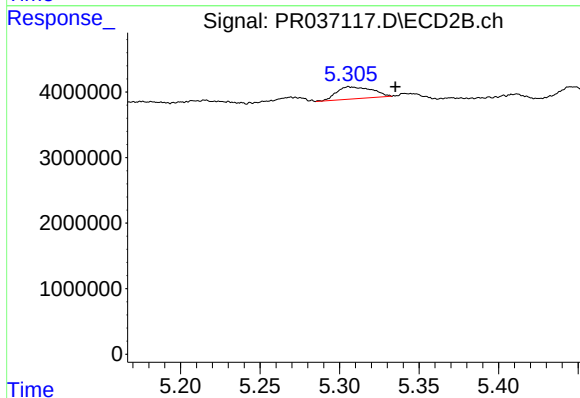


#25 AR-1248-5

R.T.: 5.306 min
Delta R.T.: -0.029 min
Response: 2842223
Conc: 14.62 ng/ml

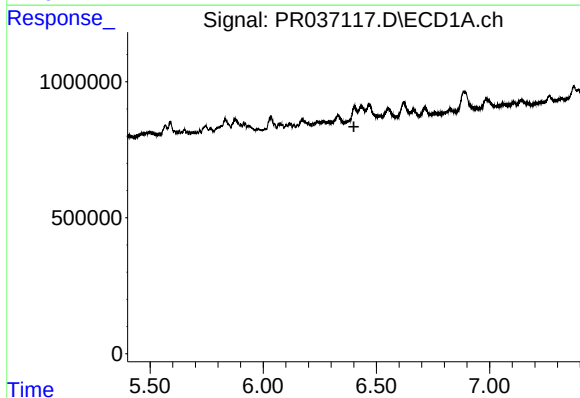


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.400 min
Response: 0
Conc: N.D.

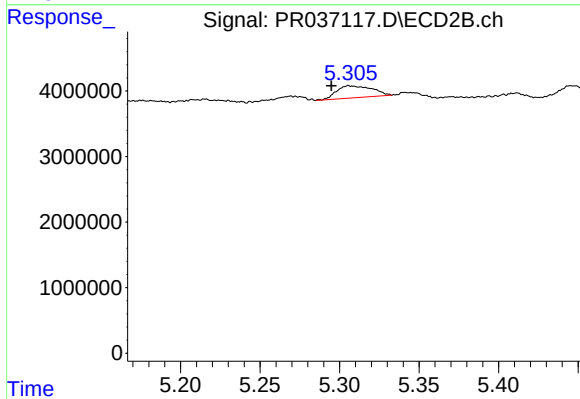

#26 AR-1254-1


R.T.: 5.306 min
Delta R.T.: 0.011 min
Response: 2842223
Conc: 8.64 ng/ml

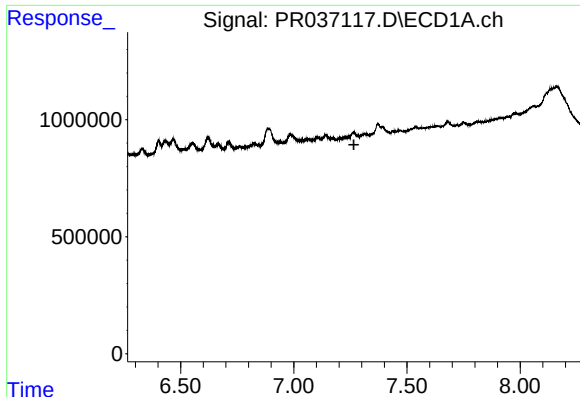

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.265 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
20190174-AMND-COMP-CS-1

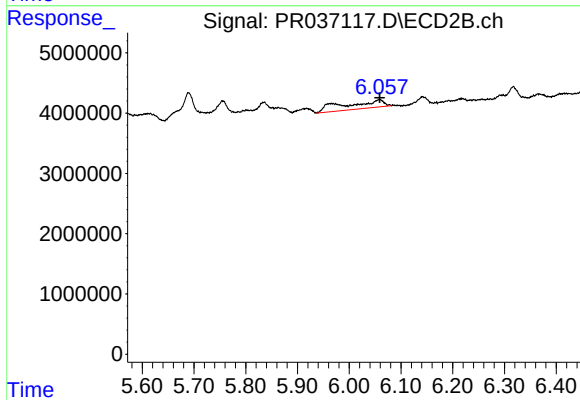


#29 AR-1254-4

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 6893076
Conc: 17.99 ng/ml

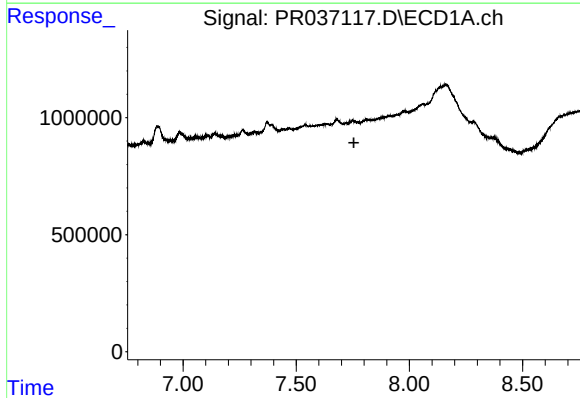

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.755 min
Response: 0
Conc: N.D.

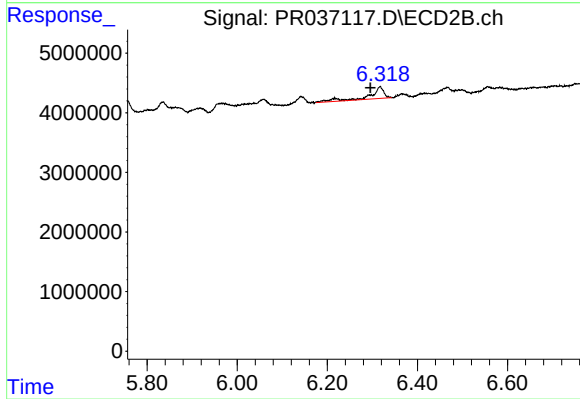

#33 AR-1260-3

R.T.: 6.317 min
Delta R.T.: 0.021 min
Response: 4161406
Conc: 7.87 ng/ml