

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041219\
 Data File : PR037119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 14:22
 Operator : SM\SJ
 Sample : K2316-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 20190176-AMND-COMP-CS-3

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:44:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 04:04:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 03 03:09:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.388	3.459	18513209	70550869	11.620m	12.044m
2) SA Decachlor...	10.028	8.316	13665194	56973871	7.294	7.138

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR041219\
Data File : PR037119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 14:22
Operator : SM\SJ
Sample : K2316-08
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
20190176-AMND-COMP-CS-3


Manual Integrations
APPROVED

mohammad
4/15/2019 4:44:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 04:04:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 03 03:09:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

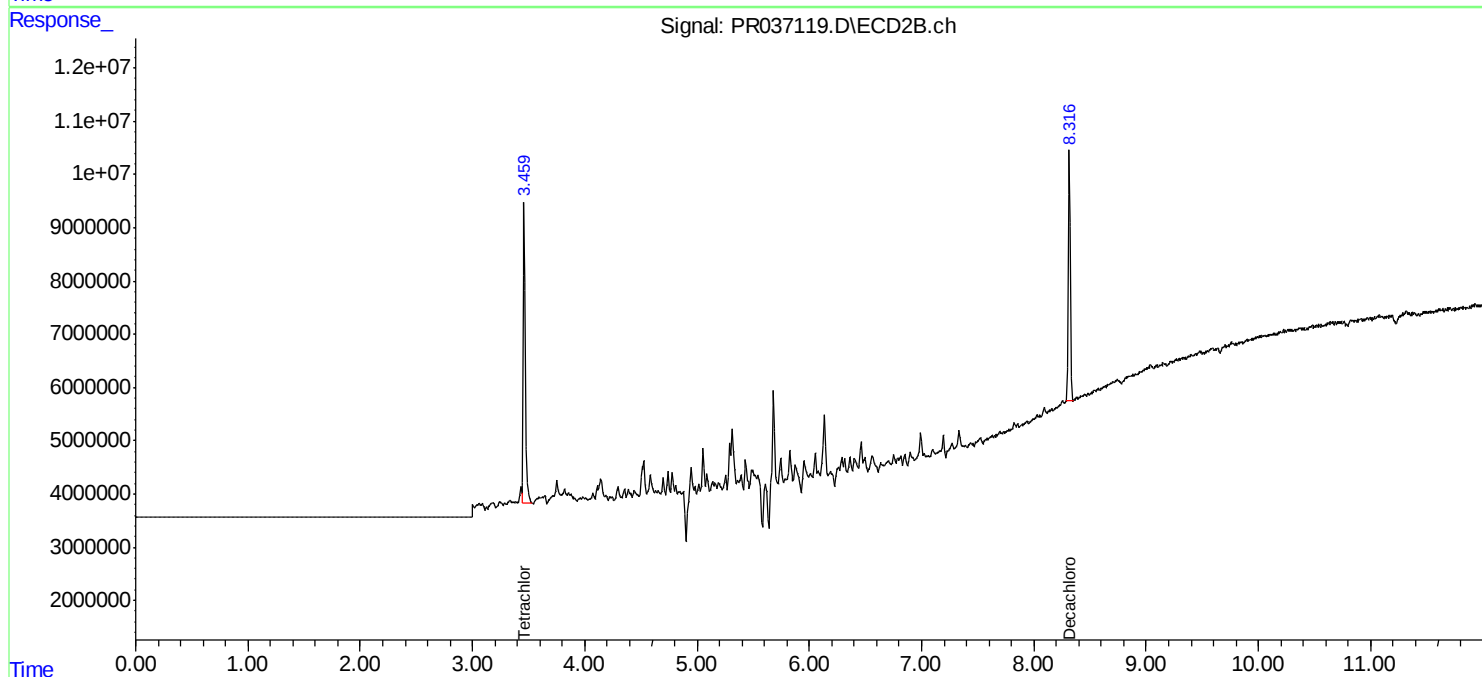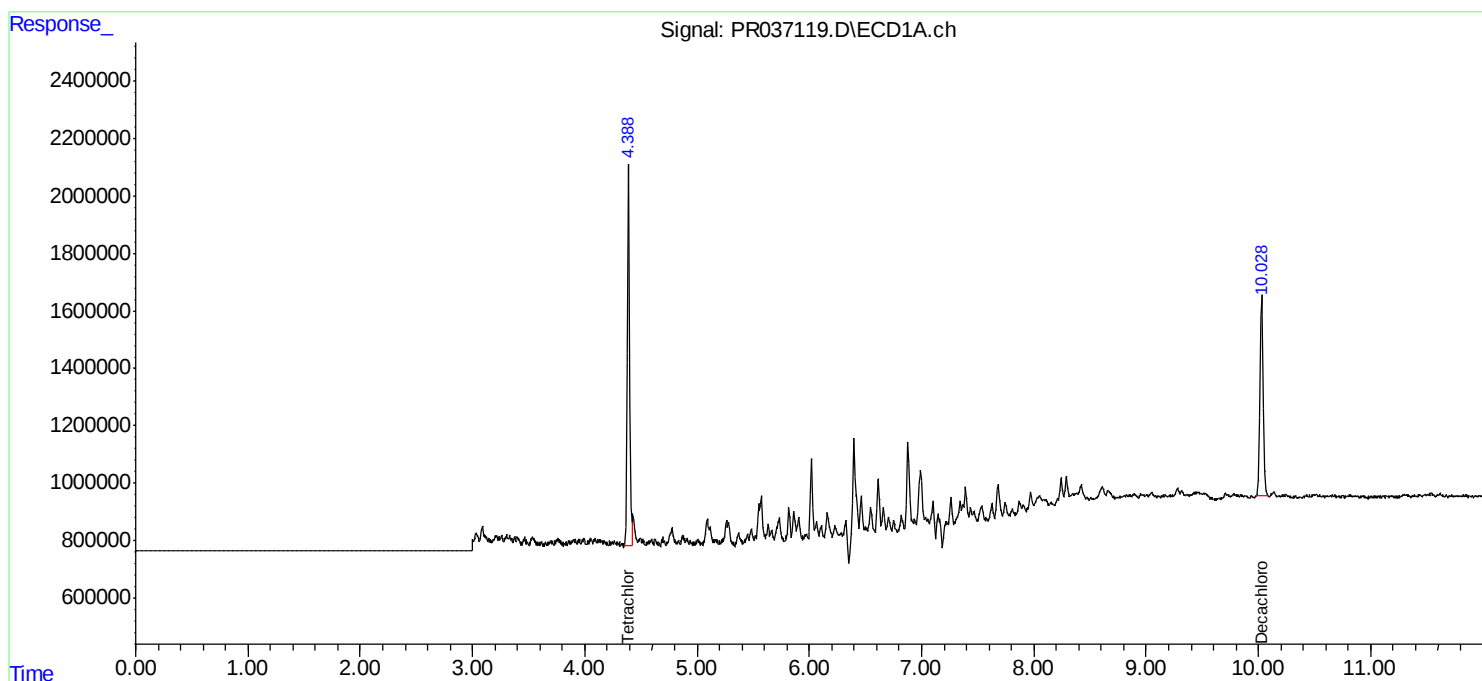

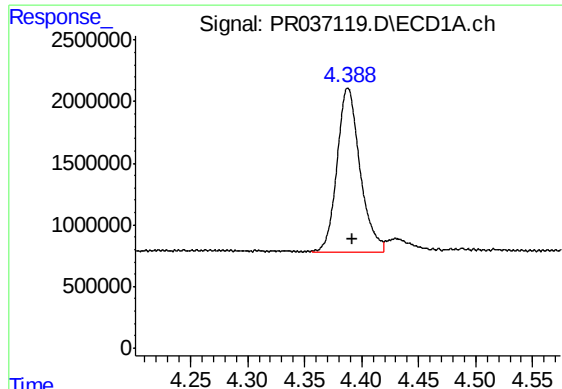


#1 Tetrachloro-m-xylene

R.T.: 4.388 min
Delta R.T.: -0.004 min
Response: 18513209
Conc: 11.62 ng/ml m

Instrument :
ECD_R
ClientSampleId :
20190176-AMND-COMP-CS-3


Manual Integrations
APPROVED

mohammad
4/15/2019 4:44:25 PM

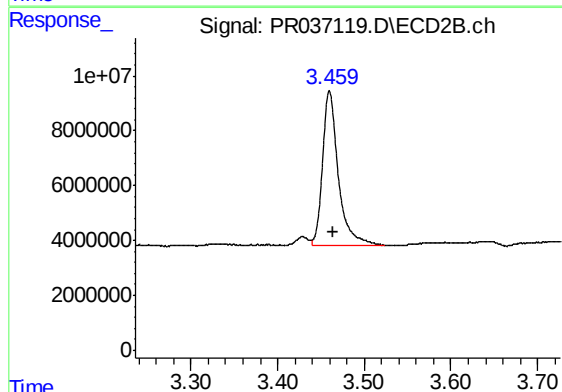


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: -0.004 min
Response: 70550869
Conc: 12.04 ng/ml m

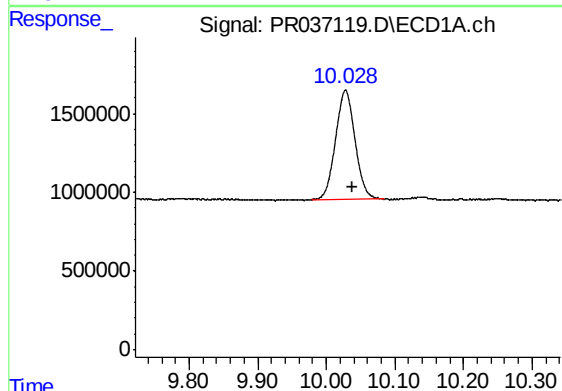

#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: -0.010 min
Response: 13665194
Conc: 7.29 ng/ml

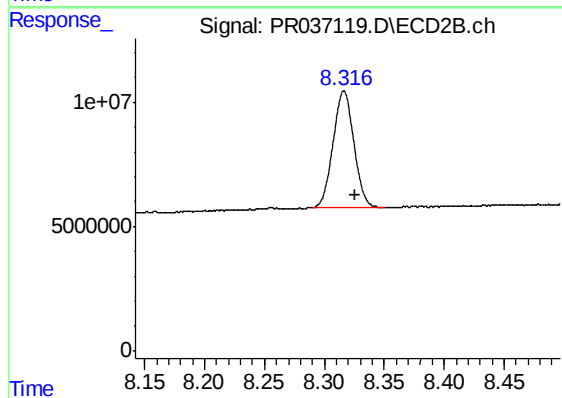

#2 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.009 min
Response: 56973871
Conc: 7.14 ng/ml